

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
 Data File : VX029804.D
 Acq On : 25 Jun 2022 07:00
 Operator : JC/MD
 Sample : N3386-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE134D2-20220616

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Title : SW846 8260

Signal : TIC: VX029804.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.331	196	204	212	rBV	92428	170349	11.47%	2.048%
2	4.501	551	560	571	rVB2	6099	16525	1.11%	0.199%
3	5.391	693	706	722	rBV	136993	399849	26.93%	4.808%
4	5.556	722	733	750	rVB	262137	733291	49.39%	8.818%
5	5.958	789	799	820	rBV	144786	382749	25.78%	4.603%
6	6.763	920	931	944	rBV	383915	923173	62.17%	11.101%
7	7.129	980	991	1003	rBV	693954	1484844	100.00%	17.855%
8	8.653	1234	1241	1257	rBV	772334	1207674	81.33%	14.522%
9	9.275	1334	1343	1356	rBV	187397	272256	18.34%	3.274%
10	10.055	1465	1471	1479	rBV	795720	1037858	69.90%	12.480%
11	11.085	1634	1640	1651	rBV	585369	756055	50.92%	9.092%
12	12.024	1789	1794	1804	rBV	767982	931303	62.72%	11.199%




Sum of corrected areas: 8315926

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
Data File : VX029804.D
Acq On : 25 Jun 2022 07:00
Operator : JC/MD
Sample : N3386-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE134D2-20220616

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

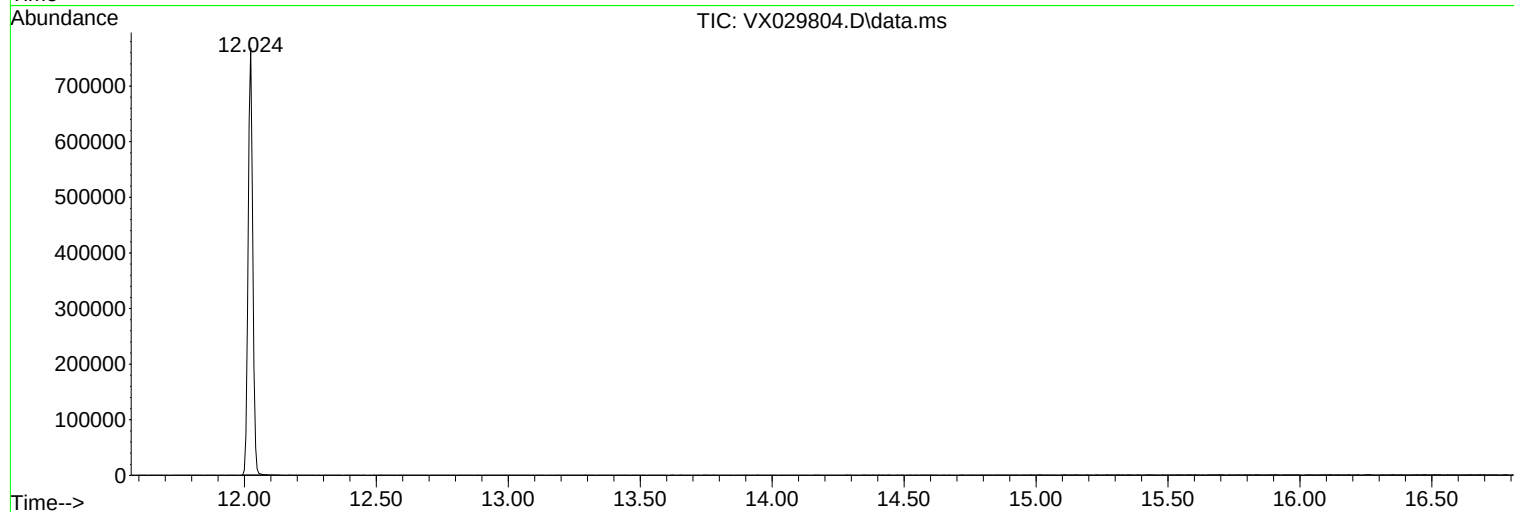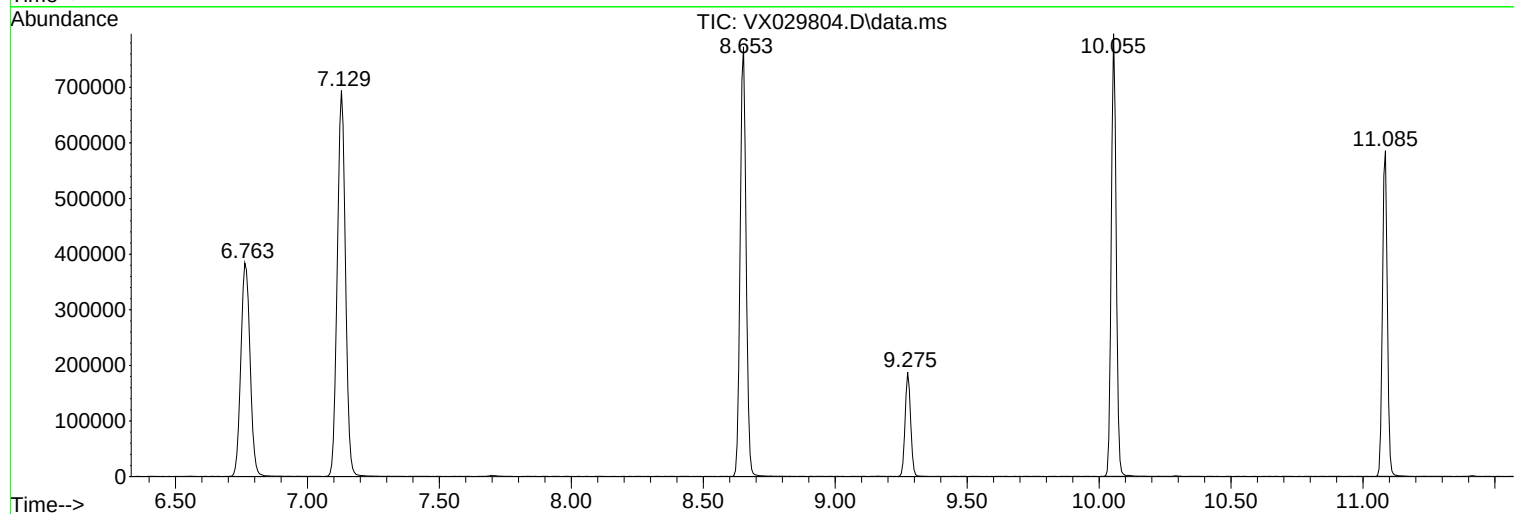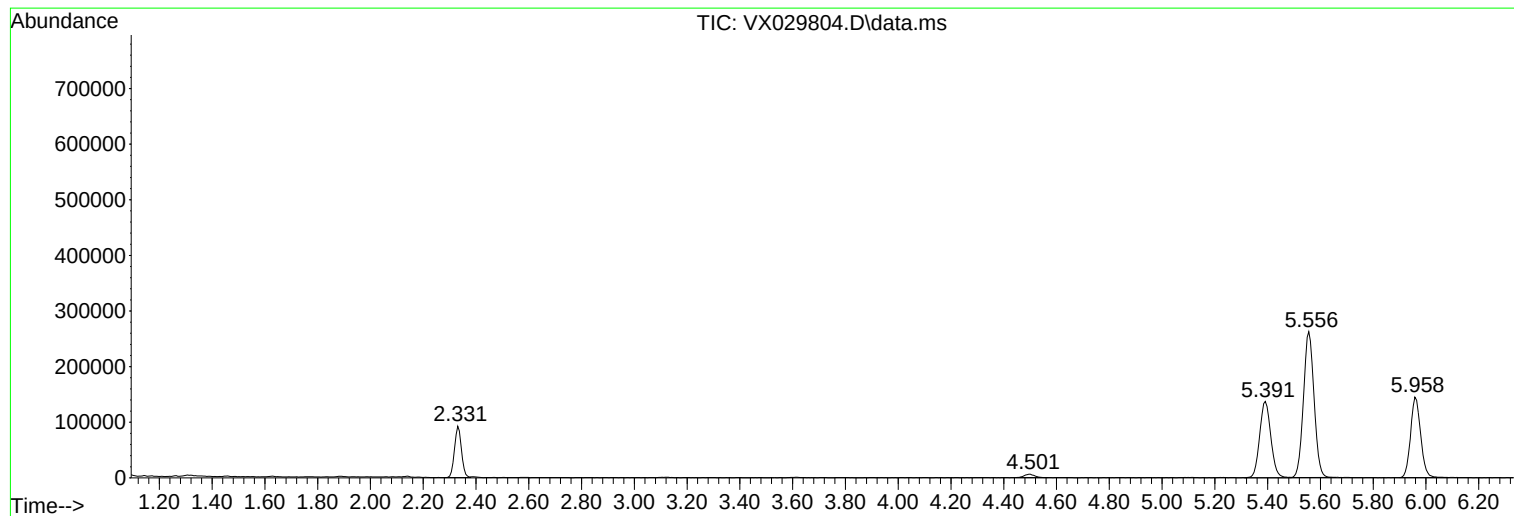

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
Data File : VX029804.D
Acq On : 25 Jun 2022 07:00
Operator : JC/MD
Sample : N3386-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE134D2-20220616

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
Data File : VX029804.D
Acq On : 25 Jun 2022 07:00
Operator : JC/MD
Sample : N3386-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE134D2-20220616

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc