

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
 Data File : VX029805.D
 Acq On : 25 Jun 2022 07:23
 Operator : JC/MD
 Sample : N3386-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE134D3-20220616

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M

Title : SW846 8260

Signal : TIC: VX029805.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.331	195	204	222	rBV	3410994	6410362	100.00%	34.327%
2	5.391	693	706	722	rBV	139698	404513	6.31%	2.166%
3	5.556	722	733	749	rVB	265291	746909	11.65%	4.000%
4	5.958	788	799	818	rBV	144679	392446	6.12%	2.102%
5	6.763	919	931	947	rBV	391458	933694	14.57%	5.000%
6	7.128	981	991	1010	rBV	1391277	2987884	46.61%	16.000%
7	8.653	1233	1241	1252	rBV	777884	1222928	19.08%	6.549%
8	9.274	1336	1343	1358	rBV	1922903	2776162	43.31%	14.866%
9	10.055	1465	1471	1487	rBV	798703	1062859	16.58%	5.692%
10	11.085	1634	1640	1653	rBV	602208	772832	12.06%	4.138%
11	12.024	1788	1794	1807	rBV	796528	963687	15.03%	5.161%




Sum of corrected areas: 18674276

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
Data File : VX029805.D
Acq On : 25 Jun 2022 07:23
Operator : JC/MD
Sample : N3386-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE134D3-20220616

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

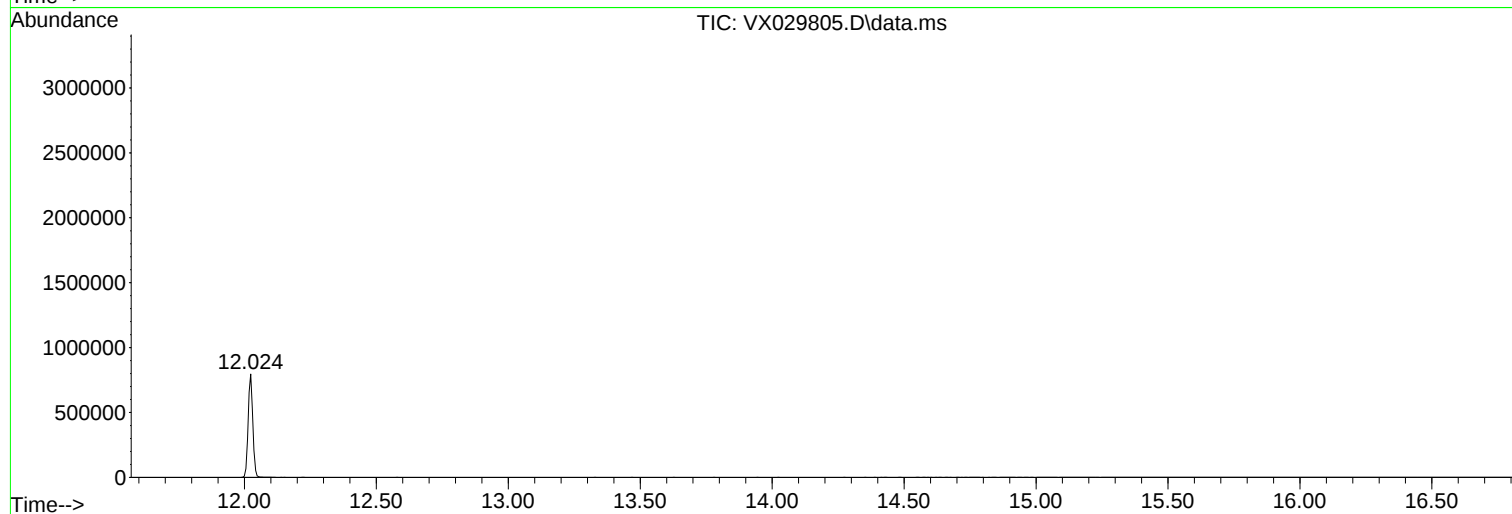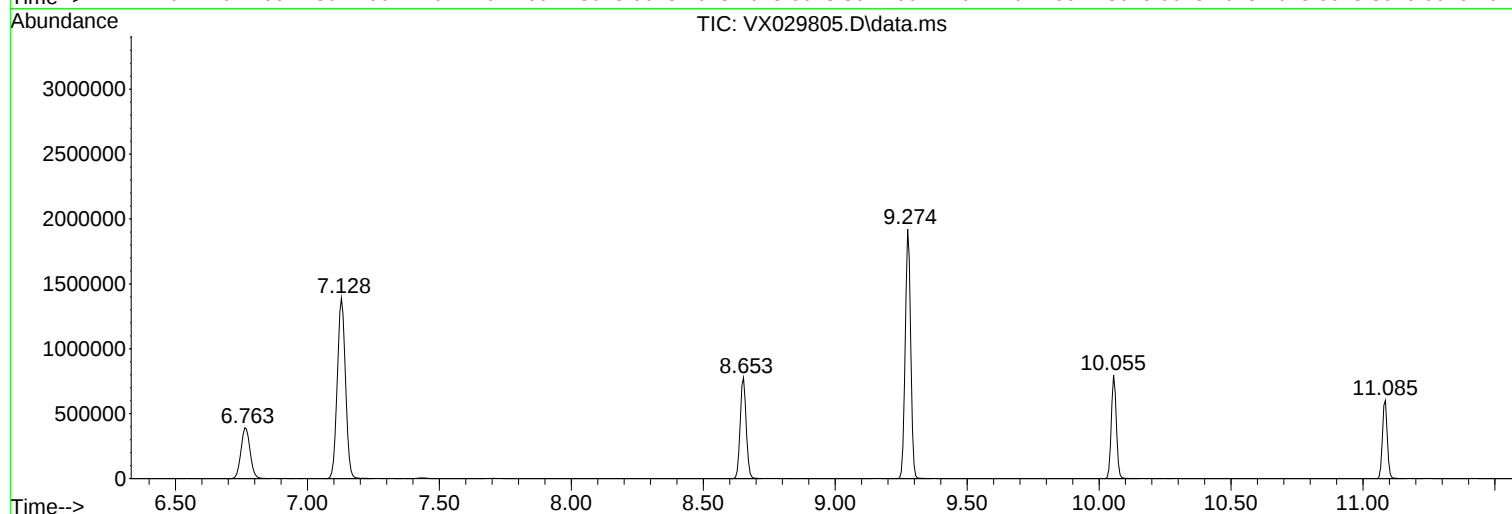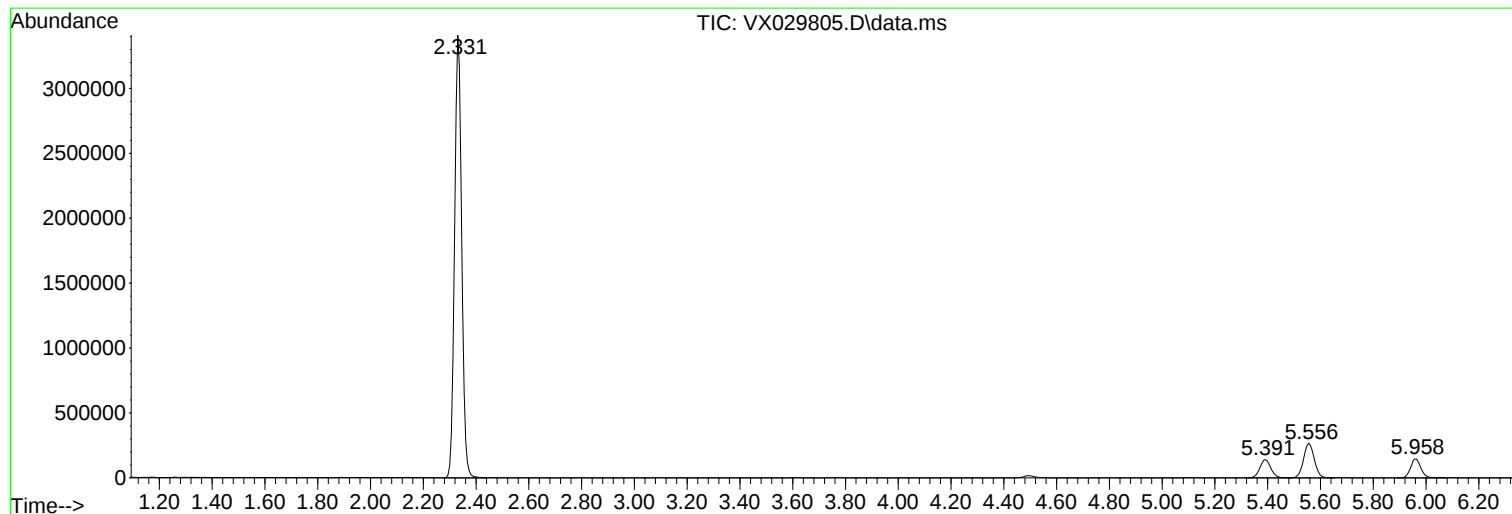

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
Data File : VX029805.D
Acq On : 25 Jun 2022 07:23
Operator : JC/MD
Sample : N3386-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE134D3-20220616

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062422\
Data File : VX029805.D
Acq On : 25 Jun 2022 07:23
Operator : JC/MD
Sample : N3386-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE134D3-20220616

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------