

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062423\
 Data File : VX036321.D
 Acq On : 24 Jun 2023 18:58
 Operator : JC/MD
 Sample : 03339-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-12

Quant Time: Jun 26 03:29:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 23 15:03:28 2023
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 06/26/2023
 Supervised By : Mahesh Dadoda 06/26/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	183195	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	357715	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	335789	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	146633	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	156126	59.455	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 118.900%#			
35) Dibromofluoromethane	5.385	113	119030	50.465	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 100.920%			
50) Toluene-d8	8.647	98	445562	50.577	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 101.160%			
62) 4-Bromofluorobenzene	11.079	95	155799	50.208	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 100.420%			
Target Compounds					Qvalue	
3) Chloromethane	1.294	50	1527	0.508	ug/l	92
6) Chloroethane	1.691	64	6111	2.531	ug/l	99
11) Tert butyl alcohol	2.995	59	1556	3.255	ug/l #	78
16) Acetone	2.398	43	80424	71.653	ug/l	93
18) Methyl Acetate	2.715	43	2216	0.480	ug/l #	74
19) Methyl tert-butyl Ether	3.111	73	17608	2.617	ug/l #	1
25) 2-Butanone	4.568	43	29445	18.258	ug/l	99
31) Cyclohexane	5.464	56	41290	12.270	ug/l	95
39) Methylcyclohexane	7.379	83	22510	5.345	ug/l	98
40) Benzene	6.038	78	2180893	222.050	ug/l	100
45) 1,2-Dichloropropane	7.440	63	1471	0.550	ug/l	93
51) 4-Methyl-2-Pentanone	8.574	43	4374	1.188	ug/l #	86
52) Toluene	8.720	92	412182	66.221	ug/l	96
59) 2-Hexanone	9.433	43	3181	1.183	ug/l	88
67) Ethyl Benzene	10.195	91	2060420	164.190	ug/l	97
68) m/p-Xylenes	10.305	106	340793	69.898	ug/l	99
69) o-Xylene	10.640	106	688335	146.198	ug/l	98
73) Isopropylbenzene	10.963	105	66706	6.037	ug/l	98
78) n-propylbenzene	11.305	91	120688	9.352	ug/l	100
80) 1,3,5-Trimethylbenzene	11.451	105	177194	18.934	ug/l	99
82) 4-Chlorotoluene	11.451	91	19432m	2.174	ug/l	
84) 1,2,4-Trimethylbenzene	11.750	105	468193	50.569	ug/l	96
85) sec-Butylbenzene	11.890	105	8034m	0.707	ug/l	
86) p-Isopropyltoluene	12.006	119	7873	0.826	ug/l #	72
90) Hexachloroethane	12.530	117	6414m	4.441	ug/l	
95) Naphthalene	13.774	128	241269	24.103	ug/l	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062423\
Data File : VX036321.D
Acq On : 24 Jun 2023 18:58
Operator : JC/MD
Sample : 03339-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
MW-12

Quant Time: Jun 26 03:29:08 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 23 15:03:28 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : John Carlone 06/26/2023
Supervised By : Mahesh Dadoda 06/26/2023

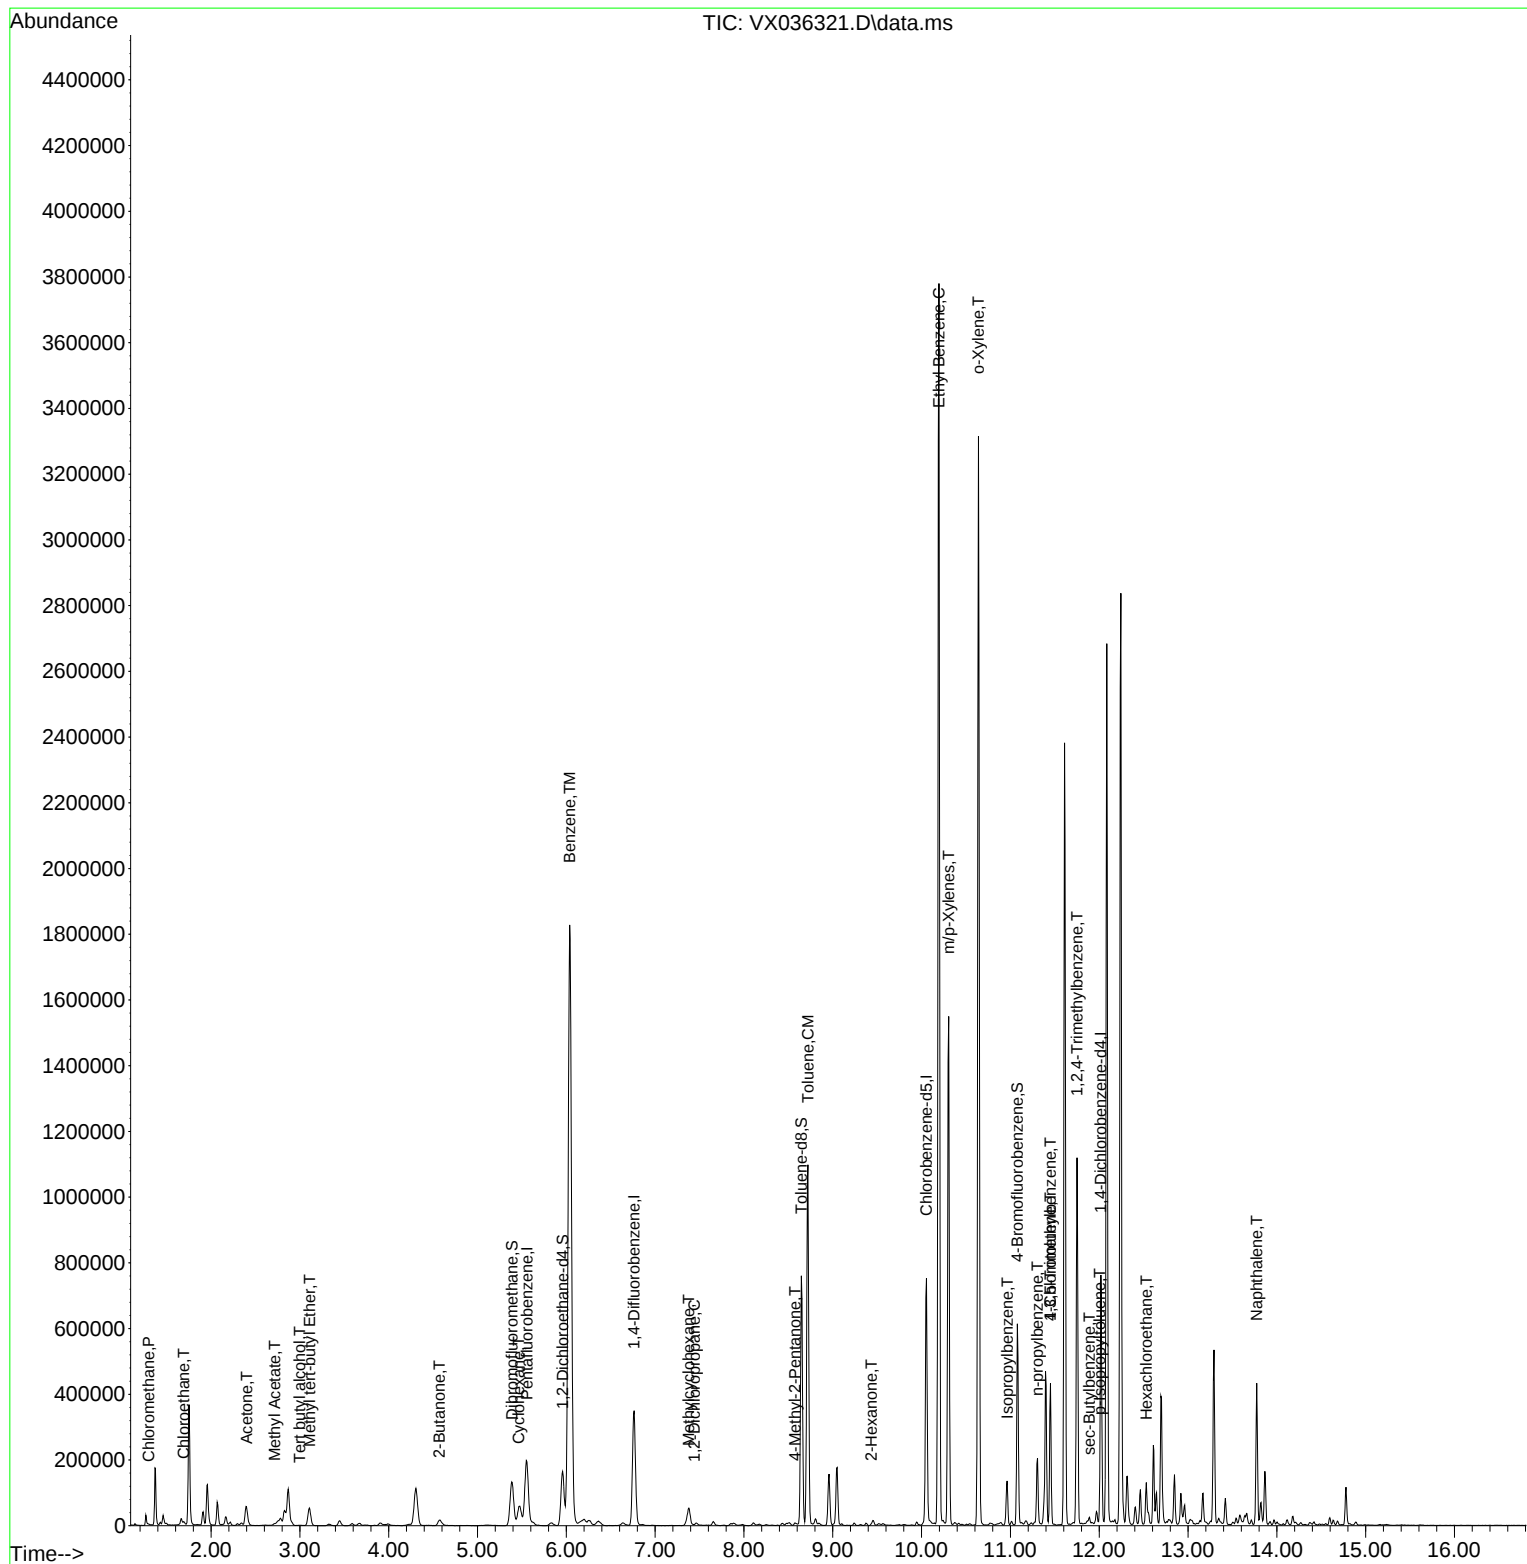



#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.007 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58




Instrument :
MSVOA_X
ClientSampleId :
MW-12



Tgt Ion:168 Resp: 18319
Ion Ratio Lower Upper
168 100
99 61.1 56.6 85.0




Manual Integrations
APPROVED


Reviewed By :John Carlone 06/26/2023
Supervised By :Mahesh Dadoda 06/26/2023

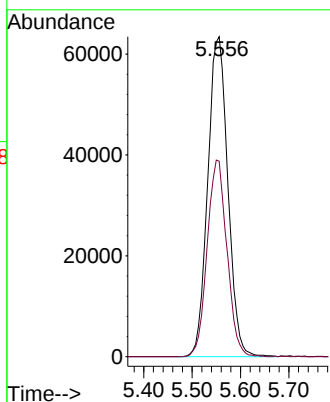

#3
Chloromethane
Concen: 0.508 ug/l
RT: 1.294 min Scan# 34
Delta R.T. 0.000 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58


Tgt Ion: 50 Resp: 1527
Ion Ratio Lower Upper
50 100
52 27.5 25.5 38.3

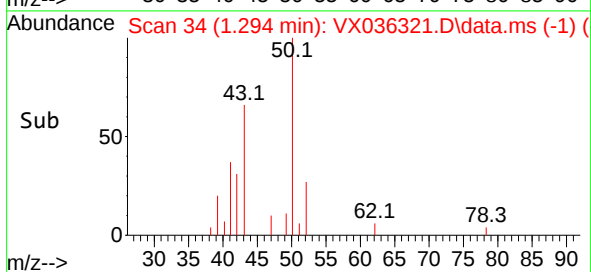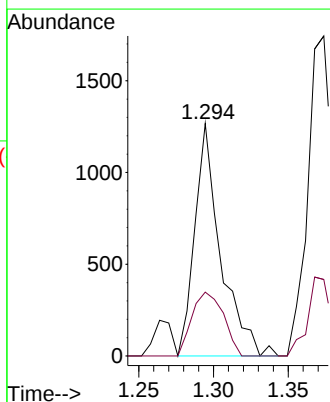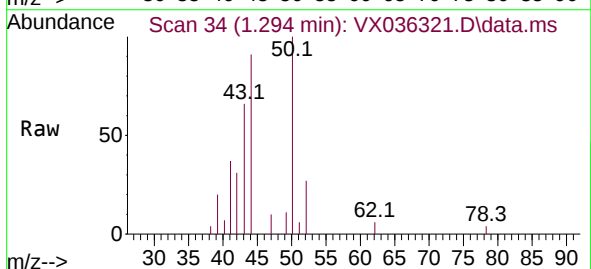

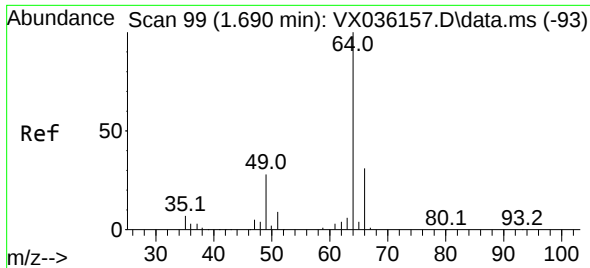

#6
Chloroethane
Concen: 2.531 ug/l
RT: 1.691 min Scan# 99
Delta R.T. 0.001 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58




Instrument :
MSVOA_X
ClientSampleId :
MW-12

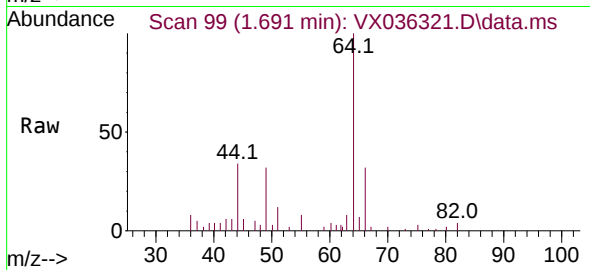

Tgt Ion: 64 Resp: 611
Ion Ratio Lower Upper
64 100
66 32.1 25.1 37.7




Manual Integrations
APPROVED


Reviewed By :John Carlone 06/26/2023
Supervised By :Mahesh Dadoda 06/26/2023

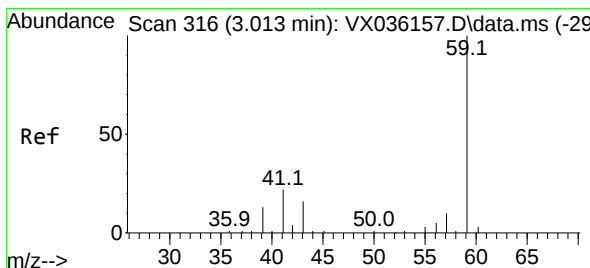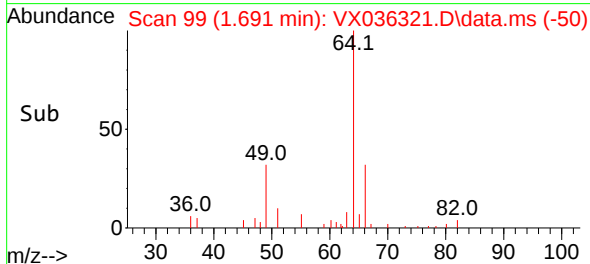

#11
Tert butyl alcohol
Concen: 3.255 ug/l
RT: 2.995 min Scan# 313
Delta R.T. -0.018 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58

Tgt Ion: 59 Resp: 1556
Ion Ratio Lower Upper
59 100
57 0.0 6.0 9.0#

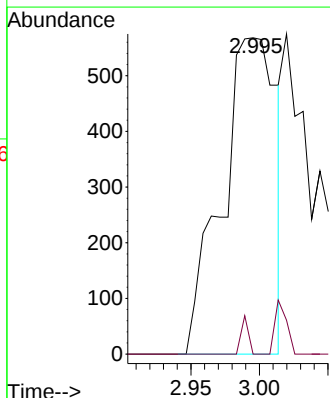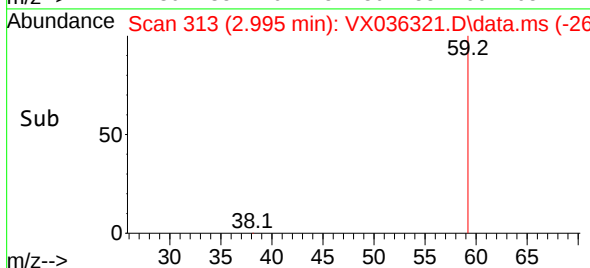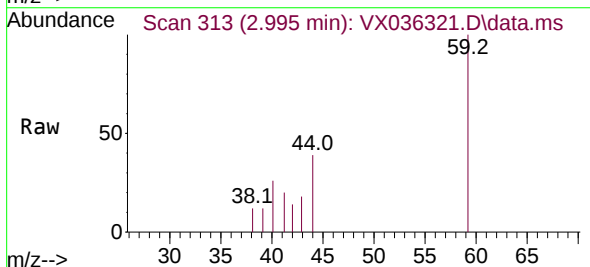







#16
Acetone
Concen: 71.653 ug/l
RT: 2.398 min Scan# 216
Delta R.T. -0.006 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58

Instrument :
MSVOA_X
ClientSampleId :
MW-12

Tgt Ion: 43 Resp: 80424
Ion Ratio Lower Upper
43 100
58 31.1 21.9 32.9




Manual Integrations
APPROVED


Reviewed By :John Carlone 06/26/2023
Supervised By :Mahesh Dadoda 06/26/2023

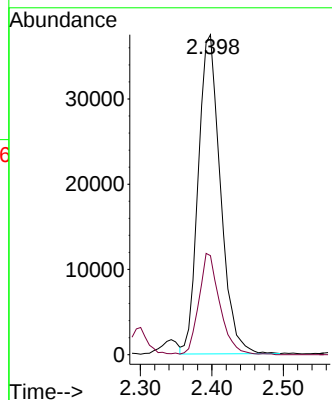

#18
Methyl Acetate
Concen: 0.480 ug/l
RT: 2.715 min Scan# 267
Delta R.T. 0.006 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58

Tgt Ion: 43 Resp: 2216
Ion Ratio Lower Upper
43 100
74 9.7 17.8 26.8#

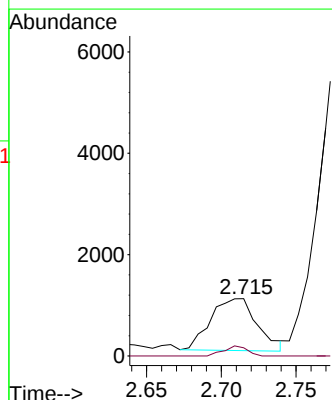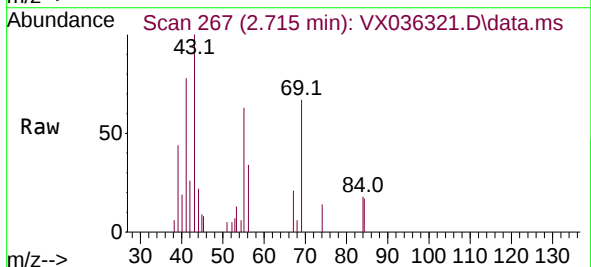



#19

Methyl tert-butyl Ether

Concen: 2.617 ug/l

RT: 3.111 min Scan# 311

Delta R.T. 0.000 min

Lab File: VX036321.D

Acq: 24 Jun 2023 18:58

Instrument :

MSVOA_X

ClientSampleId :

MW-12

Tgt Ion: 73 Resp: 17608

Ion Ratio Lower Upper

73 100





57 144.2 17.3 25.9

Manual Integrations

APPROVED

Reviewed By :John Carlone 06/26/2023

Supervised By :Mahesh Dadoda 06/26/2023



#25

2-Butanone

Concen: 18.258 ug/l

RT: 4.568 min Scan# 571

Delta R.T. 0.000 min

Lab File: VX036321.D




Acq: 24 Jun 2023 18:58


Tgt Ion: 43 Resp: 29445

Ion Ratio Lower Upper

43 100


72 24.8 19.4 29.2

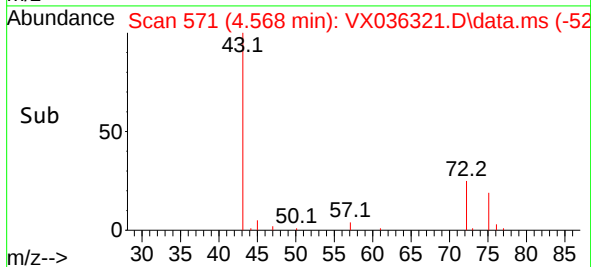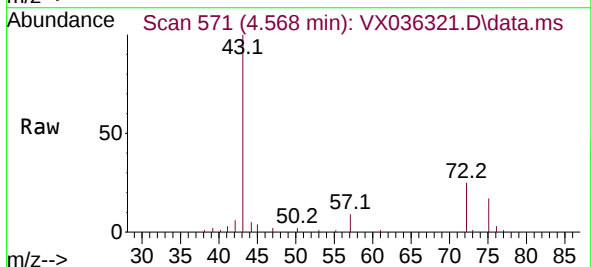



#31
Cyclohexane
Concen: 12.270 ug/l
RT: 5.464 min Scan# 718
Delta R.T. -0.006 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58




Instrument :
MSVOA_X
ClientSampleId :
MW-12



Tgt Ion: 56 Resp: 41290
Ion Ratio Lower Upper
56 100
69 30.9 23.4 35.2
84 77.5 65.9 98.9




Manual Integrations
APPROVED


Reviewed By :John Carlone 06/26/2023
Supervised By :Mahesh Dadoda 06/26/2023



#33
1,2-Dichloroethane-d4
Concen: 59.455 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58

Tgt Ion: 65 Resp: 156126
Ion Ratio Lower Upper
65 100
67 52.4 0.0 100.2

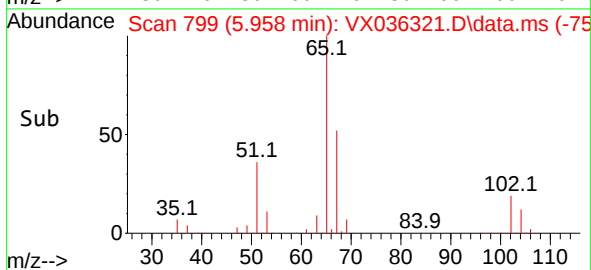







#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58

Instrument :
MSVOA_X
ClientSampleId :
MW-12

Tgt Ion:114 Resp: 357715
Ion Ratio Lower Upper
114 100
63 20.7 0.0 45.0
88 15.4 0.0 36.6




Manual Integrations
APPROVED


Reviewed By :John Carlone 06/26/2023
Supervised By :Mahesh Dadoda 06/26/2023

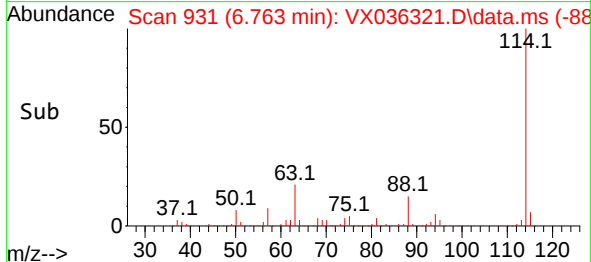

#35
Dibromofluoromethane
Concen: 50.465 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58


Tgt Ion:113 Resp: 119030
Ion Ratio Lower Upper
113 100
111 101.4 82.9 124.3
192 18.7 13.3 19.9

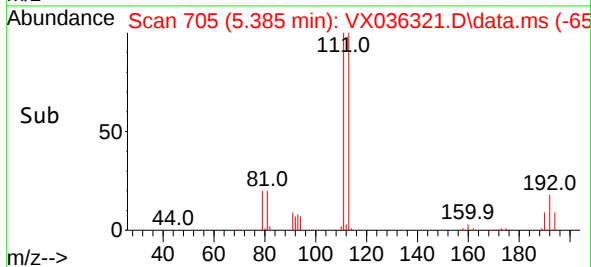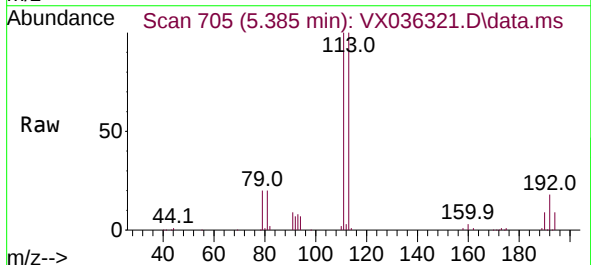

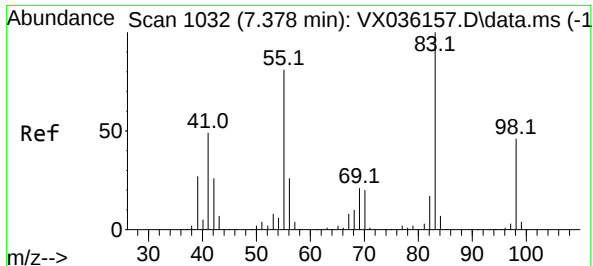

#39
Methylcyclohexane
Concen: 5.345 ug/l
RT: 7.379 min Scan# 1032
Delta R.T. 0.001 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58




Instrument :
MSVOA_X
ClientSampleId :
MW-12

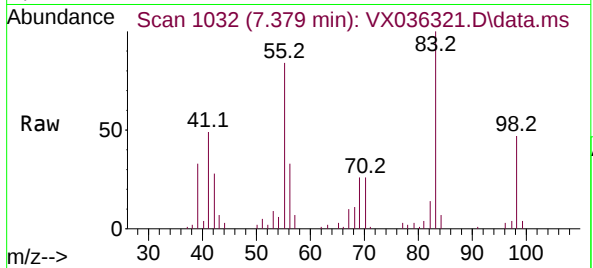

Tgt Ion: 83 Resp: 22510
Ion Ratio Lower Upper
83 100
55 83.5 64.6 97.0
98 46.7 36.7 55.1




Manual Integrations
APPROVED


Reviewed By :John Carlone 06/26/2023
Supervised By :Mahesh Dadoda 06/26/2023

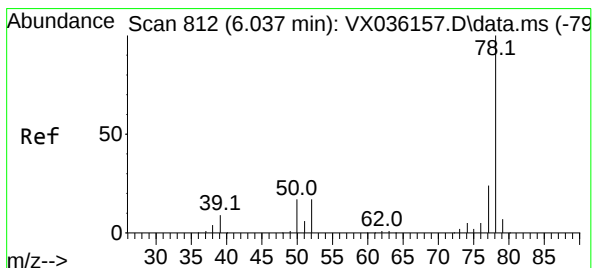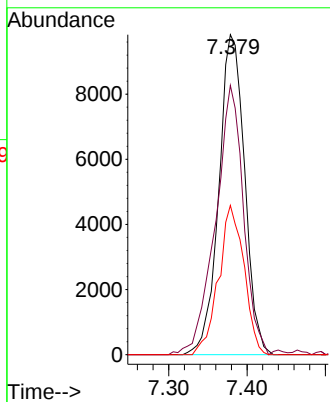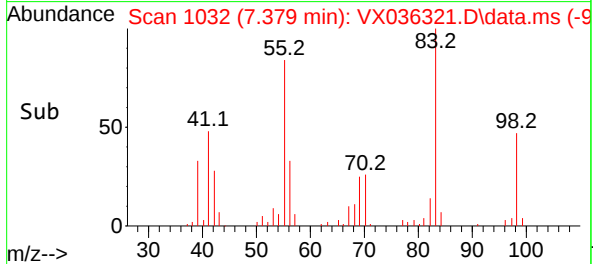

#40
Benzene
Concen: 222.050 ug/l
RT: 6.038 min Scan# 812
Delta R.T. 0.001 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58

Tgt Ion: 78 Resp: 2180893
Ion Ratio Lower Upper
78 100
77 24.3 19.3 28.9

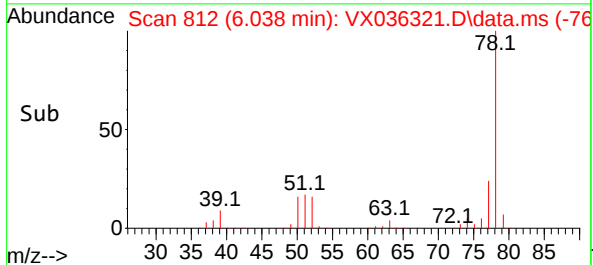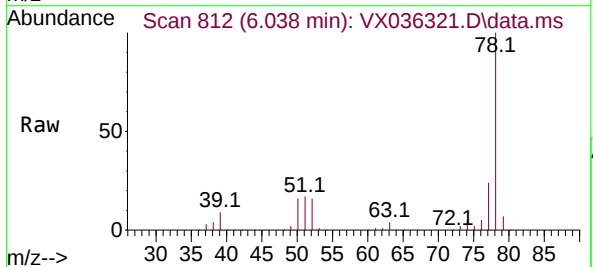

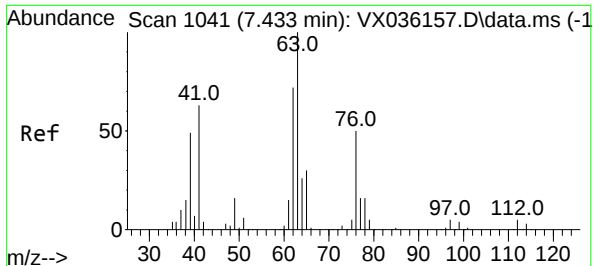

#45

1,2-Dichloropropane

Concen: 0.550 ug/l

RT: 7.440 min Scan# 1041

Delta R.T. 0.007 min

Lab File: VX036321.D

Acq: 24 Jun 2023 18:58

Instrument :

MSVOA_X

ClientSampleId :

MW-12

Tgt Ion: 63 Resp: 147

Ion Ratio Lower Upper

63 100





65 26.5 24.3 36.5

Manual Integrations

APPROVED

Reviewed By :John Carlone 06/26/2023

Supervised By :Mahesh Dadoda 06/26/2023

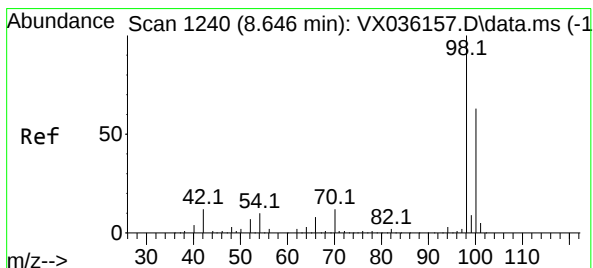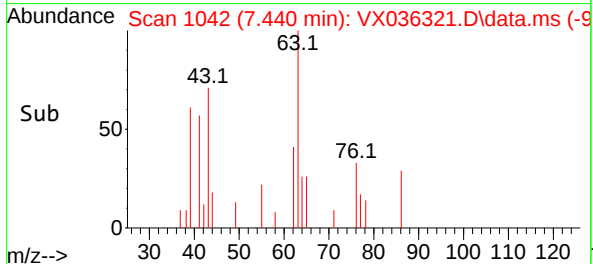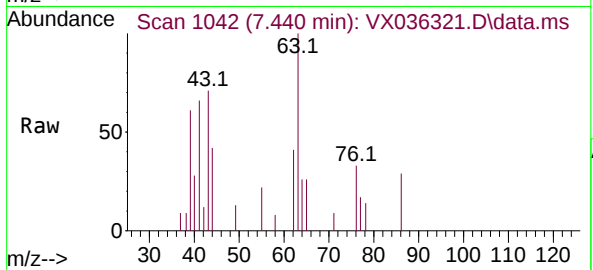

#50

Toluene-d8

Concen: 50.577 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.001 min

Lab File: VX036321.D




Acq: 24 Jun 2023 18:58


Tgt Ion: 98 Resp: 445562

Ion Ratio Lower Upper

98 100

100 64.0 53.1 79.7

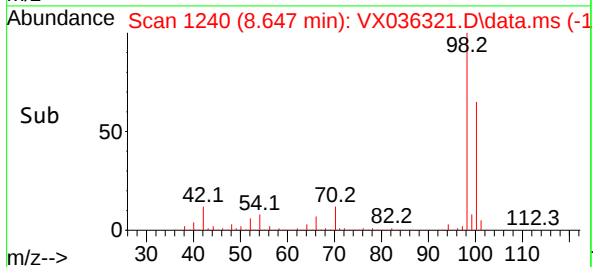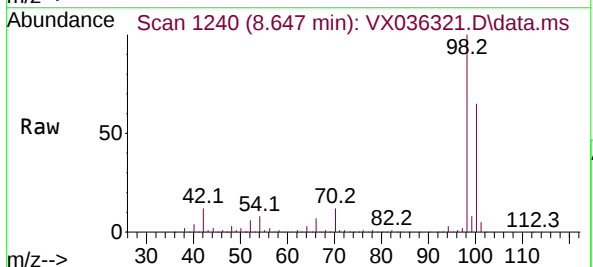



#51

4-Methyl-2-Pentanone

Concen: 1.188 ug/l

RT: 8.574 min Scan# 1228

Delta R.T. 0.001 min

Lab File: VX036321.D

Acq: 24 Jun 2023 18:58

Instrument :

MSVOA_X

ClientSampleId :

MW-12

Tgt Ion: 43 Resp: 4374

Ion Ratio Lower Upper

43 100





58 46.2 30.4 45.6

Manual Integrations

APPROVED

Reviewed By :John Carlone 06/26/2023

Supervised By :Mahesh Dadoda 06/26/2023



#52

Toluene

Concen: 66.221 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.000 min

Lab File: VX036321.D




Acq: 24 Jun 2023 18:58


Tgt Ion: 92 Resp: 412182

Ion Ratio Lower Upper

92 100

91 172.9 134.2 201.2

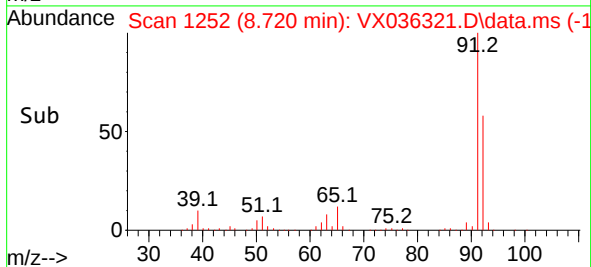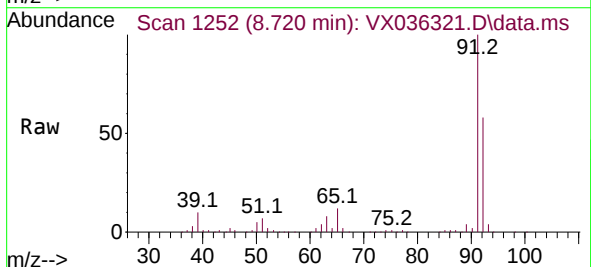







#59
2-Hexanone
Concen: 1.183 ug/l
RT: 9.433 min Scan# 1369
Delta R.T. 0.000 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58

Instrument :
MSVOA_X
ClientSampleId :
MW-12

Tgt Ion: 43 Resp: 318
Ion Ratio Lower Upper
43 100
58 60.7 26.2 78.5




Manual Integrations
APPROVED


Reviewed By :John Carlone 06/26/2023
Supervised By :Mahesh Dadoda 06/26/2023

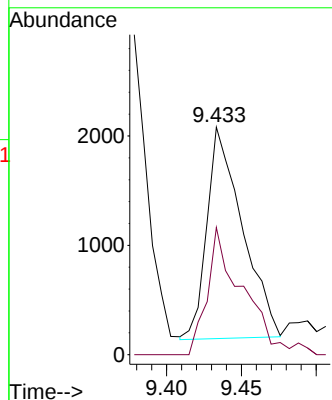

#62
4-Bromofluorobenzene
Concen: 50.208 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58


Tgt Ion: 95 Resp: 155799
Ion Ratio Lower Upper
95 100
174 77.7 0.0 135.6
176 74.8 0.0 131.0

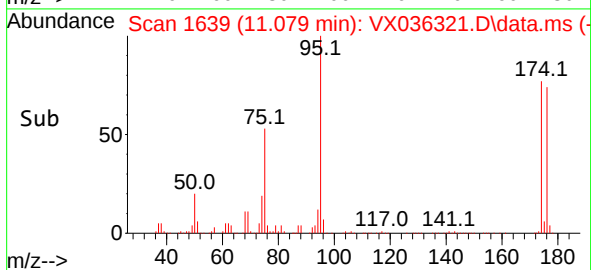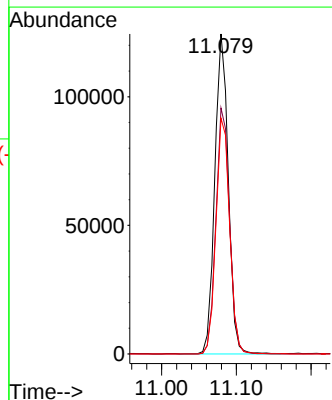



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58




Instrument :
MSVOA_X
ClientSampleId :
MW-12



Tgt Ion:117 Resp: 335789
Ion Ratio Lower Upper
117 100
82 55.6 46.2 69.4
119 32.7 25.5 38.3




Manual Integrations
APPROVED


Reviewed By :John Carlone 06/26/2023
Supervised By :Mahesh Dadoda 06/26/2023



#67
Ethyl Benzene
Concen: 164.190 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58


Tgt Ion: 91 Resp: 2060420
Ion Ratio Lower Upper
91 100
106 32.5 24.9 37.3

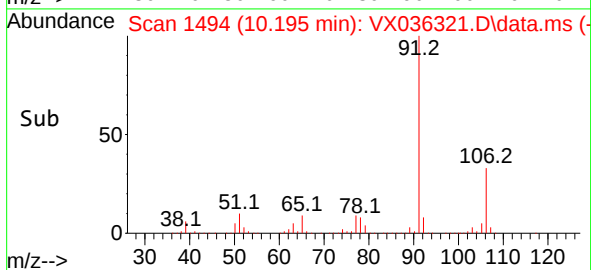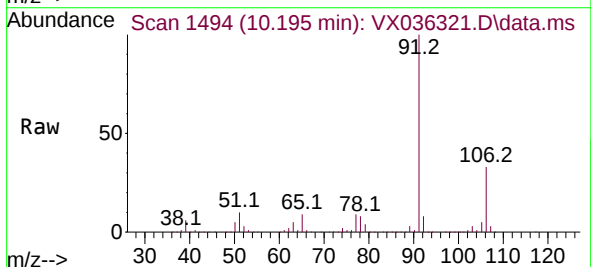

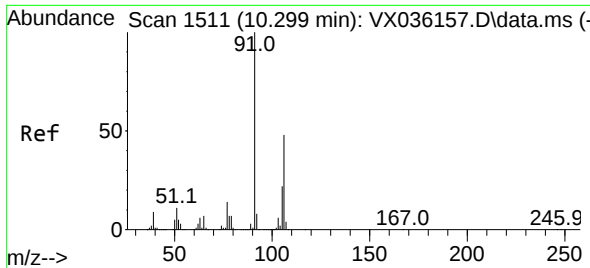

#68
m/p-Xylenes
Concen: 69.898 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.006 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58




Instrument :
MSVOA_X
ClientSampleId :
MW-12

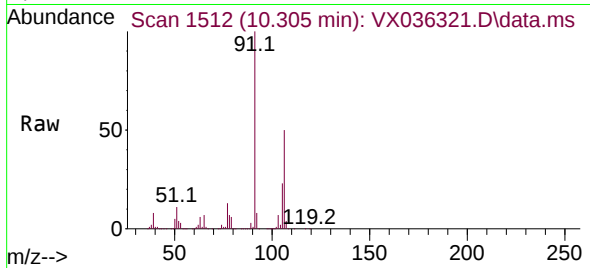

Tgt Ion:106 Resp: 340793
Ion Ratio Lower Upper
106 100
91 204.9 165.5 248.3




Manual Integrations
APPROVED


Reviewed By :John Carlone 06/26/2023
Supervised By :Mahesh Dadoda 06/26/2023

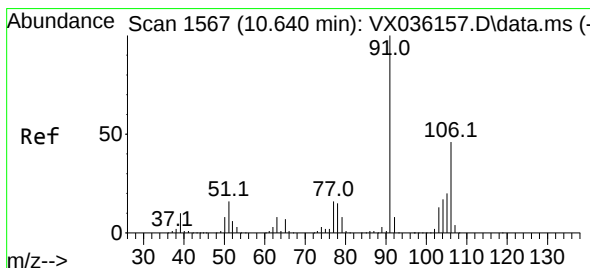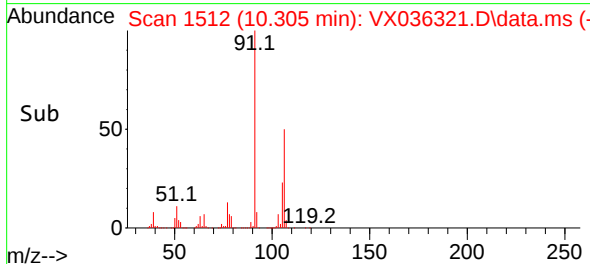

#69
o-Xylene
Concen: 146.198 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. 0.000 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58


Tgt Ion:106 Resp: 688335
Ion Ratio Lower Upper
106 100
91 214.5 108.9 326.8

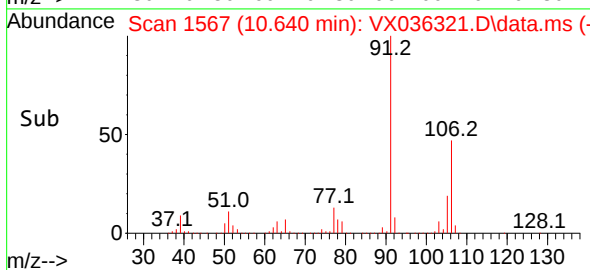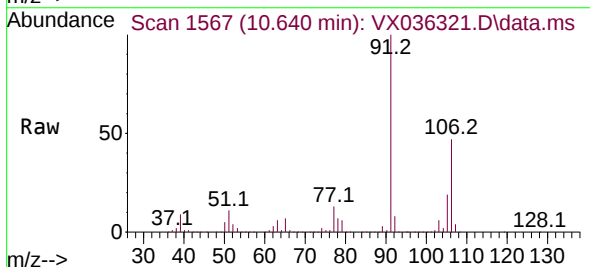



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1794
Delta R.T. -0.006 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58




Instrument :
MSVOA_X
ClientSampleId :
MW-12

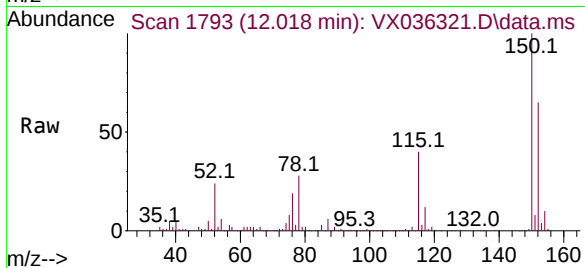


Tgt Ion:152 Resp: 146633
Ion Ratio Lower Upper
152 100
115 60.0 43.3 129.9
150 157.6 0.0 345.0

Manual Integrations
APPROVED



Reviewed By :John Carlone 06/26/2023
Supervised By :Mahesh Dadoda 06/26/2023

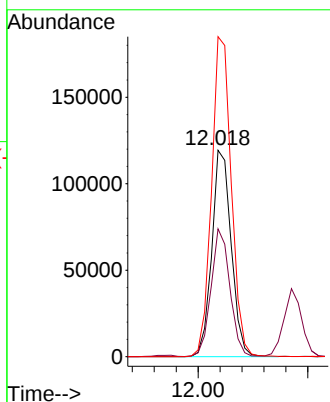


#73
Isopropylbenzene
Concen: 6.037 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58

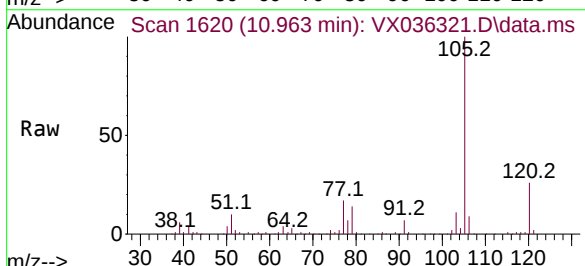

Tgt Ion:105 Resp: 66706
Ion Ratio Lower Upper
105 100
120 26.6 12.9 38.6

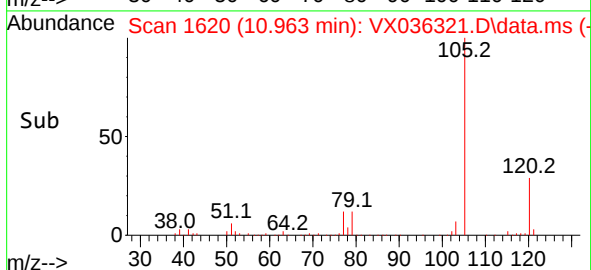







#78
n-propylbenzene
Concen: 9.352 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58

Instrument :
MSVOA_X
ClientSampleId :
MW-12

Tgt Ion: 91 Resp: 120688
Ion Ratio Lower Upper
91 100
120 23.0 11.5 34.4




Manual Integrations
APPROVED


Reviewed By :John Carlone 06/26/2023
Supervised By :Mahesh Dadoda 06/26/2023

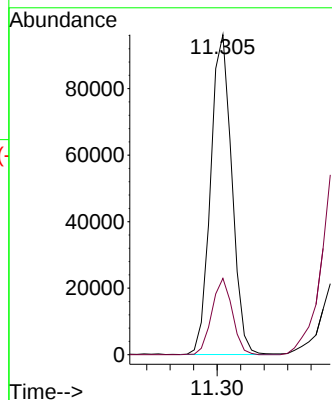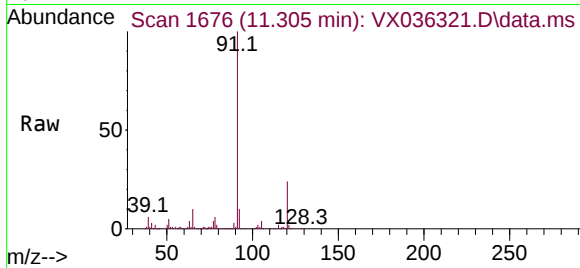

#80
1,3,5-Trimethylbenzene
Concen: 18.934 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58


Tgt Ion:105 Resp: 177194
Ion Ratio Lower Upper
105 100
120 49.1 24.1 72.3

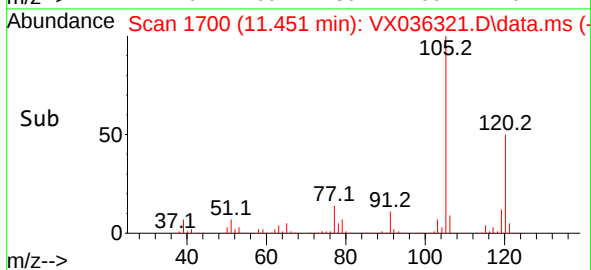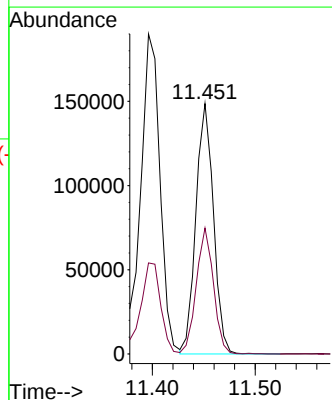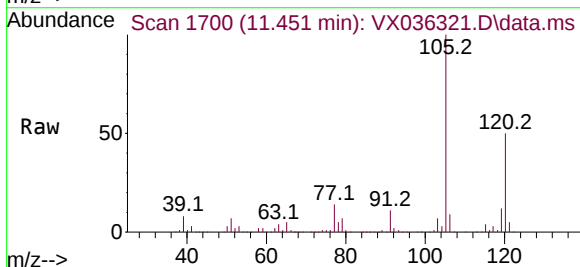



#82
4-Chlorotoluene
Concen: 2.174 ug/l m
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58




Instrument :
MSVOA_X
ClientSampleId :
MW-12

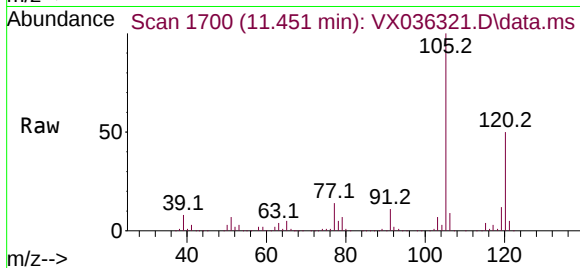

Tgt Ion: 91 Resp: 1943
Ion Ratio Lower Upper
91 100
126 0.0 14.2 42.6




Manual Integrations
APPROVED


Reviewed By :John Carlone 06/26/2023
Supervised By :Mahesh Dadoda 06/26/2023

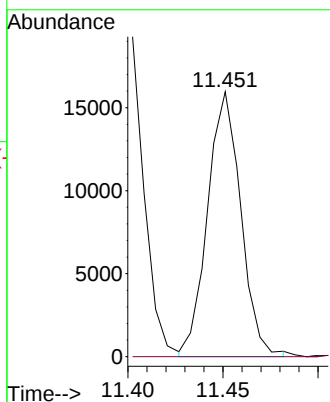

#84
1,2,4-Trimethylbenzene
Concen: 50.569 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58


Tgt Ion:105 Resp: 468193
Ion Ratio Lower Upper
105 100
120 45.0 21.2 63.6

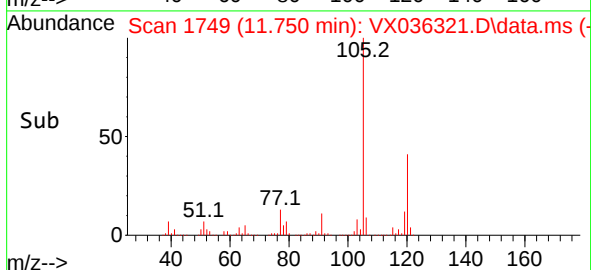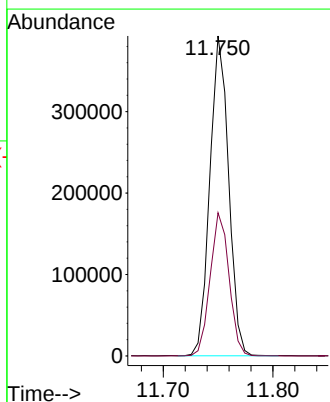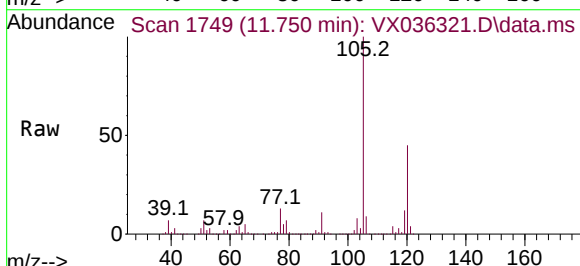



#85
 sec-Butylbenzene
 Concen: 0.707 ug/l m
 RT: 11.890 min Scan# 1772
 Delta R.T. 0.000 min
 Lab File: VX036321.D
 Acq: 24 Jun 2023 18:58




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-12




Tgt Ion:105 Resp: 8034
 Ion Ratio Lower Upper
 105 100
 134 0.0 9.8 29.4

Manual Integrations
 APPROVED



Reviewed By :John Carlone 06/26/2023
 Supervised By :Mahesh Dadoda 06/26/2023




#86
 p-Isopropyltoluene
 Concen: 0.826 ug/l
 RT: 12.006 min Scan# 1791
 Delta R.T. -0.000 min
 Lab File: VX036321.D
 Acq: 24 Jun 2023 18:58

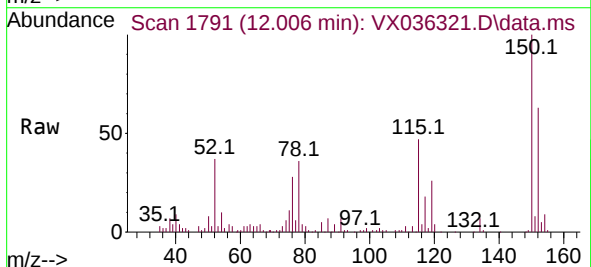

Tgt Ion:119 Resp: 7873
 Ion Ratio Lower Upper
 119 100
 134 27.2 12.8 38.3
 91 0.0 13.1 39.3

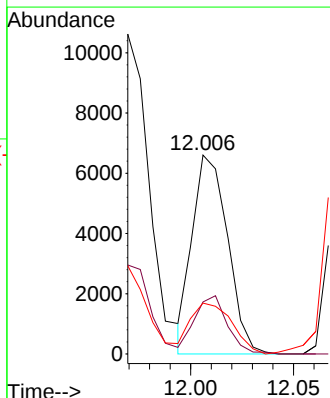







#90
Hexachloroethane
Concen: 4.441 ug/l m
RT: 12.530 min Scan# 117
Delta R.T. -0.006 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58

Instrument :
MSVOA_X
ClientSampleId :
MW-12

Tgt Ion:117 Resp: 6414
Ion Ratio Lower Upper
117 100
201 0.0 32.9 98.6

Manual Integrations
APPROVED

Reviewed By :John Carlone 06/26/2023
Supervised By :Mahesh Dadoda 06/26/2023

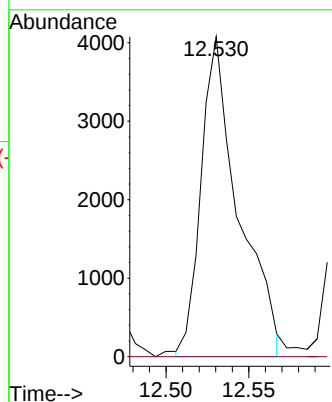

#95
Naphthalene
Concen: 24.103 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX036321.D
Acq: 24 Jun 2023 18:58

Tgt Ion:128 Resp: 241269
Ion Ratio Lower Upper
128 100
127 13.1 10.3 15.5
129 10.9 8.8 13.2

