

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX062423\  
Data File : VX036307.D  
Acq On : 24 Jun 2023 13:30  
Operator : JC/MD  
Sample : 03375-09  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
FB-5-062123

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X062323W.M

Title : SW846 8260

Signal : TIC: VX036307.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.385       | 693           | 705         | 721          | rBV2     | 113626         | 336787        | 33.43%          | 6.238%        |
| 2         | 5.550       | 721           | 732         | 752          | rVB      | 200867         | 563905        | 55.97%          | 10.444%       |
| 3         | 5.958       | 789           | 799         | 814          | rBV      | 137670         | 368713        | 36.60%          | 6.829%        |
| 4         | 6.763       | 921           | 931         | 944          | rBV      | 319682         | 754518        | 74.89%          | 13.974%       |
| 5         | 8.647       | 1233          | 1240        | 1250         | rBV      | 650500         | 1007484       | 100.00%         | 18.659%       |
| 6         | 10.055      | 1465          | 1471        | 1485         | rBV      | 658439         | 884956        | 87.84%          | 16.390%       |
| 7         | 11.079      | 1634          | 1639        | 1652         | rBV      | 514178         | 656484        | 65.16%          | 12.159%       |
| 8         | 12.018      | 1788          | 1793        | 1804         | rBV      | 663790         | 826473        | 82.03%          | 15.307%       |




Sum of corrected areas: 5399320

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX062423\  
Data File : VX036307.D  
Acq On : 24 Jun 2023 13:30  
Operator : JC/MD  
Sample : 03375-09  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
FB-5-062123

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X062323W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

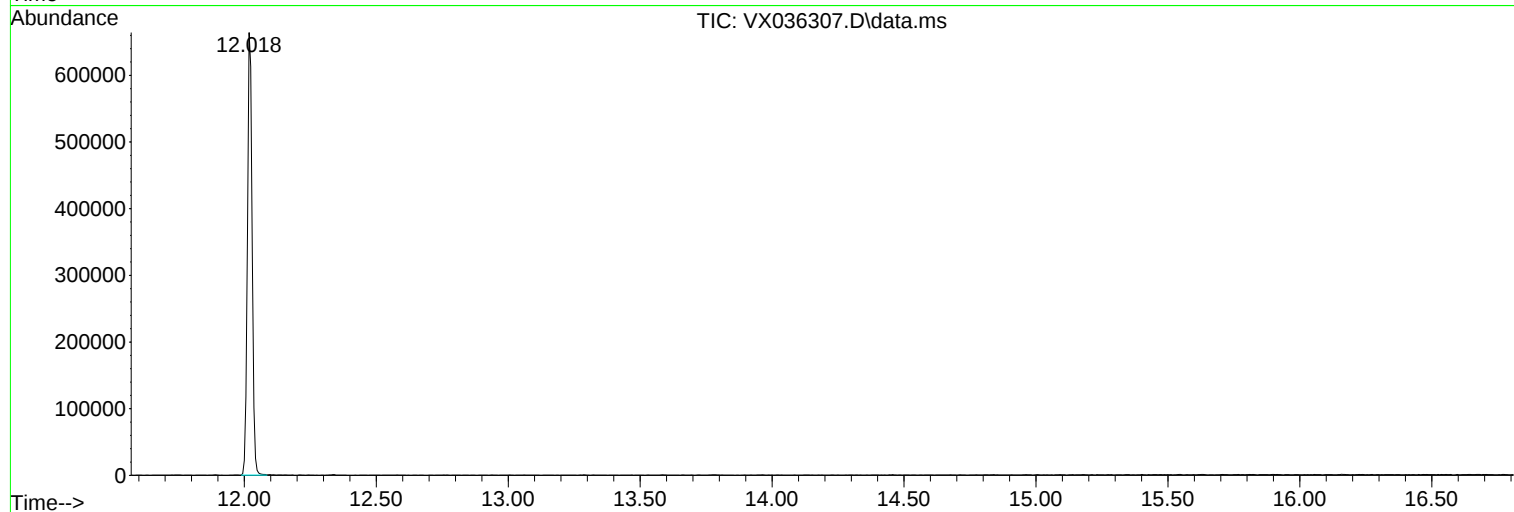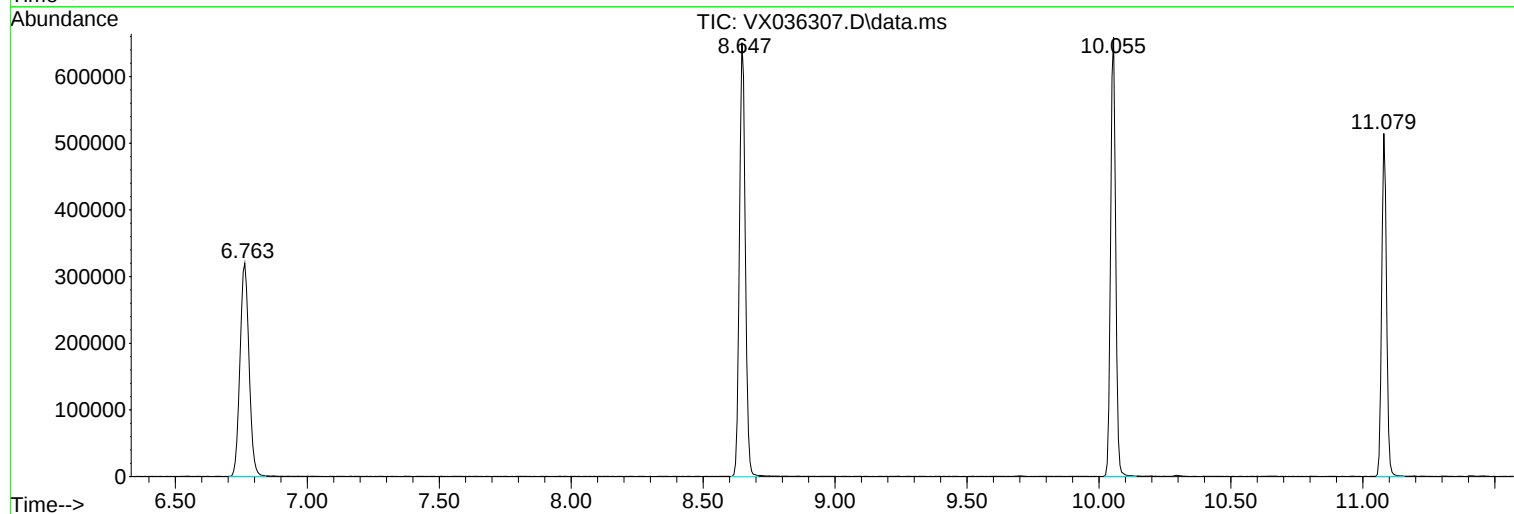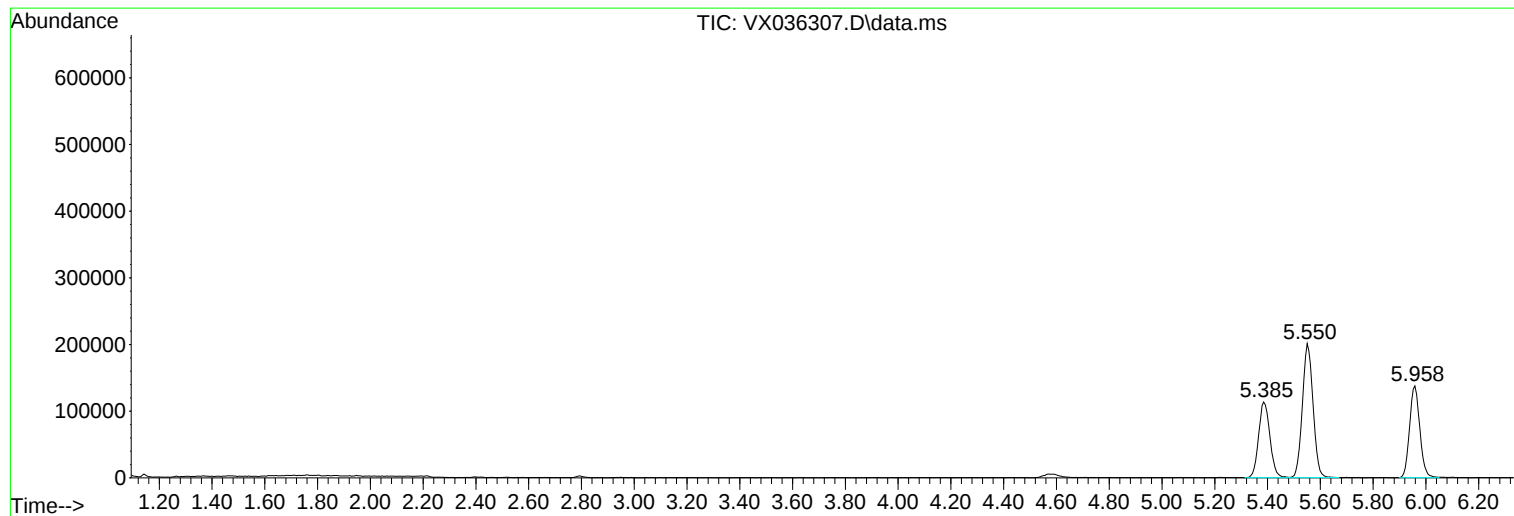

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX062423\  
Data File : VX036307.D  
Acq On : 24 Jun 2023 13:30  
Operator : JC/MD  
Sample : 03375-09  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
FB-5-062123

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X062323W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX062423\  
Data File : VX036307.D  
Acq On : 24 Jun 2023 13:30  
Operator : JC/MD  
Sample : 03375-09  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
FB-5-062123

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X062323W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|