

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062423\
Data File : VX036312.D
Acq On : 24 Jun 2023 15:27
Operator : JC/MD
Sample : 03408-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-062323

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M

Title : SW846 8260

Signal : TIC: VX036312.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	694	705	720	rBV	141447	409371	33.29%	6.394%
2	5.550	722	732	751	rVB	227882	645657	52.51%	10.085%
3	5.952	788	798	813	rBV	169697	451457	36.71%	7.051%
4	6.763	921	931	948	rBV	375321	892044	72.55%	13.933%
5	8.647	1234	1240	1254	rBV	790750	1229633	100.00%	19.206%
6	10.055	1465	1471	1488	rBV	793381	1049937	85.39%	16.399%
7	11.079	1634	1639	1651	rBV	618515	789903	64.24%	12.338%
8	12.018	1788	1793	1804	rBV	737039	934332	75.98%	14.594%




Sum of corrected areas: 6402334

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062423\
Data File : VX036312.D
Acq On : 24 Jun 2023 15:27
Operator : JC/MD
Sample : 03408-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-062323

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

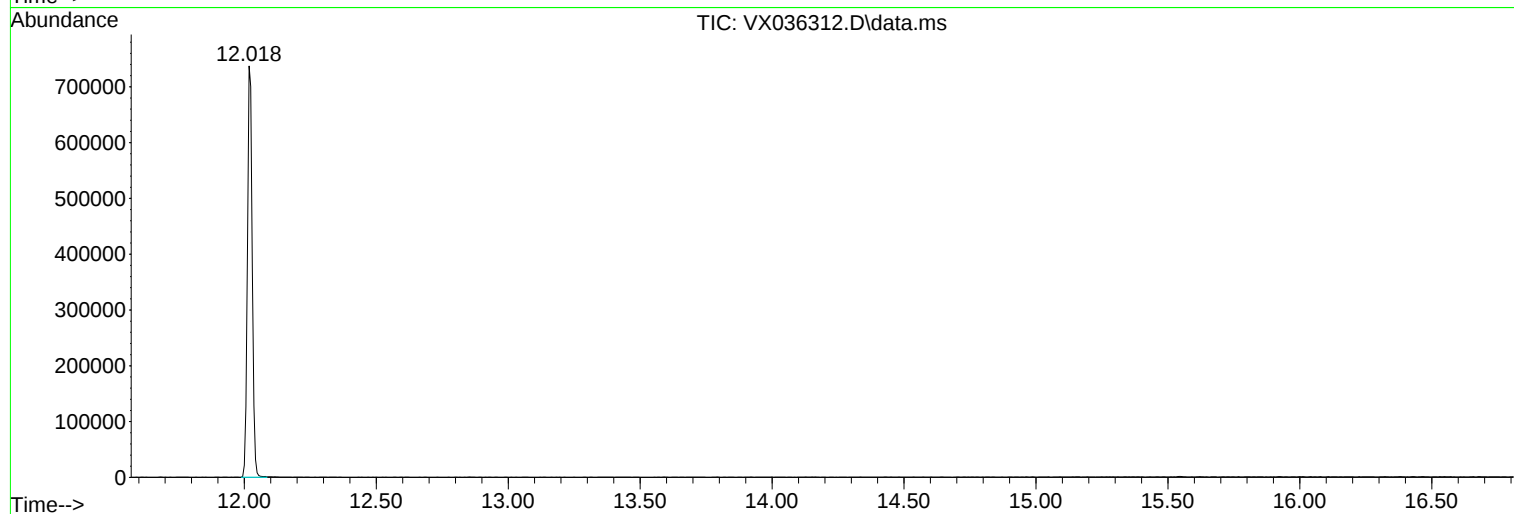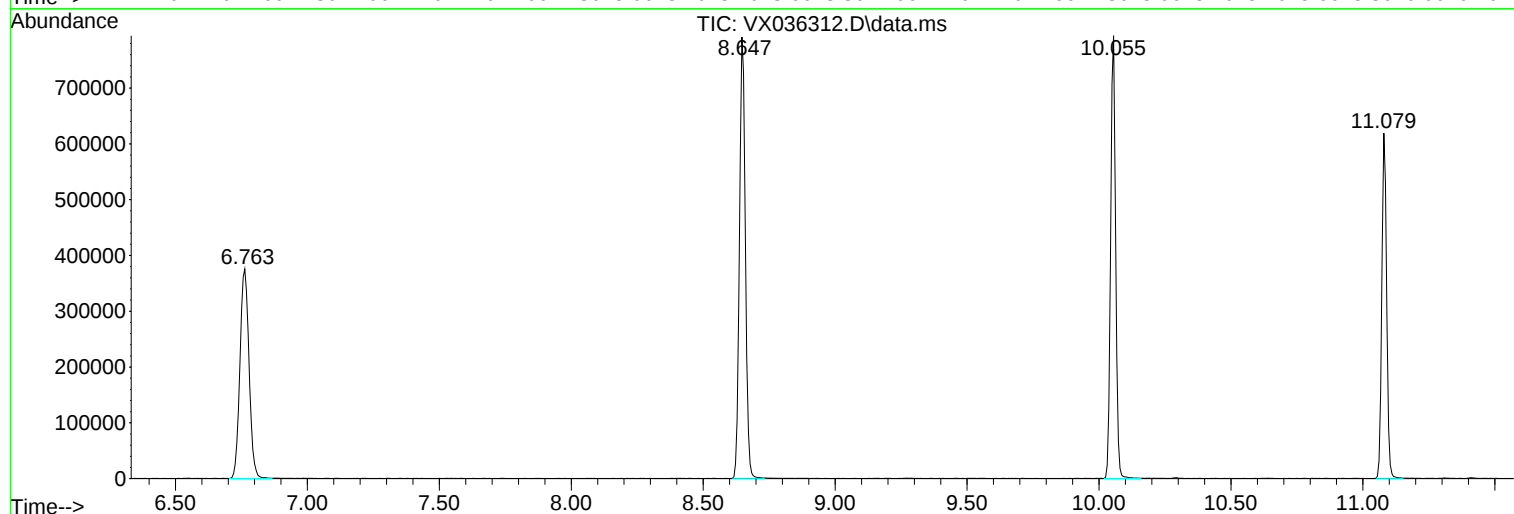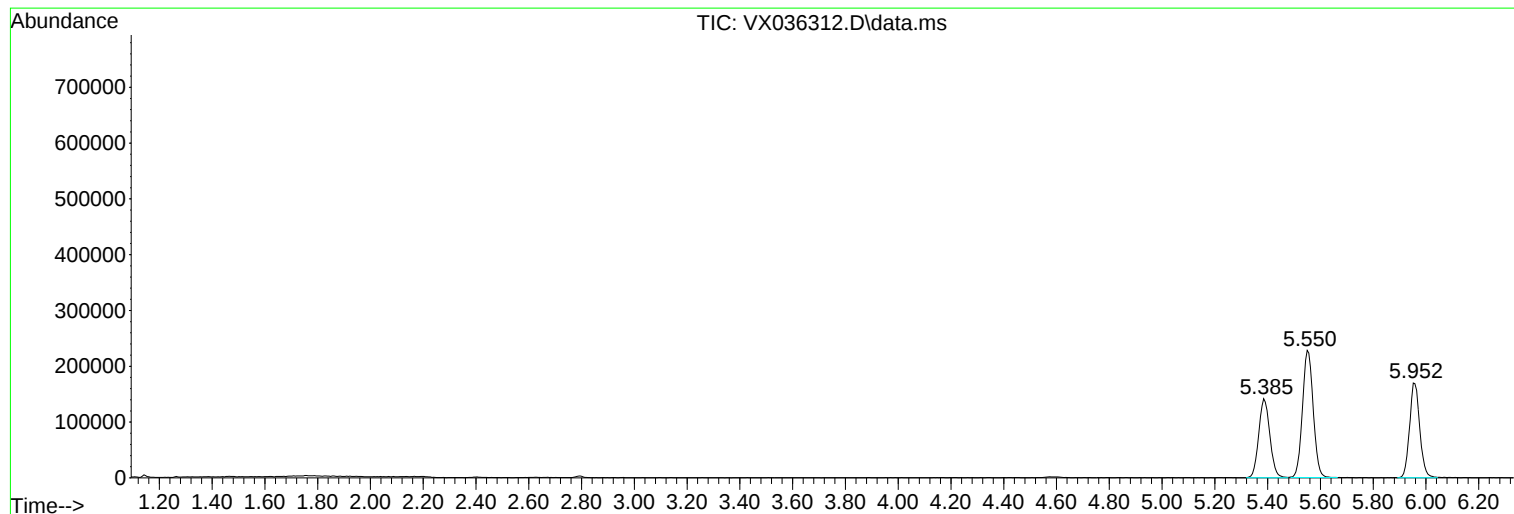

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062423\
Data File : VX036312.D
Acq On : 24 Jun 2023 15:27
Operator : JC/MD
Sample : 03408-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-062323

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062423\
Data File : VX036312.D
Acq On : 24 Jun 2023 15:27
Operator : JC/MD
Sample : 03408-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-062323

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------