

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062424\
 Data File : VX042015.D
 Acq On : 24 Jun 2024 19:24
 Operator : JC/MD
 Sample : P3027-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 240620099-03

Quant Time: Jun 25 06:47:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X061424W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Sat Jun 15 04:02:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	4.904	128	27874	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	6.763	114	147318	30.000	ug/l	0.00
57) Chlorobenzene-d5	10.055	117	132793	30.000	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	5.958	65	57670	30.055	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	100.167%
60) 4-Bromofluorobenzene	11.079	95	55311	26.908	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	89.700%
63) Toluene-d8	8.647	98	170902	30.081	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	100.267%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062424\
Data File : VX042015.D
Acq On : 24 Jun 2024 19:24
Operator : JC/MD
Sample : P3027-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
240620099-03

Quant Time: Jun 25 06:47:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X061424W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Sat Jun 15 04:02:59 2024
Response via : Initial Calibration




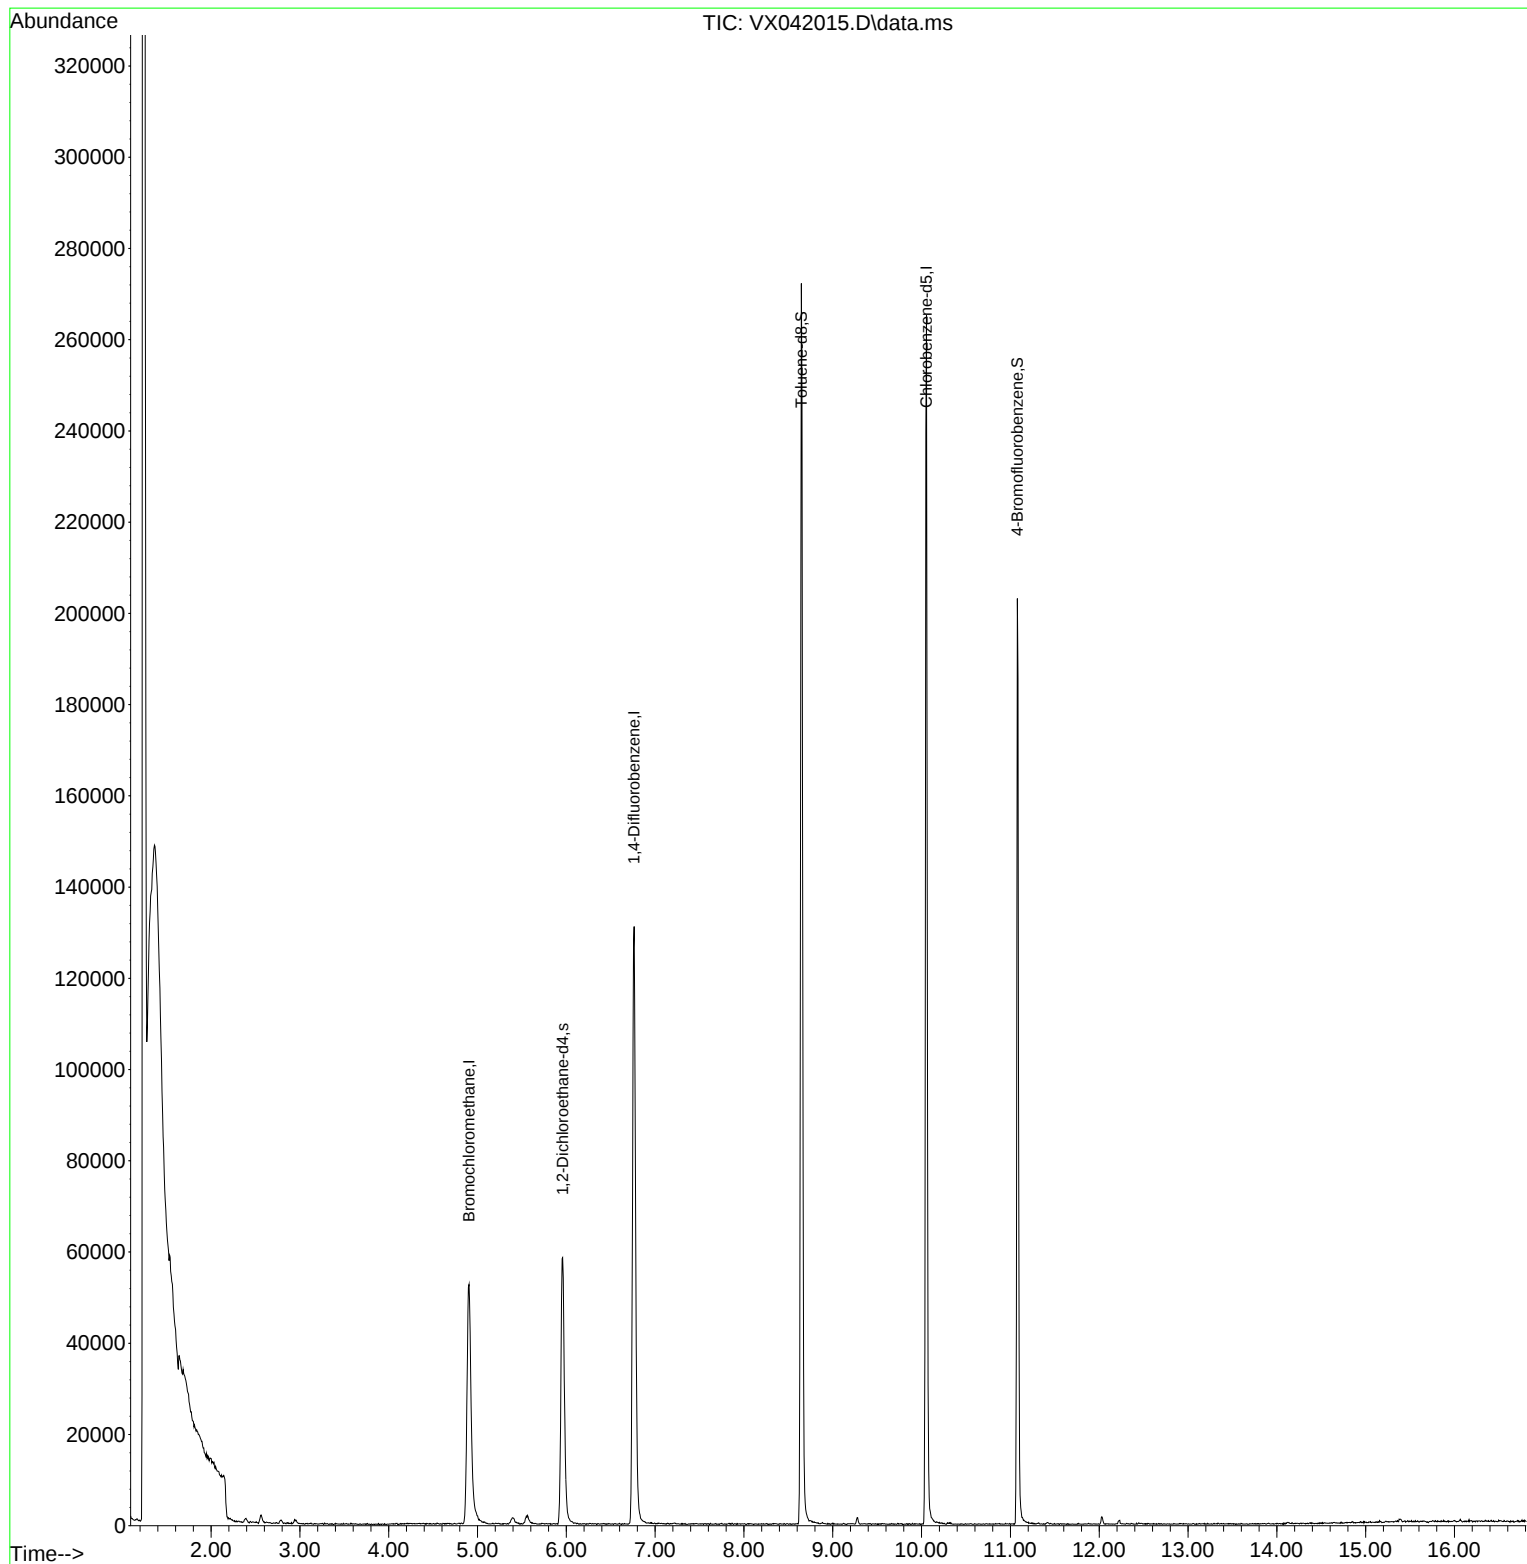


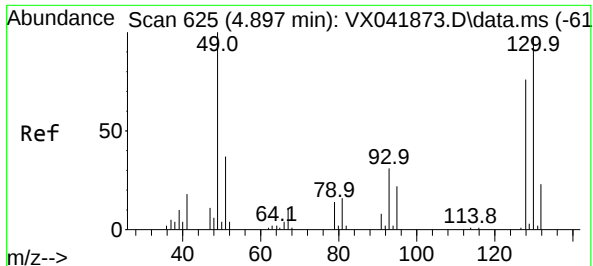

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 4.904 min Scan# 61
Delta R.T. 0.007 min
Lab File: VX042015.D
Acq: 24 Jun 2024 19:24




Instrument :
MSVOA_X
ClientSampleId :
240620099-03


Tgt Ion:128 Resp: 27874
Ion Ratio Lower Upper
128 100
49 137.8 0.0 338.5
130 133.5 0.0 324.5

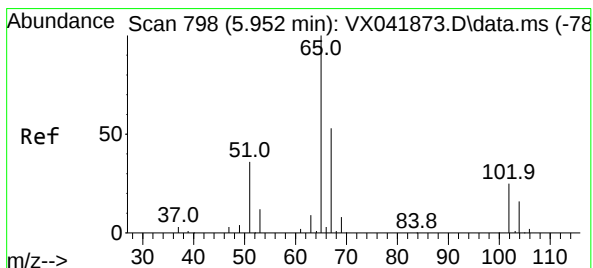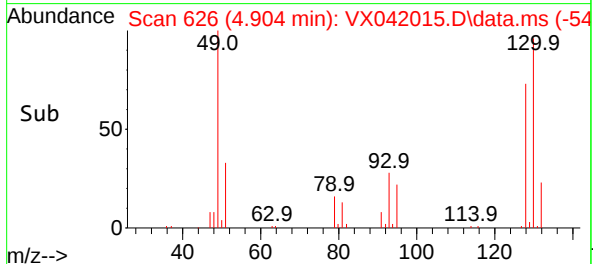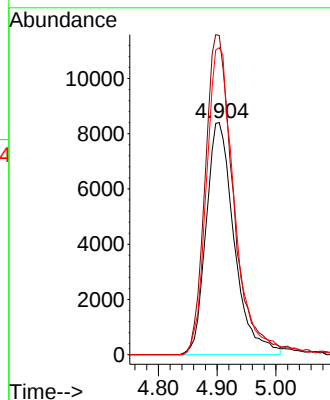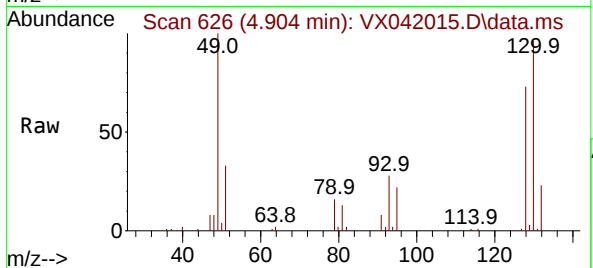

#27
1,2-Dichloroethane-d4
Concen: 30.055 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.006 min
Lab File: VX042015.D
Acq: 24 Jun 2024 19:24

Tgt Ion: 65 Resp: 57670
Ion Ratio Lower Upper
65 100
67 53.5 43.4 65.0

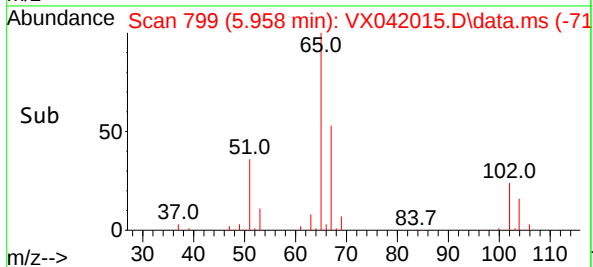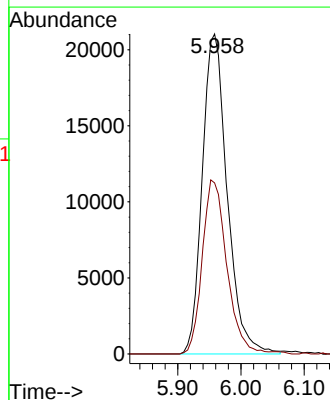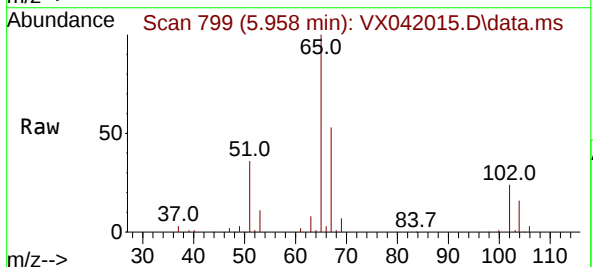

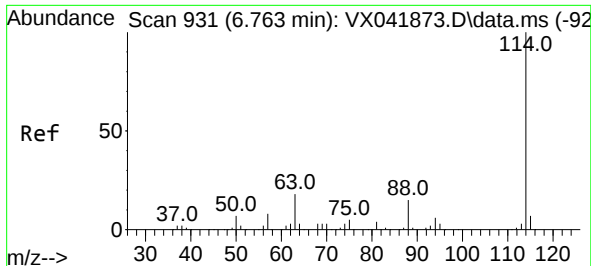

#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 6.763 min Scan# 91

Delta R.T. 0.000 min

Lab File: VX042015.D

Acq: 24 Jun 2024 19:24

Instrument :

MSVOA_X

ClientSampleId :

240620099-03





Tgt Ion:114 Resp: 147318

Ion Ratio Lower Upper

114 100

63 18.2 14.6 21.8

88 14.7 11.8 17.8

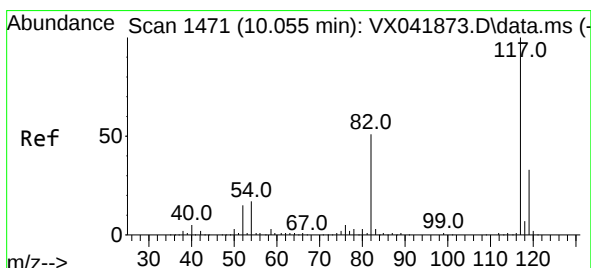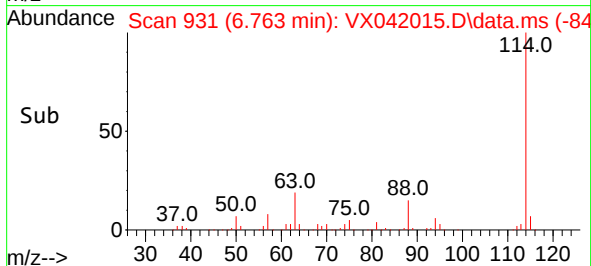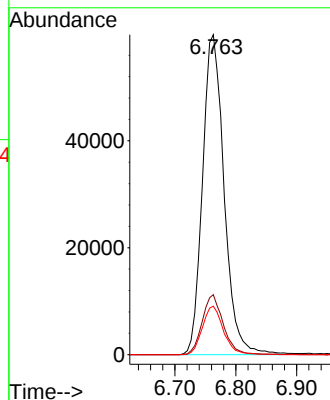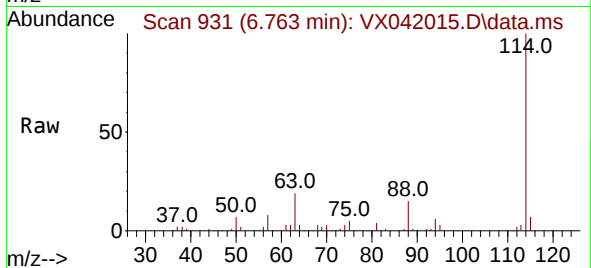

#57

Chlorobenzene-d5

Concen: 30.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX042015.D

Acq: 24 Jun 2024 19:24




Tgt Ion:117 Resp: 132793


Ion Ratio Lower Upper

117 100

82 51.9 41.1 61.7

119 32.6 26.1 39.1


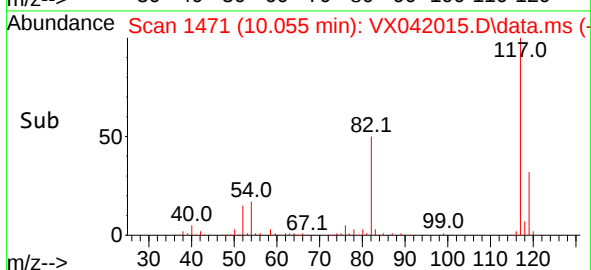
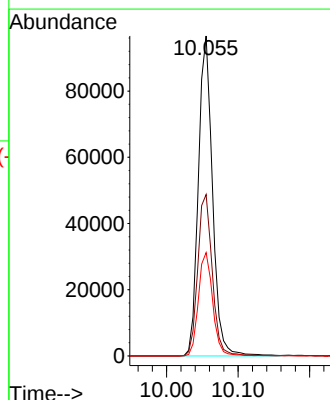
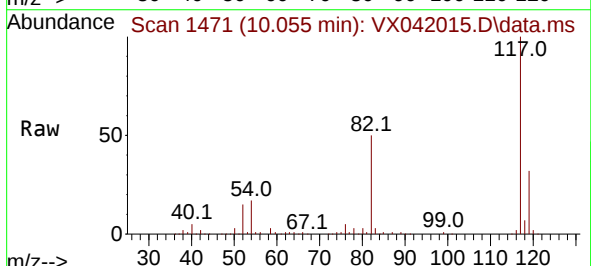


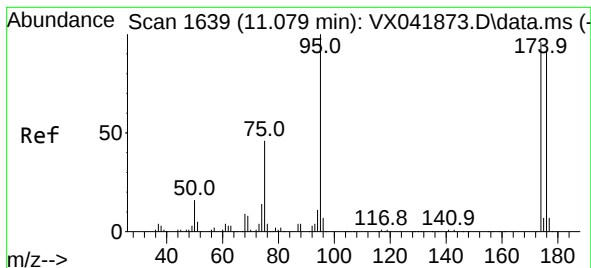

#60
4-Bromofluorobenzene
Concen: 26.908 ug/l
RT: 11.079 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX042015.D
Acq: 24 Jun 2024 19:24

Instrument :
MSVOA_X
ClientSampleId :
240620099-03

Tgt Ion: 95 Resp: 55311
Ion Ratio Lower Upper
95 100
174 96.2 78.9 118.3
176 93.7 77.1 115.7

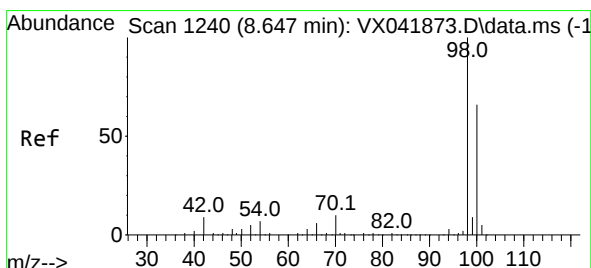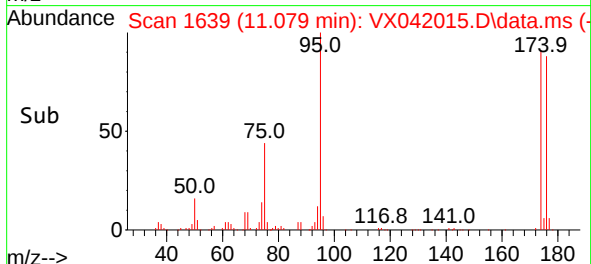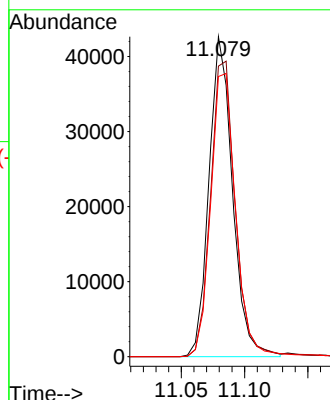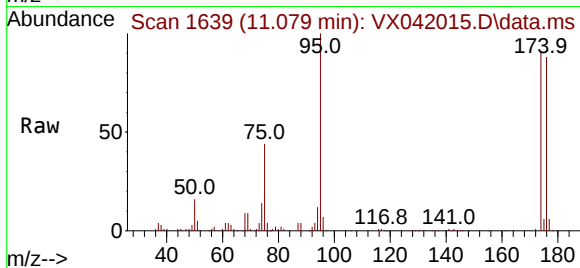

#63
Toluene-d8
Concen: 30.081 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX042015.D
Acq: 24 Jun 2024 19:24

Tgt Ion: 98 Resp: 170902
Ion Ratio Lower Upper
98 100
100 65.8 52.7 79.1

