

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX062424\  
Data File : VX042013.D  
Acq On : 24 Jun 2024 18:37  
Operator : JC/MD  
Sample : P3024-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
240620102-01

Integration Parameters: RTEINT3.P  
Integrator: RTE  
Smoothing : OFF Filtering: 5  
Sampling : 1 Min Area: 0 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\624X061424W.M  
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC: VX042013.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.587       | 70            | 82          | 83           | rBV5     | 4633           | 11526         | 2.57%           | 0.633%        |
| 2         | 1.617       | 85            | 87          | 93           | rVB3     | 5015           | 7919          | 1.76%           | 0.435%        |
| 3         | 4.903       | 615           | 626         | 645          | rBV2     | 55833          | 180737        | 40.28%          | 9.931%        |
| 4         | 5.397       | 696           | 707         | 717          | rBV3     | 1639           | 4800          | 1.07%           | 0.264%        |
| 5         | 5.958       | 790           | 799         | 816          | rBV      | 62207          | 168627        | 37.58%          | 9.265%        |
| 6         | 6.763       | 922           | 931         | 949          | rBV      | 139496         | 336983        | 75.09%          | 18.516%       |
| 7         | 8.647       | 1234          | 1240        | 1256         | rBV      | 281120         | 448749        | 100.00%         | 24.657%       |
| 8         | 10.055      | 1465          | 1471        | 1482         | rBV      | 271482         | 380902        | 84.88%          | 20.929%       |
| 9         | 11.079      | 1634          | 1639        | 1655         | rBV      | 205321         | 279717        | 62.33%          | 15.369%       |




Sum of corrected areas: 1819960

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX062424\  
Data File : VX042013.D  
Acq On : 24 Jun 2024 18:37  
Operator : JC/MD  
Sample : P3024-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
240620102-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\624X061424W.M  
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

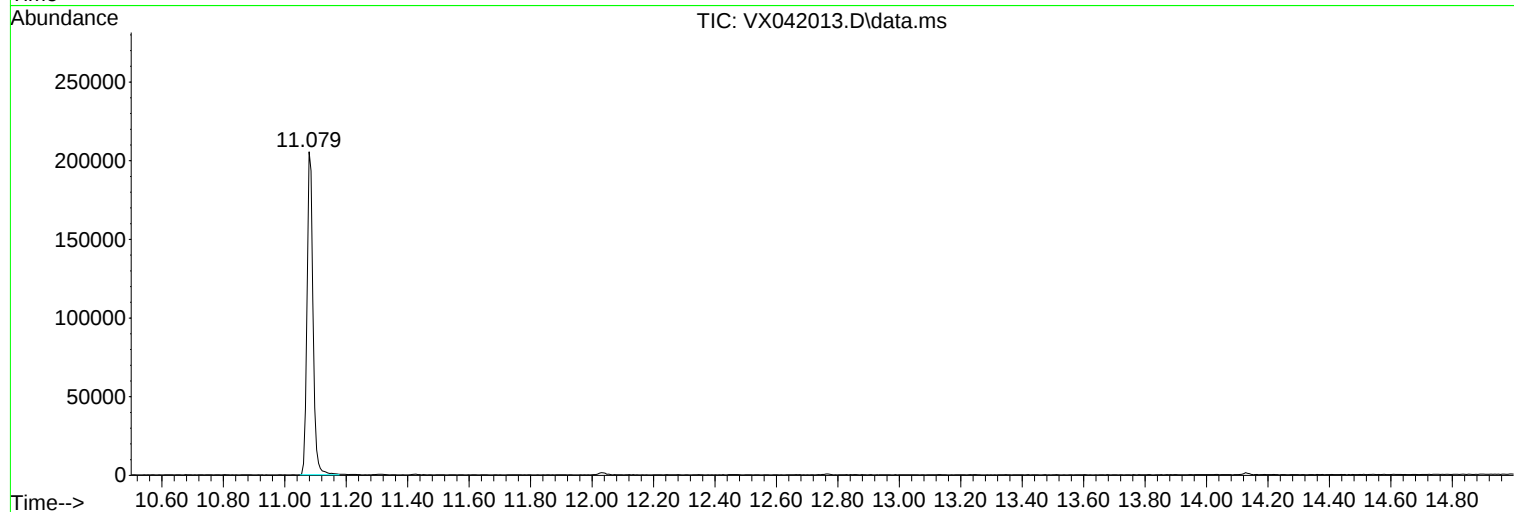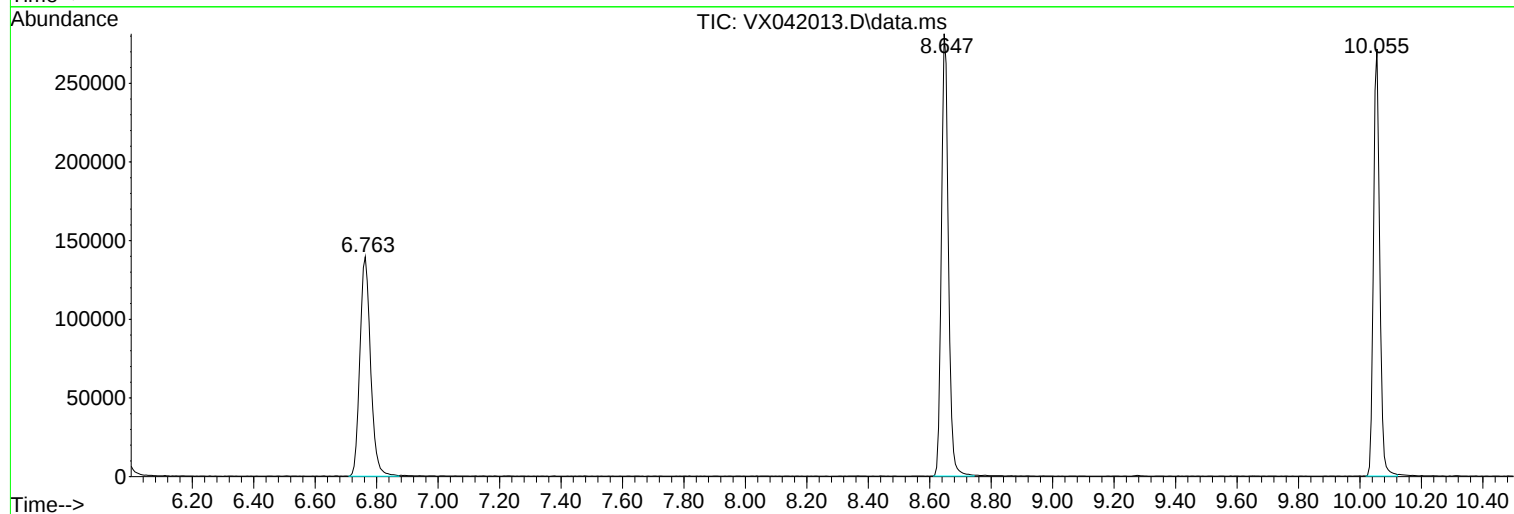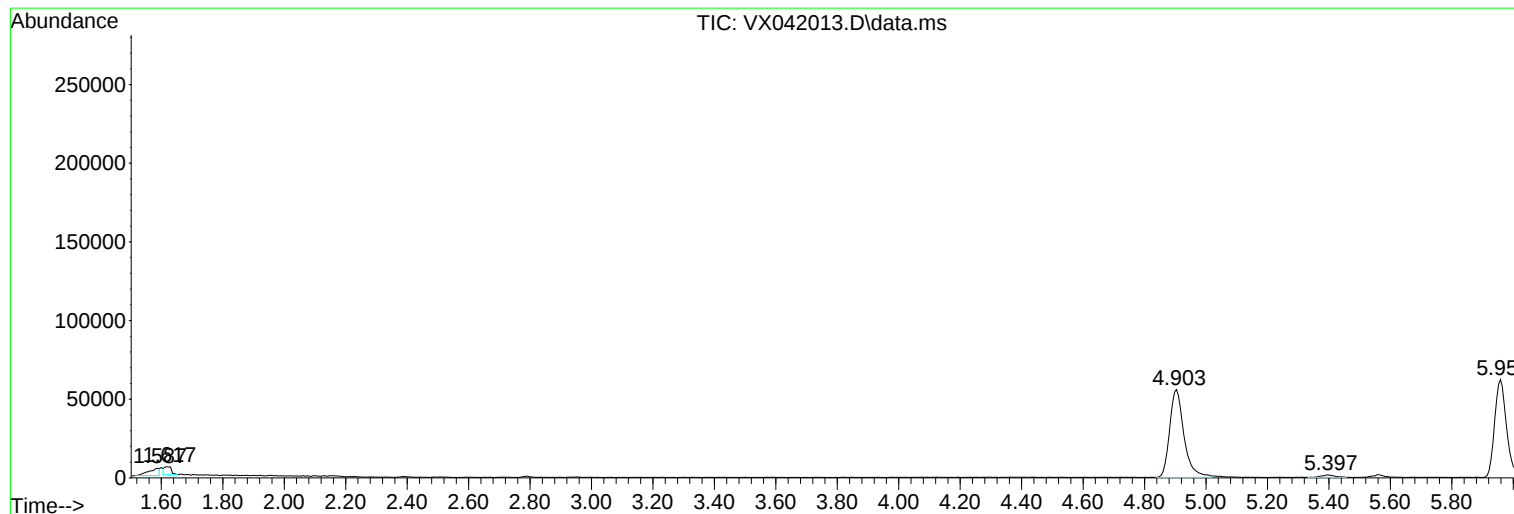

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX062424\  
Data File : VX042013.D  
Acq On : 24 Jun 2024 18:37  
Operator : JC/MD  
Sample : P3024-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
240620102-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\624X061424W.M  
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX062424\  
Data File : VX042013.D  
Acq On : 24 Jun 2024 18:37  
Operator : JC/MD  
Sample : P3024-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
240620102-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\624X061424W.M  
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|