
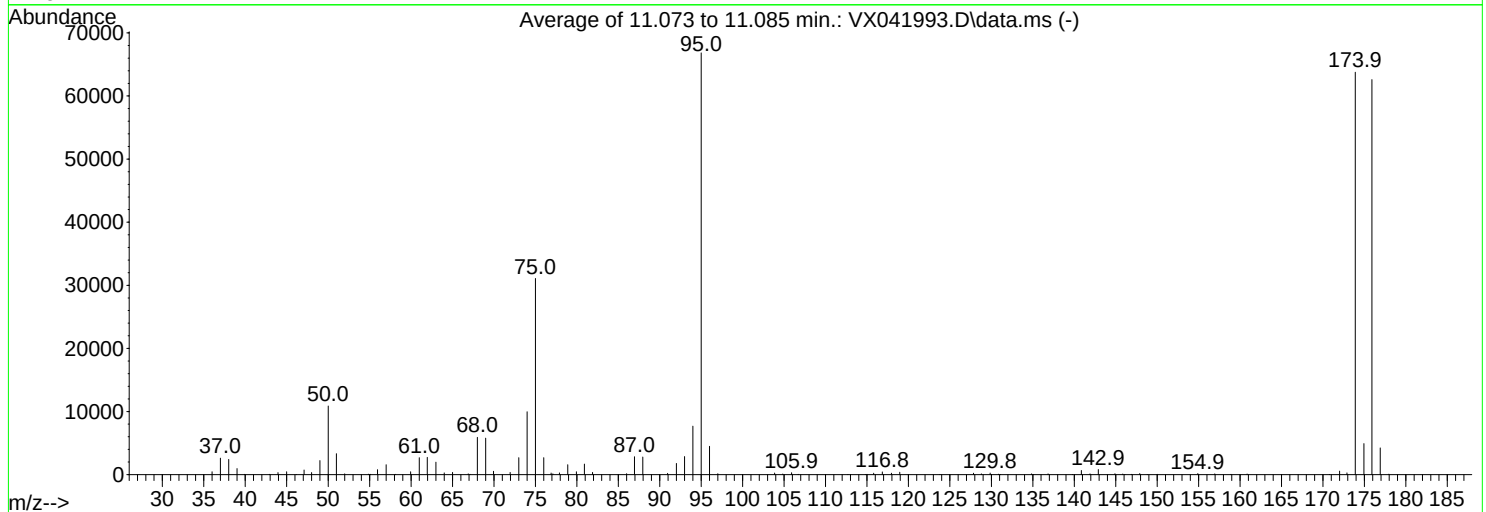


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062424\
Data File : VX041993.D
Acq On : 24 Jun 2024 08:40
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Title : SW846 8260
Last Update : Fri Jun 21 23:51:58 2024

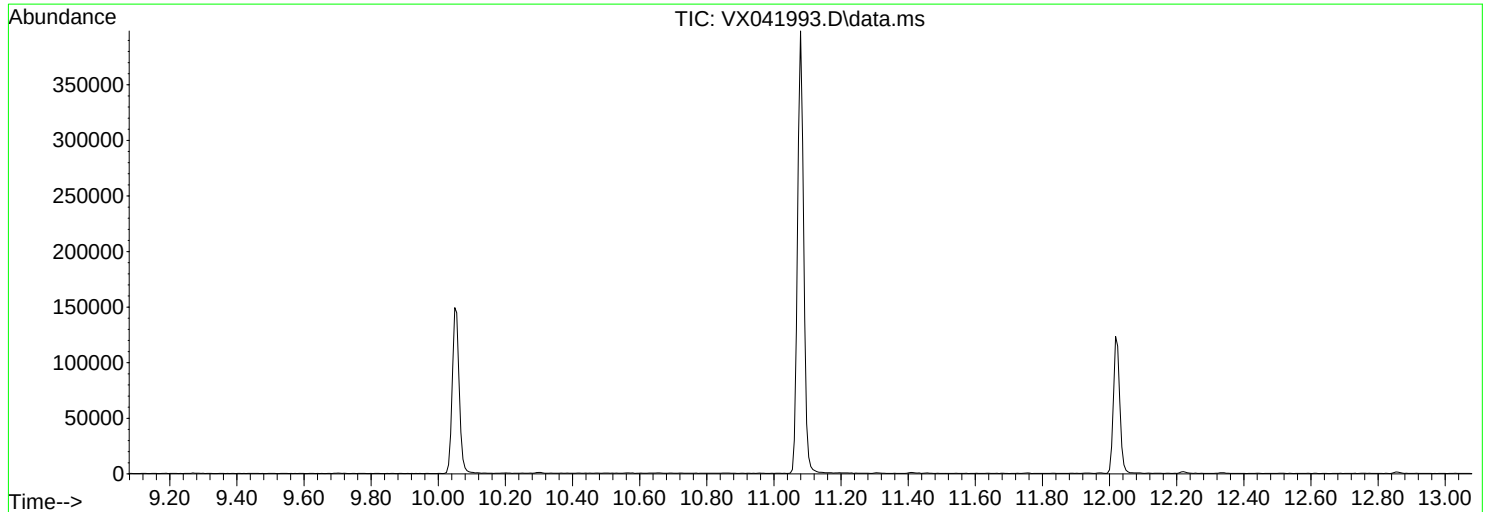

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.3	10891	PASS
75	95	30	60	46.5	31083	PASS
95	95	100	100	100.0	66837	PASS
96	95	5	9	6.7	4502	PASS
173	174	0.00	2	0.4	274	PASS
174	95	50	100	95.4	63757	PASS
175	174	5	9	7.7	4910	PASS
176	174	95	101	98.2	62603	PASS
177	176	5	9	6.8	4244	PASS