



Dichlorodifluoromethane

Response Ratio

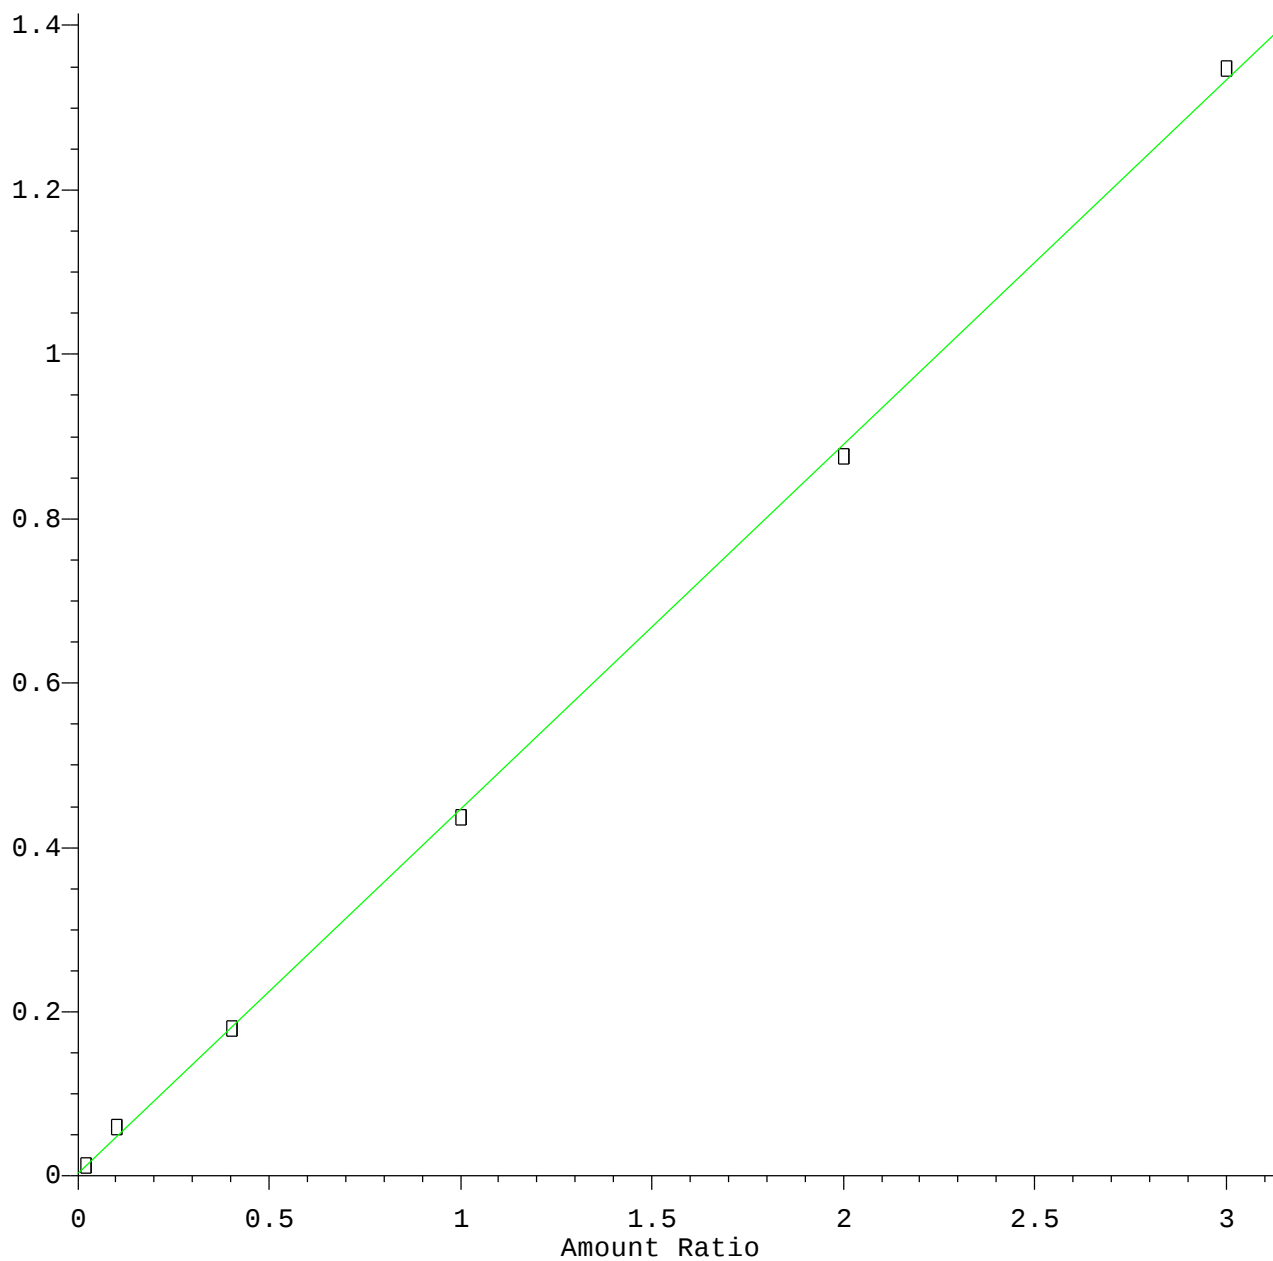


Resp Ratio = $4.44 \times 10^{-1} \times \text{Amt} + 2.68 \times 10^{-3}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Calibration Table Last Updated: Mon Jun 25 14:38:05 2018

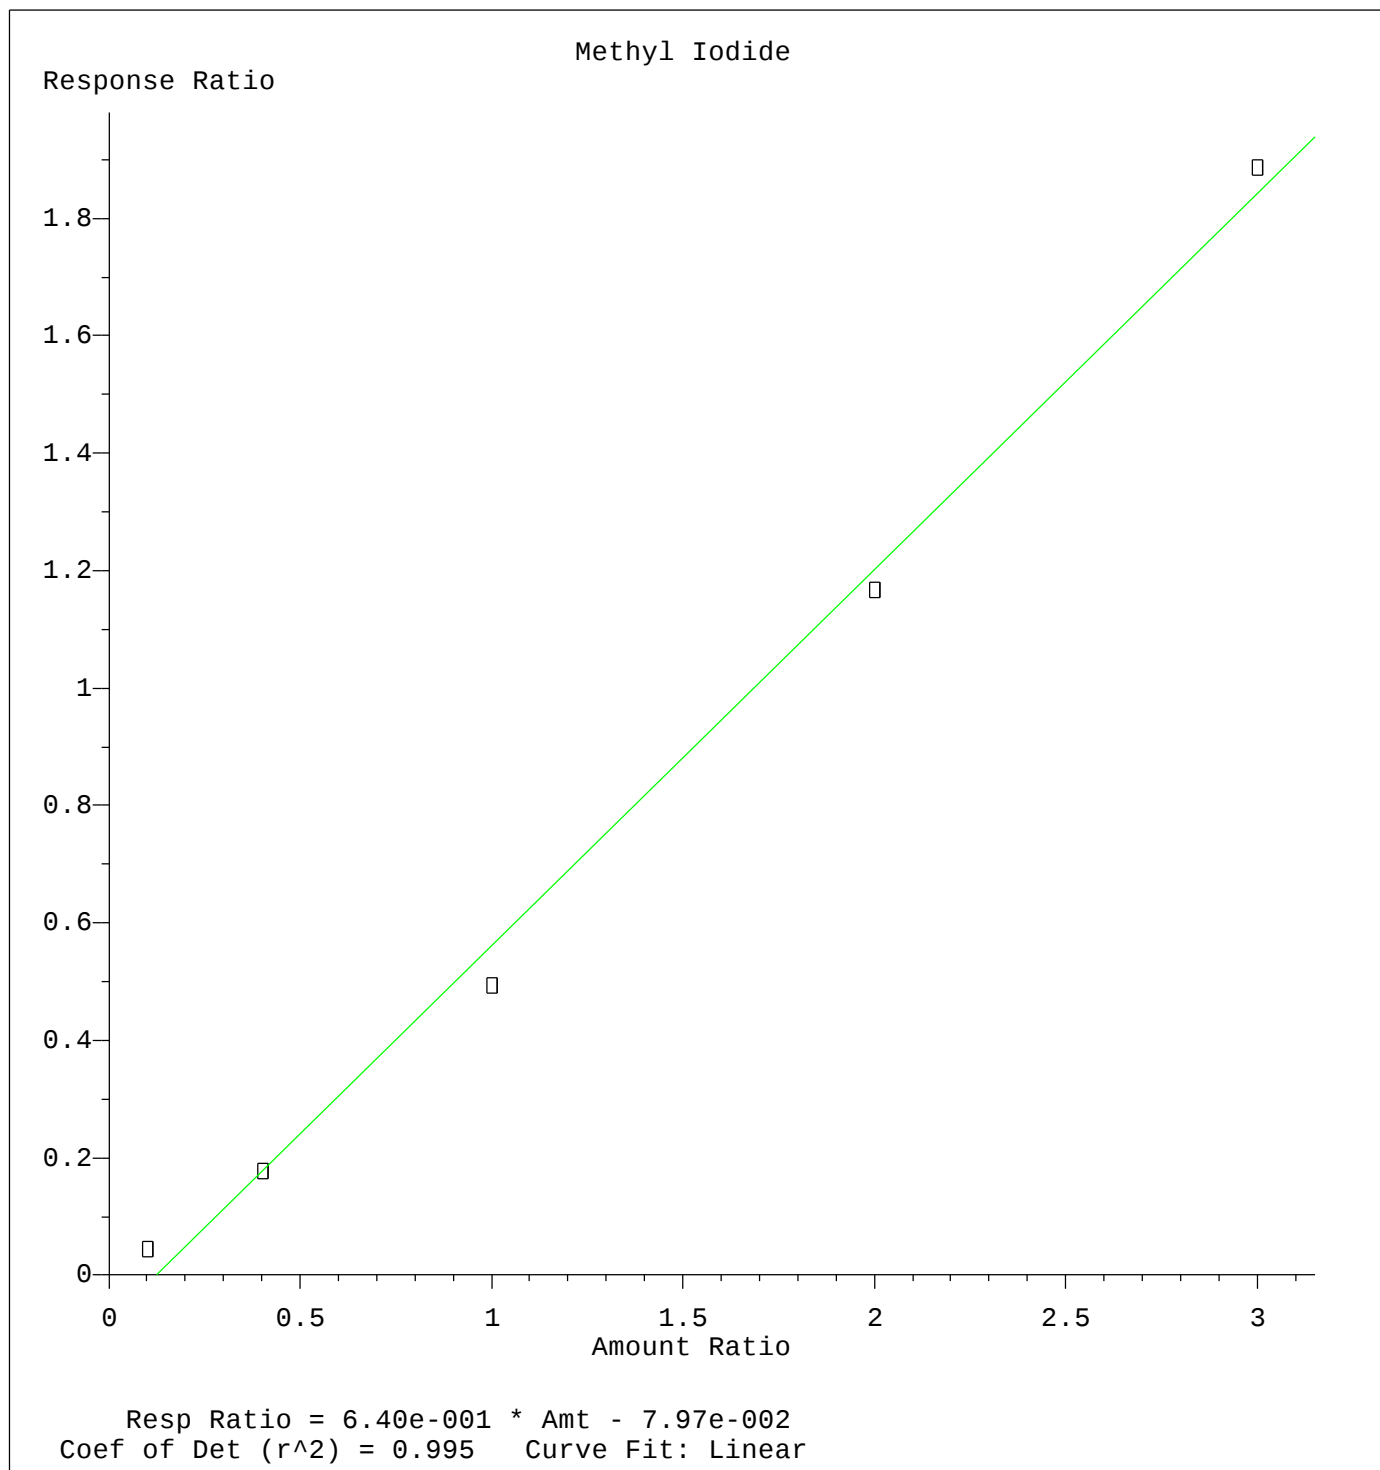


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Calibration Table Last Updated: Mon Jun 25 14:38:05 2018

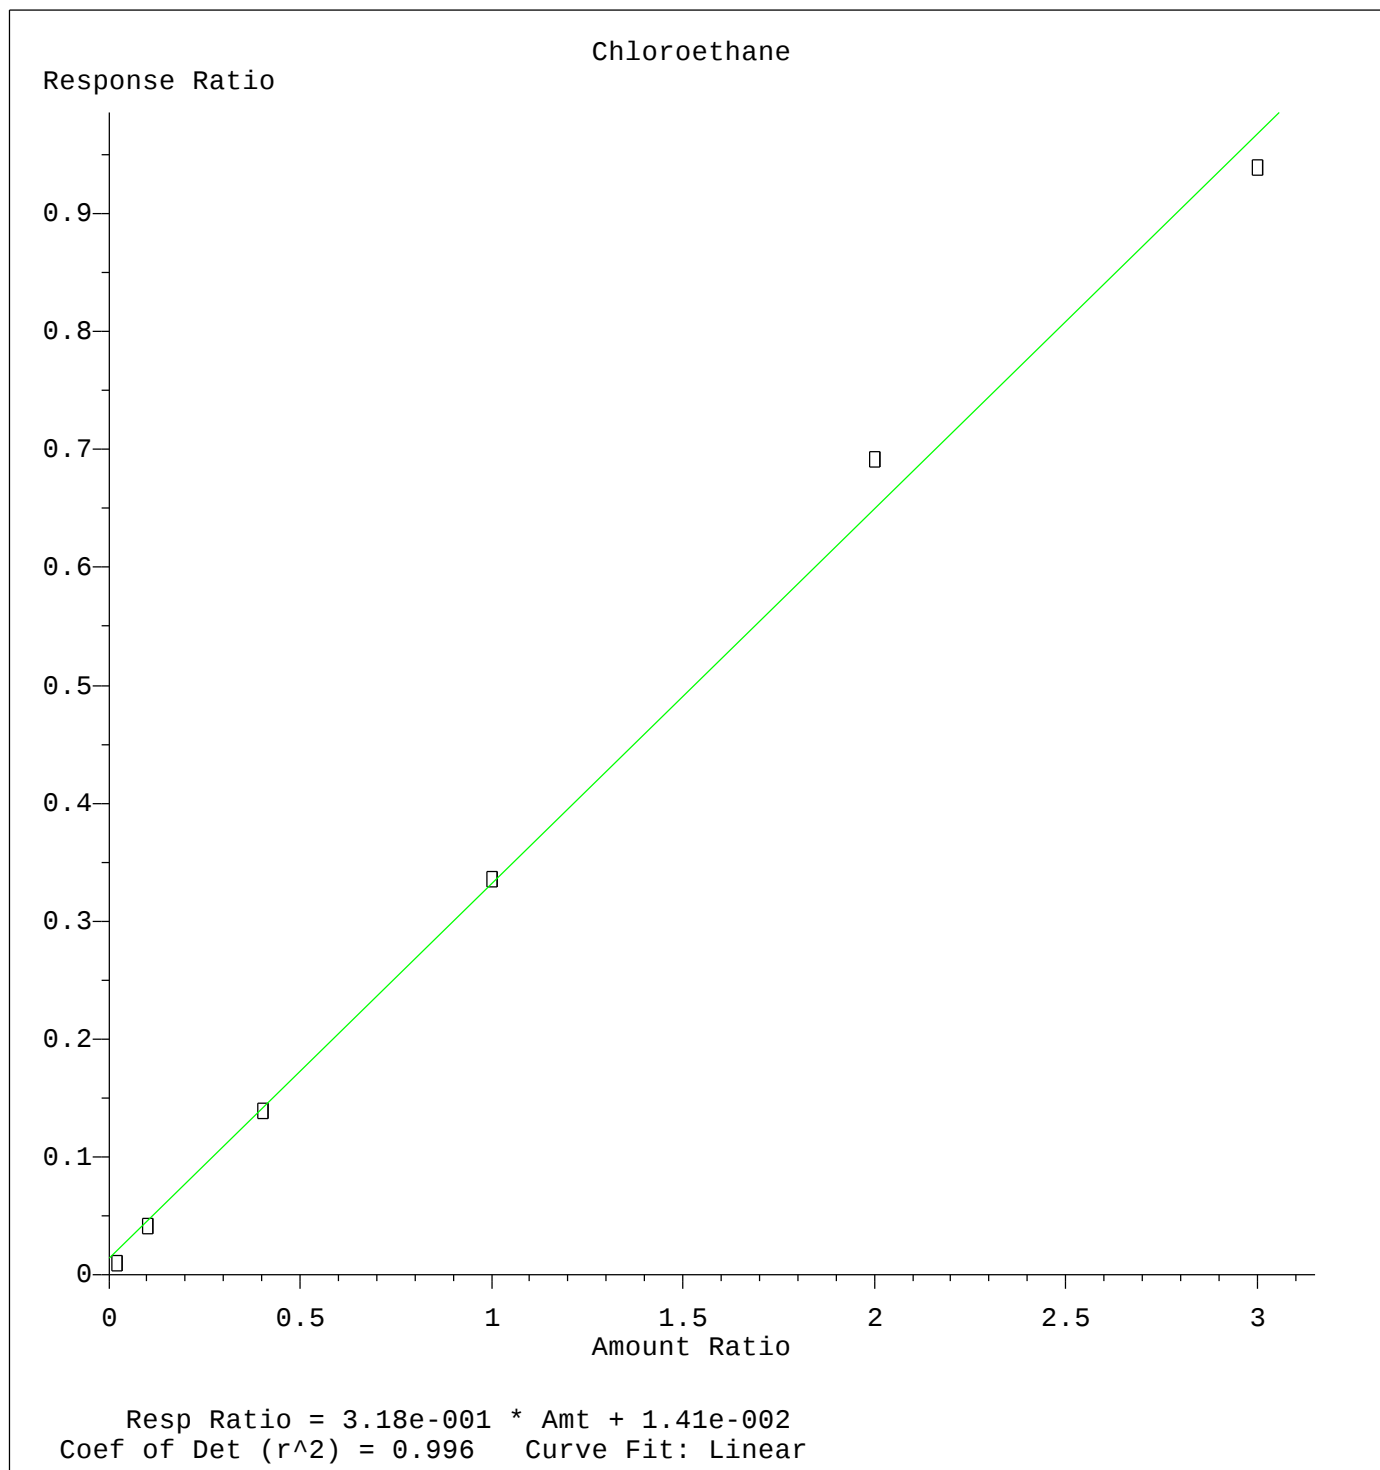

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Calibration Table Last Updated: Mon Jun 25 14:38:05 2018

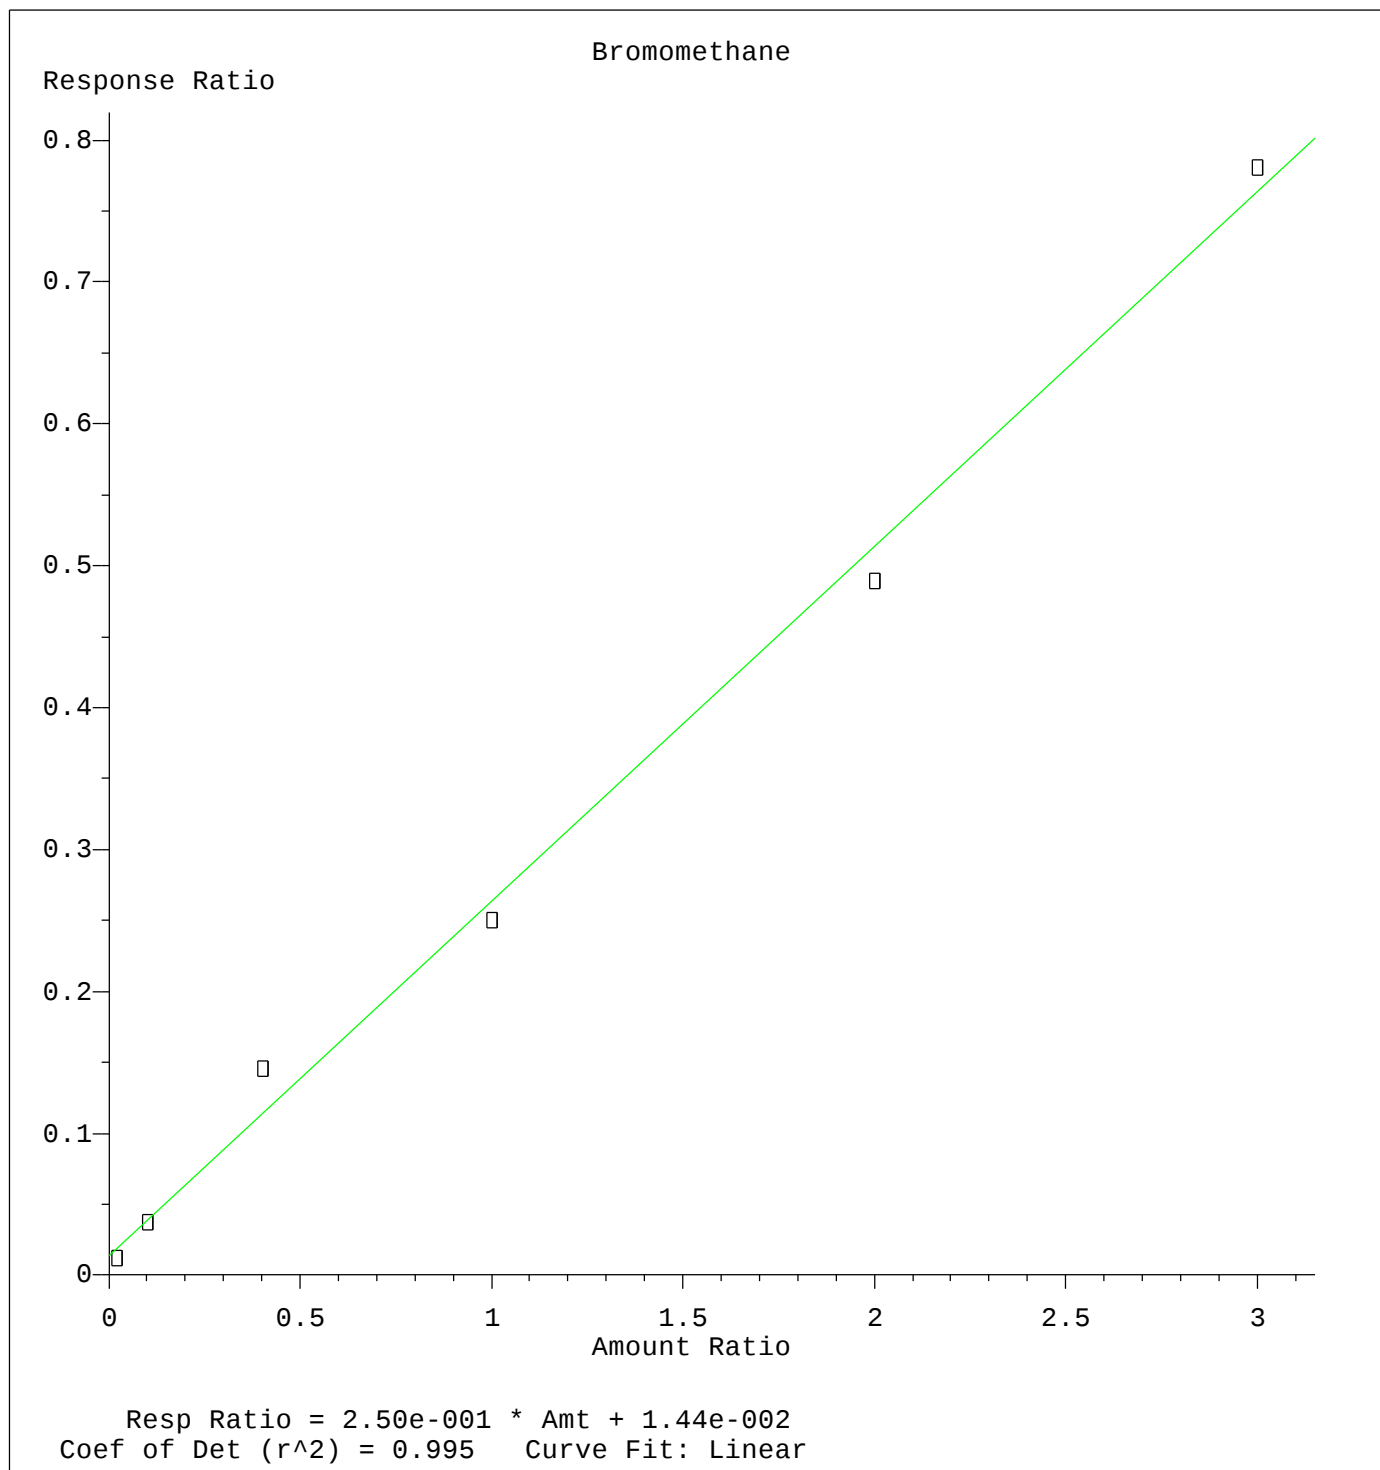


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Calibration Table Last Updated: Mon Jun 25 14:38:05 2018

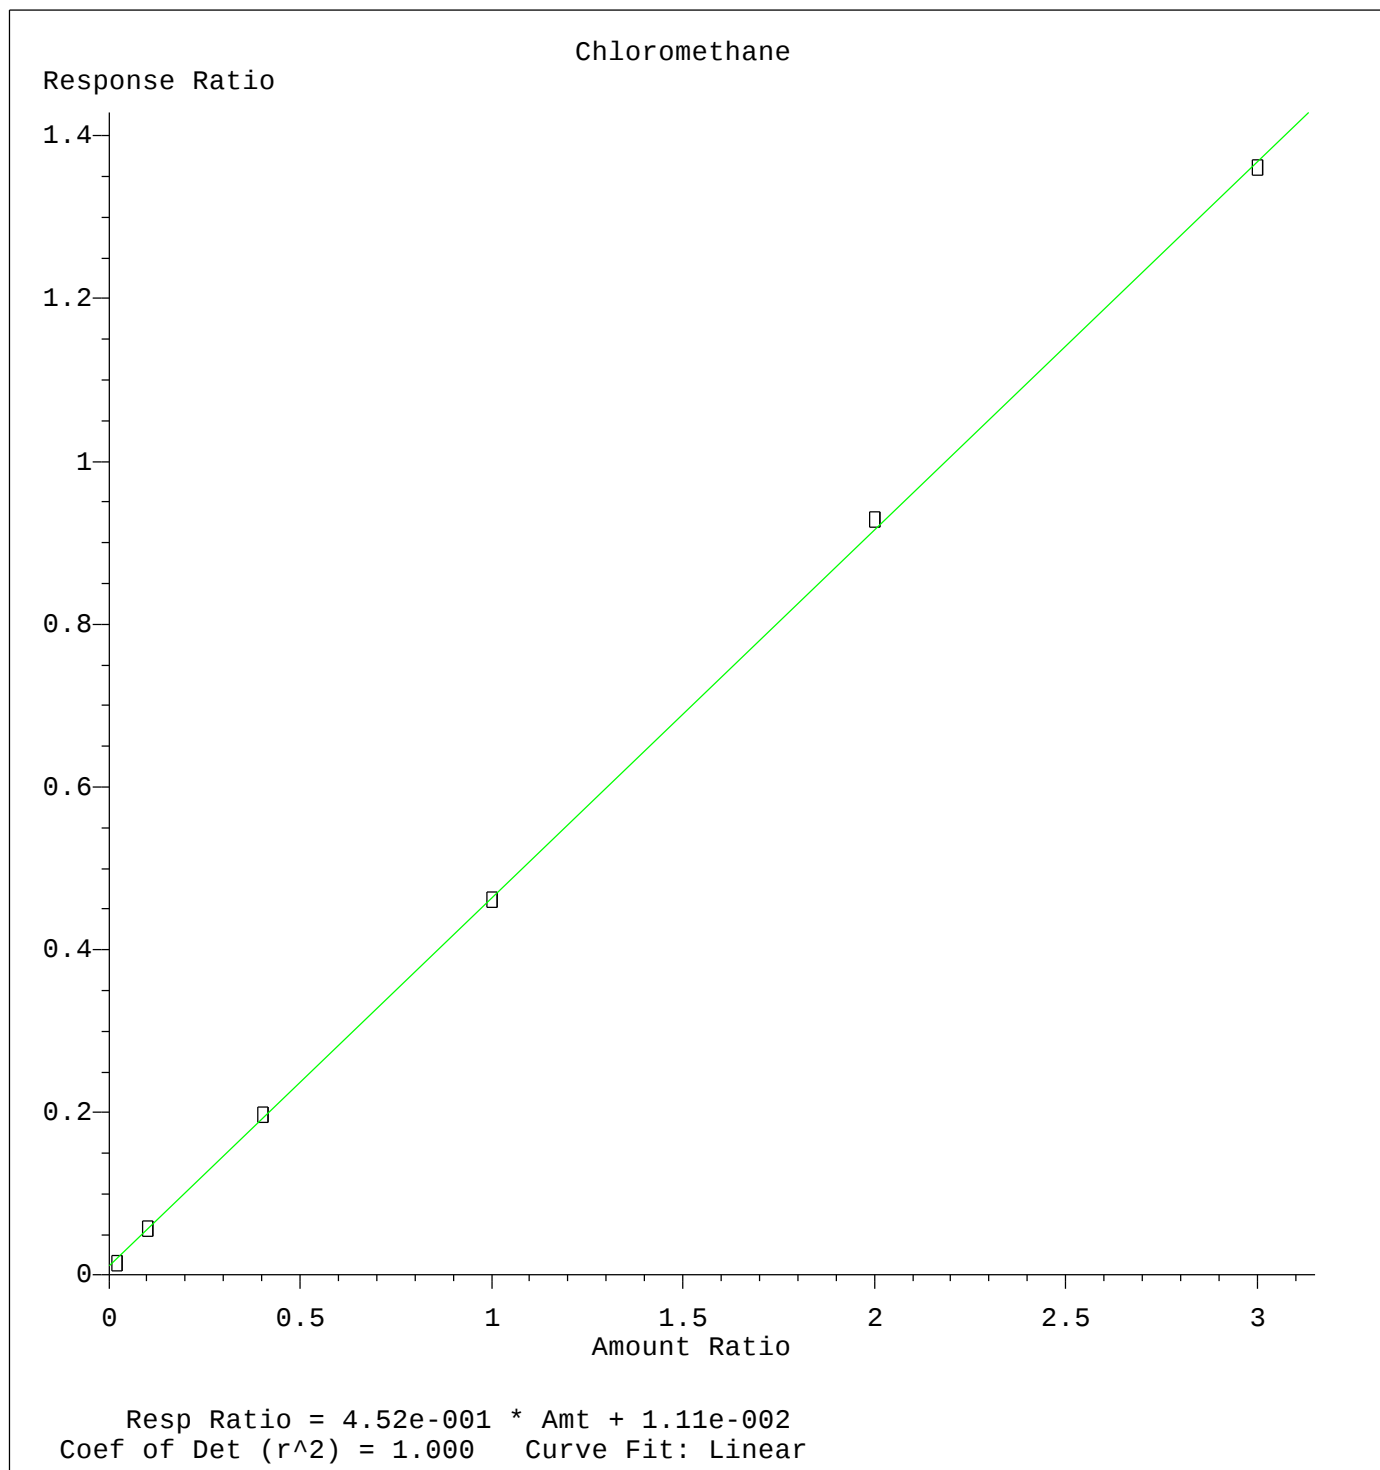

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Calibration Table Last Updated: Mon Jun 25 14:38:05 2018


trans-1,4-Dichloro-2-butene

Response Ratio

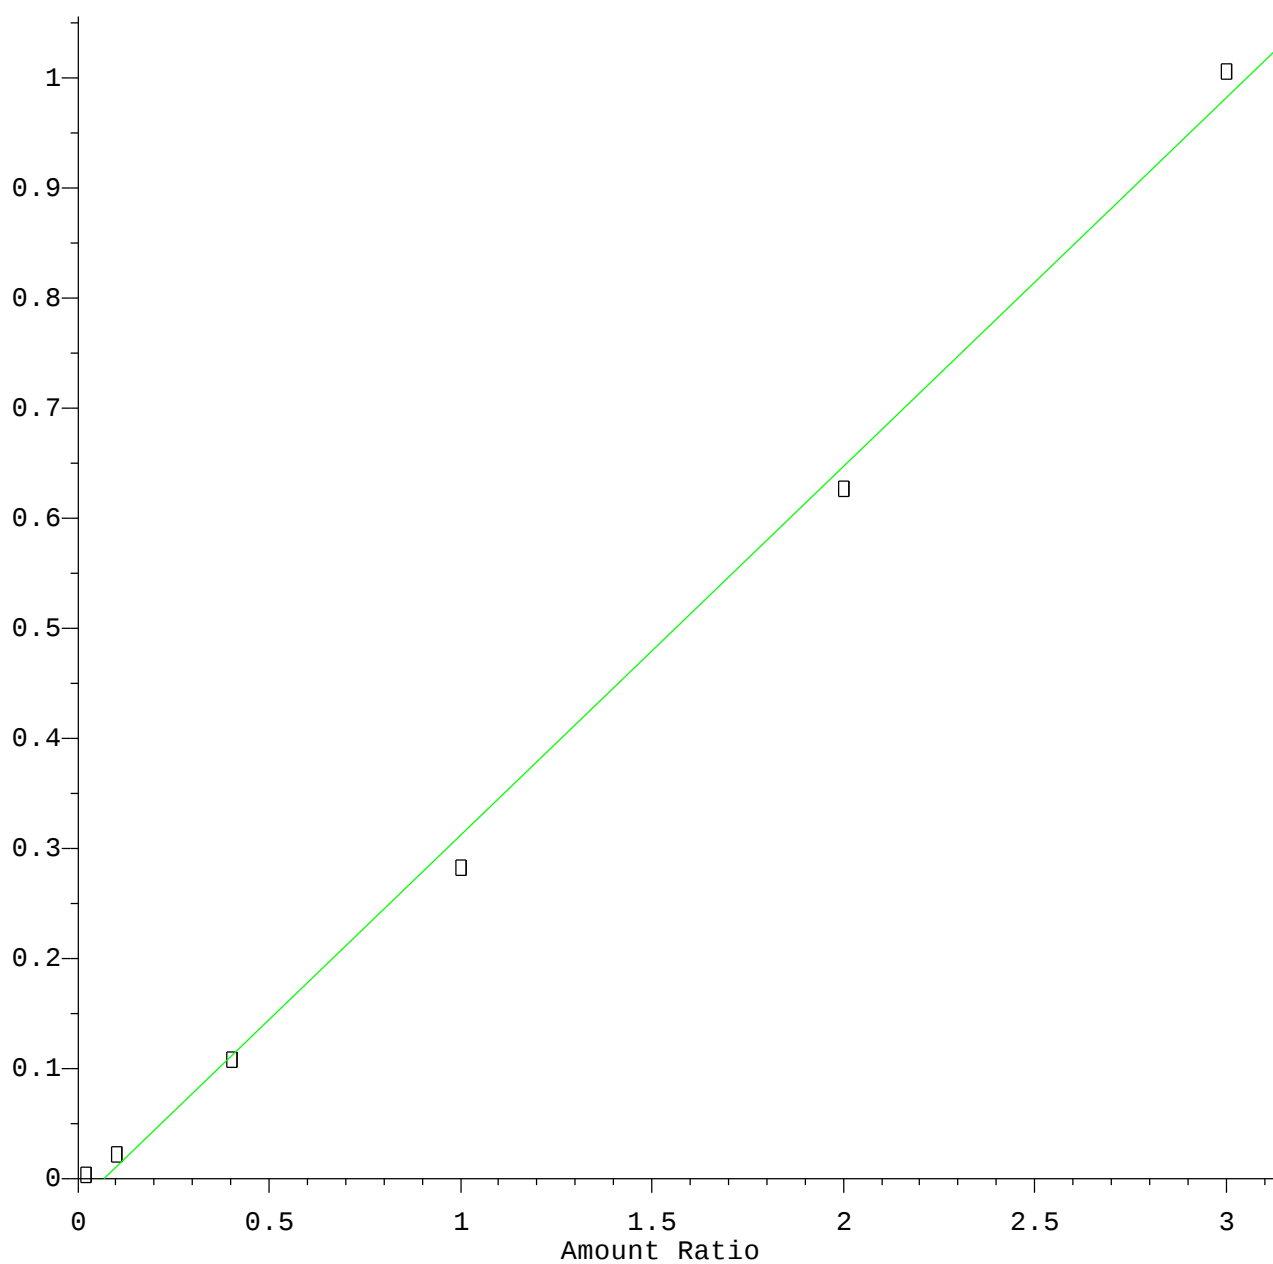

Resp Ratio = $3.35 \times 10^{-1} \times \text{Amt} - 2.25 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Calibration Table Last Updated: Mon Jun 25 14:38:05 2018

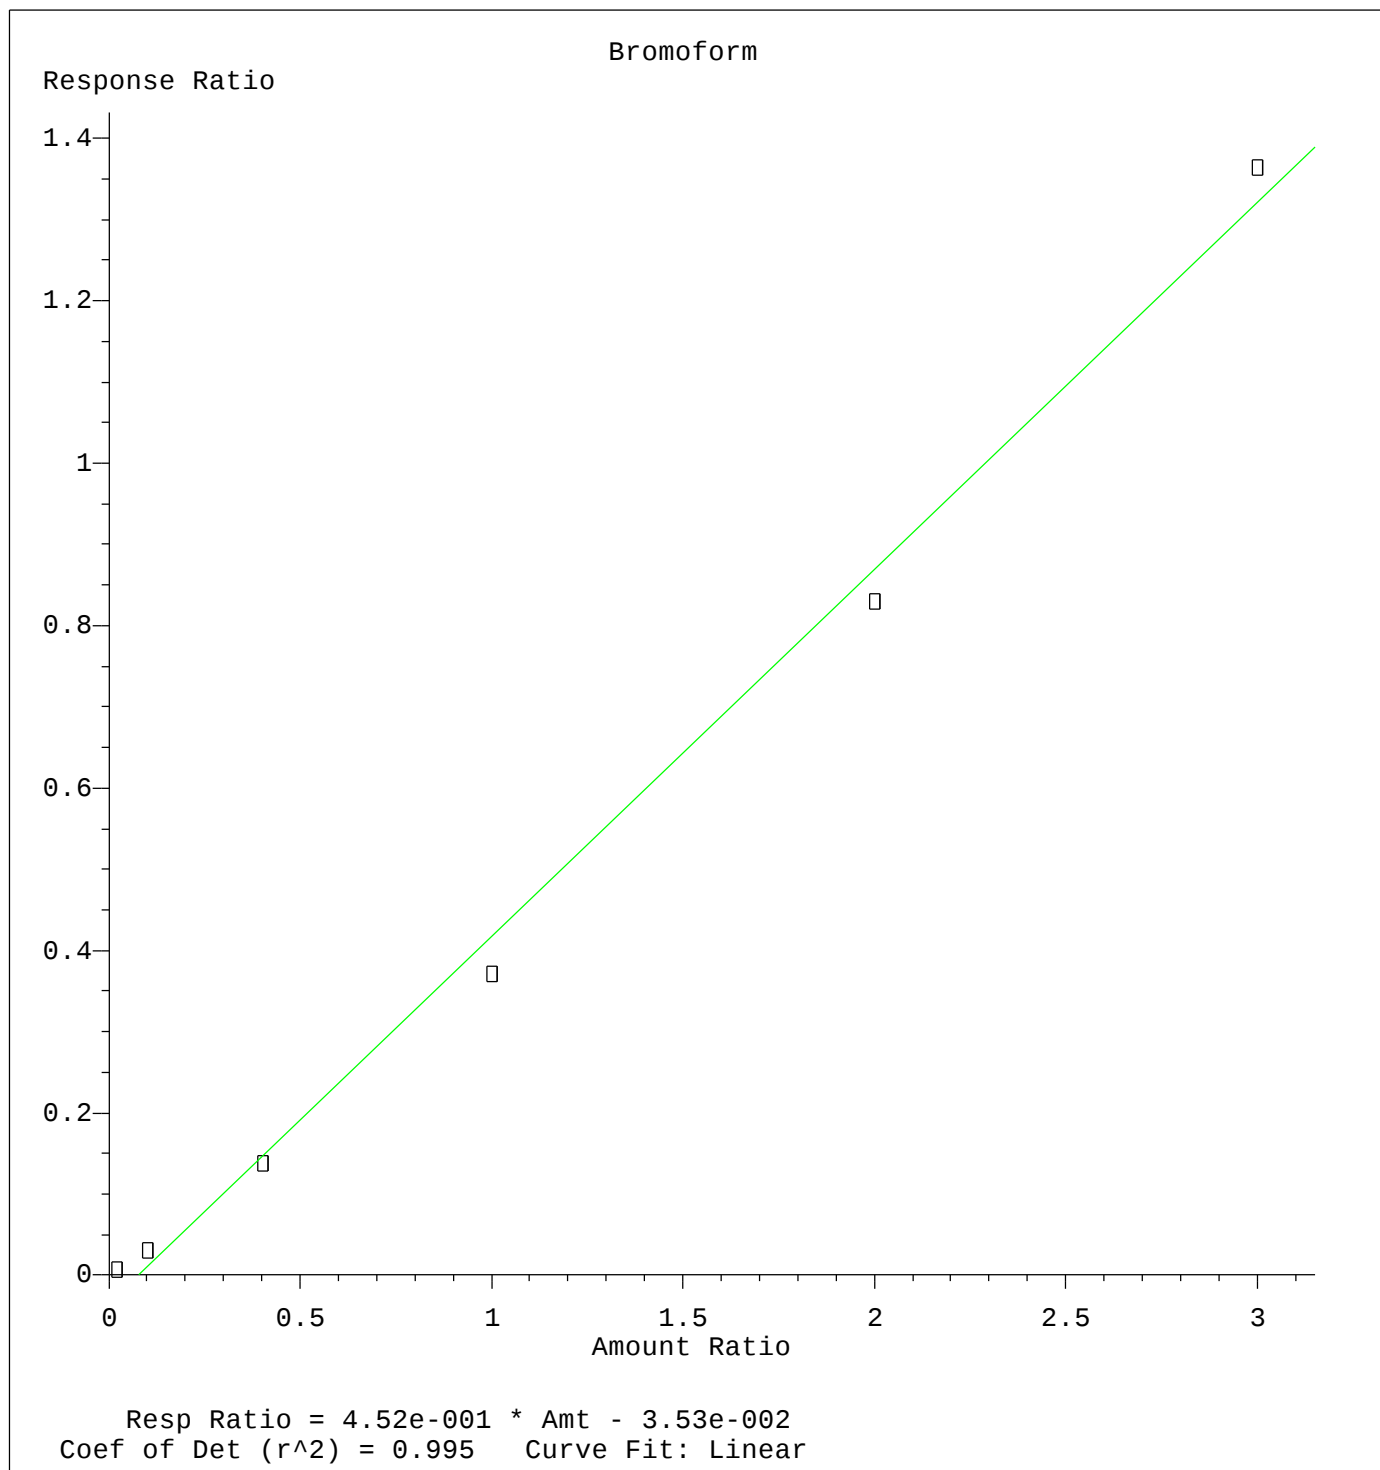

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Calibration Table Last Updated: Mon Jun 25 14:38:05 2018

Acrolein

Response Ratio

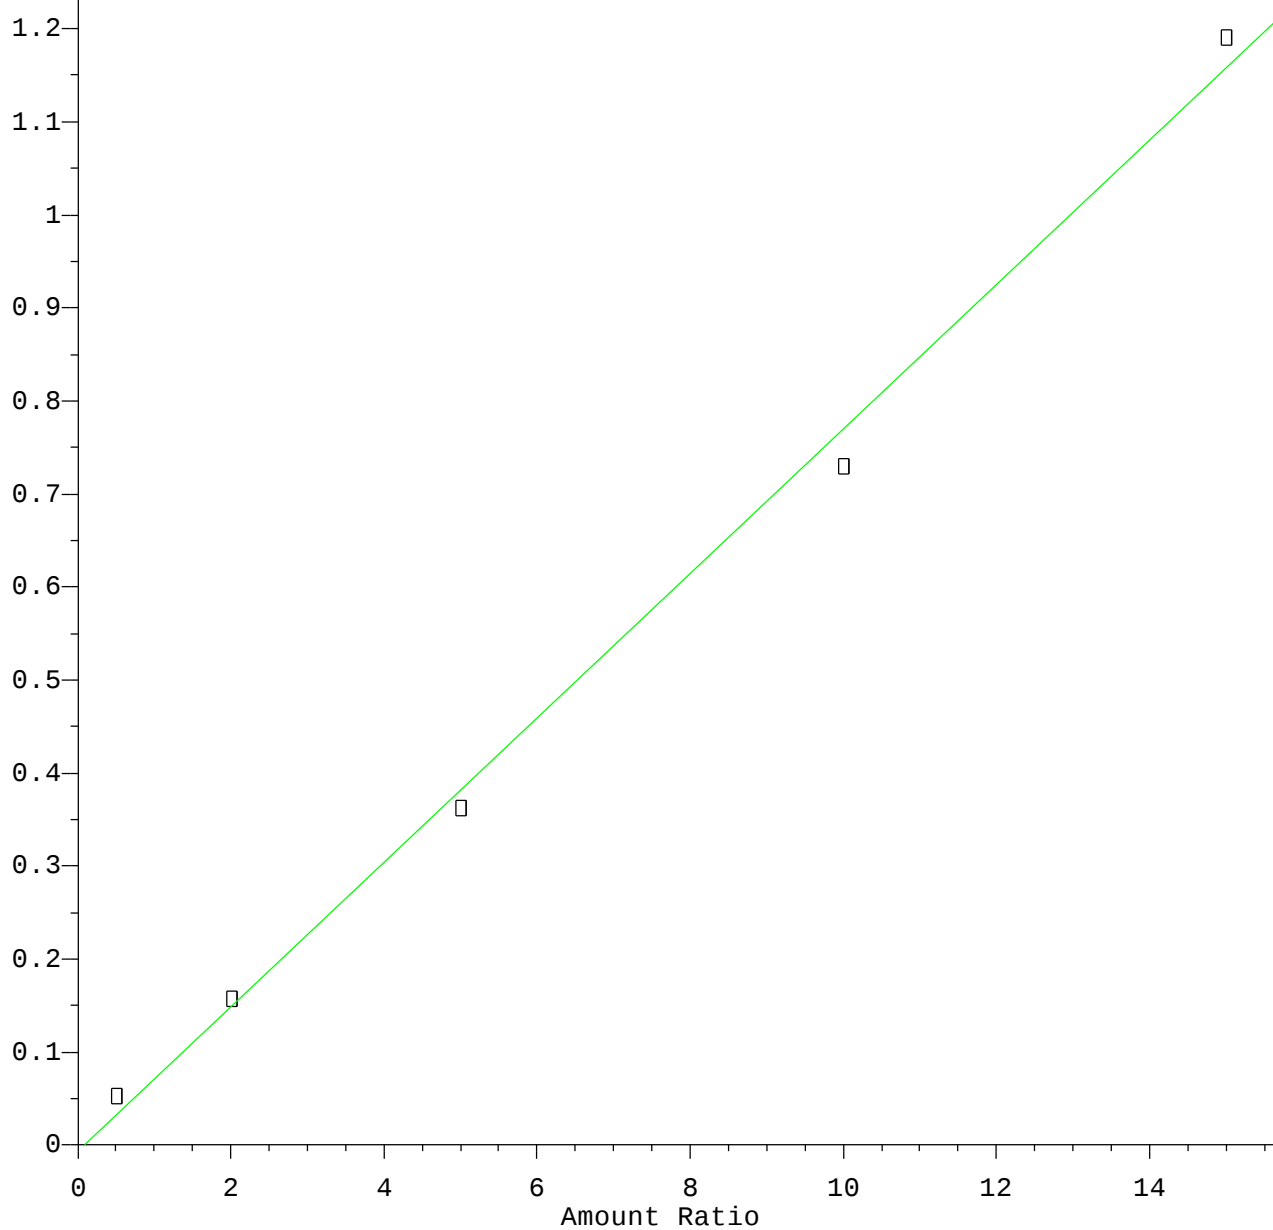

Resp Ratio = $7.76 \times 10^{-2} \times \text{Amt} - 6.57 \times 10^{-3}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Calibration Table Last Updated: Mon Jun 25 14:38:05 2018