

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062518\
 Data File : VX002885.D
 Acq On : 26 Jun 2018 02:59
 Operator : JC/MD
 Sample : J3705-07
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 W-20

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	76	80	89	rBV	1029769	1248832	67.74%	11.853%
2	1.148	89	92	105	rVB	46028	78871	4.28%	0.749%
3	1.270	108	112	115	rBV	209305	267301	14.50%	2.537%
4	1.325	115	121	144	rVB	615032	1843610	100.00%	17.497%
5	5.507	793	807	822	rBV2	168953	483545	26.23%	4.589%
6	5.665	822	833	846	rVB	252878	705587	38.27%	6.697%
7	6.074	888	900	922	rBV	177483	464463	25.19%	4.408%
8	6.866	1020	1030	1046	rBV	355575	836274	45.36%	7.937%
9	8.720	1326	1334	1343	rBV	859703	1334049	72.36%	12.661%
10	10.116	1556	1563	1577	rBV	773001	1095859	59.44%	10.401%
11	11.140	1725	1731	1737	rBV	780487	969372	52.58%	9.200%
12	11.920	1851	1859	1868	rBV3	9089	21815	1.18%	0.207%
13	12.079	1880	1885	1896	rVB	914078	1186857	64.38%	11.264%


Sum of corrected areas: 10536435

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062518\
Data File : VX002885.D
Acq On : 26 Jun 2018 02:59
Operator : JC/MD
Sample : J3705-07
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampled :
W-20

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

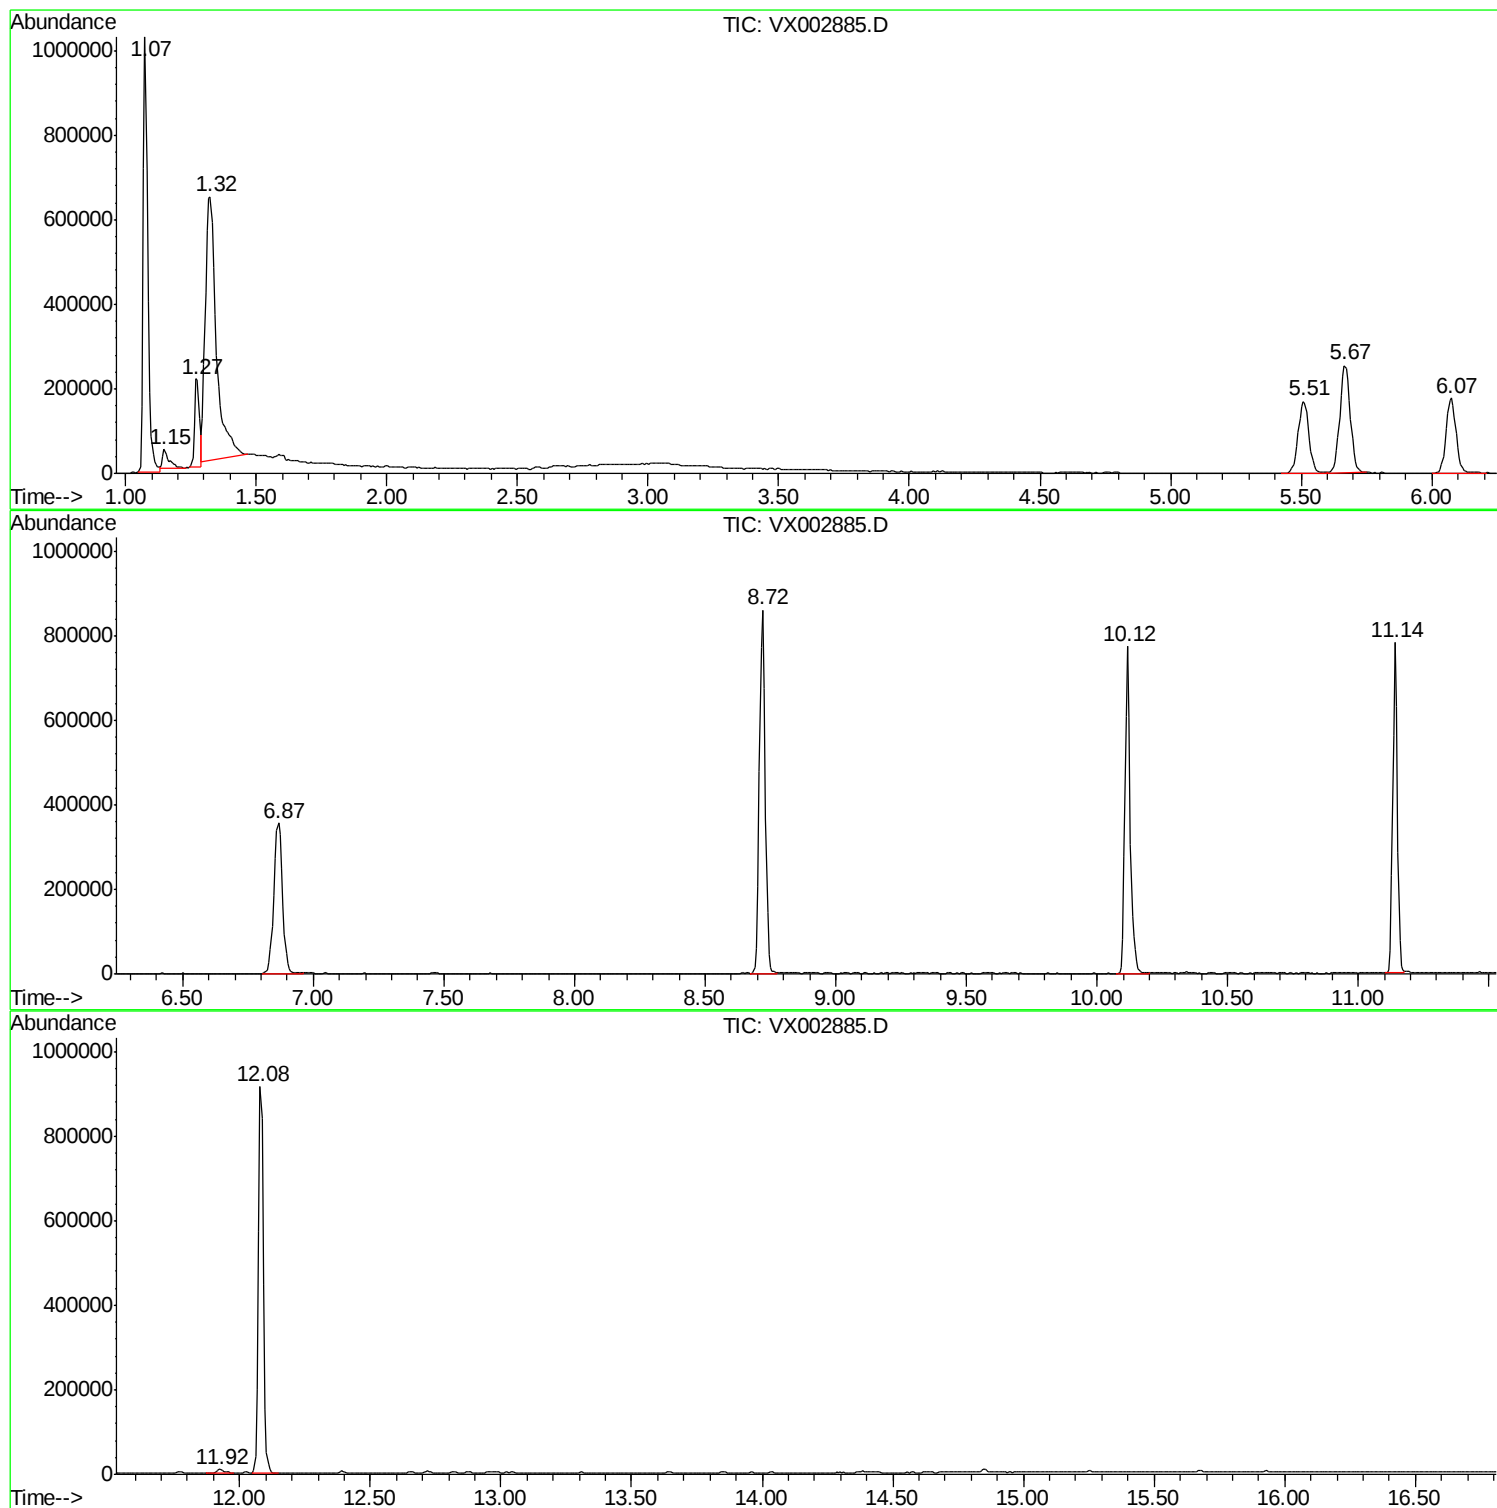

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX062518\
 Data File : VX002885.D
 Acq On : 26 Jun 2018 02:59
 Operator : JC/MD
 Sample : J3705-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 W-20

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
 Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
 TIC Integration Parameters: LSCINT.P

 Peak Number 1 unknown1.15 Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.15	5.59 ug/l	78871	Pentafluorobenzene	5.67

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Hydrogen chloride	36	ClH	007647-01-0	2
2		Methanol-D4	36	CD4O	000811-98-3	2
3		Ammonium Chloride	53	ClH4N	012125-02-9	1
4		2-Chloroethylamine	79	C2H6ClN	000689-98-5	1
5		Hydrogen sulfide	34	H2S	007783-06-4	1

 Peak Number 2 Sulfur dioxide Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.27	18.94 ug/l	267301	Pentafluorobenzene	5.67

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Sulfur dioxide	64	O2S	007446-09-5	83
2		Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3		L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4		Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5		Ethyl Chloride	64	C2H5Cl	000075-00-3	3

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX062518\
Data File : VX002885.D
Acq On : 26 Jun 2018 02:59
Operator : JC/MD
Sample : J3705-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
W-20

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.15	1.15	5.6	ug/l	78871	1	5.67	705587	50.0
Sulfur dioxide	1.27	18.9	ug/l	267301	1	5.67	705587	50.0