


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062518\
 Data File : VX002855.D
 Acq On : 25 Jun 2018 10:18
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
 Title : SW846 8260
 Last Update : Mon Jun 25 14:38:05 2018

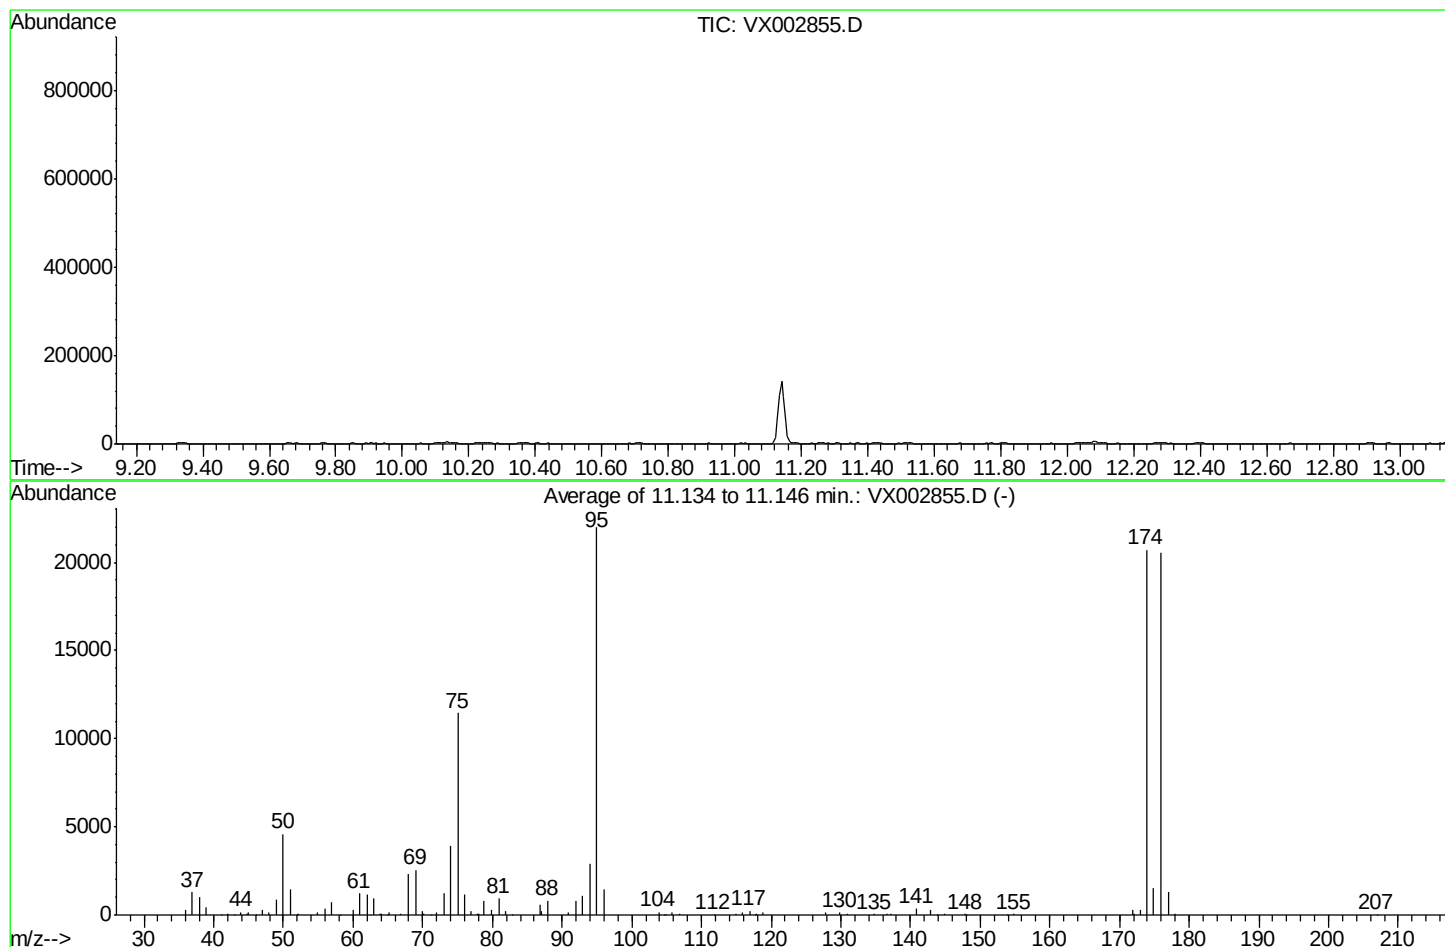

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	4606	PASS
75	95	30	60	52.1	11462	PASS
95	95	100	100	100.0	21989	PASS
96	95	5	9	6.6	1445	PASS
173	174	0.00	2	1.4	286	PASS
174	95	50	100	94.1	20693	PASS
175	174	5	9	7.5	1545	PASS
176	174	95	101	99.4	20576	PASS
177	176	5	9	6.3	1287	PASS