

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062519\  
Data File : VX010443.D  
Acq On : 25 Jun 2019 19:02  
Operator : JC/SP  
Sample : K3519-09  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SP-19-LF2MW3

## Integration Parameters: RTEINT.P

Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X061919W.M  
Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.282       | 17            | 21          | 28           | rBV      | 14556          | 23050         | 1.88%           | 0.354%        |
| 2         | 5.501       | 702           | 713         | 727          | rBV      | 148966         | 422179        | 34.39%          | 6.478%        |
| 3         | 5.665       | 727           | 740         | 754          | rVV      | 251818         | 713972        | 58.15%          | 10.955%       |
| 4         | 6.062       | 793           | 805         | 821          | rBV      | 139581         | 376654        | 30.68%          | 5.779%        |
| 5         | 6.860       | 925           | 936         | 948          | rBV      | 382618         | 886384        | 72.20%          | 13.600%       |
| 6         | 8.714       | 1233          | 1240        | 1254         | rBV      | 780587         | 1227761       | 100.00%         | 18.838%       |
| 7         | 10.110      | 1460          | 1469        | 1486         | rBV      | 759236         | 1048961       | 85.44%          | 16.095%       |
| 8         | 11.134      | 1631          | 1637        | 1651         | rBV      | 644427         | 831988        | 67.76%          | 12.765%       |
| 9         | 12.079      | 1784          | 1792        | 1802         | rBV      | 762134         | 986546        | 80.35%          | 15.137%       |


Sum of corrected areas: 6517495

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062519\  
Data File : VX010443.D  
Acq On : 25 Jun 2019 19:02  
Operator : JC/SP  
Sample : K3519-09  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SP-19-LF2MW3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X061919W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

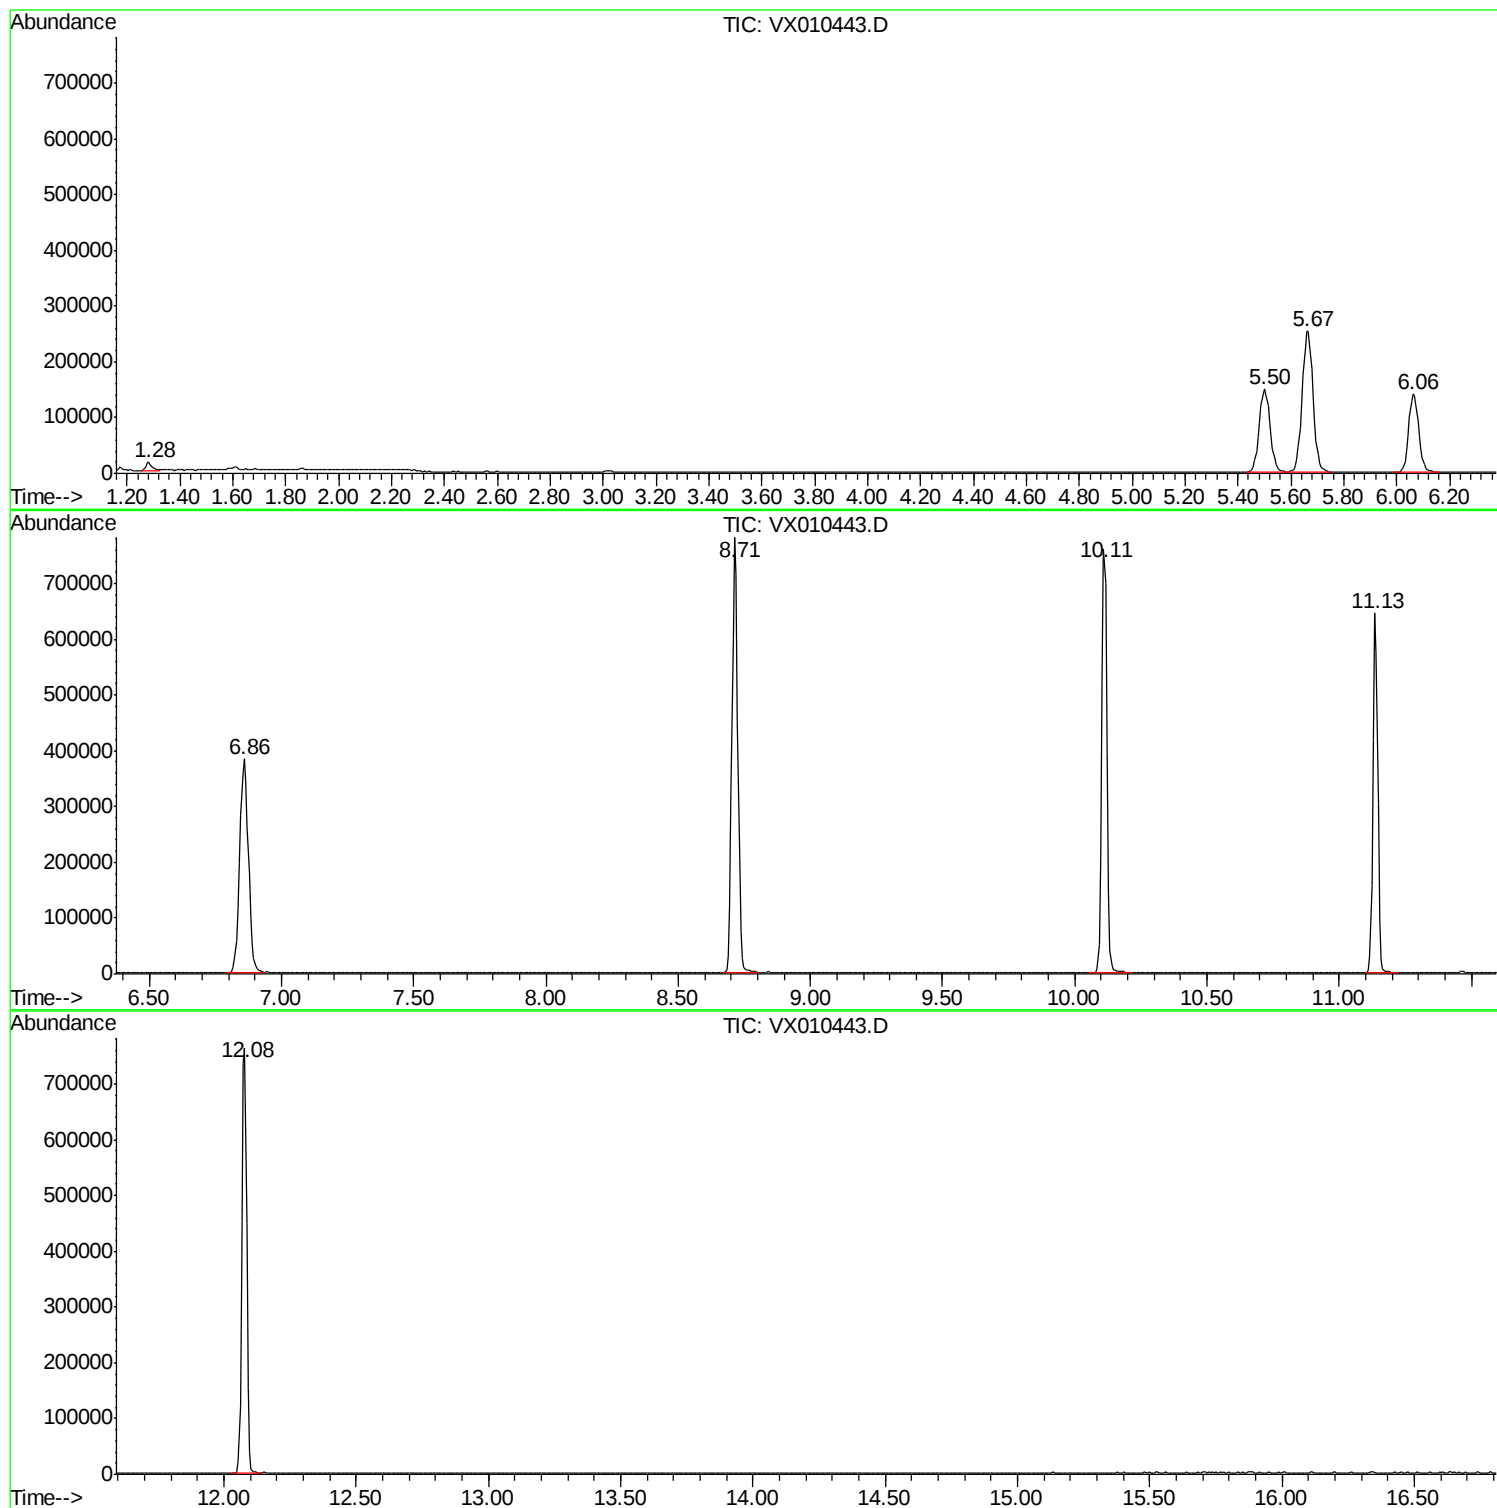

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX062519\  
Data File : VX010443.D  
Acq On : 25 Jun 2019 19:02  
Operator : JC/SP  
Sample : K3519-09  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SP-19-LF2MW3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X061919W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX062519\  
Data File : VX010443.D  
Acq On : 25 Jun 2019 19:02  
Operator : JC/SP  
Sample : K3519-09  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SP-19-LF2MW3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X061919W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |