

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062521\
 Data File : VX022959.D
 Acq On : 26 Jun 2021 06:34
 Operator : JC/MD
 Sample : M2812-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 356-349

Quant Time: Jun 26 07:38:18 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 23 19:12:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	50316	50.00	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.769	114	108688	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.061	117	104382	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	45147	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	48819	53.46	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 106.92%	
35) Dibromofluoromethane	5.397	113	33519	48.56	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 97.12%	
50) Toluene-d8	8.653	98	140994	52.12	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 104.24%	
62) 4-Bromofluorobenzene	11.085	95	50387	49.91	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 99.82%	

Target Compounds						Qvalue
11) Tert butyl alcohol	2.971	59	948	4.98	ug/l	# 83
16) Acetone	2.392	43	7563	18.68	ug/l	# 83
17) Carbon Disulfide	2.514	76	121	3.58	ug/l	# 75
18) Methyl Acetate	2.709	43	553	0.56	ug/l	# 55
20) Methylene Chloride	2.800	84	3599	4.82	ug/l	# 89
25) 2-Butanone	4.580	43	1537	2.44	ug/l	# 86
29) Tetrahydrofuran	5.031	42	232	0.57	ug/l	# 27
31) Cyclohexane	5.562	56	1610	1.25	ug/l	# 36
36) 1,1-Dichloropropene	5.550	75	5579	4.83	ug/l	# 48
38) Carbon Tetrachloride	5.556	117	6264	6.47	ug/l	# 15
40) Benzene	6.050	78	2615	0.79	ug/l	96
43) Isopropyl Acetate	6.354	43	9355	4.35	ug/l	# 91
48) Methyl methacrylate	7.805	41	49590	49.84	ug/l	# 38
49) 1,4-Dioxane	7.811	88	19	0.89	ug/l	# 1
51) 4-Methyl-2-Pentanone	8.555	43	34178	25.54	ug/l	# 44
52) Toluene	8.726	92	8468	4.21	ug/l	98
53) t-1,3-Dichloropropene	8.726	75	99	3.73	ug/l	# 1
54) cis-1,3-Dichloropropene	8.555	75	13997	11.68	ug/l	# 70
56) Ethyl methacrylate	9.250	69	114	2.65	ug/l	# 1
57) 1,3-Dichloropropane	9.488	76	8585	5.85	ug/l	# 42
59) 2-Hexanone	9.378	43	4233	4.17	ug/l	# 19
67) Ethyl Benzene	10.195	91	8147	2.01	ug/l	92
68) m/p-Xylenes	10.305	106	10211	6.79	ug/l	99
69) o-Xylene	10.646	106	6710	4.59	ug/l	94
70) Styrene	10.659	104	4422	1.82	ug/l	# 82
73) Isopropylbenzene	10.963	105	1497	0.39	ug/l	94
74) N-amyl acetate	10.823	43	177	2.13	ug/l	# 38
76) 1,2,3-Trichloropropane	11.085	75	28444	23.85	ug/l	# 39
78) n-propylbenzene	11.305	91	1121	0.24	ug/l	98
79) 2-Chlorotoluene	11.616	91	572	0.20	ug/l	81
80) 1,3,5-Trimethylbenzene	11.451	105	9031	2.88	ug/l	94
81) trans-1,4-Dichloro-2-b...	11.085	75	28444	62.55	ug/l	# 12
83) tert-Butylbenzene	11.756	119	2659	0.90	ug/l	# 44
84) 1,2,4-Trimethylbenzene	11.756	105	22467	7.12	ug/l	96
85) sec-Butylbenzene	11.756	105	22467	5.62	ug/l	# 57
89) n-Butylbenzene	12.323	91	1219	0.40	ug/l	# 19

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062521\
Data File : VX022959.D
Acq On : 26 Jun 2021 06:34
Operator : JC/MD
Sample : M2812-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
356-349

Quant Time: Jun 26 07:38:18 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 23 19:12:26 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
90) Hexachloroethane	12.414	117	19288	34.12	ug/l #	9
92) 1,2-Dibromo-3-Chloropr...	12.969	75	1910	9.65	ug/l #	1
95) Naphthalene	13.786	128	6510861	1703.06	ug/l	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062521\
Data File : VX022959.D
Acq On : 26 Jun 2021 06:34
Operator : JC/MD
Sample : M2812-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
356-349

Quant Time: Jun 26 07:38:18 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 23 19:12:26 2021
Response via : Initial Calibration




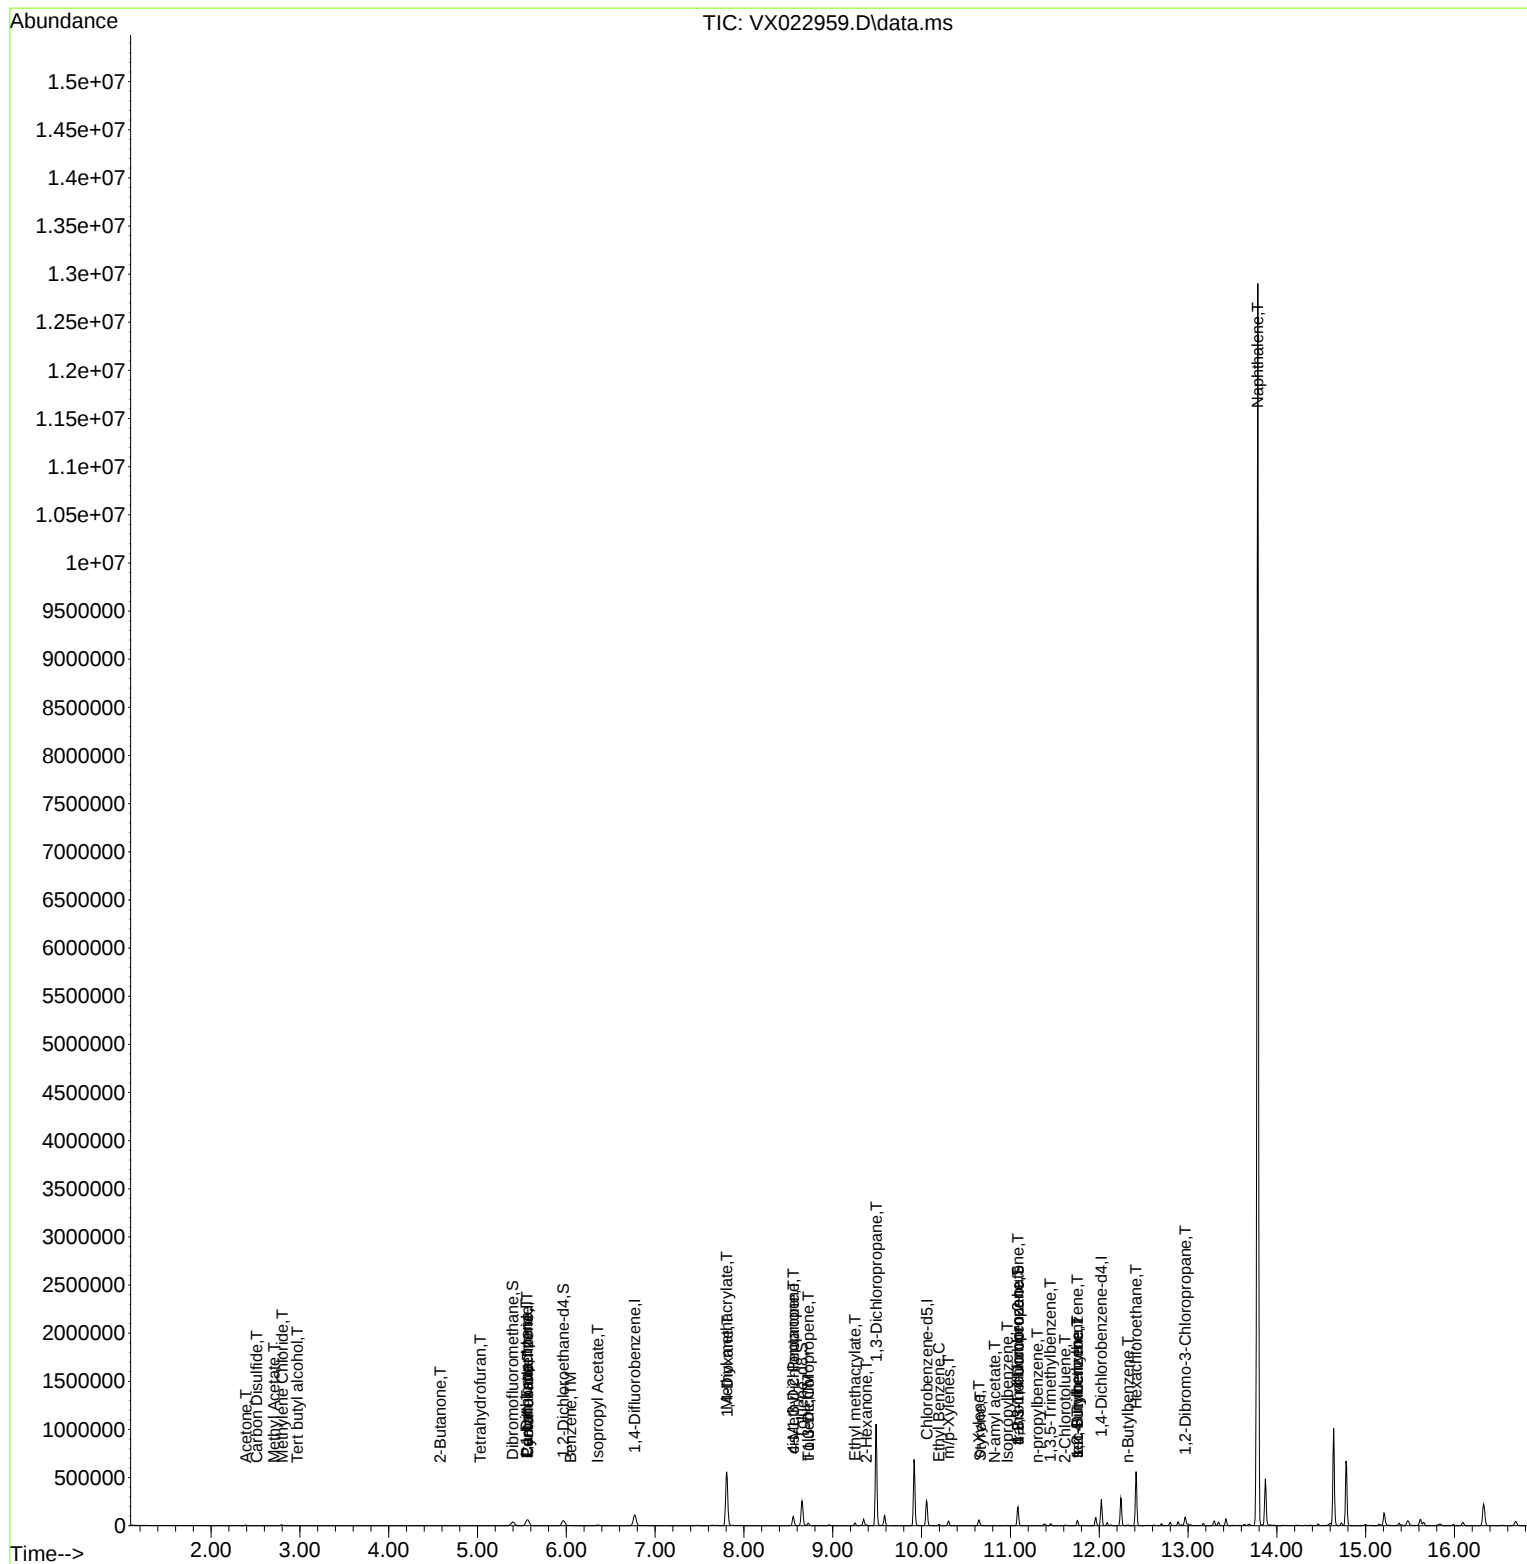




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.562 min Scan# 734
Delta R.T. 0.006 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34




Instrument :
MSVOA_X
ClientSampleId :
356-349


Tgt Ion:168 Resp: 50316
Ion Ratio Lower Upper
168 100
99 75.9 45.8 68.6#

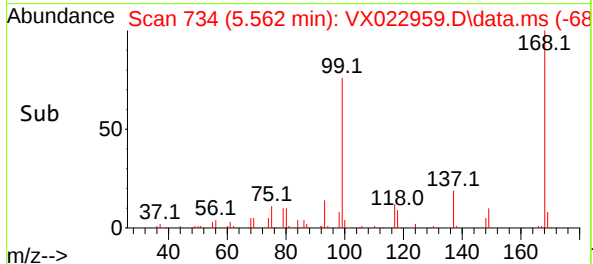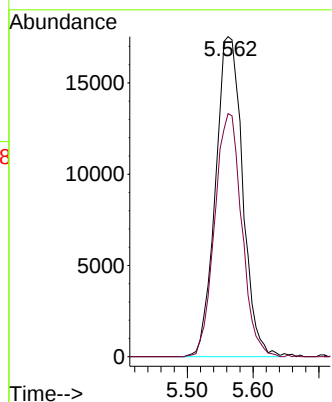

#11
Tert butyl alcohol
Concen: 4.98 ug/l
RT: 2.971 min Scan# 309
Delta R.T. -0.006 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34

Tgt Ion: 59 Resp: 948
Ion Ratio Lower Upper
59 100
57 3.5 7.8 11.8#









#16
Acetone
Concen: 18.68 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.000 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34




Instrument :
MSVOA_X
ClientSampleId :
356-349


Tgt Ion: 43 Resp: 7563
Ion Ratio Lower Upper
43 100
58 24.8 27.8 41.8#

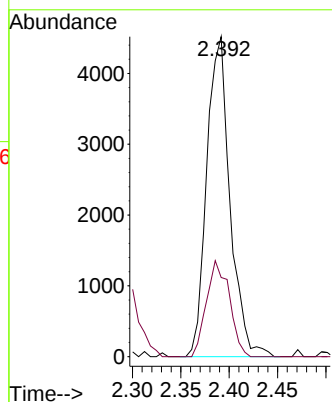

#17
Carbon Disulfide
Concen: 3.58 ug/l
RT: 2.514 min Scan# 234
Delta R.T. -0.000 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34

Tgt Ion: 76 Resp: 121
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#

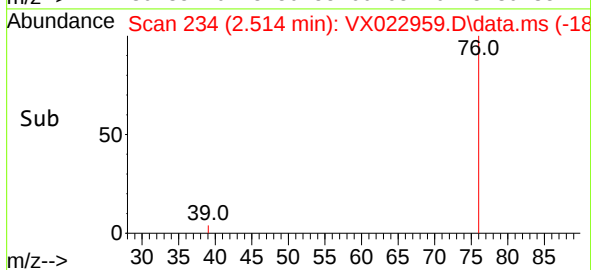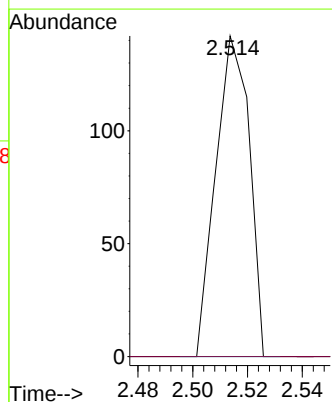



#18

Methyl Acetate

Concen: 0.56 ug/l

RT: 2.709 min Scan# 266

Delta R.T. -0.000 min

Lab File: VX022959.D





Acq: 26 Jun 2021 06:34

Tgt Ion: 43 Resp: 553

Ion Ratio Lower Upper

43 100

74 4.0 21.9 32.9#

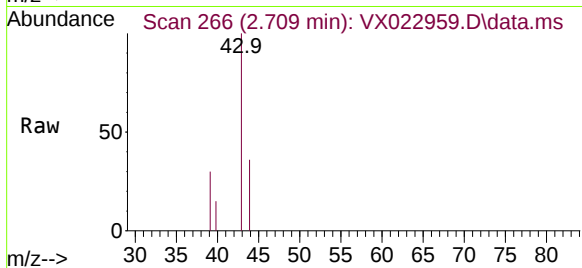

#20

Methylene Chloride

Concen: 4.82 ug/l

RT: 2.800 min Scan# 281

Delta R.T. 0.006 min

Lab File: VX022959.D

Acq: 26 Jun 2021 06:34

Tgt Ion: 84 Resp: 3599




Ion Ratio Lower Upper


84 100

49 128.4 88.6 132.8

51 40.9 27.0 40.6#

86 63.2 50.3 75.5

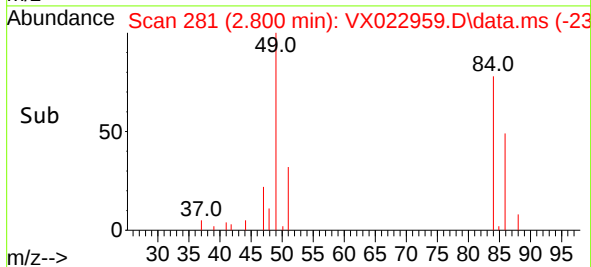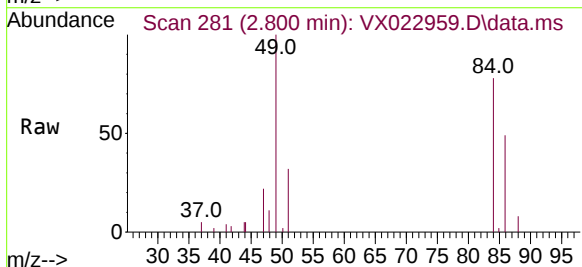



#25

2-Butanone

Concen: 2.44 ug/l

RT: 4.580 min Scan# 573

Delta R.T. 0.012 min

Lab File: VX022959.D





Acq: 26 Jun 2021 06:34

Tgt Ion: 43 Resp: 1537

Ion Ratio Lower Upper

43 100

72 22.3 23.7 35.5#

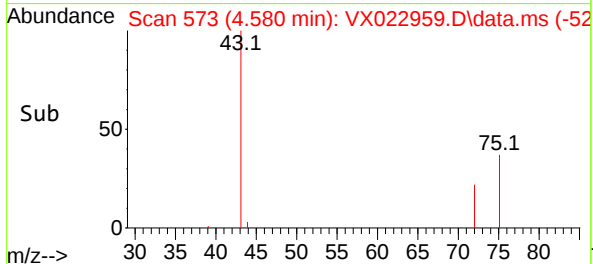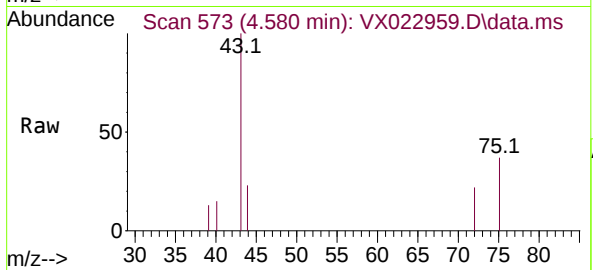

#29

Tetrahydrofuran

Concen: 0.57 ug/l

RT: 5.031 min Scan# 647

Delta R.T. 0.012 min

Lab File: VX022959.D

Acq: 26 Jun 2021 06:34




Tgt Ion: 42 Resp: 232


Ion Ratio Lower Upper

42 100

72 0.0 41.7 62.5#

71 0.0 38.4 57.6#



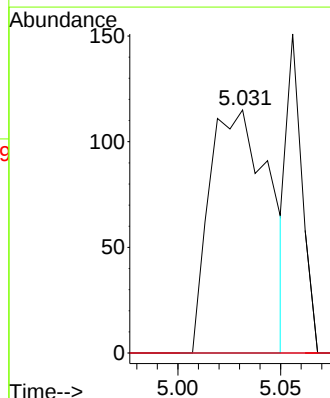





#31
Cyclohexane
Concen: 1.25 ug/l
RT: 5.562 min Scan# 734
Delta R.T. 0.086 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34




Instrument :
MSVOA_X
ClientSampleId :
356-349


Tgt Ion: 56 Resp: 1610
Ion Ratio Lower Upper
56 100
69 149.3 25.3 37.9#
84 100.5 71.4 107.0

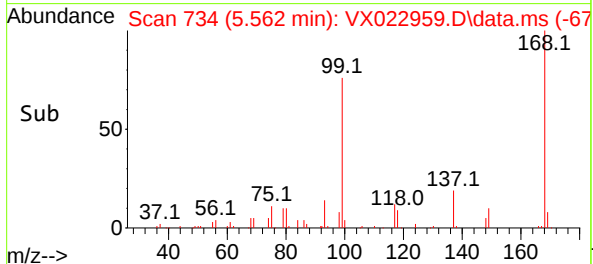

#33
1,2-Dichloroethane-d4
Concen: 53.46 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34

Tgt Ion: 65 Resp: 48819
Ion Ratio Lower Upper
65 100
67 51.1 0.0 105.4









#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.769 min Scan# 932
Delta R.T. -0.000 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34




Instrument :
MSVOA_X
ClientSampleId :
356-349


Tgt Ion:114 Resp: 108688
Ion Ratio Lower Upper
114 100
63 23.0 0.0 40.8
88 18.5 0.0 32.8

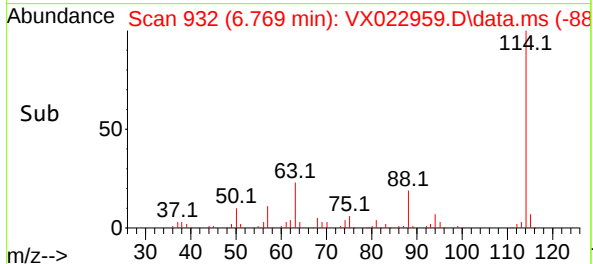

#35
Dibromofluoromethane
Concen: 48.56 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34

Tgt Ion:113 Resp: 33519
Ion Ratio Lower Upper
113 100
111 102.1 81.9 122.9
192 15.6 16.7 25.1#

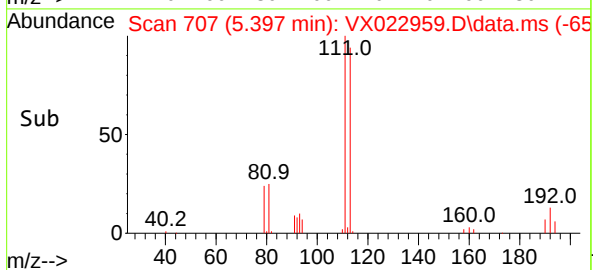



#36

1,1-Dichloropropene

Concen: 4.83 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.152 min

Lab File: VX022959.D

Acq: 26 Jun 2021 06:34

Tgt Ion: 75 Resp: 5579

Ion Ratio Lower Upper

75 100

110 8.2 18.1 54.4#





77 0.0 25.3 37.9#

Instrument :

MSVOA_X

ClientSampleId :

356-349

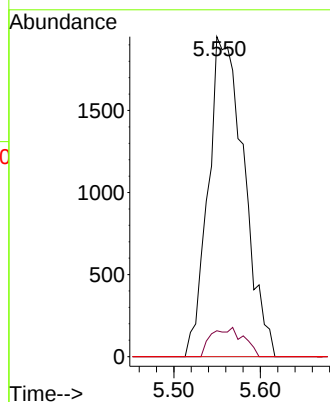

#38

Carbon Tetrachloride

Concen: 6.47 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.134 min

Lab File: VX022959.D

Acq: 26 Jun 2021 06:34




Tgt Ion: 117 Resp: 6264


Ion Ratio Lower Upper

117 100

119 3.1 76.2 114.2#

121 0.0 24.8 37.2#


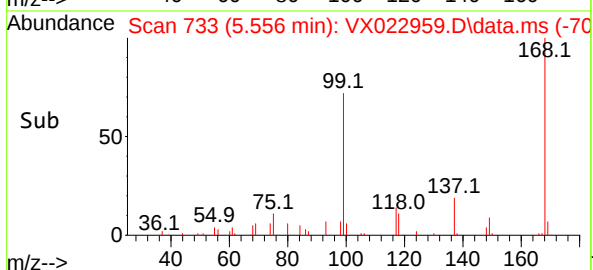






#40
Benzene
Concen: 0.79 ug/l
RT: 6.050 min Scan# 814
Delta R.T. -0.000 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34




Instrument :
MSVOA_X
ClientSampleId :
356-349


Tgt Ion: 78 Resp: 2615
Ion Ratio Lower Upper
78 100
77 25.7 18.9 28.3

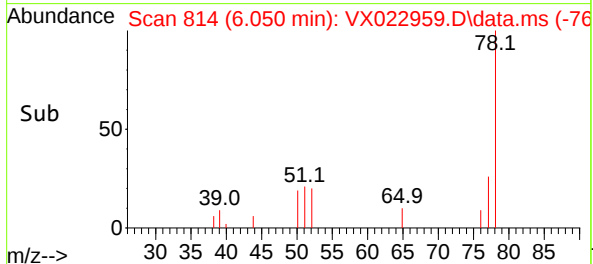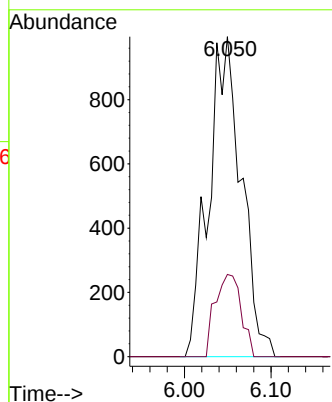

#43
Isopropyl Acetate
Concen: 4.35 ug/l
RT: 6.354 min Scan# 864
Delta R.T. 0.000 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34

Tgt Ion: 43 Resp: 9355
Ion Ratio Lower Upper
43 100
61 16.7 18.2 27.4#
87 13.6 12.5 18.7

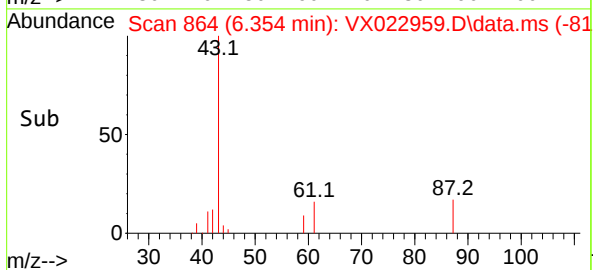



#48

Methyl methacrylate

Concen: 49.84 ug/l

RT: 7.805 min Scan# 1102

Delta R.T. 0.103 min

Lab File: VX022959.D

Acq: 26 Jun 2021 06:34

Tgt Ion: 41 Resp: 49590

Ion Ratio Lower Upper

41 100

69 0.0 76.0 114.0#





39 55.2 44.6 67.0

Instrument :

MSVOA_X

ClientSampleId :

356-349

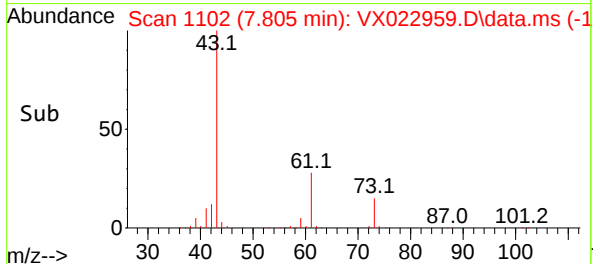

#49

1,4-Dioxane

Concen: 0.89 ug/l

RT: 7.811 min Scan# 1103

Delta R.T. 0.146 min

Lab File: VX022959.D

Acq: 26 Jun 2021 06:34




Tgt Ion: 88 Resp: 19


Ion Ratio Lower Upper

88 100

43 2732378.9 23.2 34.8#

58 12078.9 55.0 82.4#









#50
Toluene-d8
Concen: 52.12 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34




Instrument :
MSVOA_X
ClientSampleId :
356-349


Tgt Ion: 98 Resp: 140994
Ion Ratio Lower Upper
98 100
100 66.4 51.9 77.9

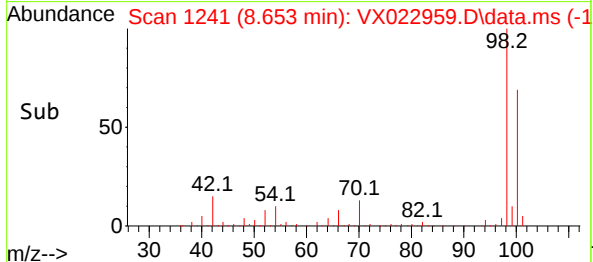

#51
4-Methyl-2-Pentanone
Concen: 25.54 ug/l
RT: 8.555 min Scan# 1225
Delta R.T. -0.025 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34

Tgt Ion: 43 Resp: 34178
Ion Ratio Lower Upper
43 100
58 7.8 35.4 53.0#


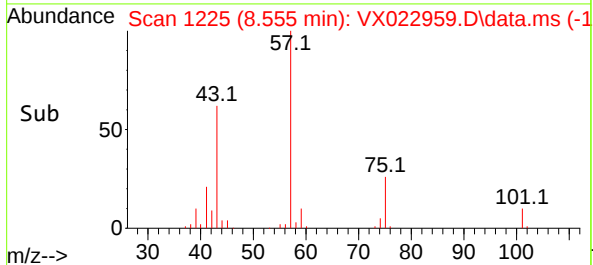






#52
Toluene
Concen: 4.21 ug/l
RT: 8.726 min Scan# 1253
Delta R.T. 0.006 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34




Instrument :
MSVOA_X
ClientSampleId :
356-349


Tgt Ion: 92 Resp: 8468
Ion Ratio Lower Upper
92 100
91 174.2 137.1 205.7

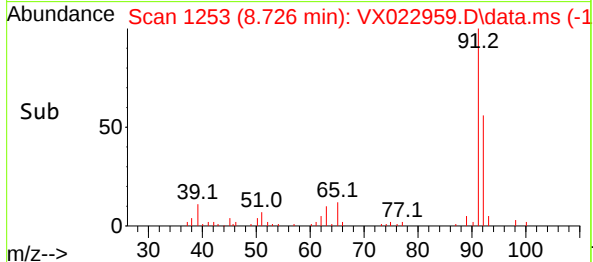

#53
t-1,3-Dichloropropene
Concen: 3.73 ug/l
RT: 8.726 min Scan# 1253
Delta R.T. -0.256 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34

Tgt Ion: 75 Resp: 99
Ion Ratio Lower Upper
75 100
77 106.7 24.9 37.3#









#54
cis-1,3-Dichloropropene
Concen: 11.68 ug/l
RT: 8.555 min Scan# 1225
Delta R.T. 0.183 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34




Instrument :
MSVOA_X
ClientSampleId :
356-349


Tgt Ion: 75 Resp: 13997
Ion Ratio Lower Upper
75 100
77 0.0 25.7 38.5#
39 37.3 35.1 52.7

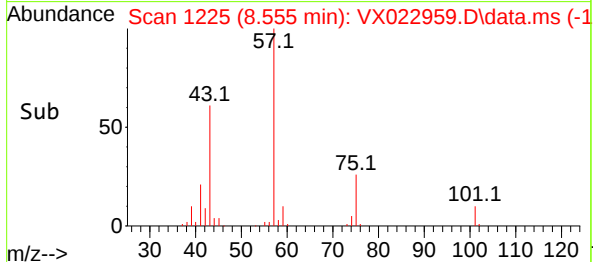

#56
Ethyl methacrylate
Concen: 2.65 ug/l
RT: 9.250 min Scan# 1339
Delta R.T. 0.128 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34

Tgt Ion: 69 Resp: 114
Ion Ratio Lower Upper
69 100
41 4066.7 46.8 70.2#
39 2222.8 24.7 37.1#

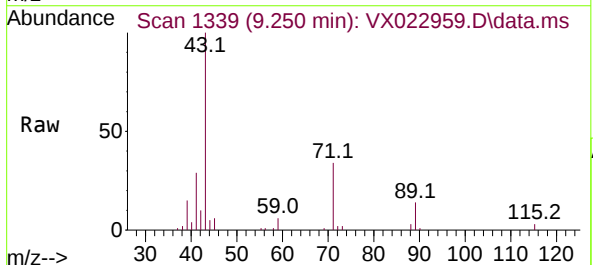







#57

1,3-Dichloropropane
Concen: 5.85 ug/l
RT: 9.488 min Scan# 1378
Delta R.T. 0.177 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34

Instrument :
MSVOA_X
ClientSampleId :
356-349




Tgt Ion: 76 Resp: 8585
Ion Ratio Lower Upper
76 100
78 0.0 26.2 39.2#

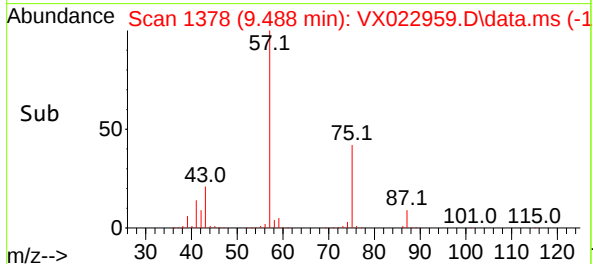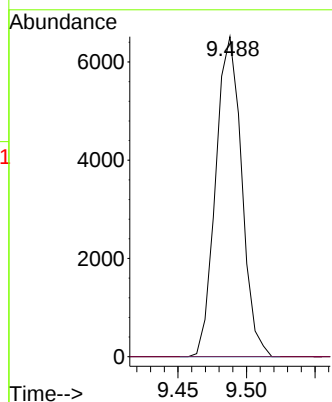


#59

2-Hexanone
Concen: 4.17 ug/l
RT: 9.378 min Scan# 1360
Delta R.T. -0.055 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34

Tgt Ion: 43 Resp: 4233
Ion Ratio Lower Upper
43 100
58 0.0 30.9 92.8#



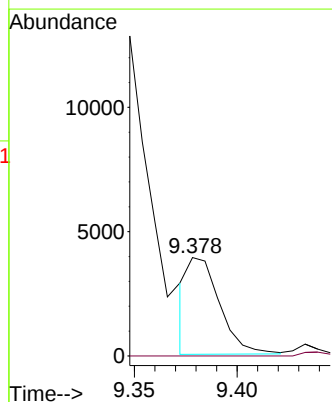





#62
4-Bromofluorobenzene
Concen: 49.91 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34




Instrument :
MSVOA_X
ClientSampleId :
356-349


Tgt Ion: 95 Resp: 50387
Ion Ratio Lower Upper
95 100
174 62.7 0.0 154.6
176 60.0 0.0 155.8

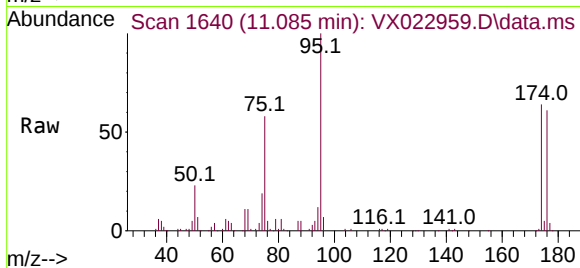

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.061 min Scan# 1472
Delta R.T. 0.006 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34

Tgt Ion: 117 Resp: 104382
Ion Ratio Lower Upper
117 100
82 60.5 47.4 71.2
119 33.4 26.6 39.8


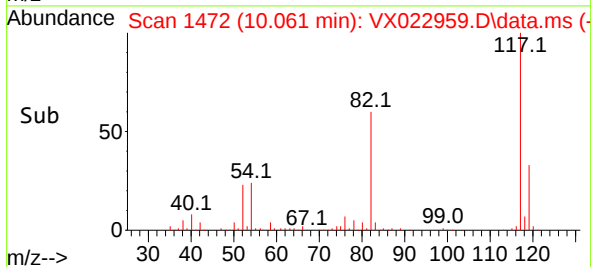

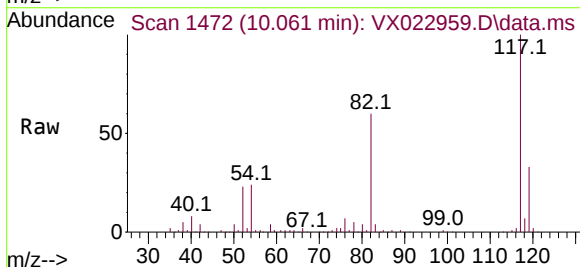




#67
Ethyl Benzene
Concen: 2.01 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34




Instrument :
MSVOA_X
ClientSampleId :
356-349


Tgt Ion: 91 Resp: 8147
Ion Ratio Lower Upper
91 100
106 26.3 24.6 37.0

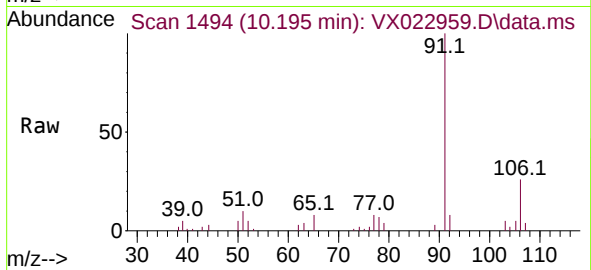

#68
m/p-Xylenes
Concen: 6.79 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34

Tgt Ion: 106 Resp: 10211
Ion Ratio Lower Upper
106 100
91 205.5 162.8 244.2




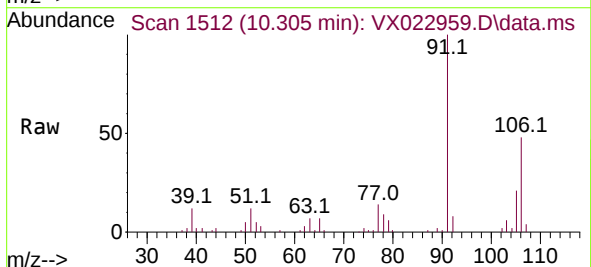




#69
o-Xylene
Concen: 4.59 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.000 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34




Instrument :
MSVOA_X
ClientSampled :
356-349


Tgt Ion:106 Resp: 6710
Ion Ratio Lower Upper
106 100
91 225.6 108.1 324.2

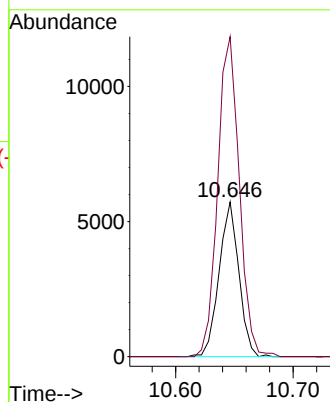

#70
Styrene
Concen: 1.82 ug/l
RT: 10.659 min Scan# 1570
Delta R.T. 0.001 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34

Tgt Ion:104 Resp: 4422
Ion Ratio Lower Upper
104 100
78 66.3 40.0 60.0#
103 63.8 43.4 65.0


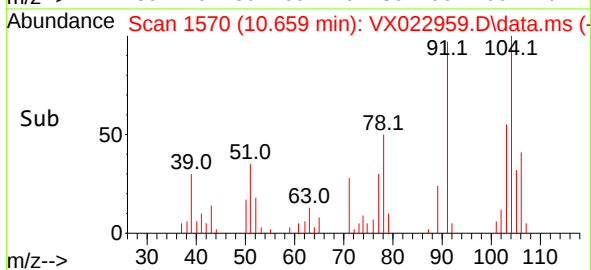

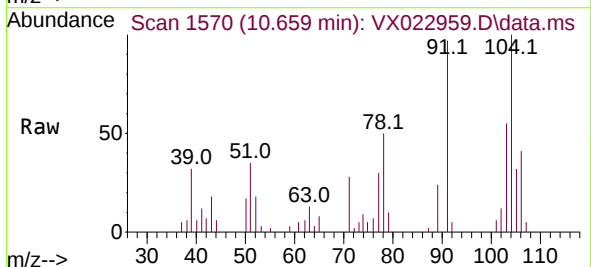




#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34




Instrument :
MSVOA_X
ClientSampleId :
356-349


Tgt Ion:152 Resp: 45147
Ion Ratio Lower Upper
152 100
115 68.7 41.1 123.3
150 157.7 0.0 349.0

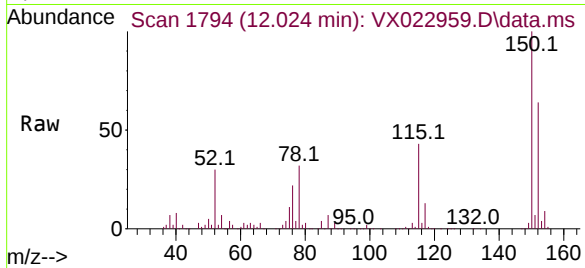

#73
Isopropylbenzene
Concen: 0.39 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34

Tgt Ion:105 Resp: 1497
Ion Ratio Lower Upper
105 100
120 23.2 13.2 39.6


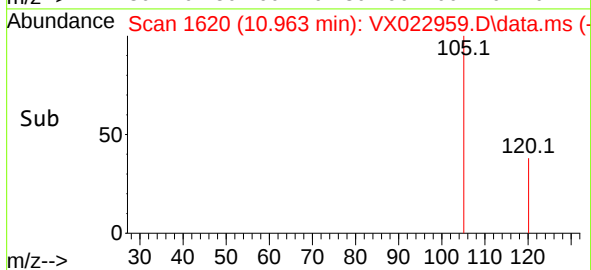

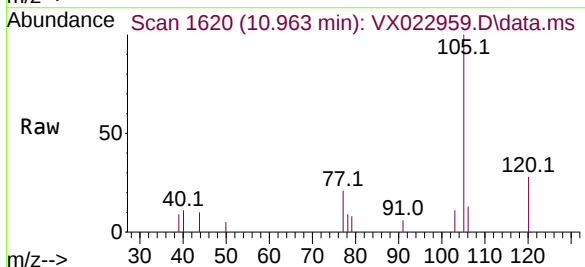




#74
N-amy1 acetate
Concen: 2.13 ug/l
RT: 10.823 min Scan# 1597
Delta R.T. -0.024 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34




Instrument :
MSVOA_X
ClientSampleId :
356-349


Tgt Ion: 43	Resp: 177
Ion Ratio	Lower Upper
43 100	
70 0.0	39.0 58.6#
55 0.0	21.5 32.3#
61 0.0	22.1 33.1#

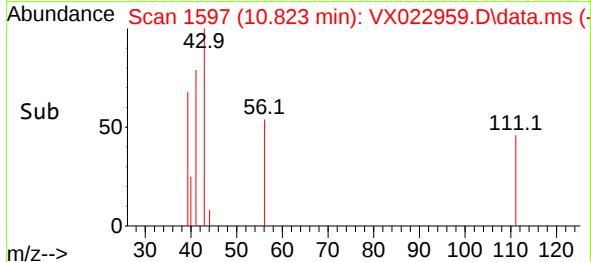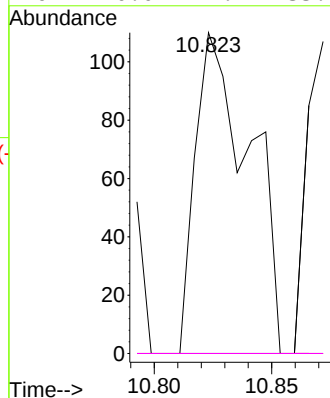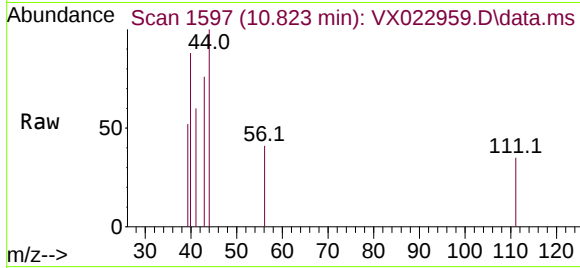

#76
1,2,3-Trichloropropane
Concen: 23.85 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34

Tgt Ion: 75	Resp: 28444
Ion Ratio	Lower Upper
75 100	
77 1.4	19.1 57.5#


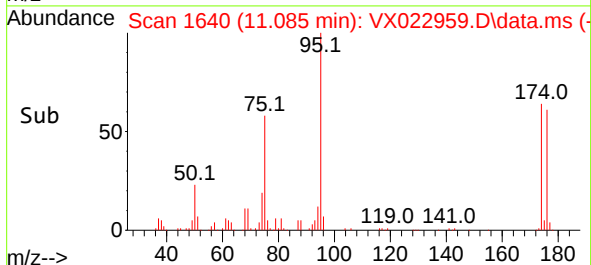
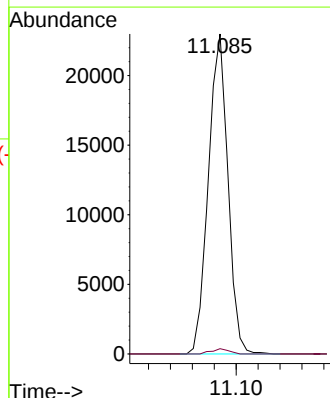
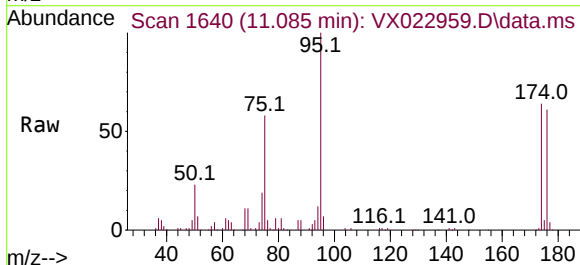




#78
n-propylbenzene
Concen: 0.24 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34




Instrument :
MSVOA_X
ClientSampleId :
356-349


Tgt Ion: 91 Resp: 1121
Ion Ratio Lower Upper
91 100
120 24.2 11.5 34.5

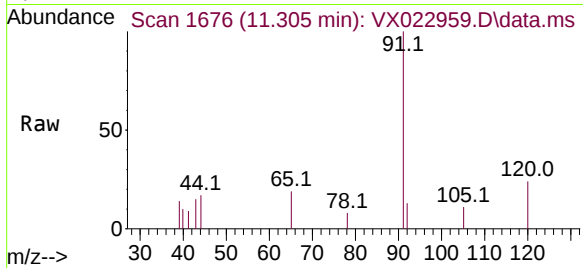

#79
2-Chlorotoluene
Concen: 0.20 ug/l
RT: 11.616 min Scan# 1727
Delta R.T. 0.250 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34

Tgt Ion: 91 Resp: 572
Ion Ratio Lower Upper
91 100
126 22.4 16.6 49.8


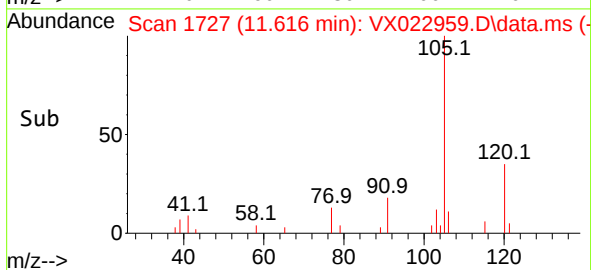

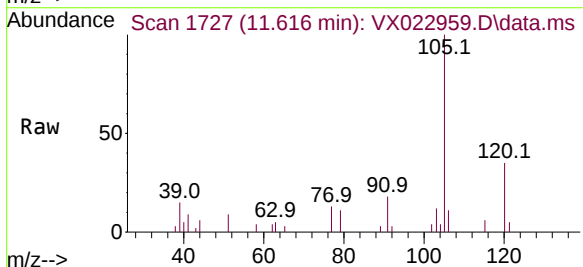




#80
1,3,5-Trimethylbenzene
Concen: 2.88 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34




Instrument :
MSVOA_X
ClientSampleId :
356-349


Tgt Ion:105 Resp: 9031
Ion Ratio Lower Upper
105 100
120 43.6 23.8 71.5

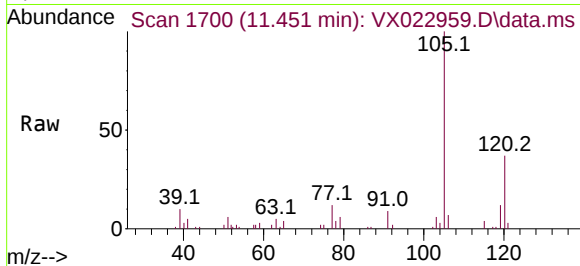

#81
trans-1,4-Dichloro-2-butene
Concen: 62.55 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.061 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34

Tgt Ion: 75 Resp: 28444
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#


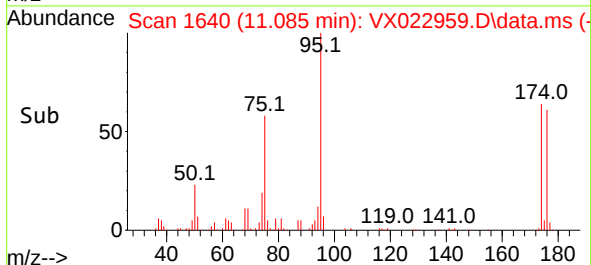
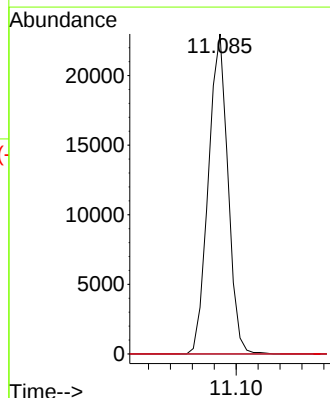
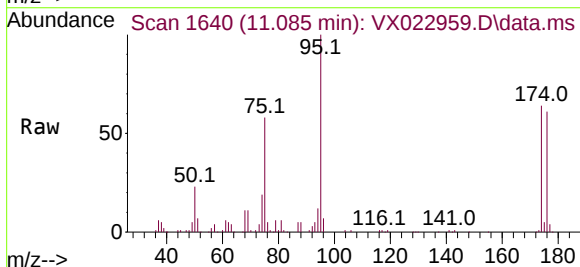


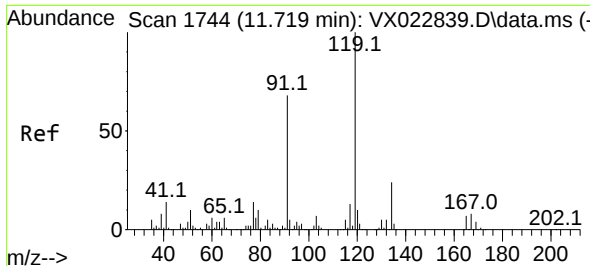

#83
tert-Butylbenzene
Concen: 0.90 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.037 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34




Instrument :
MSVOA_X
ClientSampleId :
356-349


Tgt Ion:119 Resp: 2659
Ion Ratio Lower Upper
119 100
91 99.5 27.9 83.7#
134 0.0 11.3 33.9#

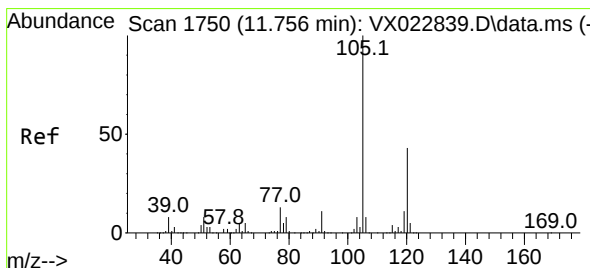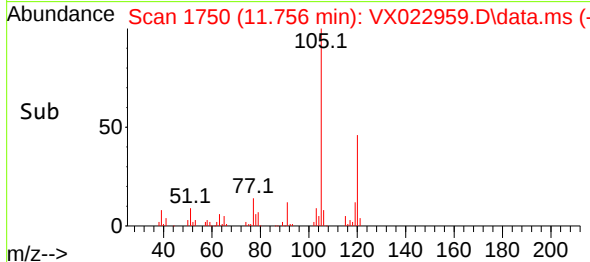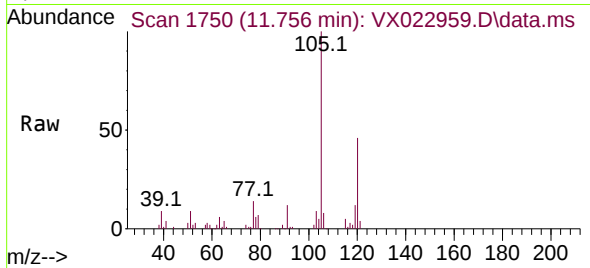

#84
1,2,4-Trimethylbenzene
Concen: 7.12 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34

Tgt Ion:105 Resp: 22467
Ion Ratio Lower Upper
105 100
120 42.6 22.4 67.3


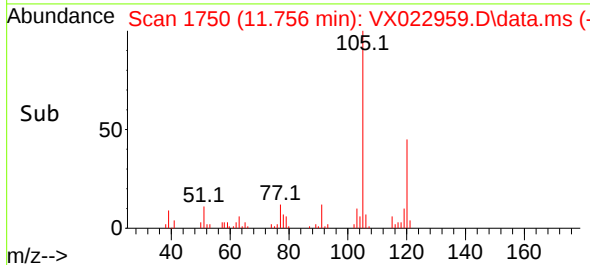

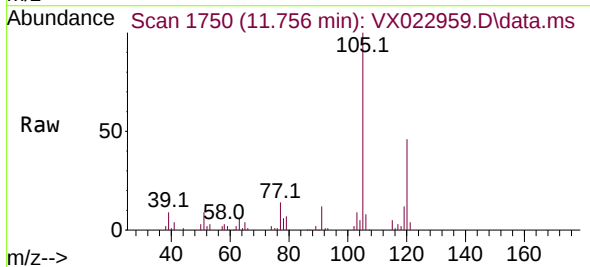




#85
sec-Butylbenzene
Concen: 5.62 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.140 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34




Instrument :
MSVOA_X
ClientSampleId :
356-349


Tgt Ion:105 Resp: 22467
Ion Ratio Lower Upper
105 100
134 0.0 10.0 29.8#



#89
n-Butylbenzene
Concen: 0.40 ug/l
RT: 12.323 min Scan# 1843
Delta R.T. -0.012 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34

Tgt Ion: 91 Resp: 1219
Ion Ratio Lower Upper
91 100
92 21.2 27.4 82.0#
134 104.8 13.2 39.5#


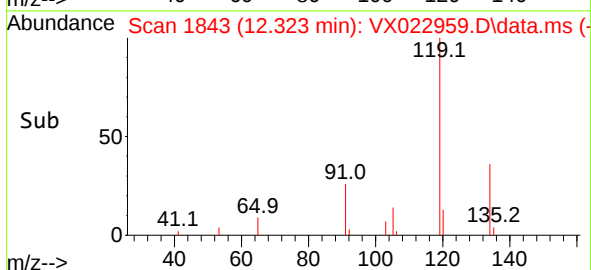






#90
Hexachloroethane
Concen: 34.12 ug/l
RT: 12.414 min Scan# 1858
Delta R.T. -0.128 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34




Instrument :
MSVOA_X
ClientSampleId :
356-349


Tgt Ion:117 Resp: 19288
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#

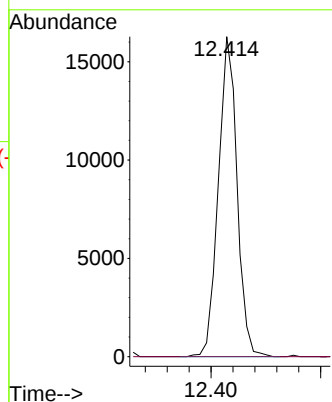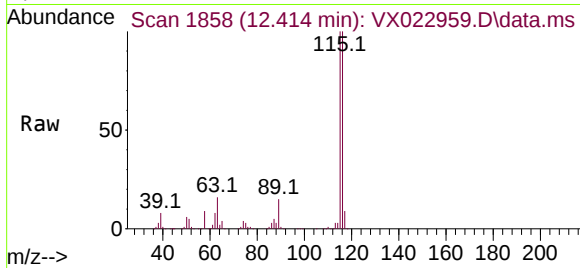

#92
1,2-Dibromo-3-Chloropropane
Concen: 9.65 ug/l
RT: 12.969 min Scan# 1949
Delta R.T. 0.024 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34


Tgt Ion: 75 Resp: 1910
Ion Ratio Lower Upper
75 100
155 0.0 45.3 135.9#
157 0.0 57.7 173.1#

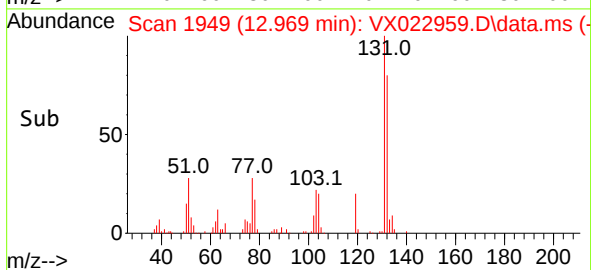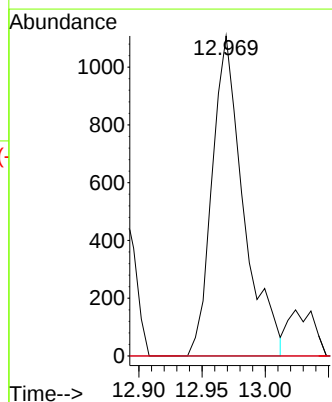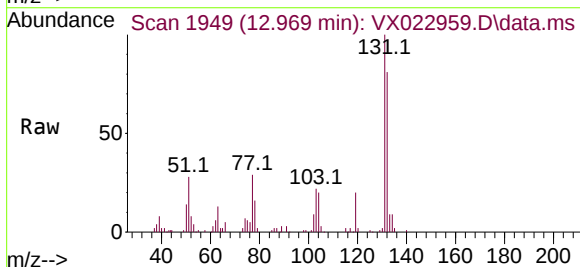

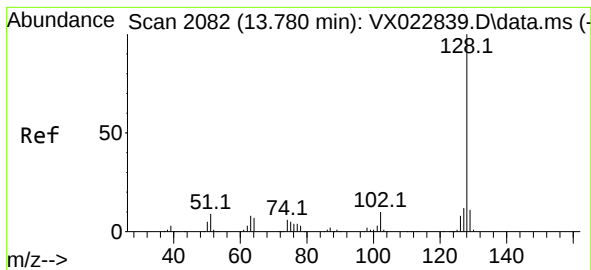

#95
Naphthalene
Concen: 1703.06 ug/l
RT: 13.786 min Scan# 2083
Delta R.T. 0.006 min
Lab File: VX022959.D
Acq: 26 Jun 2021 06:34

Instrument :
MSVOA_X
ClientSampleId :
356-349

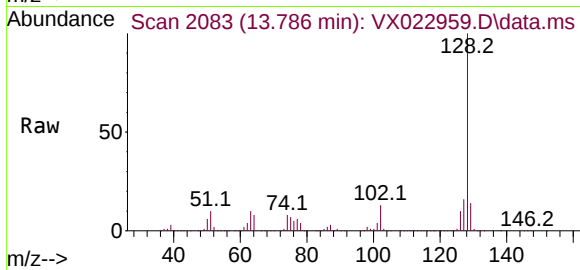

Tgt Ion:128 Resp: 6510861
Ion Ratio Lower Upper
128 100
127 14.8 10.3 15.5
129 12.7 8.8 13.2

