

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062521\
 Data File : VX022932.D
 Acq On : 25 Jun 2021 18:47
 Operator : JC/MD
 Sample : M2838-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE126D3-20210622

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M

Title : SW846 8260

Signal : TIC: VX022932.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.544	232	239	251	rVB	4076	8153	2.13%	0.406%
2	5.397	696	707	719	rBV2	40108	113930	29.70%	5.676%
3	5.562	723	734	745	rBV2	61694	175273	45.69%	8.732%
4	5.964	790	800	813	rBV	53390	139857	36.45%	6.968%
5	6.769	923	932	950	rBV	112110	265428	69.18%	13.224%
6	7.135	985	992	998	rBV4	4717	10242	2.67%	0.510%
7	8.653	1234	1241	1253	rBV	249536	383650	100.00%	19.113%
8	9.275	1339	1343	1348	rBV3	4113	6084	1.59%	0.303%
9	10.055	1466	1471	1482	rBV	247723	341688	89.06%	17.023%
10	11.085	1634	1640	1648	rVB	195993	245553	64.00%	12.233%
11	12.024	1789	1794	1802	rVB	255287	317383	82.73%	15.812%




Sum of corrected areas: 2007241

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062521\
Data File : VX022932.D
Acq On : 25 Jun 2021 18:47
Operator : JC/MD
Sample : M2838-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE126D3-20210622

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

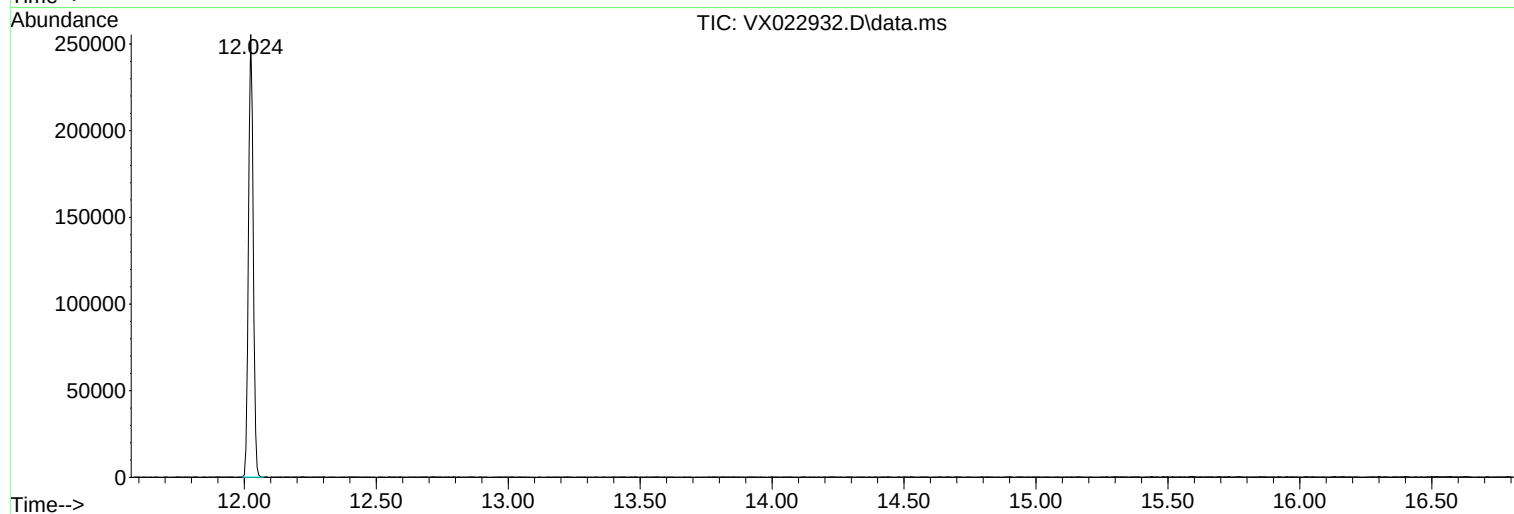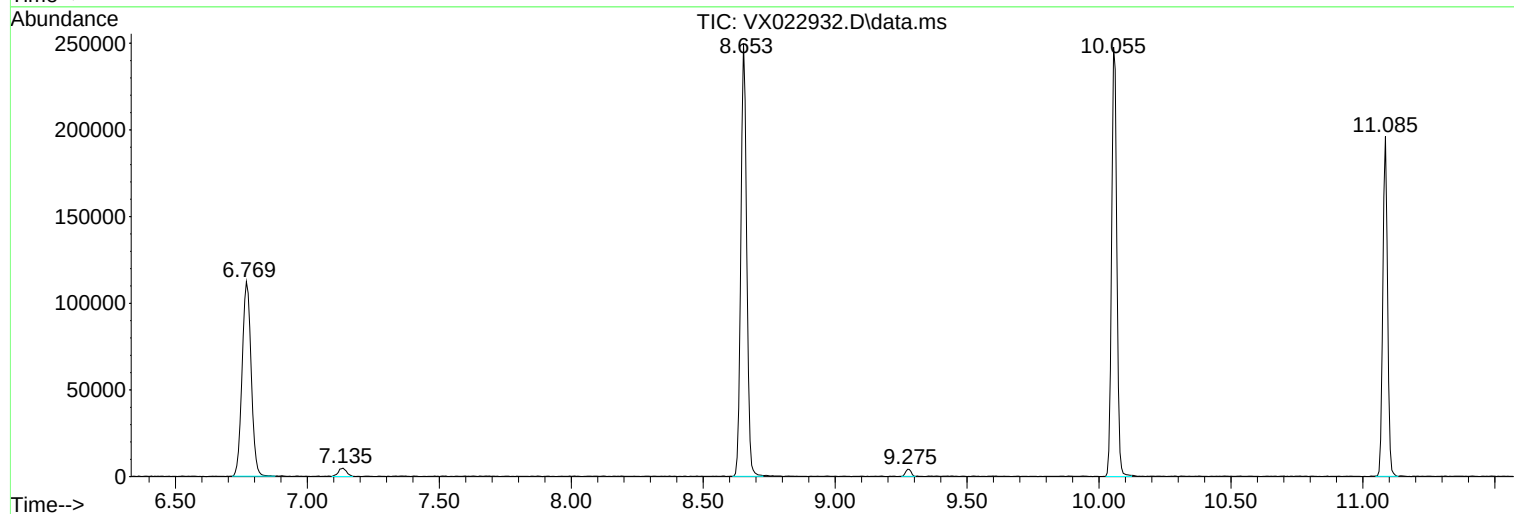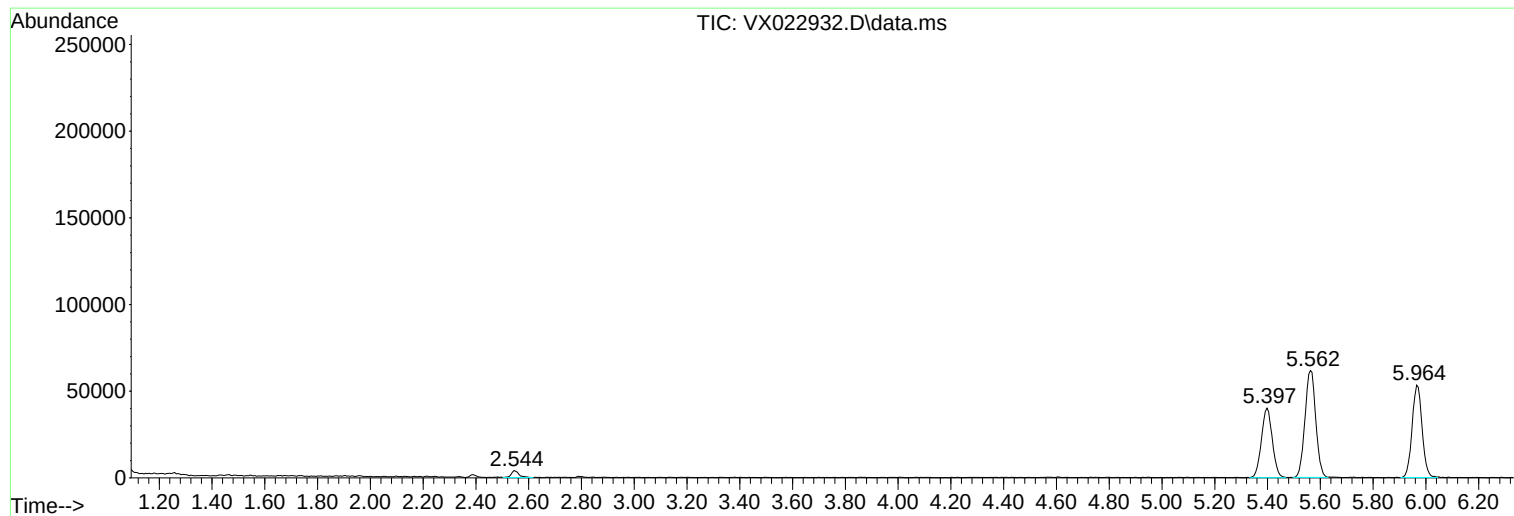

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062521\
Data File : VX022932.D
Acq On : 25 Jun 2021 18:47
Operator : JC/MD
Sample : M2838-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE126D3-20210622

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062521\
Data File : VX022932.D
Acq On : 25 Jun 2021 18:47
Operator : JC/MD
Sample : M2838-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE126D3-20210622

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
