

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062524\
 Data File : VX042036.D
 Acq On : 25 Jun 2024 16:44
 Operator : JC/MD
 Sample : P3056-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-196-DUP-20240620

Quant Time: Jun 26 05:40:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 21 23:51:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	130964	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	202843	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	196811	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	93806	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	66890	44.293	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	88.580%
35) Dibromofluoromethane	5.391	113	63340	44.008	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	88.020%
50) Toluene-d8	8.647	98	232834	46.049	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	92.100%
62) 4-Bromofluorobenzene	11.079	95	85834	46.052	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	92.100%
Target Compounds						
16) Acetone	2.392	43	2670	4.026	ug/l	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062524\
Data File : VX042036.D
Acq On : 25 Jun 2024 16:44
Operator : JC/MD
Sample : P3056-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-196-DUP-20240620

Quant Time: Jun 26 05:40:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 21 23:51:58 2024
Response via : Initial Calibration




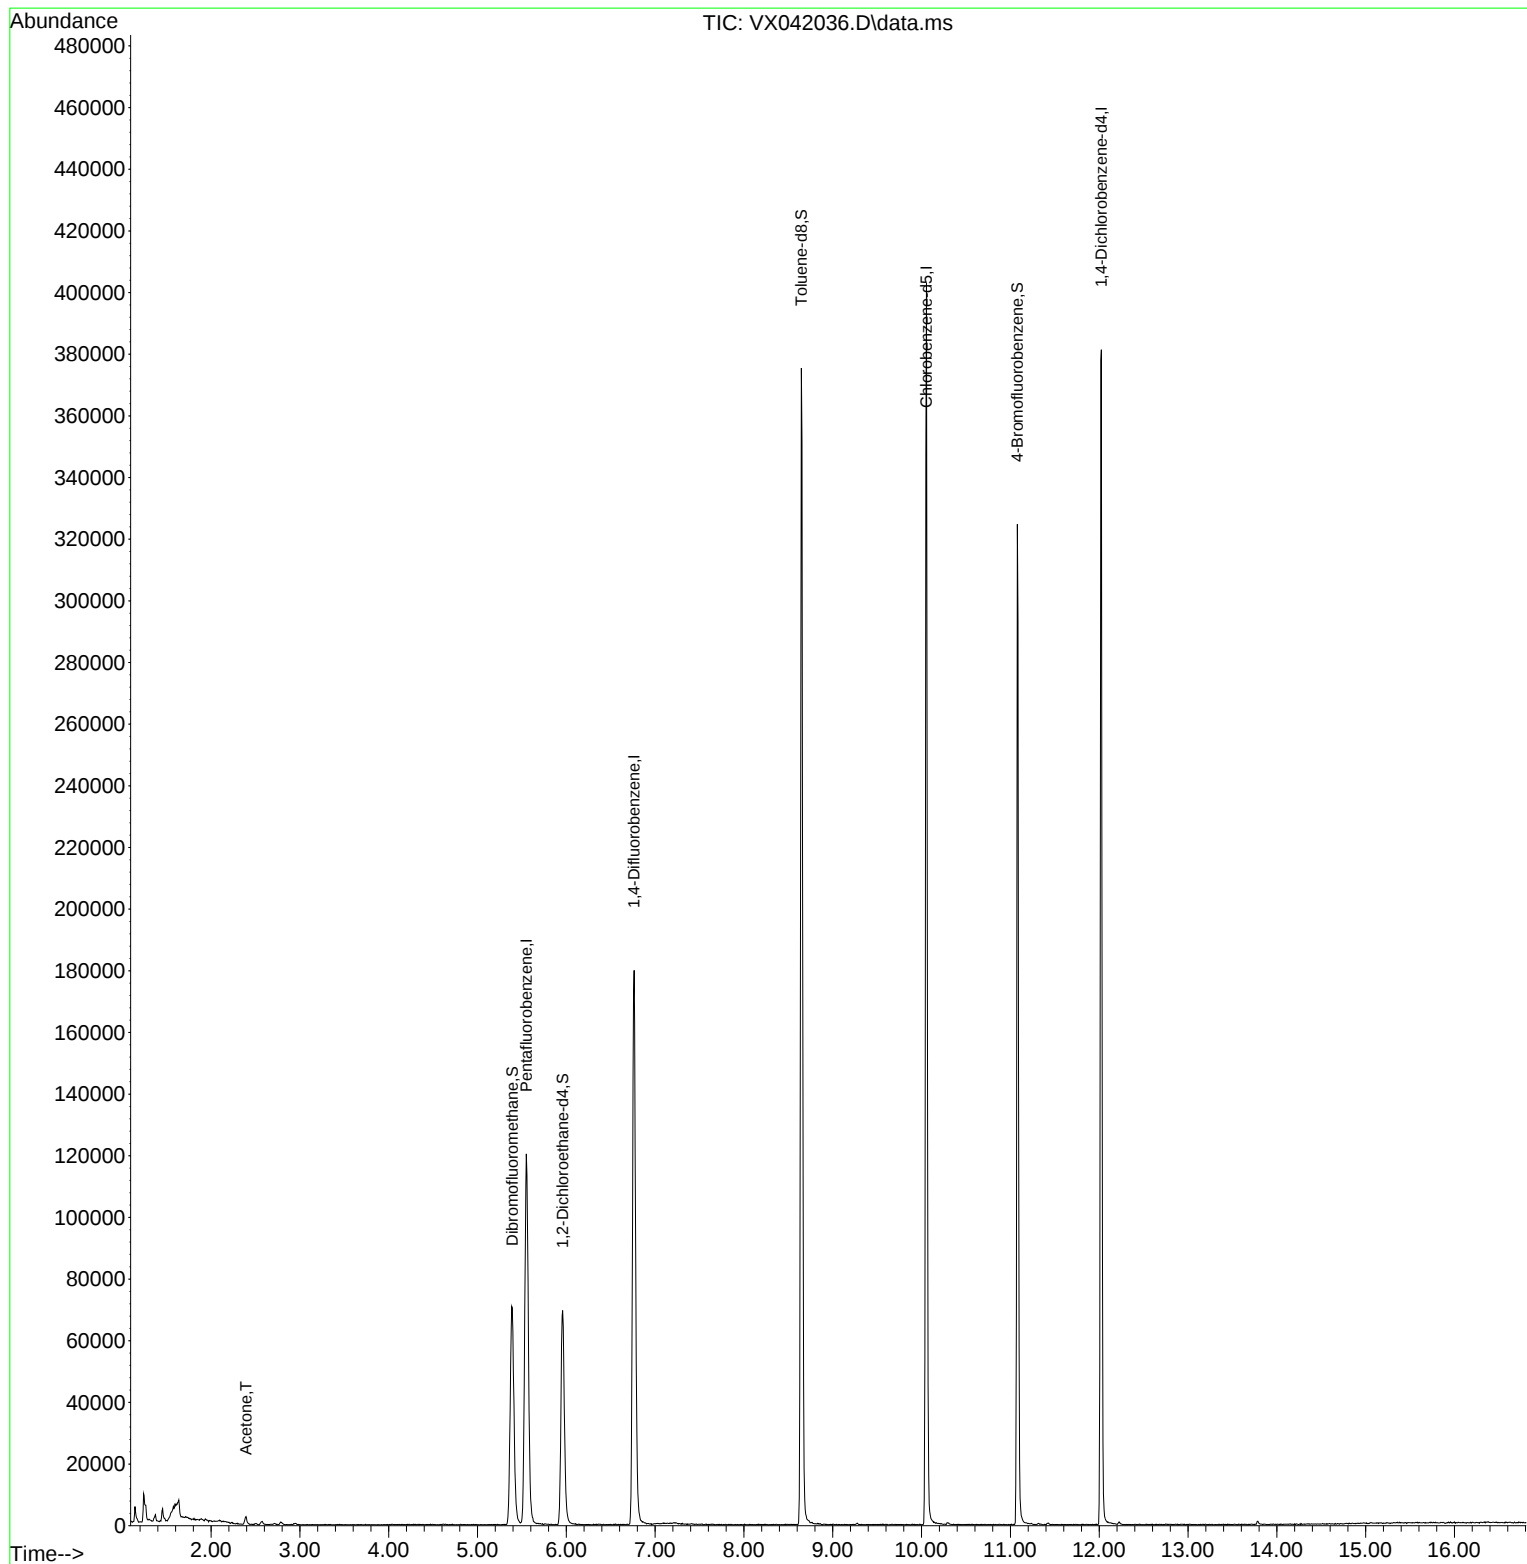


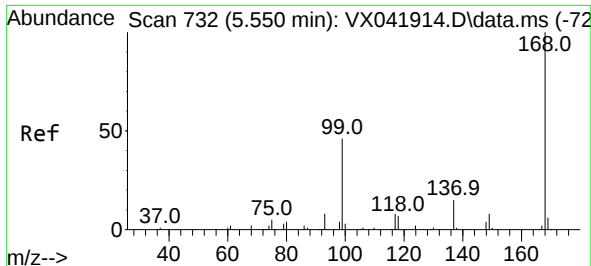

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX042036.D
Acq: 25 Jun 2024 16:44




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-196-DUP-20240620


Tgt Ion:168 Resp: 130964
Ion Ratio Lower Upper
168 100
99 46.3 56.6 85.0#

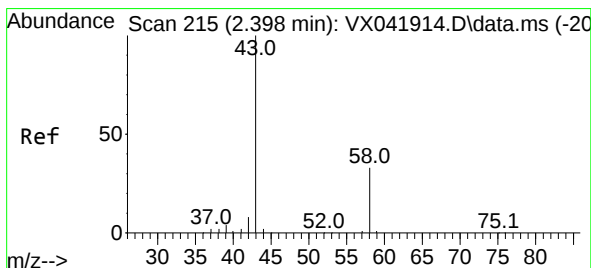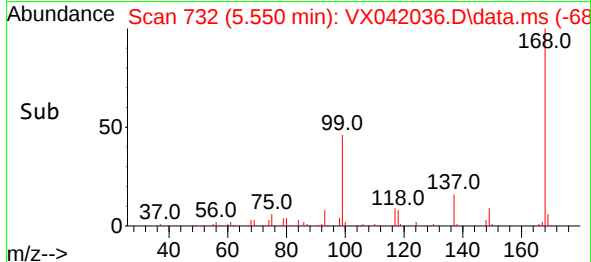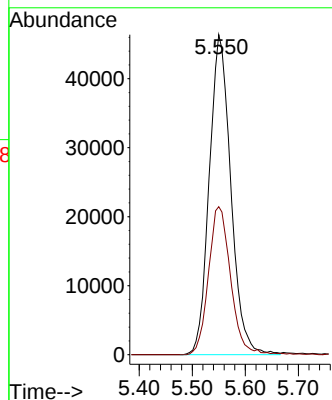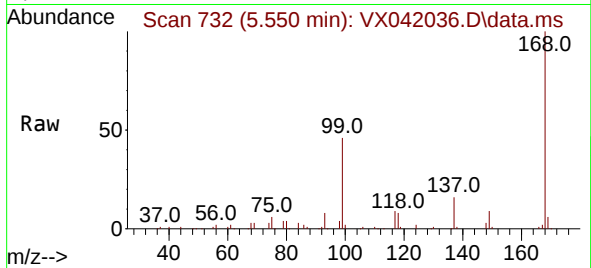

#16
Acetone
Concen: 4.026 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.006 min
Lab File: VX042036.D
Acq: 25 Jun 2024 16:44

Tgt Ion: 43 Resp: 2670
Ion Ratio Lower Upper
43 100
58 31.6 21.9 32.9

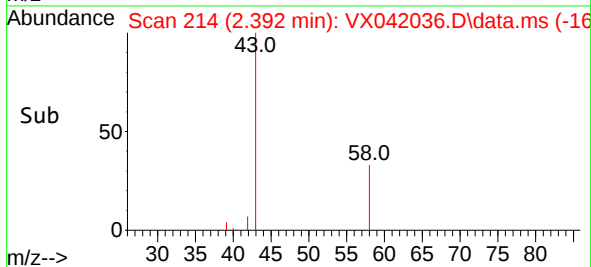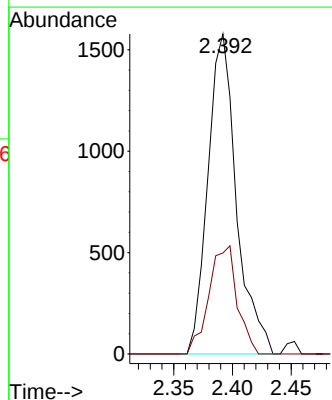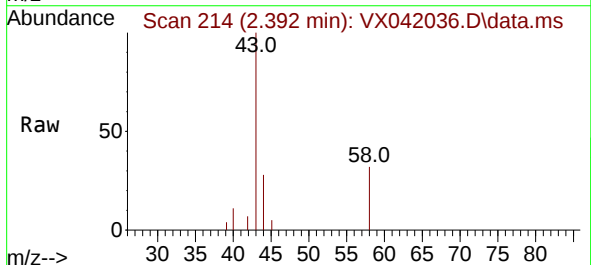

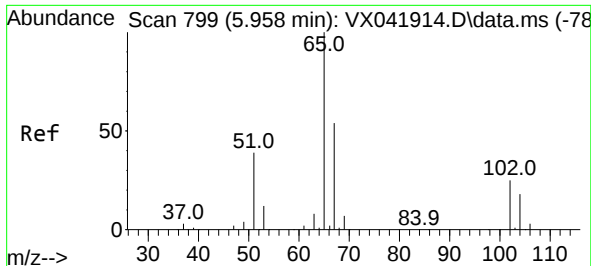

#33

1,2-Dichloroethane-d4

Concen: 44.293 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX042036.D

Acq: 25 Jun 2024 16:44

Instrument :

MSVOA_X

ClientSampleId :





BP-VPB-196-DUP-20240620

Tgt Ion: 65 Resp: 66890

Ion Ratio Lower Upper

65 100

67 53.2 0.0 100.2

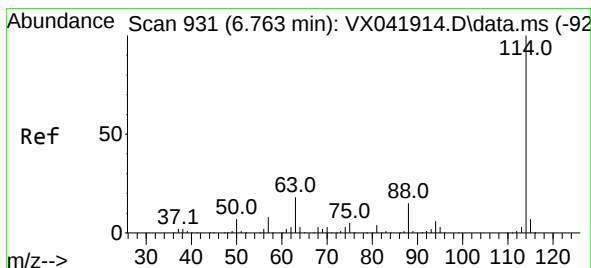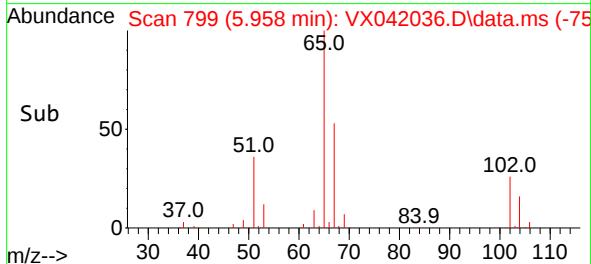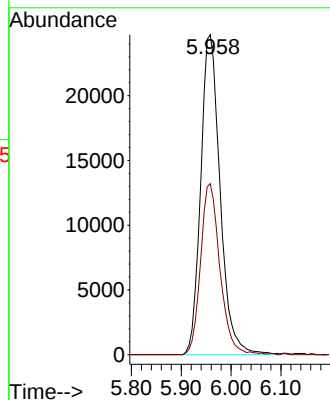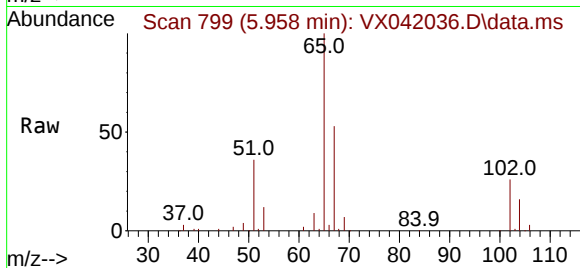

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.000 min

Lab File: VX042036.D

Acq: 25 Jun 2024 16:44




Tgt Ion: 114 Resp: 202843


Ion Ratio Lower Upper

114 100

63 17.1 0.0 45.0

88 14.7 0.0 36.6


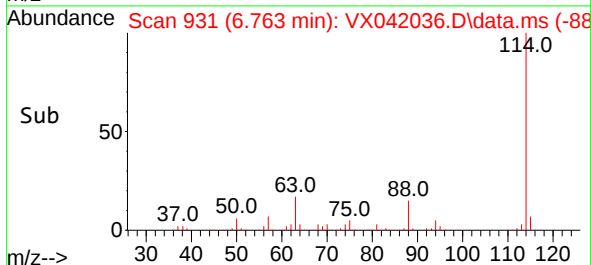
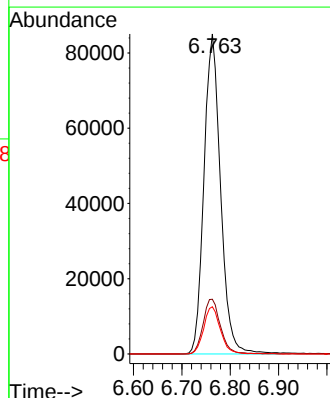
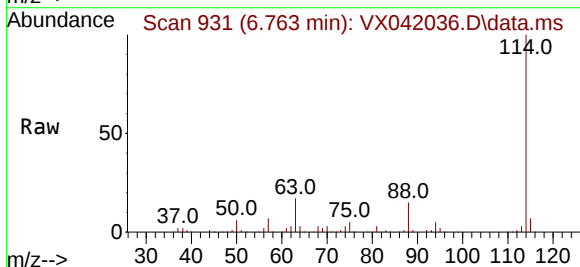


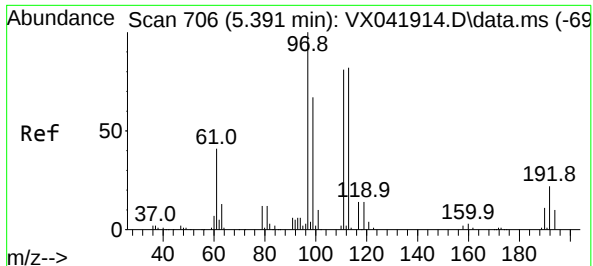

#35
Dibromofluoromethane
Concen: 44.008 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX042036.D
Acq: 25 Jun 2024 16:44




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-196-DUP-20240620


Tgt Ion:113 Resp: 63340
Ion Ratio Lower Upper
113 100
111 102.6 82.9 124.3
192 25.7 13.3 19.9#

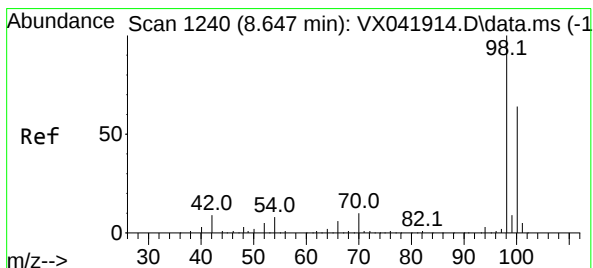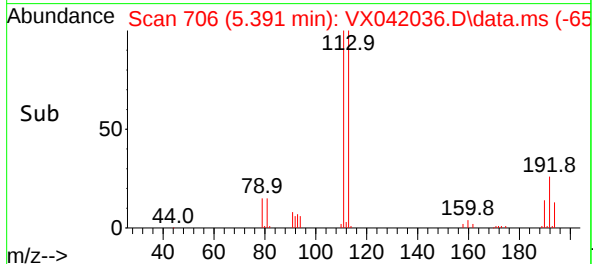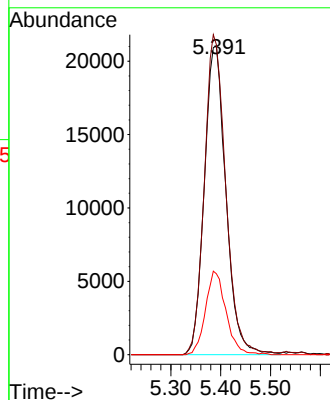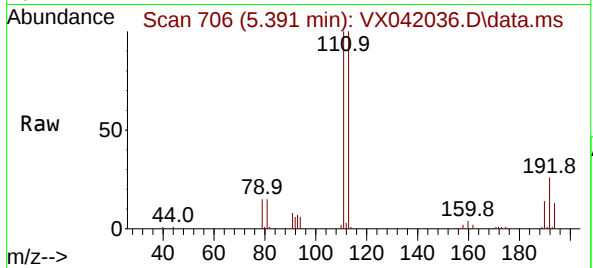

#50
Toluene-d8
Concen: 46.049 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX042036.D
Acq: 25 Jun 2024 16:44

Tgt Ion: 98 Resp: 232834
Ion Ratio Lower Upper
98 100
100 68.1 53.1 79.7


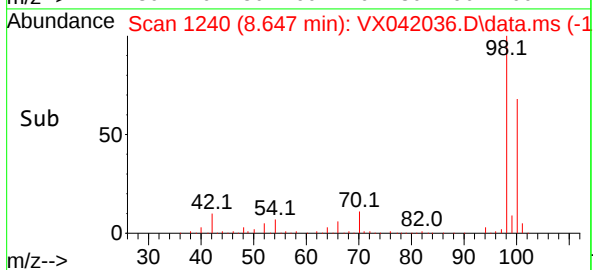
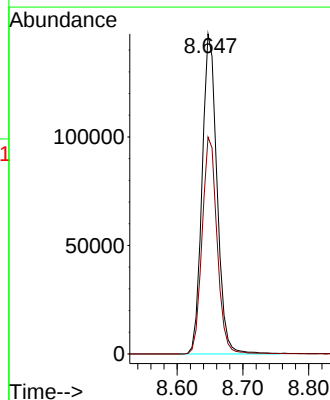
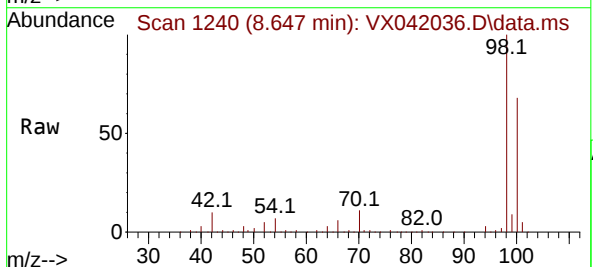


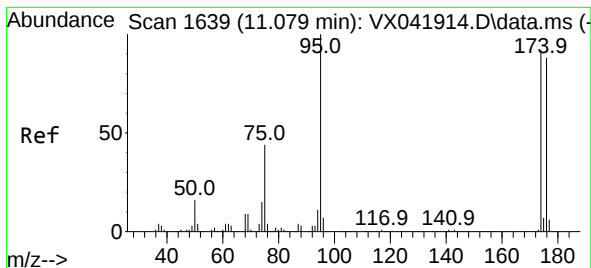

#62
4-Bromofluorobenzene
Concen: 46.052 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX042036.D
Acq: 25 Jun 2024 16:44




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-196-DUP-20240620


Tgt Ion: 95 Resp: 85834
Ion Ratio Lower Upper
95 100
174 97.4 0.0 135.6
176 95.4 0.0 131.0

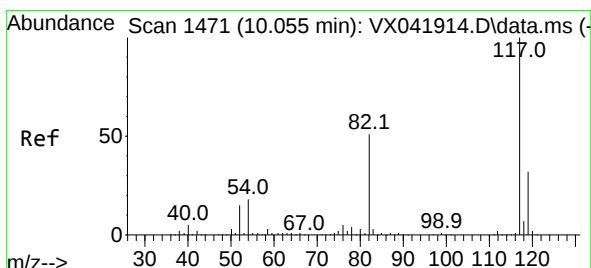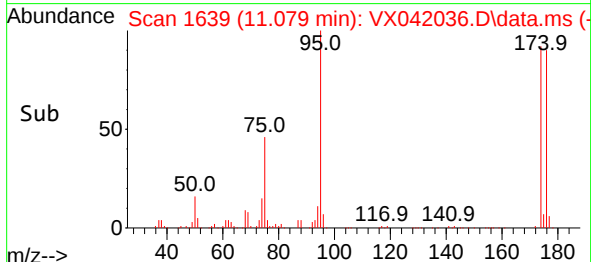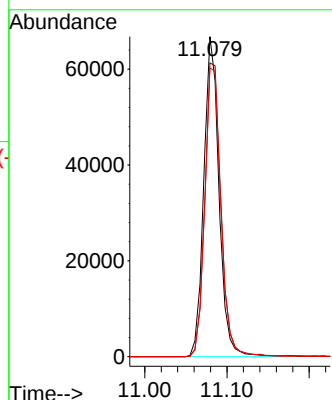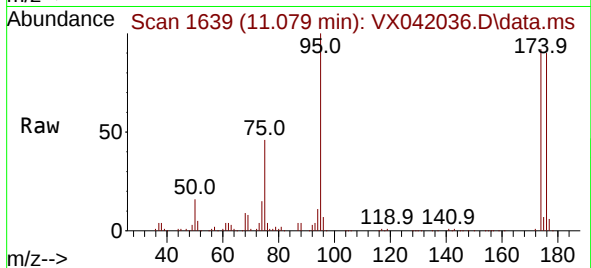

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX042036.D
Acq: 25 Jun 2024 16:44


Tgt Ion: 117 Resp: 196811
Ion Ratio Lower Upper
117 100
82 50.4 46.2 69.4
119 33.5 25.5 38.3

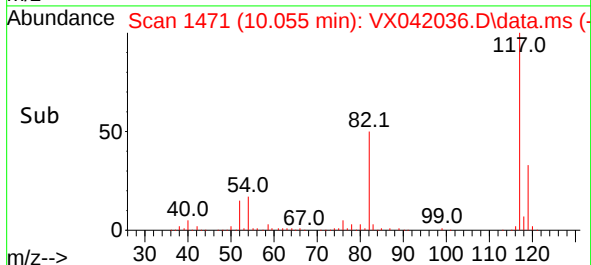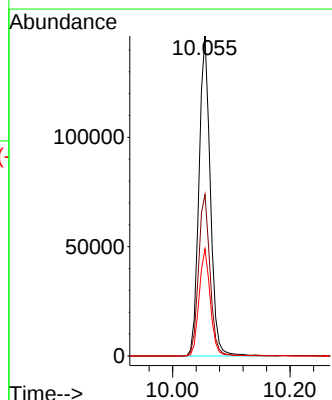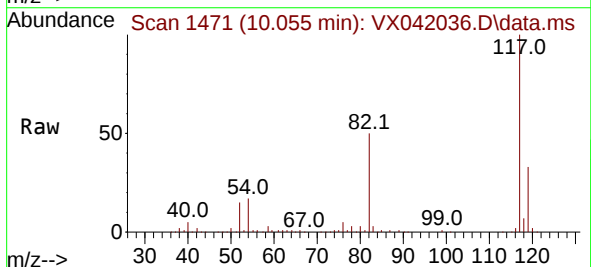

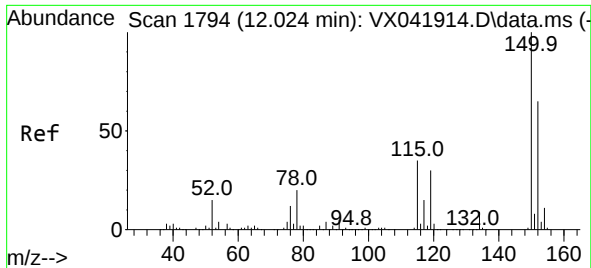

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX042036.D
 Acq: 25 Jun 2024 16:44

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-196-DUP-20240620

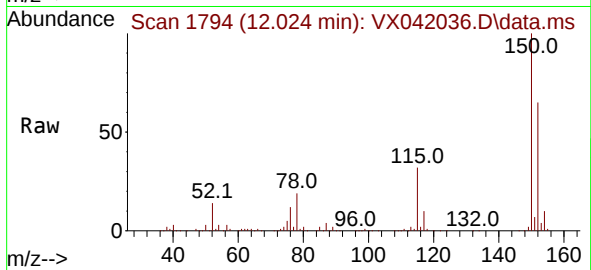

Tgt Ion:152 Resp: 93806
 Ion Ratio Lower Upper
 152 100
 115 52.8 43.3 129.9
 150 157.2 0.0 345.0

