

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062618\
 Data File : VX002894.D
 Acq On : 26 Jun 2018 13:15
 Operator : JC/MD
 Sample : J3497-01 25X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CAS1-WC-L-01

Quant Time: Jun 27 12:54:44 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 25 14:38:05 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	237798	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	329215	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	301804	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	166325	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	157508	47.92	ug/l	0.00
Spiked Amount			Recovery	=	95.84%	
35) Dibromofluoromethane	5.51	113	126845	48.65	ug/l	0.00
Spiked Amount			Recovery	=	97.30%	
50) Toluene-d8	8.72	98	463552	48.69	ug/l	0.00
Spiked Amount			Recovery	=	97.38%	
62) 4-Bromofluorobenzene	11.14	95	160274	43.65	ug/l	0.00
Spiked Amount			Recovery	=	87.30%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
16) Acetone	2.45	43	17456	12.82	ug/l	98
29) Tetrahydrofuran	5.17	42	15661	12.09	ug/l	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062618\
Data File : VX002894.D
Acq On : 26 Jun 2018 13:15
Operator : JC/MD
Sample : J3497-01 25X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CAS1-WC-L-01

Quant Time: Jun 27 12:54:44 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 25 14:38:05 2018
Response via : Initial Calibration

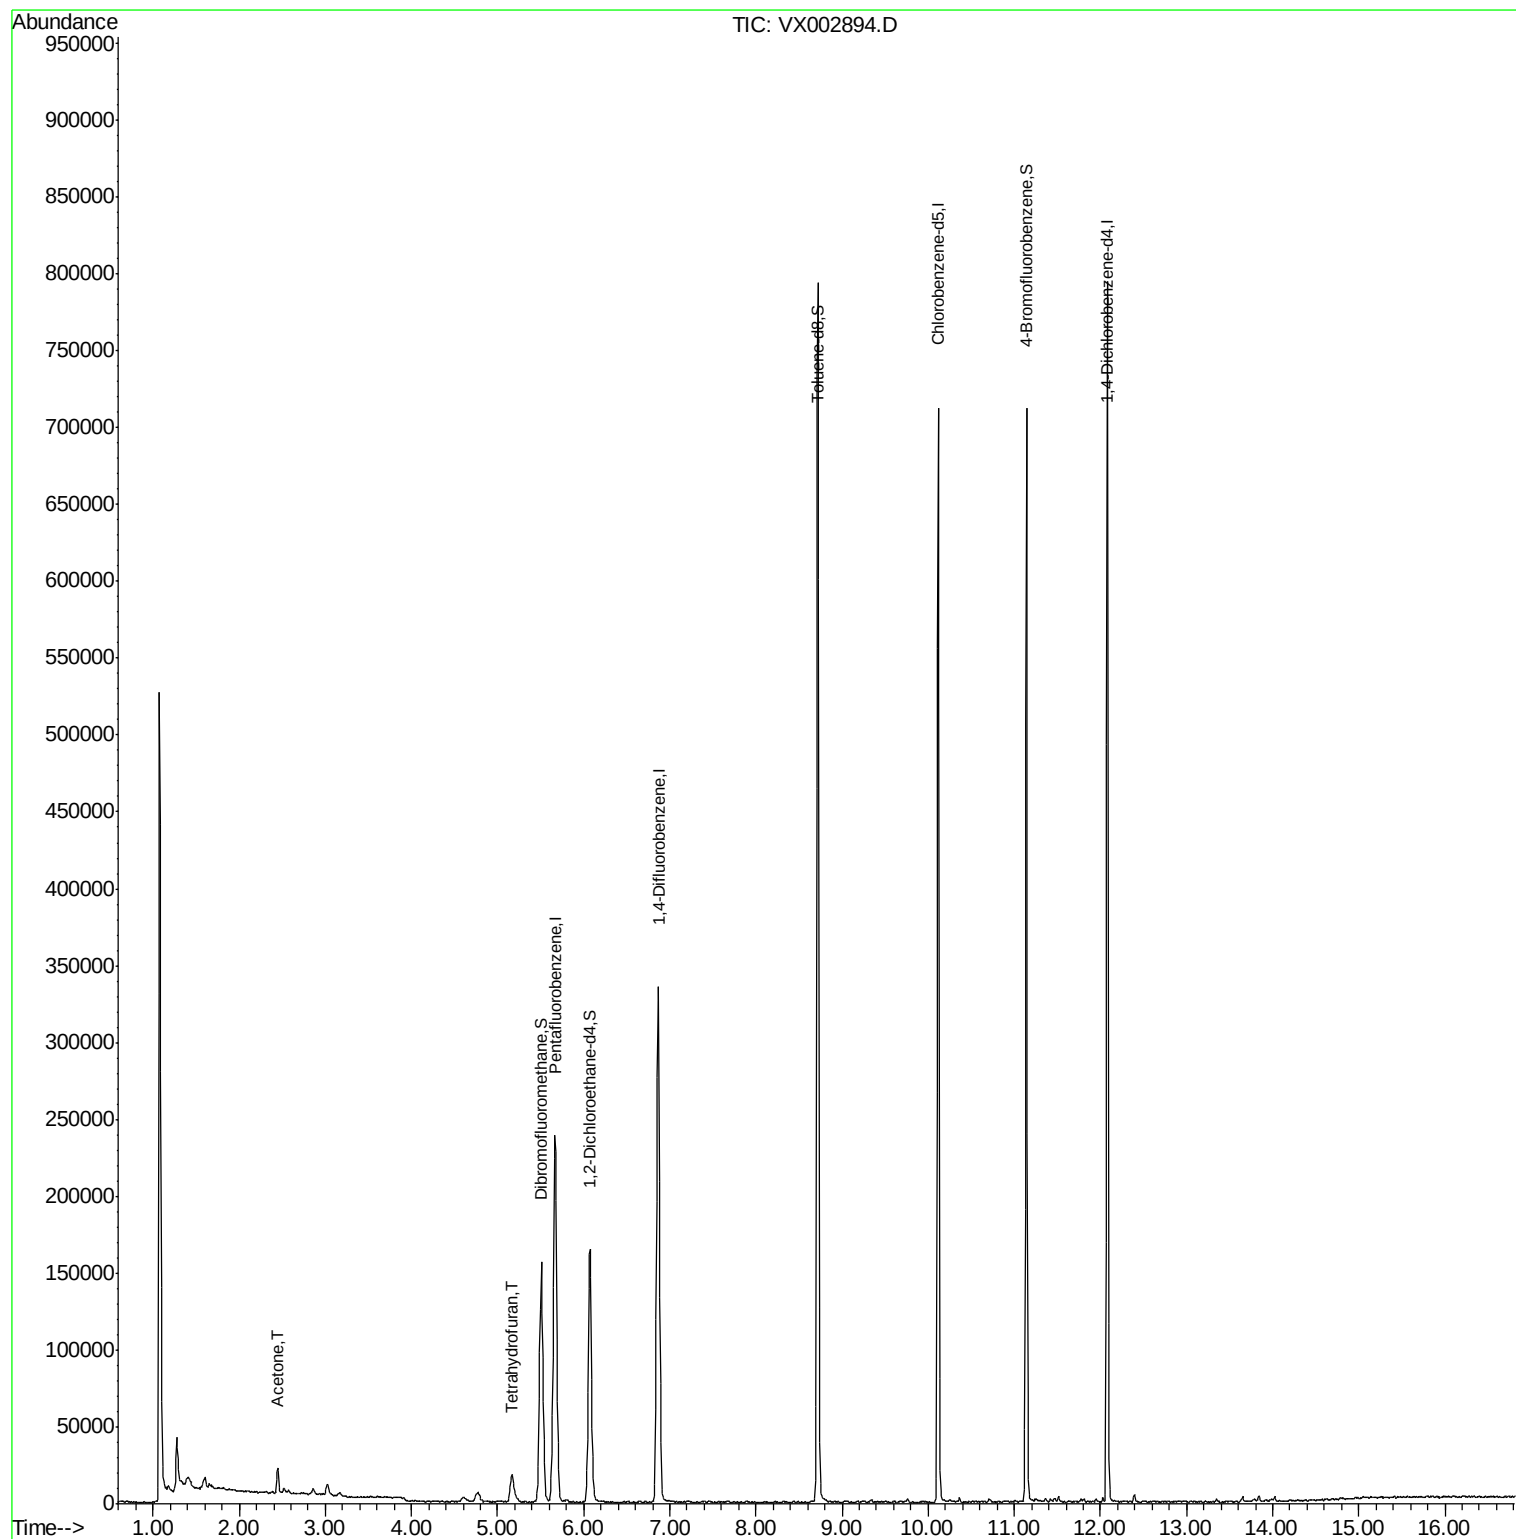

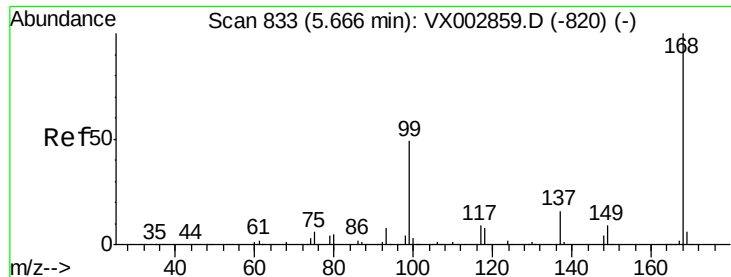

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 833

Delta R.T. -0.00 min

Lab File: VX002894.D

Acq: 26 Jun 2018 13:15

Instrument :

MSVOA_X

ClientSampleId :


CAS1-WC-L-01

Tot Ion:168 Resp: 237798

Ion Ratio Lower Upper

168 100

99 50.8 39.3 58.9

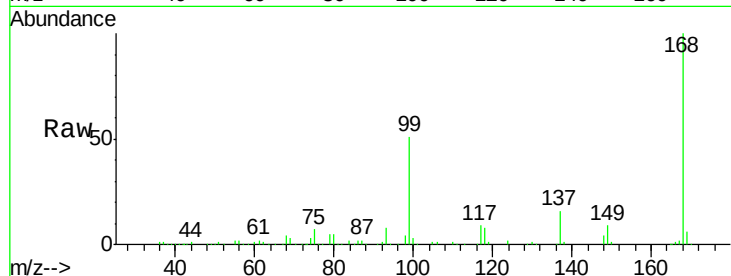

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

80000



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80

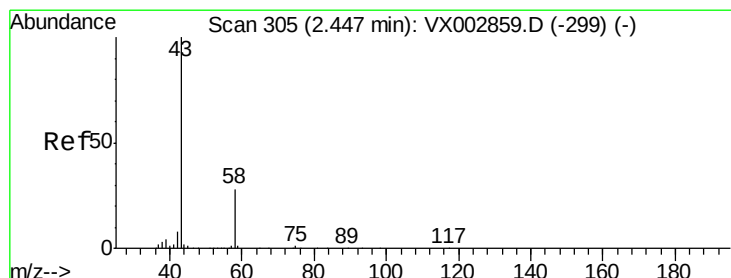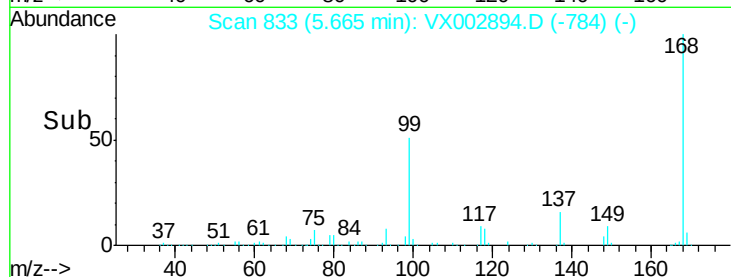

#16

Acetone

Concen: 12.82 ug/l

RT: 2.45 min Scan# 305

Delta R.T. -0.00 min

Lab File: VX002894.D


Acq: 26 Jun 2018 13:15

Tgt Ion: 43 Resp: 17456

Ion Ratio Lower Upper

43 100

58 28.6 22.1 33.1

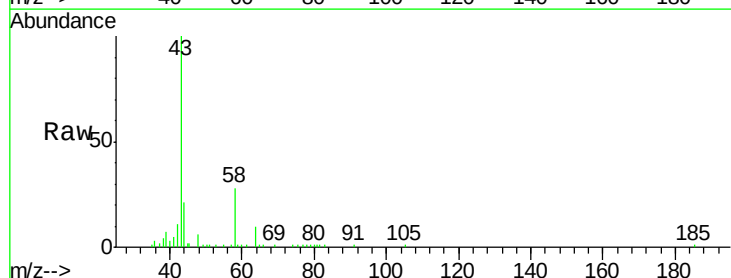

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

2.45

12000

10000

8000


6000


4000

2000

0

Time--> 2.35 2.40 2.45 2.50 2.55

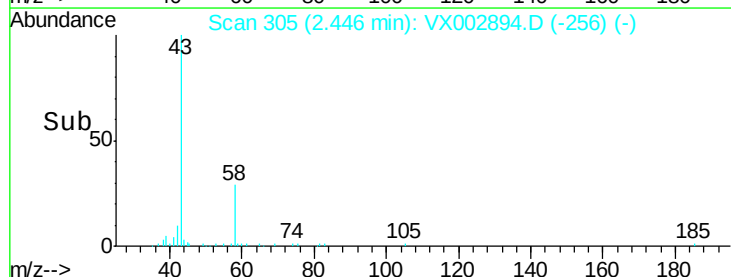

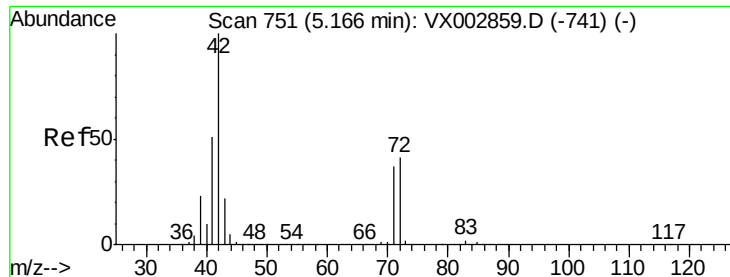

#29

Tetrahydrofuran

Concen: 12.09 ug/l

RT: 5.17 min Scan# 751

Delta R.T. -0.00 min

Lab File: VX002894.D

Acq: 26 Jun 2018 13:15

Instrument :

MSVOA_X

ClientSampleId :

CAS1-WC-L-01





Tot Ion: 42 Resp: 15661

Ion Ratio Lower Upper

42 100

72 42.8 32.0 48.0

71 40.6 30.1 45.1

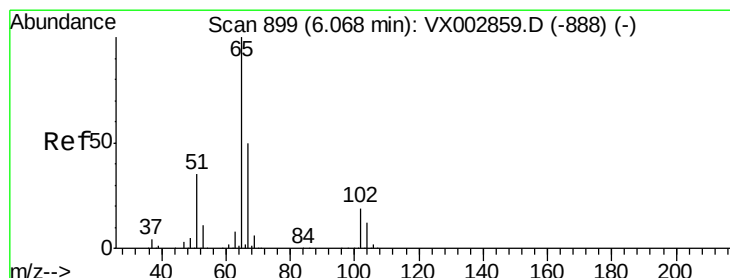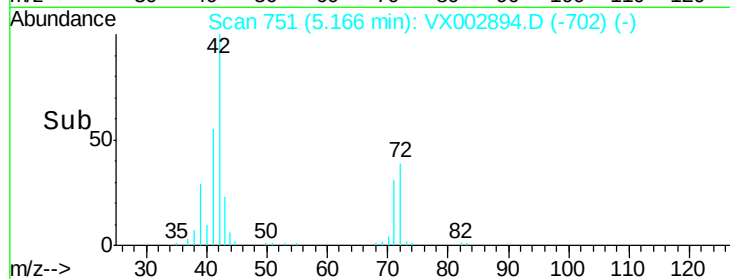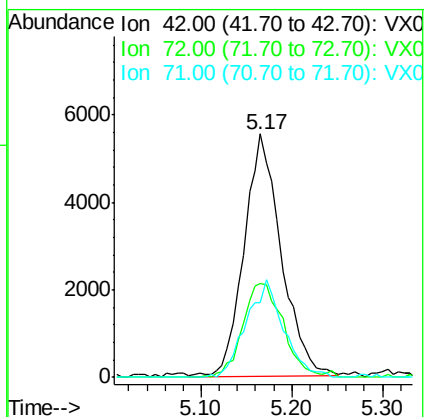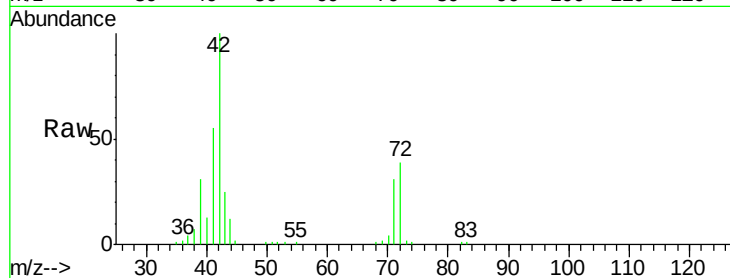

#33

1,2-Dichloroethane-d4

Concen: 47.92 ug/l

RT: 6.07 min Scan# 900

Delta R.T. 0.01 min

Lab File: VX002894.D




Acq: 26 Jun 2018 13:15


Tgt Ion: 65 Resp: 157508

Ion Ratio Lower Upper

65 100

67 51.2 0.0 102.6

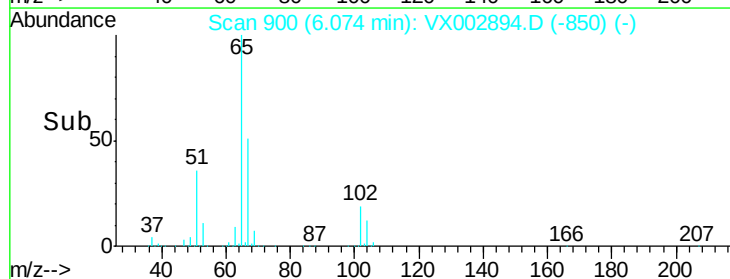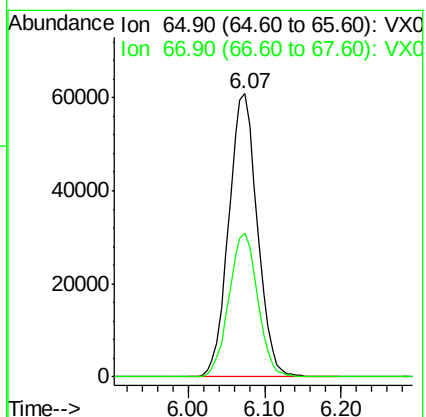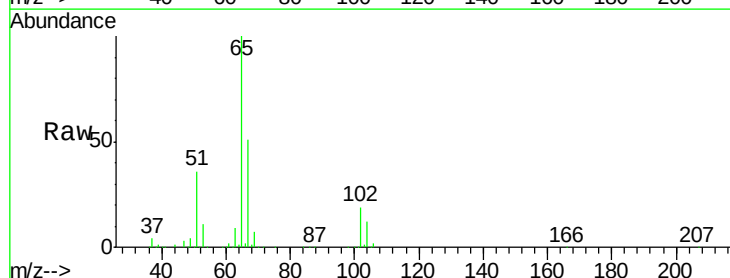

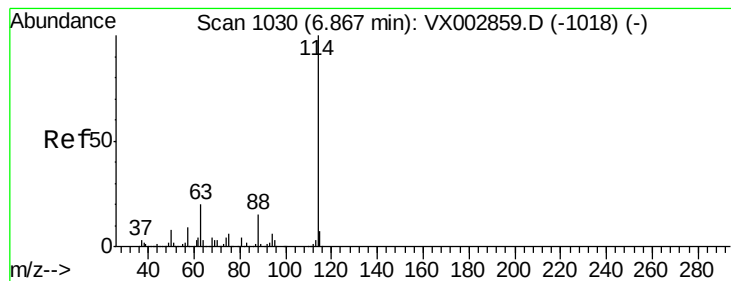

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.87 min Scan# 1030

Delta R.T. -0.00 min

Lab File: VX002894.D

Acq: 26 Jun 2018 13:15

Instrument :

MSVOA_X

ClientSampleId :

CAS1-WC-L-01


Tot Ion:114 Resp: 329215

Ion Ratio Lower Upper

114 100

63 20.1 0.0 41.4




88 15.5 0.0 30.0

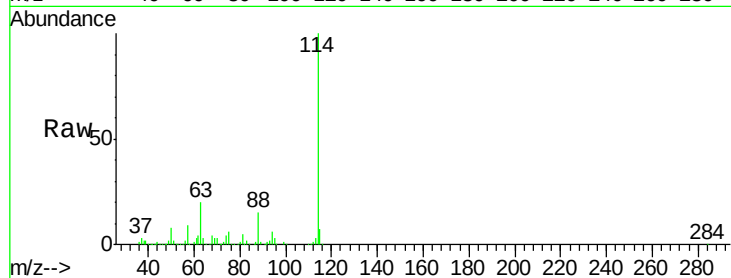

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

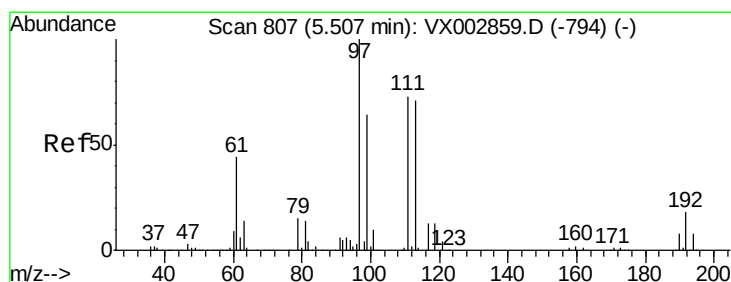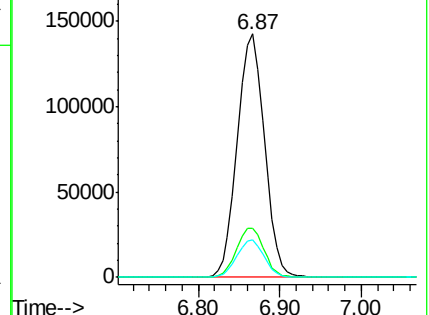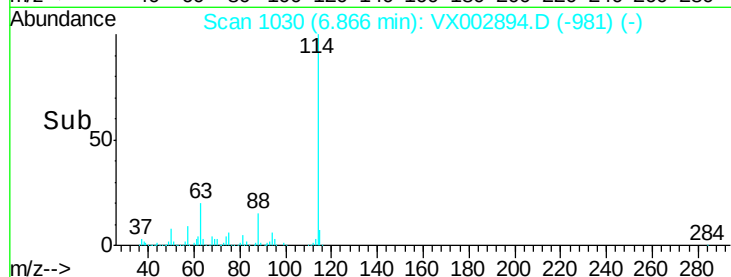

#35

Dibromofluoromethane

Concen: 48.65 ug/l

RT: 5.51 min Scan# 807

Delta R.T. -0.00 min

Lab File: VX002894.D

Acq: 26 Jun 2018 13:15


Tgt Ion:113 Resp: 126845

Ion Ratio Lower Upper

113 100

111 101.7 81.4 122.0



192 24.1 19.1 28.7

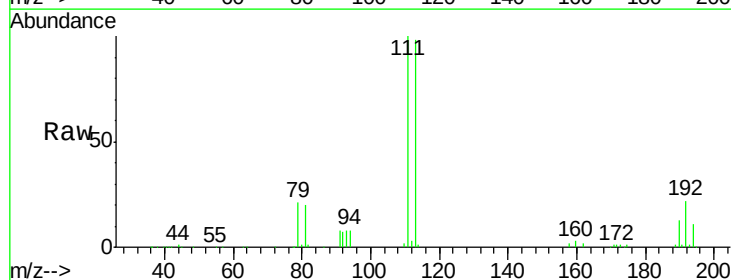


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

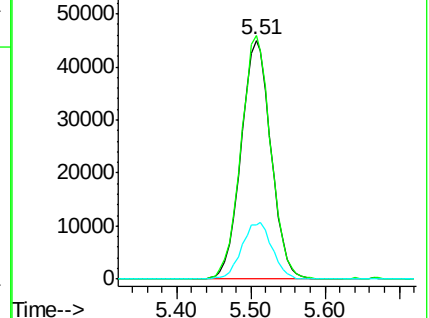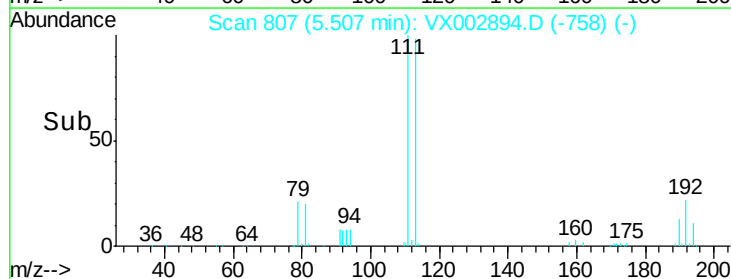

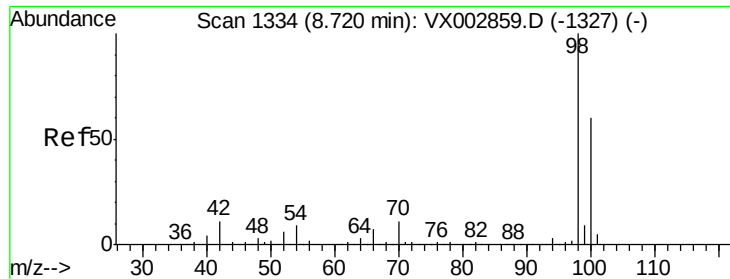

#50

Toluene-d8

Concen: 48.69 ug/l

RT: 8.72 min Scan# 1334

Delta R.T. 0.00 min

Lab File: VX002894.D

Acq: 26 Jun 2018 13:15

Instrument :

MSVOA_X

ClientSampleId :


CAS1-WC-L-01

Tot Ion: 98 Resp: 46352

Ion Ratio Lower Upper




98 100

100 63.8 50.9 76.3

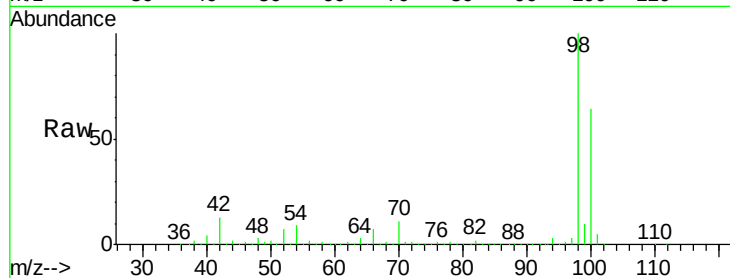

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

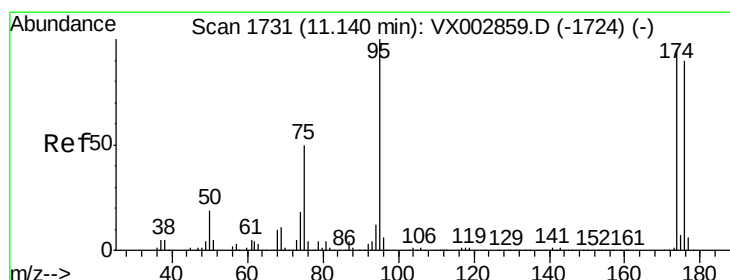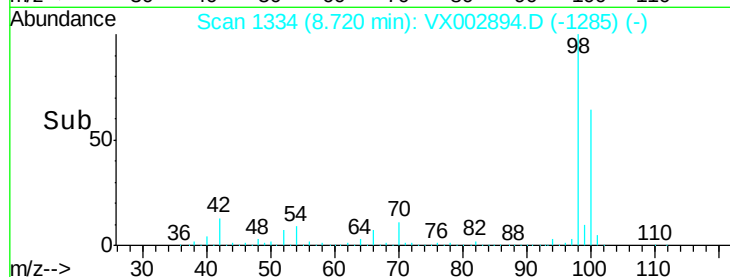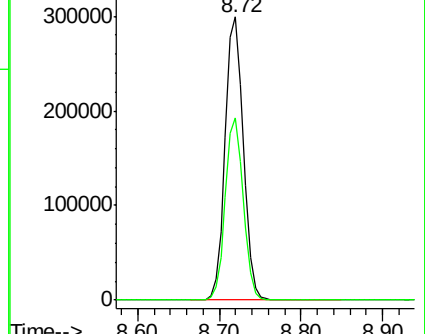

#62

4-Bromofluorobenzene

Concen: 43.65 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.00 min

Lab File: VX002894.D

Acq: 26 Jun 2018 13:15


Tgt Ion: 95 Resp: 160274

Ion Ratio Lower Upper

95 100

174 96.2 0.0 187.4



176 93.3 0.0 181.0

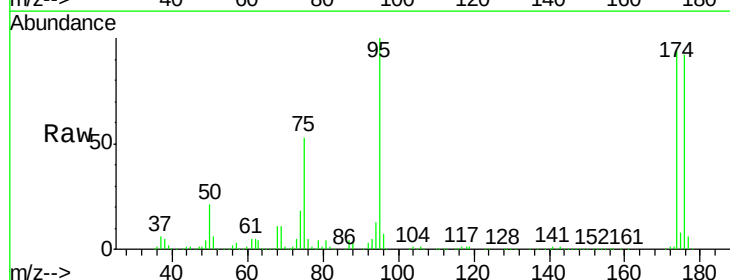


Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

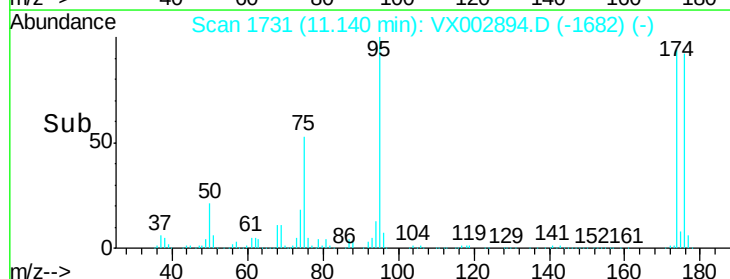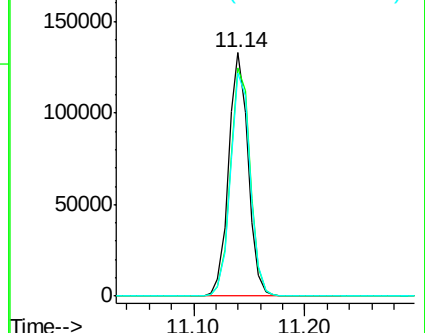


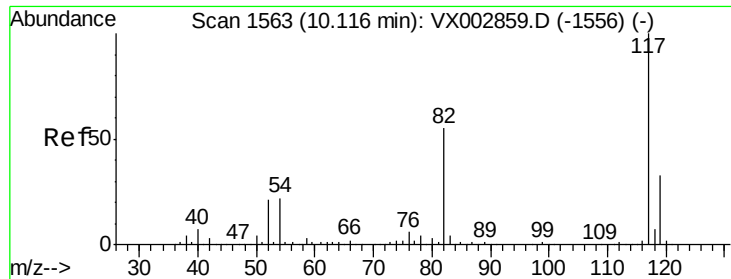




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1563
Delta R.T. -0.00 min
Lab File: VX002894.D
Acq: 26 Jun 2018 13:15

Instrument :
MSVOA_X
ClientSampled :
CAS1-WC-L-01

Tot Ion:117 Resp: 301804
Ion Ratio Lower Upper
117 100
82 54.1 45.0 67.4
119 31.9 25.8 38.6

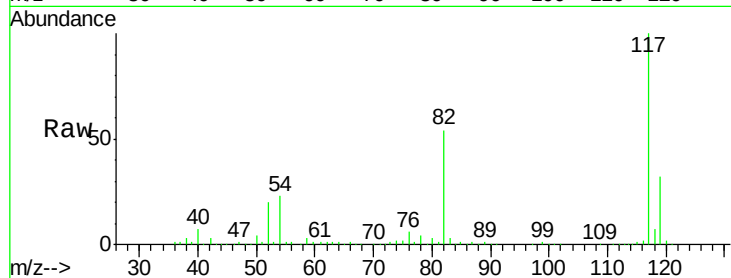


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

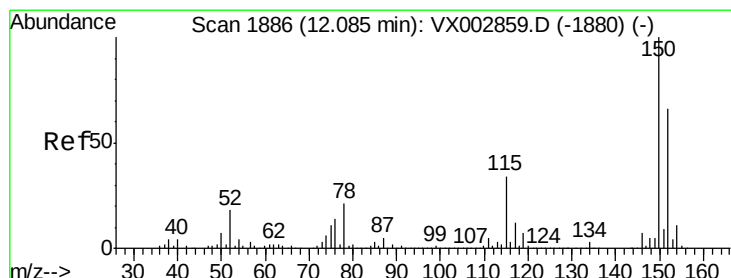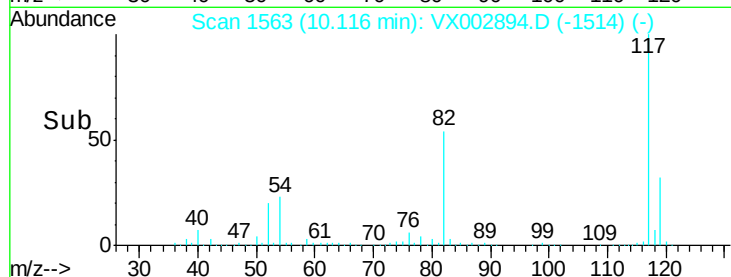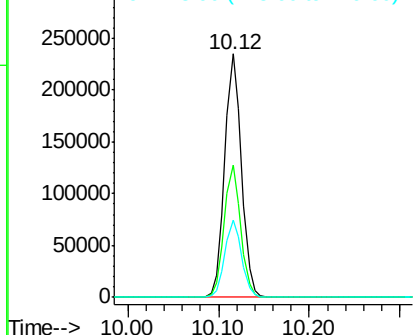

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.08 min Scan# 1885
Delta R.T. -0.01 min
Lab File: VX002894.D
Acq: 26 Jun 2018 13:15

Tgt Ion:152 Resp: 166325
Ion Ratio Lower Upper
152 100
115 54.5 40.1 120.2
150 155.6 0.0 347.2

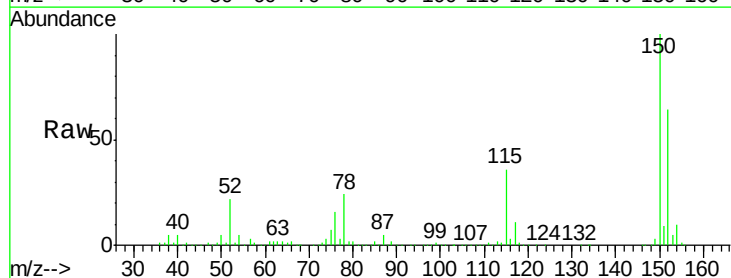

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

