

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062618\
 Data File : VX002914.D
 Acq On : 27 Jun 2018 00:36
 Operator : JC/MD
 Sample : J3707-08 50X
 Misc : 5.97g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WP021SB480-13-15-180622

Quant Time: Jun 27 04:34:41 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 25 14:38:05 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	251517	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	352129	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	327973	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	183933	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	169984	48.90	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.80%	
35) Dibromofluoromethane	5.51	113	134979	48.40	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.80%	
50) Toluene-d8	8.72	98	497040	48.81	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.62%	
62) 4-Bromofluorobenzene	11.14	95	174897	44.54	ug/l	0.00
Spiked Amount 50.000			Recovery	=	89.08%	
Target Compounds						
10) Methyl Iodide	2.52	142	1589	6.72	ug/l	# 93
27) cis-1,2-Dichloroethene	4.60	96	9764	3.22	ug/l	78
44) Trichloroethene	7.21	130	1832	0.55	ug/l	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062618\
Data File : VX002914.D
Acq On : 27 Jun 2018 00:36
Operator : JC/MD
Sample : J3707-08 50X
Misc : 5.97µ/5mL/100µL/5.00mL/MSVOA_X/MEOH
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WP021SB480-13-15-180622

Quant Time: Jun 27 04:34:41 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 25 14:38:05 2018
Response via : Initial Calibration

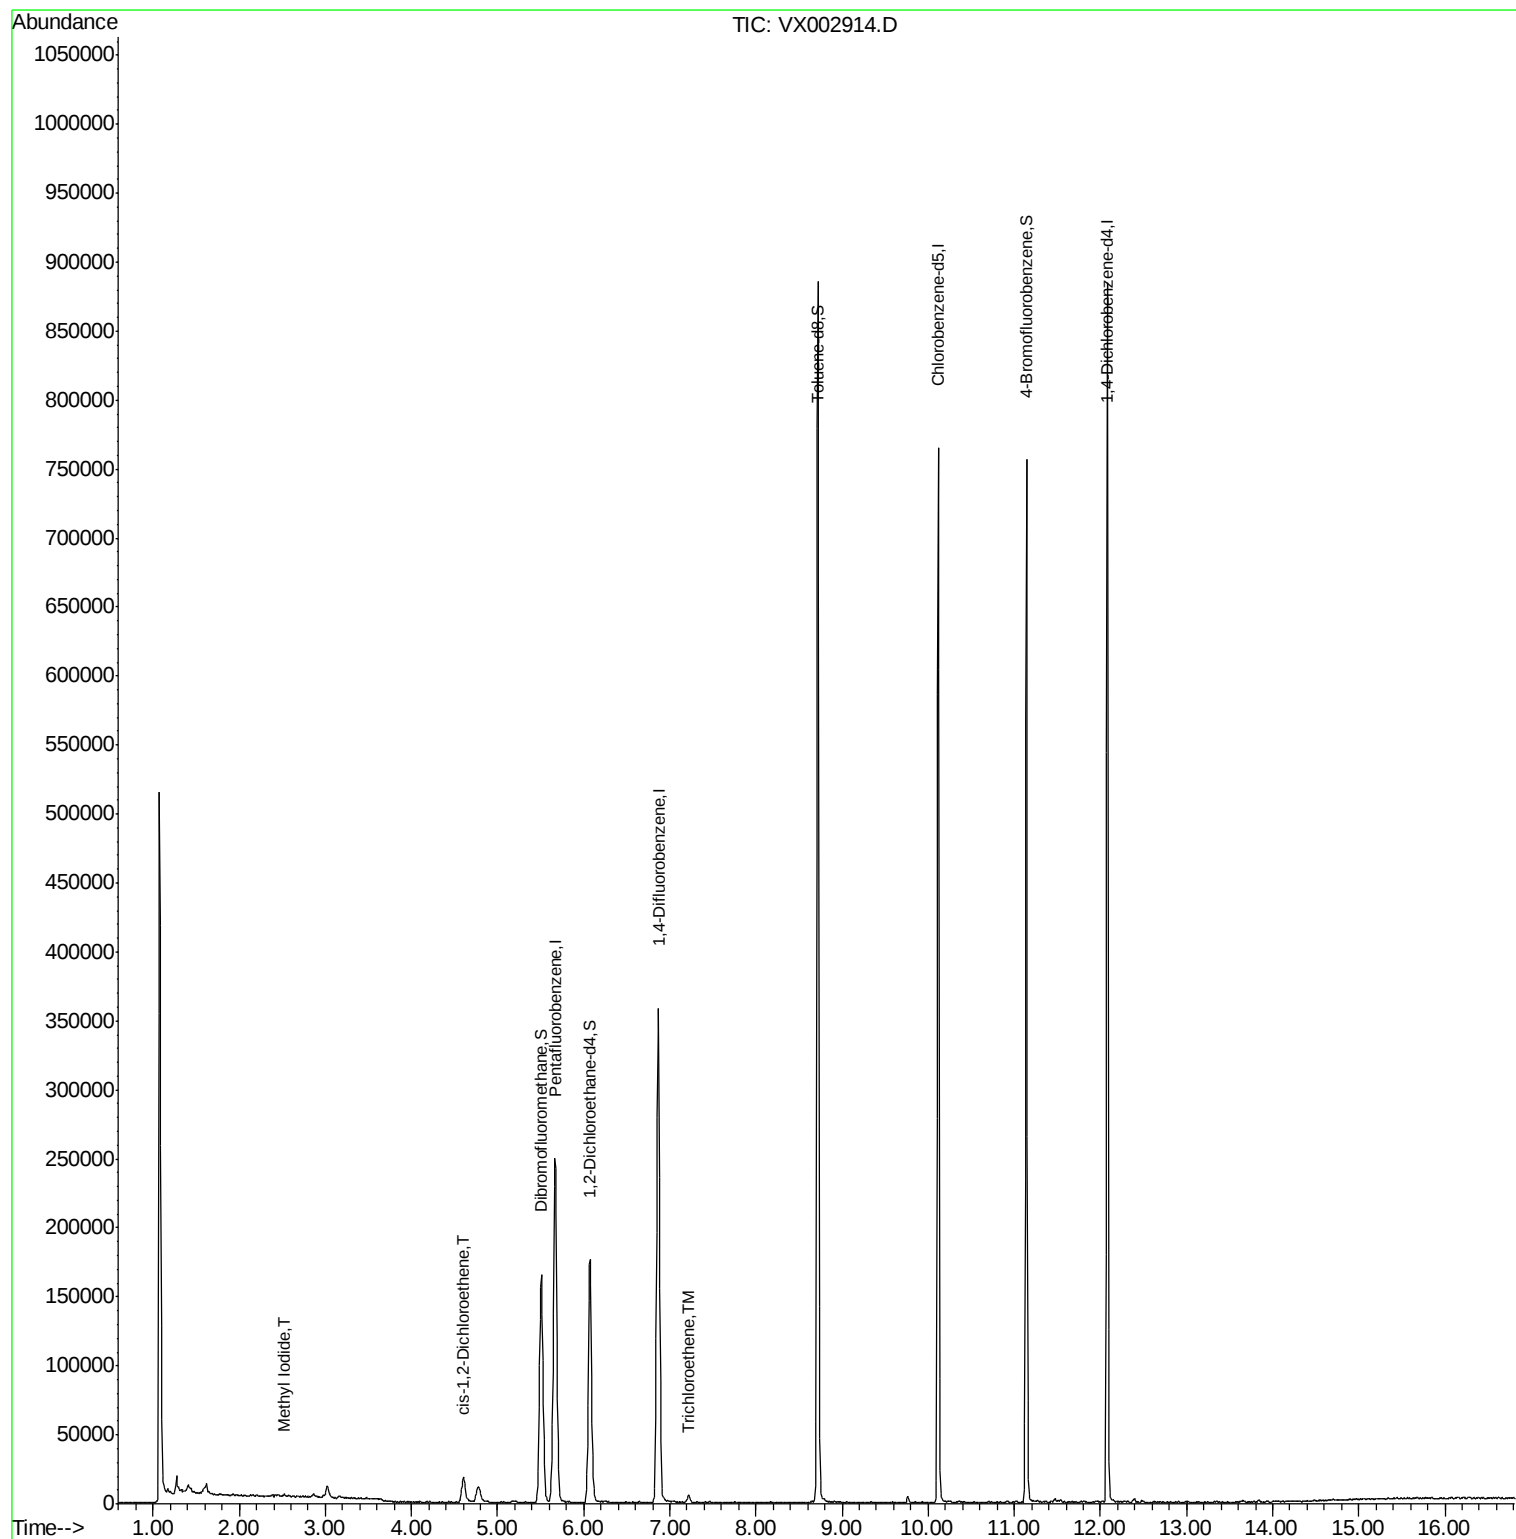



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 833

Delta R.T. -0.00 min

Lab File: VX002914.D

Acq: 27 Jun 2018 00:36

Instrument :

MSVOA_X

ClientSampleId :


WP021SB480-13-15-180622

Tot Ion:168 Resp: 251517

Ion Ratio Lower Upper

168 100

99 51.5 39.3 58.9


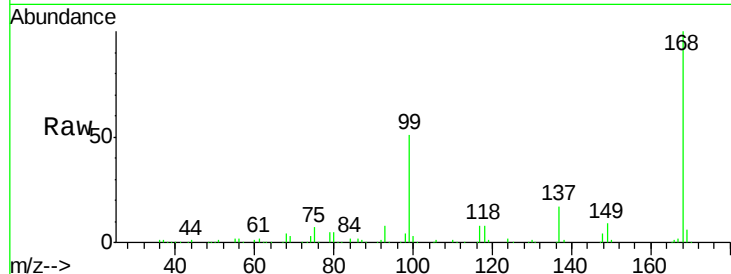


Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

Time-->

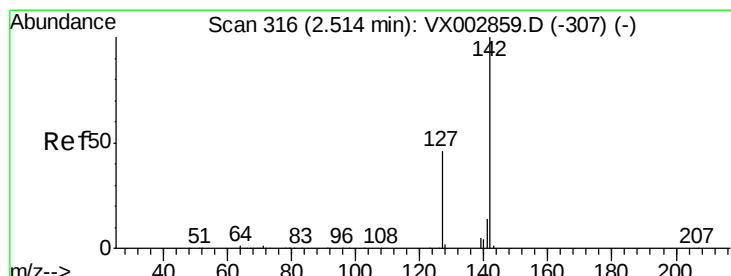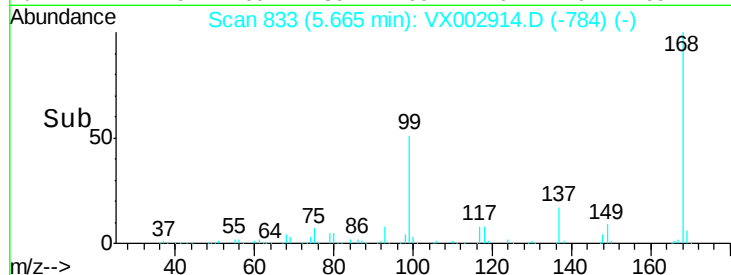

#10

Methyl Iodide

Concen: 6.72 ug/l

RT: 2.52 min Scan# 317

Delta R.T. 0.01 min

Lab File: VX002914.D

Acq: 27 Jun 2018 00:36


Tgt Ion:142 Resp: 1589

Ion Ratio Lower Upper

142 100

127 41.8 36.6 55.0

141 18.0 11.3 16.9#

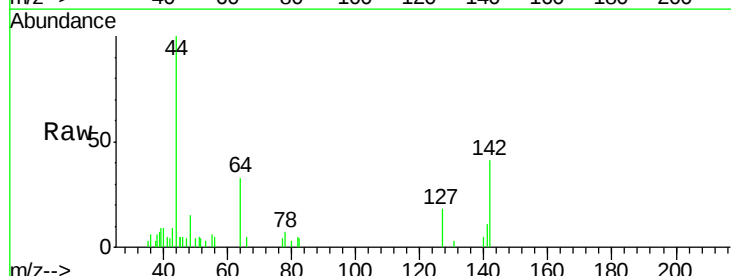


Abundance Ion 141.80 (141.50 to 142.50): V


Ion 126.80 (126.50 to 127.50): V

Ion 140.80 (140.50 to 141.50): V

2.52

Time-->

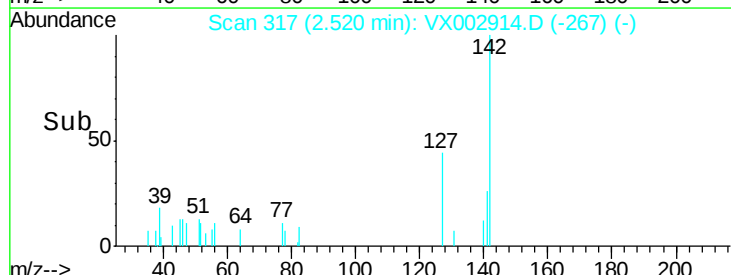

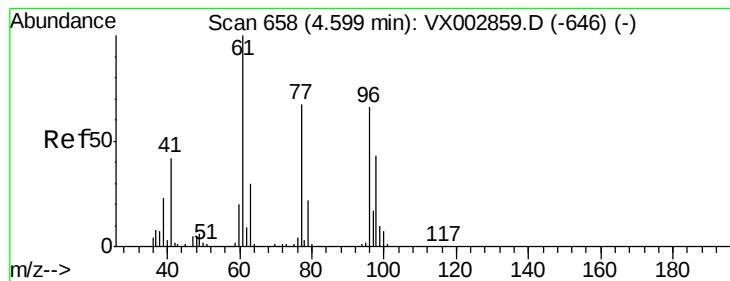

#27

cis-1,2-Dichloroethene

Concen: 3.22 ug/l

RT: 4.60 min Scan# 659

Delta R.T. 0.01 min

Lab File: VX002914.D

Acq: 27 Jun 2018 00:36

Instrument :

MSVOA_X

ClientSampleId :

WP021SB480-13-15-180622


Tot Ion: 96 Resp: 9764

Ion Ratio Lower Upper

96 100

61 202.0 0.0 330.2




98 71.3 0.0 130.2

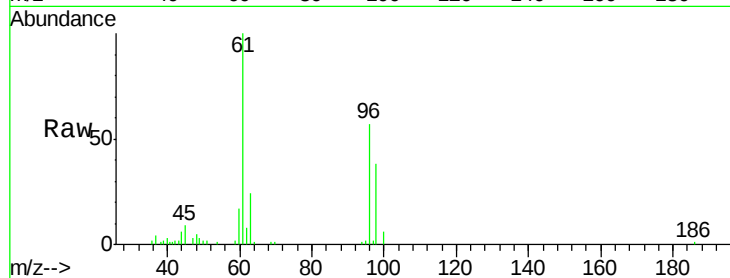

Abundance Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

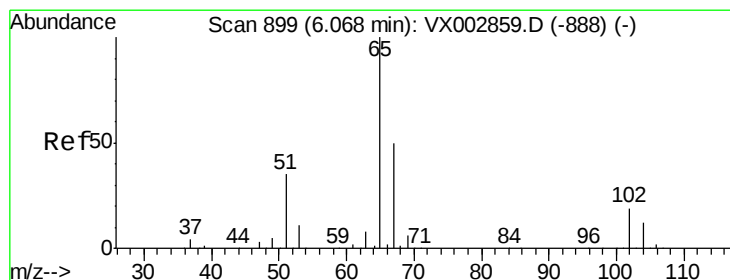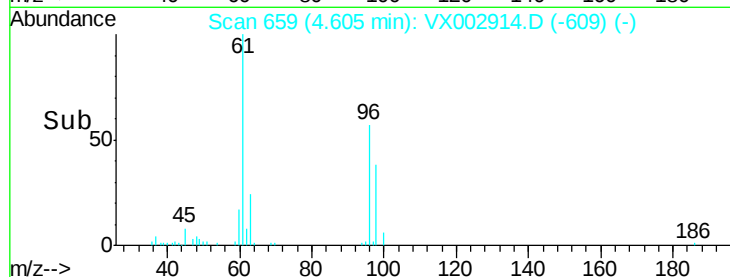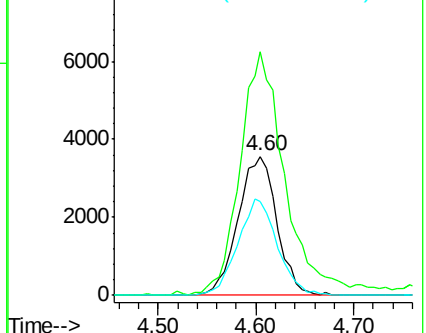

#33

1,2-Dichloroethane-d4

Concen: 48.90 ug/l

RT: 6.07 min Scan# 900

Delta R.T. 0.01 min

Lab File: VX002914.D


Acq: 27 Jun 2018 00:36

Tgt Ion: 65 Resp: 169984

Ion Ratio Lower Upper



65 100


67 51.0 0.0 102.6

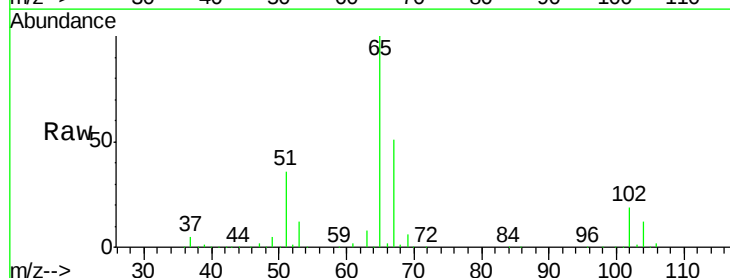

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

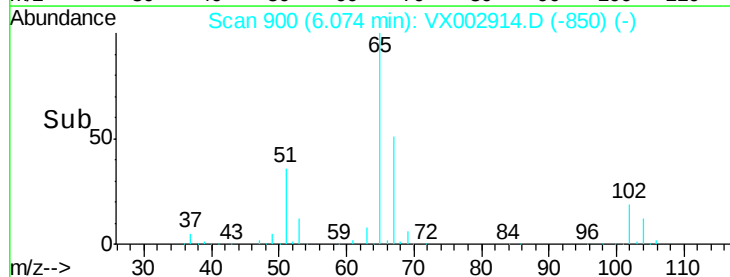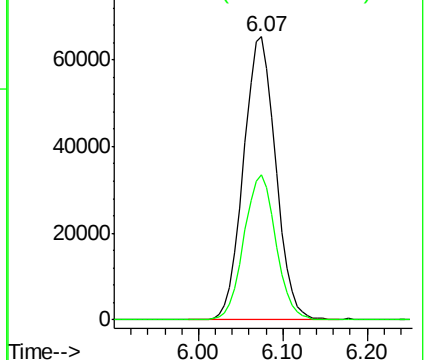

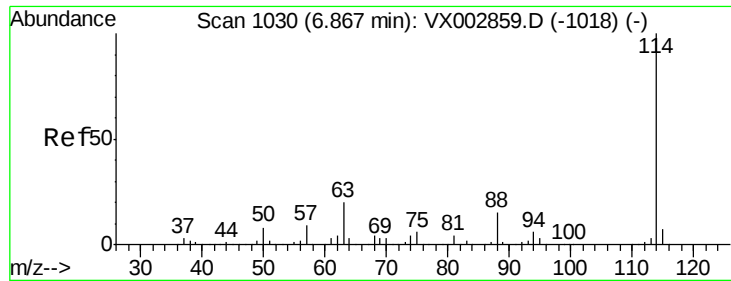

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.87 min Scan# 1030

Delta R.T. -0.00 min

Lab File: VX002914.D

Acq: 27 Jun 2018 00:36

Instrument :

MSVOA_X

ClientSampleId :

WP021SB480-13-15-180622


Tot Ion:114 Resp: 352129

Ion Ratio Lower Upper

114 100

63 20.4 0.0 41.4




88 15.7 0.0 30.0

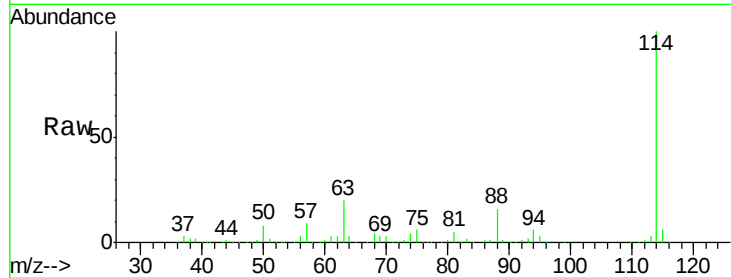

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

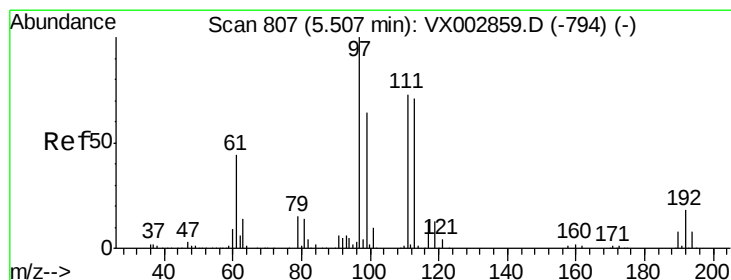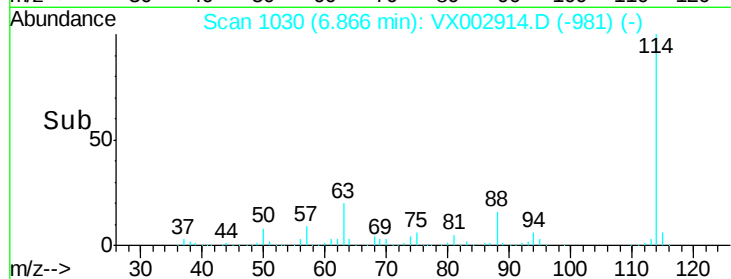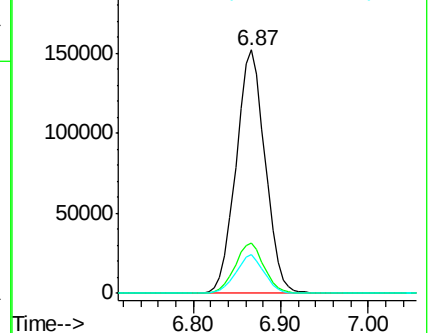

#35

Dibromofluoromethane

Concen: 48.40 ug/l

RT: 5.51 min Scan# 807

Delta R.T. -0.00 min

Lab File: VX002914.D

Acq: 27 Jun 2018 00:36


Tgt Ion:113 Resp: 134979

Ion Ratio Lower Upper

113 100

111 102.1 81.4 122.0



192 23.7 19.1 28.7

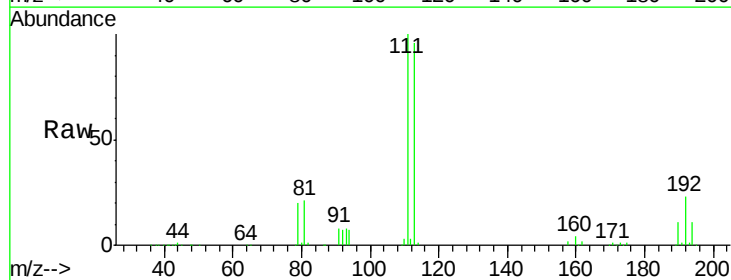


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

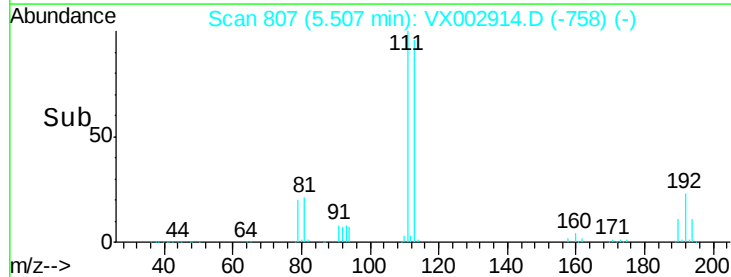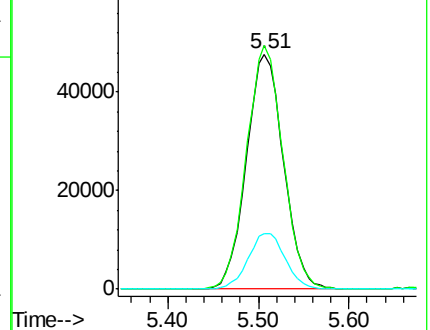

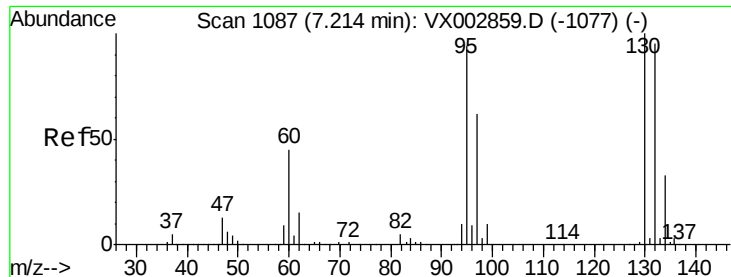

#44

Trichloroethene

Concen: 0.55 ug/l

RT: 7.21 min Scan# 1086

Delta R.T. -0.01 min

Lab File: VX002914.D

Acq: 27 Jun 2018 00:36

Instrument :

MSVOA_X

ClientSampleId :


WP021SB480-13-15-180622

Tot Ion:130 Resp: 1832

Ion Ratio Lower Upper




130 100

95 72.1 0.0 185.4

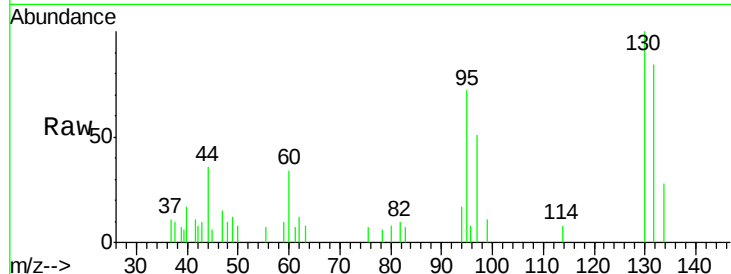

Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0

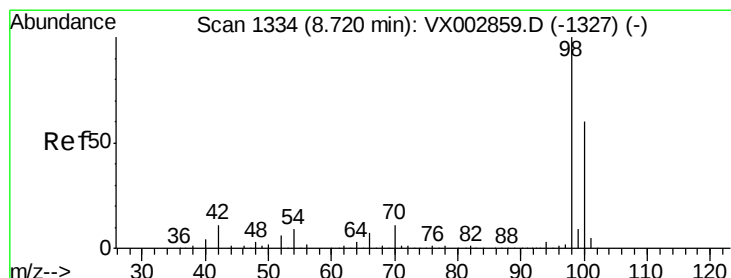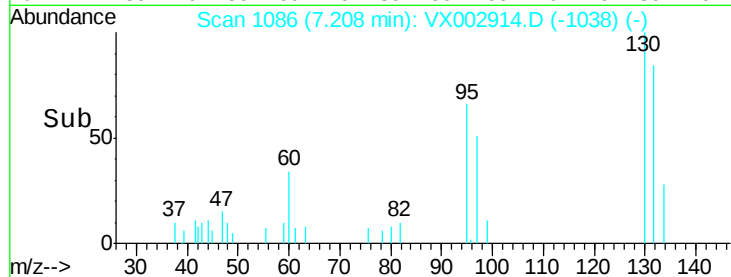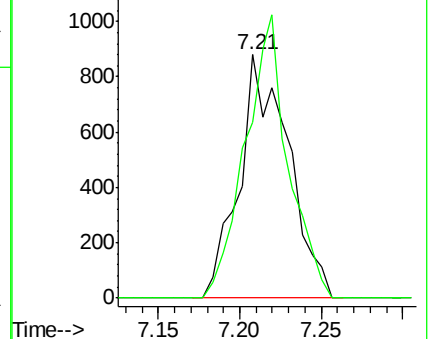

#50

Toluene-d8

Concen: 48.81 ug/l

RT: 8.72 min Scan# 1334

Delta R.T. 0.00 min

Lab File: VX002914.D


Acq: 27 Jun 2018 00:36

Tgt Ion: 98 Resp: 497040

Ion Ratio Lower Upper



98 100


100 64.1 50.9 76.3

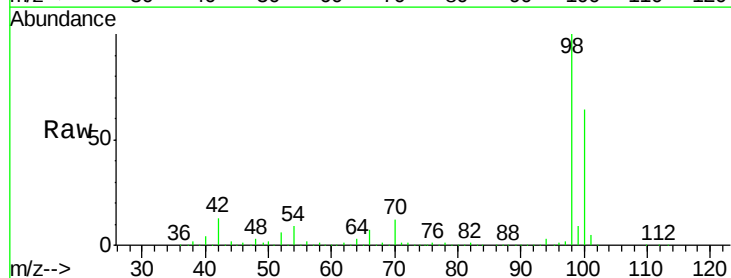

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX0

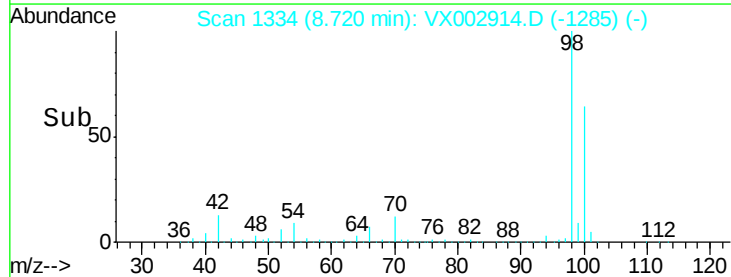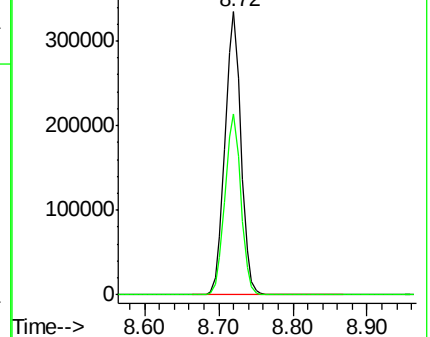

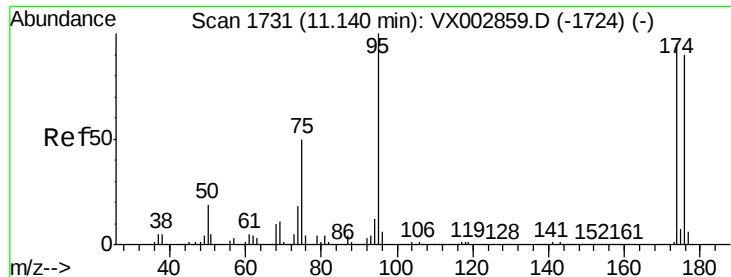

#62

4-Bromofluorobenzene

Concen: 44.54 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.00 min

Lab File: VX002914.D

Acq: 27 Jun 2018 00:36

Instrument :

MSVOA_X

ClientSampleId :

WP021SB480-13-15-180622


Tot Ion: 95 Resp: 174897

Ion Ratio Lower Upper

95 100

174 96.7 0.0 187.4




176 93.0 0.0 181.0

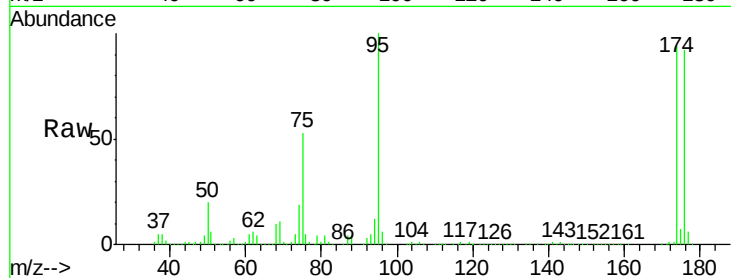

Abundance Ion 94.90 (94.60 to 95.60): VX002914.D (-1682) (-)

Ion 173.80 (173.50 to 174.50): VX002914.D (-1682) (-)

Ion 175.80 (175.50 to 176.50): VX002914.D (-1682) (-)

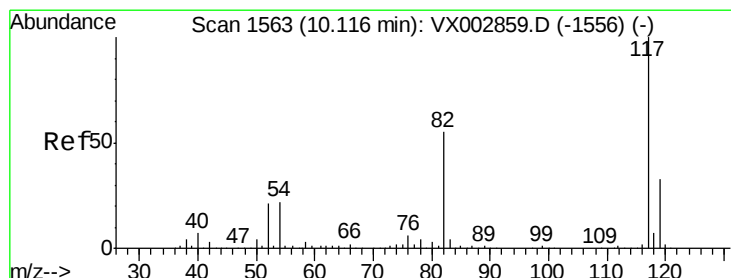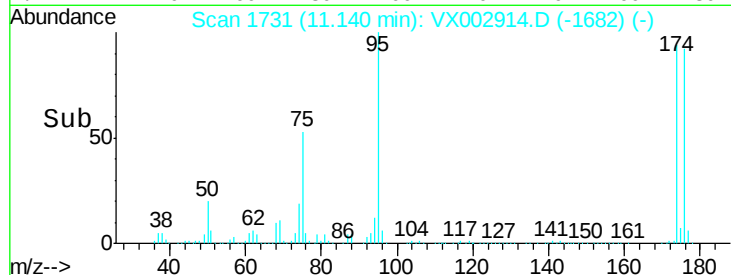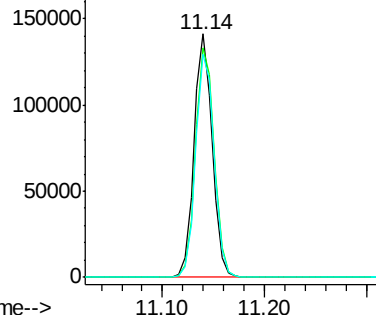

#63

Chlorobenzene-d5

Concen: 50.00 ug/l

RT: 10.12 min Scan# 1563

Delta R.T. -0.00 min

Lab File: VX002914.D

Acq: 27 Jun 2018 00:36


Tgt Ion: 117 Resp: 327973

Ion Ratio Lower Upper

117 100

82 54.5 45.0 67.4



119 32.3 25.8 38.6

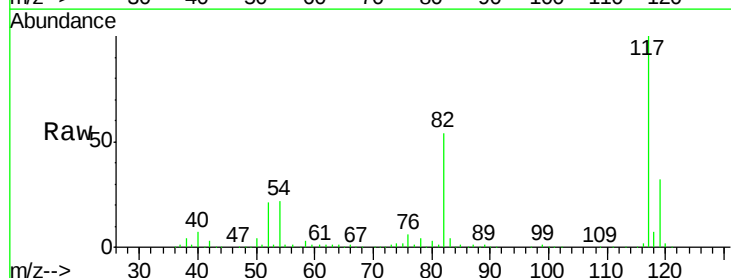


Abundance Ion 116.90 (116.60 to 117.60): VX002914.D (-1514) (-)

Ion 82.00 (81.70 to 82.70): VX002914.D (-1514) (-)

Ion 118.90 (118.60 to 119.60): VX002914.D (-1514) (-)

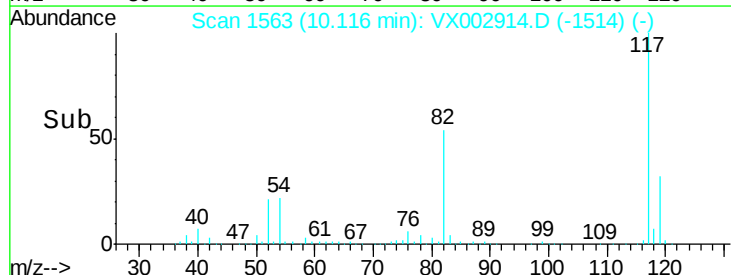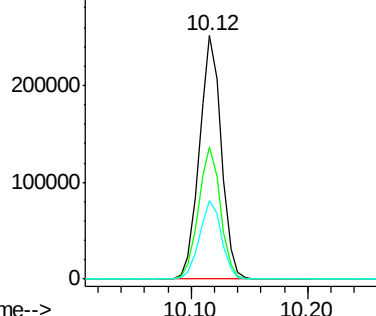

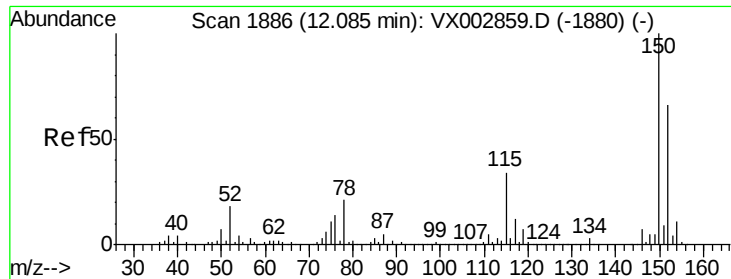

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 12.08 min Scan# 1885

Delta R.T. -0.01 min

Lab File: VX002914.D

Acq: 27 Jun 2018 00:36

Instrument :

MSVOA_X

ClientSampleId :

WP021SB480-13-15-180622


Tot Ion:152 Resp: 183933

Ion Ratio Lower Upper

152 100

115 55.2 40.1 120.2

150 157.9 0.0 347.2

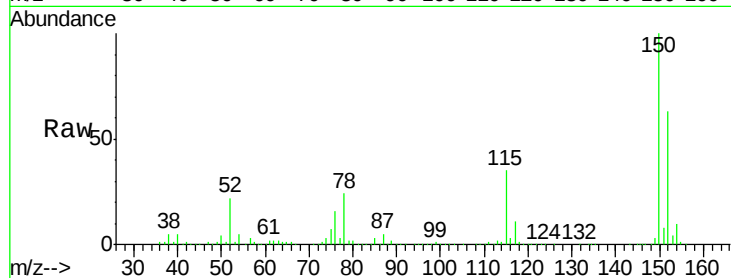

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

