


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX062618\
Data File : VX002902.D
Acq On : 26 Jun 2018 18:45
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Title : SW846 8260
Last Update : Mon Jun 25 14:38:05 2018

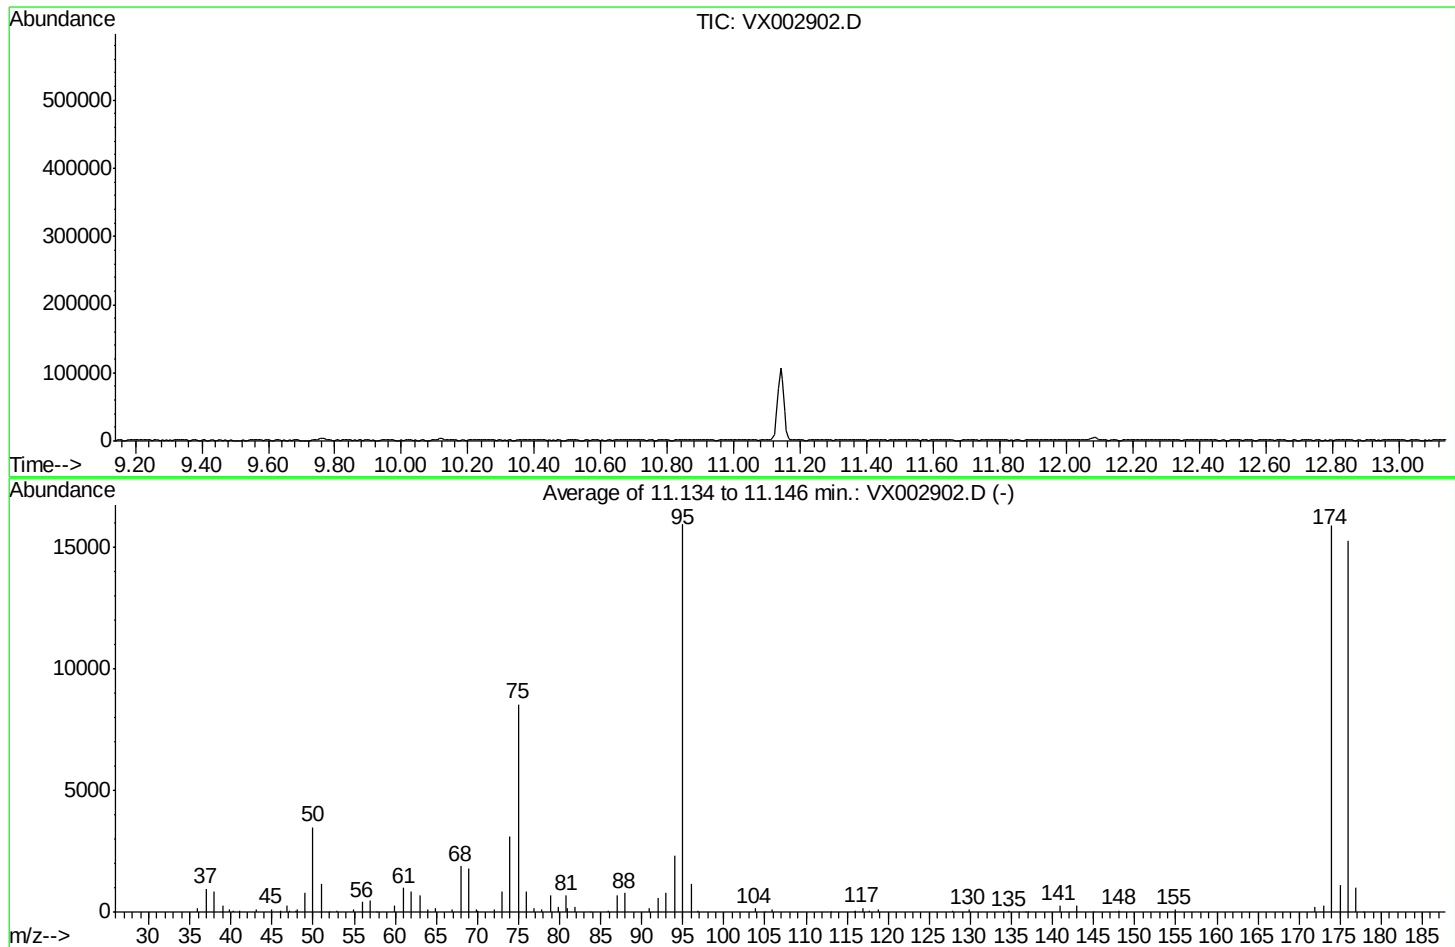

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	3488	PASS
75	95	30	60	53.5	8537	PASS
95	95	100	100	100.0	15954	PASS
96	95	5	9	7.2	1141	PASS
173	174	0.00	2	1.7	264	PASS
174	95	50	100	99.8	15926	PASS
175	174	5	9	7.0	1107	PASS
176	174	95	101	95.9	15273	PASS
177	176	5	9	6.6	1002	PASS