

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062619\
Data File : VX010454.D
Acq On : 26 Jun 2019 11:52
Operator : JC/SP
Sample : K3527-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CPA-AMW-4-M24W1-062119

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	14	21	27	rBV2	7339	12897	1.10%	0.203%
2	2.605	233	238	248	rVB	17748	33476	2.85%	0.528%
3	3.019	298	306	313	rBV2	5075	12468	1.06%	0.197%
4	5.501	700	713	725	rBV	143894	410033	34.88%	6.464%
5	5.665	729	740	756	rVB	238641	682523	58.06%	10.760%
6	6.062	793	805	821	rBV	132297	357431	30.41%	5.635%
7	6.860	924	936	950	rBV	359790	852827	72.55%	13.445%
8	8.714	1233	1240	1249	rBV	766071	1175473	100.00%	18.532%
9	9.335	1337	1342	1349	rBV2	47674	73460	6.25%	1.158%
10	10.110	1462	1469	1480	rBV	733509	1002744	85.31%	15.809%
11	11.134	1631	1637	1648	rBV	626405	789118	67.13%	12.441%
12	12.073	1786	1791	1800	rBV	731997	940472	80.01%	14.827%


Sum of corrected areas: 6342922

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062619\
Data File : VX010454.D
Acq On : 26 Jun 2019 11:52
Operator : JC/SP
Sample : K3527-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CPA-AMW-4-M24W1-062119

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

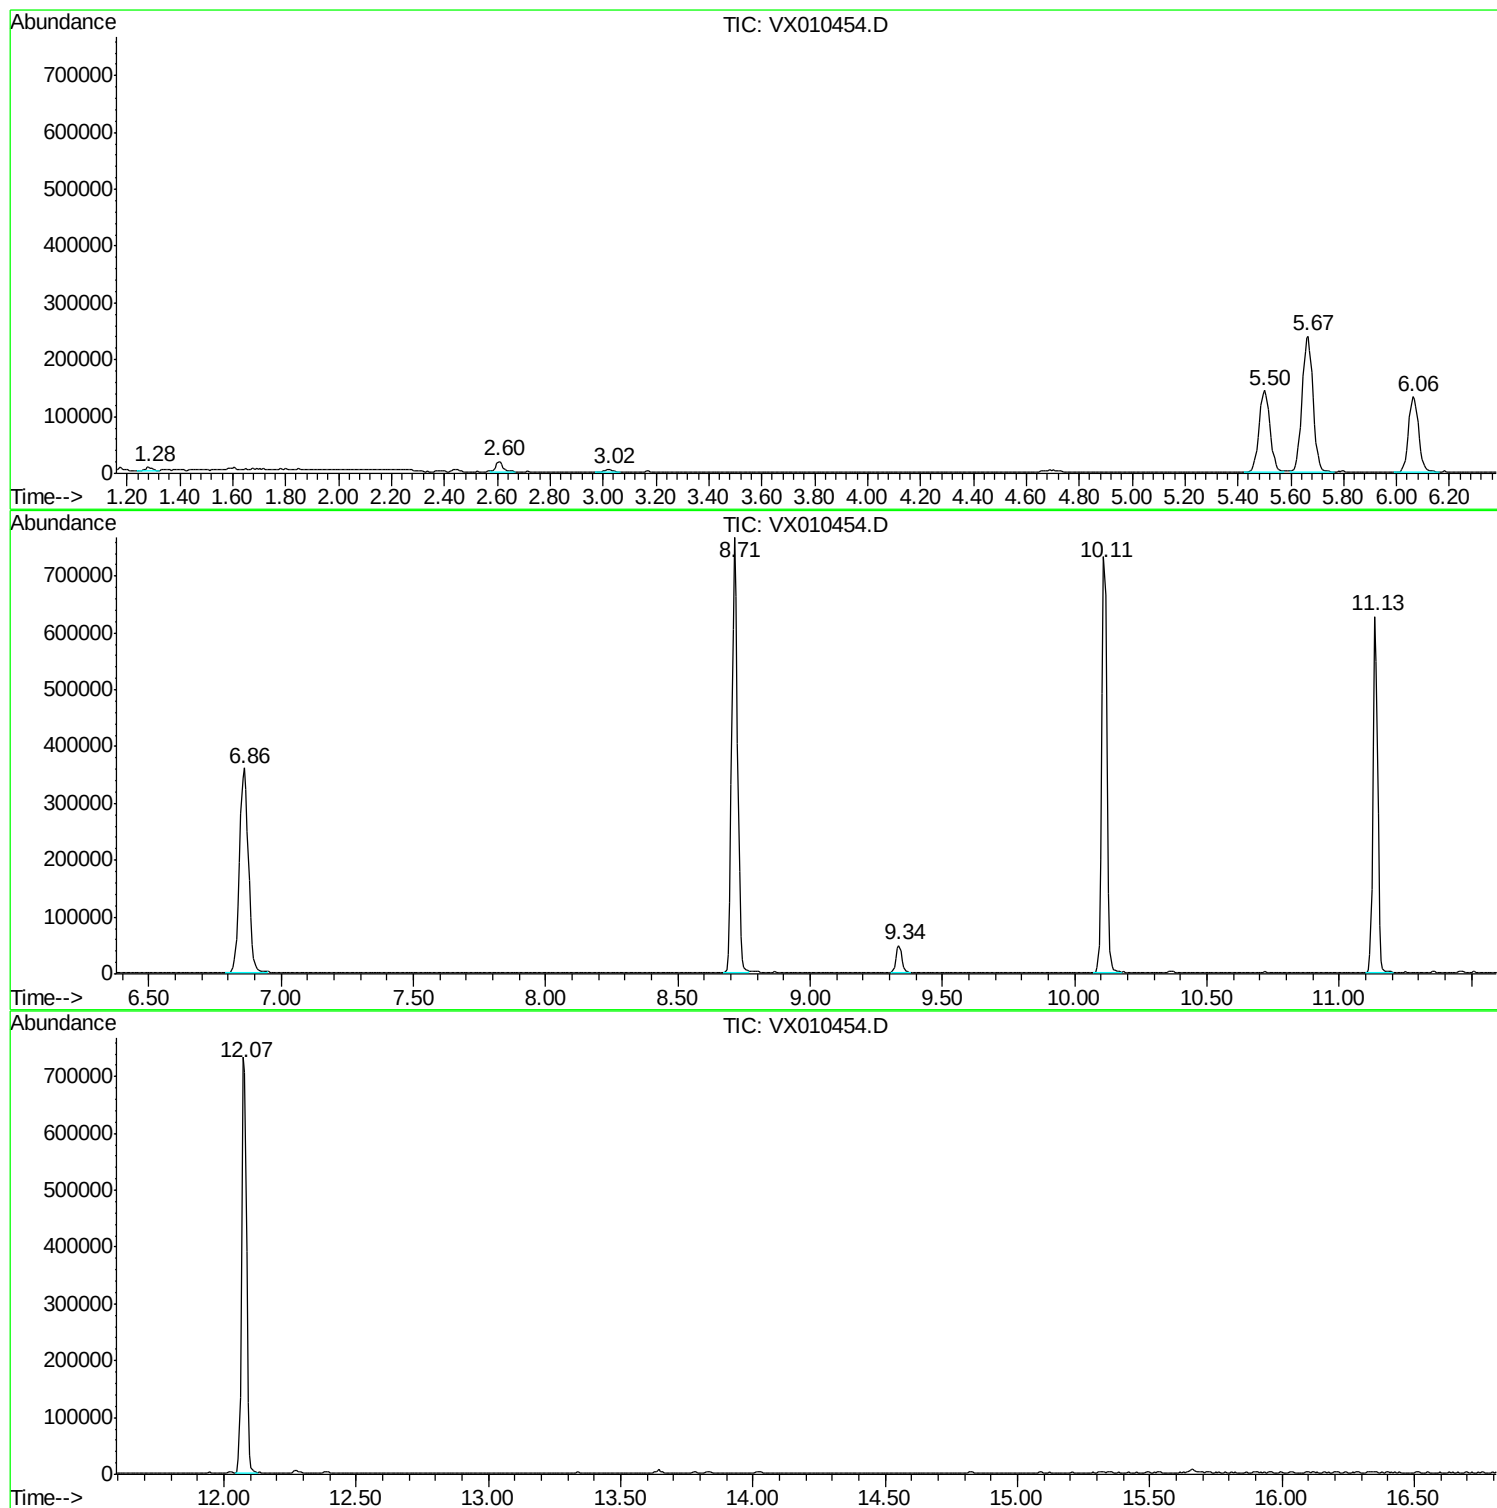

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX062619\
Data File : VX010454.D
Acq On : 26 Jun 2019 11:52
Operator : JC/SP
Sample : K3527-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CPA-AMW-4-M24W1-062119

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX062619\
Data File : VX010454.D
Acq On : 26 Jun 2019 11:52
Operator : JC/SP
Sample : K3527-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CPA-AMW-4-M24W1-062119

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc