

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062619\
 Data File : VX010460.D
 Acq On : 26 Jun 2019 14:12
 Operator : JC/SP
 Sample : K3527-06
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CPA-CPMW04S-M24W1-062019

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	18	21	27	rBV	12490	19002	1.68%	0.311%
2	2.605	232	238	246	rBV	26482	48388	4.28%	0.792%
3	3.013	300	305	315	rVB	6243	15808	1.40%	0.259%
4	4.690	571	580	589	rBV3	5522	17975	1.59%	0.294%
5	5.501	702	713	726	rBV2	136104	387789	34.32%	6.344%
6	5.665	728	740	755	rVB	231856	653228	57.81%	10.687%
7	6.061	795	805	820	rBV	128257	340368	30.12%	5.568%
8	6.860	926	936	949	rBV	342870	806929	71.42%	13.201%
9	8.713	1232	1240	1249	rBV	739693	1129905	100.00%	18.485%
10	9.335	1336	1342	1349	rVB	43487	63380	5.61%	1.037%
11	10.109	1462	1469	1481	rBV	725092	968100	85.68%	15.838%
12	11.134	1630	1637	1648	rBV	603827	761068	67.36%	12.451%
13	12.073	1784	1791	1798	rBV	687841	900653	79.71%	14.734%


Sum of corrected areas: 6112593

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062619\
Data File : VX010460.D
Acq On : 26 Jun 2019 14:12
Operator : JC/SP
Sample : K3527-06
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CPA-CPMW04S-M24W1-062019

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

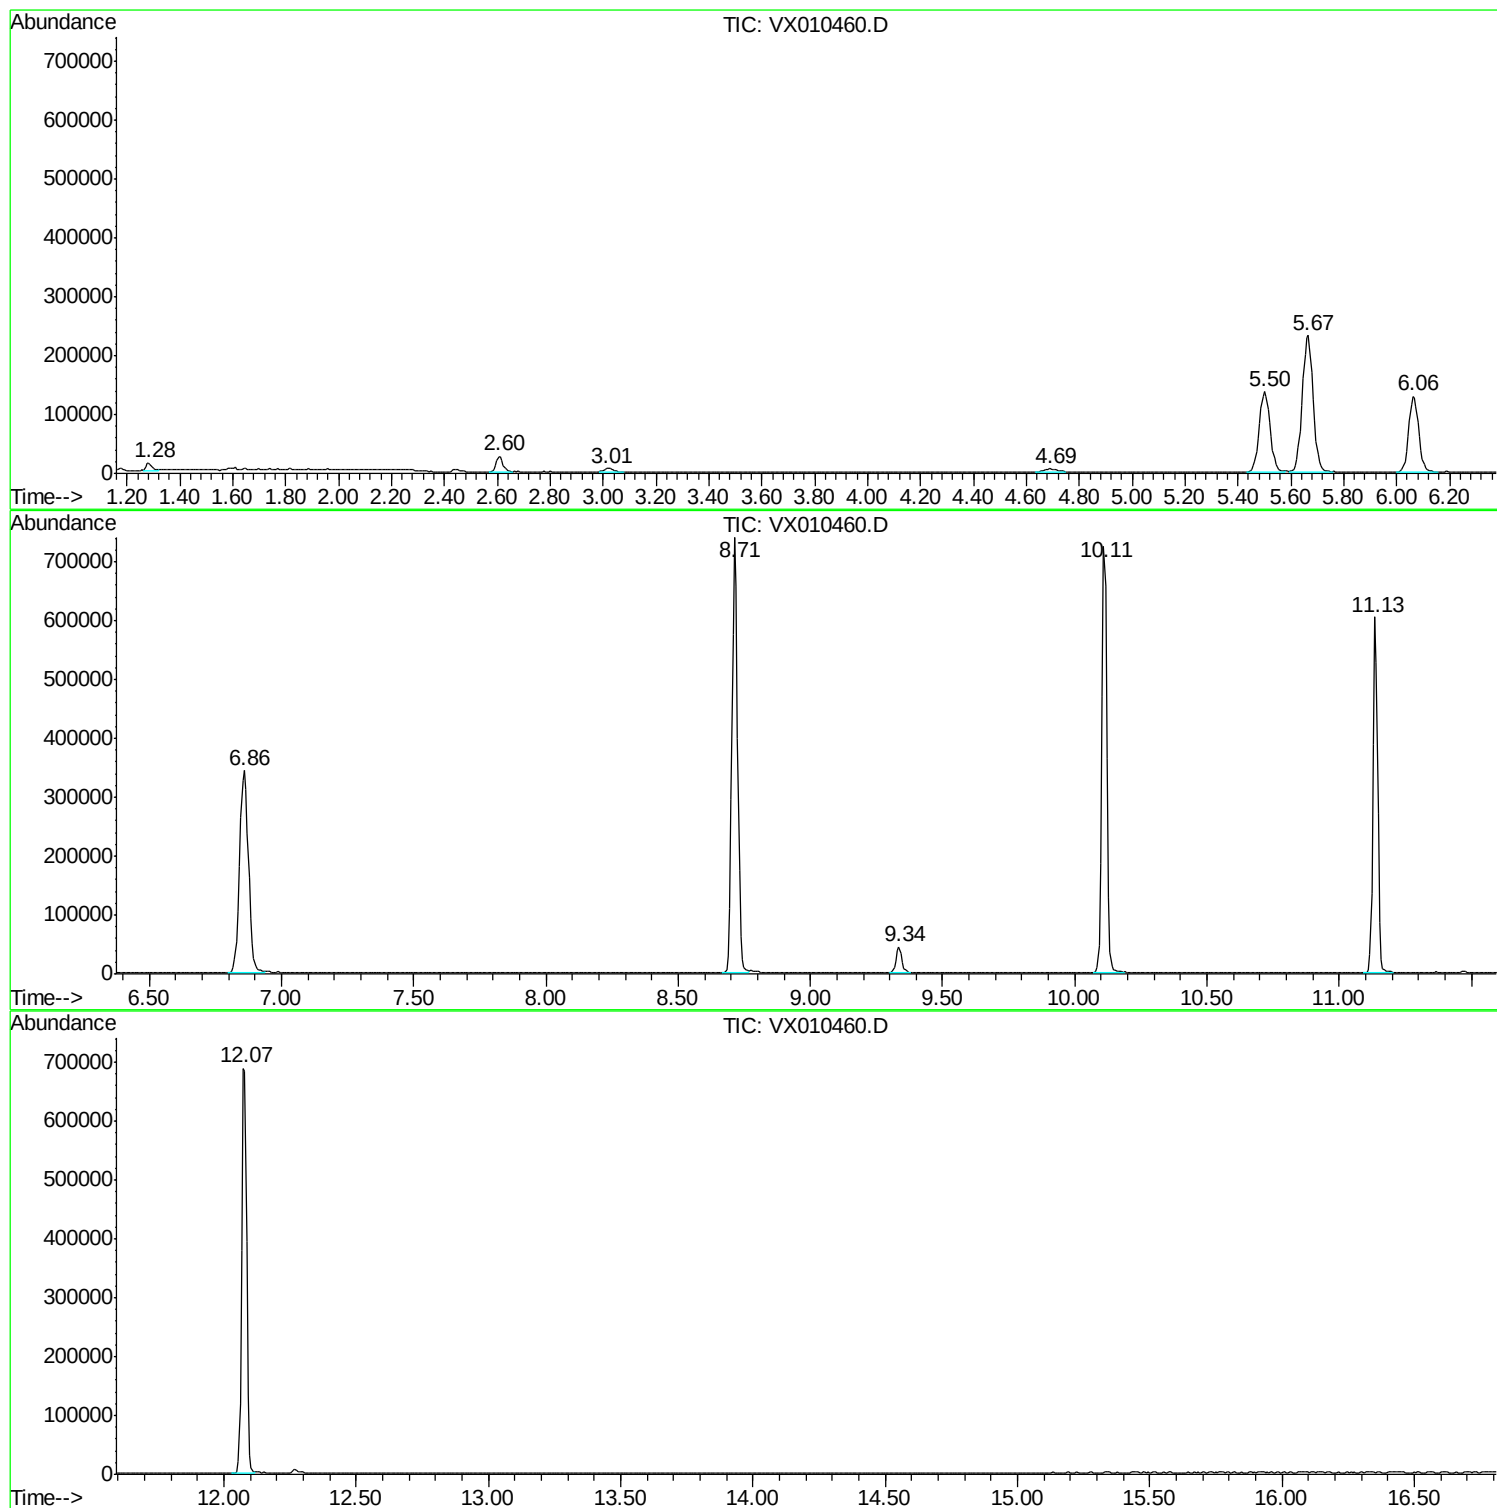

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX062619\
Data File : VX010460.D
Acq On : 26 Jun 2019 14:12
Operator : JC/SP
Sample : K3527-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CPA-CPMW04S-M24W1-062019

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX062619\
Data File : VX010460.D
Acq On : 26 Jun 2019 14:12
Operator : JC/SP
Sample : K3527-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CPA-CPMW04S-M24W1-062019

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc