

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062619\
 Data File : VX010461.D
 Acq On : 26 Jun 2019 14:36
 Operator : JC/SP
 Sample : K3527-07
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CPA-CPMW05D-M24W1-062219

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	17	21	28	rBV	12867	20122	1.75%	0.327%
2	2.611	233	239	246	rBV	12798	25633	2.23%	0.416%
3	3.019	299	306	313	rBV	4951	12051	1.05%	0.196%
4	5.141	641	654	659	rBV7	4432	14095	1.22%	0.229%
5	5.501	702	713	726	rBV2	138988	401613	34.89%	6.522%
6	5.665	727	740	758	rVB	235990	664866	57.77%	10.797%
7	6.061	794	805	816	rBV	132557	350579	30.46%	5.693%
8	6.860	924	936	950	rBV	356071	836064	72.64%	13.577%
9	8.713	1233	1240	1253	rBV	730014	1150978	100.00%	18.691%
10	9.335	1337	1342	1348	rVB2	18610	29381	2.55%	0.477%
11	10.110	1463	1469	1480	rBV	718491	976849	84.87%	15.863%
12	11.134	1631	1637	1649	rBV	600803	769204	66.83%	12.491%
13	12.079	1786	1792	1801	rBV	692679	906531	78.76%	14.721%


Sum of corrected areas: 6157966

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062619\
Data File : VX010461.D
Acq On : 26 Jun 2019 14:36
Operator : JC/SP
Sample : K3527-07
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CPA-CPMW05D-M24W1-062219

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

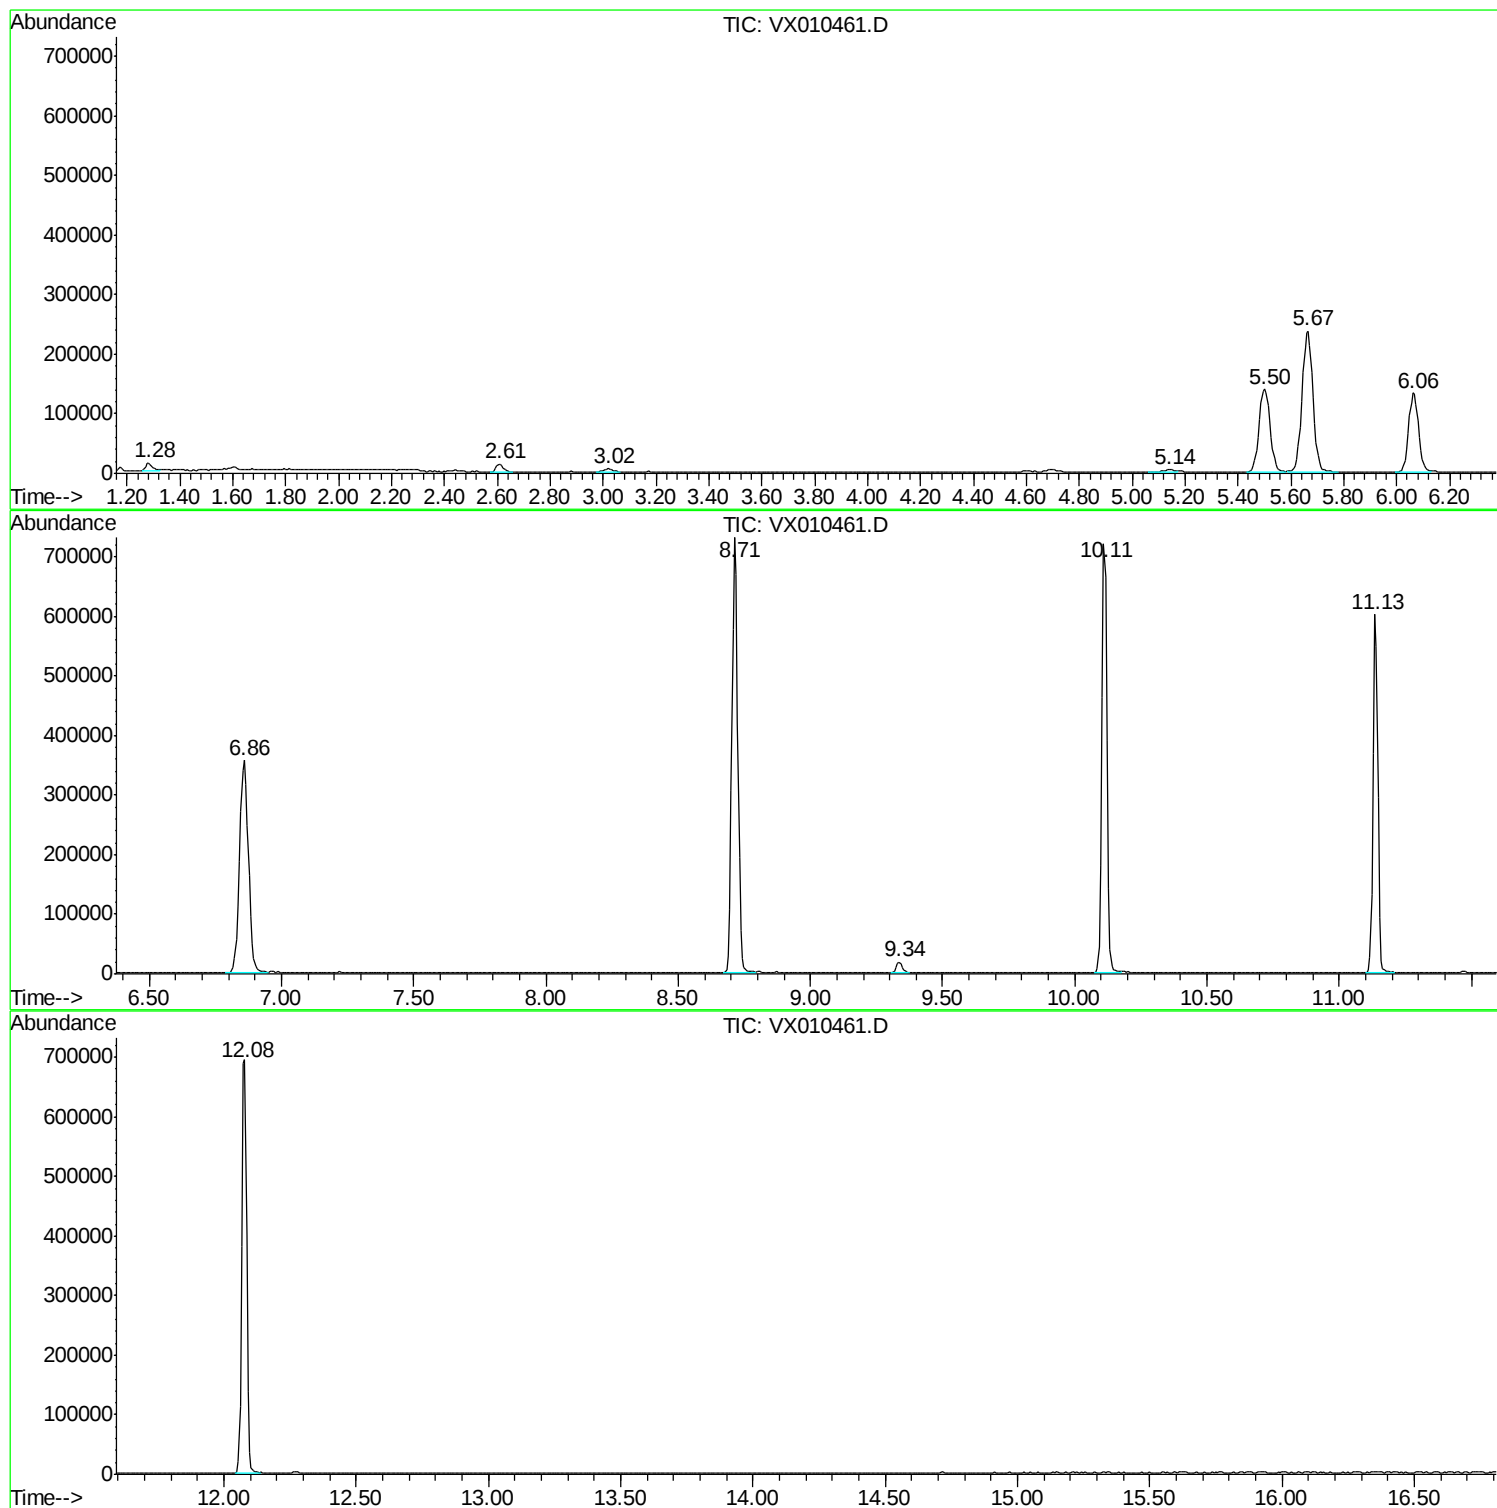

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX062619\
Data File : VX010461.D
Acq On : 26 Jun 2019 14:36
Operator : JC/SP
Sample : K3527-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CPA-CPMW05D-M24W1-062219

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX062619\
Data File : VX010461.D
Acq On : 26 Jun 2019 14:36
Operator : JC/SP
Sample : K3527-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CPA-CPMW05D-M24W1-062219

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc