

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062619\
 Data File : VX010466.D
 Acq On : 26 Jun 2019 16:33
 Operator : JC/SP
 Sample : K3527-12
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CPA-CPMW10D-M24W1-062219

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	16	20	27	rBV	13721	22877	1.95%	0.365%
2	2.605	232	238	246	rBV	18914	33889	2.88%	0.541%
3	3.025	297	307	314	rBV3	4470	12822	1.09%	0.205%
4	5.500	701	713	724	rBV	139921	398409	33.91%	6.361%
5	5.659	729	739	754	rVB	238963	673279	57.31%	10.749%
6	6.061	795	805	819	rBV2	134340	355071	30.22%	5.669%
7	6.860	926	936	953	rVB	354887	839479	71.46%	13.403%
8	8.713	1233	1240	1251	rBV	765156	1174763	100.00%	18.756%
9	9.335	1335	1342	1349	rBV2	15652	24768	2.11%	0.395%
10	10.109	1463	1469	1480	rBV	742974	1006363	85.67%	16.067%
11	11.134	1631	1637	1648	rBV	614499	781540	66.53%	12.478%
12	12.079	1785	1792	1801	rBV	726524	940116	80.03%	15.010%


Sum of corrected areas: 6263376

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062619\
Data File : VX010466.D
Acq On : 26 Jun 2019 16:33
Operator : JC/SP
Sample : K3527-12
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CPA-CPMW10D-M24W1-062219

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

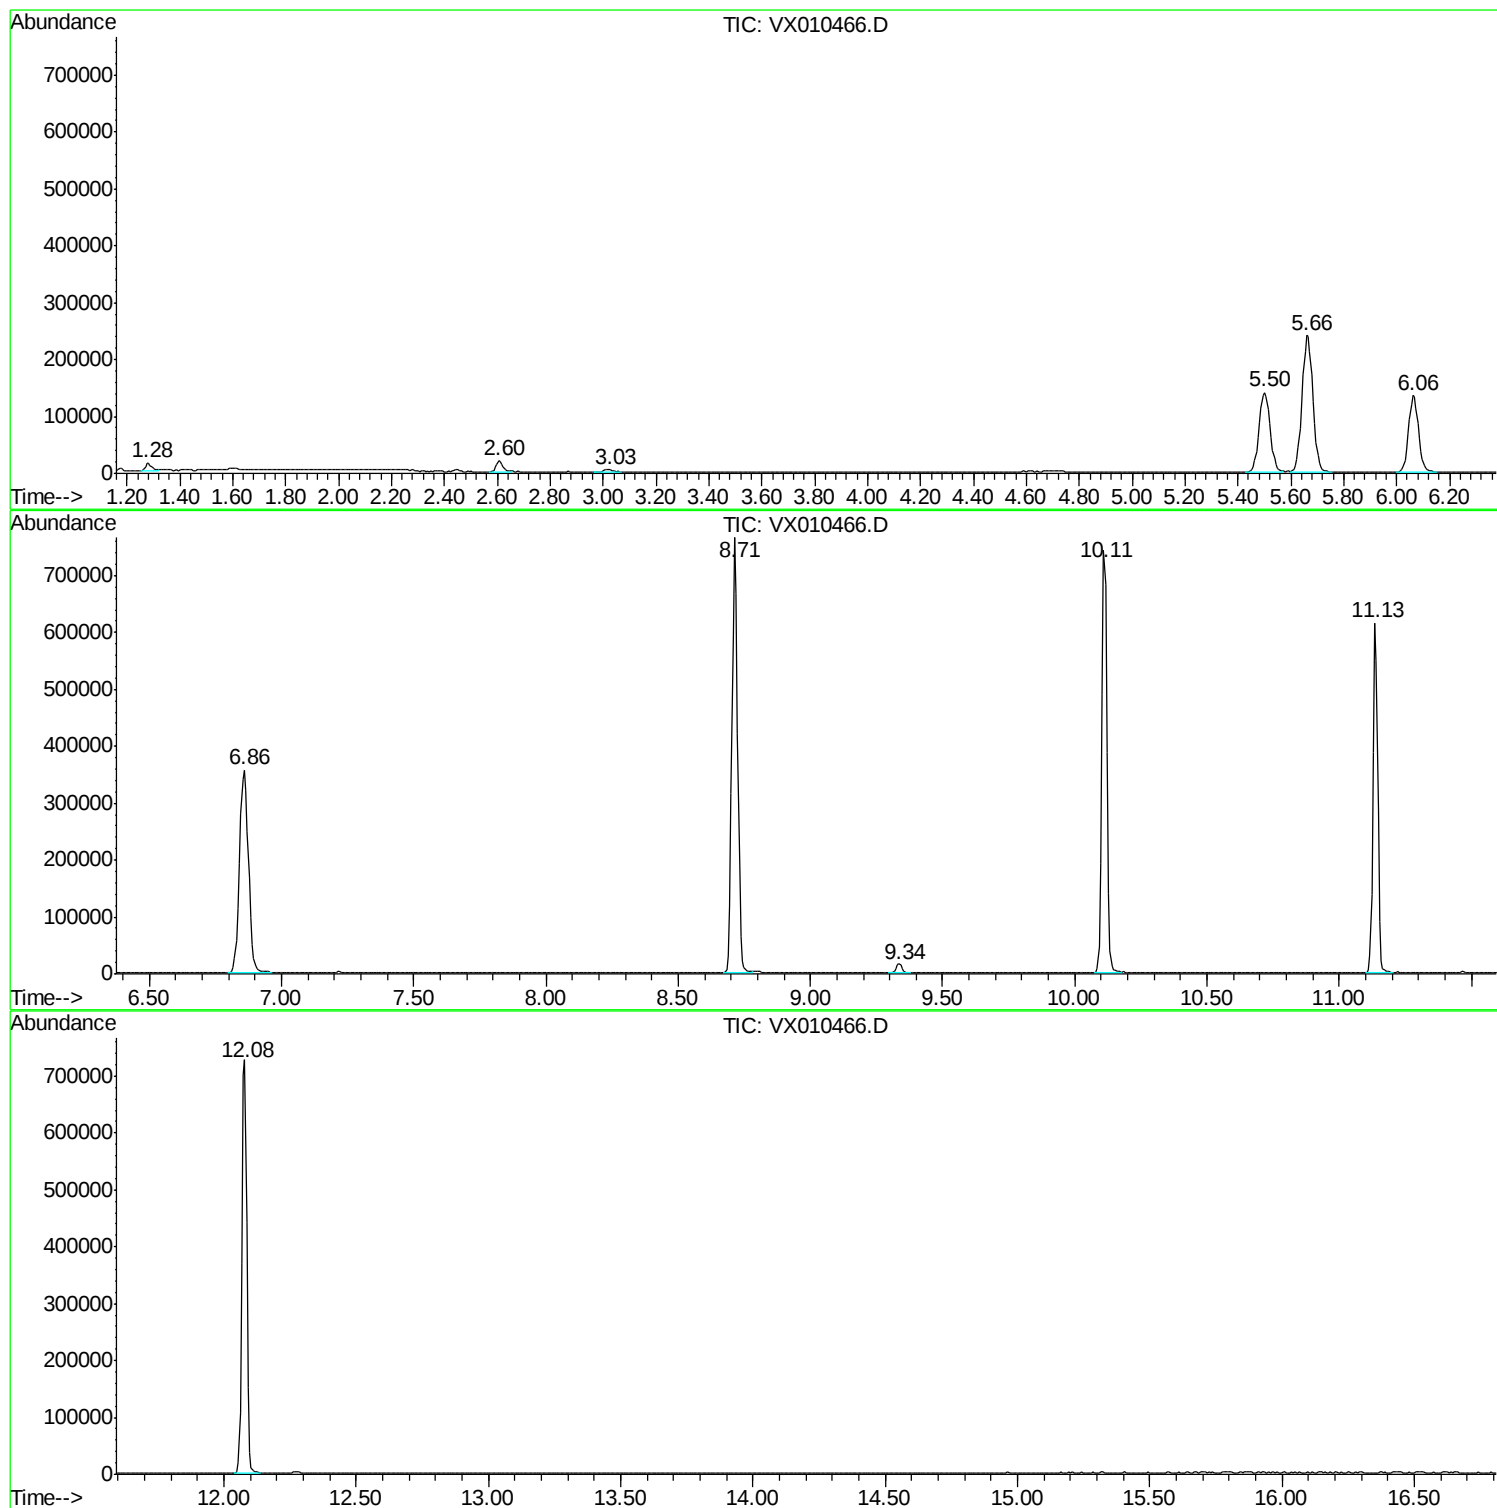

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX062619\
Data File : VX010466.D
Acq On : 26 Jun 2019 16:33
Operator : JC/SP
Sample : K3527-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CPA-CPMW10D-M24W1-062219

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX062619\
Data File : VX010466.D
Acq On : 26 Jun 2019 16:33
Operator : JC/SP
Sample : K3527-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CPA-CPMW10D-M24W1-062219

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc