

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062619\
 Data File : VX010469.D
 Acq On : 26 Jun 2019 17:43
 Operator : JC/SP
 Sample : K3527-15
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CPA-CPMW11D-M24W1-062219-D

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	16	20	27	rBV	26425	32626	2.75%	0.510%
2	2.611	233	239	246	rVB	25441	45978	3.87%	0.718%
3	3.013	297	305	314	rBV2	11243	31023	2.61%	0.485%
4	4.696	573	581	589	rBV	5045	13894	1.17%	0.217%
5	5.501	699	713	726	rBV	146457	415832	35.03%	6.496%
6	5.659	726	739	756	rVB	247182	685512	57.75%	10.709%
7	6.061	792	805	817	rBV	136191	361479	30.45%	5.647%
8	6.860	927	936	948	rBV	364238	850235	71.62%	13.282%
9	8.713	1231	1240	1257	rBV	766018	1187122	100.00%	18.545%
10	9.335	1334	1342	1348	rBV	18125	28800	2.43%	0.450%
11	10.110	1463	1469	1480	rBV	733596	1011754	85.23%	15.805%
12	11.134	1632	1637	1650	rBV	624404	796139	67.06%	12.437%
13	12.079	1784	1792	1801	rBV	744860	940992	79.27%	14.700%


Sum of corrected areas: 6401386

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062619\
Data File : VX010469.D
Acq On : 26 Jun 2019 17:43
Operator : JC/SP
Sample : K3527-15
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CPA-CPMW11D-M24W1-062219-D

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

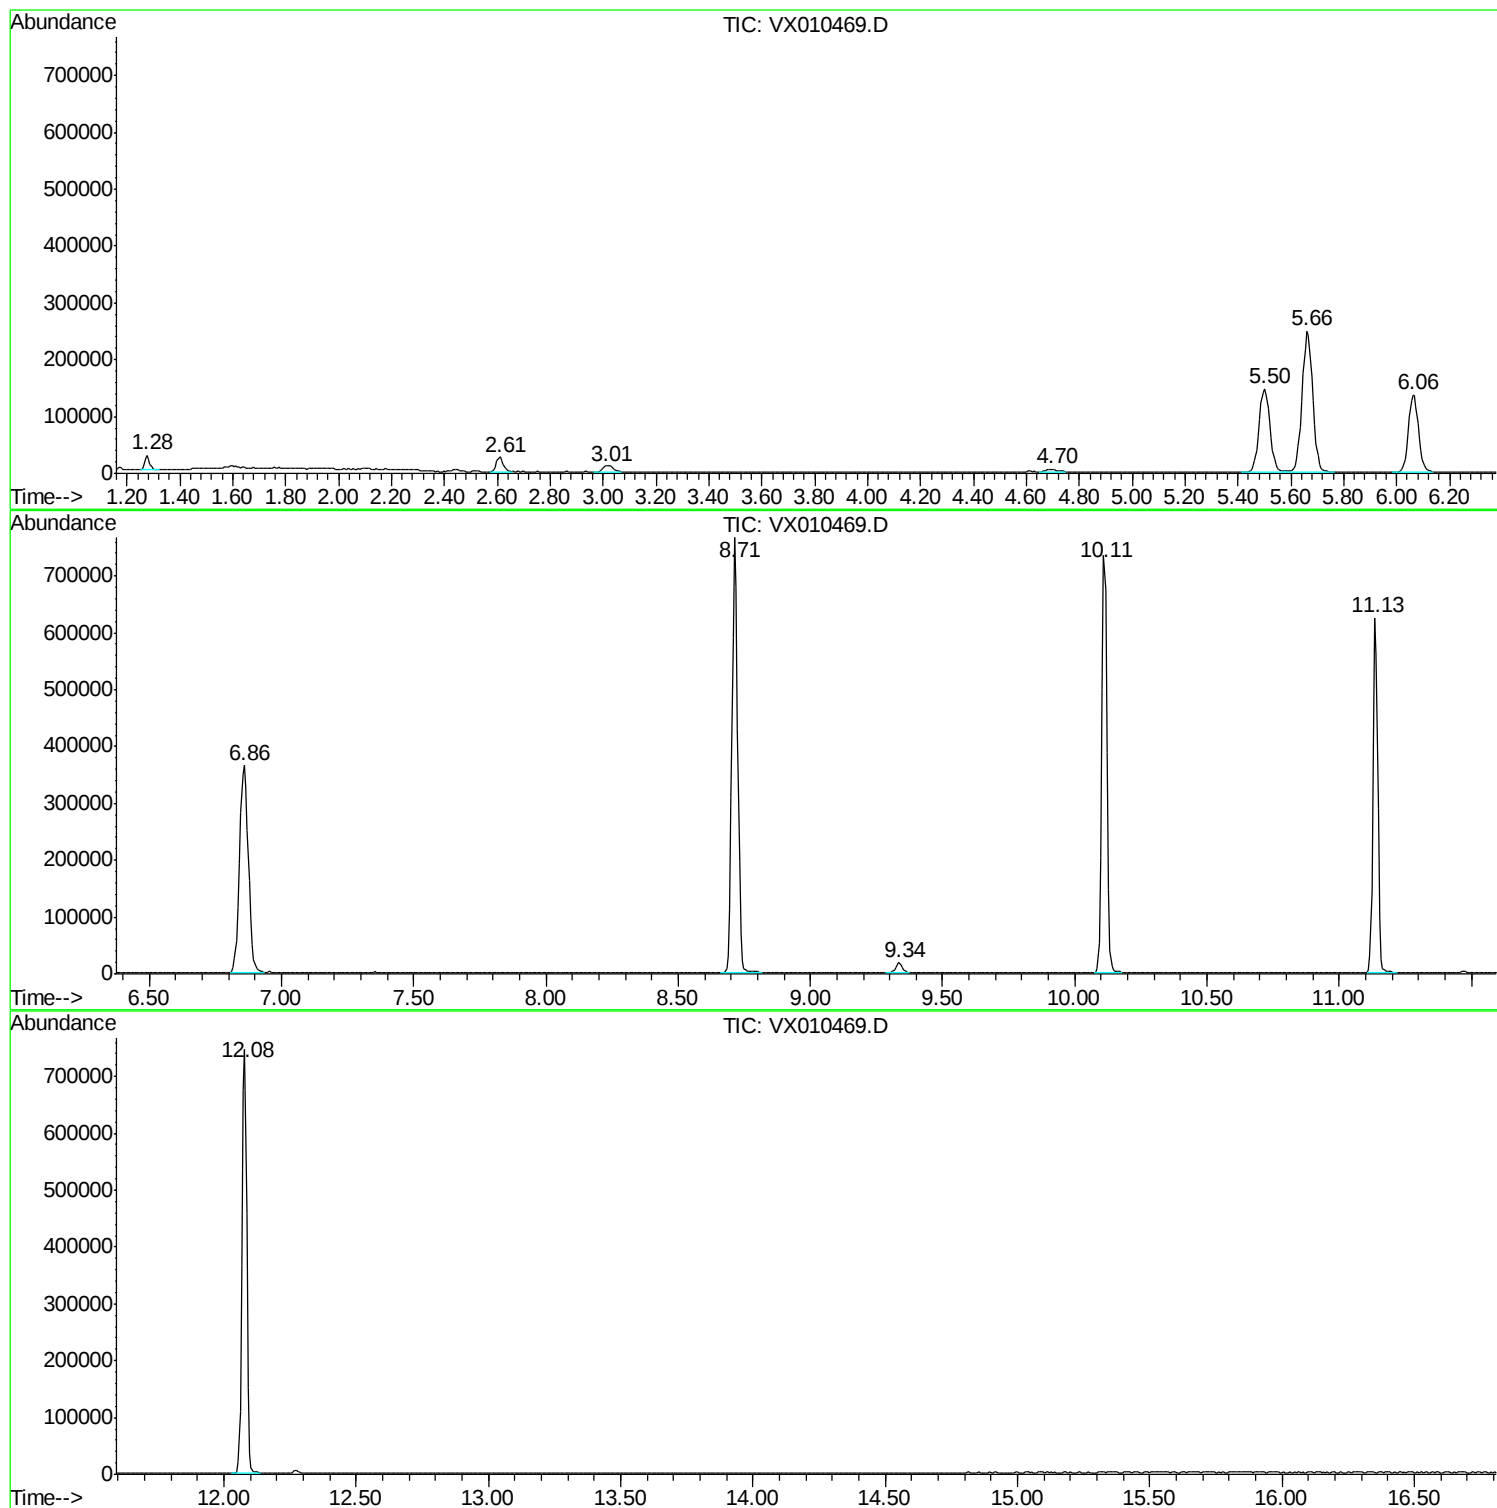

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX062619\
Data File : VX010469.D
Acq On : 26 Jun 2019 17:43
Operator : JC/SP
Sample : K3527-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CPA-CPMW11D-M24W1-062219-D

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX062619\
Data File : VX010469.D
Acq On : 26 Jun 2019 17:43
Operator : JC/SP
Sample : K3527-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CPA-CPMW11D-M24W1-062219-D

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc