

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062619\
 Data File : VX010471.D
 Acq On : 26 Jun 2019 18:30
 Operator : JC/SP
 Sample : K3527-18
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CPA-GMW-5S-R-M24W1-061919

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	16	20	28	rBV	38428	51787	4.43%	0.825%
2	2.611	232	239	247	rBV	21219	39845	3.41%	0.635%
3	3.013	298	305	317	rBV2	12067	33305	2.85%	0.530%
4	4.696	571	581	589	rBV	5343	17240	1.48%	0.275%
5	5.500	698	713	726	rBV	141029	407497	34.89%	6.491%
6	5.665	729	740	753	rVB	238146	667393	57.14%	10.630%
7	6.061	795	805	818	rBV	133642	356692	30.54%	5.682%
8	6.860	926	936	949	rBV	358470	843348	72.20%	13.433%
9	8.713	1231	1240	1252	rBV	751579	1168060	100.00%	18.605%
10	10.109	1463	1469	1482	rBV	720959	990412	84.79%	15.776%
11	11.134	1631	1637	1646	rBV	617540	781812	66.93%	12.453%
12	12.072	1786	1791	1799	rBV	708995	920716	78.82%	14.666%


Sum of corrected areas: 6278107

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062619\
Data File : VX010471.D
Acq On : 26 Jun 2019 18:30
Operator : JC/SP
Sample : K3527-18
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CPA-GMW-5S-R-M24W1-061919

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

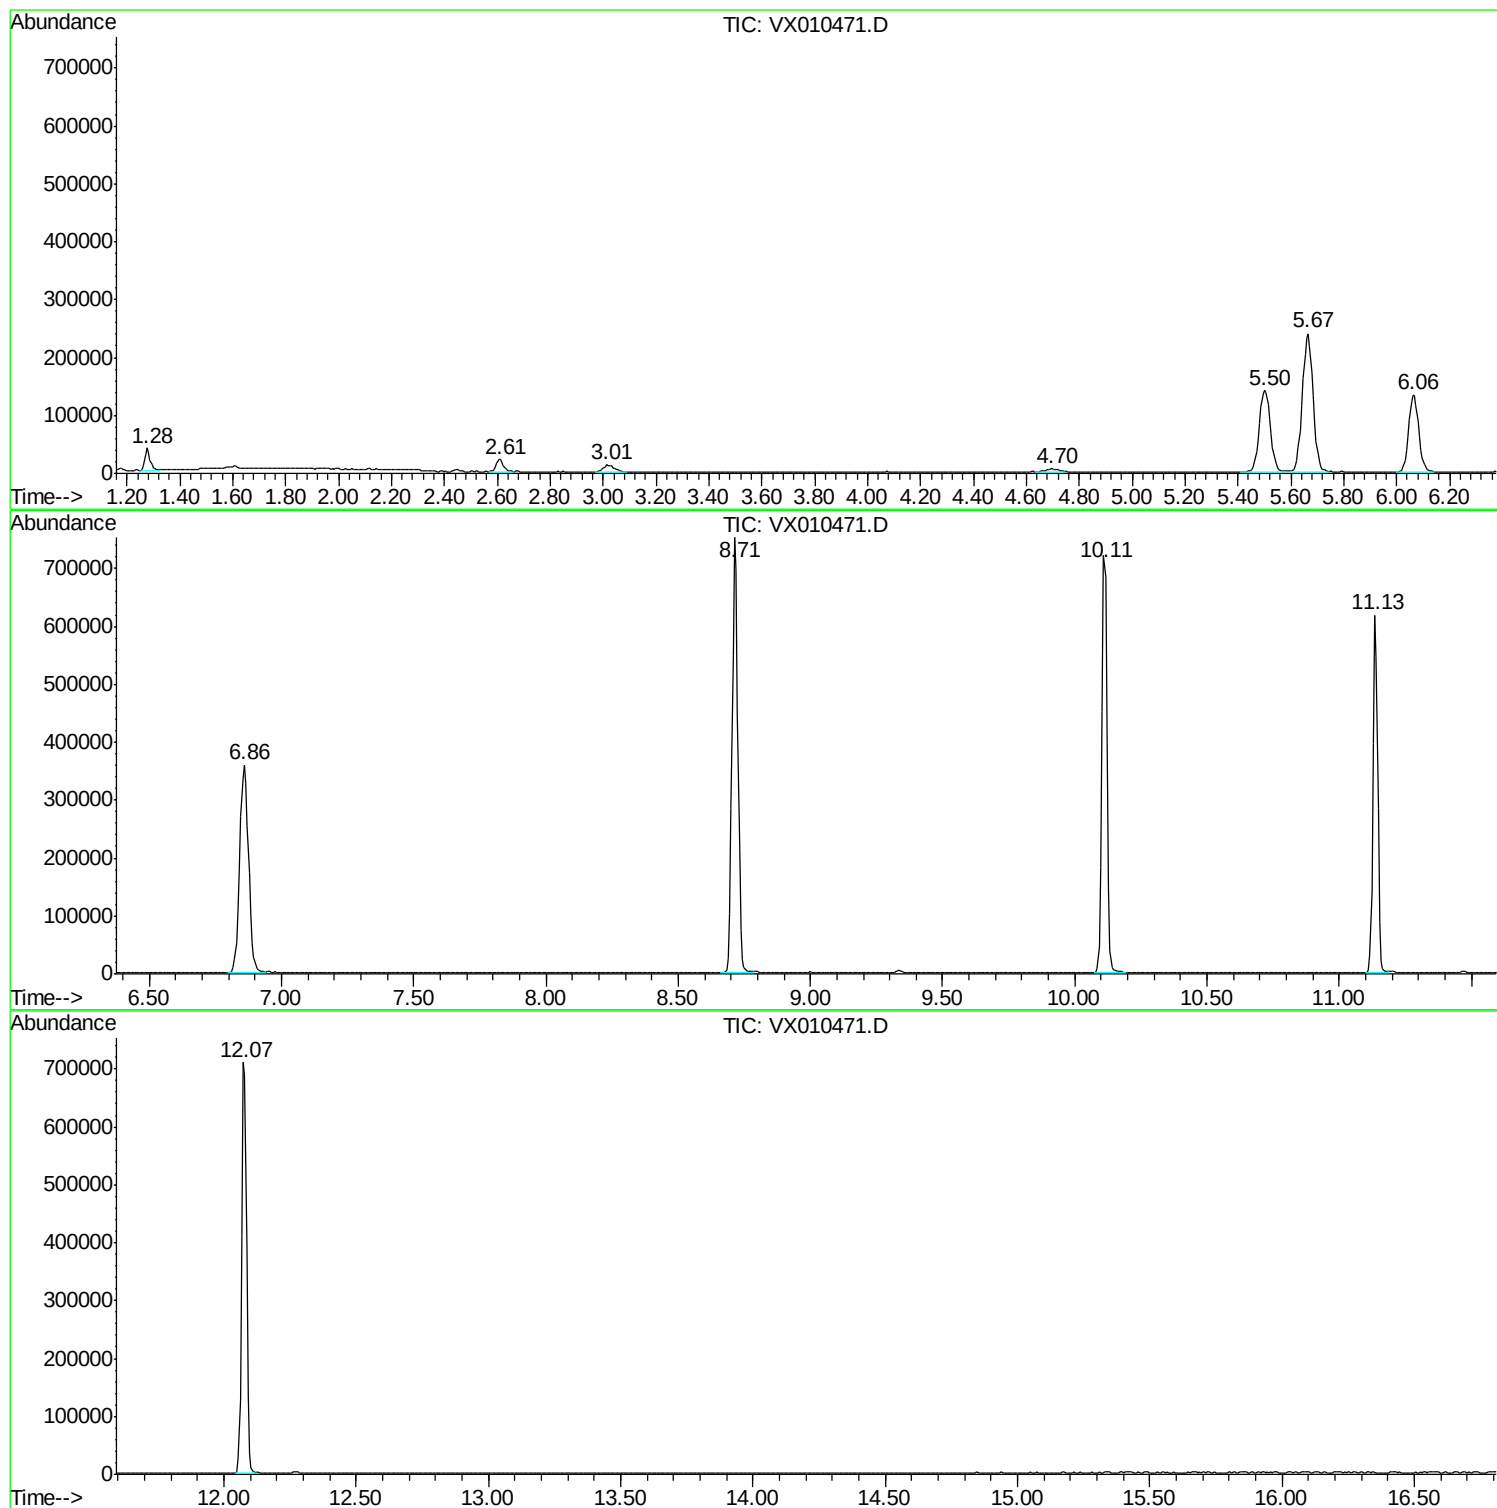

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX062619\
Data File : VX010471.D
Acq On : 26 Jun 2019 18:30
Operator : JC/SP
Sample : K3527-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CPA-GMW-5S-R-M24W1-061919

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX062619\
Data File : VX010471.D
Acq On : 26 Jun 2019 18:30
Operator : JC/SP
Sample : K3527-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CPA-GMW-5S-R-M24W1-061919

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc