

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062620\
 Data File : VX016973.D
 Acq On : 26 Jun 2020 11:19
 Operator : JC/SP
 Sample : L3020-25
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jun 27 02:59:38 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062620W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 26 08:34:16 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	201372	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	358982	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	357758	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	180693	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.03	65	151804	49.92	ug/l	0.00
Spiked Amount			Recovery	=	99.84%	
35) Dibromofluoromethane	5.47	113	116762	49.25	ug/l	0.00
Spiked Amount			Recovery	=	98.50%	
50) Toluene-d8	8.70	98	448447	51.60	ug/l	0.00
Spiked Amount			Recovery	=	103.20%	
62) 4-Bromofluorobenzene	11.12	95	178091	52.99	ug/l	0.00
Spiked Amount			Recovery	=	105.98%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.32	50	650	0.263	ug/l	91
5) Bromomethane	1.64	94	791	Below Cal	#	45
10) Methyl Iodide	2.49	142	808	3.059	ug/l #	77
11) Tert butyl alcohol	3.00	59	2052	3.574	ug/l	97
12) 1,1-Dichloroethene	2.36	96	600	0.269	ug/l #	62
13) Acrolein	2.28	56	502	1.180	ug/l #	53
15) Acrylonitrile	3.10	53	806	0.605	ug/l #	82
16) Acetone	2.42	43	8910	7.496	ug/l	97
17) Carbon Disulfide	2.56	76	3209	0.453	ug/l #	86
18) Methyl Acetate	2.75	43	1210	0.418	ug/l #	65
20) Methylene Chloride	2.84	84	2138	0.791	ug/l #	94
21) trans-1,2-Dichloroethene	3.14	96	580	0.230	ug/l #	47
25) 2-Butanone	4.65	43	5903	3.258	ug/l #	83
29) Tetrahydrofuran	5.12	42	910	0.764	ug/l #	34
38) Carbon Tetrachloride	5.63	117	21899	5.821	ug/l #	15
49) 1,4-Dioxane	7.71	88	58	0.929	ug/l #	1
51) 4-Methyl-2-Pentanone	8.62	43	2228	0.606	ug/l	99
76) 1,2,3-Trichloropropane	11.12	75	98881	26.076	ug/l #	37
81) trans-1,4-Dichloro-2-buten	11.12	75	98881	66.203	ug/l #	9
89) n-Butylbenzene	12.37	91	2435	0.241	ug/l	97
92) 1,2-Dibromo-3-Chloropropan	12.98	75	290	0.303	ug/l #	28
93) 1,2,4-Trichlorobenzene	13.63	180	1116	0.312	ug/l	72
94) Hexachlorobutadiene	13.77	225	638	0.497	ug/l	95
95) Naphthalene	13.82	128	2560	0.218	ug/l	95
96) 1,2,3-Trichlorobenzene	14.00	180	1274	0.371	ug/l	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062620\
Data File : VX016973.D
Acq On : 26 Jun 2020 11:19
Operator : JC/SP
Sample : L3020-25
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jun 27 02:59:38 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062620W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 26 08:34:16 2020
Response via : Initial Calibration

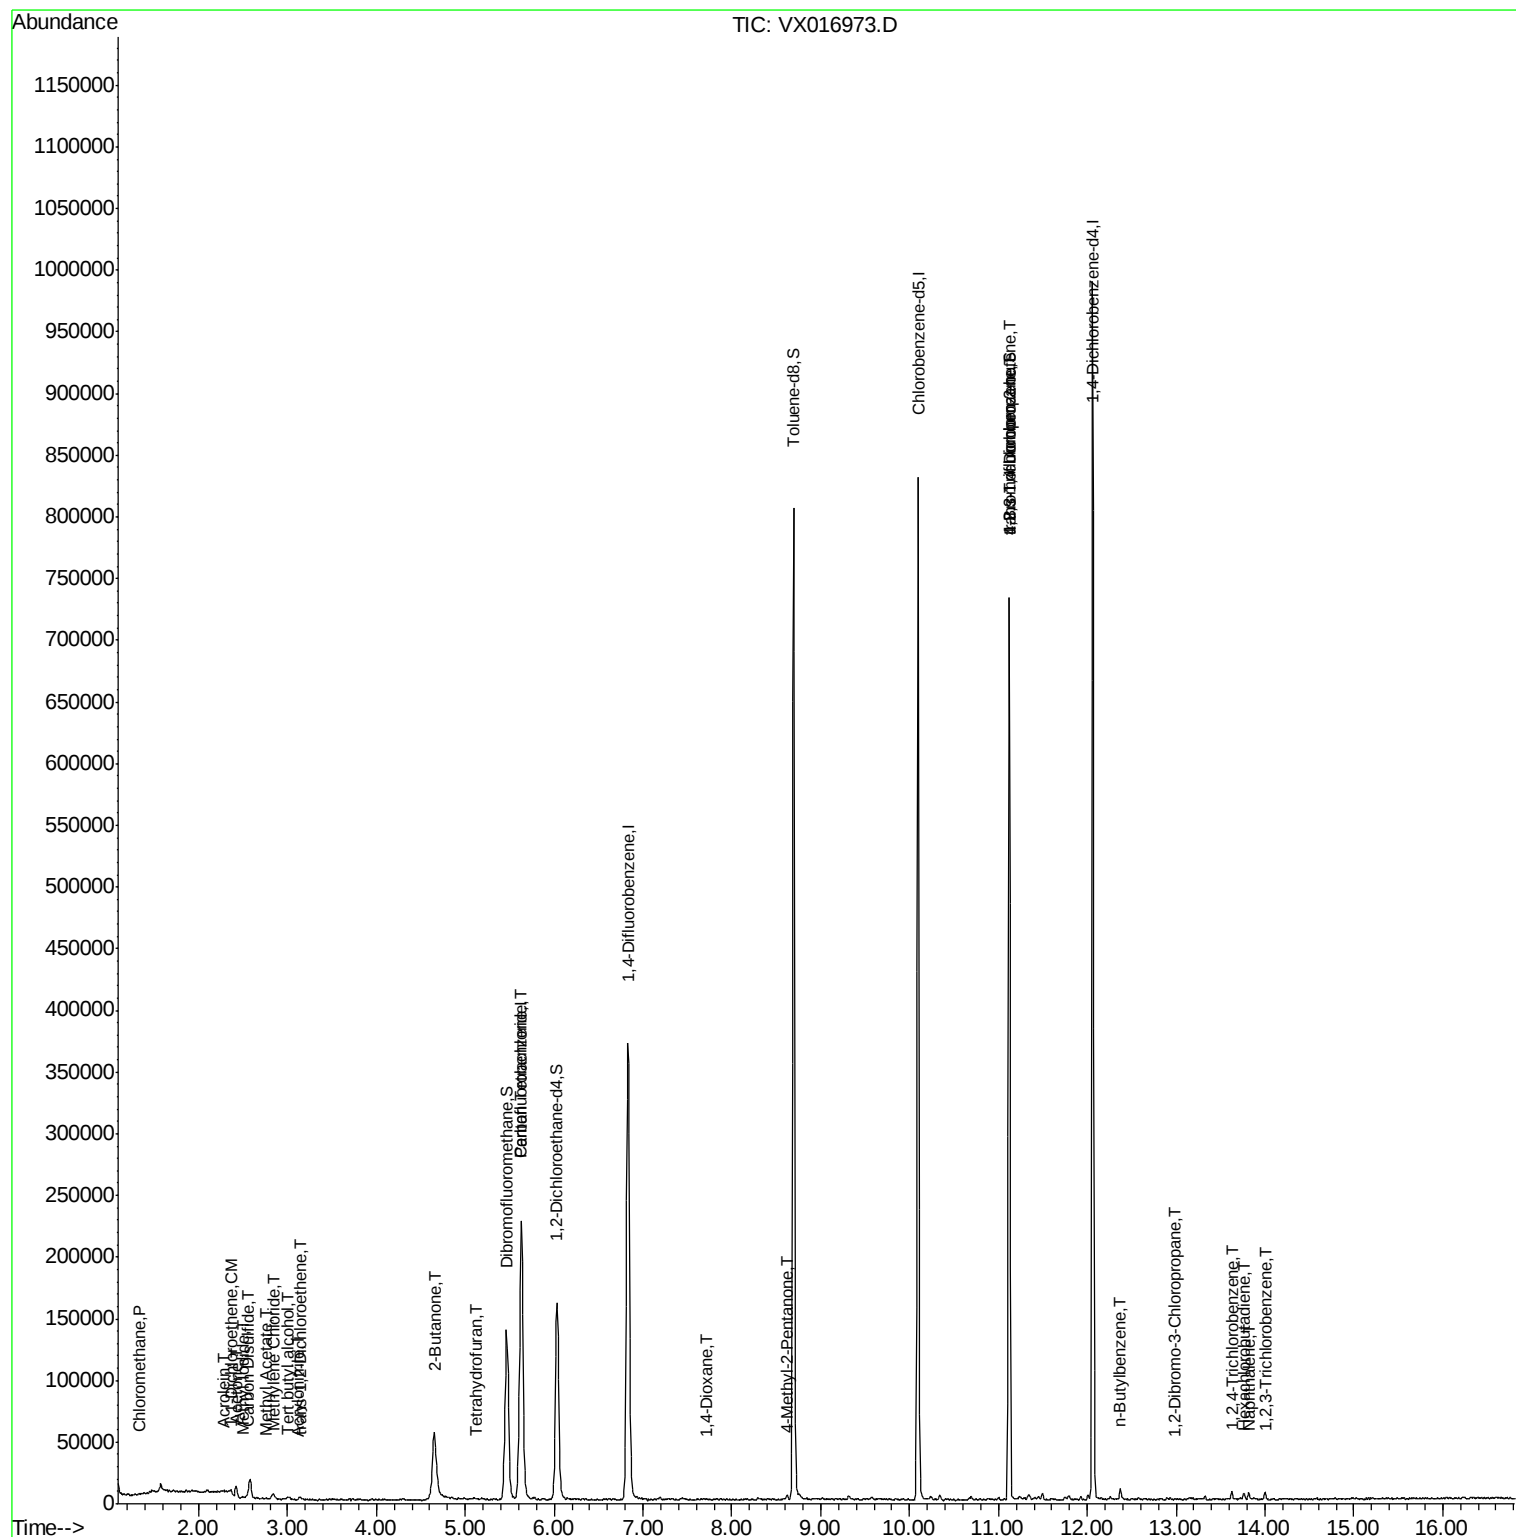

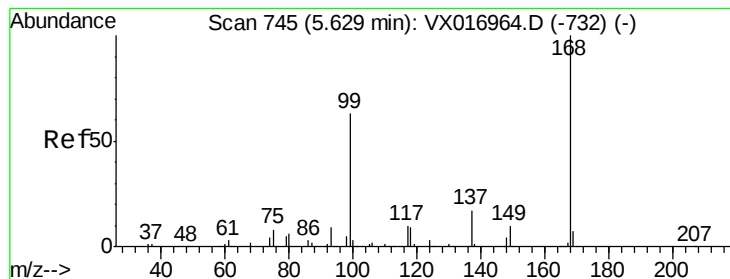

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 746

Delta R.T. 0.01 min

Lab File: VX016973.D

Acq: 26 Jun 2020 11:19

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion:168 Resp: 201372

Ion Ratio Lower Upper




168 100

99 60.0 50.2 75.2



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

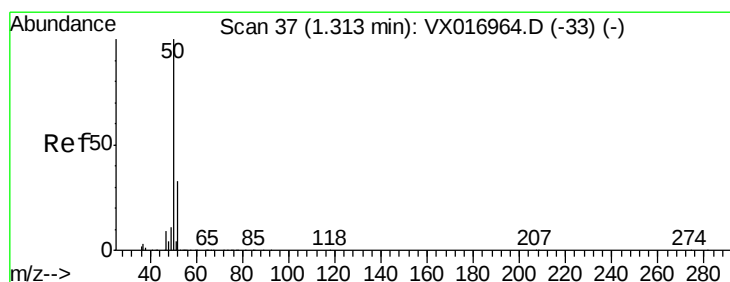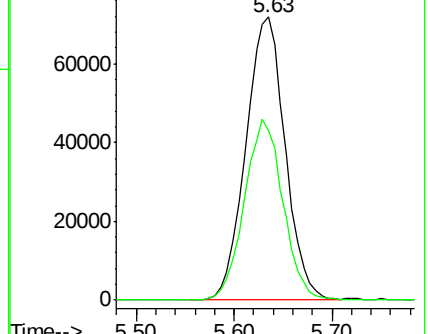

#3

Chloromethane

Concen: 0.263 ug/l

RT: 1.32 min Scan# 38

Delta R.T. 0.01 min

Lab File: VX016973.D


Acq: 26 Jun 2020 11:19

Tgt Ion: 50 Resp: 650

Ion Ratio Lower Upper



50 100


52 38.4 26.6 40.0

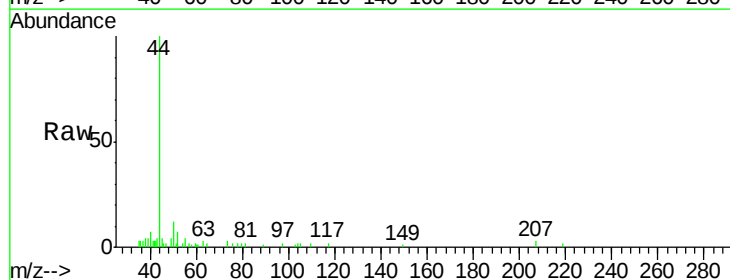

Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

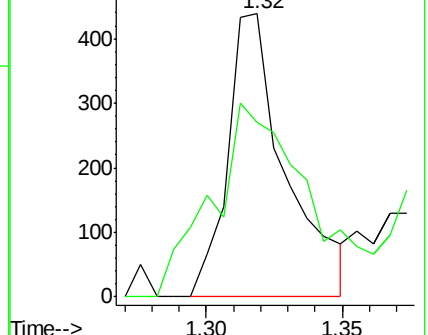

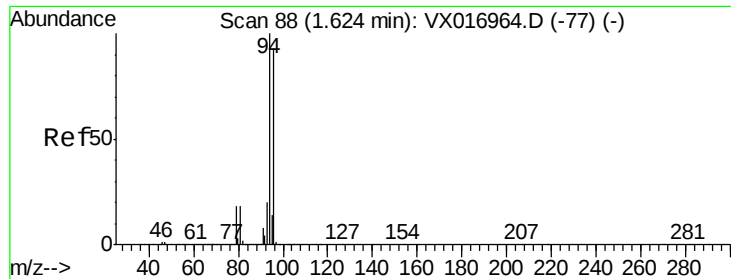

#5

Bromomethane

Concen: Below Cal

RT: 1.64 min Scan# 91

Delta R.T. 0.02 min

Lab File: VX016973.D

Acq: 26 Jun 2020 11:19

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion: 94 Resp: 791

Ion Ratio Lower Upper


94 100

96 39.9 74.2 111.2#


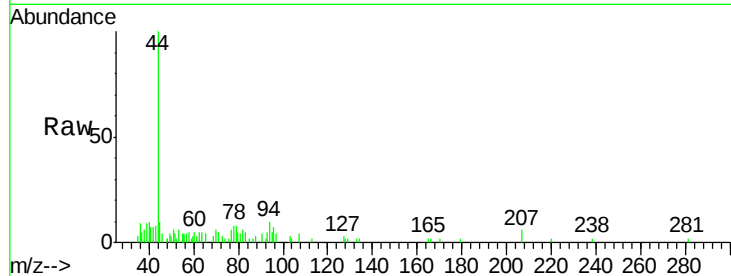


Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

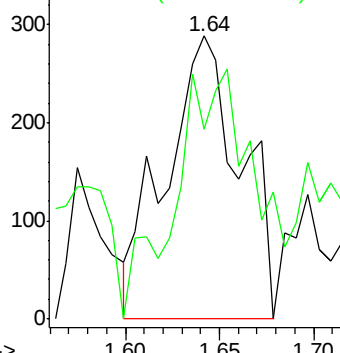

Time-->

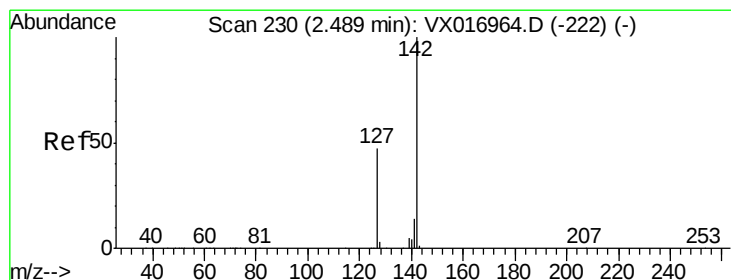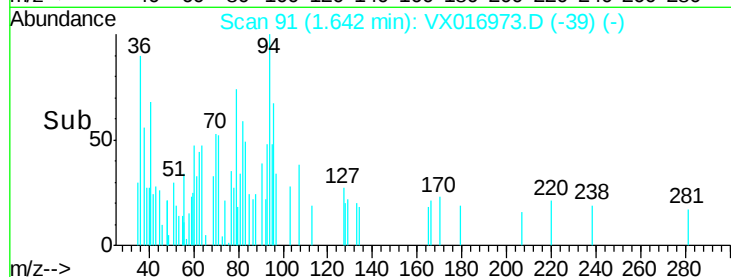

#10

Methyl Iodide

Concen: 3.059 ug/l

RT: 2.49 min Scan# 230

Delta R.T. 0.00 min

Lab File: VX016973.D

Acq: 26 Jun 2020 11:19


Tgt Ion:142 Resp: 808

Ion Ratio Lower Upper

142 100

127 65.1 37.4 56.0#


141 18.6 11.7 17.5#

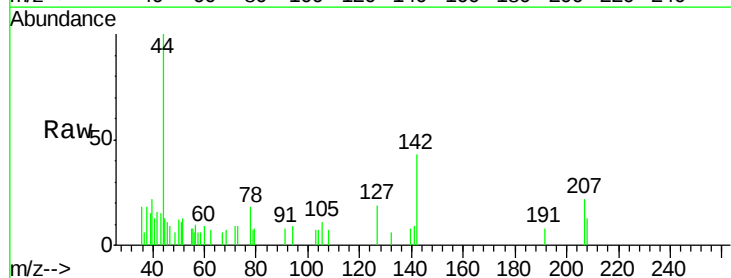


Abundance Ion 141.80 (141.50 to 142.50): V


Ion 126.80 (126.50 to 127.50): V

Ion 140.80 (140.50 to 141.50): V

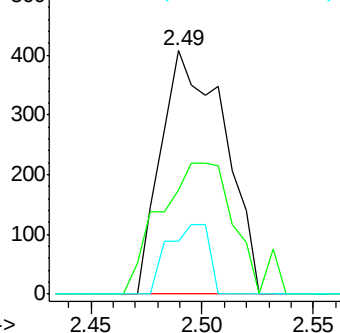

Time-->

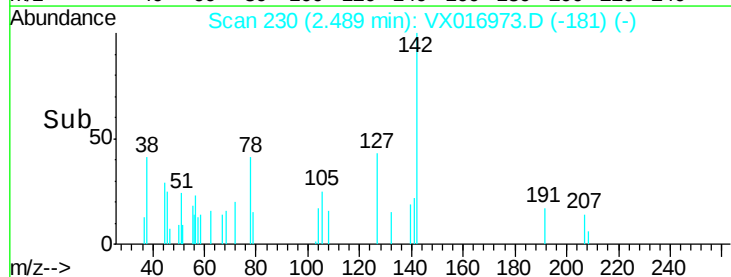




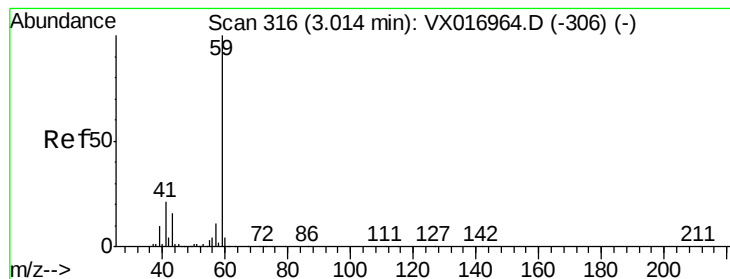


#11

Tert butyl alcohol
Concen: 3.574 ug/l
RT: 3.00 min Scan# 314
Delta R.T. -0.01 min
Lab File: VX016973.D
Acq: 26 Jun 2020 11:19

Instrument :
MSVOA_X
ClientSampleId :




Tot Ion: 59 Resp: 2052
Ion Ratio Lower Upper
59 100
57 9.4 8.5 12.7

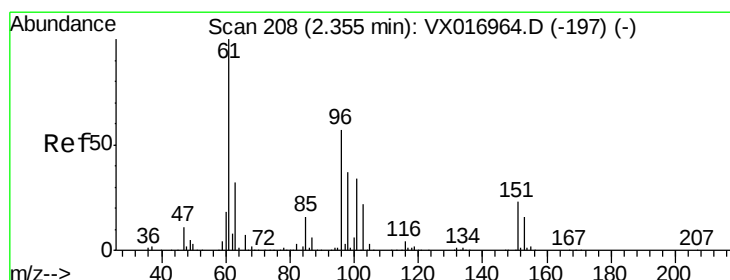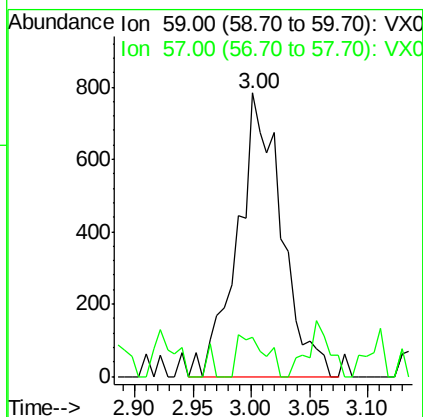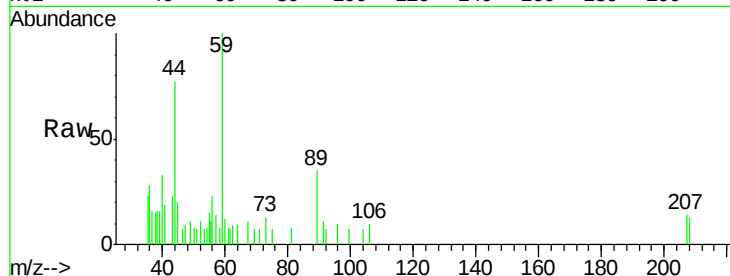


#12

1,1-Dichloroethene
Concen: 0.269 ug/l
RT: 2.36 min Scan# 209
Delta R.T. 0.01 min
Lab File: VX016973.D
Acq: 26 Jun 2020 11:19

Tgt Ion: 96 Resp: 600
Ion Ratio Lower Upper
96 100
61 103.9 139.7 209.5#
98 62.1 51.0 76.6

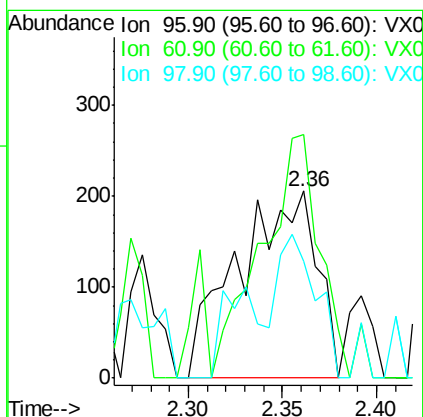



#13

Acrolein

Concen: 1.180 ug/l

RT: 2.28 min Scan# 196

Delta R.T. 0.01 min

Lab File: VX016973.D

Acq: 26 Jun 2020 11:19


Instrument :
MSVOA_X
ClientSampled :

Tot Ion: 56 Resp: 502

Ion Ratio Lower Upper




56 100

55 111.4 57.5 86.3#

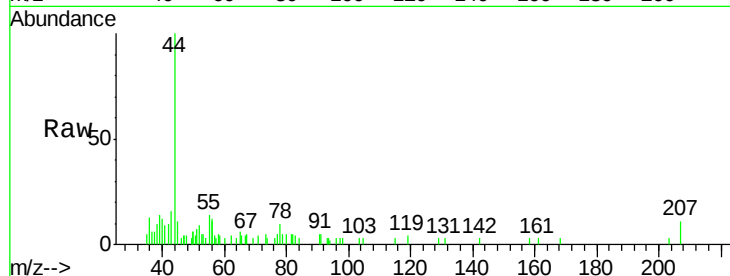

Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

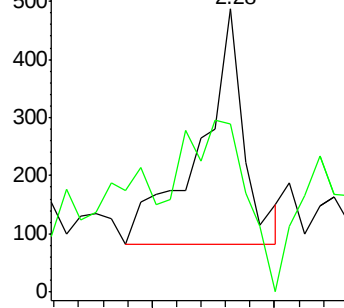

#15

Acrylonitrile

Concen: 0.605 ug/l

RT: 3.10 min Scan# 331

Delta R.T. -0.01 min

Lab File: VX016973.D

Acq: 26 Jun 2020 11:19


Tgt Ion: 53 Resp: 806

Ion Ratio Lower Upper

53 100

52 76.9 66.3 99.5



51 61.3 29.0 43.6#




Abundance Ion 53.00 (52.70 to 53.70): VX0

Ion 52.00 (51.70 to 52.70): VX0

Ion 51.00 (50.70 to 51.70): VX0

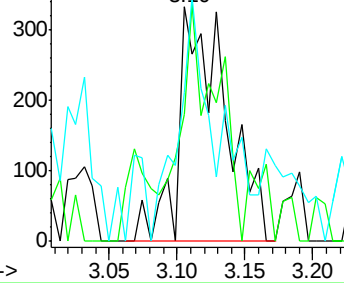

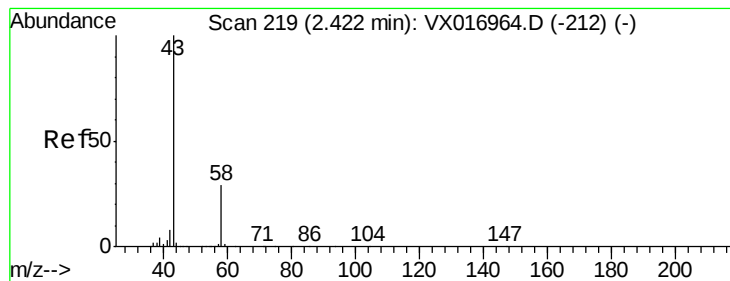

#16

Acetone

Concen: 7.496 ug/l

RT: 2.42 min Scan# 219

Delta R.T. -0.00 min

Lab File: VX016973.D

Acq: 26 Jun 2020 11:19

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion: 43 Resp: 8910

Ion Ratio Lower Upper




43 100

58 27.9 23.5 35.3



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

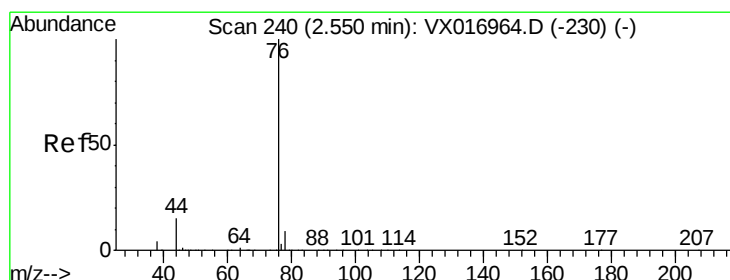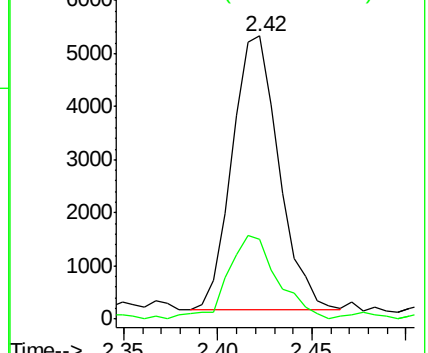

#17

Carbon Disulfide

Concen: 0.453 ug/l

RT: 2.56 min Scan# 241

Delta R.T. 0.01 min

Lab File: VX016973.D


Acq: 26 Jun 2020 11:19

Tgt Ion: 76 Resp: 3209

Ion Ratio Lower Upper



76 100


78 13.8 7.0 10.4#



Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

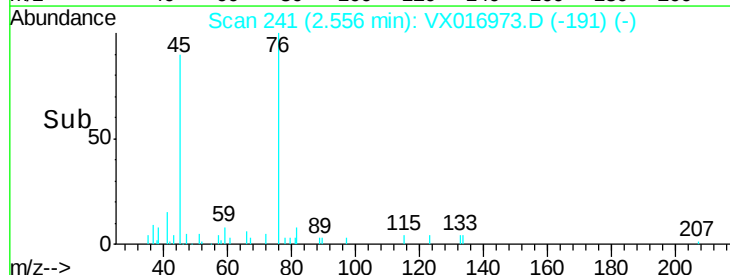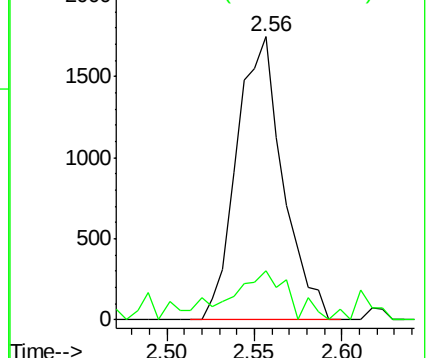

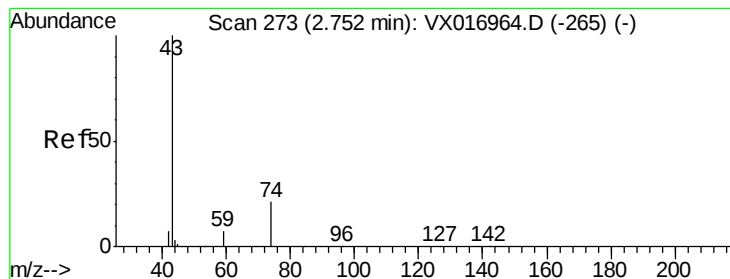

#18

Methyl Acetate

Concen: 0.418 ug/l

RT: 2.75 min Scan# 273

Delta R.T. -0.00 min

Lab File: VX016973.D

Acq: 26 Jun 2020 11:19

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion: 43 Resp: 1210

Ion Ratio Lower Upper




43 100

74 39.8 18.3 27.5#

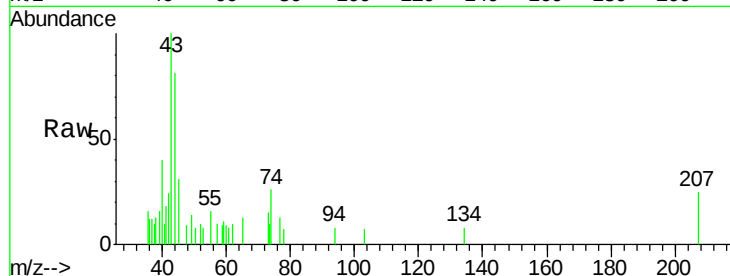

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 74.00 (73.70 to 74.70): VX0

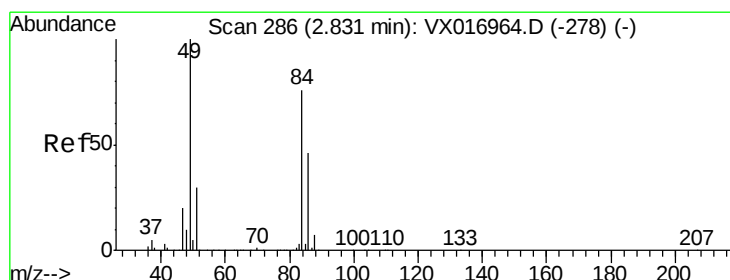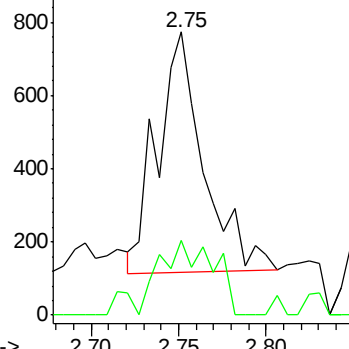

#20

Methylene Chloride

Concen: 0.791 ug/l

RT: 2.84 min Scan# 287

Delta R.T. 0.01 min

Lab File: VX016973.D

Acq: 26 Jun 2020 11:19

Tgt Ion: 84 Resp: 2138


Ion Ratio Lower Upper

84 100

49 131.1 105.6 158.4

51 38.8 31.2 46.8

86 77.9 48.8 73.2#






Abundance Ion 83.90 (83.60 to 84.60): VX0

Ion 48.90 (48.60 to 49.60): VX0

Ion 50.90 (50.60 to 51.60): VX0

Ion 85.90 (85.60 to 86.60): VX0

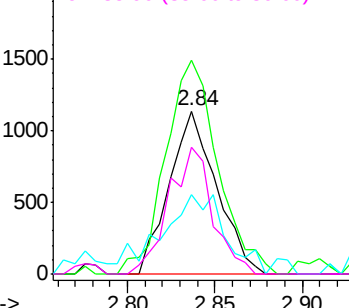

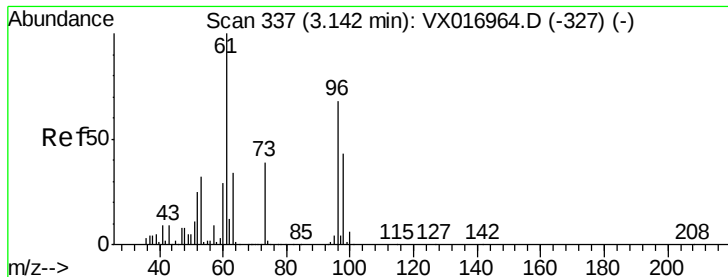

#21

trans-1,2-Dichloroethene

Concen: 0.230 ug/l

RT: 3.14 min Scan# 337

Delta R.T. -0.00 min

Lab File: VX016973.D

Acq: 26 Jun 2020 11:19

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion: 96 Resp: 580

Ion Ratio Lower Upper




96 100

61 52.7 116.7 175.1#

98 61.7 50.7 76.1

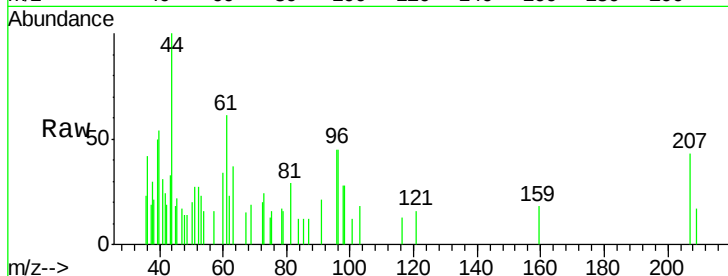

Abundance Ion 95.90 (95.60 to 96.60): VX0
Ion 60.90 (60.60 to 61.60): VX0
Ion 97.90 (97.60 to 98.60): VX0

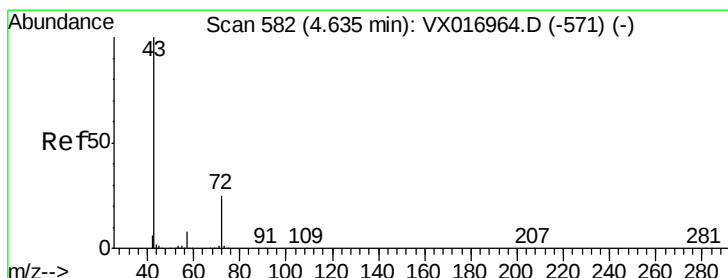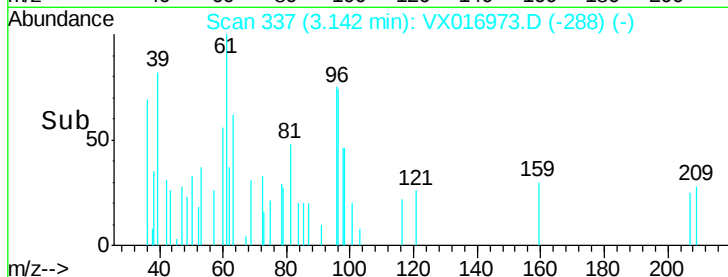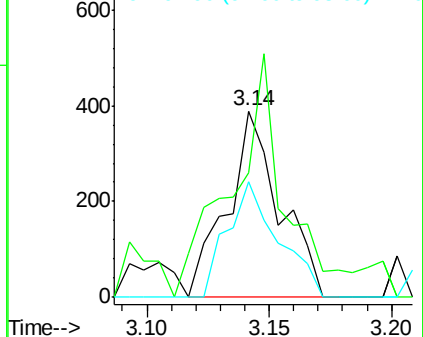

#25

2-Butanone

Concen: 3.258 ug/l

RT: 4.65 min Scan# 585

Delta R.T. 0.02 min

Lab File: VX016973.D


Acq: 26 Jun 2020 11:19

Tgt Ion: 43 Resp: 5903



Ion Ratio Lower Upper


43 100

72 16.6 20.0 30.0#

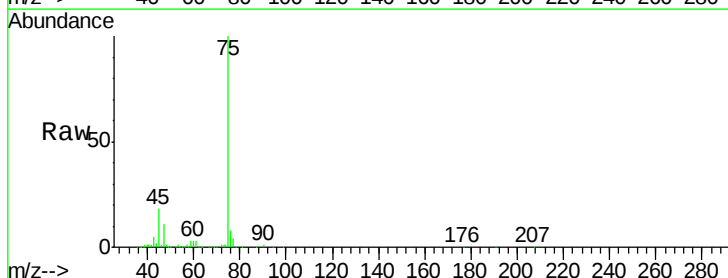

Abundance Ion 43.00 (42.70 to 43.70): VX0
Ion 72.00 (71.70 to 72.70): VX0



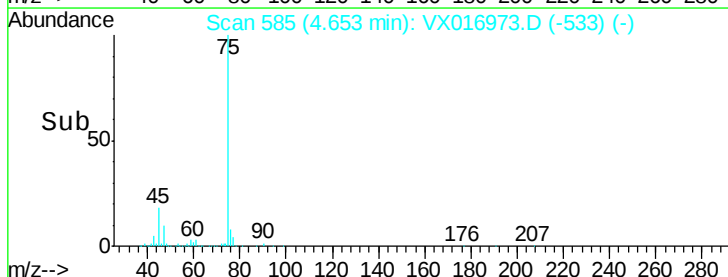
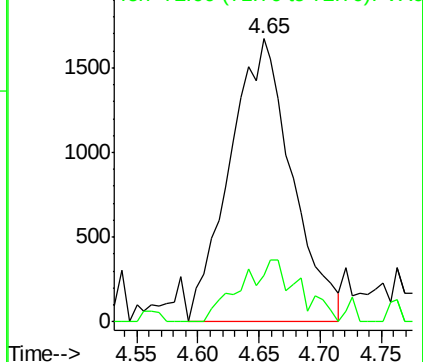




#29
Tetrahydrofuran
Concen: 0.764 ug/l
RT: 5.12 min Scan# 662
Delta R.T. 0.04 min
Lab File: VX016973.D
Acq: 26 Jun 2020 11:19




Instrument :
MSVOA_X
ClientSampled :


Tot Ion: 42 Resp: 910
Ion Ratio Lower Upper
42 100
72 0.0 34.1 51.1#
71 0.0 32.1 48.1#

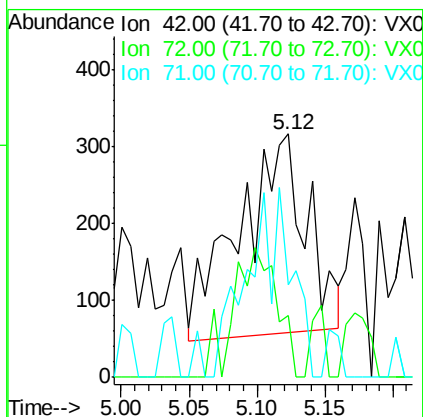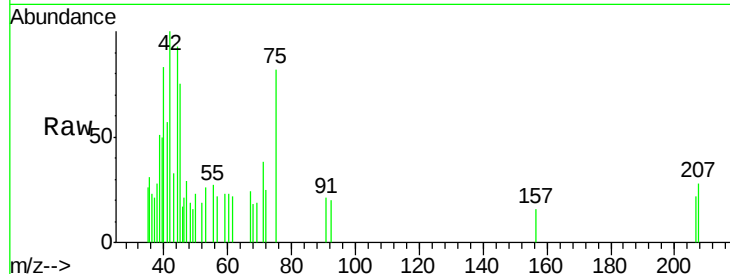

#33
1,2-Dichloroethane-d4
Concen: 49.920 ug/l
RT: 6.03 min Scan# 811
Delta R.T. -0.00 min
Lab File: VX016973.D
Acq: 26 Jun 2020 11:19

Tgt Ion: 65 Resp: 151804
Ion Ratio Lower Upper
65 100
67 50.5 0.0 102.8

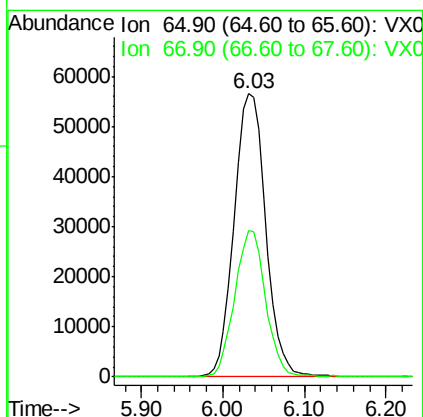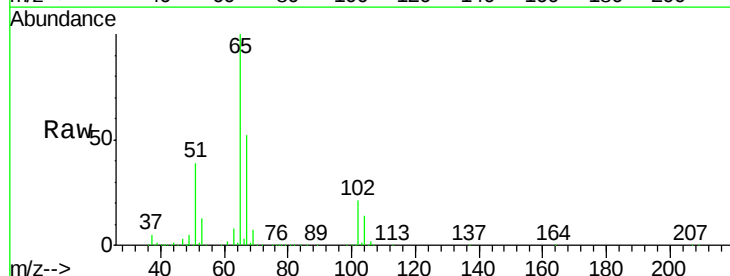

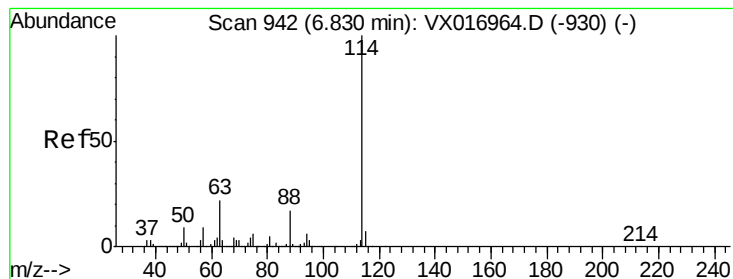

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX016973.D

Acq: 26 Jun 2020 11:19

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion:114 Resp: 358982

Ion Ratio Lower Upper

114 100

63 21.6 0.0 44.4




88 15.9 0.0 33.2

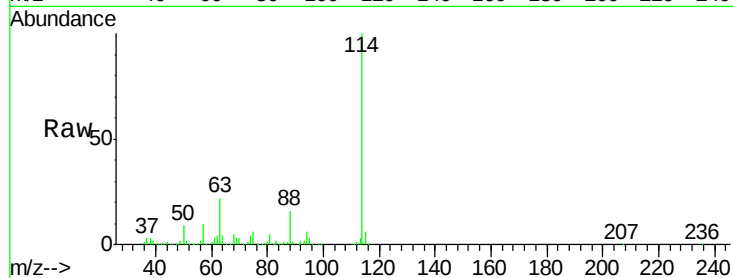

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

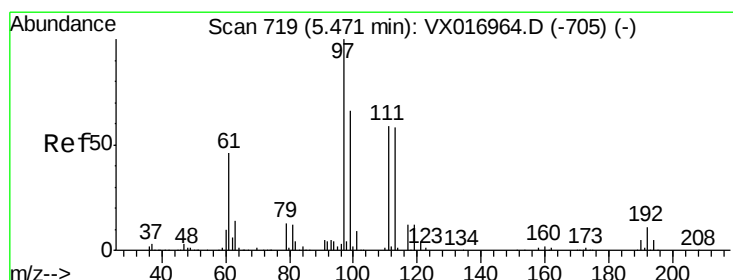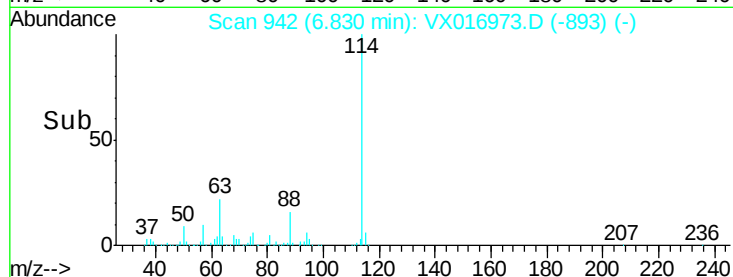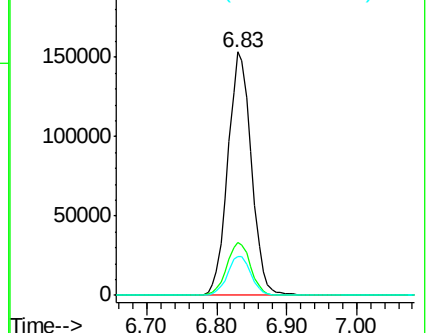

#35

Dibromofluoromethane

Concen: 49.246 ug/l

RT: 5.47 min Scan# 719

Delta R.T. -0.00 min

Lab File: VX016973.D

Acq: 26 Jun 2020 11:19


Tgt Ion:113 Resp: 116762

Ion Ratio Lower Upper

113 100

111 103.6 84.3 126.5



192 19.0 15.2 22.8

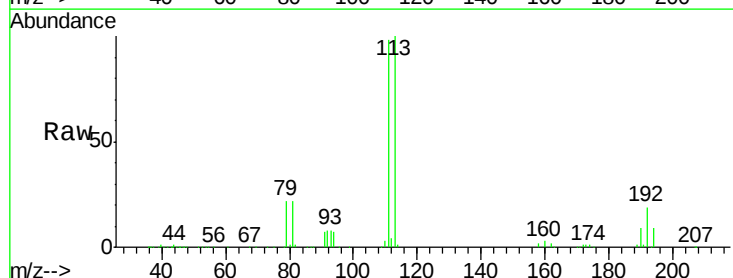


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

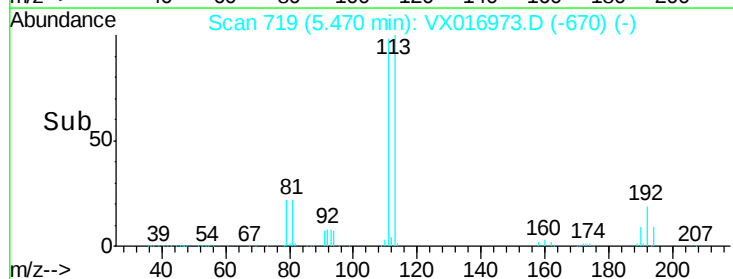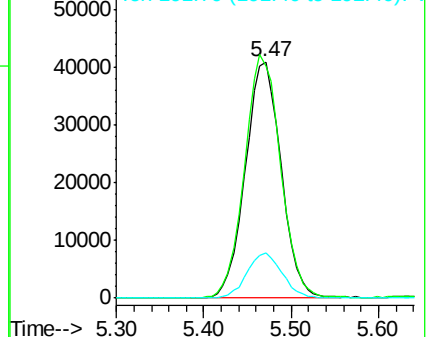

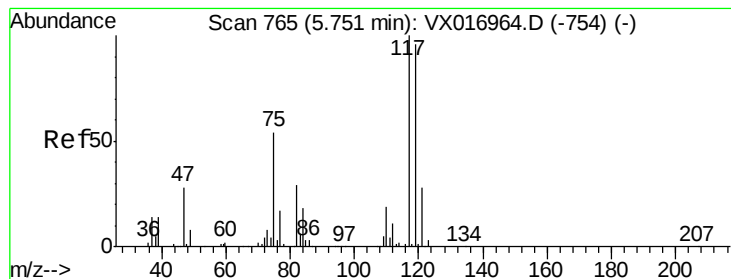

#38

Carbon Tetrachloride

Concen: 5.821 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.12 min

Lab File: VX016973.D

Acq: 26 Jun 2020 11:19

Instrument :

MSVOA_X

ClientSampled :


Tot Ion:117 Resp: 21899

Ion Ratio Lower Upper

117 100

119 3.9 76.6 114.8#




121 0.0 22.5 33.7#

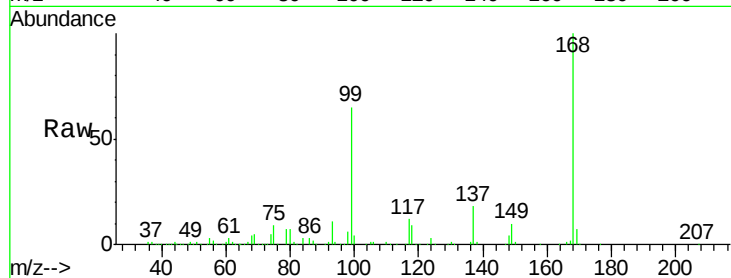

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

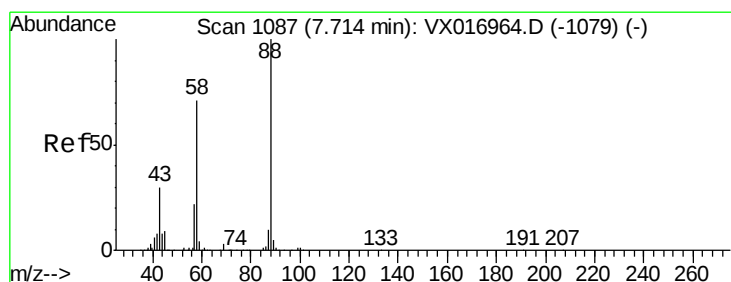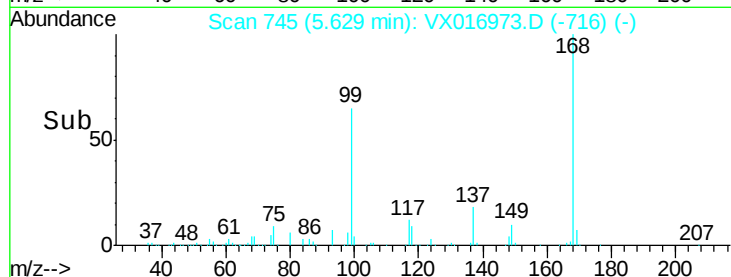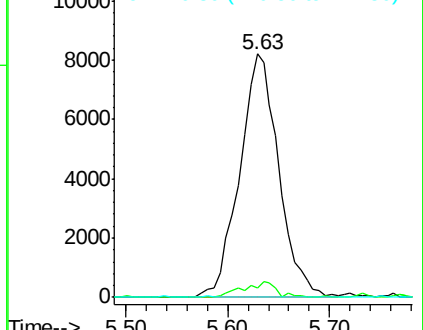

#49

1,4-Dioxane

Concen: 0.929 ug/l

RT: 7.71 min Scan# 1087

Delta R.T. -0.00 min

Lab File: VX016973.D

Acq: 26 Jun 2020 11:19


Tgt Ion: 88 Resp: 58

Ion Ratio Lower Upper

88 100

43 0.0 28.1 42.1#



58 308.6 56.1 84.1#

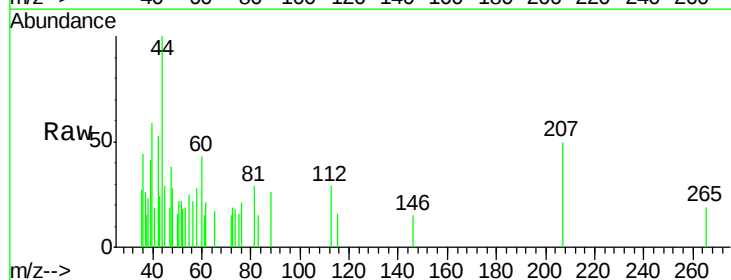


Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

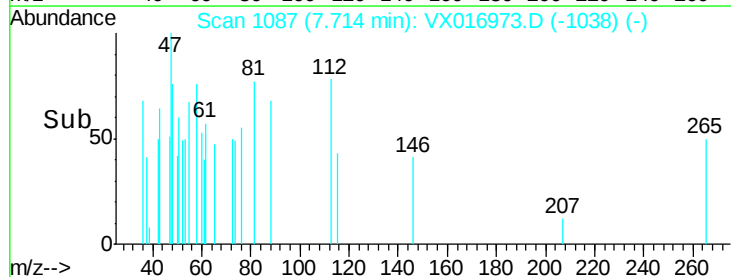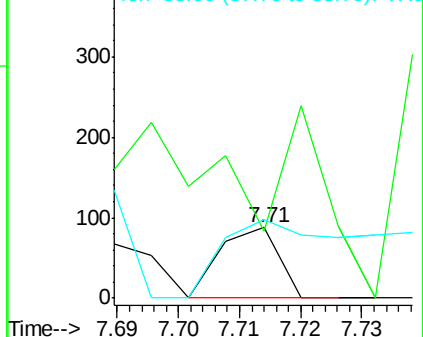

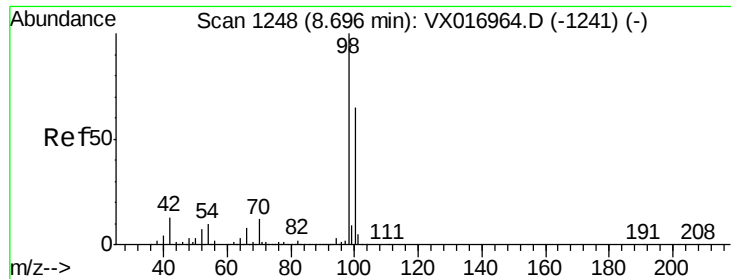

#50

Toluene-d8

Concen: 51.599 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. -0.00 min

Lab File: VX016973.D

Acq: 26 Jun 2020 11:19

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion: 98 Resp: 448447

Ion Ratio Lower Upper




98 100

100 66.1 52.2 78.2

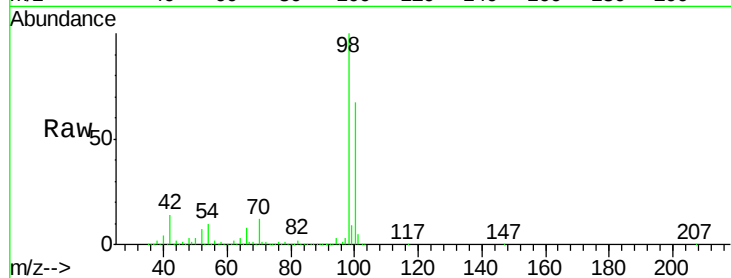

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

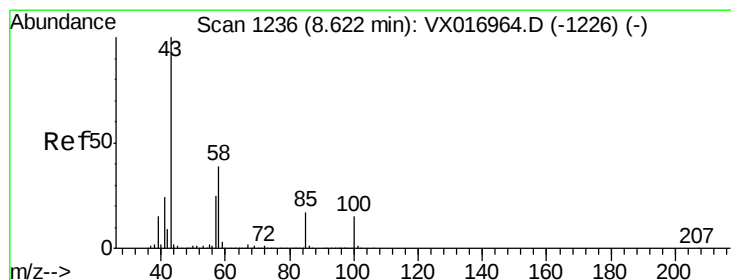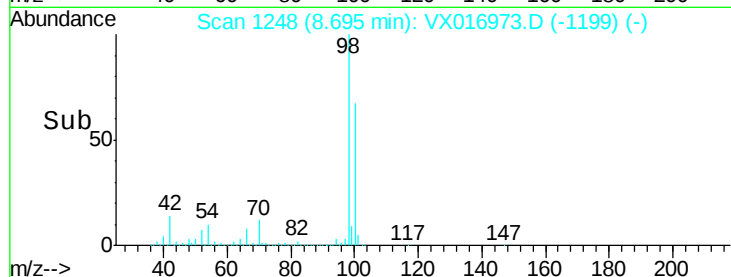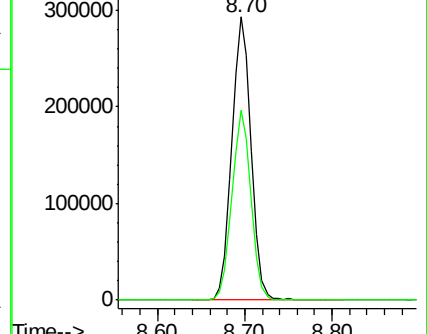

#51

4-Methyl-2-Pentanone

Concen: 0.606 ug/l

RT: 8.62 min Scan# 1235

Delta R.T. -0.01 min

Lab File: VX016973.D


Acq: 26 Jun 2020 11:19

Tgt Ion: 43 Resp: 2228

Ion Ratio Lower Upper



43 100


58 37.6 30.4 45.6

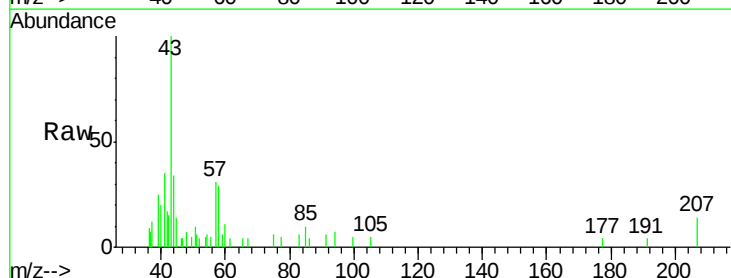

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

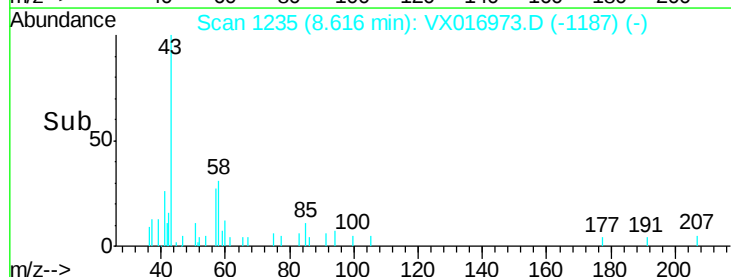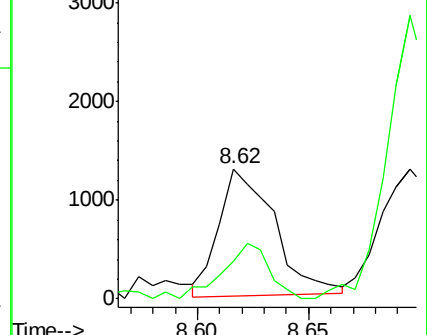

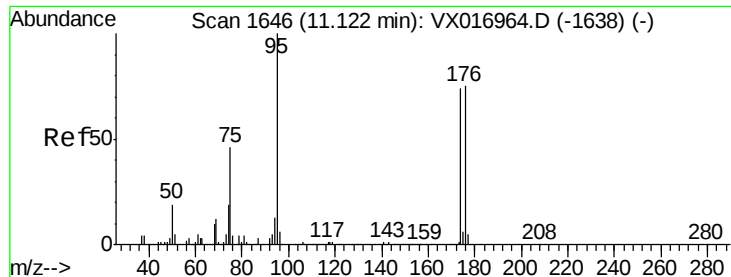

#62

4-Bromofluorobenzene

Concen: 52.991 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX016973.D

Acq: 26 Jun 2020 11:19

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion: 95 Resp: 178091

Ion Ratio Lower Upper

95 100

174 76.1 0.0 149.6




176 73.7 0.0 148.2

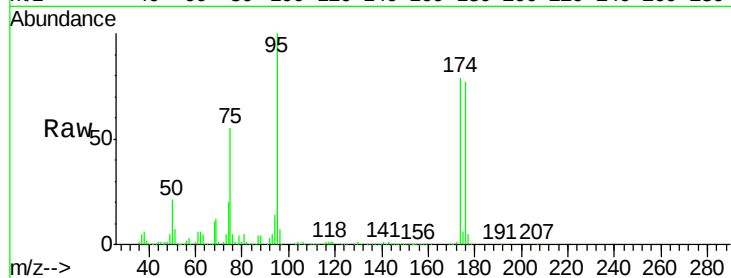

Abundance Ion 94.90 (94.60 to 95.60): VX016973.D (-1597) (-)

Ion 173.80 (173.50 to 174.50): VX016973.D (-1597) (-)

Ion 175.80 (175.50 to 176.50): VX016973.D (-1597) (-)

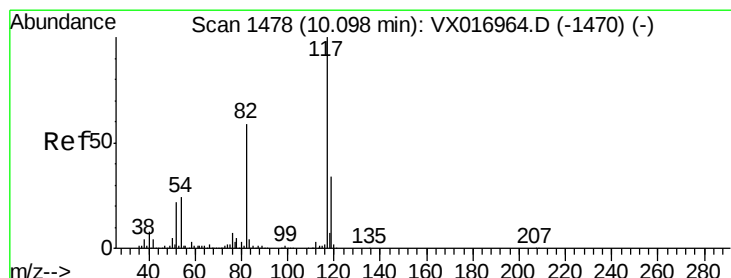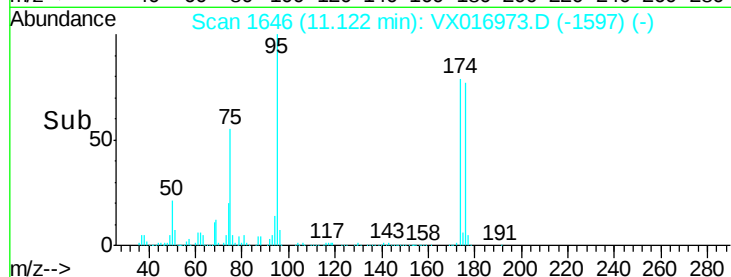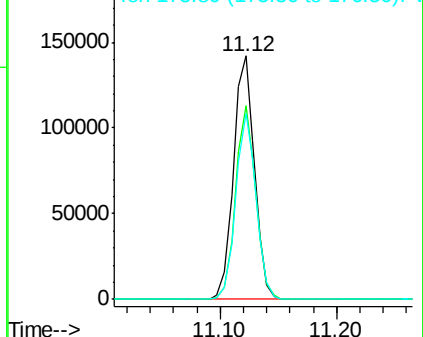

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.10 min Scan# 1478

Delta R.T. -0.00 min

Lab File: VX016973.D

Acq: 26 Jun 2020 11:19


Tgt Ion: 117 Resp: 357758

Ion Ratio Lower Upper

117 100

82 54.9 46.8 70.2



119 31.2 27.3 40.9

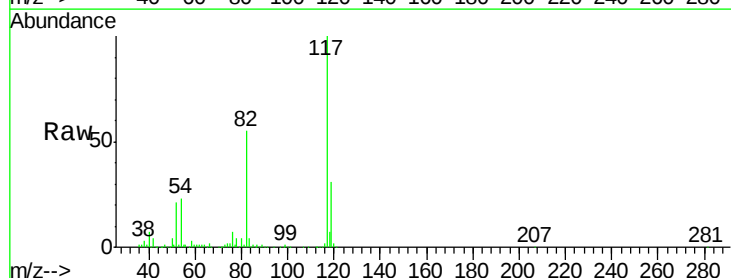


Abundance Ion 116.90 (116.60 to 117.60): VX016973.D (-1429) (-)

Ion 82.00 (81.70 to 82.70): VX016973.D (-1429) (-)

Ion 118.90 (118.60 to 119.60): VX016973.D (-1429) (-)

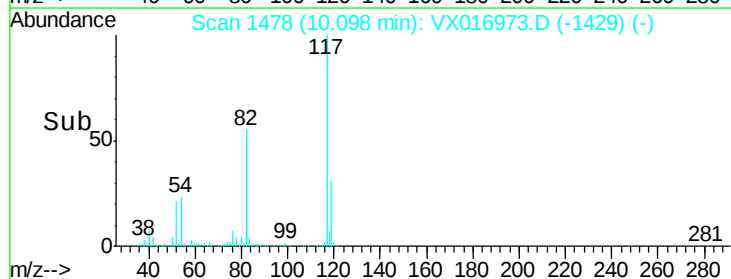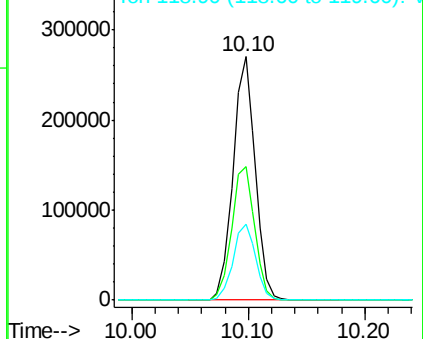

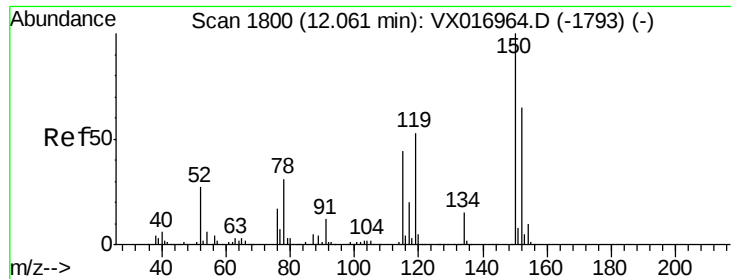

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX016973.D

Acq: 26 Jun 2020 11:19

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion:152 Resp: 180693

Ion Ratio Lower Upper

152 100

115 61.5 42.8 128.4




150 157.2 0.0 347.8

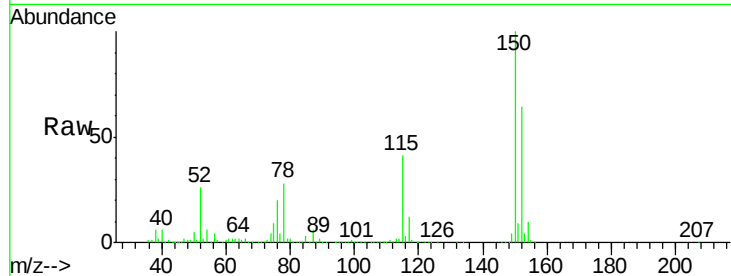

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

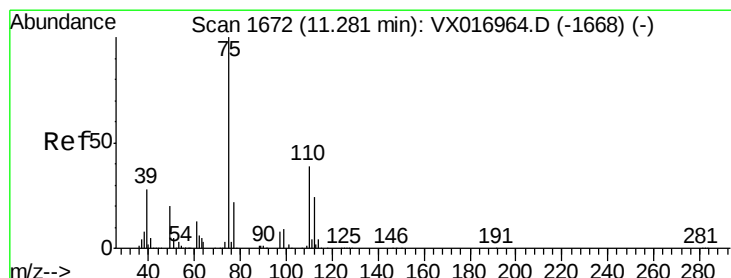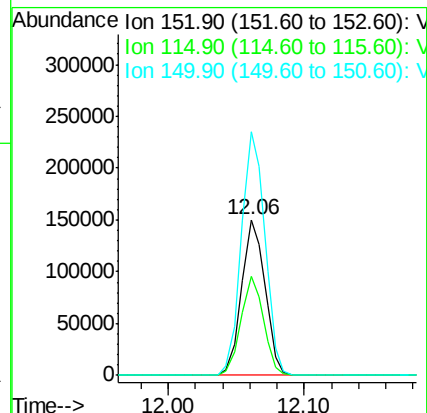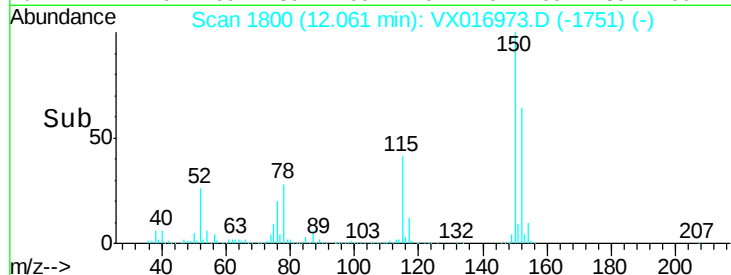

#76

1,2,3-Trichloropropane

Concen: 26.076 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX016973.D


Acq: 26 Jun 2020 11:19

Tgt Ion: 75 Resp: 98881

Ion Ratio Lower Upper



75 100


77 1.2 20.3 61.0#

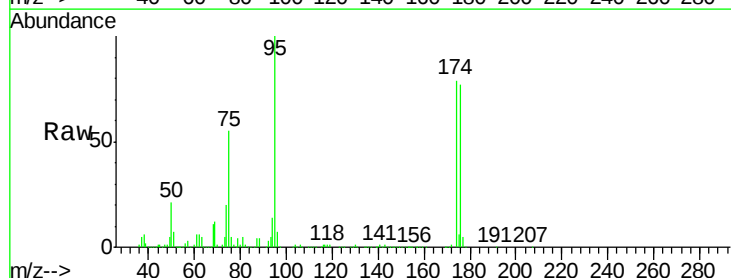

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

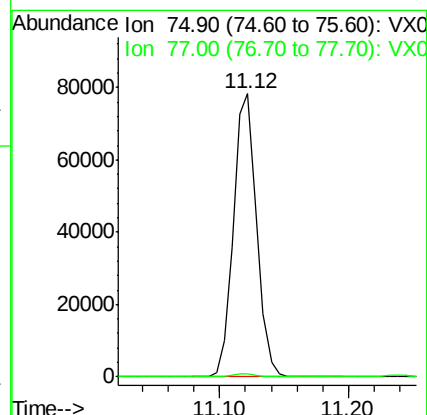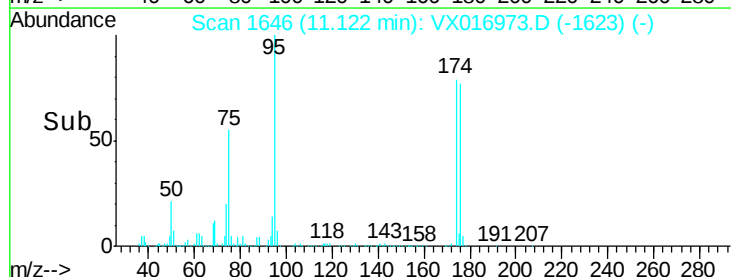



#81

trans-1,4-Dichloro-2-butene

Concen: 66.203 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.06 min

Lab File: VX016973.D

Acq: 26 Jun 2020 11:19

Instrument :

MSVOA_X

ClientSampled :


Tot Ion: 75 Resp: 98881

Ion Ratio Lower Upper

75 100

53 0.5 81.9 122.9#




89 0.0 35.5 53.3#

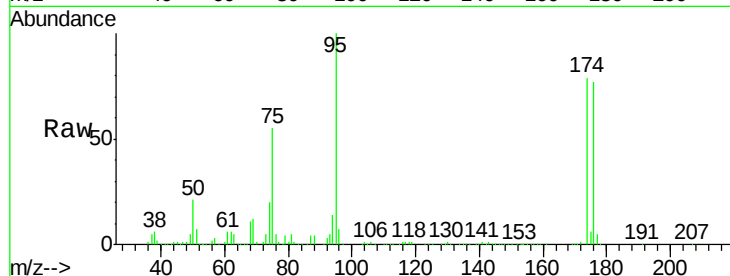

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

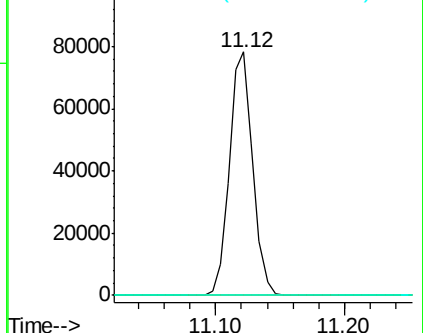

#89

n-Butylbenzene

Concen: 0.241 ug/l

RT: 12.37 min Scan# 1851

Delta R.T. -0.00 min

Lab File: VX016973.D

Acq: 26 Jun 2020 11:19


Tgt Ion: 91 Resp: 2435

Ion Ratio Lower Upper

91 100

92 52.9 26.6 79.7



134 21.3 12.6 37.8




Abundance Ion 91.00 (90.70 to 91.70): VX0

Ion 92.00 (91.70 to 92.70): VX0

Ion 134.00 (133.70 to 134.70): V



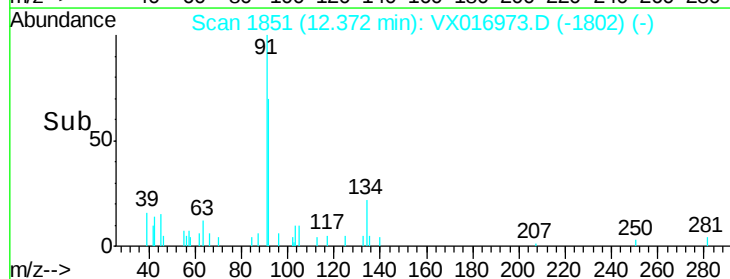
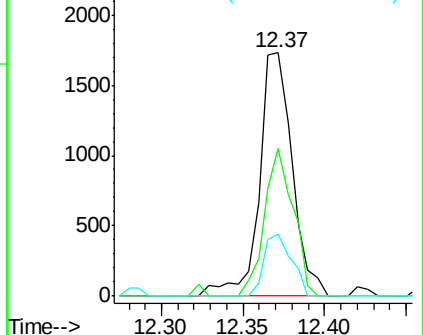




#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.303 ug/l
 RT: 12.98 min Scan# 1951
 Delta R.T. -0.00 min
 Lab File: VX016973.D
 Acq: 26 Jun 2020 11:19




Instrument :
 MSVOA_X
 ClientSampleId :


Tot Ion: 75 Resp: 290
 Ion Ratio Lower Upper
 75 100
 155 15.5 39.0 117.0#
 157 27.6 50.0 150.1#

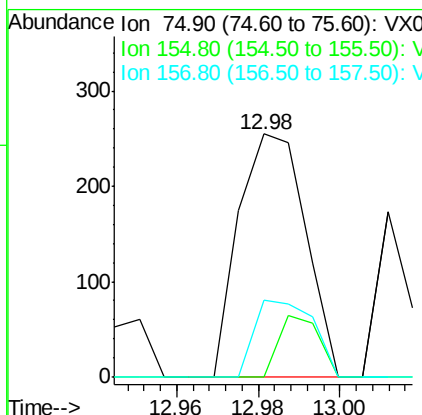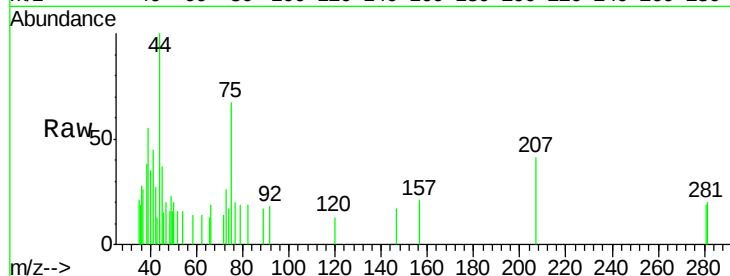

#93
 1,2,4-Trichlorobenzene
 Concen: 0.312 ug/l
 RT: 13.63 min Scan# 2057
 Delta R.T. -0.00 min
 Lab File: VX016973.D
 Acq: 26 Jun 2020 11:19

Tgt Ion:180 Resp: 1116
 Ion Ratio Lower Upper
 180 100
 182 123.7 46.4 139.1
 145 38.7 15.5 46.5

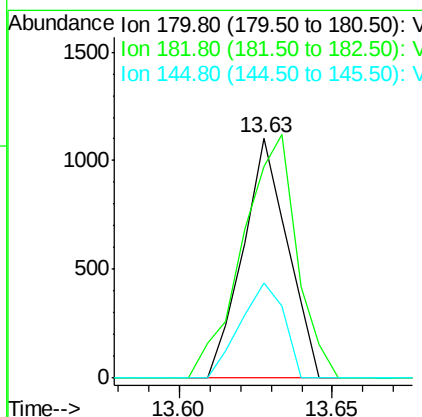



#94

Hexachlorobutadiene

Concen: 0.497 ug/l

RT: 13.77 min Scan# 2080

Delta R.T. 0.01 min

Lab File: VX016973.D

Acq: 26 Jun 2020 11:19

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion:225 Resp: 638

Ion Ratio Lower Upper




225 100

223 58.3 31.1 93.2

227 64.7 30.3 90.9



Abundance Ion 224.70 (224.40 to 225.40): V
Ion 222.70 (222.40 to 223.40): V
Ion 226.70 (226.40 to 227.40): V

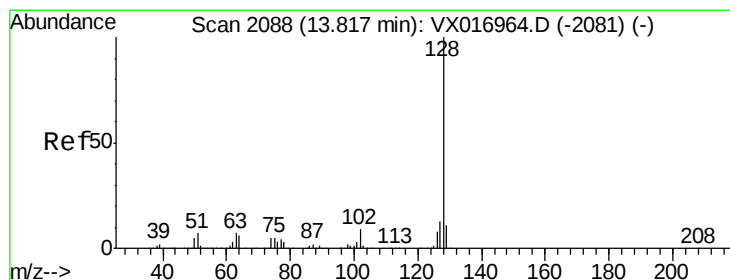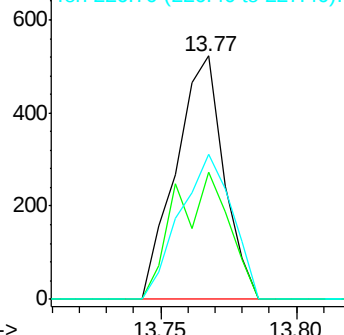

#95

Naphthalene

Concen: 0.218 ug/l

RT: 13.82 min Scan# 2088

Delta R.T. -0.00 min

Lab File: VX016973.D

Acq: 26 Jun 2020 11:19


Tgt Ion:128 Resp: 2560

Ion Ratio Lower Upper



128 100


127 15.5 10.6 15.8

129 12.3 8.7 13.1



Abundance Ion 128.00 (127.70 to 128.70): V
Ion 127.00 (126.70 to 127.70): V
Ion 129.00 (128.70 to 129.70): V

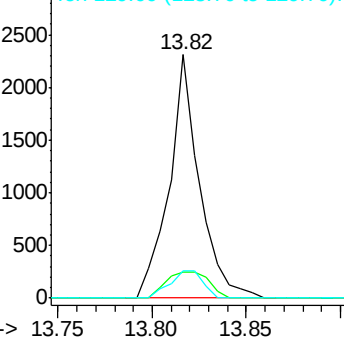

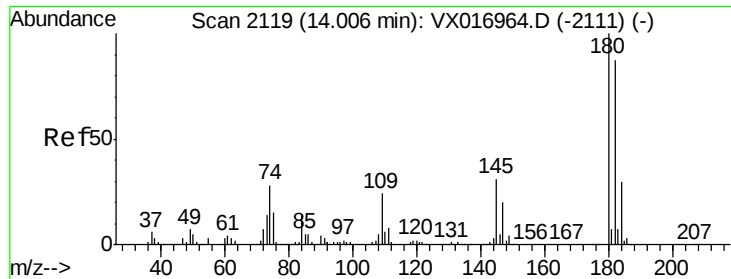

#96
 1,2,3-Trichlorobenzene
 Concen: 0.371 ug/l
 RT: 14.00 min Scan# 2118
 Delta R.T. -0.01 min
 Lab File: VX016973.D
 Acq: 26 Jun 2020 11:19

Instrument :
 MSVOA_X
 ClientSampleId :

Tot Ion:180 Resp: 1274
 Ion Ratio Lower Upper
 180 100
 182 80.1 47.8 143.3
 145 29.7 16.9 50.6

