


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062620\
Data File : VX016968.D
Acq On : 26 Jun 2020 08:55
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062620W.M
Title : SW846 8260
Last Update : Fri Jun 26 08:34:16 2020

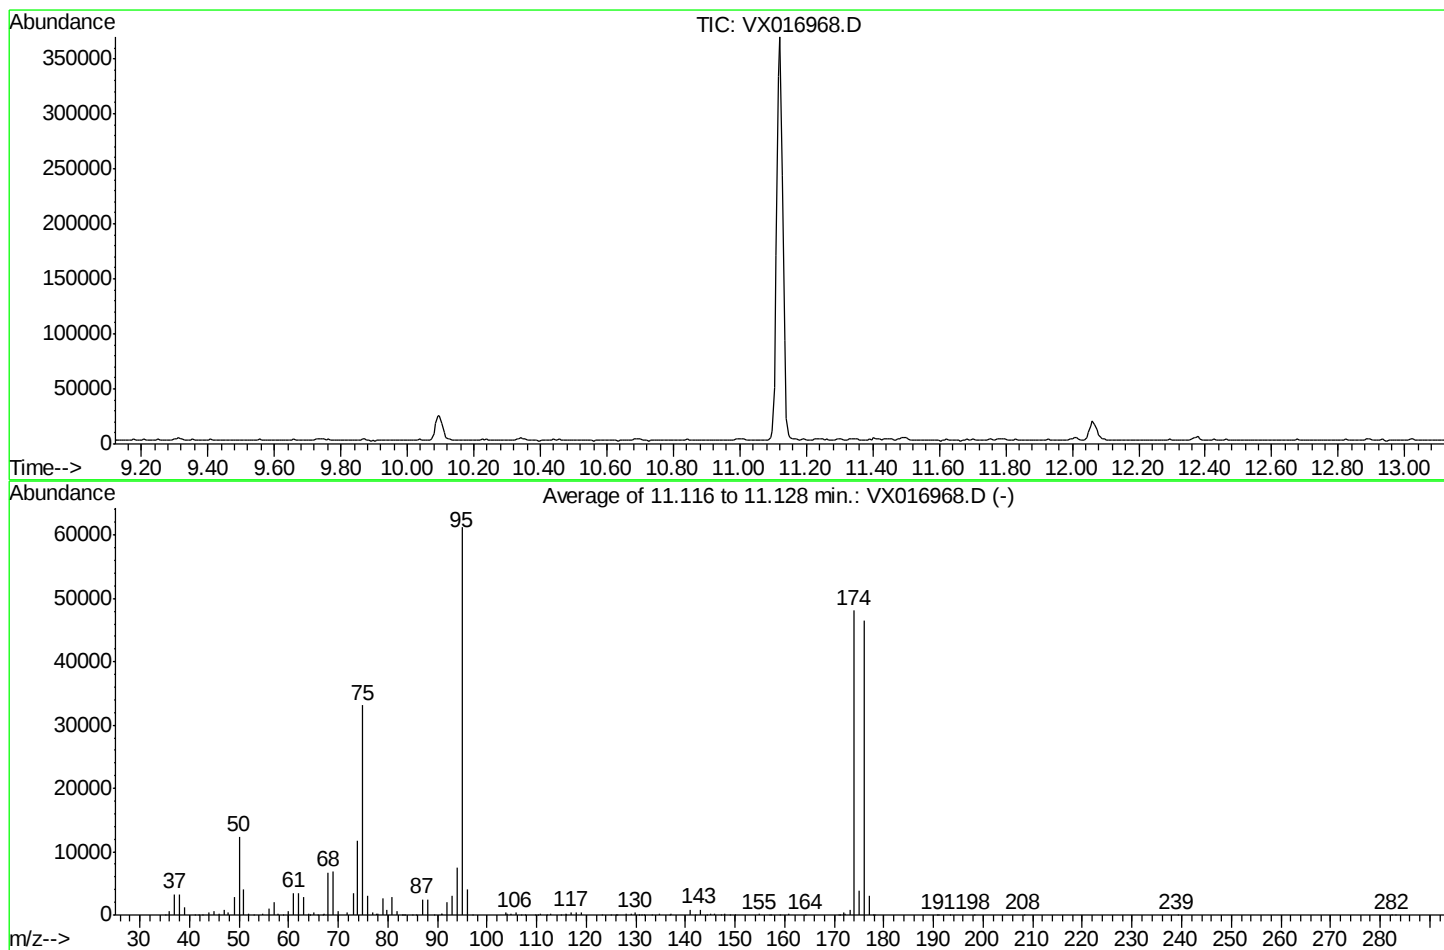

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	12398	PASS
75	95	30	60	54.1	33130	PASS
95	95	100	100	100.0	61232	PASS
96	95	5	9	6.7	4132	PASS
173	174	0.00	2	1.8	884	PASS
174	95	50	100	78.6	48104	PASS
175	174	5	9	7.9	3815	PASS
176	174	95	101	96.8	46554	PASS
177	176	5	9	6.4	2971	PASS