


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062620\
 Data File : VX016996.D
 Acq On : 26 Jun 2020 20:25
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X062520W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Jun 26 09:03:25 2020

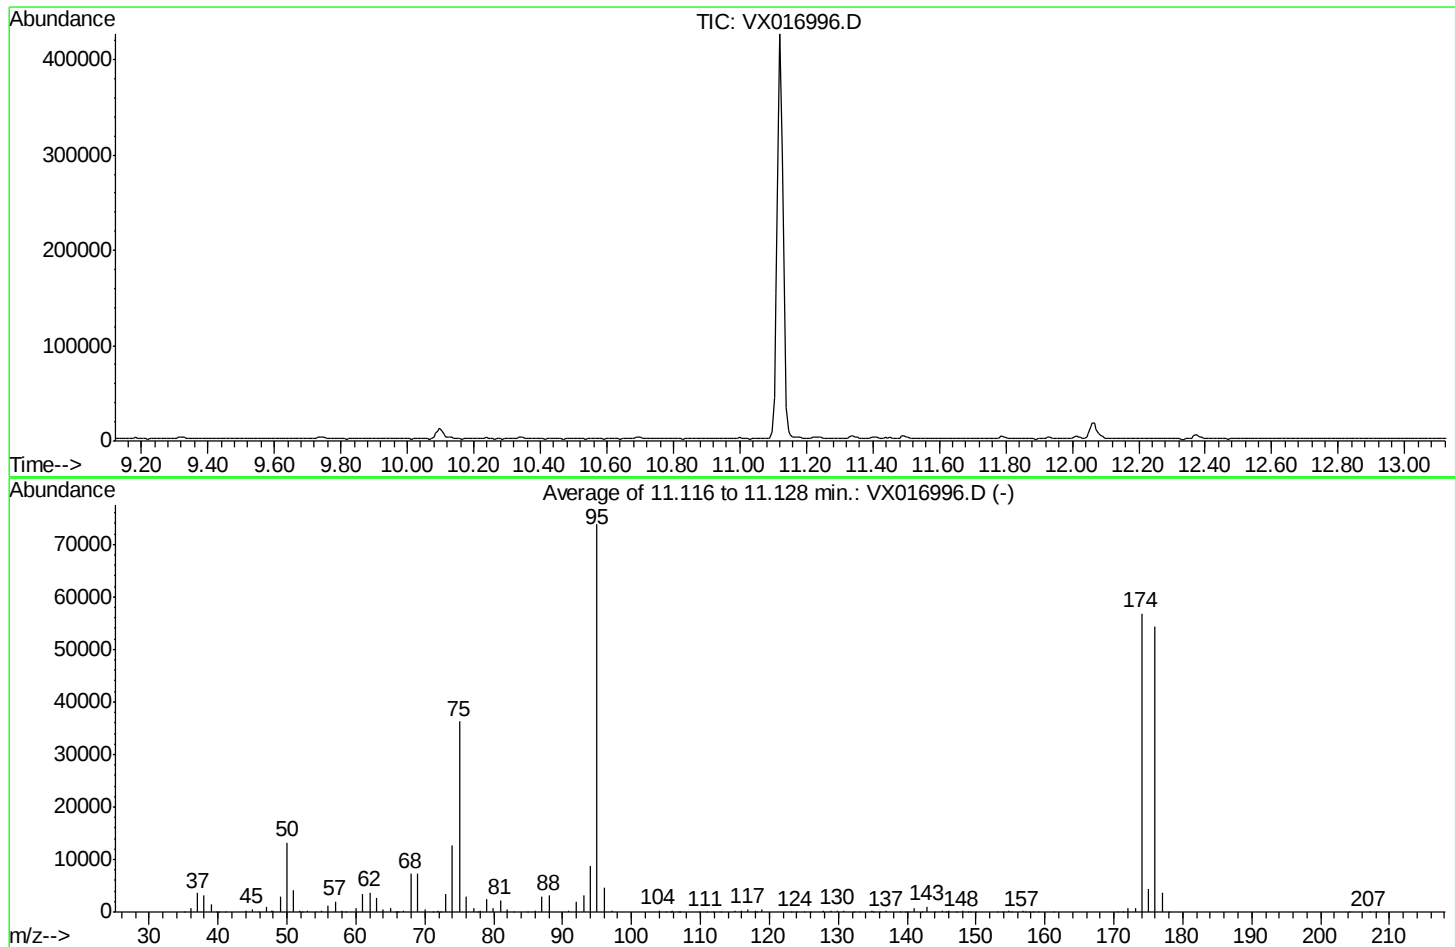

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1639

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	13251	PASS
75	95	30	60	49.2	36301	PASS
95	95	100	100	100.0	73802	PASS
96	95	5	9	6.4	4697	PASS
173	174	0.00	2	1.4	792	PASS
174	95	50	100	77.0	56810	PASS
175	174	5	9	7.7	4359	PASS
176	174	95	101	95.7	54344	PASS
177	176	5	9	6.6	3587	PASS