

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062623\
 Data File : VX036337.D
 Acq On : 26 Jun 2023 18:27
 Operator : JC/MD
 Sample : 03291-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
 Title : SW846 8260

Signal : TIC: VX036337.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	52	rBV	51003	53329	3.28%	0.189%
2	1.752	104	109	120	rVB	374877	495474	30.48%	1.756%
3	1.953	138	142	153	rVV	180030	256105	15.75%	0.908%
4	2.069	156	161	168	rVV	32146	47429	2.92%	0.168%
5	2.166	172	177	181	rVV	19367	32608	2.01%	0.116%
6	2.215	181	185	192	rVB	36642	53387	3.28%	0.189%
7	2.337	197	205	211	rBV2	20085	41284	2.54%	0.146%
8	2.715	259	267	272	rBV4	16674	44842	2.76%	0.159%
9	2.782	272	278	281	rVV	67653	145560	8.95%	0.516%
10	2.825	281	285	289	rVV	131680	268109	16.49%	0.950%
11	2.867	289	292	307	rVB3	71501	185565	11.41%	0.658%
12	3.099	321	330	342	rBV	146379	330532	20.33%	1.172%
13	3.331	358	368	378	rBV3	22538	58614	3.61%	0.208%
14	3.447	378	387	397	rVB	46194	100894	6.21%	0.358%
15	3.666	415	423	430	rBV	28504	65081	4.00%	0.231%
16	3.837	441	451	457	rBV2	19633	53003	3.26%	0.188%
17	3.904	457	462	466	rBV	13679	30575	1.88%	0.108%
18	4.306	517	528	540	rVB	295089	845062	51.98%	2.996%
19	4.818	595	612	618	rBV5	11524	35436	2.18%	0.126%
20	5.385	691	705	712	rBV	148286	449968	27.68%	1.595%
21	5.471	712	719	726	rVV	205178	643526	39.58%	2.281%
22	5.556	726	733	764	rVB	201113	721149	44.36%	2.557%
23	5.836	767	779	789	rBV6	39128	136576	8.40%	0.484%
24	5.958	789	799	810	rBV	172370	452732	27.85%	1.605%
25	6.159	819	832	842	rBV5	55049	208957	12.85%	0.741%
26	6.257	842	848	856	rVV2	52926	147939	9.10%	0.524%
27	6.355	856	864	875	rVB2	55492	153624	9.45%	0.545%
28	6.763	922	931	939	rBV	360891	853151	52.48%	3.024%
29	6.842	939	944	952	rVB3	23343	64678	3.98%	0.229%
30	7.178	990	999	1007	rBV4	14803	35472	2.18%	0.126%
31	7.379	1018	1032	1043	rBV	303561	741534	45.61%	2.629%
32	7.659	1071	1078	1087	rVB	31247	61730	3.80%	0.219%
33	7.854	1103	1110	1111	rBV	25905	39241	2.41%	0.139%
34	7.885	1112	1115	1121	rVV2	31682	55352	3.40%	0.196%
35	8.141	1144	1157	1163	rBV3	28749	69684	4.29%	0.247%
36	8.440	1200	1206	1211	rBV4	16568	32901	2.02%	0.117%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062623\
 Data File : VX036337.D
 Acq On : 26 Jun 2023 18:27
 Operator : JC/MD
 Sample : 03291-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
 Title : SW846 8260

37	8.507	1211	1217	1224	rVB2	57480	100774	6.20%	0.357%
38	8.598	1224	1232	1235	rBV5	29356	70064	4.31%	0.248%
39	8.647	1235	1240	1247	rVB	773437	1186941	73.01%	4.208%
40	8.720	1247	1252	1257	rVB	214677	330020	20.30%	1.170%

41	8.842	1269	1272	1279	rVB2	24251	43705	2.69%	0.155%
42	8.976	1289	1294	1300	rVB3	28570	47421	2.92%	0.168%
43	9.104	1305	1315	1320	rVV	20311	41529	2.55%	0.147%
44	9.159	1320	1324	1336	rVB	39474	65644	4.04%	0.233%
45	9.433	1364	1369	1371	rBV2	21303	35910	2.21%	0.127%

46	9.531	1376	1385	1389	rBV	75270	138041	8.49%	0.489%
47	10.055	1461	1471	1476	rBV	745746	1065557	65.54%	3.777%
48	10.128	1476	1483	1484	rVV3	24135	44804	2.76%	0.159%
49	10.189	1488	1493	1498	rVV2	178127	285233	17.55%	1.011%
50	10.299	1505	1511	1518	rVB	1195075	1625721	100.00%	5.763%

51	10.640	1562	1567	1578	rVB	1057844	1311308	80.66%	4.649%
52	10.963	1614	1620	1628	rVB	194753	255523	15.72%	0.906%
53	11.079	1634	1639	1644	rBV	677449	818784	50.36%	2.903%
54	11.305	1667	1676	1683	rBV	251455	325730	20.04%	1.155%
55	11.378	1683	1688	1696	rVV	880371	1474529	90.70%	5.227%

56	11.451	1696	1700	1708	rVB	206058	253450	15.59%	0.898%
57	11.610	1721	1726	1735	rVB	713660	879272	54.09%	3.117%
58	11.750	1744	1749	1755	rVB	1267223	1473201	90.62%	5.223%
59	11.866	1762	1768	1770	rBV	26280	43578	2.68%	0.154%
60	11.890	1770	1772	1780	rVB	44729	56632	3.48%	0.201%

61	11.969	1780	1785	1788	rBV	103444	118935	7.32%	0.422%
62	12.018	1788	1793	1799	rVV	819101	1043349	64.18%	3.699%
63	12.085	1799	1804	1809	rVB	489315	577746	35.54%	2.048%
64	12.244	1823	1830	1832	rBV2	272403	360391	22.17%	1.278%
65	12.268	1832	1834	1837	rVV	198694	208567	12.83%	0.739%

66	12.311	1837	1841	1849	rVB4	181099	301365	18.54%	1.068%
67	12.402	1851	1856	1861	rBV2	37713	54162	3.33%	0.192%
68	12.463	1861	1866	1871	rVB	85089	104178	6.41%	0.369%
69	12.530	1871	1877	1879	rBV	179968	231136	14.22%	0.819%
70	12.555	1879	1881	1885	rVB	139907	142604	8.77%	0.506%

71	12.610	1885	1890	1894	rBV	540026	647390	39.82%	2.295%
72	12.646	1894	1896	1900	rVB	59742	60805	3.74%	0.216%
73	12.701	1900	1905	1912	rBV2	430164	634752	39.04%	2.250%
74	12.798	1917	1921	1924	rVV	31079	40093	2.47%	0.142%
75	12.847	1924	1929	1934	rVB2	127613	172151	10.59%	0.610%

76	12.920	1934	1941	1945	rBV	293978	348927	21.46%	1.237%
----	--------	------	------	------	-----	--------	--------	--------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062623\
 Data File : VX036337.D
 Acq On : 26 Jun 2023 18:27
 Operator : JC/MD
 Sample : 03291-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
 Title : SW846 8260

77	12.963	1945	1948	1953	rVB	120647	141111	8.68%	0.500%
78	13.042	1953	1961	1967	rBV4	40559	94886	5.84%	0.336%
79	13.134	1972	1976	1978	rBV	36954	42635	2.62%	0.151%
80	13.164	1978	1981	1986	rVB	193570	226090	13.91%	0.802%
81	13.256	1992	1996	1997	rBV2	31578	37174	2.29%	0.132%
82	13.292	1997	2002	2007	rVV2	481820	667514	41.06%	2.366%
83	13.341	2007	2010	2013	rVV4	30469	50205	3.09%	0.178%
84	13.365	2013	2014	2019	rVV	26337	28828	1.77%	0.102%
85	13.420	2019	2023	2030	rVB	78459	102552	6.31%	0.364%
86	13.506	2031	2037	2039	rBV2	49928	67395	4.15%	0.239%
87	13.542	2039	2043	2046	rVV	118808	159418	9.81%	0.565%
88	13.585	2046	2050	2055	rVV4	105787	191472	11.78%	0.679%
89	13.640	2055	2059	2060	rVV	78178	99699	6.13%	0.353%
90	13.664	2060	2063	2068	rVV2	133584	196936	12.11%	0.698%
91	13.707	2068	2070	2074	rVV2	23135	28318	1.74%	0.100%
92	13.774	2074	2081	2087	rVV	393960	502137	30.89%	1.780%
93	13.865	2092	2096	2100	rVV2	31989	48080	2.96%	0.170%
94	13.926	2100	2106	2110	rVV2	35487	50234	3.09%	0.178%
95	13.969	2110	2113	2117	rVB	37690	44245	2.72%	0.157%
96	14.073	2126	2130	2137	rBV	50499	63050	3.88%	0.224%
97	14.213	2148	2153	2162	rBV3	45686	86020	5.29%	0.305%
98	14.371	2175	2179	2183	rVB	35191	42220	2.60%	0.150%
99	14.634	2219	2222	2233	rVB	86749	115984	7.13%	0.411%
100	14.780	2241	2246	2252	rBV	68266	90905	5.59%	0.322%




Sum of corrected areas: 28208133

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062623\
Data File : VX036337.D
Acq On : 26 Jun 2023 18:27
Operator : JC/MD
Sample : 03291-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

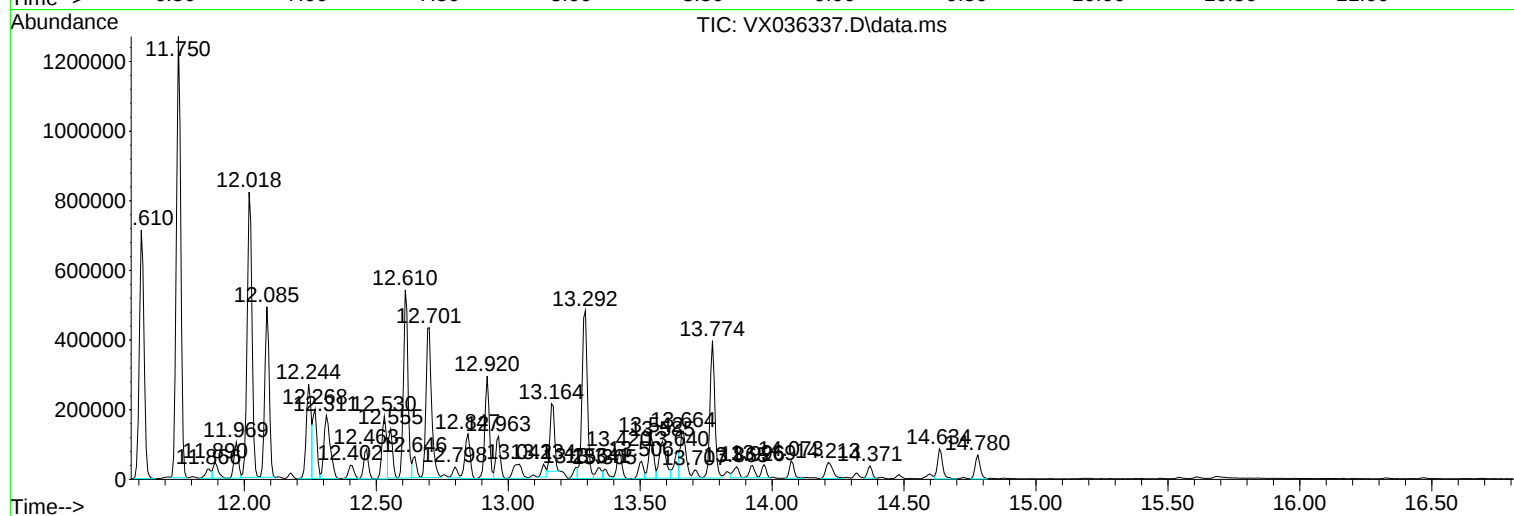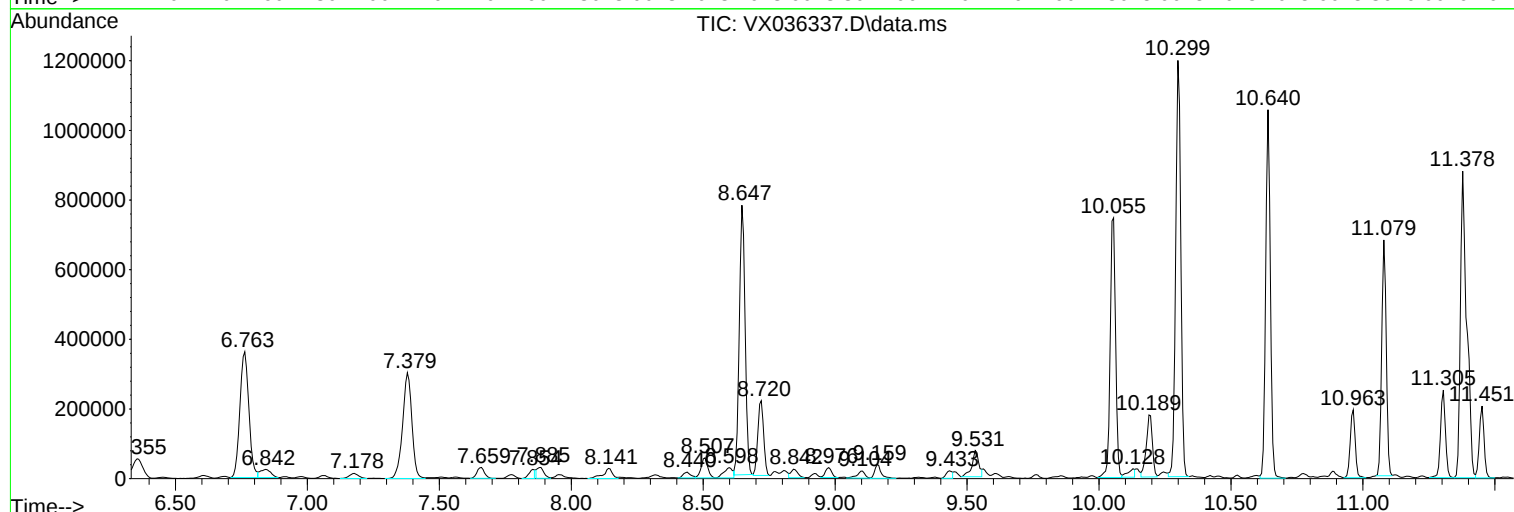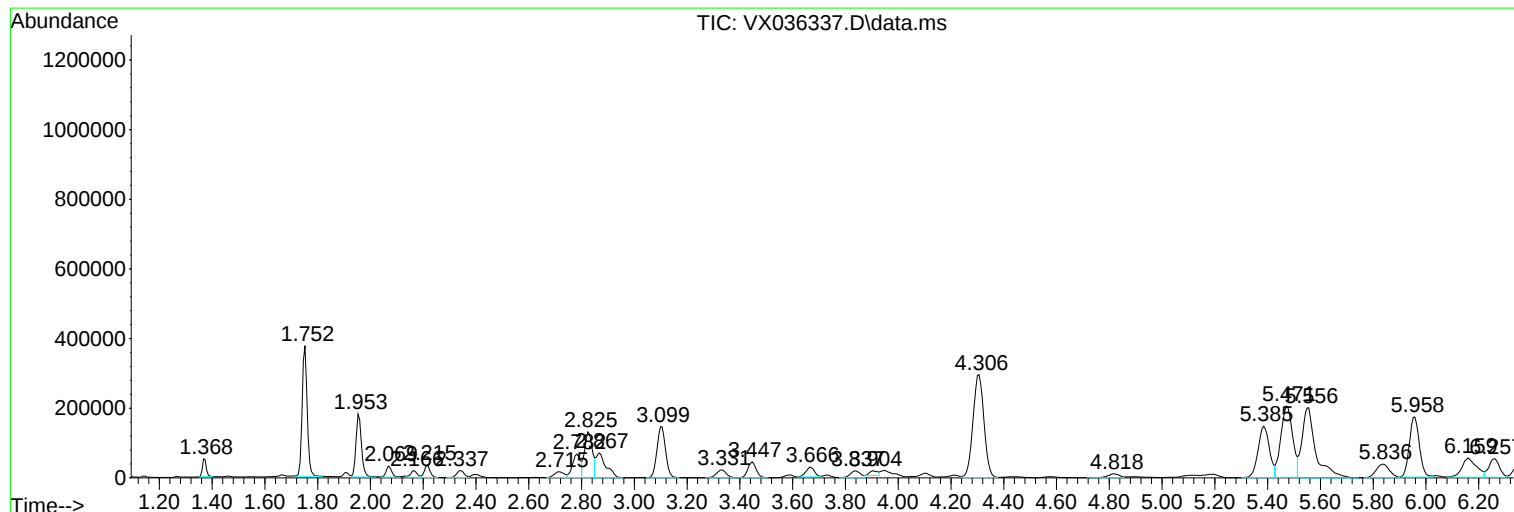

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062623\
Data File : VX036337.D
Acq On : 26 Jun 2023 18:27
Operator : JC/MD
Sample : 03291-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062623\
Data File : VX036337.D
Acq On : 26 Jun 2023 18:27
Operator : JC/MD
Sample : 03291-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------