

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062624\
 Data File : VX042046.D
 Acq On : 26 Jun 2024 12:26
 Operator : JC/MD
 Sample : VX0626MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jun 27 03:42:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 21 23:51:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	138769	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	212280	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	207361	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	106649	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	67235	42.017	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	84.040%
35) Dibromofluoromethane	5.385	113	66636	44.240	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	88.480%
50) Toluene-d8	8.647	98	245868	46.465	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	92.920%
62) 4-Bromofluorobenzene	11.079	95	94895	48.650	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	97.300%
Target Compounds						
						Qvalue
3) Chloromethane	1.300	50	463	0.349	ug/l	# 86
5) Bromomethane	1.599	94	616	0.938	ug/l	# 65
6) Chloroethane	1.666	64	230	Below Cal	#	54
10) Methyl Iodide	2.447	142	618	0.414	ug/l	# 68
11) Tert butyl alcohol	2.940	59	4328	14.251	ug/l	# 78
12) 1,1-Dichloroethene	2.306	96	267	0.223	ug/l	# 68
13) Acrolein	2.239	56	559	1.642	ug/l	90
15) Acrylonitrile	3.081	53	765	0.964	ug/l	97
16) Acetone	2.392	43	1554	2.212	ug/l	# 89
17) Carbon Disulfide	2.501	76	2341	0.959	ug/l	# 81
18) Methyl Acetate	2.715	43	522	0.272	ug/l	91
20) Methylene Chloride	2.788	84	1334	0.867	ug/l	# 86
21) trans-1,2-Dichloroethene	3.087	96	394	0.324	ug/l	83
23) Vinyl Acetate	3.745	43	1032	0.301	ug/l	# 73
29) Tetrahydrofuran	5.056	42	345	0.489	ug/l	# 63
36) 1,1-Dichloropropene	5.690	75	502	0.314	ug/l	# 42
38) Carbon Tetrachloride	5.550	117	11676	6.607	ug/l	# 15
51) 4-Methyl-2-Pentanone	8.580	43	733	0.333	ug/l	# 77
53) t-1,3-Dichloropropene	8.994	75	262	1.032	ug/l	# 43
59) 2-Hexanone	9.464	43	838	0.497	ug/l	# 42
64) Tetrachloroethene	9.281	164	347	0.230	ug/l	# 63
68) m/p-Xylenes	10.305	106	766	0.281	ug/l	89
71) Bromoform	10.805	173	79	0.931	ug/l	# 29
76) 1,2,3-Trichloropropane	11.079	75	43348	22.389	ug/l	# 39
77) Bromobenzene	11.201	156	393	0.203	ug/l	87
81) trans-1,4-Dichloro-2-b...	11.079	75	43348	63.583	ug/l	# 5
82) 4-Chlorotoluene	11.457	91	1195	0.238	ug/l	92
87) 1,3-Dichlorobenzene	11.975	146	847	0.250	ug/l	89
88) 1,4-Dichlorobenzene	11.975	146	847	0.243	ug/l	88
89) n-Butylbenzene	12.335	91	961	0.213	ug/l	94
91) 1,2-Dichlorobenzene	12.347	146	727	0.209	ug/l	97
93) 1,2,4-Trichlorobenzene	13.591	180	1356	0.596	ug/l	95
94) Hexachlorobutadiene	13.725	225	267	0.232	ug/l	95
95) Naphthalene	13.780	128	5938	1.513	ug/l	98
96) 1,2,3-Trichlorobenzene	13.963	180	1513	0.630	ug/l	95

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062624\
Data File : VX042046.D
Acq On : 26 Jun 2024 12:26
Operator : JC/MD
Sample : VX0626MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jun 27 03:42:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 21 23:51:58 2024
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062624\
Data File : VX042046.D
Acq On : 26 Jun 2024 12:26
Operator : JC/MD
Sample : VX0626MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jun 27 03:42:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 21 23:51:58 2024
Response via : Initial Calibration

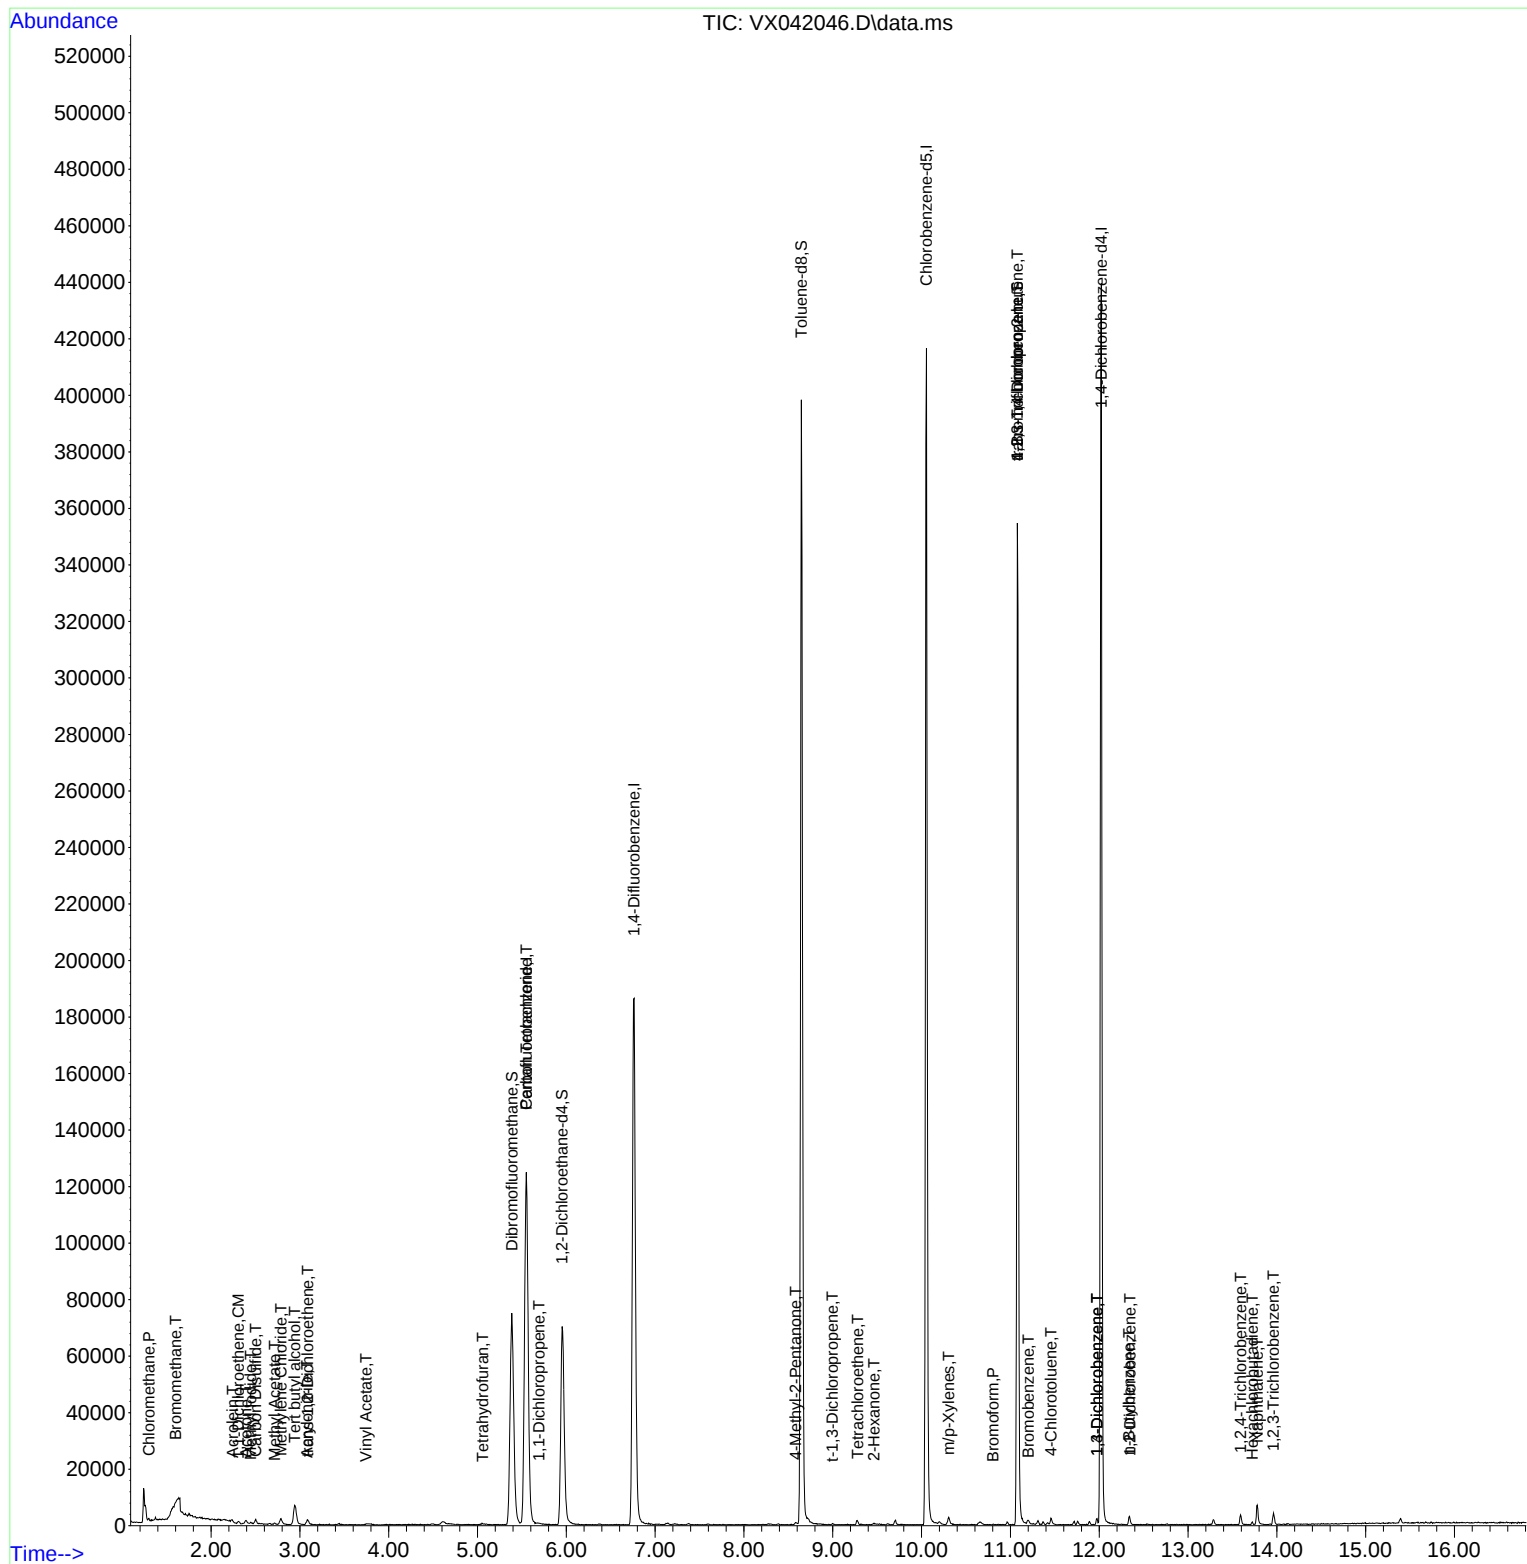





#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26

Instrument :
MSVOA_X
ClientSampleId :



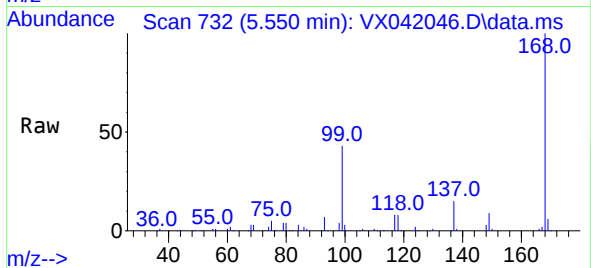



Tgt Ion:168 Resp: 138769
Ion Ratio Lower Upper
168 100
99 43.4 56.6 85.0#

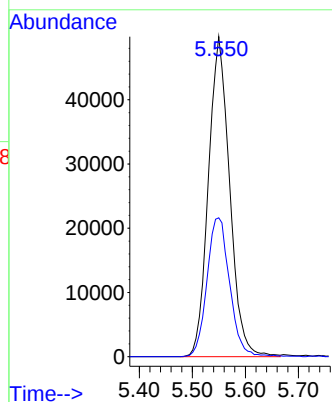

#3
Chloromethane
Concen: 0.349 ug/l
RT: 1.300 min Scan# 35
Delta R.T. -0.006 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26


Tgt Ion: 50 Resp: 463
Ion Ratio Lower Upper
50 100
52 23.9 25.5 38.3#

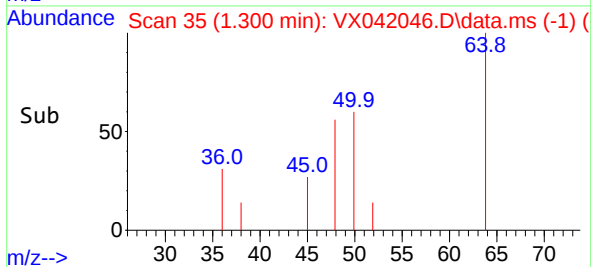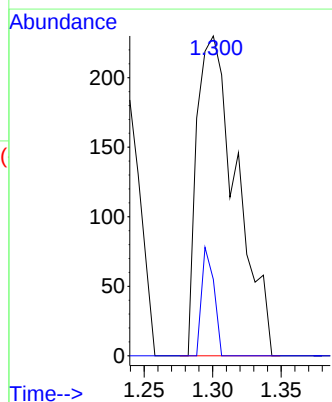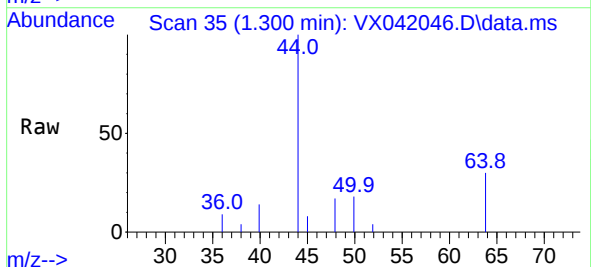



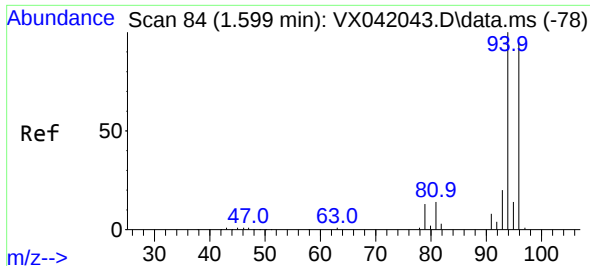


#5
Bromomethane
Concen: 0.938 ug/l
RT: 1.599 min Scan# 84
Delta R.T. 0.000 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26

Instrument :
MSVOA_X
ClientSampleId :



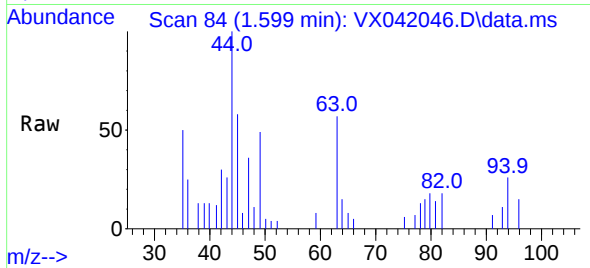



Tgt Ion: 94 Resp: 616
Ion Ratio Lower Upper
94 100
96 59.4 74.6 111.8#

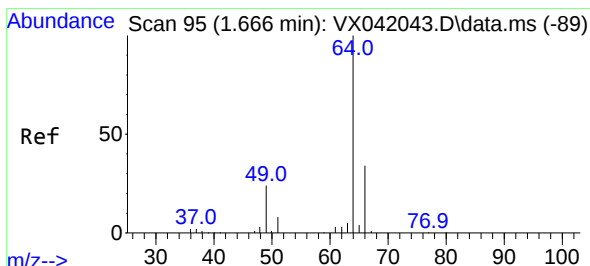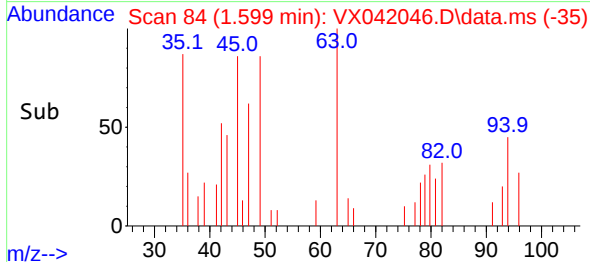

#6
Chloroethane
Concen: Below Cal
RT: 1.666 min Scan# 95
Delta R.T. 0.006 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26


Tgt Ion: 64 Resp: 230
Ion Ratio Lower Upper
64 100
66 6.2 25.1 37.7#

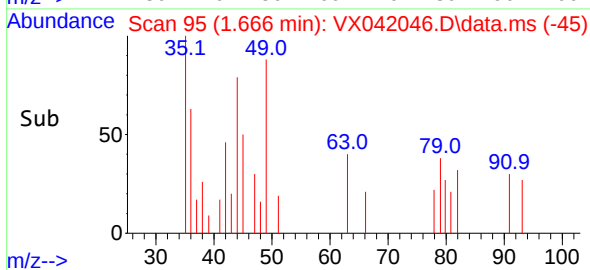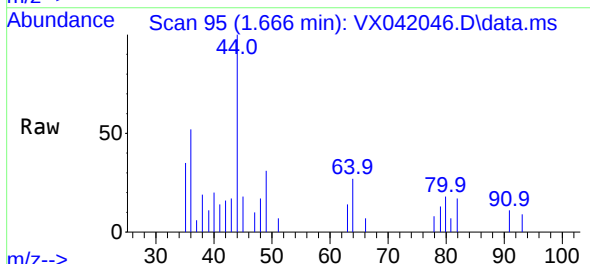



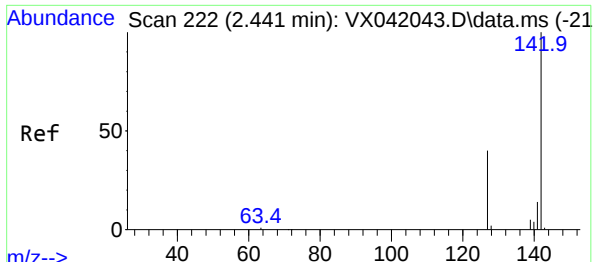


#10
Methyl Iodide
Concen: 0.414 ug/l
RT: 2.447 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26

Instrument :
MSVOA_X
ClientSampleId :



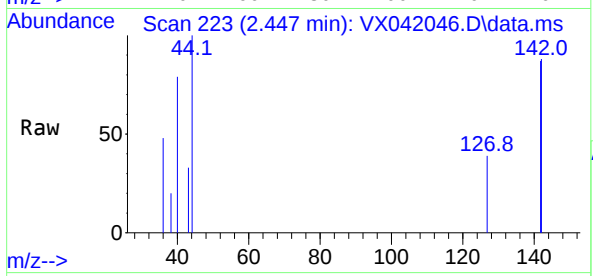



Tgt Ion:142 Resp: 618
Ion Ratio Lower Upper
142 100
127 30.3 41.6 62.4#
141 0.0 11.6 17.4#

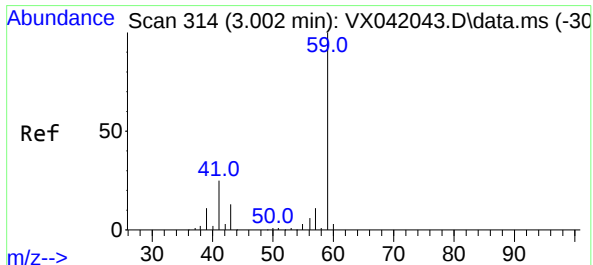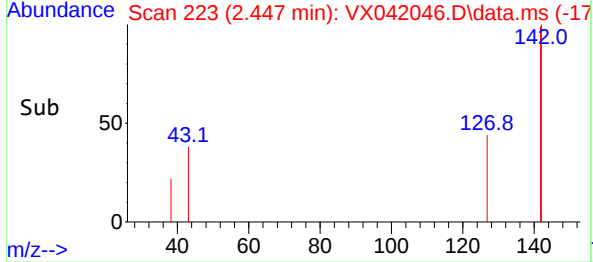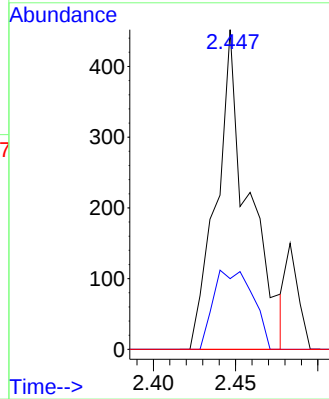

#11
Tert butyl alcohol
Concen: 14.251 ug/l
RT: 2.940 min Scan# 304
Delta R.T. -0.067 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26


Tgt Ion: 59 Resp: 4328
Ion Ratio Lower Upper
59 100
57 0.0 6.0 9.0#

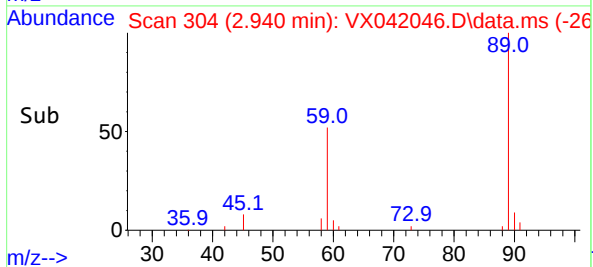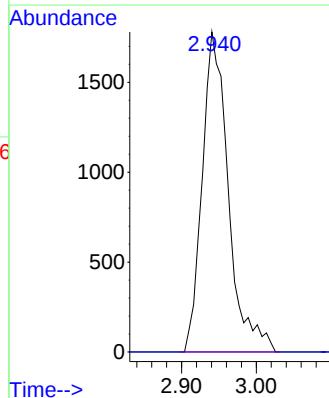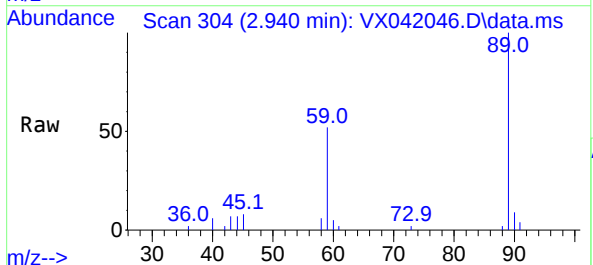






#12
1,1-Dichloroethene
Concen: 0.223 ug/l
RT: 2.306 min Scan# 20
Delta R.T. 0.000 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 96 Resp: 267
Ion Ratio Lower Upper
96 100
61 126.4 144.6 216.8#
98 52.7 50.4 75.6



#13
Acrolein
Concen: 1.642 ug/l
RT: 2.239 min Scan# 189
Delta R.T. 0.000 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26

Tgt Ion: 56 Resp: 559
Ion Ratio Lower Upper
56 100
55 63.0 57.1 85.7

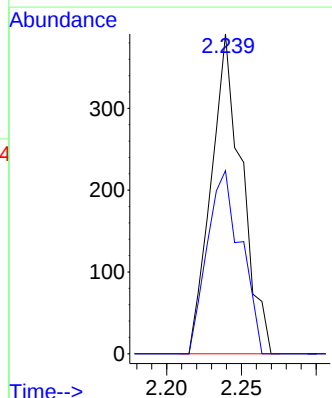



#15

Acrylonitrile

Concen: 0.964 ug/l

RT: 3.081 min Scan# 31

Delta R.T. 0.006 min

Lab File: VX042046.D

Acq: 26 Jun 2024 12:26

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 53 Resp: 765

Ion Ratio Lower Upper

53 100

52 83.8 66.0 99.0

51 33.2 29.8 44.6

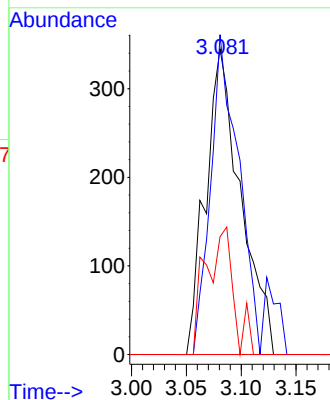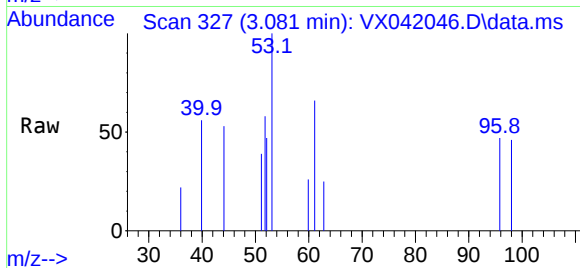

#16

Acetone

Concen: 2.212 ug/l

RT: 2.392 min Scan# 214

Delta R.T. -0.006 min

Lab File: VX042046.D




Acq: 26 Jun 2024 12:26


Tgt Ion: 43 Resp: 1554

Ion Ratio Lower Upper

43 100


58 33.0 21.9 32.9#

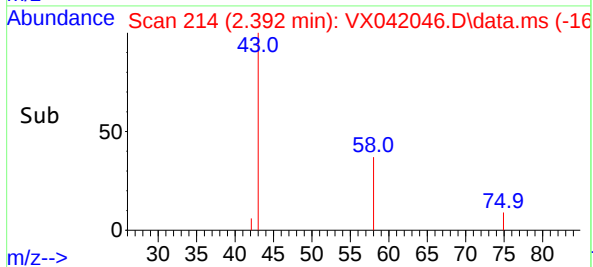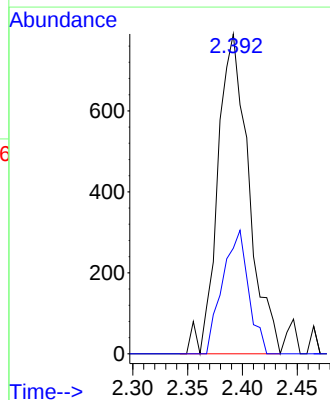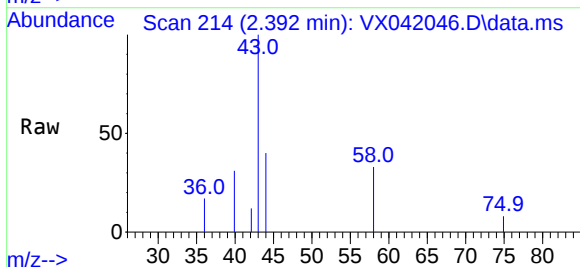






#17
Carbon Disulfide
Concen: 0.959 ug/l
RT: 2.501 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 76 Resp: 2341
Ion Ratio Lower Upper
76 100
78 15.8 7.0 10.6#

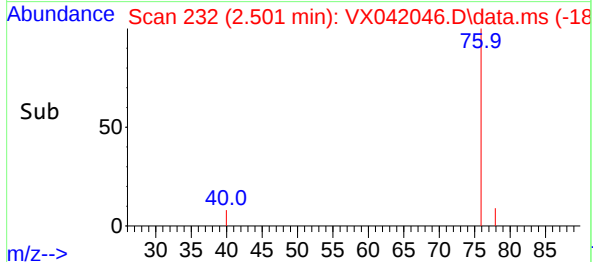

#18
Methyl Acetate
Concen: 0.272 ug/l
RT: 2.715 min Scan# 267
Delta R.T. 0.006 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26


Tgt Ion: 43 Resp: 522
Ion Ratio Lower Upper
43 100
74 18.2 17.8 26.8

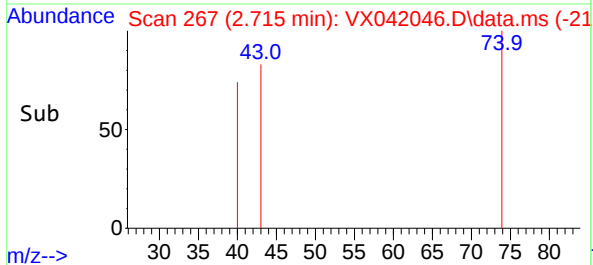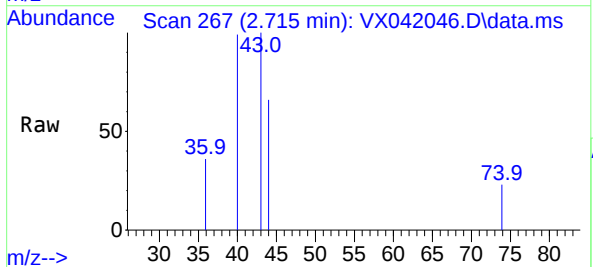






#20
Methylene Chloride
Concen: 0.867 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26

Instrument :
MSVOA_X
ClientSampleId :



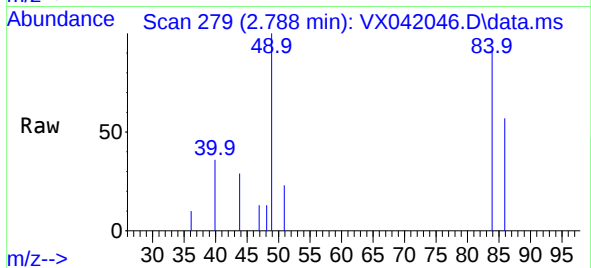



Tgt Ion: 84 Resp: 1334
Ion Ratio Lower Upper
84 100
49 110.3 103.6 155.4
51 25.4 33.8 50.6#
86 62.7 49.4 74.0

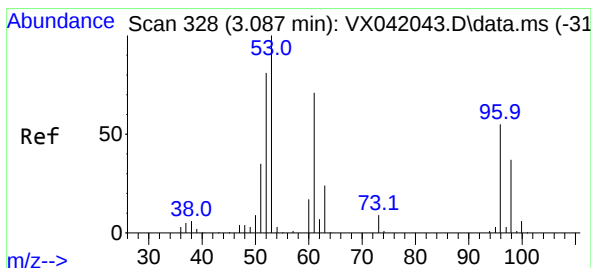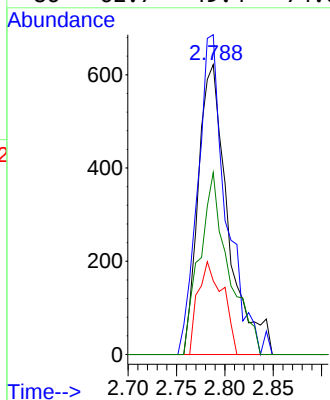

#21
trans-1,2-Dichloroethene
Concen: 0.324 ug/l
RT: 3.087 min Scan# 328
Delta R.T. 0.000 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26

Tgt Ion: 96 Resp: 394
Ion Ratio Lower Upper
96 100
61 126.9 119.2 178.8
98 49.3 48.7 73.1


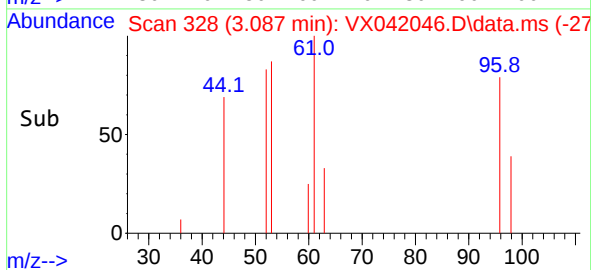
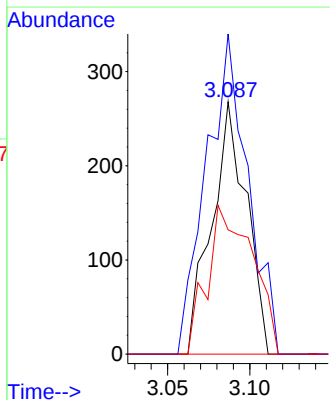
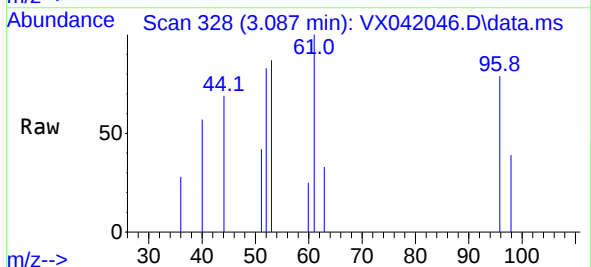




#23
Vinyl Acetate
Concen: 0.301 ug/l
RT: 3.745 min Scan# 41
Delta R.T. 0.018 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 1032
Ion Ratio Lower Upper
43 100
86 0.0 7.8 11.8#



#29
Tetrahydrofuran
Concen: 0.489 ug/l
RT: 5.056 min Scan# 651
Delta R.T. 0.037 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26

Tgt Ion: 42 Resp: 345
Ion Ratio Lower Upper
42 100
72 29.0 34.2 51.4#
71 7.0 32.2 48.2#


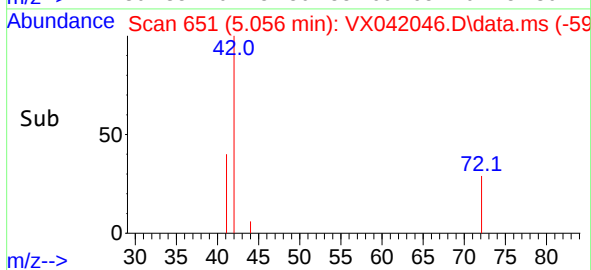






#33
1,2-Dichloroethane-d4
Concen: 42.017 ug/l
RT: 5.952 min Scan# 799
Delta R.T. -0.006 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 65 Resp: 67235
Ion Ratio Lower Upper
65 100
67 54.2 0.0 100.2

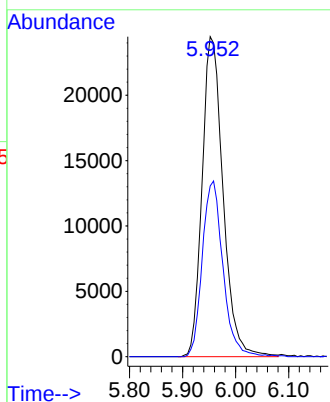

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. 0.000 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26


Tgt Ion: 114 Resp: 212280
Ion Ratio Lower Upper
114 100
63 17.7 0.0 45.0
88 14.9 0.0 36.6

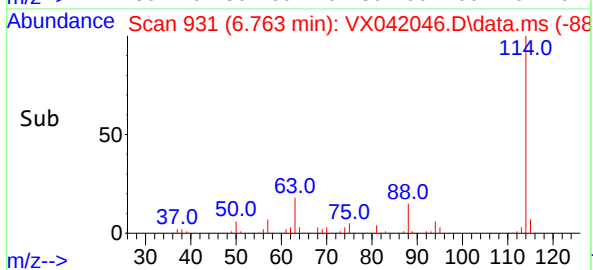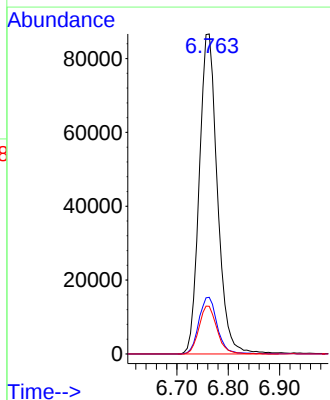






#35
 Dibromofluoromethane
 Concen: 44.240 ug/l
 RT: 5.385 min Scan# 705
 Delta R.T. -0.006 min
 Lab File: VX042046.D
 Acq: 26 Jun 2024 12:26

Instrument :
 MSVOA_X
 ClientSampleId :







Tgt Ion:113 Resp: 66636
 Ion Ratio Lower Upper
 113 100
 111 100.3 82.9 124.3
 192 25.4 13.3 19.9#



#36
 1,1-Dichloropropene
 Concen: 0.314 ug/l
 RT: 5.690 min Scan# 755
 Delta R.T. 0.000 min
 Lab File: VX042046.D
 Acq: 26 Jun 2024 12:26


Tgt Ion: 75 Resp: 502
 Ion Ratio Lower Upper
 75 100
 110 0.0 17.0 50.9#
 77 0.0 24.7 37.1#

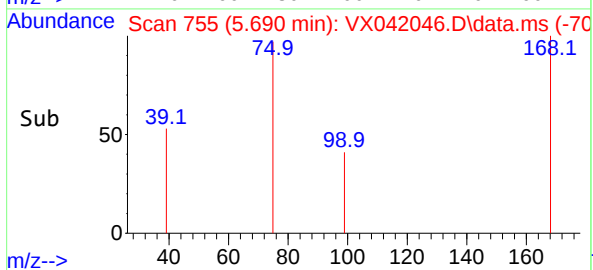



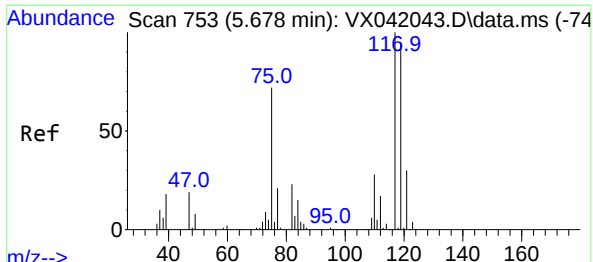


#38
Carbon Tetrachloride
Concen: 6.607 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26

Instrument :
MSVOA_X
ClientSampleId :



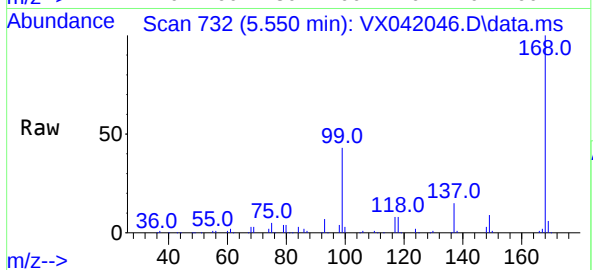



Tgt Ion:117 Resp: 11676
Ion Ratio Lower Upper
117 100
119 4.8 78.2 117.2#
121 0.0 24.4 36.6#



#50
Toluene-d8
Concen: 46.465 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26

Tgt Ion: 98 Resp: 245868
Ion Ratio Lower Upper
98 100
100 66.5 53.1 79.7


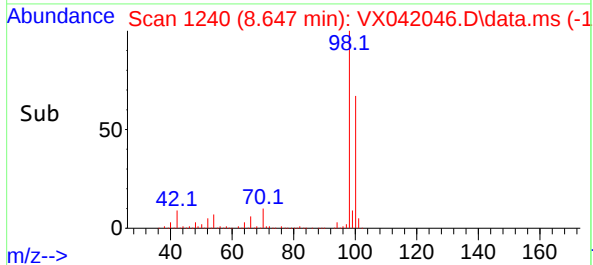

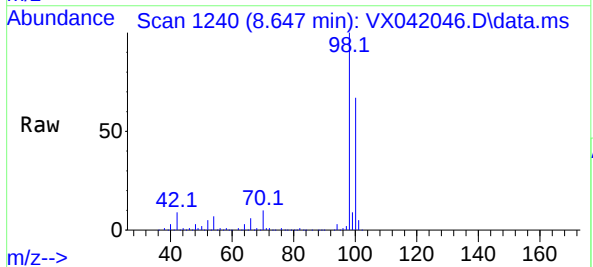




#51
4-Methyl-2-Pentanone
Concen: 0.333 ug/l
RT: 8.580 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 733
Ion Ratio Lower Upper
43 100
58 24.1 30.4 45.6#

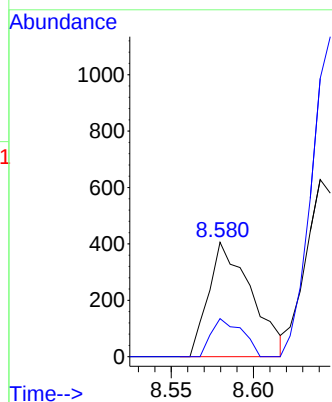

#53
t-1,3-Dichloropropene
Concen: 1.032 ug/l
RT: 8.994 min Scan# 1297
Delta R.T. 0.012 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26

Tgt Ion: 75 Resp: 262
Ion Ratio Lower Upper
75 100
77 0.0 25.7 38.5#

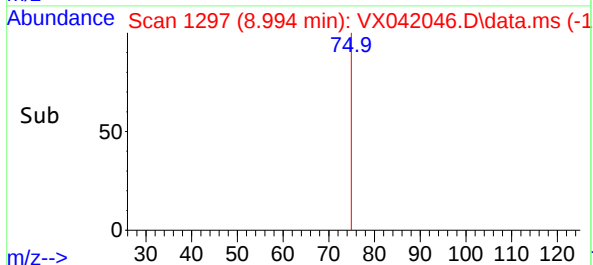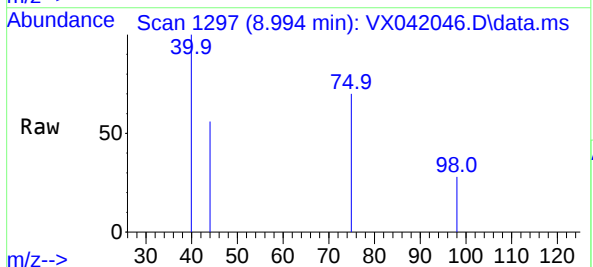



#59

2-Hexanone

Concen: 0.497 ug/l

RT: 9.464 min Scan# 11

Delta R.T. 0.030 min

Lab File: VX042046.D

Acq: 26 Jun 2024 12:26

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 838

Ion Ratio Lower Upper

43 100

58 11.3 26.2 78.5#



#62

4-Bromofluorobenzene

Concen: 48.650 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX042046.D

Acq: 26 Jun 2024 12:26




Tgt Ion: 95 Resp: 94895


Ion Ratio Lower Upper

95 100

174 98.4 0.0 135.6


176 95.4 0.0 131.0

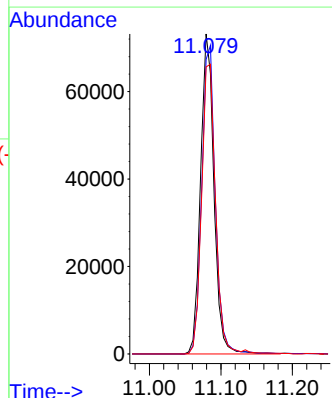






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26

Instrument :
MSVOA_X
ClientSampleId :



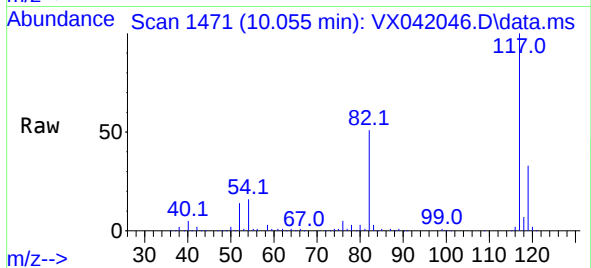



Tgt Ion:117 Resp: 207361
Ion Ratio Lower Upper
117 100
82 50.6 46.2 69.4
119 32.8 25.5 38.3

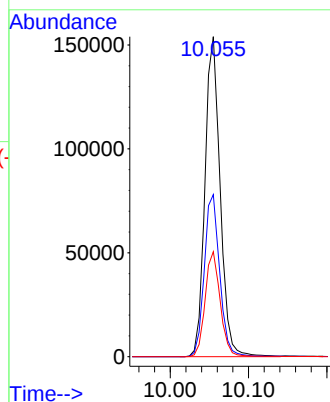

#64
Tetrachloroethene
Concen: 0.230 ug/l
RT: 9.281 min Scan# 1344
Delta R.T. 0.006 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26

Tgt Ion:164 Resp: 347
Ion Ratio Lower Upper
164 100
166 87.0 102.7 154.1#
129 57.1 80.4 120.6#
131 64.5 76.5 114.7#


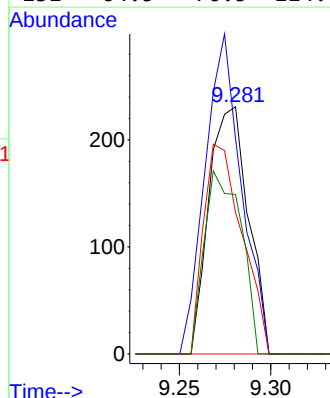
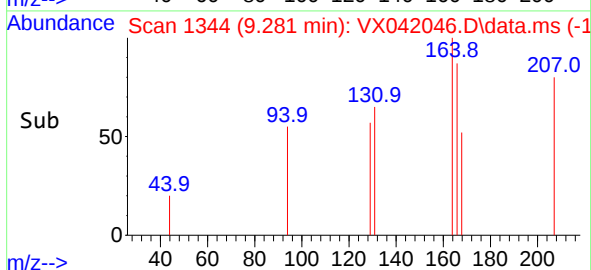
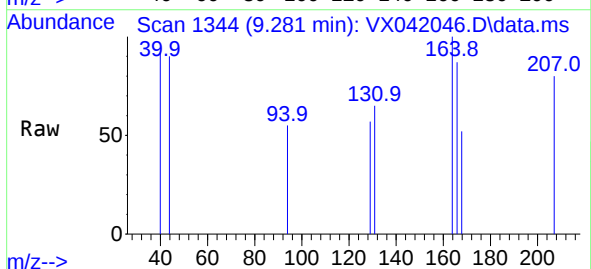




#68
m/p-Xylenes
Concen: 0.281 ug/l
RT: 10.305 min Scan# 1511
Delta R.T. 0.006 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 766
Ion Ratio Lower Upper
106 100
91 223.2 165.5 248.3



#71
Bromoform
Concen: 0.931 ug/l
RT: 10.805 min Scan# 1594
Delta R.T. 0.006 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26


Tgt Ion:173 Resp: 79
Ion Ratio Lower Upper
173 100
175 0.0 24.1 72.4#
254 0.0 0.0 0.0

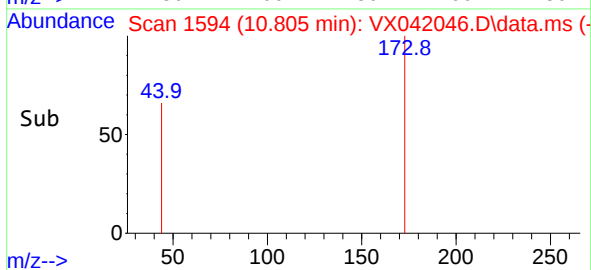






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26

Instrument :
MSVOA_X
ClientSampleId :



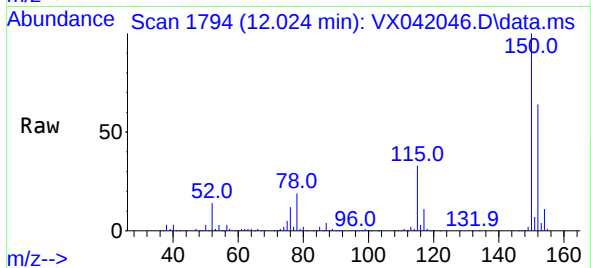



Tgt Ion:152 Resp: 106649
Ion Ratio Lower Upper
152 100
115 53.5 43.3 129.9
150 158.3 0.0 345.0

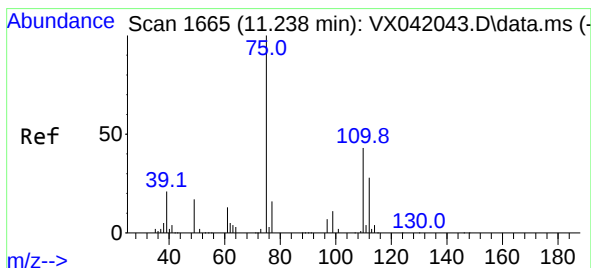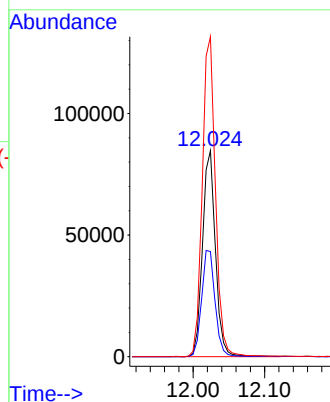

#76
1,2,3-Trichloropropane
Concen: 22.389 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26


Tgt Ion: 75 Resp: 43348
Ion Ratio Lower Upper
75 100
77 1.2 19.1 57.5#

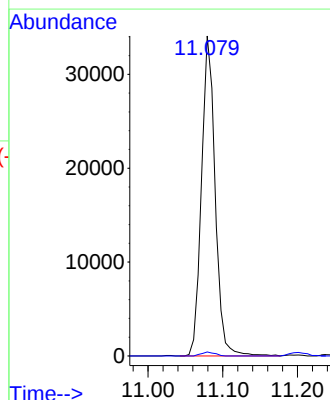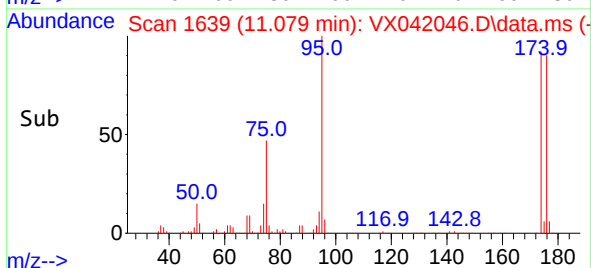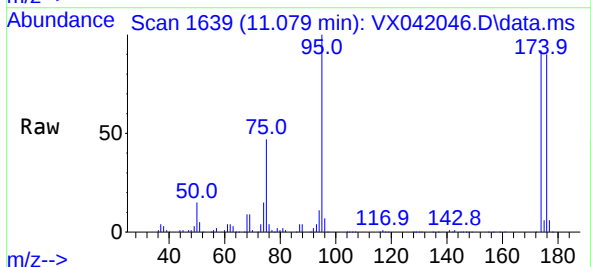






#77
Bromobenzene
Concen: 0.203 ug/l
RT: 11.201 min Scan# 1659
Delta R.T. 0.000 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26

Instrument :
MSVOA_X
ClientSampleId :



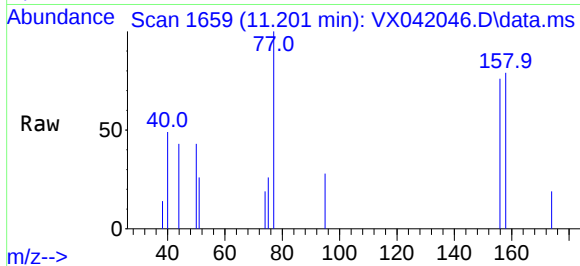



Tgt Ion:156 Resp: 393
Ion Ratio Lower Upper
156 100
77 155.7 88.4 265.3
158 86.0 48.0 144.0



#81
trans-1,4-Dichloro-2-butene
Concen: 63.583 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26

Tgt Ion: 75 Resp: 43348
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#


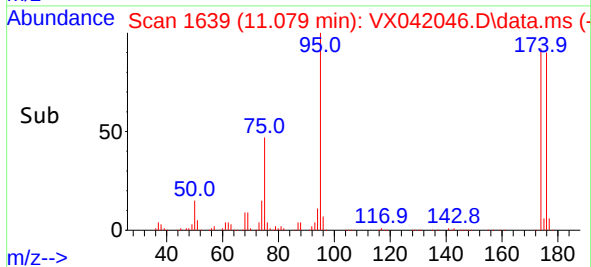

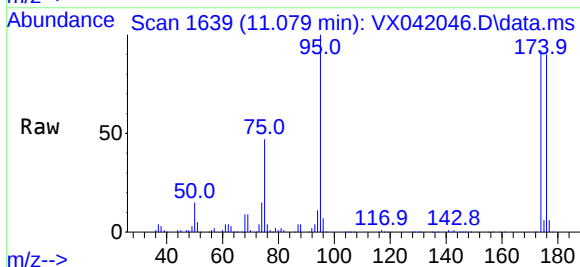




#82
4-Chlorotoluene
Concen: 0.238 ug/l
RT: 11.457 min Scan# 1195
Delta R.T. 0.000 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 1195
Ion Ratio Lower Upper
91 100
126 32.9 14.2 42.6

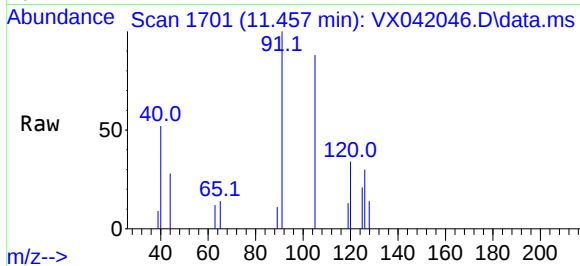

#87
1,3-Dichlorobenzene
Concen: 0.250 ug/l
RT: 11.975 min Scan# 1786
Delta R.T. 0.006 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26


Tgt Ion: 146 Resp: 847
Ion Ratio Lower Upper
146 100
111 44.2 22.1 66.1
148 78.3 31.8 95.3

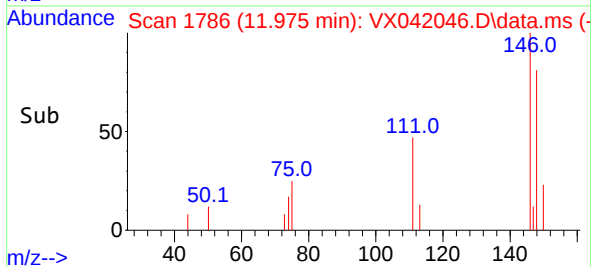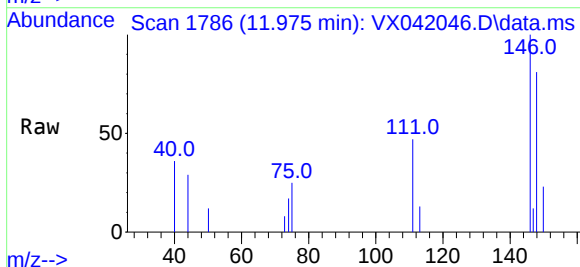






#88
1,4-Dichlorobenzene
Concen: 0.243 ug/l
RT: 11.975 min Scan# 11
Delta R.T. -0.067 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26

Instrument :
MSVOA_X
ClientSampleId :



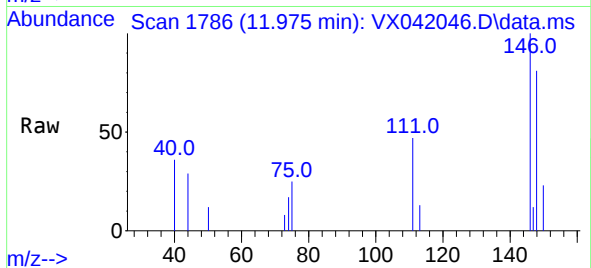



Tgt Ion:146 Resp: 847
Ion Ratio Lower Upper
146 100
111 44.2 21.3 63.7
148 78.3 31.8 95.4

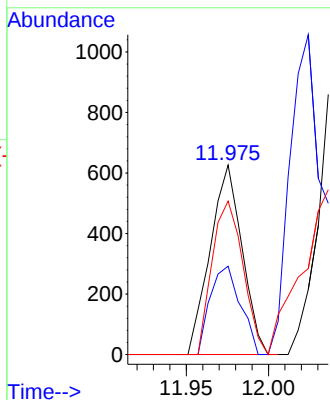

#89
n-Butylbenzene
Concen: 0.213 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26

Tgt Ion: 91 Resp: 961
Ion Ratio Lower Upper
91 100
92 49.6 27.4 82.0
134 26.3 12.6 37.8


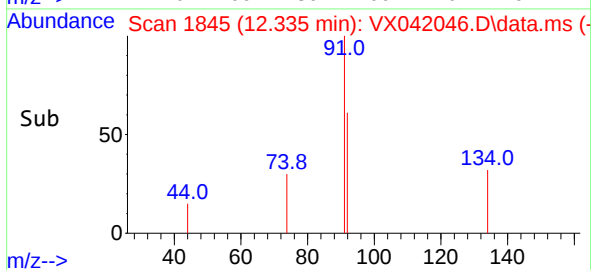
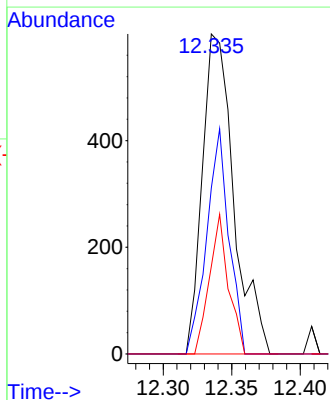





#91
1,2-Dichlorobenzene
Concen: 0.209 ug/l
RT: 12.347 min Scan# 1847
Delta R.T. 0.012 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:146 Resp: 727
Ion Ratio Lower Upper
146 100
111 42.0 22.4 67.0
148 65.1 31.6 95.0

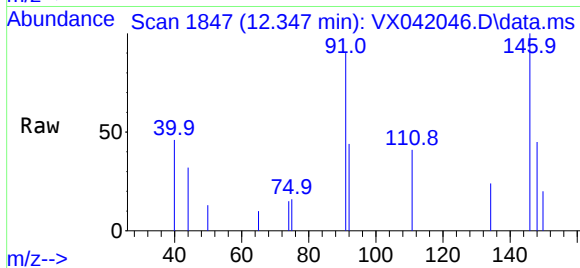

#93
1,2,4-Trichlorobenzene
Concen: 0.596 ug/l
RT: 13.591 min Scan# 2051
Delta R.T. 0.006 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26


Tgt Ion:180 Resp: 1356
Ion Ratio Lower Upper
180 100
182 98.3 48.3 144.8
145 28.2 18.0 54.0

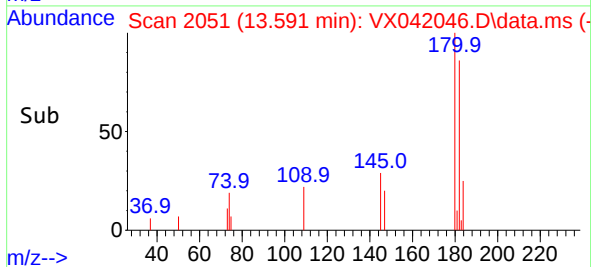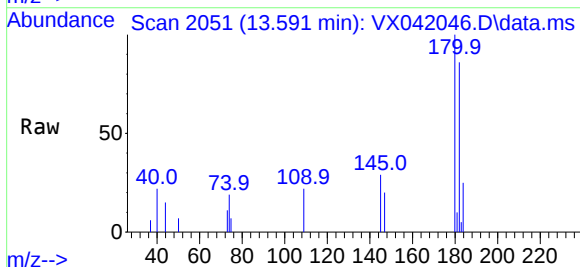






#94
Hexachlorobutadiene
Concen: 0.232 ug/l
RT: 13.725 min Scan# 2073
Delta R.T. 0.000 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26


Instrument :
MSVOA_X
ClientSampleId :

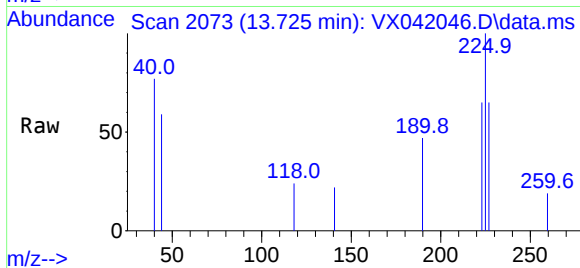



Tgt Ion:225 Resp: 267
Ion Ratio Lower Upper
225 100
223 57.7 31.1 93.2
227 62.2 32.5 97.5

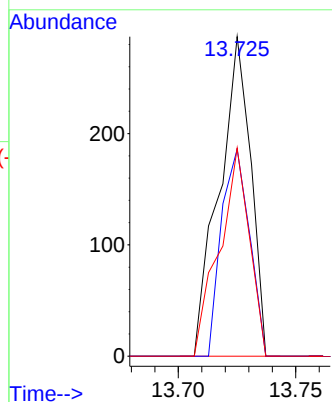


#95
Naphthalene
Concen: 1.513 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX042046.D
Acq: 26 Jun 2024 12:26

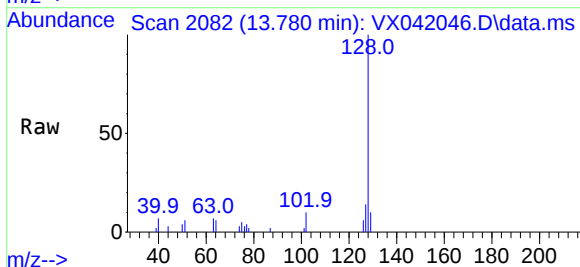

Tgt Ion:128 Resp: 5938
Ion Ratio Lower Upper
128 100
127 13.5 10.3 15.5
129 10.1 8.8 13.2

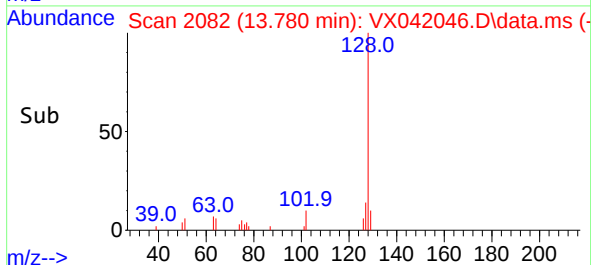



#96

1,2,3-Trichlorobenzene

Concen: 0.630 ug/l

RT: 13.963 min Scan# 21

Delta R.T. 0.000 min


Lab File: VX042046.D

Acq: 26 Jun 2024 12:26

Instrument :

MSVOA_X

ClientSampleId :

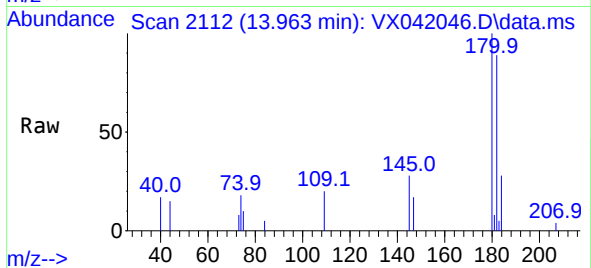

Tgt Ion:180 Resp: 1513

Ion Ratio Lower Upper

180 100

182 100.2 46.9 140.6

145 34.6 17.8 53.5

