

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062624\
Data File : VX042047.D
Acq On : 26 Jun 2024 12:49
Operator : JC/MD
Sample : VX0626WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0626WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M

Title : SW846 8260

Signal : TIC: VX042047.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	39	rBV2	13114	21104	2.96%	0.541%
2	1.605	78	85	86	rVV6	4800	10876	1.53%	0.279%
3	2.947	297	305	312	rBV	6962	16158	2.27%	0.414%
4	5.385	693	705	721	rBV	87888	252943	35.48%	6.480%
5	5.550	722	732	748	rVB	141913	404256	56.71%	10.356%
6	5.952	789	798	815	rBV	80737	220482	30.93%	5.648%
7	6.763	918	931	948	rBV	216713	523323	73.41%	13.406%
8	8.647	1233	1240	1256	rBV	446344	712902	100.00%	18.262%
9	10.055	1465	1471	1487	rBV	454540	638689	89.59%	16.361%
10	11.079	1634	1639	1656	rBV	381310	505578	70.92%	12.951%
11	12.024	1788	1794	1805	rBV	453703	597394	83.80%	15.303%




Sum of corrected areas: 3903705

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062624\
Data File : VX042047.D
Acq On : 26 Jun 2024 12:49
Operator : JC/MD
Sample : VX0626WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0626WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

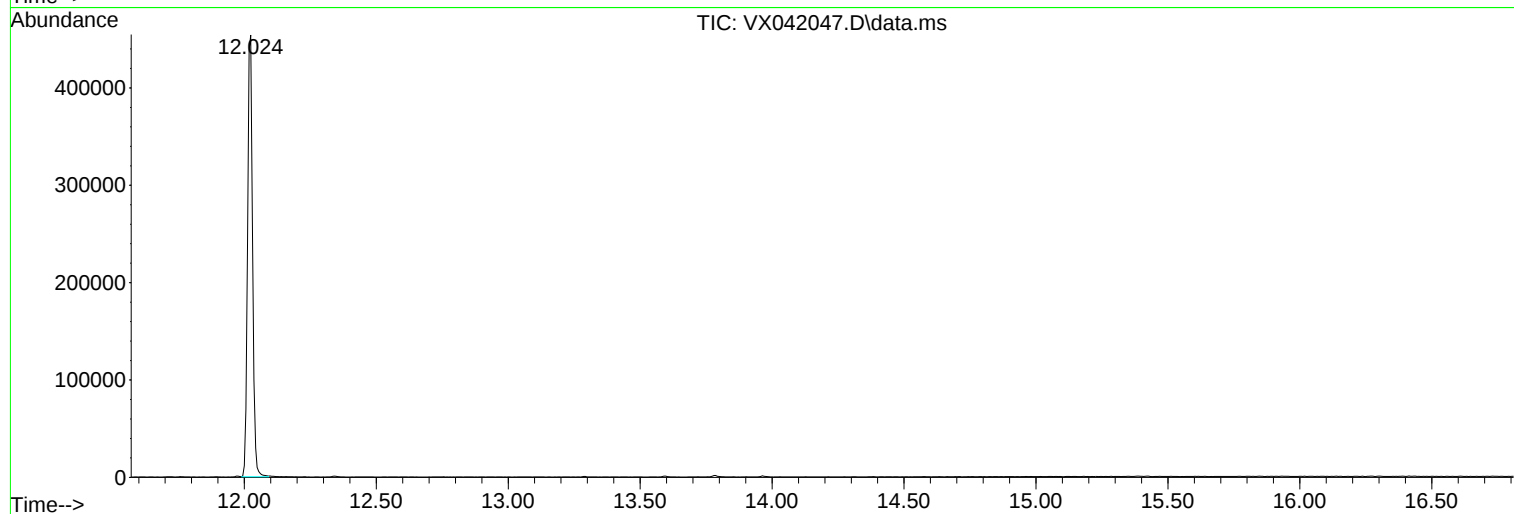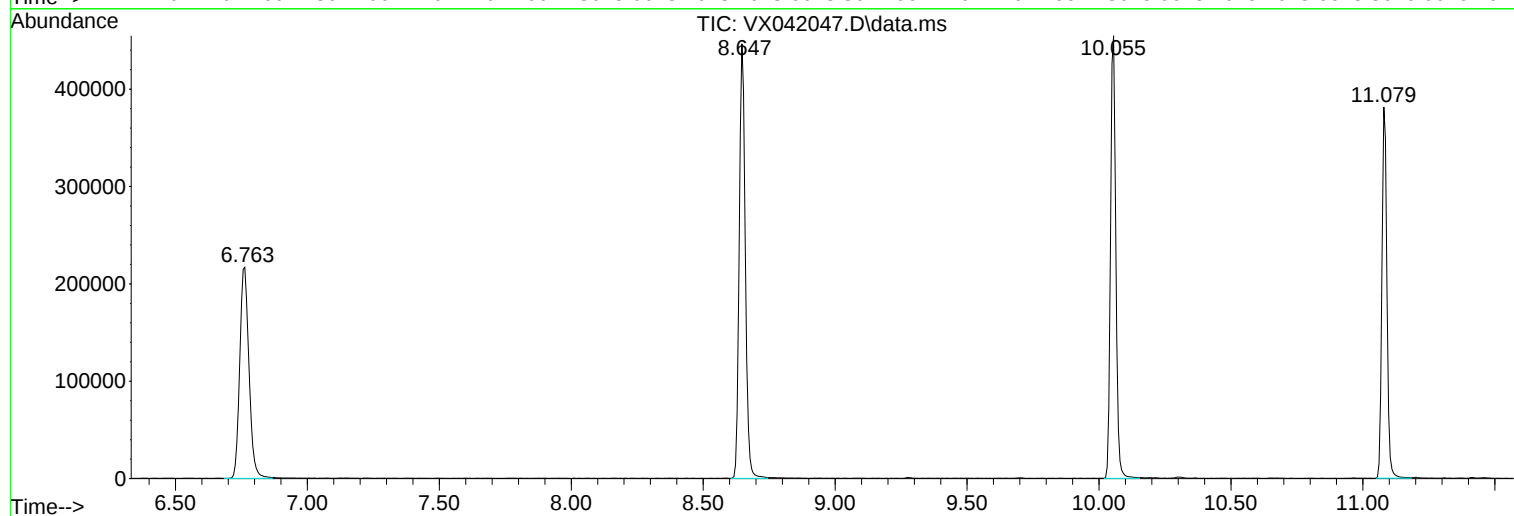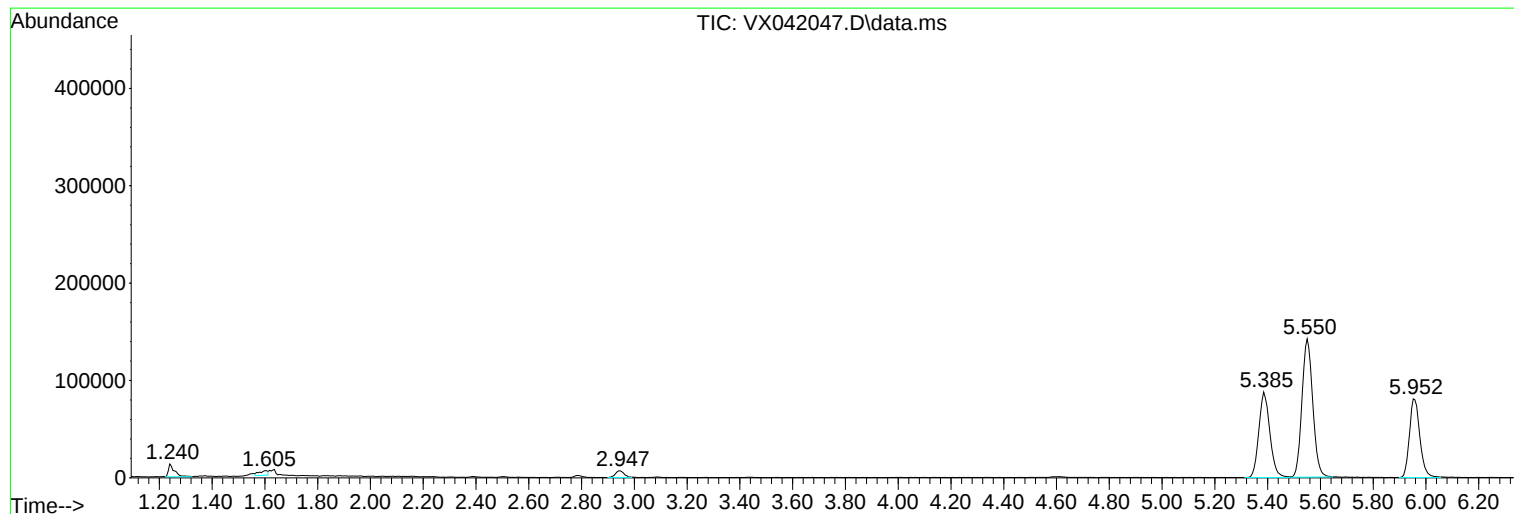

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062624\
Data File : VX042047.D
Acq On : 26 Jun 2024 12:49
Operator : JC/MD
Sample : VX0626WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0626WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062624\
Data File : VX042047.D
Acq On : 26 Jun 2024 12:49
Operator : JC/MD
Sample : VX0626WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0626WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc