


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062624\
Data File : VX042044.D
Acq On : 26 Jun 2024 08:18
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Title : SW846 8260
Last Update : Fri Jun 21 23:51:58 2024

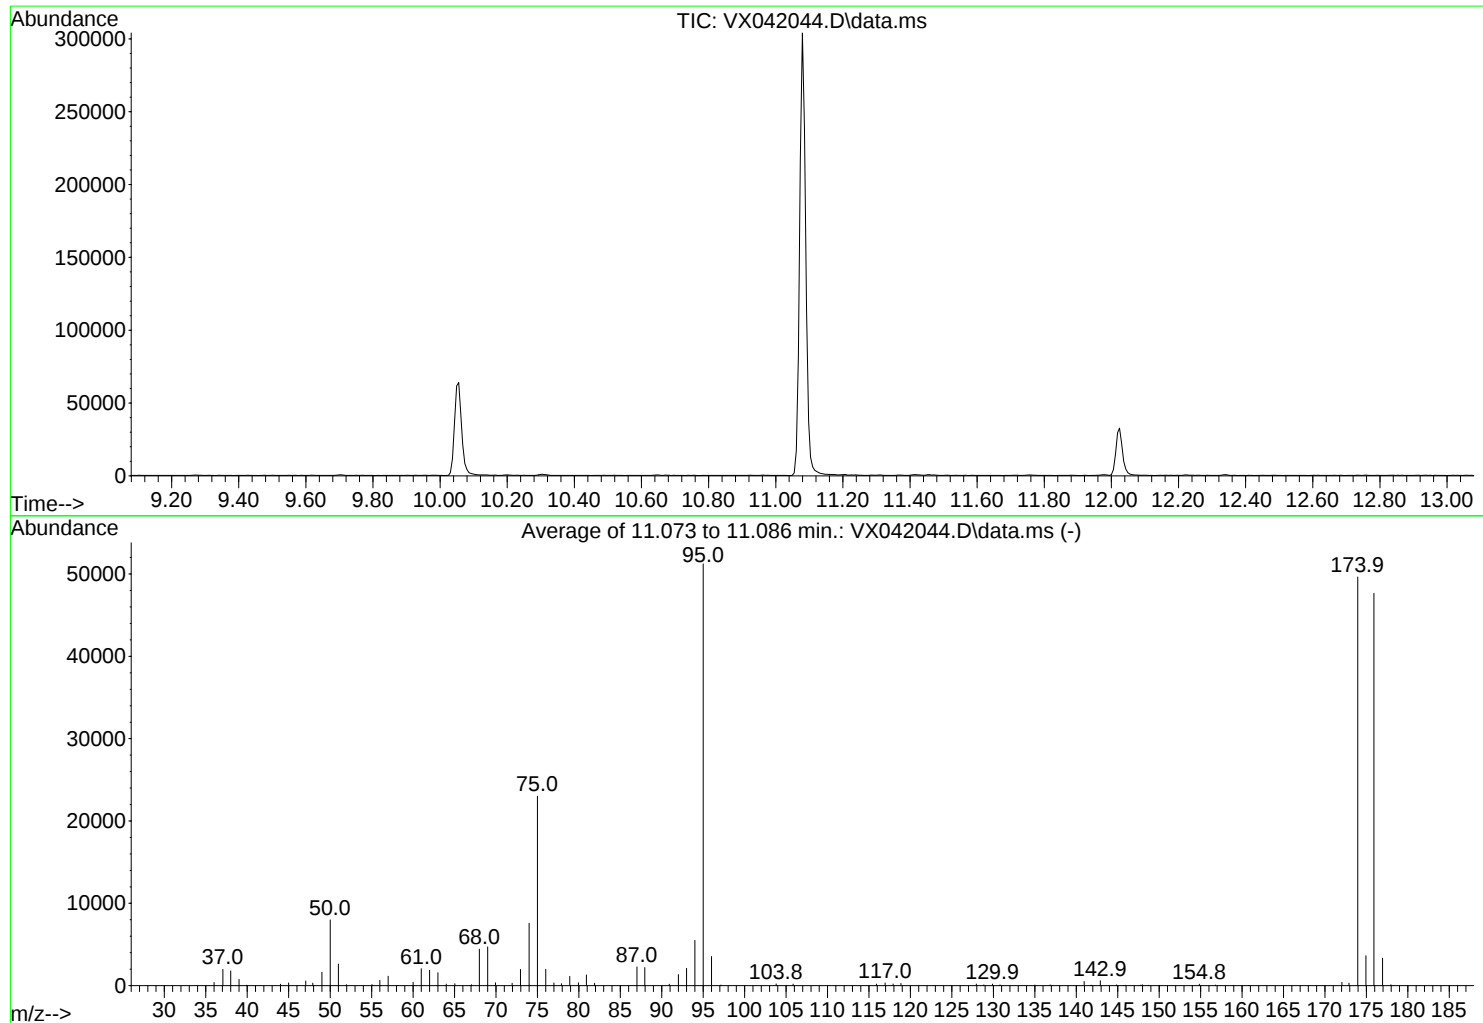

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.6	7992	PASS
75	95	30	60	44.9	23005	PASS
95	95	100	100	100.0	51235	PASS
96	95	5	9	6.9	3547	PASS
173	174	0.00	2	0.6	314	PASS
174	95	50	100	96.9	49643	PASS
175	174	5	9	7.3	3644	PASS
176	174	95	101	96.0	47664	PASS
177	176	5	9	7.0	3334	PASS