

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062718\
 Data File : VX002956.D
 Acq On : 28 Jun 2018 00:53
 Operator : JC/MD
 Sample : J3631-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S83-0020

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	76	80	92	rBV	712696	949663	71.94%	5.501%
2	1.404	128	134	142	rBV3	9892	27359	2.07%	0.158%
3	1.788	192	197	207	rVB	97739	141667	10.73%	0.821%
4	2.001	228	232	240	rVB	22320	30804	2.33%	0.178%
5	2.392	289	296	301	rBV	25153	50071	3.79%	0.290%
6	2.446	301	305	314	rVB	27911	44418	3.36%	0.257%
7	2.843	364	370	374	rBV	30483	65987	5.00%	0.382%
8	2.892	374	378	380	rVV2	25237	47375	3.59%	0.274%
9	2.928	380	384	396	rVB	47406	101908	7.72%	0.590%
10	3.172	415	424	438	rVB	81047	186481	14.13%	1.080%
11	4.306	599	610	617	rBV3	7381	21884	1.66%	0.127%
12	4.403	617	626	639	rVB2	45139	133442	10.11%	0.773%
13	5.507	795	807	815	rBV	160788	473874	35.90%	2.745%
14	5.574	815	818	825	rVV2	36225	101336	7.68%	0.587%
15	5.665	825	833	854	rVB	243231	780285	59.11%	4.520%
16	5.940	868	878	888	rBV7	14966	51256	3.88%	0.297%
17	6.074	890	900	919	rVV	174974	458093	34.70%	2.654%
18	6.269	919	932	940	rVV5	19017	73160	5.54%	0.424%
19	6.354	940	946	955	rVV4	20420	58283	4.42%	0.338%
20	6.452	955	962	971	rVB5	11406	32512	2.46%	0.188%
21	6.866	1018	1030	1047	rBV	348603	822970	62.34%	4.767%
22	7.458	1116	1127	1136	rVB3	35174	91310	6.92%	0.529%
23	7.848	1183	1191	1200	rBV4	12984	28566	2.16%	0.165%
24	8.031	1211	1221	1236	rVB4	14794	46368	3.51%	0.269%
25	8.177	1236	1245	1253	rBV2	12479	28928	2.19%	0.168%
26	8.391	1273	1280	1285	rBV3	12731	25284	1.92%	0.146%
27	8.671	1319	1326	1328	rBV3	18566	33015	2.50%	0.191%
28	8.720	1328	1334	1342	rVV	848438	1320062	100.00%	7.647%
29	8.787	1342	1345	1349	rVV	14118	22910	1.74%	0.133%
30	8.842	1349	1354	1359	rVV2	27699	48247	3.65%	0.279%
31	9.043	1381	1387	1398	rVB	55347	90358	6.84%	0.523%
32	9.165	1400	1407	1414	rVB	21740	36918	2.80%	0.214%
33	9.573	1468	1474	1479	rBV3	20458	34969	2.65%	0.203%
34	9.683	1487	1492	1496	rVV	40536	65980	5.00%	0.382%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062718\
 Data File : VX002956.D
 Acq On : 28 Jun 2018 00:53
 Operator : JC/MD
 Sample : J3631-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S83-0020

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
 Title : SW846 8260

35	9.896	1519	1527	1534	rBV3	11952	23327	1.77%	0.135%
36	10.116	1557	1563	1570	rBV	732276	974998	73.86%	5.648%
37	10.189	1570	1575	1579	rVV	25139	38093	2.89%	0.221%
38	10.256	1579	1586	1591	rVV	277598	371365	28.13%	2.151%
39	10.366	1595	1604	1609	rVV2	82283	155986	11.82%	0.904%
40	10.512	1623	1628	1635	rVB	18508	27953	2.12%	0.162%
41	10.658	1642	1652	1656	rBV6	23904	67511	5.11%	0.391%
42	10.707	1656	1660	1669	rVB2	21096	37330	2.83%	0.216%
43	10.841	1678	1682	1686	rVB2	21321	31288	2.37%	0.181%
44	10.914	1686	1694	1698	rBV4	17270	30154	2.28%	0.175%
45	11.024	1707	1712	1715	rBV	30896	42013	3.18%	0.243%
46	11.140	1725	1731	1736	rBV	768806	939576	71.18%	5.443%
47	11.183	1736	1738	1743	rVV	18116	24454	1.85%	0.142%
48	11.280	1751	1754	1759	rVB3	22133	31296	2.37%	0.181%
49	11.360	1764	1767	1775	rVV	24161	38203	2.89%	0.221%
50	11.457	1778	1783	1787	rVV	40970	58734	4.45%	0.340%
51	11.670	1810	1818	1827	rBV	167607	223919	16.96%	1.297%
52	11.768	1827	1834	1837	rBV	17174	28400	2.15%	0.165%
53	11.811	1837	1841	1852	rVB	427891	515432	39.05%	2.986%
54	12.079	1880	1885	1891	rBV	888209	1143470	86.62%	6.624%
55	12.146	1891	1896	1905	rVB	529493	639925	48.48%	3.707%
56	12.237	1906	1911	1916	rVB	42138	55854	4.23%	0.324%
57	12.304	1917	1922	1927	rBV	172363	210028	15.91%	1.217%
58	12.372	1928	1933	1942	rVB2	72828	117113	8.87%	0.678%
59	12.463	1943	1948	1953	rBV	81192	104574	7.92%	0.606%
60	12.524	1953	1958	1963	rVB	166233	212000	16.06%	1.228%
61	12.591	1963	1969	1971	rBV	100017	141859	10.75%	0.822%
62	12.615	1971	1973	1976	rVV	115212	113873	8.63%	0.660%
63	12.670	1978	1982	1985	rVV	152849	179254	13.58%	1.038%
64	12.707	1985	1988	1993	rVV2	59197	85246	6.46%	0.494%
65	12.768	1993	1998	2004	rVB3	127554	242421	18.36%	1.404%
66	12.908	2017	2021	2026	rVB2	172321	237816	18.02%	1.378%
67	12.981	2026	2033	2036	rBV2	171953	243327	18.43%	1.410%
68	13.024	2036	2040	2046	rVV	324555	401621	30.42%	2.326%
69	13.085	2046	2050	2057	rVB3	64205	100068	7.58%	0.580%
70	13.152	2057	2061	2065	rBV	40490	56669	4.29%	0.328%
71	13.201	2065	2069	2072	rVV2	71618	98212	7.44%	0.569%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062718\
Data File : VX002956.D
Acq On : 28 Jun 2018 00:53
Operator : JC/MD
Sample : J3631-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S83-0020

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 3 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Title : SW846 8260

72	13.231	2072	2074	2076	rVV	29044	31849	2.41%	0.184%
73	13.268	2076	2080	2083	rVV2	27402	46028	3.49%	0.267%
74	13.310	2083	2087	2089	rVV2	61627	80423	6.09%	0.466%
75	13.347	2089	2093	2098	rVV2	494961	704606	53.38%	4.082%
76	13.390	2098	2100	2104	rVV3	30116	47163	3.57%	0.273%
77	13.426	2104	2106	2109	rVV	24971	29260	2.22%	0.169%
78	13.481	2109	2115	2122	rVB2	110960	172341	13.06%	0.998%
79	13.566	2124	2129	2132	rBV3	29228	50364	3.82%	0.292%
80	13.603	2132	2135	2137	rVV2	26296	35121	2.66%	0.203%
81	13.646	2137	2142	2147	rVV3	106888	234580	17.77%	1.359%
82	13.701	2148	2151	2153	rVV	59005	90766	6.88%	0.526%
83	13.725	2153	2155	2161	rVB2	81237	128317	9.72%	0.743%
84	13.810	2166	2169	2171	rVV	34861	47571	3.60%	0.276%
85	13.841	2171	2174	2182	rVB2	81889	164020	12.43%	0.950%
86	13.914	2182	2186	2191	rVB3	42832	61473	4.66%	0.356%
87	13.987	2191	2198	2202	rBV2	71308	113152	8.57%	0.655%
88	14.030	2202	2205	2209	rVV3	34185	53618	4.06%	0.311%
89	14.133	2218	2222	2225	rBV4	23040	33776	2.56%	0.196%
90	14.274	2240	2245	2253	rVB2	60703	102097	7.73%	0.591%
91	14.383	2259	2263	2267	rVB	34086	39953	3.03%	0.231%
92	14.432	2267	2271	2275	rVB3	31062	39533	2.99%	0.229%
93	14.481	2275	2279	2284	rVB2	19017	26946	2.04%	0.156%
94	14.542	2284	2289	2298	rBV2	77638	118678	8.99%	0.687%
95	14.700	2308	2315	2318	rVV3	27677	51764	3.92%	0.300%
96	14.737	2318	2321	2325	rVV	18126	22312	1.69%	0.129%
97	14.847	2334	2339	2343	rVV2	49788	83250	6.31%	0.482%
98	15.255	2400	2406	2413	rBV4	14077	28196	2.14%	0.163%
99	15.554	2447	2455	2459	rBV2	16631	29518	2.24%	0.171%
100	15.688	2473	2477	2481	rBV3	16843	27520	2.08%	0.159%


Sum of corrected areas: 17263300

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062718\
Data File : VX002956.D
Acq On : 28 Jun 2018 00:53
Operator : JC/MD
Sample : J3631-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S83-0020

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

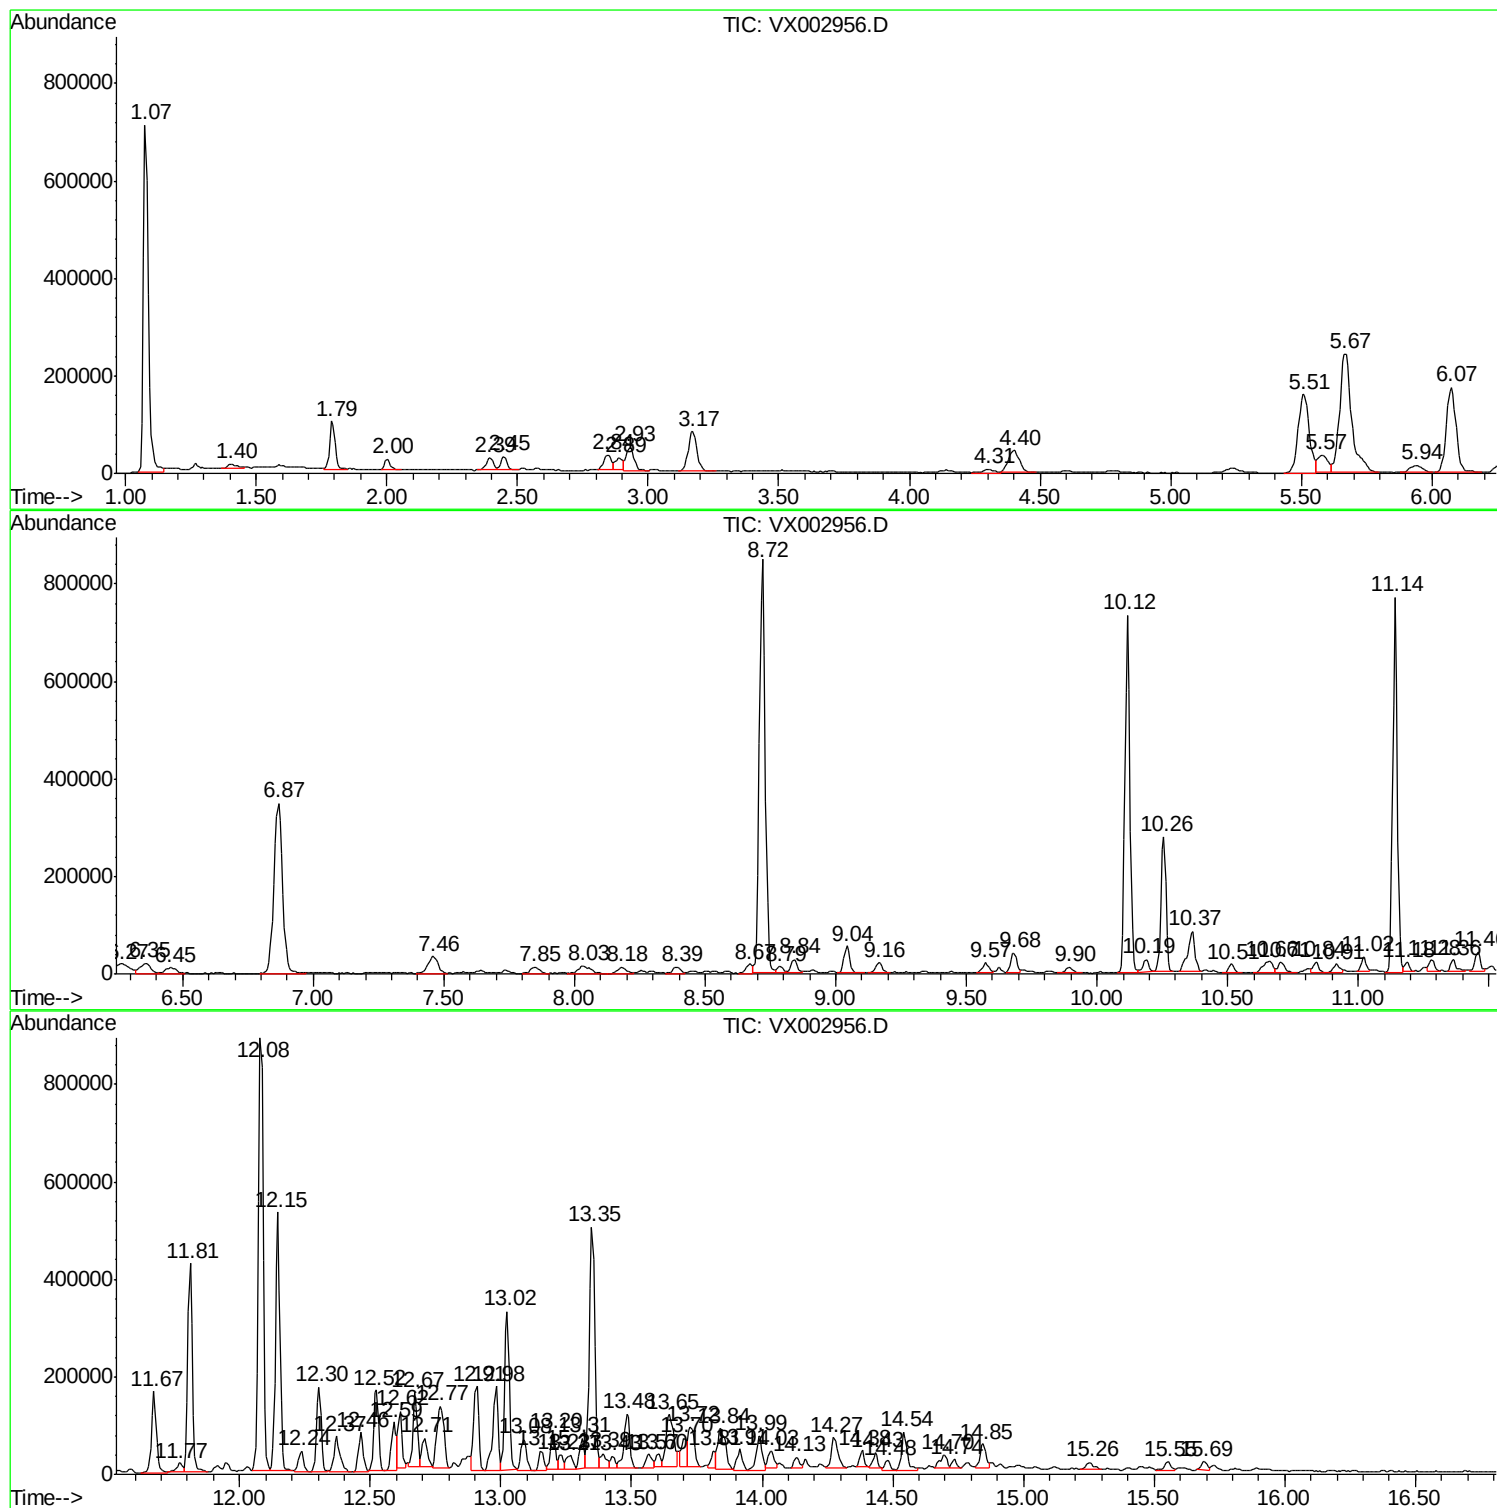

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX062718\
Data File : VX002956.D
Acq On : 28 Jun 2018 00:53
Operator : JC/MD
Sample : J3631-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S83-0020

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX062718\
Data File : VX002956.D
Acq On : 28 Jun 2018 00:53
Operator : JC/MD
Sample : J3631-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S83-0020

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc