

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062718\
 Data File : VX002958.D
 Acq On : 28 Jun 2018 01:46
 Operator : JC/MD
 Sample : J3631-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S83-0019

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	76	80	93	rBV	956130	1211610	9.15%	0.987%
2	1.794	192	198	208	rVB	258428	372986	2.82%	0.304%
3	2.843	362	370	375	rBV	203508	468970	3.54%	0.382%
4	2.928	381	384	397	rVB	159514	318585	2.41%	0.260%
5	3.172	415	424	436	rVB	151615	347622	2.63%	0.283%
6	4.306	599	610	617	rBV	111570	335545	2.53%	0.273%
7	4.397	617	625	641	rVB	335282	983692	7.43%	0.802%
8	5.507	794	807	812	rBV	176372	499699	3.77%	0.407%
9	5.580	812	819	827	rVV2	418576	1352853	10.22%	1.102%
10	5.672	827	834	837	rVV	285879	756529	5.71%	0.616%
11	5.726	838	843	862	rVV	416056	1223178	9.24%	0.997%
12	5.934	864	877	891	rVV3	114922	394945	2.98%	0.322%
13	6.074	891	900	904	rVV	184723	465685	3.52%	0.379%
14	6.153	904	913	924	rVV	2658795	6998776	52.86%	5.703%
15	6.263	924	931	937	rVV2	90953	304245	2.30%	0.248%
16	6.354	937	946	955	rVV	406953	1262279	9.53%	1.029%
17	6.458	955	963	978	rVB	114866	324552	2.45%	0.264%
18	6.866	1020	1030	1039	rBV	377982	887506	6.70%	0.723%
19	7.263	1084	1095	1104	rBV	106061	239117	1.81%	0.195%
20	7.464	1115	1128	1139	rBV	712934	1620640	12.24%	1.321%
21	7.738	1168	1173	1184	rVB	97282	185312	1.40%	0.151%
22	8.055	1214	1225	1235	rVB	527800	1125616	8.50%	0.917%
23	8.183	1235	1246	1253	rBV	851390	1701862	12.85%	1.387%
24	8.256	1253	1258	1263	rVV	104887	167052	1.26%	0.136%
25	8.671	1318	1326	1329	rBV3	253288	497115	3.75%	0.405%
26	8.720	1329	1334	1340	rVV	958914	1583198	11.96%	1.290%
27	8.787	1340	1345	1350	rVV	342494	525179	3.97%	0.428%
28	8.842	1350	1354	1358	rVV	139465	234266	1.77%	0.191%
29	9.043	1381	1387	1393	rVB	262695	420765	3.18%	0.343%
30	9.165	1398	1407	1413	rBV	134604	228829	1.73%	0.186%
31	9.573	1469	1474	1478	rBV2	113796	172130	1.30%	0.140%
32	9.628	1478	1483	1487	rVB	213495	300887	2.27%	0.245%
33	9.683	1487	1492	1496	rBV	226387	340767	2.57%	0.278%
34	10.116	1558	1563	1568	rBV	810889	1036311	7.83%	0.844%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062718\
 Data File : VX002958.D
 Acq On : 28 Jun 2018 01:46
 Operator : JC/MD
 Sample : J3631-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S83-0019

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
 Title : SW846 8260

35	10.189	1568	1575	1580	rVB	166107	247879	1.87%	0.202%
36	10.256	1580	1586	1595	rBV	6811381	8629063	65.17%	7.031%
37	10.360	1595	1603	1610	rBV	9551501	13241378	100.00%	10.790%
38	10.646	1642	1650	1655	rBV4	69794	195460	1.48%	0.159%
39	10.701	1655	1659	1670	rVB	1191259	1530535	11.56%	1.247%
40	10.841	1670	1682	1689	rBV2	120167	221580	1.67%	0.181%
41	11.024	1706	1712	1725	rVB	842661	1121771	8.47%	0.914%
42	11.140	1725	1731	1736	rBV	884815	1098950	8.30%	0.895%
43	11.360	1762	1767	1774	rVV	816277	1054801	7.97%	0.859%
44	11.439	1774	1780	1787	rVV	1952201	3756555	28.37%	3.061%
45	11.512	1787	1792	1800	rVB	3232827	3915708	29.57%	3.191%
46	11.670	1809	1818	1828	rBV	4197234	5054540	38.17%	4.119%
47	11.811	1836	1841	1847	rVB	8215804	9369148	70.76%	7.634%
48	11.951	1861	1864	1869	rVB	208747	248747	1.88%	0.203%
49	12.030	1872	1877	1880	rBV	538455	631433	4.77%	0.515%
50	12.079	1880	1885	1890	rVB2	1167273	1665830	12.58%	1.357%
51	12.146	1891	1896	1901	rBV	5332872	6404511	48.37%	5.219%
52	12.237	1905	1911	1916	rVB	213110	266736	2.01%	0.217%
53	12.304	1916	1922	1925	rBV	1530379	2166052	16.36%	1.765%
54	12.378	1929	1934	1943	rVB2	1627042	2251767	17.01%	1.835%
55	12.463	1943	1948	1953	rBV2	447068	556175	4.20%	0.453%
56	12.524	1953	1958	1964	rVB	1150296	1390238	10.50%	1.133%
57	12.591	1964	1969	1971	rBV	1081914	1509223	11.40%	1.230%
58	12.615	1971	1973	1977	rVV	1335404	1308284	9.88%	1.066%
59	12.670	1977	1982	1985	rVV	1630776	1894085	14.30%	1.543%
60	12.707	1985	1988	1992	rVB	327418	411606	3.11%	0.335%
61	12.762	1992	1997	2004	rBV4	1040365	1997617	15.09%	1.628%
62	12.853	2009	2012	2016	rBV2	201568	237205	1.79%	0.193%
63	12.908	2016	2021	2026	rVB2	1206410	1582401	11.95%	1.289%
64	12.981	2026	2033	2036	rBV	1153862	1495436	11.29%	1.219%
65	13.024	2036	2040	2045	rVB	1990205	2310616	17.45%	1.883%
66	13.085	2045	2050	2055	rBV3	258772	523893	3.96%	0.427%
67	13.152	2059	2061	2065	rVB	144135	152685	1.15%	0.124%
68	13.201	2065	2069	2071	rBV2	276480	350057	2.64%	0.285%
69	13.225	2071	2073	2077	rVB	246898	265371	2.00%	0.216%
70	13.268	2077	2080	2083	rVB2	146509	189827	1.43%	0.155%
71	13.310	2083	2087	2089	rBV2	266320	351640	2.66%	0.287%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062718\
 Data File : VX002958.D
 Acq On : 28 Jun 2018 01:46
 Operator : JC/MD
 Sample : J3631-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S83-0019

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
 Title : SW846 8260

72	13.347	2089	2093	2099	rVB2	2911908	3840432	29.00%	3.129%
73	13.481	2111	2115	2122	rVB	1132115	1421977	10.74%	1.159%
74	13.566	2124	2129	2132	rVV3	152547	235140	1.78%	0.192%
75	13.603	2132	2135	2138	rVV	205884	294000	2.22%	0.240%
76	13.646	2138	2142	2147	rVV3	481877	1006965	7.60%	0.821%
77	13.701	2148	2151	2153	rVV	261418	398623	3.01%	0.325%
78	13.725	2153	2155	2161	rVV2	387321	552195	4.17%	0.450%
79	13.835	2165	2173	2182	rVB2	981775	1628601	12.30%	1.327%
80	13.914	2182	2186	2191	rVB	191893	252374	1.91%	0.206%
81	13.987	2191	2198	2202	rBV2	305823	457120	3.45%	0.372%
82	14.030	2202	2205	2209	rBV	109899	134078	1.01%	0.109%
83	14.133	2218	2222	2225	rBV2	94840	133994	1.01%	0.109%
84	14.292	2240	2248	2255	rBV2	351025	678992	5.13%	0.553%
85	14.383	2259	2263	2267	rVV	107841	134292	1.01%	0.109%
86	14.432	2267	2271	2275	rVB2	111537	142073	1.07%	0.116%
87	14.542	2284	2289	2298	rBV2	373103	515780	3.90%	0.420%
88	14.700	2308	2315	2319	rBV	726907	932249	7.04%	0.760%
89	14.841	2333	2338	2347	rBV	652494	904166	6.83%	0.737%
90	15.554	2449	2455	2460	rBV	94606	152485	1.15%	0.124%
91	15.694	2470	2478	2481	rBV	153227	252926	1.91%	0.206%
92	15.731	2481	2484	2491	rVB	116833	168018	1.27%	0.137%


Sum of corrected areas: 122723586

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062718\
Data File : VX002958.D
Acq On : 28 Jun 2018 01:46
Operator : JC/MD
Sample : J3631-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S83-0019

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

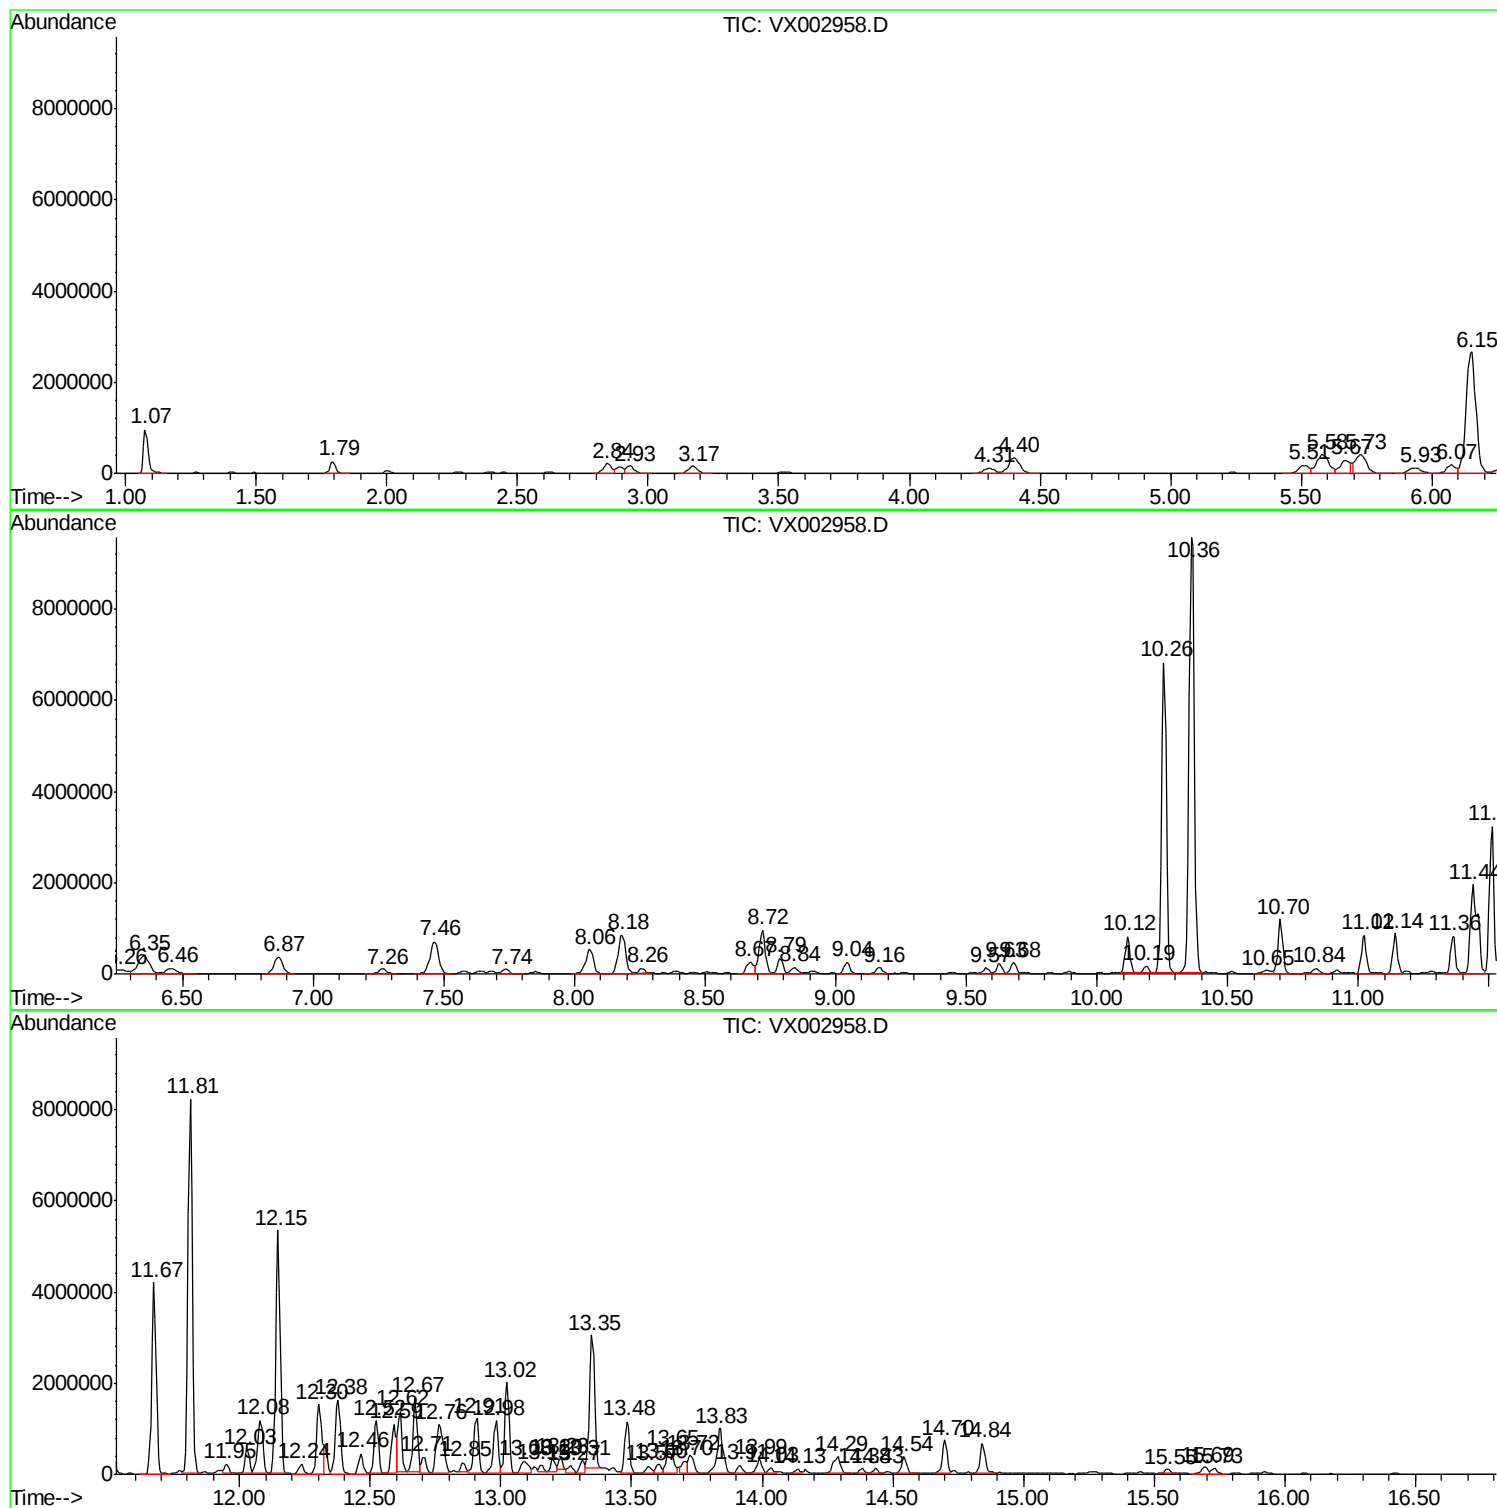

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX062718\
Data File : VX002958.D
Acq On : 28 Jun 2018 01:46
Operator : JC/MD
Sample : J3631-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S83-0019

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX062718\
Data File : VX002958.D
Acq On : 28 Jun 2018 01:46
Operator : JC/MD
Sample : J3631-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S83-0019

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc