

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062719\
 Data File : VX010482.D
 Acq On : 27 Jun 2019 12:35
 Operator : JC/SP
 Sample : K3527-21
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CPA-MW16-001-M24W1-061919

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	16	20	26	rBV	17698	24780	2.18%	0.408%
2	1.611	64	75	79	rBV5	4940	12973	1.14%	0.214%
3	2.611	234	239	247	rVB	10320	19229	1.69%	0.317%
4	5.501	699	713	725	rBV	139599	394343	34.62%	6.500%
5	5.659	729	739	755	rVB	235359	656117	57.60%	10.815%
6	6.061	794	805	819	rBV	131108	348506	30.60%	5.745%
7	6.860	923	936	946	rBV	349355	818403	71.85%	13.491%
8	8.713	1233	1240	1250	rBV	737926	1138998	100.00%	18.775%
9	9.335	1336	1342	1350	rBV2	14369	22885	2.01%	0.377%
10	10.110	1463	1469	1480	rBV	719255	964533	84.68%	15.899%
11	11.134	1632	1637	1645	rBV	593375	760903	66.80%	12.543%
12	12.079	1786	1792	1802	rBV	684160	904826	79.44%	14.915%


Sum of corrected areas: 6066496

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062719\
Data File : VX010482.D
Acq On : 27 Jun 2019 12:35
Operator : JC/SP
Sample : K3527-21
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CPA-MW16-001-M24W1-061919

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

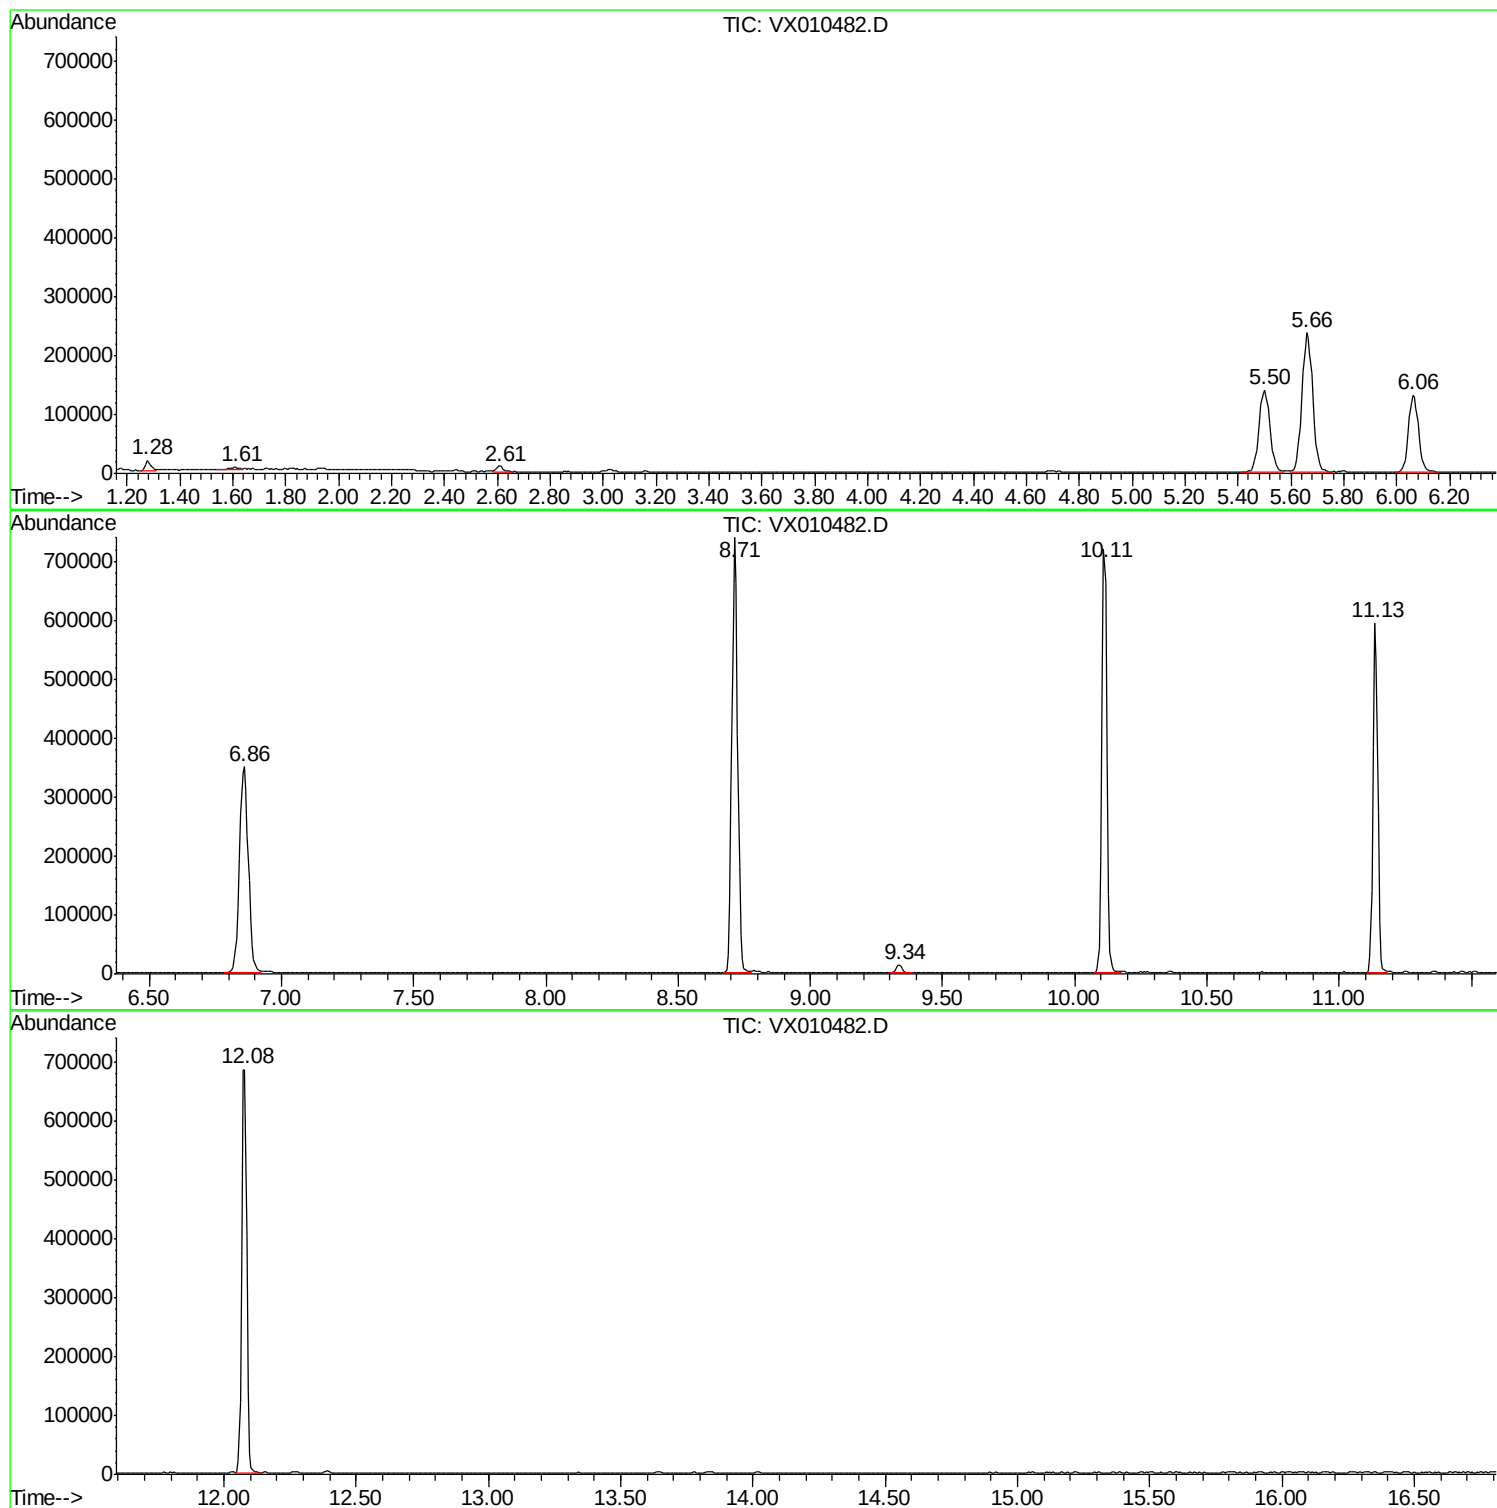

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX062719\
Data File : VX010482.D
Acq On : 27 Jun 2019 12:35
Operator : JC/SP
Sample : K3527-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CPA-MW16-001-M24W1-061919

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX062719\
Data File : VX010482.D
Acq On : 27 Jun 2019 12:35
Operator : JC/SP
Sample : K3527-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CPA-MW16-001-M24W1-061919

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc