


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX062719\
Data File : VX010475.D
Acq On : 27 Jun 2019 09:11
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Title : SW846 8260
Last Update : Thu Jun 20 03:31:56 2019

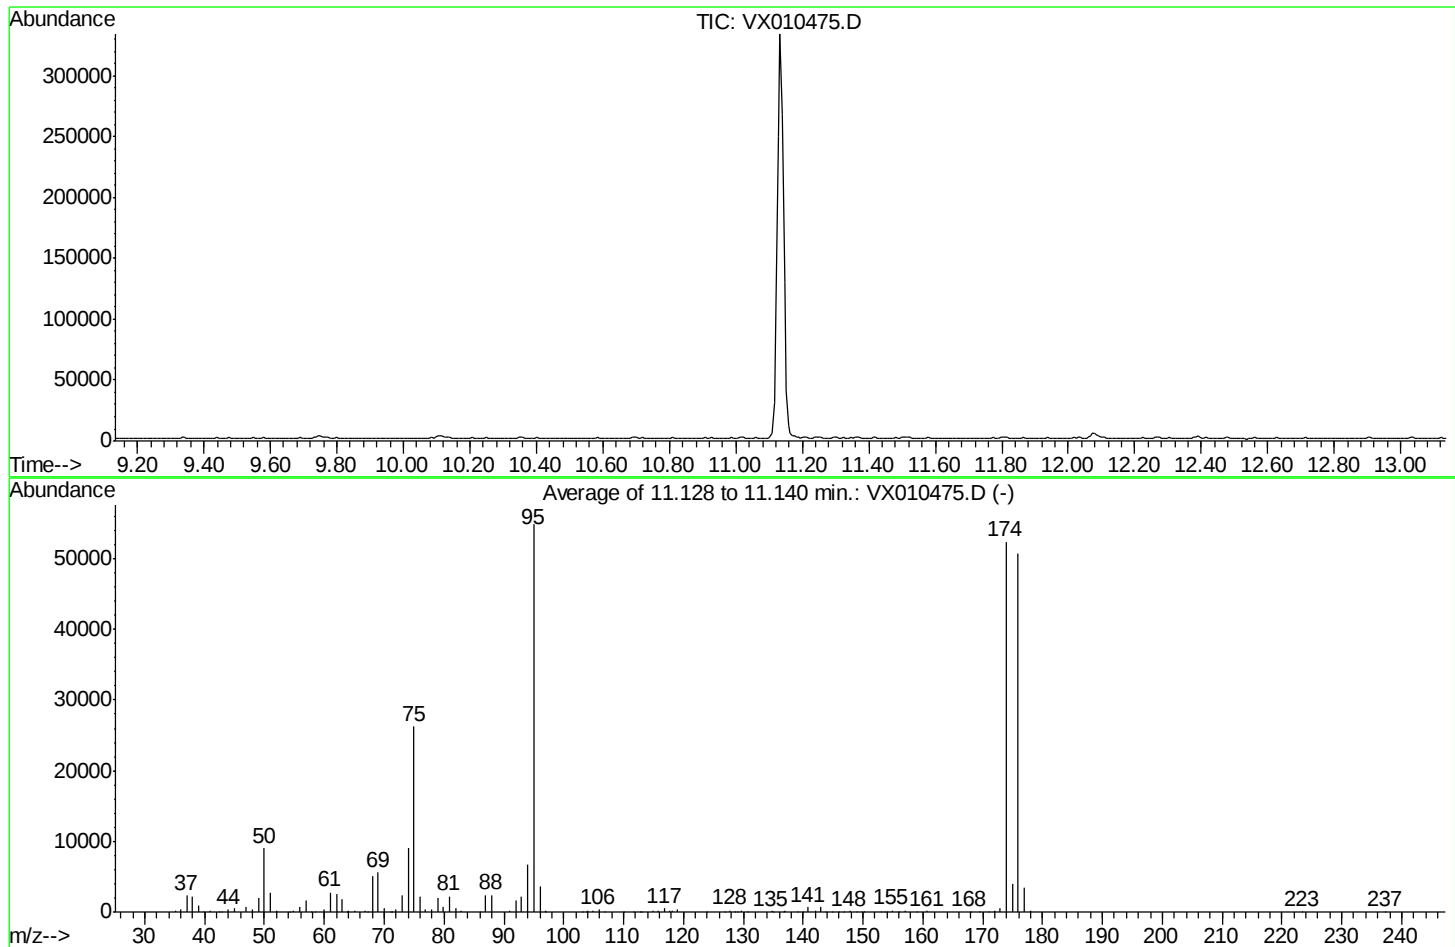

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	8977	PASS
75	95	30	60	47.8	26248	PASS
95	95	100	100	100.0	54866	PASS
96	95	5	9	6.6	3647	PASS
173	174	0.00	2	1.0	538	PASS
174	95	50	100	95.6	52442	PASS
175	174	5	9	7.6	3990	PASS
176	174	95	101	96.9	50808	PASS
177	176	5	9	6.6	3364	PASS