

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062723\
 Data File : VX036345.D
 Acq On : 27 Jun 2023 12:50
 Operator : JC/MD
 Sample : VX0627MBL02
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0627MBL02

Quant Time: Jun 28 04:18:57 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 23 15:03:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.549	168	219149	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	375415	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	342237	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	162184	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	163267	51.974	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	103.940%
35) Dibromofluoromethane	5.385	113	126195	50.980	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	101.960%
50) Toluene-d8	8.646	98	453053	49.002	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.000%
62) 4-Bromofluorobenzene	11.079	95	165811	50.916	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	101.840%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062723\
Data File : VX036345.D
Acq On : 27 Jun 2023 12:50
Operator : JC/MD
Sample : VX0627MBL02
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0627MBL02

Quant Time: Jun 28 04:18:57 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 23 15:03:28 2023
Response via : Initial Calibration




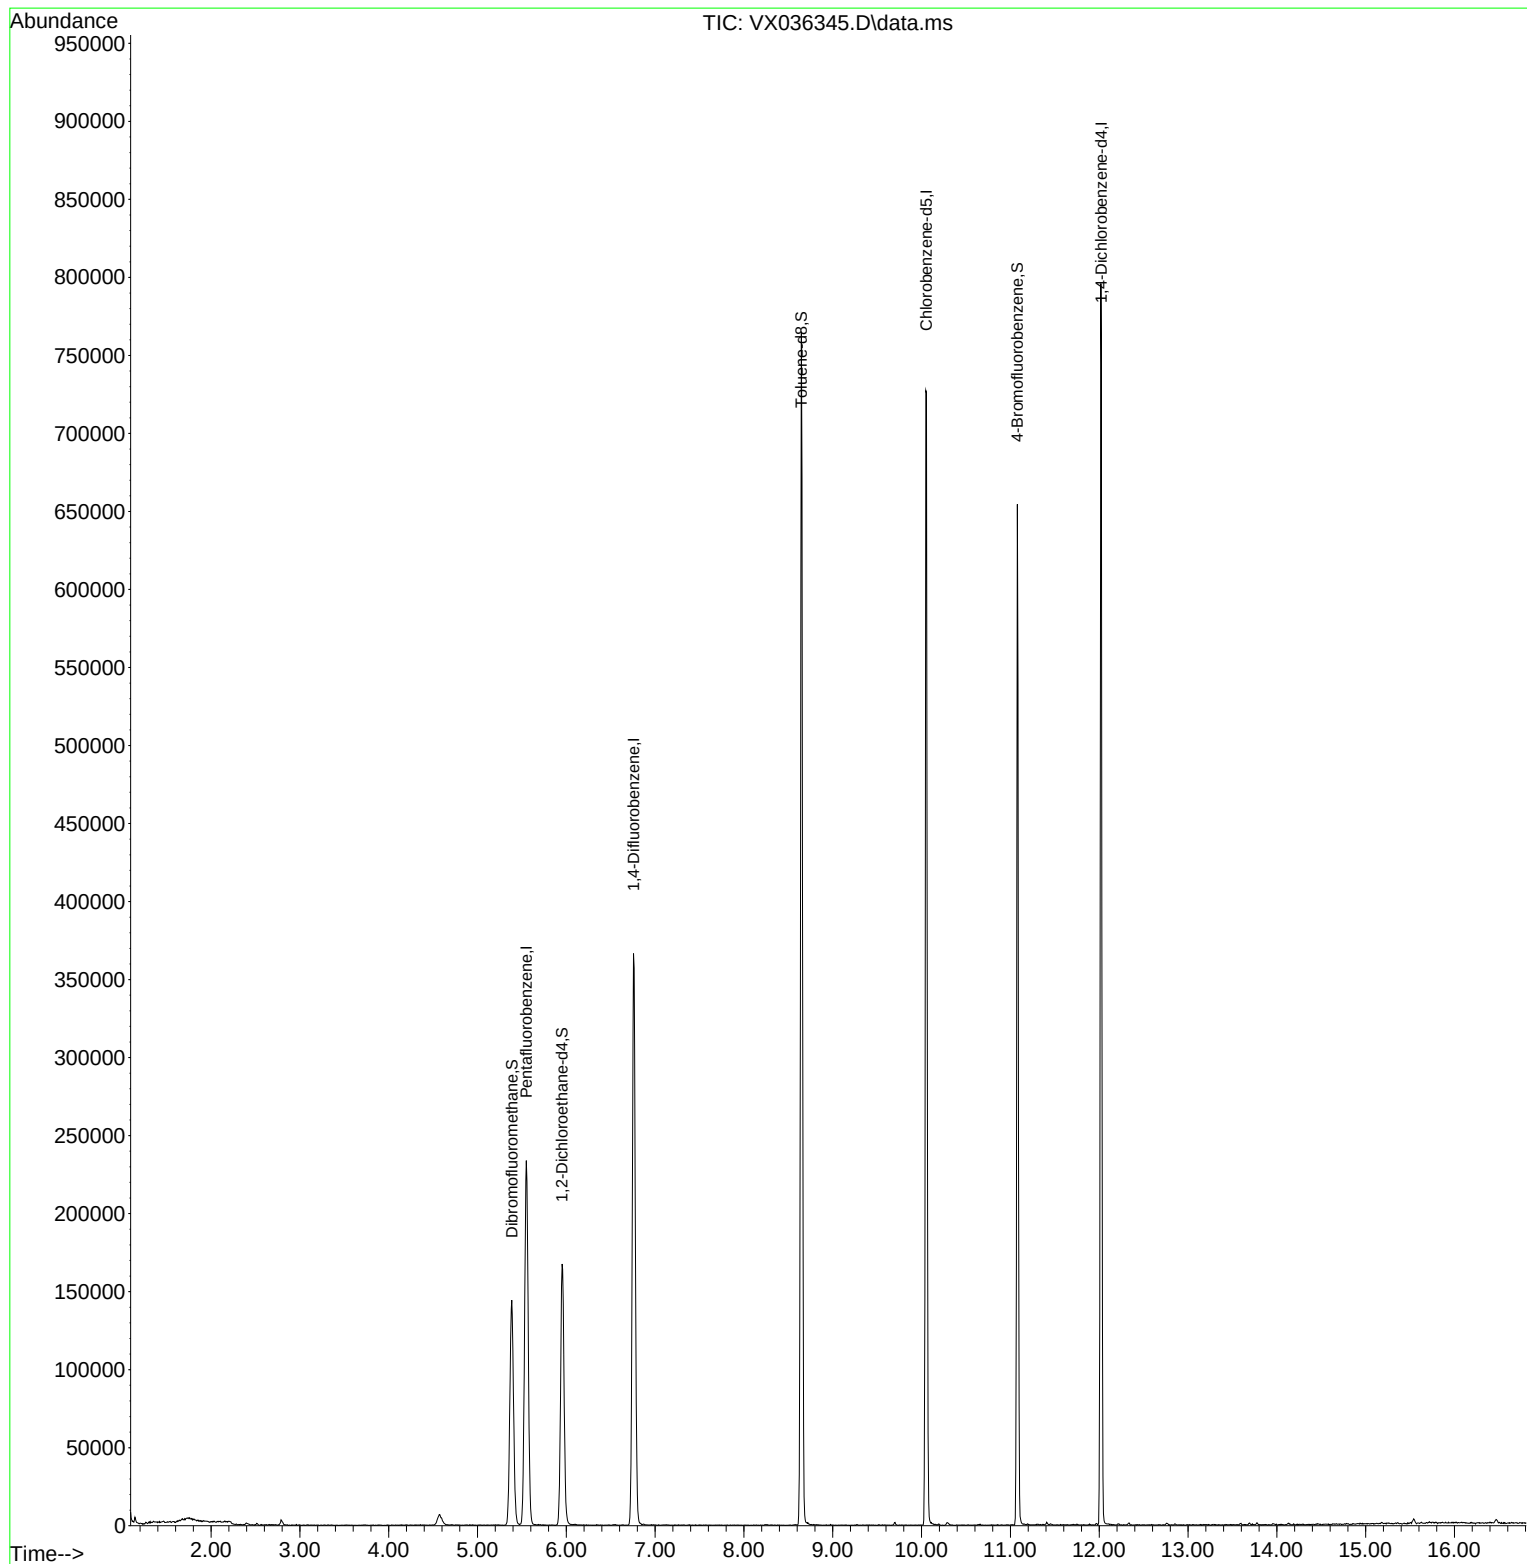


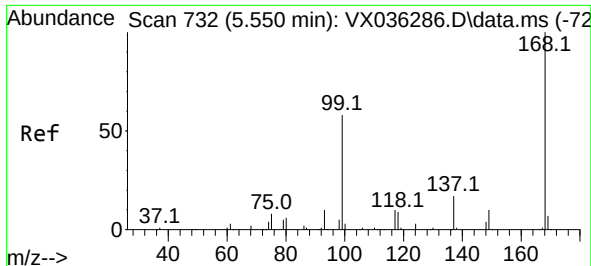

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.549 min Scan# 71
Delta R.T. 0.000 min
Lab File: VX036345.D
Acq: 27 Jun 2023 12:50




Instrument :
MSVOA_X
ClientSampleId :
VX0627MBL02


Tgt Ion:168 Resp: 219149
Ion Ratio Lower Upper
168 100
99 61.3 56.6 85.0

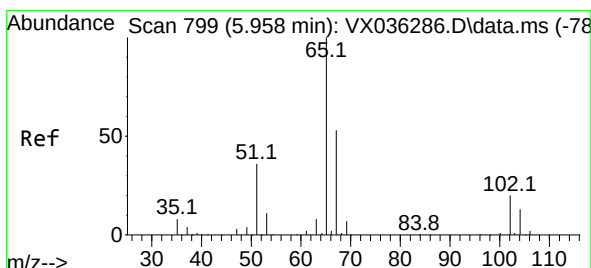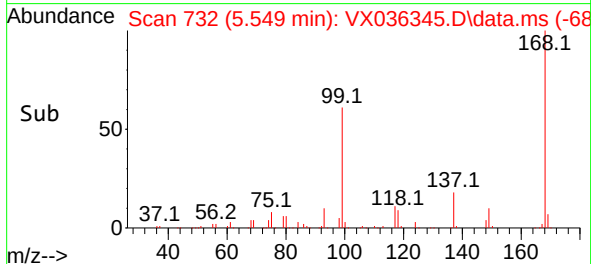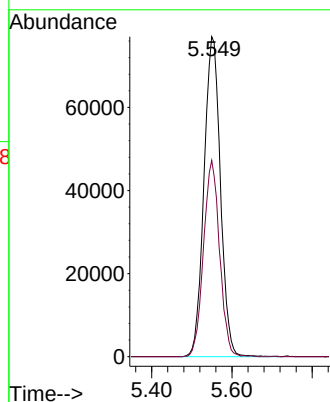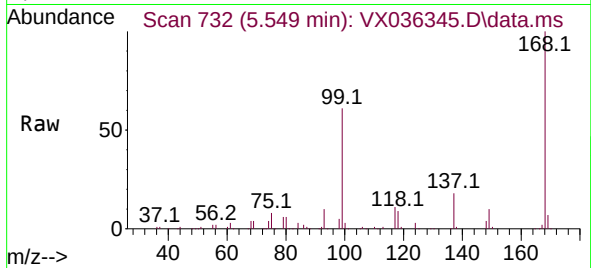

#33
1,2-Dichloroethane-d4
Concen: 51.974 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX036345.D
Acq: 27 Jun 2023 12:50

Tgt Ion: 65 Resp: 163267
Ion Ratio Lower Upper
65 100
67 51.8 0.0 100.2


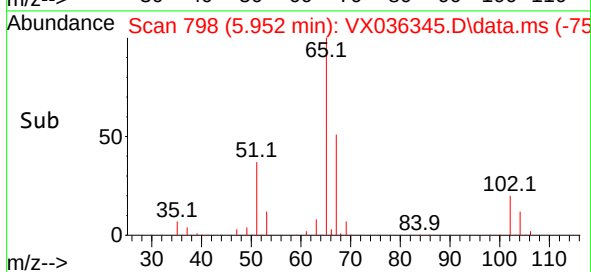
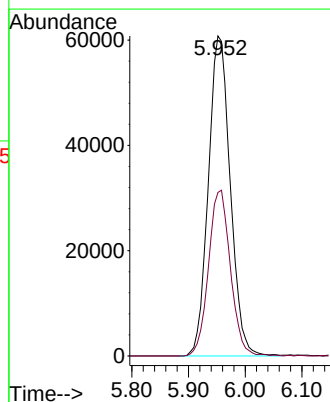
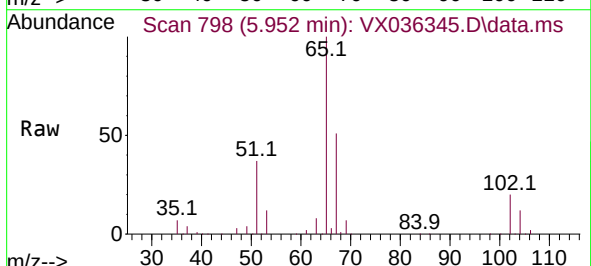


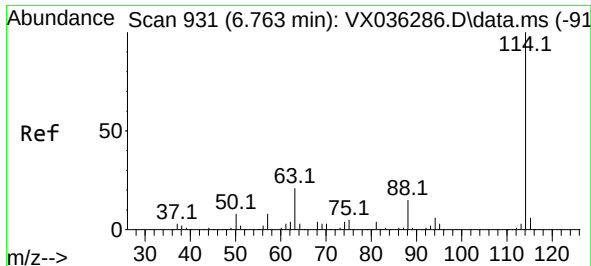

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 911
Delta R.T. -0.006 min
Lab File: VX036345.D
Acq: 27 Jun 2023 12:50




Instrument :
MSVOA_X
ClientSampleId :
VX0627MBL02


Tgt Ion:114 Resp: 375415
Ion Ratio Lower Upper
114 100
63 21.0 0.0 45.0
88 15.6 0.0 36.6

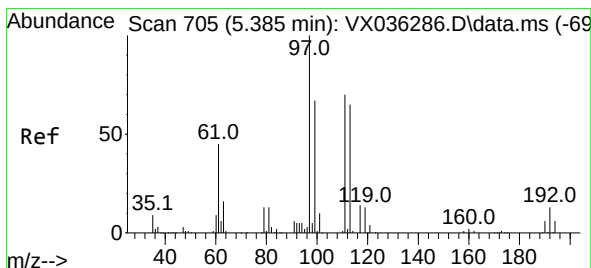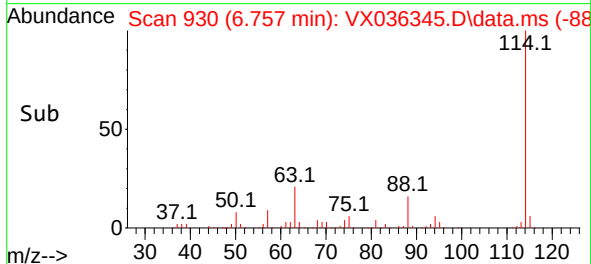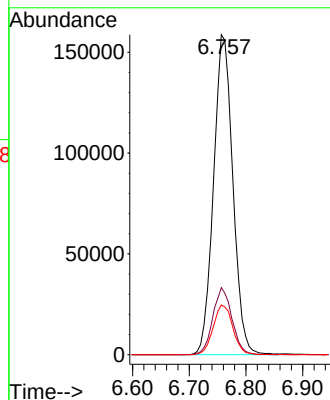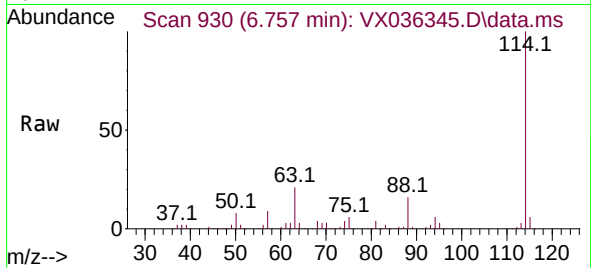

#35
Dibromofluoromethane
Concen: 50.980 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX036345.D
Acq: 27 Jun 2023 12:50

Tgt Ion:113 Resp: 126195
Ion Ratio Lower Upper
113 100
111 102.3 82.9 124.3
192 19.0 13.3 19.9

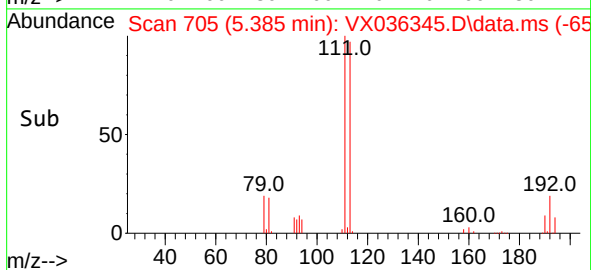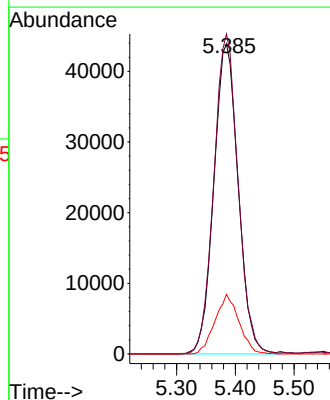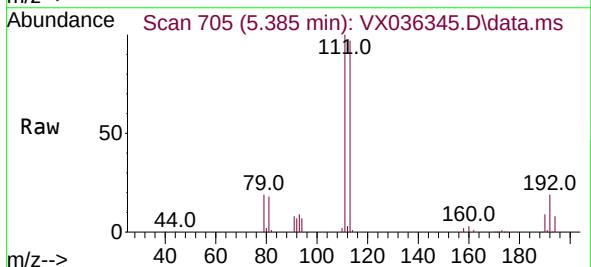

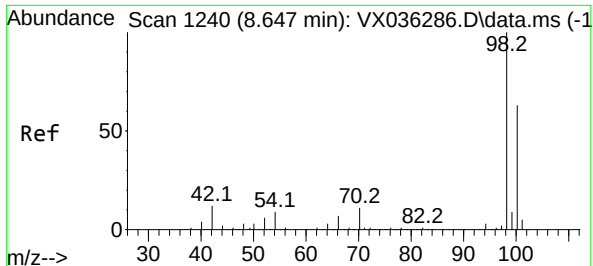

#50

Toluene-d8

Concen: 49.002 ug/l

RT: 8.646 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX036345.D

Acq: 27 Jun 2023 12:50

Instrument :

MSVOA_X

ClientSampleId :





VX0627MBL02

Tgt Ion: 98 Resp: 453053

Ion Ratio Lower Upper

98 100

100 63.6 53.1 79.7

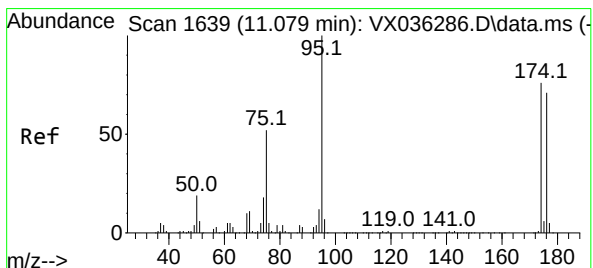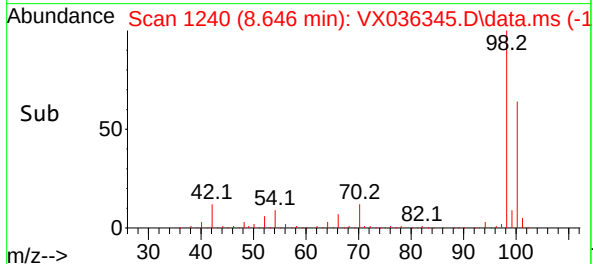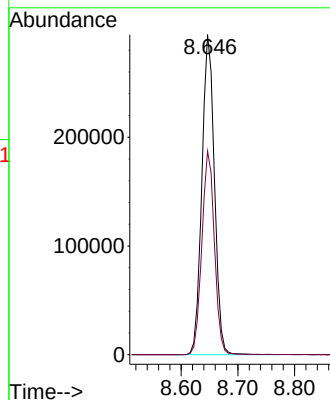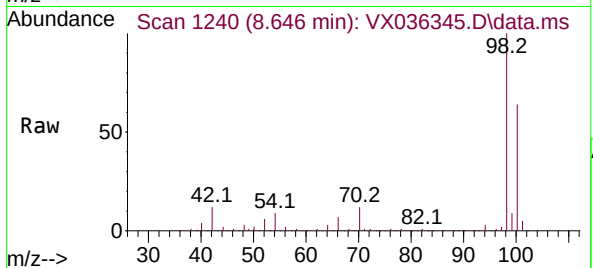

#62

4-Bromofluorobenzene

Concen: 50.916 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.000 min

Lab File: VX036345.D

Acq: 27 Jun 2023 12:50




Tgt Ion: 95 Resp: 165811


Ion Ratio Lower Upper

95 100

174 79.0 0.0 135.6

176 74.4 0.0 131.0


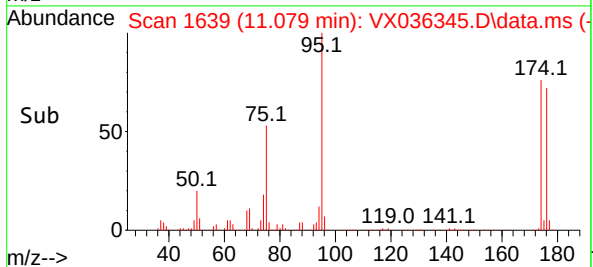
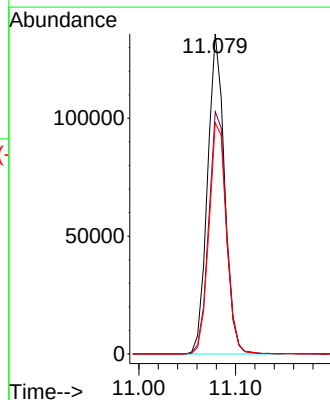
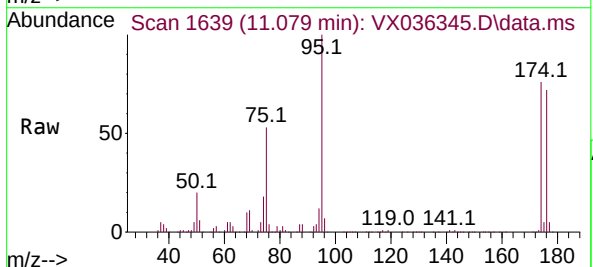


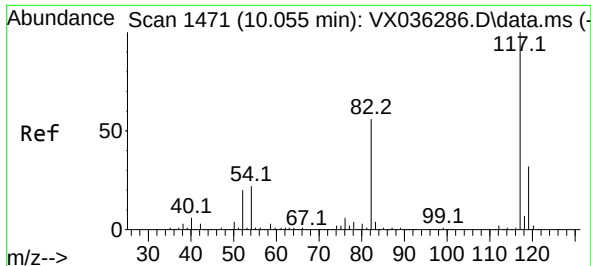

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX036345.D
Acq: 27 Jun 2023 12:50

Instrument :
MSVOA_X
ClientSampleId :
VX0627MBL02

Tgt Ion:117 Resp: 342237
Ion Ratio Lower Upper
117 100
82 56.0 46.2 69.4
119 32.1 25.5 38.3

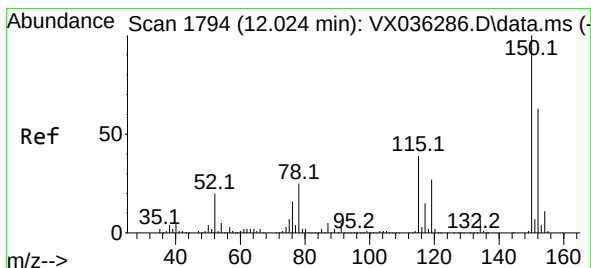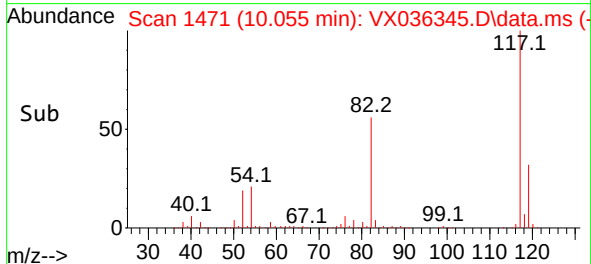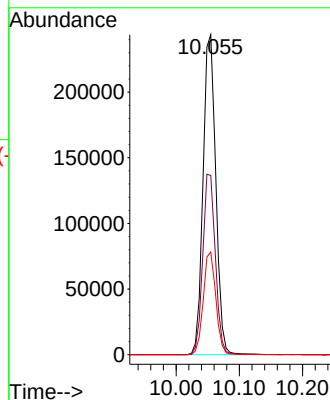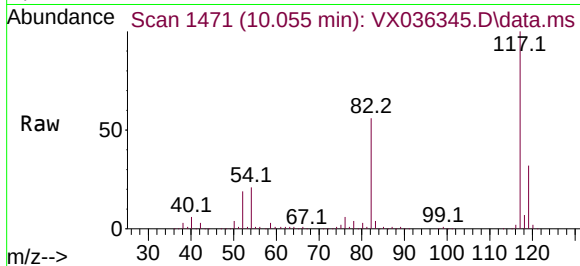

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX036345.D
Acq: 27 Jun 2023 12:50

Tgt Ion:152 Resp: 162184
Ion Ratio Lower Upper
152 100
115 60.5 43.3 129.9
150 154.9 0.0 345.0

