

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062818\
 Data File : VX003012.D
 Acq On : 29 Jun 2018 04:29
 Operator : JC/MD
 Sample : J3720-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 ULMER-PARK-TRIP-BLANK-1-6-25-

Quant Time: Jun 29 10:17:22 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 25 14:38:05 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	293759	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	410765	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	380005	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.09	152	217128	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	193418	47.64	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.28%	
35) Dibromofluoromethane	5.51	113	156340	48.06	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.12%	
50) Toluene-d8	8.72	98	573944	48.32	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.64%	
62) 4-Bromofluorobenzene	11.14	95	203520	44.43	ug/l	0.00
Spiked Amount	50.000		Recovery	=	88.86%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062818\
Data File : VX003012.D
Acq On : 29 Jun 2018 04:29
Operator : JC/MD
Sample : J3720-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ULMER-PARK-TRIP-BLANK-1-6-25-

Quant Time: Jun 29 10:17:22 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 25 14:38:05 2018
Response via : Initial Calibration

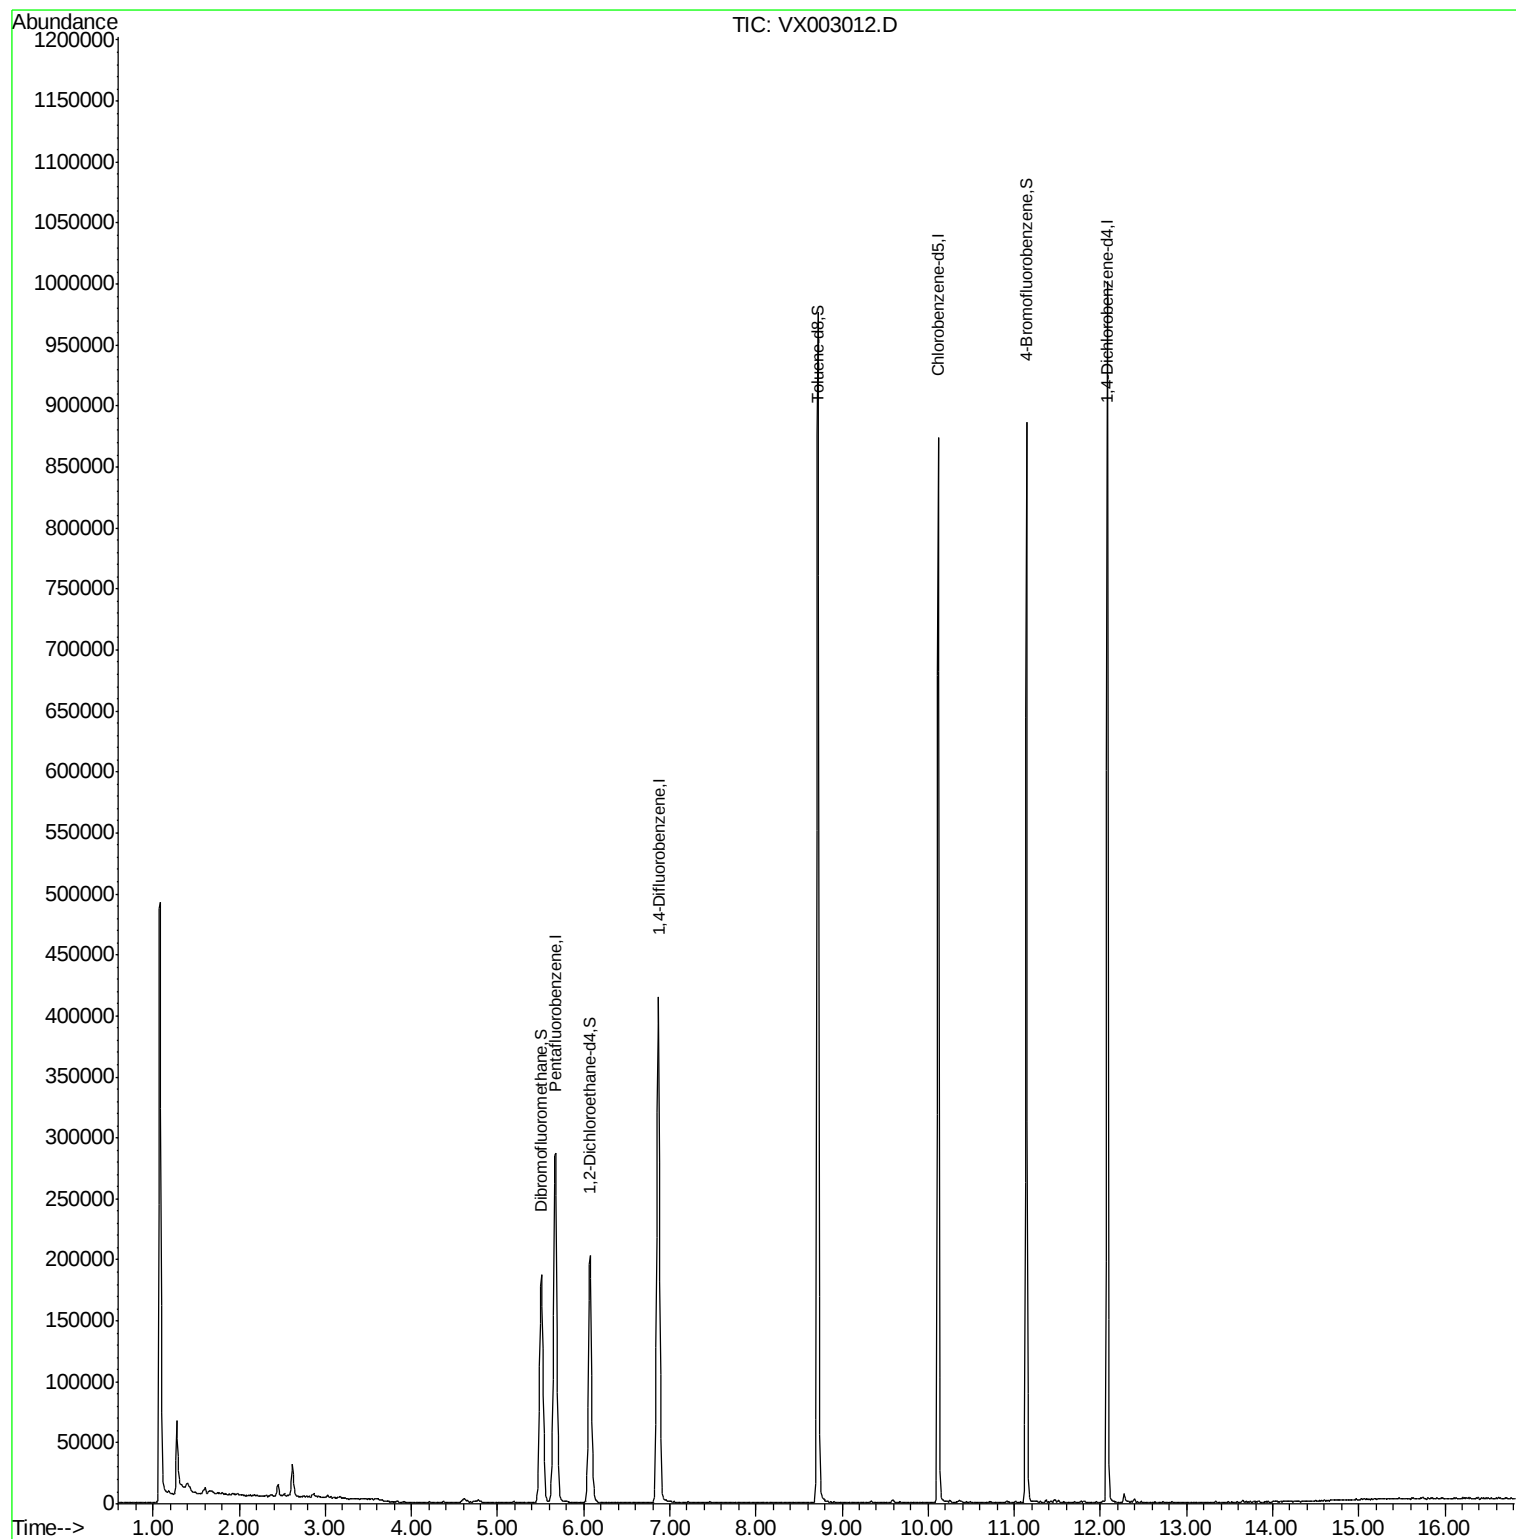

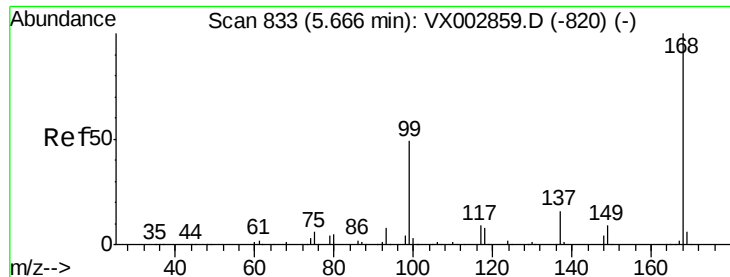

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 834

Delta R.T. 0.01 min

Lab File: VX003012.D

Acq: 29 Jun 2018 04:29

Instrument :

MSVOA_X

ClientSampleId :


ULMER-PARK-TRIP-BLANK-1-6-25-

Tot Ion:168 Resp: 293759

Ion Ratio Lower Upper

168 100

99 49.7 39.3 58.9

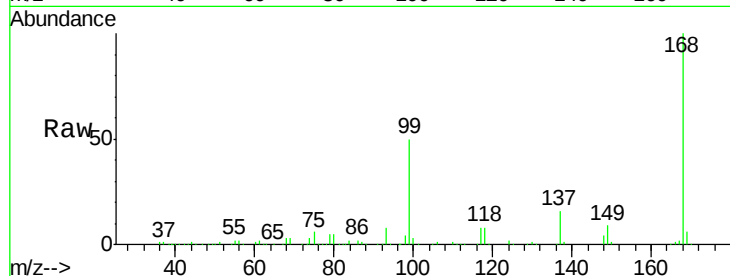

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

100000

80000



60000

40000

20000

0

Time-->

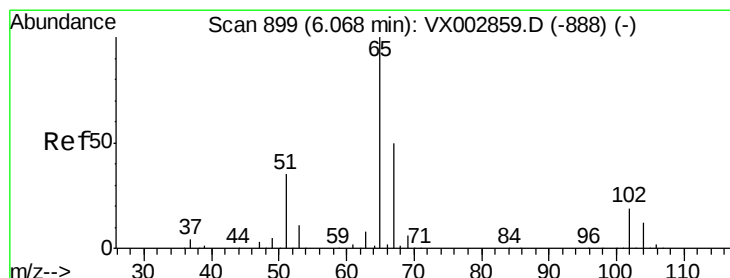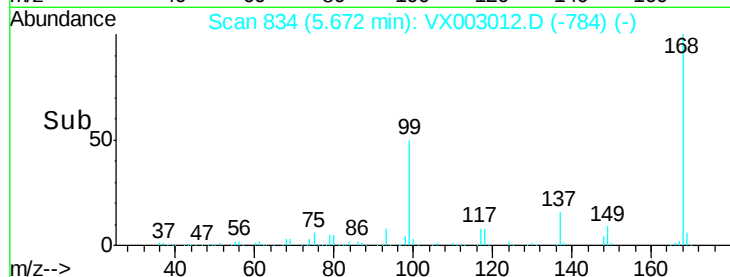

#33

1,2-Dichloroethane-d4

Concen: 47.64 ug/l

RT: 6.07 min Scan# 900

Delta R.T. 0.01 min

Lab File: VX003012.D


Acq: 29 Jun 2018 04:29

Tgt Ion: 65 Resp: 193418

Ion Ratio Lower Upper

65 100

67 51.5 0.0 102.6

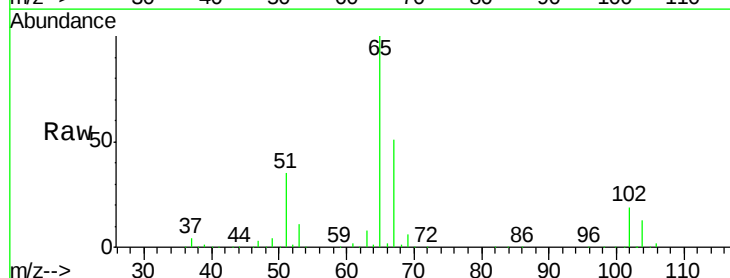

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07

80000


60000


40000

20000

0

Time-->

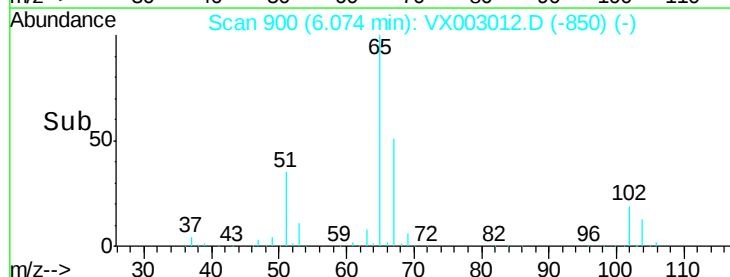

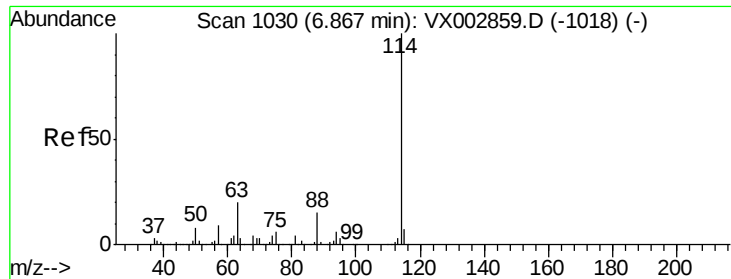

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.87 min Scan# 1030

Delta R.T. -0.00 min

Lab File: VX003012.D

Acq: 29 Jun 2018 04:29

Instrument :

MSVOA_X

ClientSampleId :

ULMER-PARK-TRIP-BLANK-1-6-25-


Tot Ion:114 Resp: 410765

Ion Ratio Lower Upper

114 100

63 19.7 0.0 41.4




88 15.4 0.0 30.0

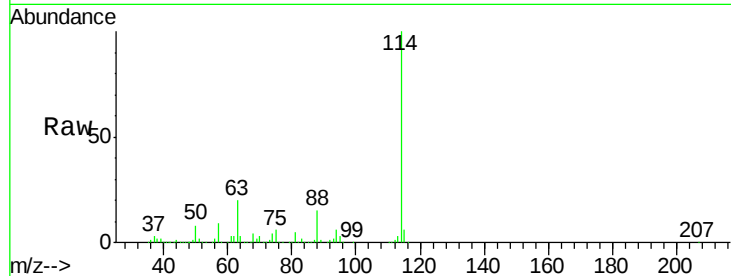

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

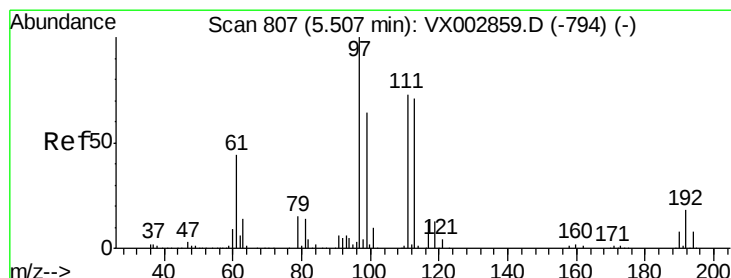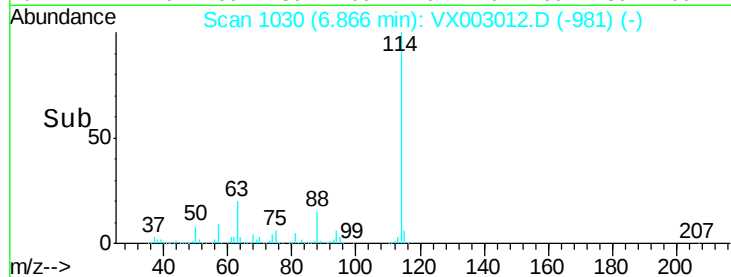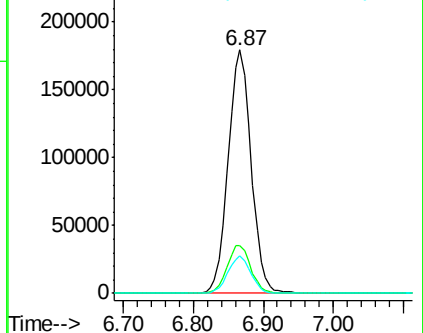

#35

Dibromofluoromethane

Concen: 48.06 ug/l

RT: 5.51 min Scan# 807

Delta R.T. -0.00 min

Lab File: VX003012.D

Acq: 29 Jun 2018 04:29


Tgt Ion:113 Resp: 156340

Ion Ratio Lower Upper

113 100

111 102.8 81.4 122.0



192 24.6 19.1 28.7

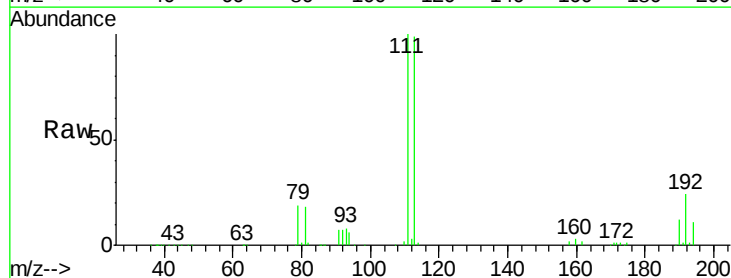


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

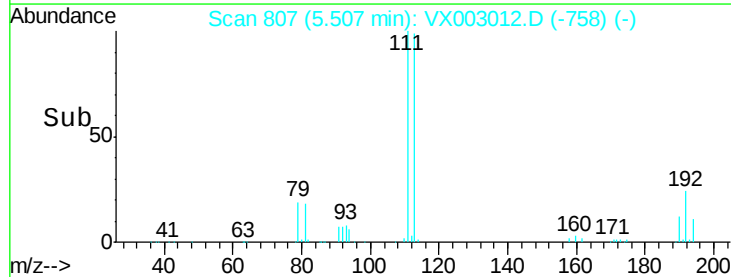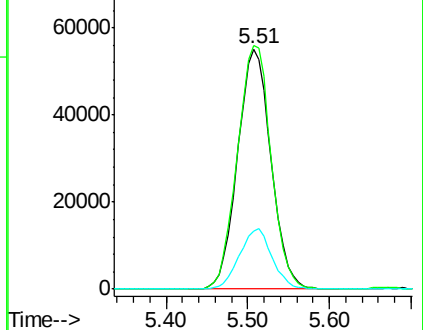

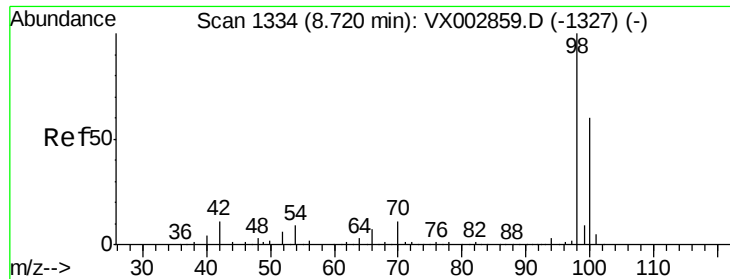

#50

Toluene-d8

Concen: 48.32 ug/l

RT: 8.72 min Scan# 1334

Delta R.T. 0.00 min

Lab File: VX003012.D

Acq: 29 Jun 2018 04:29

Instrument :

MSVOA_X

ClientSampleId :


ULMER-PARK-TRIP-BLANK-1-6-25-

Tot Ion: 98 Resp: 573944

Ion Ratio Lower Upper

98 100

100 64.2 50.9 76.3

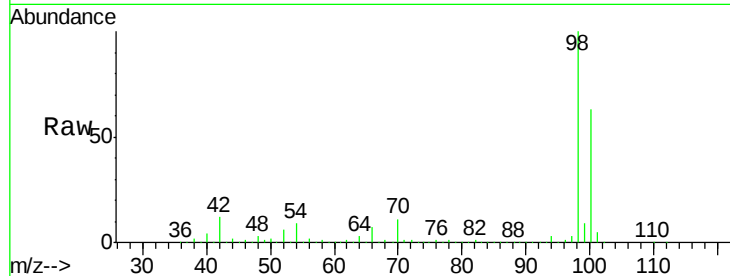

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

8.72

400000



300000

200000

100000

0

Time--> 8.60 8.70 8.80 8.90

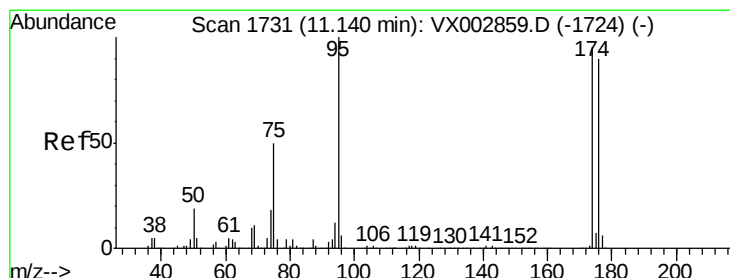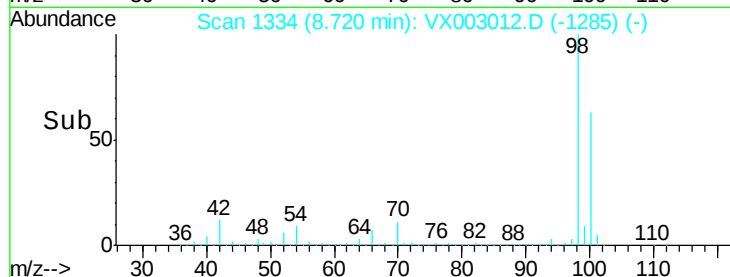

#62

4-Bromofluorobenzene

Concen: 44.43 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.00 min

Lab File: VX003012.D

Acq: 29 Jun 2018 04:29


Tgt Ion: 95 Resp: 203520

Ion Ratio Lower Upper

95 100

174 97.3 0.0 187.4

176 93.9 0.0 181.0

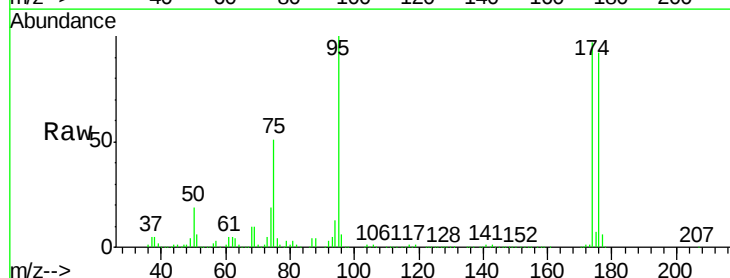

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

11.14

200000


150000


100000

50000

0

Time--> 11.10 11.20

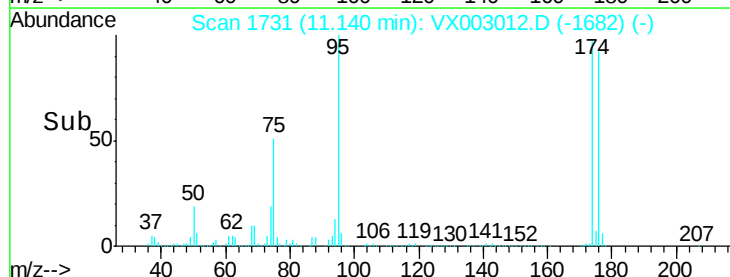


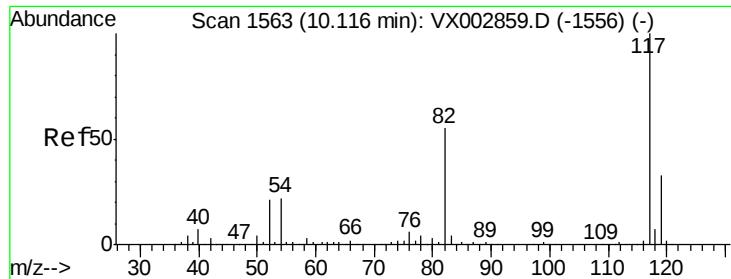




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1563
Delta R.T. -0.00 min
Lab File: VX003012.D
Acq: 29 Jun 2018 04:29

Instrument :
MSVOA_X
ClientSampleId :
ULMER-PARK-TRIP-BLANK-1-6-25-

Tot Ion:117 Resp: 380005
Ion Ratio Lower Upper
117 100
82 53.2 45.0 67.4
119 32.2 25.8 38.6

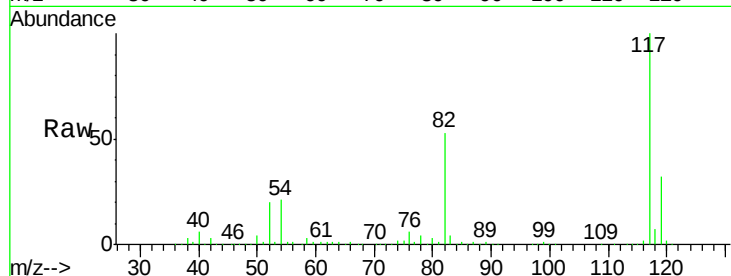


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

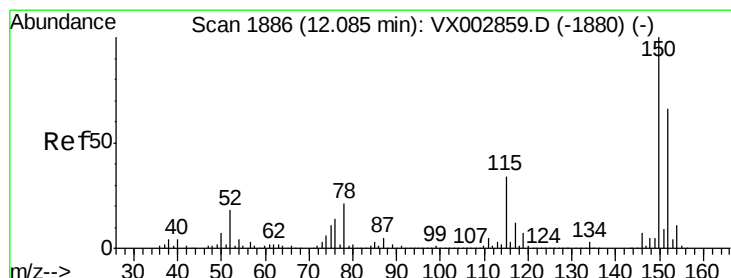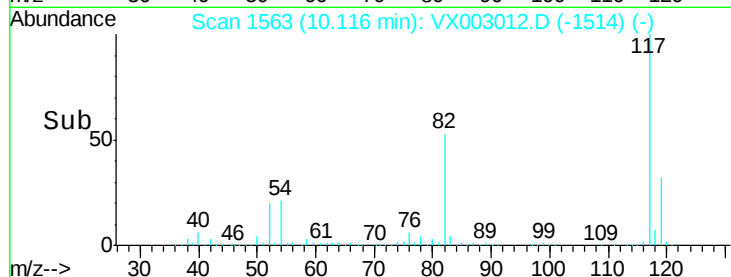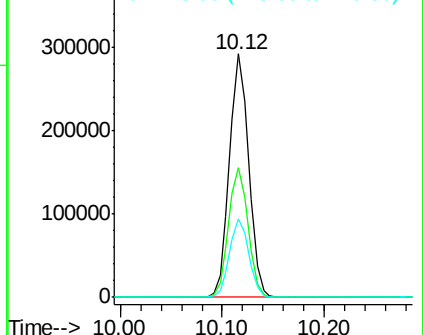

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.09 min Scan# 1886
Delta R.T. -0.00 min
Lab File: VX003012.D
Acq: 29 Jun 2018 04:29

Tgt Ion:152 Resp: 217128
Ion Ratio Lower Upper
152 100
115 54.8 40.1 120.2
150 154.7 0.0 347.2

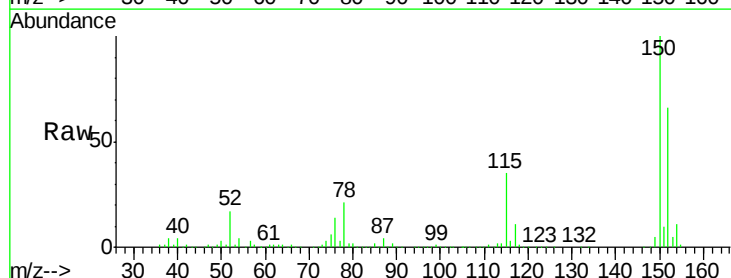

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

