


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX062818\
Data File : VX002977.D
Acq On : 28 Jun 2018 10:28
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X061818W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Mon Jun 18 15:18:02 2018

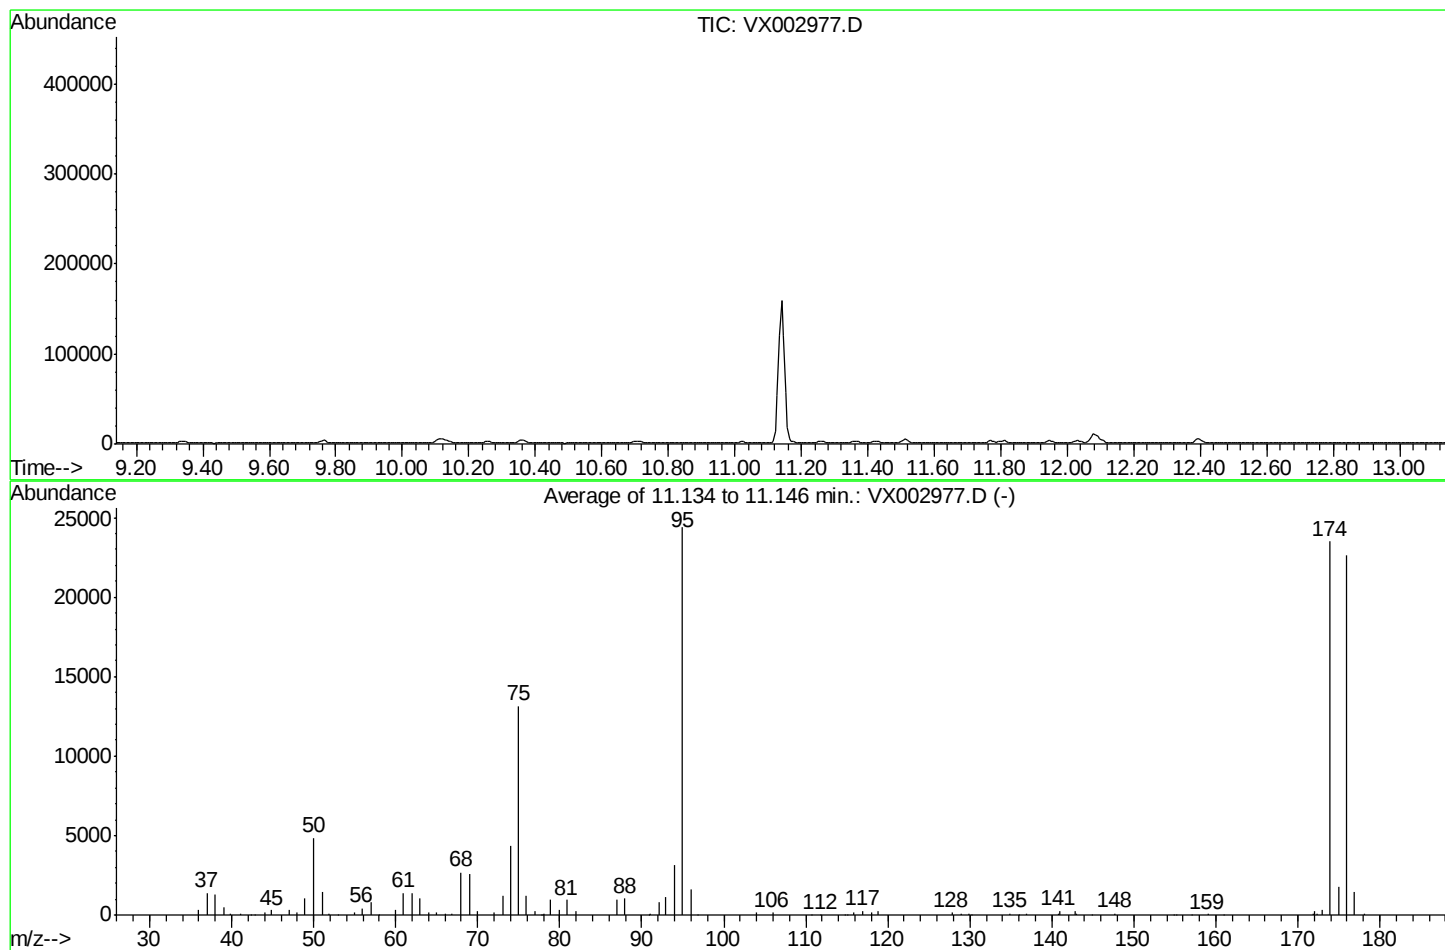

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	4848	PASS
75	95	30	60	53.9	13149	PASS
95	95	100	100	100.0	24389	PASS
96	95	5	9	6.8	1650	PASS
173	174	0.00	2	1.3	309	PASS
174	95	50	100	96.3	23488	PASS
175	174	5	9	7.7	1813	PASS
176	174	95	101	96.4	22645	PASS
177	176	5	9	6.4	1450	PASS