


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062818\
Data File : VX003006.D
Acq On : 29 Jun 2018 00:58
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Title : SW846 8260
Last Update : Mon Jun 25 14:38:05 2018

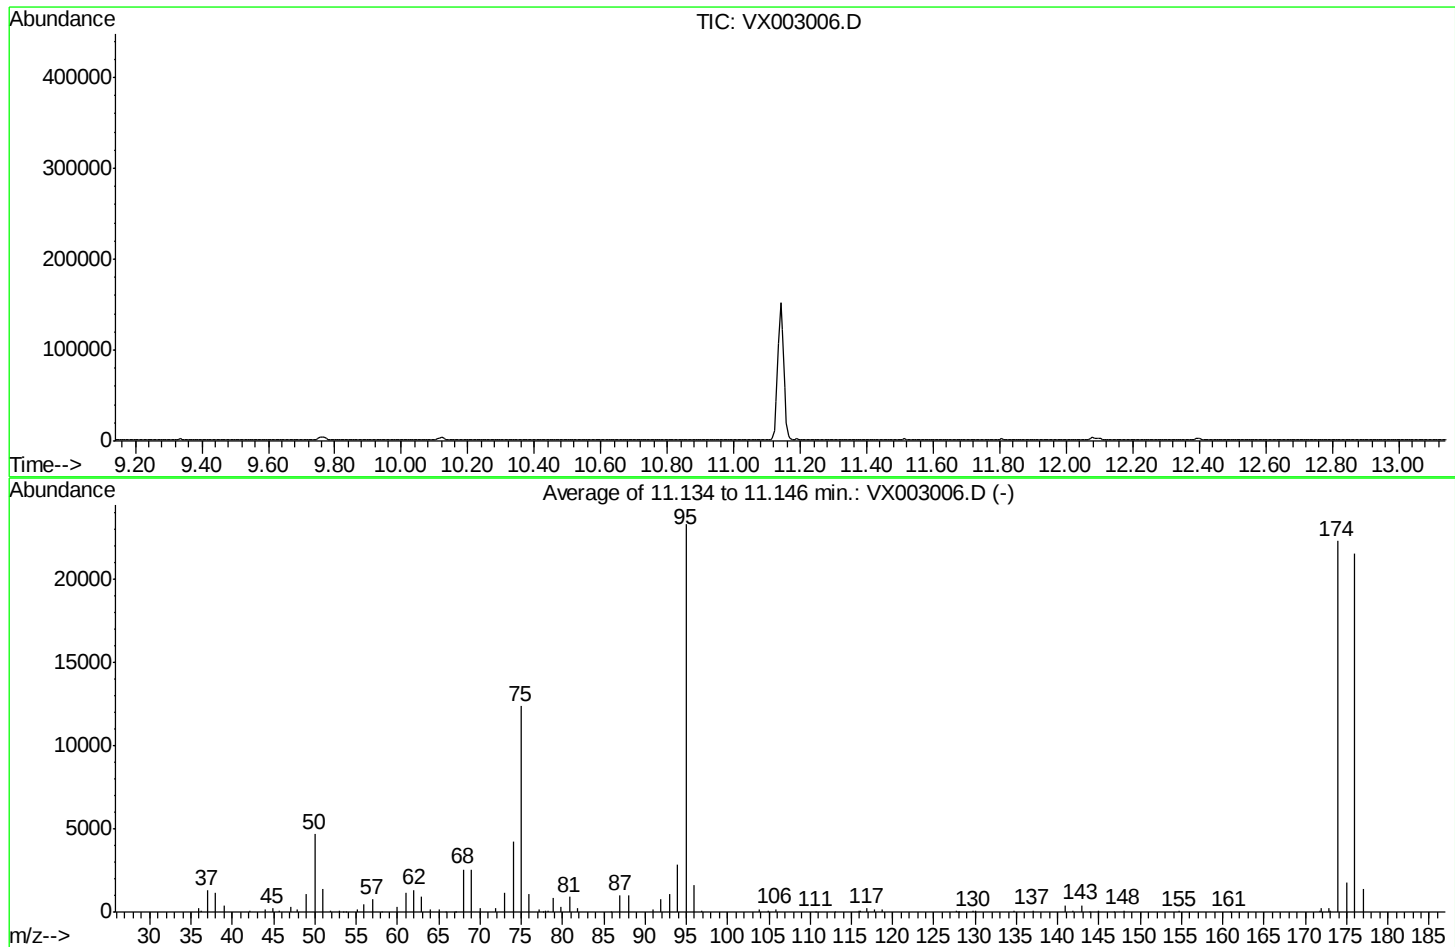

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	4669	PASS
75	95	30	60	53.0	12368	PASS
95	95	100	100	100.0	23317	PASS
96	95	5	9	6.8	1586	PASS
173	174	0.00	2	1.0	222	PASS
174	95	50	100	95.7	22324	PASS
175	174	5	9	8.0	1791	PASS
176	174	95	101	96.6	21566	PASS
177	176	5	9	6.5	1410	PASS