

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062819\
 Data File : VX010535.D
 Acq On : 28 Jun 2019 14:38
 Operator : JC/SP
 Sample : K3565-10
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FL-0575

Quant Time: Jun 29 04:38:21 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 20 03:31:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	249872	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	387470	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	344694	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	157420	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.06	65	120417	51.40	ug/l	0.00
Spiked Amount			Recovery	=	102.80%	
35) Dibromofluoromethane	5.50	113	116300	49.06	ug/l	0.00
Spiked Amount			Recovery	=	98.12%	
50) Toluene-d8	8.71	98	450563	49.68	ug/l	0.00
Spiked Amount			Recovery	=	99.36%	
62) 4-Bromofluorobenzene	11.13	95	148738	45.42	ug/l	0.00
Spiked Amount			Recovery	=	90.84%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.33	50	789	0.390	ug/l #	76
5) Bromomethane	1.65	94	655	0.607	ug/l #	43
6) Chloroethane	1.73	64	660	0.505	ug/l #	47
10) Methyl Iodide	2.51	142	624	0.205	ug/l	91
11) Tert butyl alcohol	3.02	59	2675	4.364	ug/l #	83
13) Acrolein	2.29	56	324	0.797	ug/l #	56
16) Acetone	2.45	43	1219	1.038	ug/l	90
25) 2-Butanone	4.68	43	368	0.214	ug/l #	46
31) Cyclohexane	5.58	56	3561	1.052	ug/l	84
36) 1,1-Dichloropropene	5.67	75	15882	5.158	ug/l #	48
38) Carbon Tetrachloride	5.67	117	22261	6.677	ug/l #	15
39) Methylcyclohexane	7.46	83	8376	2.070	ug/l	96
49) 1,4-Dioxane	7.86	88	19	0.271	ug/l #	1
55) 1,1,2-Trichloroethane	9.16	97	845	0.324	ug/l #	23
67) Ethyl Benzene	10.25	91	7716	0.653	ug/l	99
68) m/p-Xylenes	10.36	106	5531	1.208	ug/l	98
73) Isopropylbenzene	11.02	105	9828	0.921	ug/l	99
76) 1,2,3-Trichloropropane	11.13	75	71806	25.032	ug/l #	33
78) n-propylbenzene	11.36	91	7785	0.664	ug/l	98
80) 1,3,5-Trimethylbenzene	11.45	105	5638	0.641	ug/l	75
81) trans-1,4-Dichloro-2-buten	11.13	75	71806	58.396	ug/l #	16
84) 1,2,4-Trimethylbenzene	11.80	105	30988	3.506	ug/l	99
85) sec-Butylbenzene	11.94	105	2491	0.240	ug/l #	70
90) Hexachloroethane	12.58	117	334	0.201	ug/l #	5
95) Naphthalene	13.83	128	10203	0.926	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062819\
Data File : VX010535.D
Acq On : 28 Jun 2019 14:38
Operator : JC/SP
Sample : K3565-10
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0575

Quant Time: Jun 29 04:38:21 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260
QLast Update : Thu Jun 20 03:31:56 2019
Response via : Initial Calibration

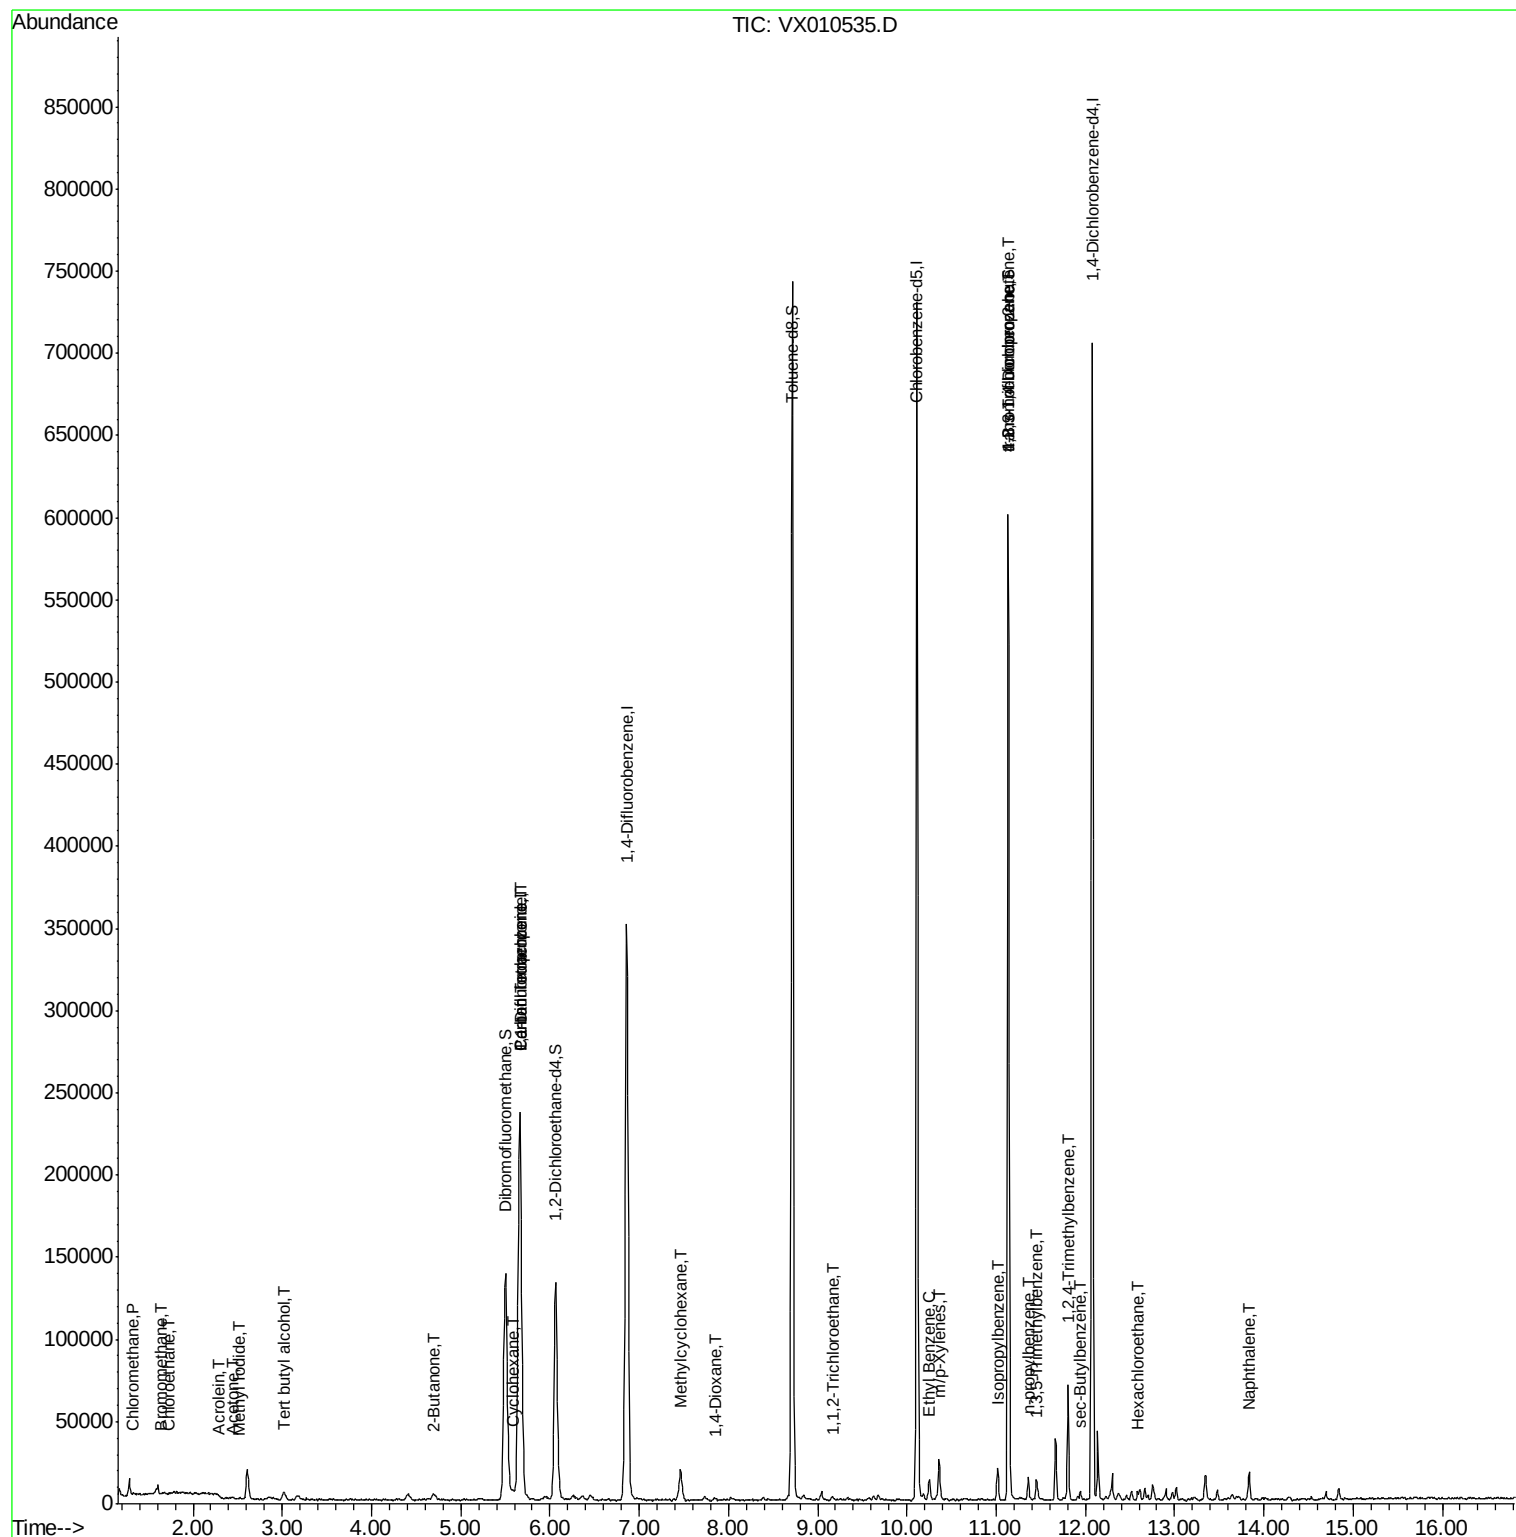

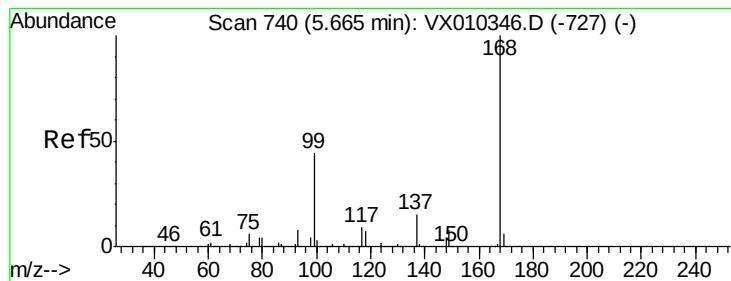

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.01 min

Lab File: VX010535.D

Acq: 28 Jun 2019 14:38

Instrument :

MSVOA_X

ClientSampleId :


FL-0575

Tot Ion:168 Resp: 249872

Ion Ratio Lower Upper

168 100

99 46.6 35.5 53.3



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.66

80000



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80

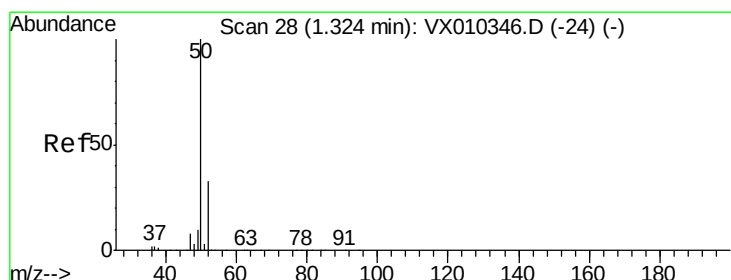

#3

Chloromethane

Concen: 0.390 ug/l

RT: 1.33 min Scan# 29

Delta R.T. 0.01 min

Lab File: VX010535.D


Acq: 28 Jun 2019 14:38

Tgt Ion: 50 Resp: 789

Ion Ratio Lower Upper

50 100

52 46.7 26.5 39.7#



Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

1.33

500

400


300


200

100

0

Time--> 1.30 1.35





#5

Bromomethane

Concen: 0.607 ug/l

RT: 1.65 min Scan# 81

Delta R.T. 0.01 min

Lab File: VX010535.D

Acq: 28 Jun 2019 14:38

Instrument :

MSVOA_X

ClientSampleId :





FL-0575

Tot Ion: 94 Resp: 655

Ion Ratio Lower Upper

94 100

96 39.3 75.5 113.3#

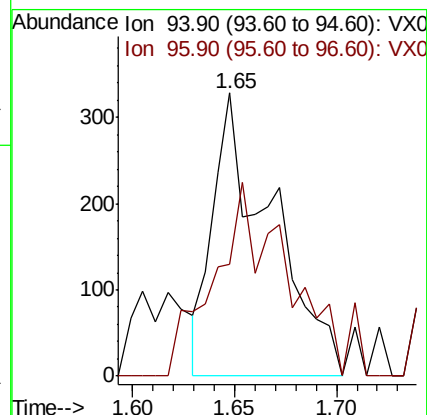

#6

Chloroethane

Concen: 0.505 ug/l

RT: 1.73 min Scan# 94

Delta R.T. 0.01 min

Lab File: VX010535.D




Acq: 28 Jun 2019 14:38


Tgt Ion: 64 Resp: 660

Ion Ratio Lower Upper

64 100

66 3.2 26.6 40.0#

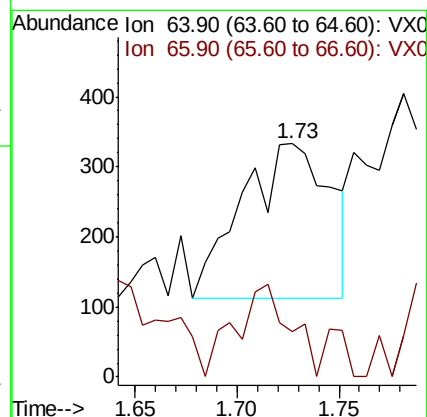







#10
Methvl Iodide
Concen: 0.205 ug/l
RT: 2.51 min Scan# 223
Delta R.T. 0.01 min
Lab File: VX010535.D
Acq: 28 Jun 2019 14:38

Instrument :
MSVOA_X
ClientSampleId :
FL-0575

Tot Ion:142 Resp: 624
Ion Ratio Lower Upper
142 100
127 45.2 31.1 46.7
141 11.5 11.2 16.8

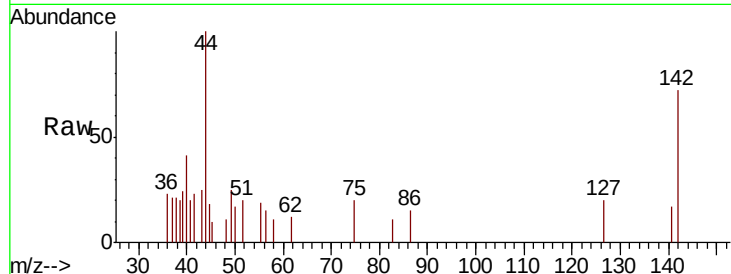


Abundance Ion 141.80 (141.50 to 142.50): V
Ion 126.80 (126.50 to 127.50): V
Ion 140.80 (140.50 to 141.50): V


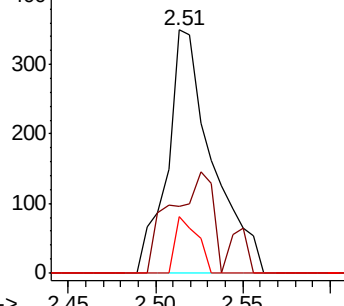



#11
Tert butyl alcohol
Concen: 4.364 ug/l
RT: 3.02 min Scan# 306
Delta R.T. -0.03 min
Lab File: VX010535.D
Acq: 28 Jun 2019 14:38

Tgt Ion: 59 Resp: 2675
Ion Ratio Lower Upper
59 100
57 3.5 7.7 11.5#



Abundance Ion 59.00 (58.70 to 59.70): VX0
Ion 57.00 (56.70 to 57.70): VX0

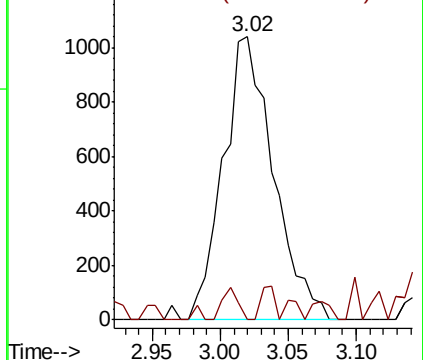



#13

Acrolein

Concen: 0.797 ug/l

RT: 2.29 min Scan# 187

Delta R.T. 0.00 min

Lab File: VX010535.D

Acq: 28 Jun 2019 14:38

Instrument :

MSVOA_X

ClientSampleId :


FL-0575

Tot Ion: 56 Resp: 324

Ion Ratio Lower Upper


56 100

55 34.6 56.9 85.3#


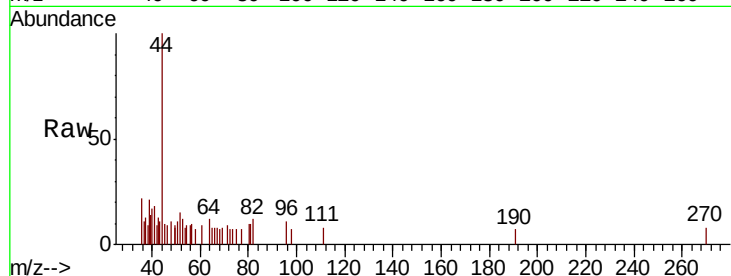


Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

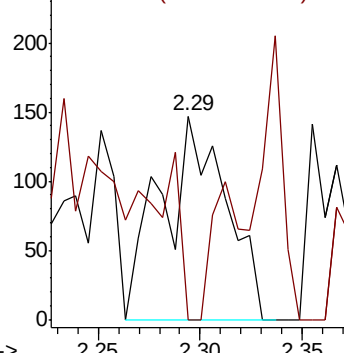

Time-->



#16

Acetone

Concen: 1.038 ug/l

RT: 2.45 min Scan# 213

Delta R.T. 0.01 min

Lab File: VX010535.D


Acq: 28 Jun 2019 14:38

Tgt Ion: 43 Resp: 1219

Ion Ratio Lower Upper


43 100

58 42.0 28.9 43.3





Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

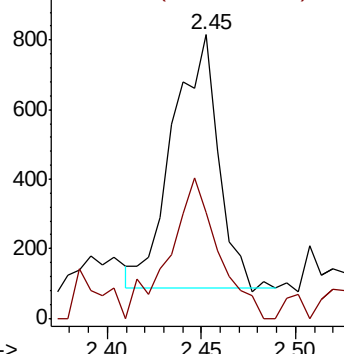

Time-->



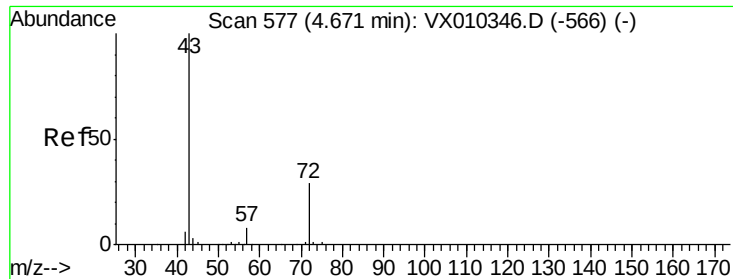

#25

2-Butanone

Concen: 0.214 ug/l

RT: 4.68 min Scan# 579

Delta R.T. 0.01 min

Lab File: VX010535.D

Acq: 28 Jun 2019 14:38

Instrument :

MSVOA_X

ClientSampled :


FL-0575

Tot Ion: 43 Resp: 368




Ion Ratio Lower Upper

43 100

72 0.0 23.3 34.9#

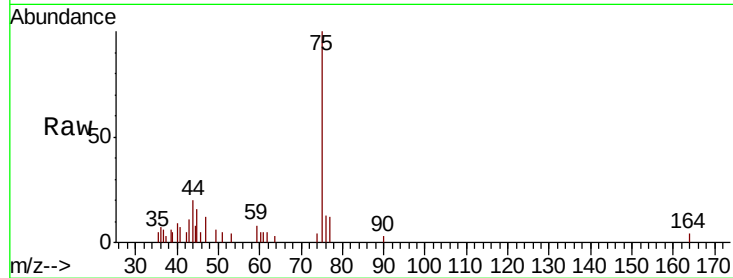

Abundance Ion 43.00 (42.70 to 43.70): VX0

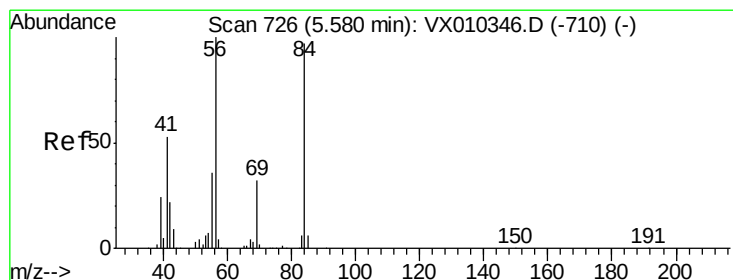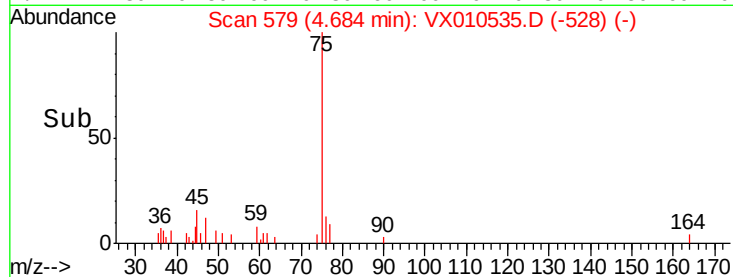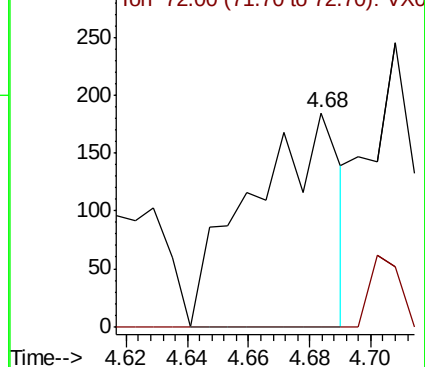

#31

Cyclohexane

Concen: 1.052 ug/l

RT: 5.58 min Scan# 726

Delta R.T. 0.00 min

Lab File: VX010535.D

Acq: 28 Jun 2019 14:38


Tgt Ion: 56 Resp: 3561

Ion Ratio Lower Upper



56 100


69 27.3 25.9 38.9

84 79.1 78.0 117.0

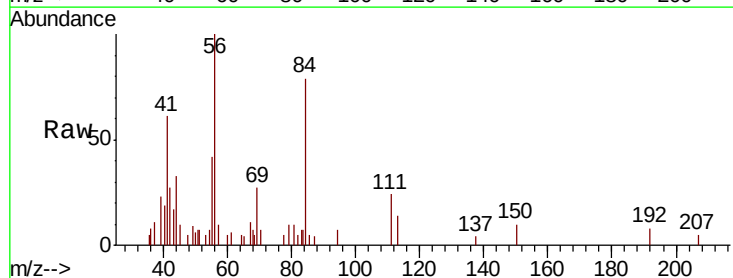

Abundance Ion 56.00 (55.70 to 56.70): VX0



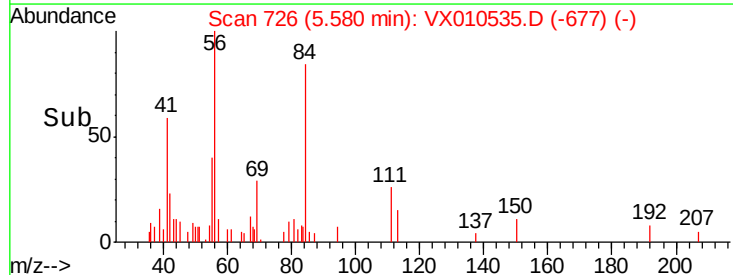
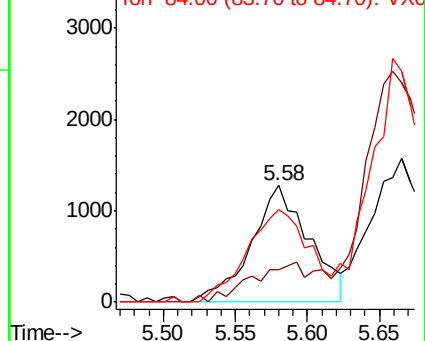


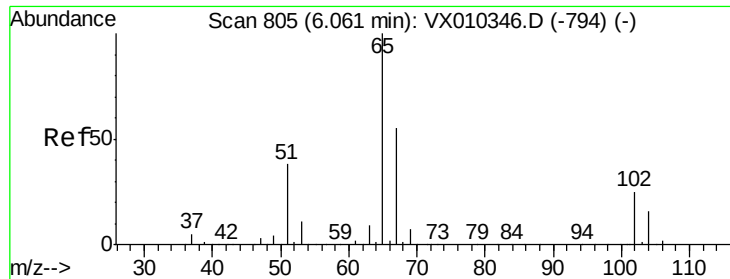

#33
 1,2-Dichloroethane-d4
 Concen: 51.399 ug/l
 RT: 6.06 min Scan# 805
 Delta R.T. 0.00 min
 Lab File: VX010535.D
 Acq: 28 Jun 2019 14:38




Instrument :
 MSVOA_X
 ClientSampled :
 FL-0575


Tot Ion: 65 Resp: 120417
 Ion Ratio Lower Upper
 65 100
 67 54.4 0.0 110.2

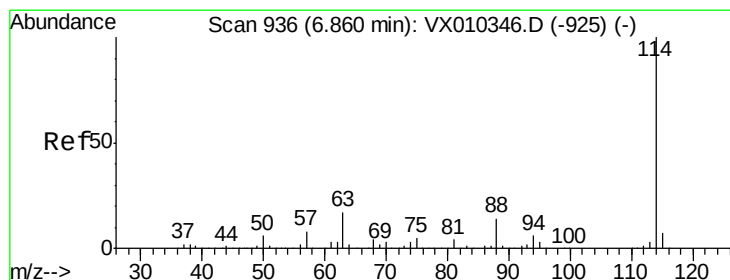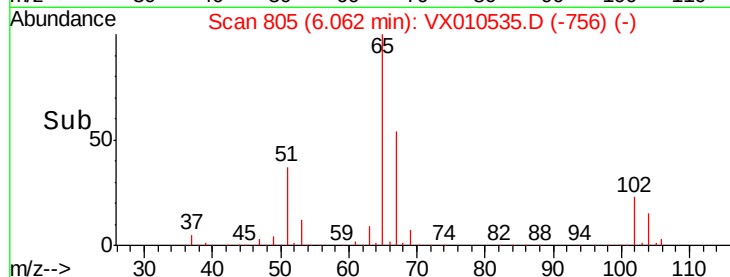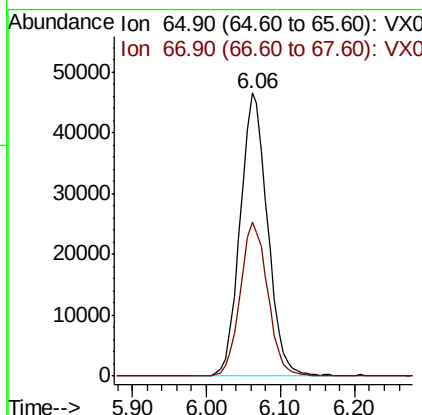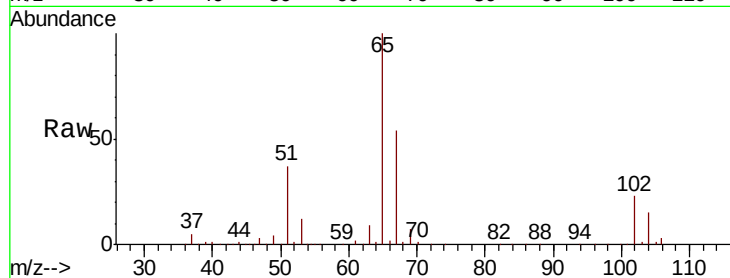

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. 0.00 min
 Lab File: VX010535.D
 Acq: 28 Jun 2019 14:38

Tgt Ion: 114 Resp: 387470
 Ion Ratio Lower Upper
 114 100
 63 16.7 0.0 33.8
 88 14.1 0.0 27.6

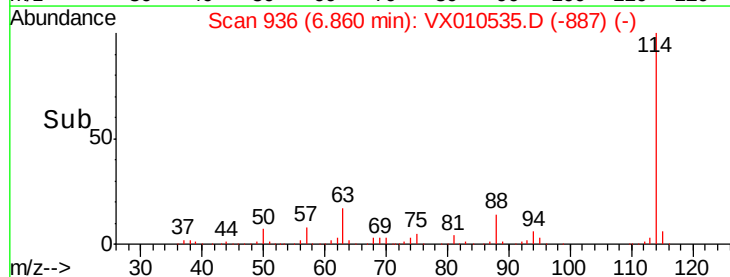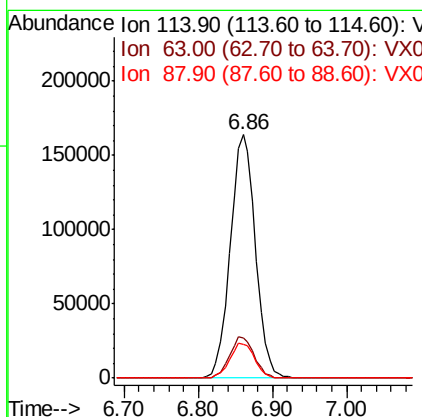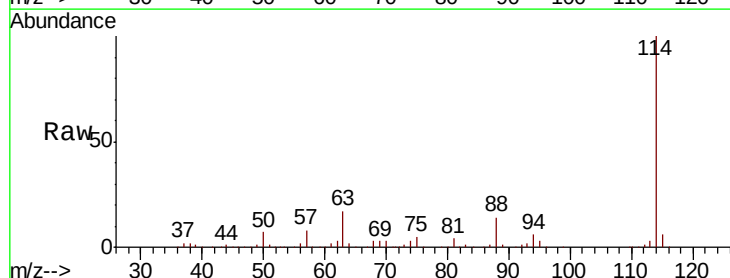

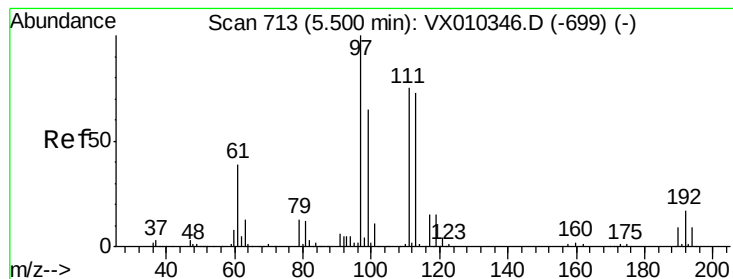

#35

Dibromofluoromethane

Concen: 49.058 ug/l

RT: 5.50 min Scan# 713

Delta R.T. 0.00 min

Lab File: VX010535.D

Acq: 28 Jun 2019 14:38

Instrument :

MSVOA_X

ClientSampled :

FL-0575





Tot Ion:113 Resp: 116300

Ion Ratio Lower Upper

113 100

111 101.2 81.2 121.8

192 22.6 18.6 27.8

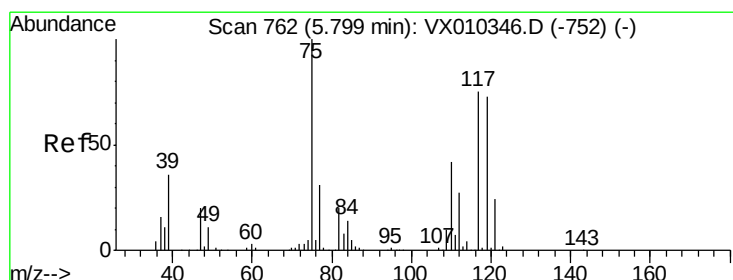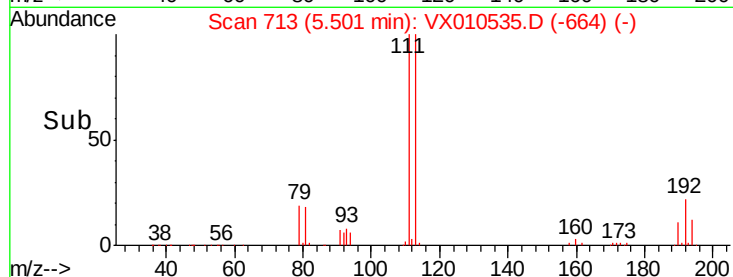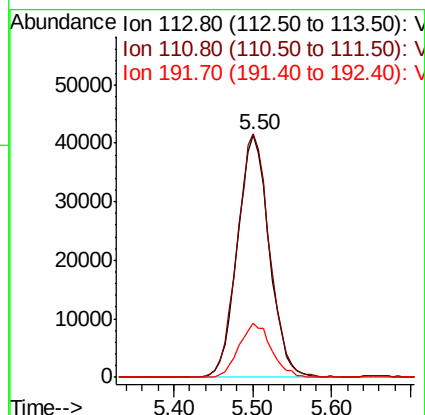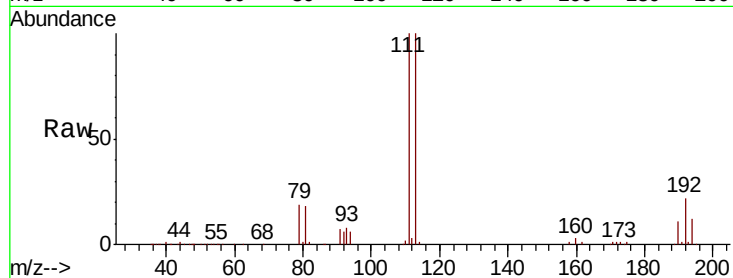

#36

1,1-Dichloropropene

Concen: 5.158 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.13 min

Lab File: VX010535.D

Acq: 28 Jun 2019 14:38




Tgt Ion: 75 Resp: 15882


Ion Ratio Lower Upper

75 100

110 10.4 20.8 62.2#

77 0.5 25.4 38.0#

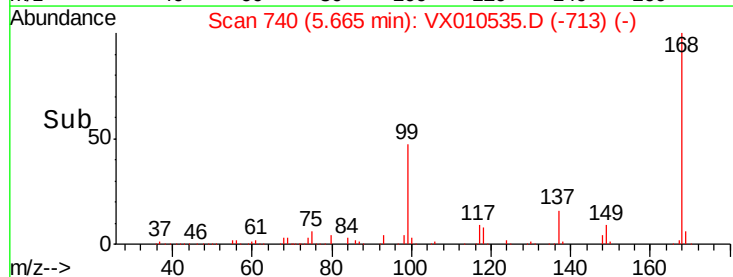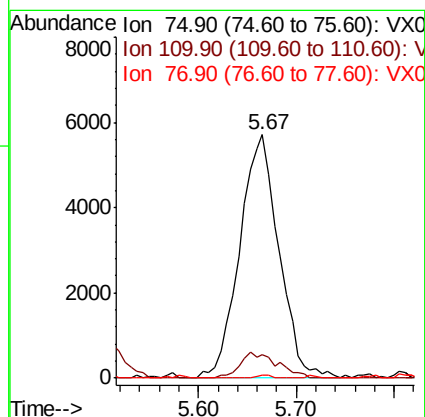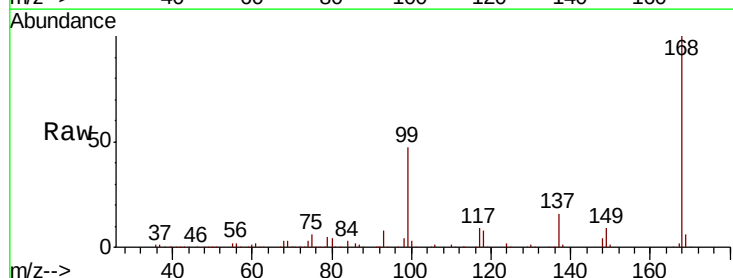


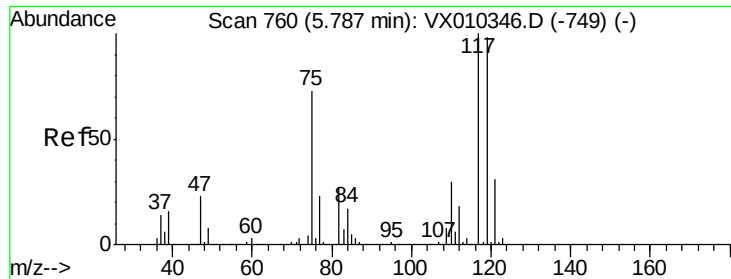




#38
Carbon Tetrachloride
Concen: 6.677 ug/l
RT: 5.67 min Scan# 740
Delta R.T. -0.12 min
Lab File: VX010535.D
Acq: 28 Jun 2019 14:38

Instrument :
MSVOA_X
ClientSampled :
FL-0575

Tot Ion:117 Resp: 22261
Ion Ratio Lower Upper
117 100
119 5.1 78.2 117.4#
121 0.0 24.7 37.1#




Abundance Ion 116.80 (116.50 to 117.50): V
Ion 118.80 (118.50 to 119.50): V
Ion 120.80 (120.50 to 121.50): V


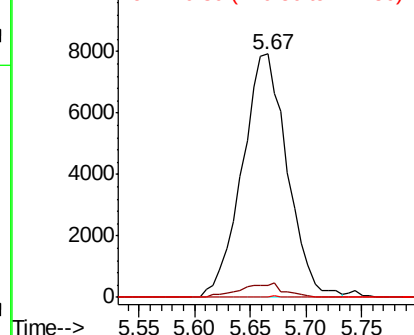



#39
Methylcyclohexane
Concen: 2.070 ug/l
RT: 7.46 min Scan# 1035
Delta R.T. 0.00 min
Lab File: VX010535.D
Acq: 28 Jun 2019 14:38

Tgt Ion: 83 Resp: 8376
Ion Ratio Lower Upper
83 100
55 64.5 53.0 79.6
98 43.6 37.8 56.8



Abundance Ion 83.00 (82.70 to 83.70): VX0
Ion 55.00 (54.70 to 55.70): VX0
Ion 98.00 (97.70 to 98.70): VX0

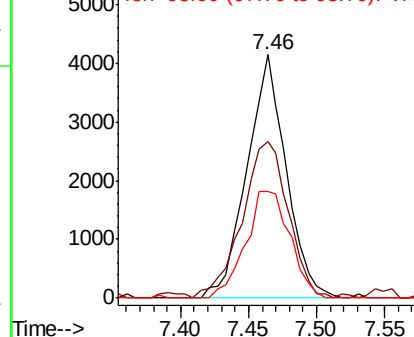



#49

1,4-Dioxane

Concen: 0.271 ug/l

RT: 7.86 min Scan# 1100

Delta R.T. 0.12 min

Lab File: VX010535.D

Acq: 28 Jun 2019 14:38

Instrument :

MSVOA_X

ClientSampled :

FL-0575


Tot Ion: 88 Resp: 19

Ion Ratio Lower Upper

88 100

43 2968.4 20.2 30.2#




58 157.9 49.5 74.3#

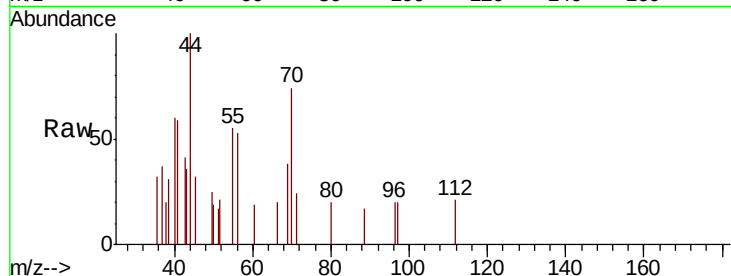

Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

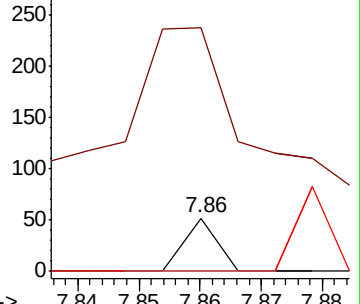

#50

Toluene-d8

Concen: 49.677 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX010535.D


Acq: 28 Jun 2019 14:38

Tgt Ion: 98 Resp: 450563

Ion Ratio Lower Upper



98 100


100 64.7 51.6 77.4



Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX0

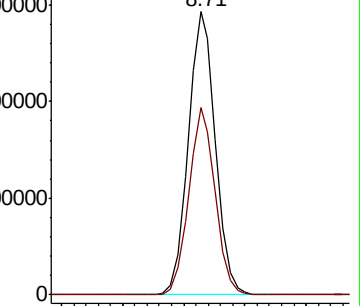

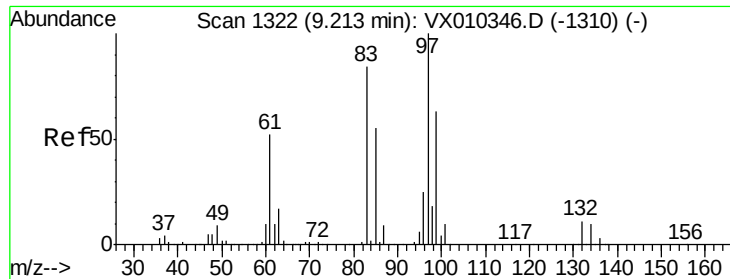

#55

1,1,2-Trichloroethane

Concen: 0.324 ug/l

RT: 9.16 min Scan# 1314

Delta R.T. -0.05 min

Lab File: VX010535.D

Acq: 28 Jun 2019 14:38

Instrument :

MSVOA_X

ClientSampleId :

FL-0575

Tot Ion: 97 Resp: 845


Ion Ratio Lower Upper

97 100

83 17.4 67.4 101.0#

85 0.0 43.8 65.8#

99 0.0 50.3 75.5#



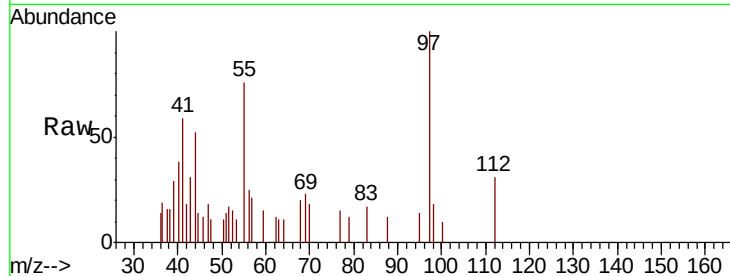


Abundance Ion 96.90 (96.60 to 97.60): VX0

Ion 82.90 (82.60 to 83.60): VX0

Ion 84.90 (84.60 to 85.60): VX0

Ion 98.90 (98.60 to 99.60): VX0

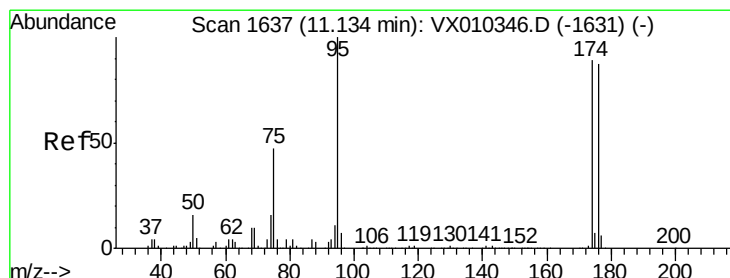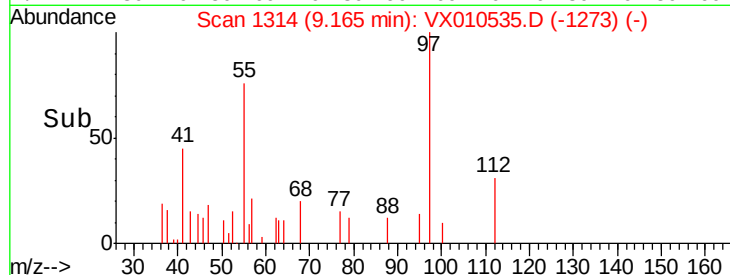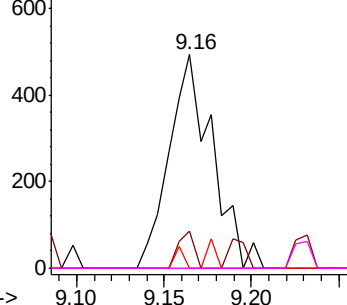

#62

4-Bromofluorobenzene

Concen: 45.424 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.00 min

Lab File: VX010535.D

Acq: 28 Jun 2019 14:38


Tgt Ion: 95 Resp: 148738

Ion Ratio Lower Upper

95 100

174 96.0 0.0 187.6



176 90.0 0.0 184.0

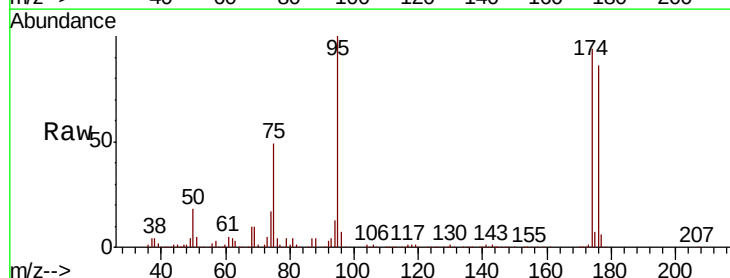


Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

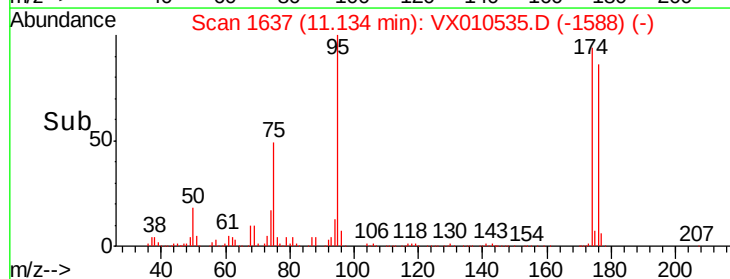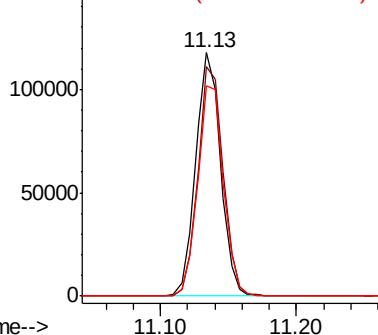


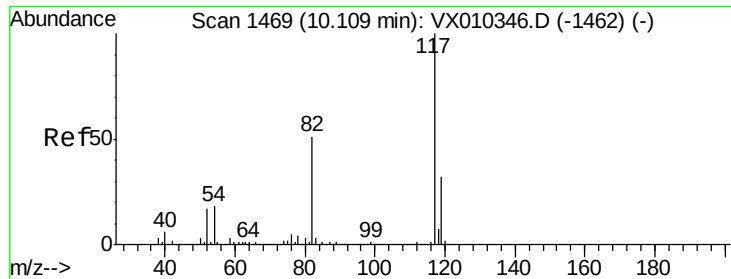




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. 0.00 min
Lab File: VX010535.D
Acq: 28 Jun 2019 14:38

Instrument :
MSVOA_X
ClientSampleId :
FL-0575

Tot Ion:117 Resp: 344694
Ion Ratio Lower Upper
117 100
82 51.0 41.2 61.8
119 32.6 25.5 38.3

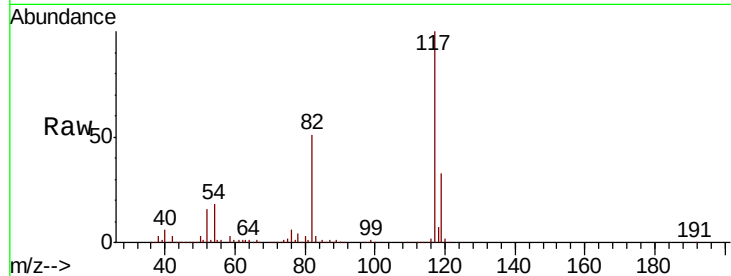


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

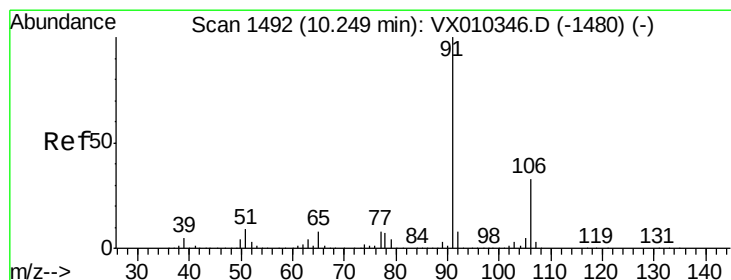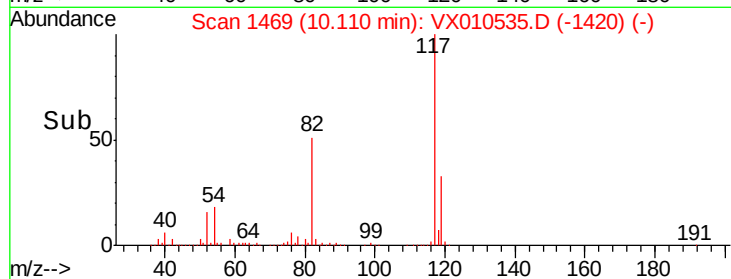
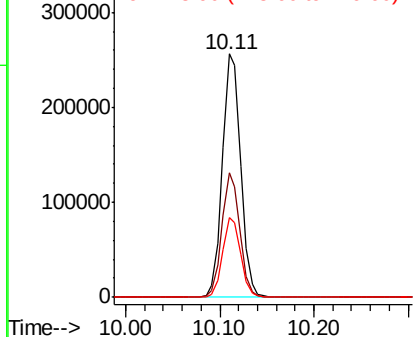



#67
Ethyl Benzene
Concen: 0.653 ug/l
RT: 10.25 min Scan# 1492
Delta R.T. 0.00 min
Lab File: VX010535.D
Acq: 28 Jun 2019 14:38

Tgt Ion: 91 Resp: 7716
Ion Ratio Lower Upper
91 100
106 32.0 26.2 39.2



Abundance Ion 91.00 (90.70 to 91.70): VX0
Ion 106.00 (105.70 to 106.70): V

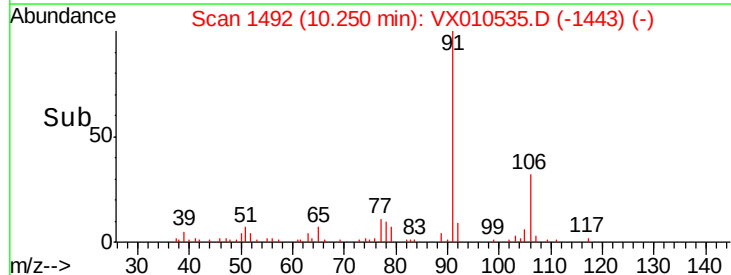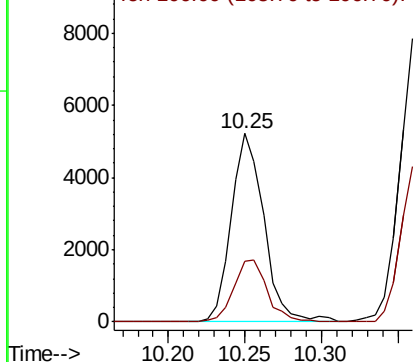


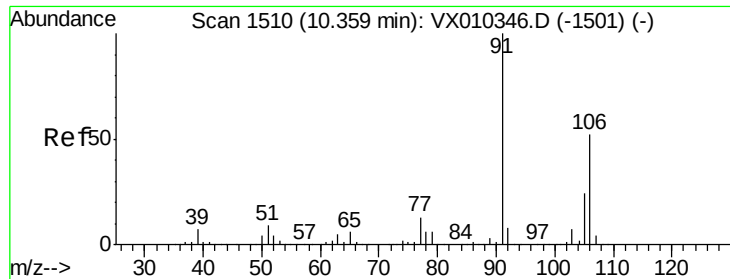




#68
m/p-Xvlenes
Concen: 1.208 ug/l
RT: 10.36 min Scan# 1510
Delta R.T. 0.00 min
Lab File: VX010535.D
Acq: 28 Jun 2019 14:38

Instrument :
MSVOA_X
ClientSampleId :
FL-0575

Tot Ion:106 Resp: 5531
Ion Ratio Lower Upper
106 100
91 191.4 155.3 232.9

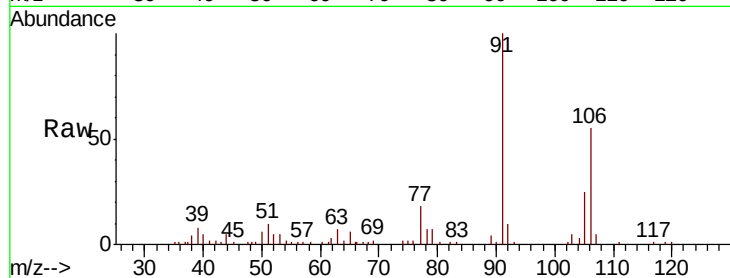


Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VX0

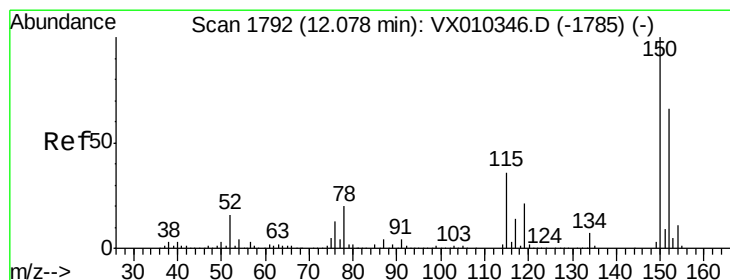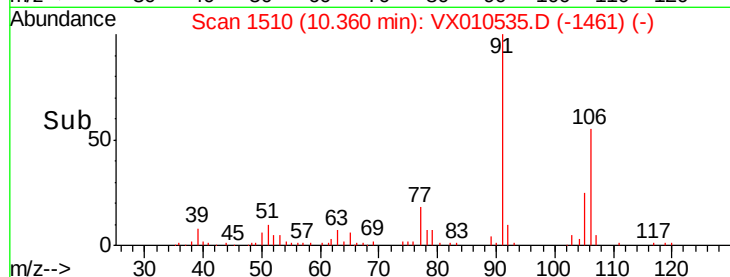
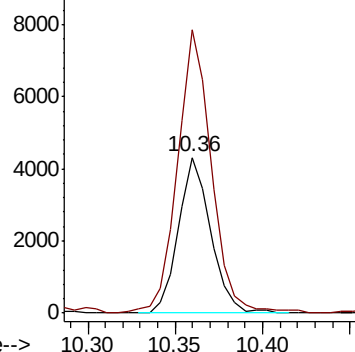



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. 0.00 min
Lab File: VX010535.D
Acq: 28 Jun 2019 14:38

Tgt Ion:152 Resp: 157420
Ion Ratio Lower Upper
152 100
115 54.7 38.6 115.7
150 156.2 0.0 347.4

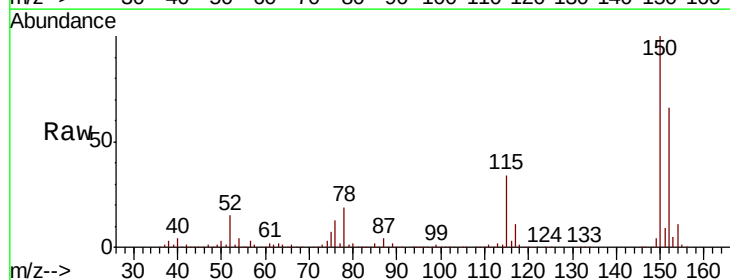

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

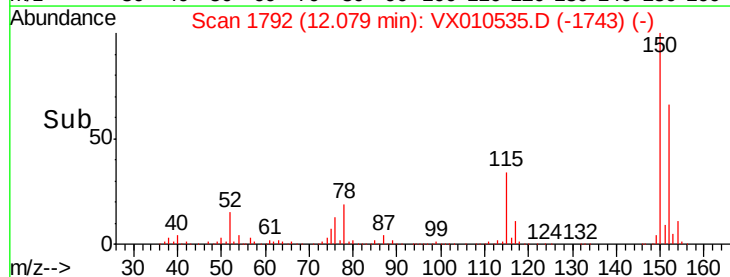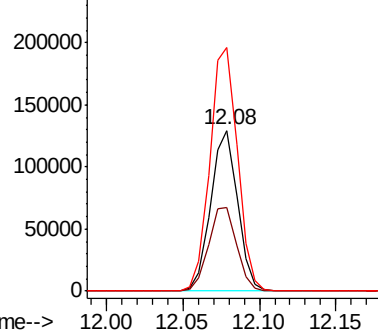

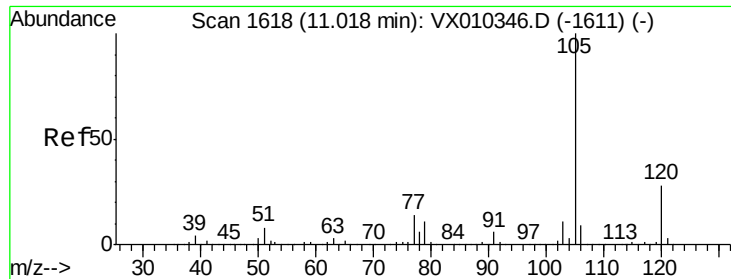

#73

Isopropylbenzene

Concen: 0.921 ug/l

RT: 11.02 min Scan# 1618

Delta R.T. 0.00 min

Lab File: VX010535.D

Acq: 28 Jun 2019 14:38

Instrument :

MSVOA_X

ClientSampleId :


FL-0575

Tot Ion:105 Resp: 9828

Ion Ratio Lower Upper




105 100

120 28.0 14.1 42.4

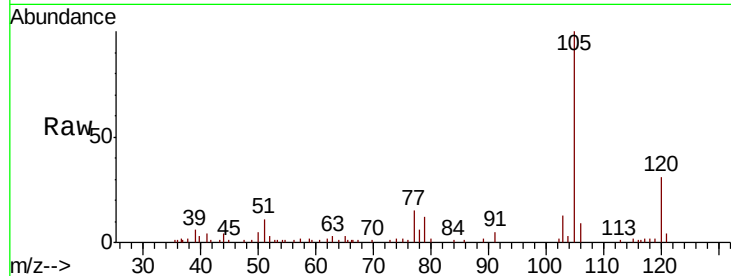

Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

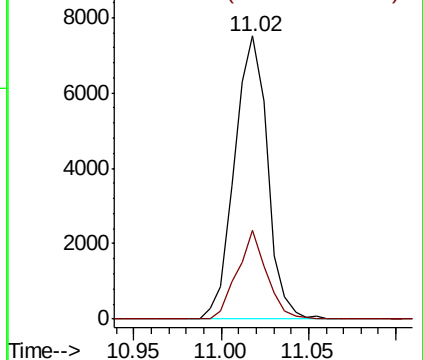

#76

1,2,3-Trichloropropane

Concen: 25.032 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.16 min

Lab File: VX010535.D


Acq: 28 Jun 2019 14:38

Tgt Ion: 75 Resp: 71806

Ion Ratio Lower Upper



75 100


77 1.3 22.6 67.8#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

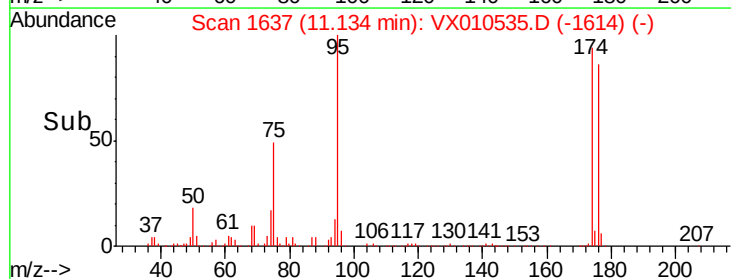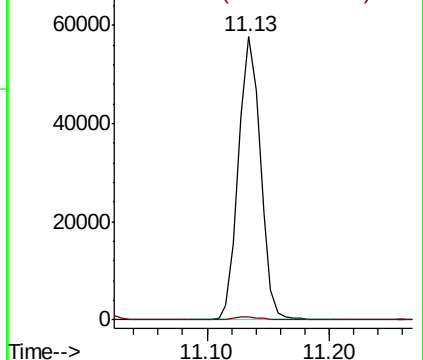



#78

n-propylbenzene

Concen: 0.664 ug/l

RT: 11.36 min Scan# 1674

Delta R.T. 0.00 min

Lab File: VX010535.D

Acq: 28 Jun 2019 14:38

Instrument :

MSVOA_X

ClientSampleId :


FL-0575

Tot Ion: 91 Resp: 7785

Ion Ratio Lower Upper




91 100

120 24.1 12.4 37.4



Abundance Ion 91.00 (90.70 to 91.70): VX010535.D (-1669) (-)

Ion 120.00 (119.70 to 120.70): VX010535.D (-1669) (-)

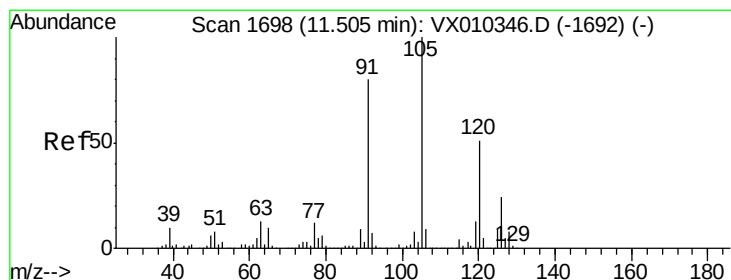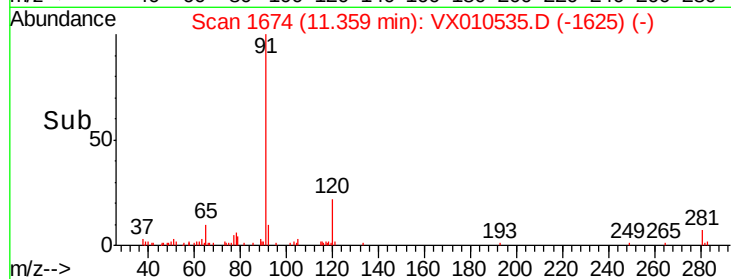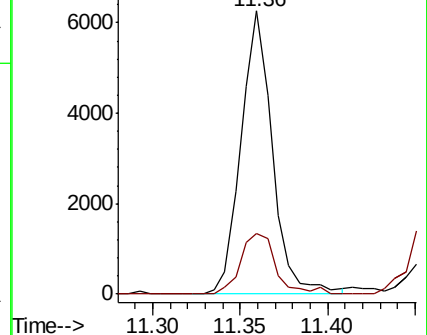

#80

1,3,5-Trimethylbenzene

Concen: 0.641 ug/l

RT: 11.45 min Scan# 1689

Delta R.T. -0.05 min

Lab File: VX010535.D


Acq: 28 Jun 2019 14:38

Tgt Ion: 105 Resp: 5638

Ion Ratio Lower Upper



105 100


120 33.4 25.2 75.6



Abundance Ion 105.00 (104.70 to 105.70): VX010535.D (-1649) (-)

Ion 120.00 (119.70 to 120.70): VX010535.D (-1649) (-)

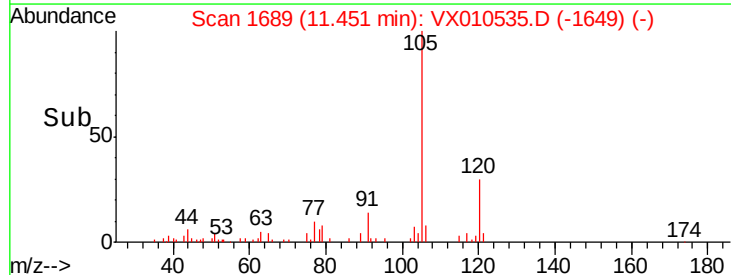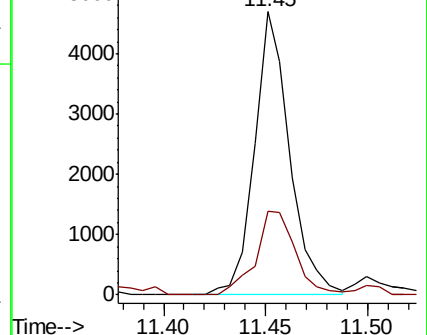

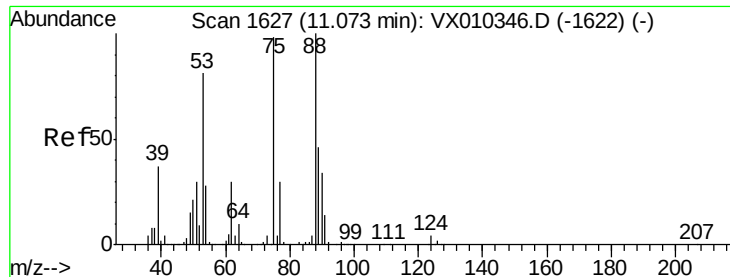

#81

trans-1,4-Dichloro-2-butene

Concen: 58.396 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.06 min

Lab File: VX010535.D

Acq: 28 Jun 2019 14:38

Instrument :

MSVOA_X

ClientSampleId :

FL-0575


Tot Ion: 75 Resp: 71806

Ion Ratio Lower Upper




75 100

53 0.1 66.1 99.1#

89 0.0 37.8 56.6#

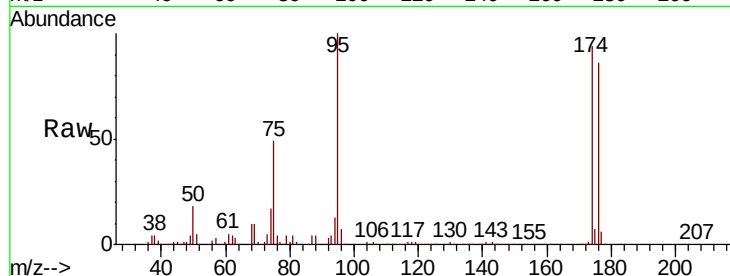

Abundance Ion 74.90 (74.60 to 75.60): VX0
Ion 53.00 (52.70 to 53.70): VX0
Ion 88.90 (88.60 to 89.60): VX0

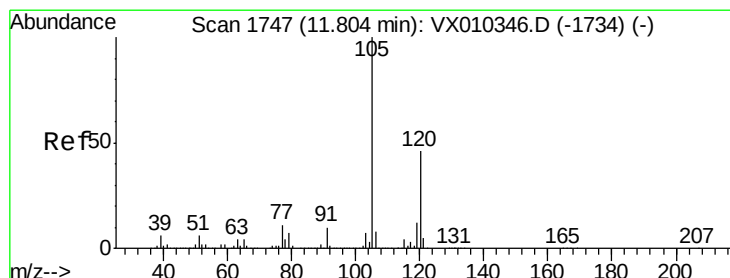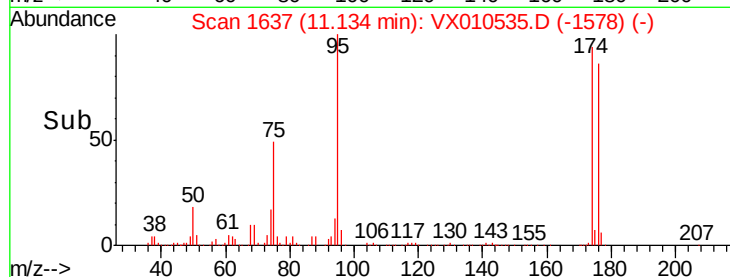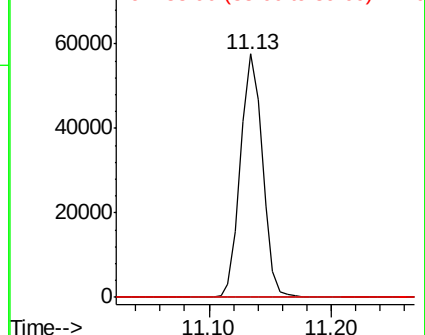

#84

1,2,4-Trimethylbenzene

Concen: 3.506 ug/l

RT: 11.80 min Scan# 1747

Delta R.T. 0.00 min

Lab File: VX010535.D


Acq: 28 Jun 2019 14:38

Tgt Ion: 105 Resp: 30988



Ion Ratio Lower Upper


105 100

120 45.6 23.1 69.2

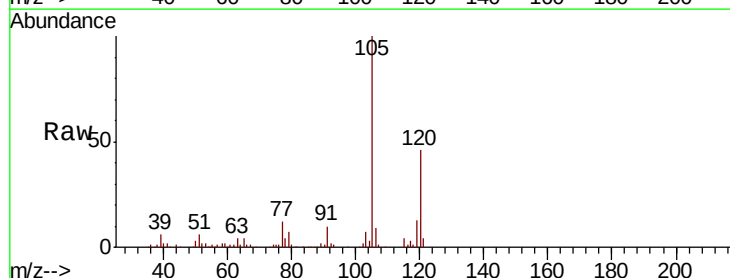

Abundance Ion 105.00 (104.70 to 105.70): V
Ion 120.00 (119.70 to 120.70): V

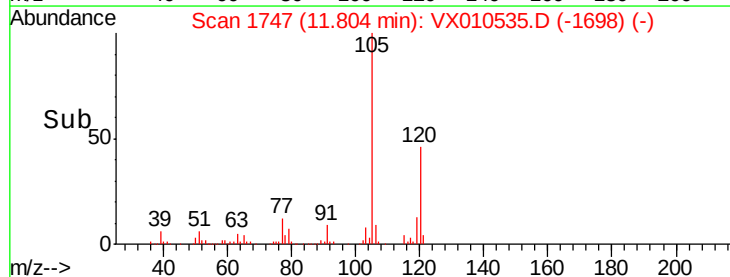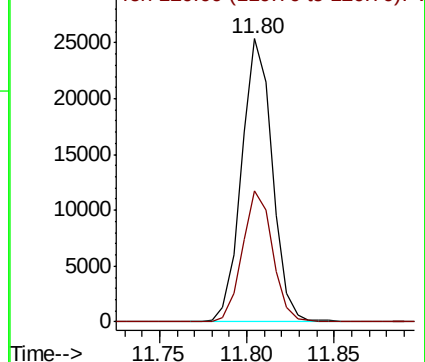



#85

sec-Butylbenzene

Concen: 0.240 ug/l

RT: 11.94 min Scan# 1770

Delta R.T. 0.00 min

Lab File: VX010535.D

Acq: 28 Jun 2019 14:38

Instrument :

MSVOA_X

ClientSampleId :


FL-0575

Tot Ion:105 Resp: 2491

Ion Ratio Lower Upper

105 100

134 35.2 10.7 31.9#



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 134.00 (133.70 to 134.70): V

2500

2000

1500

1000

500



0

11.90

11.95

11.94

Time-->



#90

Hexachloroethane

Concen: 0.201 ug/l

RT: 12.58 min Scan# 1875

Delta R.T. -0.01 min

Lab File: VX010535.D


Acq: 28 Jun 2019 14:38

Tgt Ion:117 Resp: 334

Ion Ratio Lower Upper

117 100

201 0.0 44.0 131.8#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 200.70 (200.40 to 201.40): V

300

200

100


0


12.56

12.58

12.60

Time-->



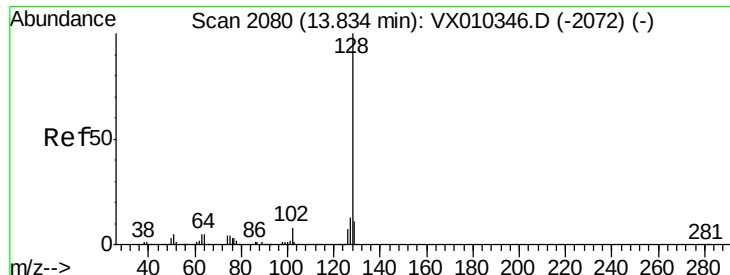

#95

Naphthalene

Concen: 0.926 ug/l

RT: 13.83 min Scan# 2080

Delta R.T. 0.00 min

Lab File: VX010535.D

Acq: 28 Jun 2019 14:38

Instrument :

MSVOA_X

ClientSampleId :

FL-0575


Tot Ion:128 Resp: 10203

Ion Ratio Lower Upper

128 100

127 12.3 10.2 15.4

129 11.9 8.9 13.3

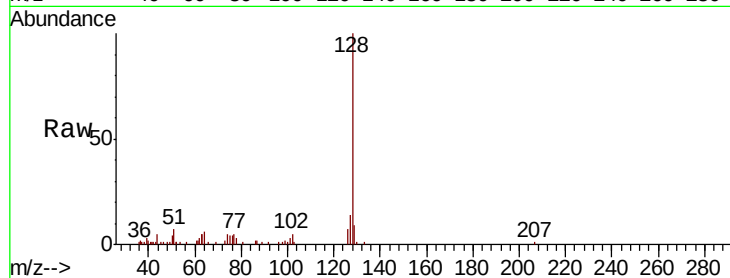

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

