

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062821\
 Data File : VX022980.D
 Acq On : 28 Jun 2021 15:49
 Operator : JC/MD
 Sample : M2875-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-15

Quant Time: Jun 29 03:06:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 23 19:12:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	53868	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.769	114	113343	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.061	117	96986	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	34400	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.970	65	50125	51.274	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 102.540%			
35) Dibromofluoromethane	5.391	113	34339	47.709	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 95.420%			
50) Toluene-d8	8.653	98	136426	48.363	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 96.720%			
62) 4-Bromofluorobenzene	11.085	95	45230	42.963	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 85.920%			
Target Compounds						Qvalue
3) Chloromethane	1.300	50	270	0.324	ug/l	# 79
5) Bromomethane	1.611	94	272	0.641	ug/l	89
10) Methyl Iodide	2.459	142	385	4.301	ug/l	# 73
11) Tert butyl alcohol	2.971	59	103	0.506	ug/l	# 73
13) Acrolein	2.245	56	46	0.363	ug/l	# 14
15) Acrylonitrile	3.075	53	149	0.320	ug/l	# 44
16) Acetone	2.386	43	1369	3.159	ug/l	92
17) Carbon Disulfide	2.514	76	844	3.928	ug/l	# 76
20) Methylene Chloride	2.806	84	197	0.600	ug/l	# 66
25) 2-Butanone	4.580	43	157	0.233	ug/l	# 45
30) Chloroform	5.105	83	2734	1.842	ug/l	98
31) Cyclohexane	5.568	56	1774	1.285	ug/l	# 51
36) 1,1-Dichloropropene	5.562	75	5880	4.884	ug/l	# 48
38) Carbon Tetrachloride	5.562	117	6520	6.457	ug/l	# 16
54) cis-1,3-Dichloropropene	8.372	75	22	2.603	ug/l	# 1
60) Dibromochloromethane	9.281	129	1868	5.750	ug/l	# 11
64) Tetrachloroethene	9.275	164	1740	2.553	ug/l	91
74) N-amyl acetate	10.854	43	77	2.100	ug/l	# 34
76) 1,2,3-Trichloropropane	11.085	75	25236	27.773	ug/l	# 39
81) trans-1,4-Dichloro-2-b...	11.085	75	25236	71.760	ug/l	# 12
85) sec-Butylbenzene	11.896	105	697	0.229	ug/l	82
86) p-Isopropyltoluene	12.012	119	537	0.222	ug/l	# 71
87) 1,3-Dichlorobenzene	11.981	146	269	0.230	ug/l	# 60
88) 1,4-Dichlorobenzene	12.048	146	375	0.307	ug/l	# 27
89) n-Butylbenzene	12.341	91	671	0.292	ug/l	95
91) 1,2-Dichlorobenzene	12.341	146	275	0.241	ug/l	# 57
93) 1,2,4-Trichlorobenzene	13.591	180	403	0.638	ug/l	84
94) Hexachlorobutadiene	13.725	225	103	0.416	ug/l	98
95) Naphthalene	13.780	128	898	2.230	ug/l	# 78
96) 1,2,3-Trichlorobenzene	13.969	180	238	0.374	ug/l	# 55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062821\
Data File : VX022980.D
Acq On : 28 Jun 2021 15:49
Operator : JC/MD
Sample : M2875-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-15

Quant Time: Jun 29 03:06:40 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 23 19:12:26 2021
Response via : Initial Calibration




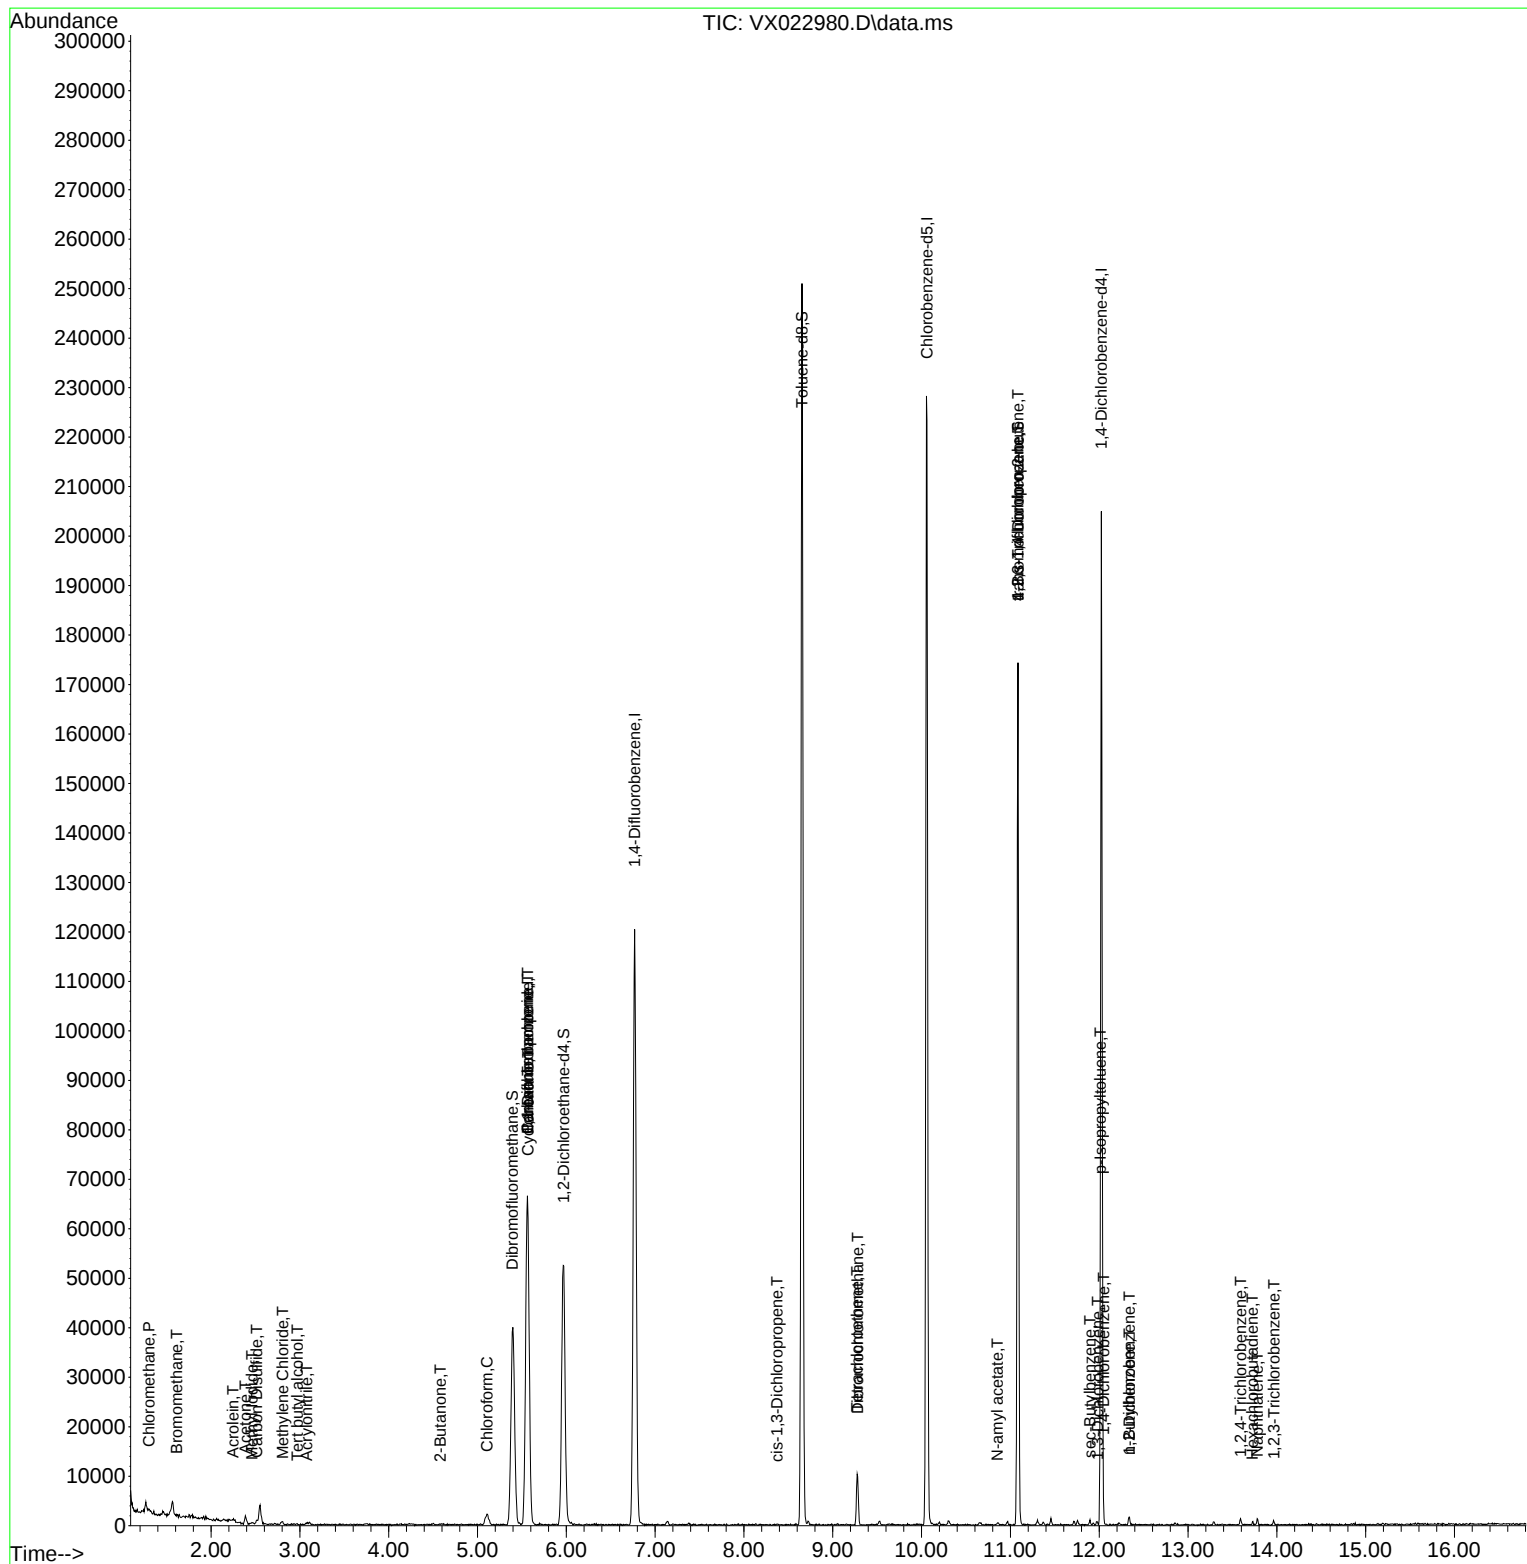




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. 0.006 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49




Instrument :
MSVOA_X
ClientSampleId :
MW-15


Tgt Ion:168 Resp: 53868
Ion Ratio Lower Upper
168 100
99 74.9 45.8 68.6#

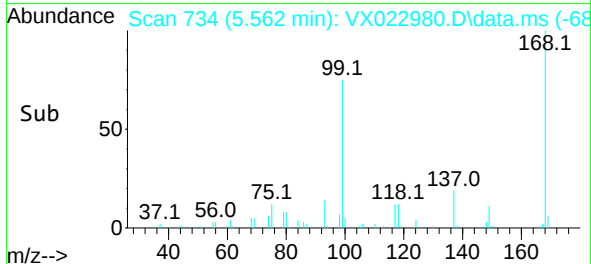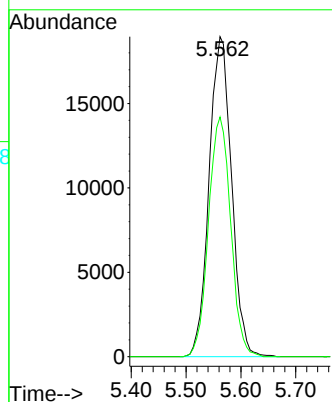

#3
Chloromethane
Concen: 0.324 ug/l
RT: 1.300 min Scan# 35
Delta R.T. 0.006 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49

Tgt Ion: 50 Resp: 270
Ion Ratio Lower Upper
50 100
52 21.2 26.4 39.6#


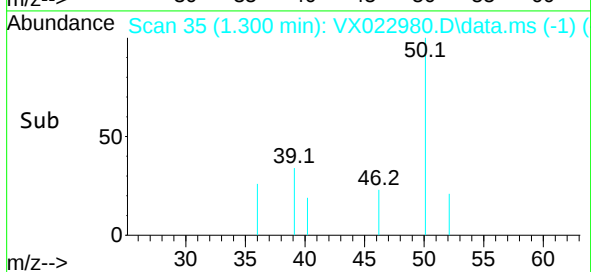
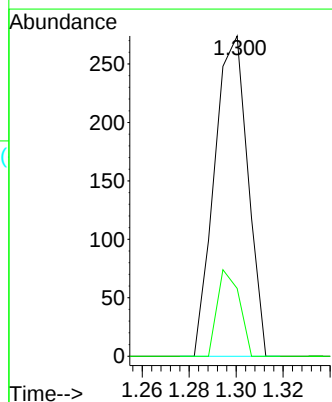



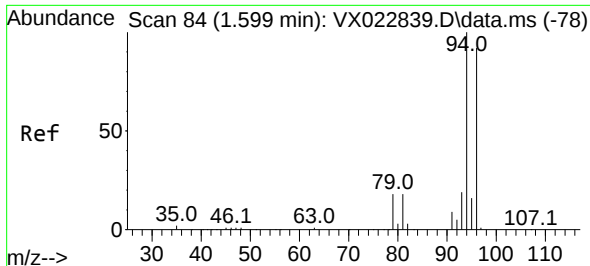

#5
Bromomethane
Concen: 0.641 ug/l
RT: 1.611 min Scan# 86
Delta R.T. 0.012 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49




Instrument :
MSVOA_X
ClientSampled :
MW-15


Tgt Ion: 94 Resp: 272
Ion Ratio Lower Upper
94 100
96 106.4 76.4 114.6

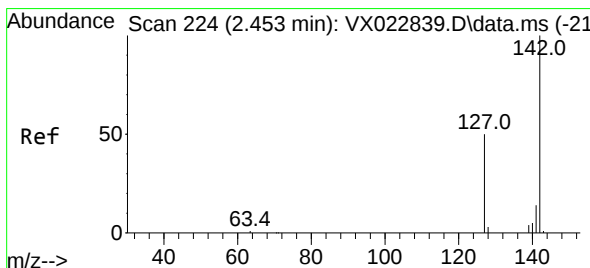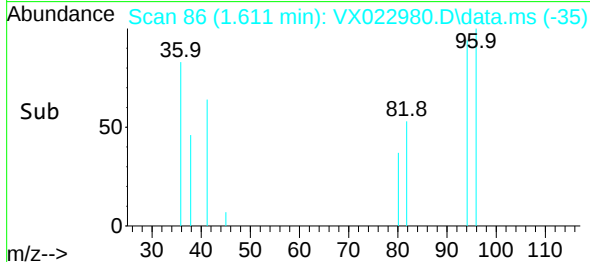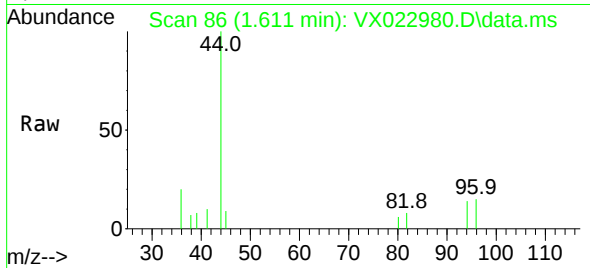

#10
Methyl Iodide
Concen: 4.301 ug/l
RT: 2.459 min Scan# 225
Delta R.T. 0.006 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49

Tgt Ion: 142 Resp: 385
Ion Ratio Lower Upper
142 100
127 26.5 33.3 49.9#
141 0.0 11.4 17.0#

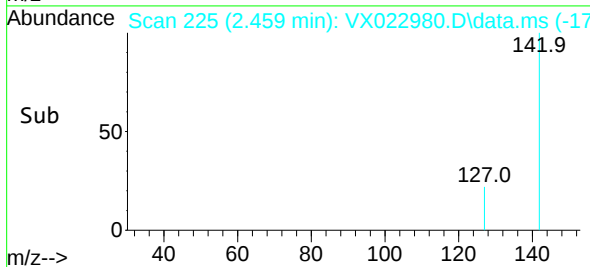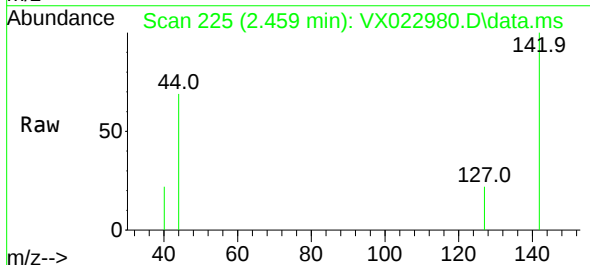




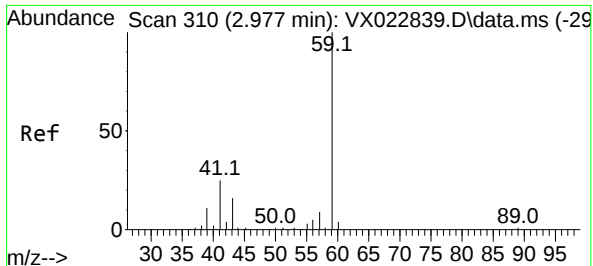


#11

Tert butyl alcohol
Concen: 0.506 ug/l
RT: 2.971 min Scan# 309
Delta R.T. -0.006 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49

Instrument :
MSVOA_X
ClientSampleId :
MW-15




Tgt Ion: 59 Resp: 103
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#

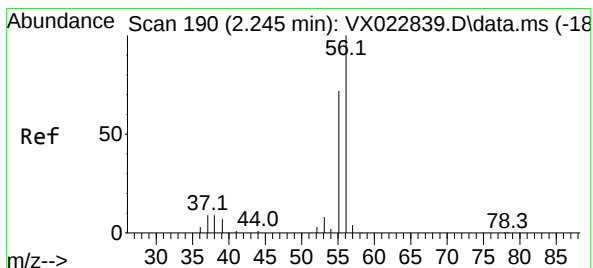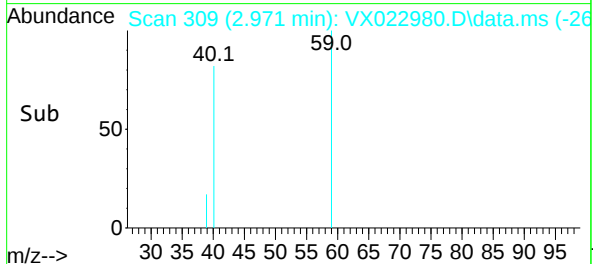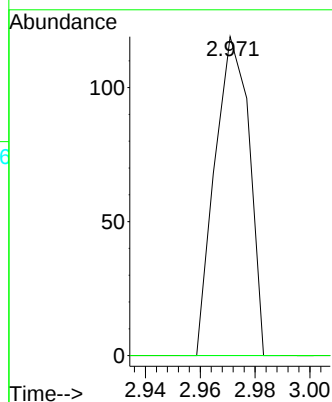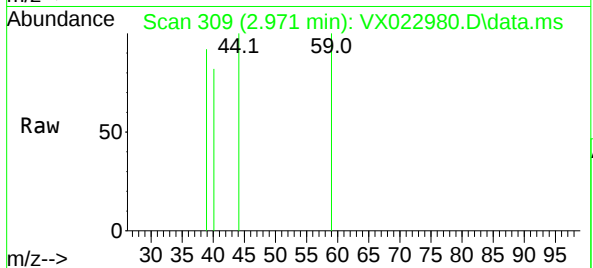


#13

Acrolein
Concen: 0.363 ug/l
RT: 2.245 min Scan# 190
Delta R.T. 0.000 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49

Tgt Ion: 56 Resp: 46
Ion Ratio Lower Upper
56 100
55 0.0 56.4 84.6#


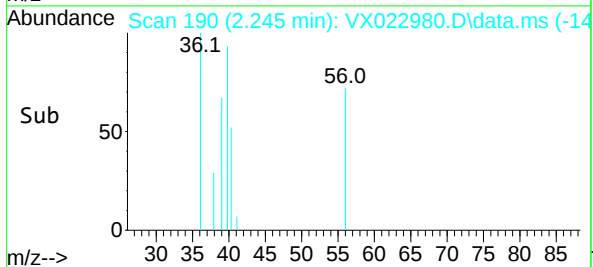
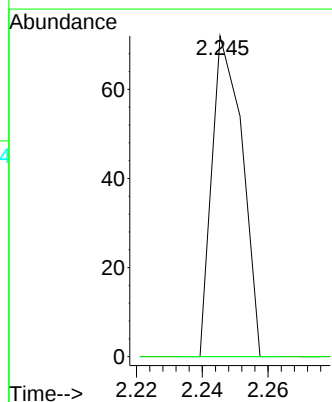
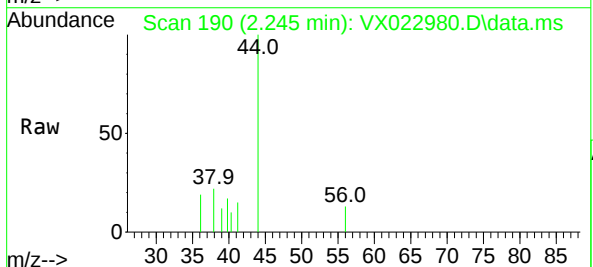




#15
Acrylonitrile
Concen: 0.320 ug/l
RT: 3.075 min Scan# 326
Delta R.T. 0.001 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49




Instrument :
MSVOA_X
ClientSampleId :
MW-15


Tgt Ion:	53	Resp:	149
Ion	Ratio	Lower	Upper
53	100		
52	129.5	65.3	97.9#
51	0.0	28.2	42.2#

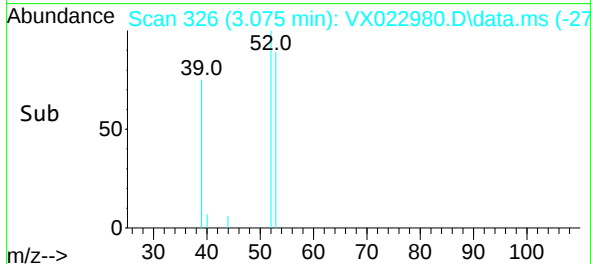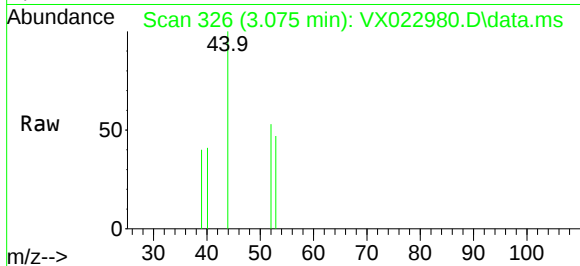

#16
Acetone
Concen: 3.159 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49

Tgt Ion:	43	Resp:	1369
Ion	Ratio	Lower	Upper
43	100		
58	30.0	27.8	41.8


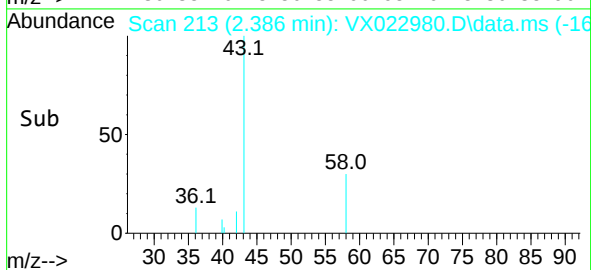

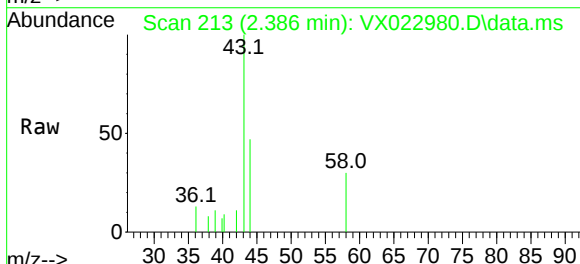




#17
Carbon Disulfide
Concen: 3.928 ug/l
RT: 2.514 min Scan# 234
Delta R.T. -0.000 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49




Instrument :
MSVOA_X
ClientSampleId :
MW-15


Tgt Ion: 76 Resp: 844
Ion Ratio Lower Upper
76 100
78 17.5 7.2 10.8#

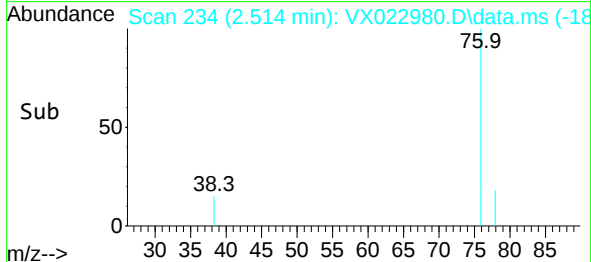

#20
Methylene Chloride
Concen: 0.600 ug/l
RT: 2.806 min Scan# 282
Delta R.T. 0.012 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49

Tgt Ion: 84 Resp: 197
Ion Ratio Lower Upper
84 100
49 63.2 88.6 132.8#
51 0.0 27.0 40.6#
86 61.2 50.3 75.5


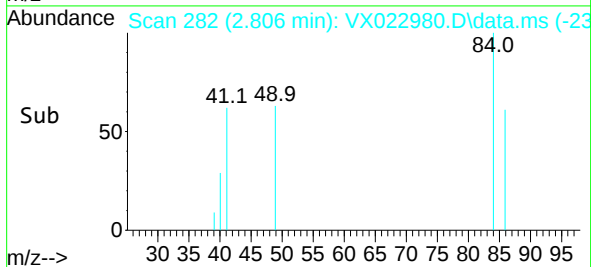

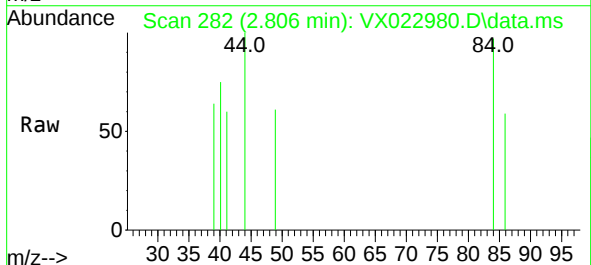


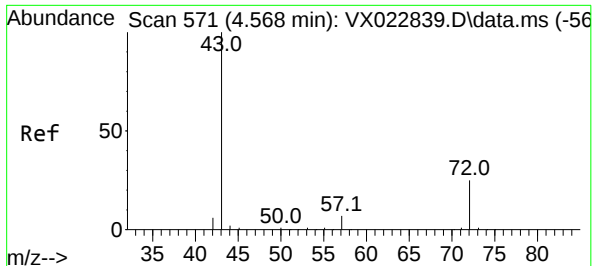

#25
2-Butanone
Concen: 0.233 ug/l
RT: 4.580 min Scan# 573
Delta R.T. 0.012 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49




Instrument :
MSVOA_X
ClientSampleId :
MW-15


Tgt Ion: 43 Resp: 157
Ion Ratio Lower Upper
43 100
72 0.0 23.7 35.5#

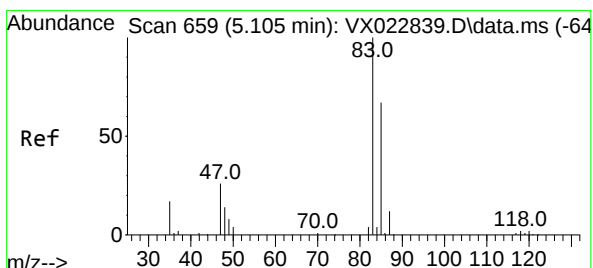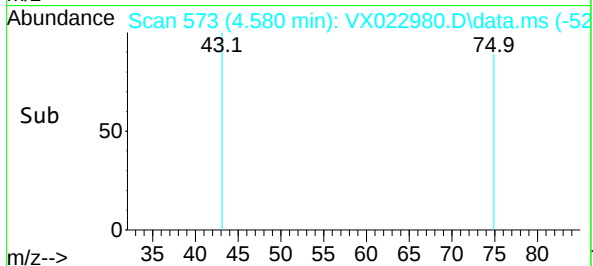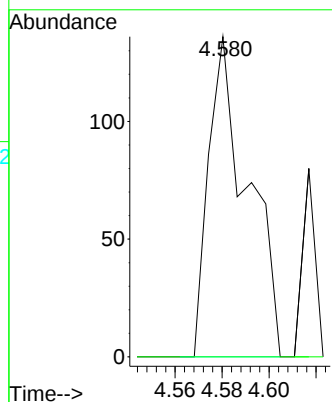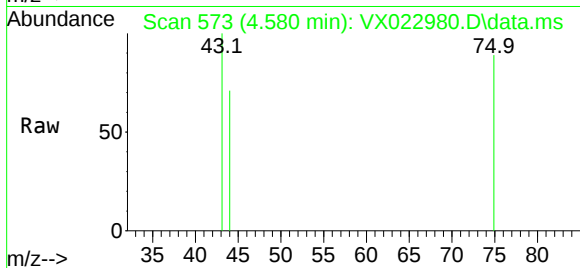

#30
Chloroform
Concen: 1.842 ug/l
RT: 5.105 min Scan# 659
Delta R.T. -0.000 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49

Tgt Ion: 83 Resp: 2734
Ion Ratio Lower Upper
83 100
85 66.5 52.0 78.0


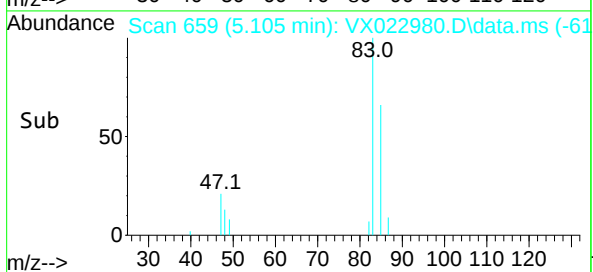
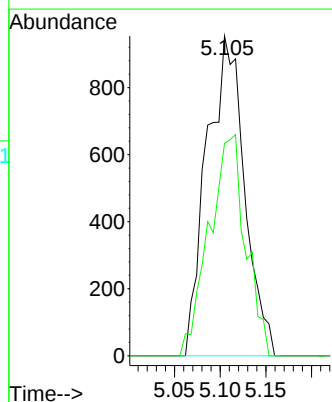
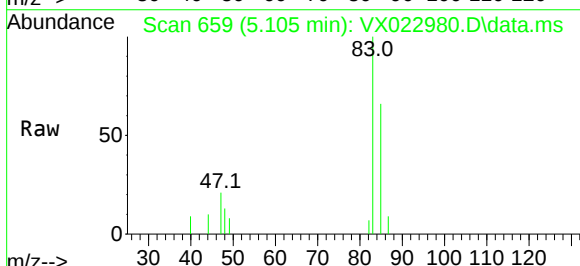


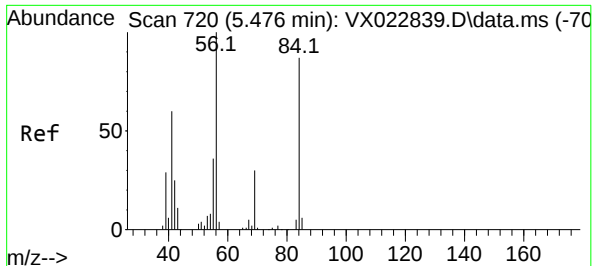

#31
Cyclohexane
Concen: 1.285 ug/l
RT: 5.568 min Scan# 735
Delta R.T. 0.092 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49




Instrument :
MSVOA_X
ClientSampled :
MW-15


Tgt Ion: 56 Resp: 1774
Ion Ratio Lower Upper
56 100
69 133.0 25.3 37.9#
84 90.7 71.4 107.0

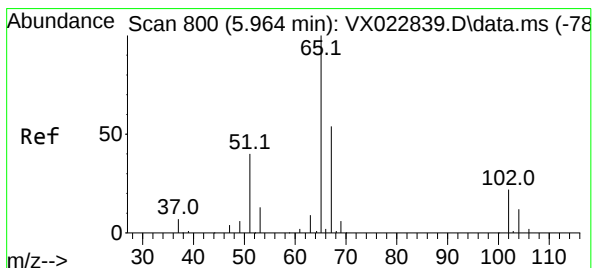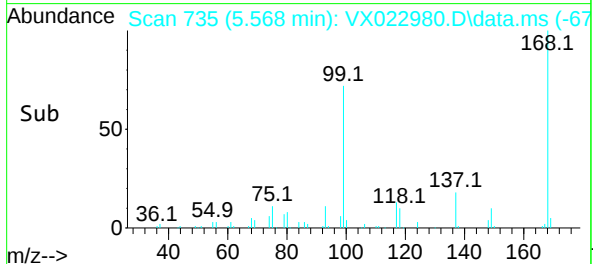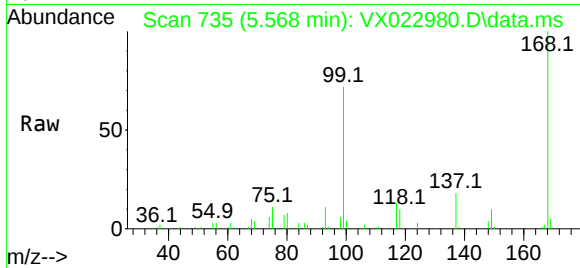

#33
1,2-Dichloroethane-d4
Concen: 51.274 ug/l
RT: 5.970 min Scan# 801
Delta R.T. 0.006 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49

Tgt Ion: 65 Resp: 50125
Ion Ratio Lower Upper
65 100
67 51.7 0.0 105.4


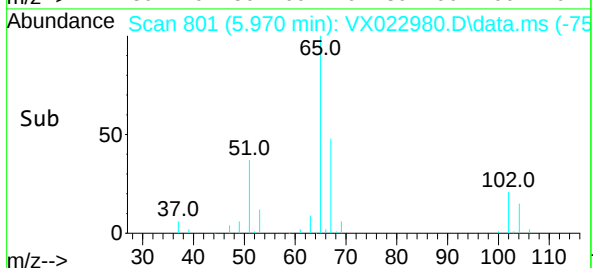

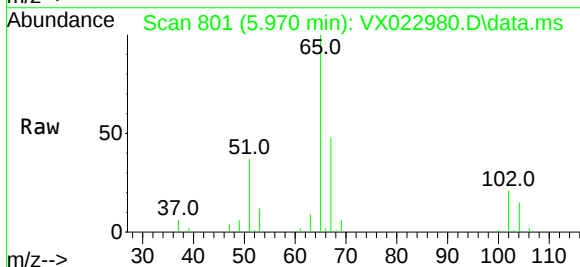


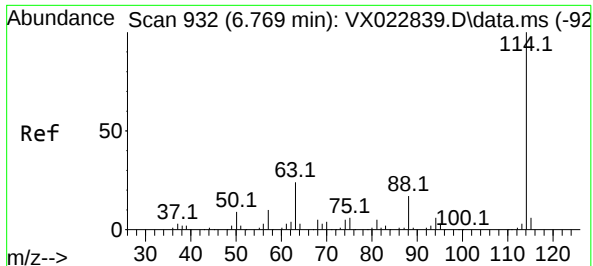

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. -0.000 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49




Instrument :
MSVOA_X
ClientSampleId :
MW-15


Tgt Ion:114 Resp: 113343
Ion Ratio Lower Upper
114 100
63 22.6 0.0 40.8
88 15.7 0.0 32.8

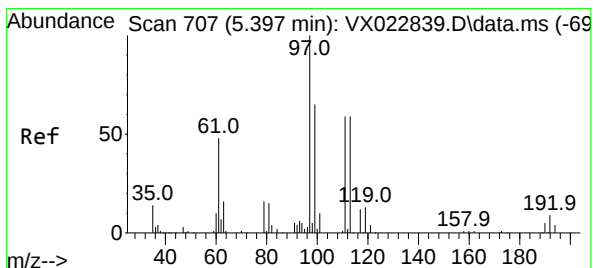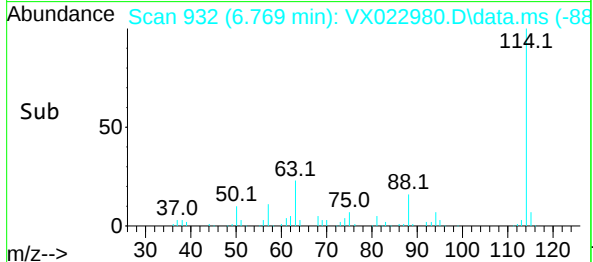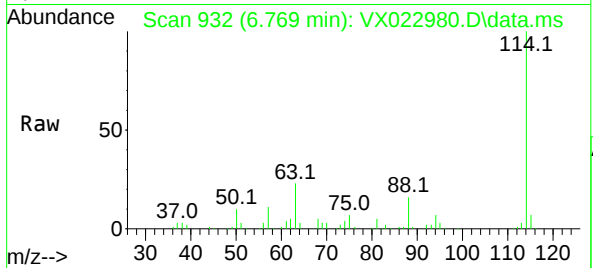

#35
Dibromofluoromethane
Concen: 47.709 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.006 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49

Tgt Ion:113 Resp: 34339
Ion Ratio Lower Upper
113 100
111 104.4 81.9 122.9
192 15.2 16.7 25.1#

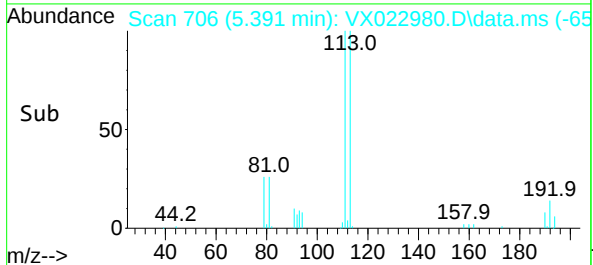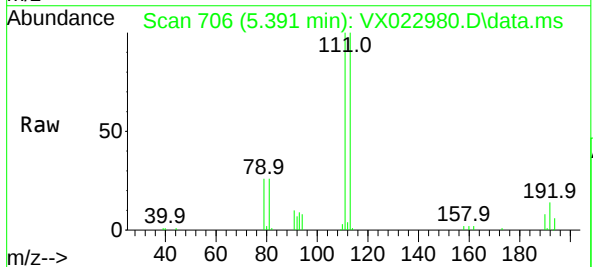



#36

1,1-Dichloropropene

Concen: 4.884 ug/l

RT: 5.562 min Scan# 734





Delta R.T. -0.140 min

Lab File: VX022980.D

Acq: 28 Jun 2021 15:49

Tgt Ion:	75	Resp:	5880
Ion	Ratio	Lower	Upper
75	100		
110	8.1	18.1	54.4#
77	0.0	25.3	37.9#

Instrument :
MSVOA_X
ClientSampled :
MW-15

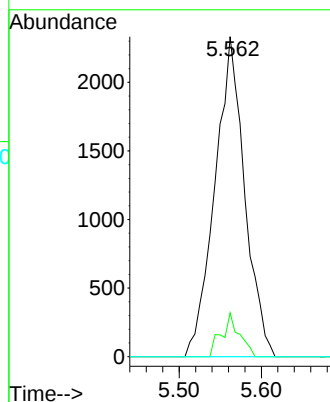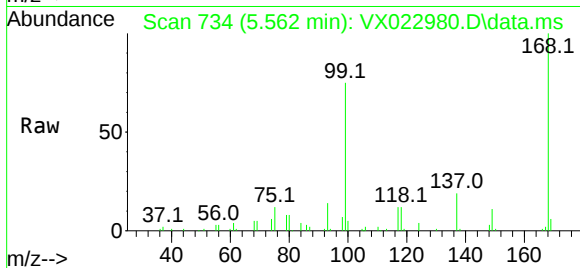

#38

Carbon Tetrachloride

Concen: 6.457 ug/l




RT: 5.562 min Scan# 734


Delta R.T. -0.128 min

Lab File: VX022980.D

Acq: 28 Jun 2021 15:49

Tgt Ion:	117	Resp:	6520
Ion	Ratio	Lower	Upper
117	100		
119	5.0	76.2	114.2#
121	0.0	24.8	37.2#


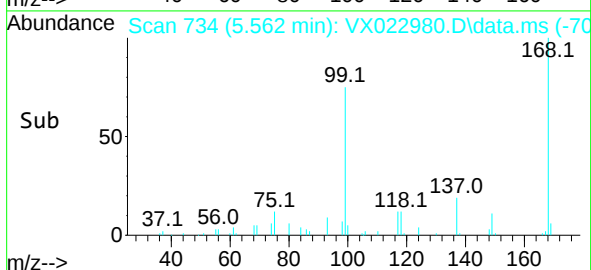
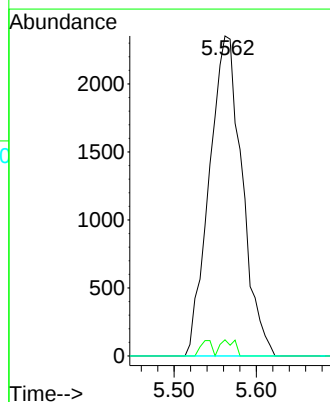
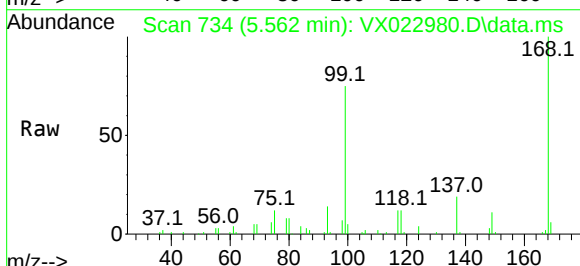


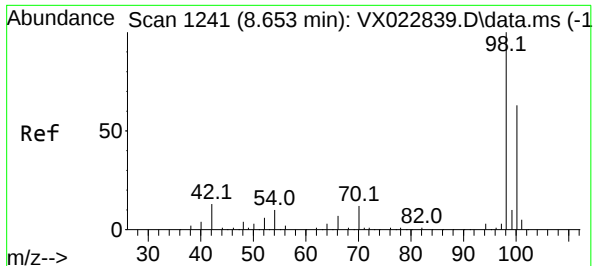

#50
Toluene-d8
Concen: 48.363 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49




Instrument :
MSVOA_X
ClientSampled :
MW-15


Tgt Ion: 98 Resp: 136426
Ion Ratio Lower Upper
98 100
100 64.7 51.9 77.9

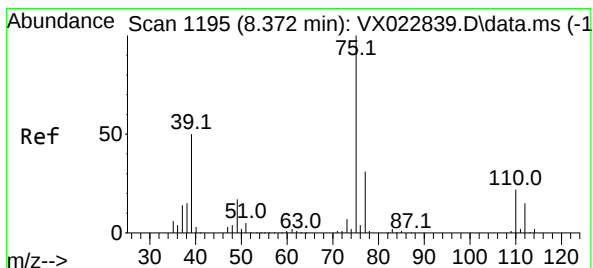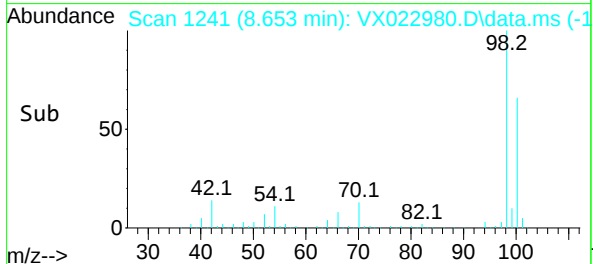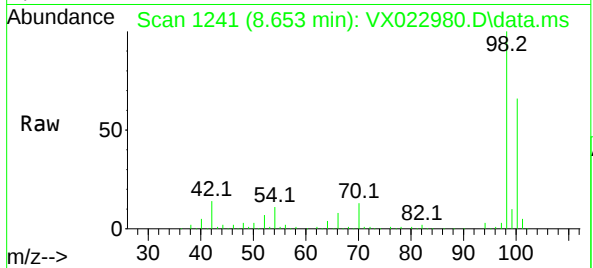

#54
cis-1,3-Dichloropropene
Concen: 2.603 ug/l
RT: 8.372 min Scan# 1195
Delta R.T. 0.000 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49

Tgt Ion: 75 Resp: 22
Ion Ratio Lower Upper
75 100
77 0.0 25.7 38.5#
39 135.0 35.1 52.7#


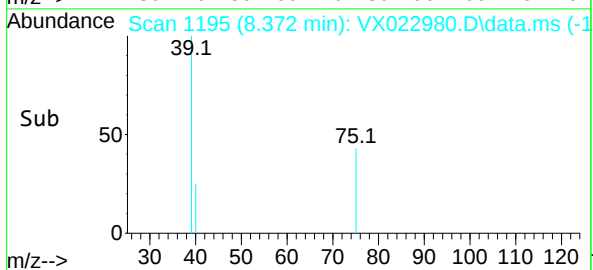

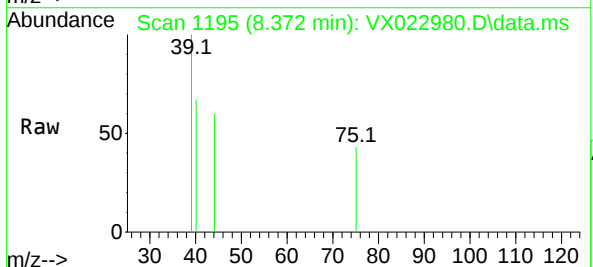




#60
Dibromochloromethane
Concen: 5.750 ug/l
RT: 9.281 min Scan# 1344
Delta R.T. -0.243 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49




Instrument :
MSVOA_X
ClientSampleId :
MW-15


Tgt Ion:129 Resp: 1868
Ion Ratio Lower Upper
129 100
127 0.0 38.4 115.2#

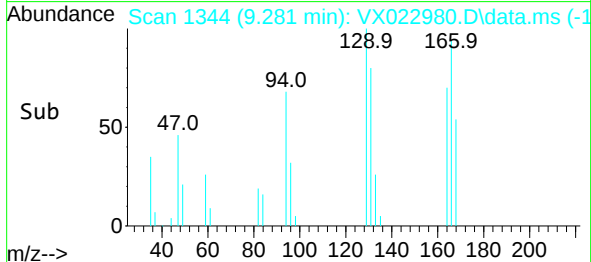

#62
4-Bromofluorobenzene
Concen: 42.963 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49

Tgt Ion: 95 Resp: 45230
Ion Ratio Lower Upper
95 100
174 60.1 0.0 154.6
176 59.6 0.0 155.8


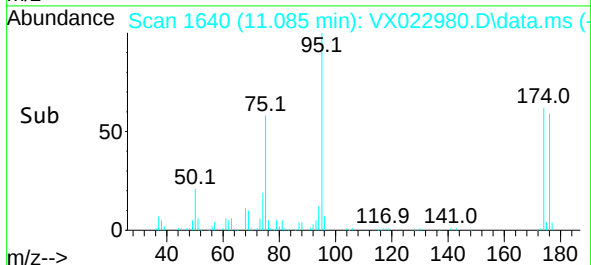
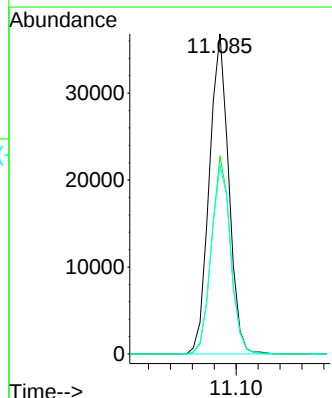
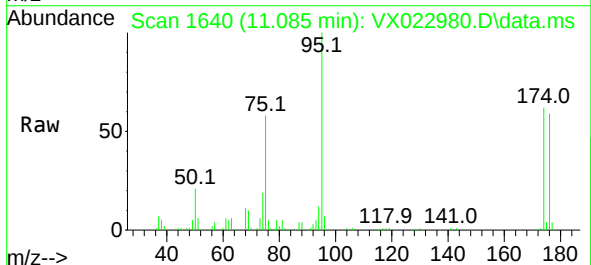




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.061 min Scan# 1472
Delta R.T. 0.006 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49




Instrument :
MSVOA_X
ClientSampled :
MW-15


Tgt Ion:117 Resp: 96986
Ion Ratio Lower Upper
117 100
82 60.2 47.4 71.2
119 30.8 26.6 39.8

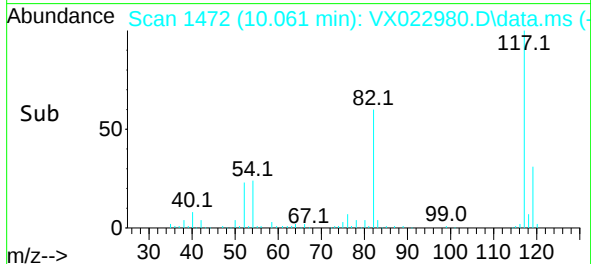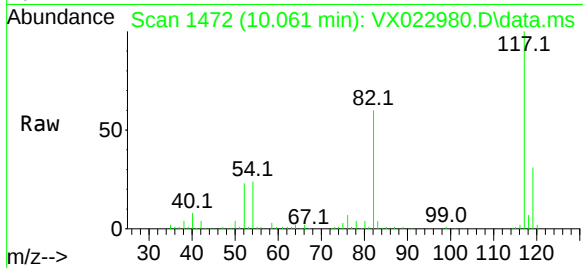

#64
Tetrachloroethene
Concen: 2.553 ug/l
RT: 9.275 min Scan# 1343
Delta R.T. -0.000 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49

Tgt Ion:164 Resp: 1740
Ion Ratio Lower Upper
164 100
166 116.4 103.4 155.2
129 100.6 70.8 106.2
131 88.4 72.5 108.7


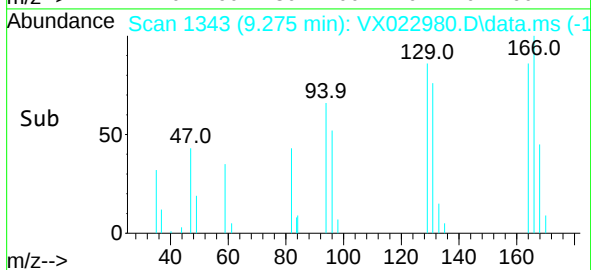

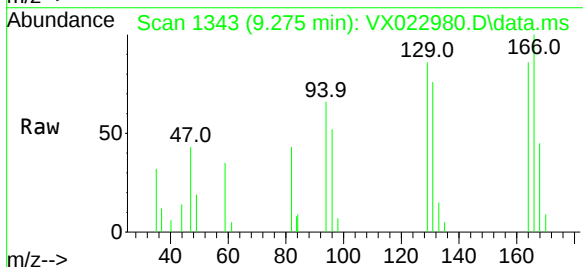




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49




Instrument :
MSVOA_X
ClientSampled :
MW-15


Tgt Ion:152 Resp: 34400
Ion Ratio Lower Upper
152 100
115 67.7 41.1 123.3
150 161.9 0.0 349.0

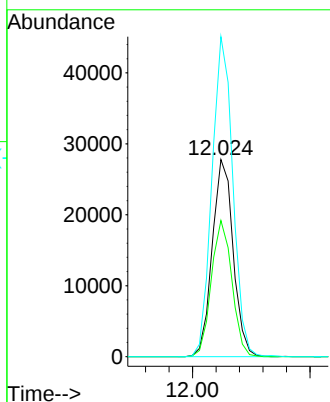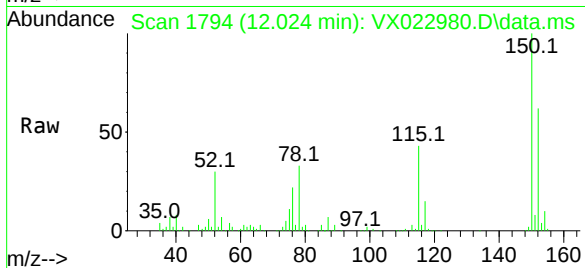

#74
N-ethyl acetate
Concen: 2.100 ug/l
RT: 10.854 min Scan# 1602
Delta R.T. 0.007 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49

Tgt Ion: 43 Resp: 77
Ion Ratio Lower Upper
43 100
70 29.9 39.0 58.6#
55 103.9 21.5 32.3#
61 0.0 22.1 33.1#


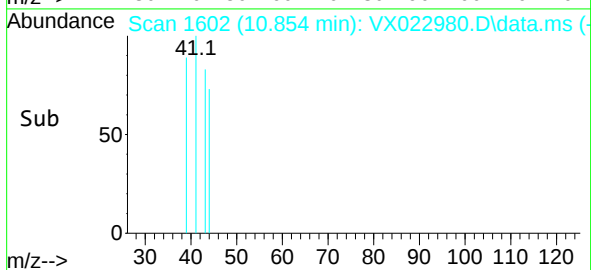
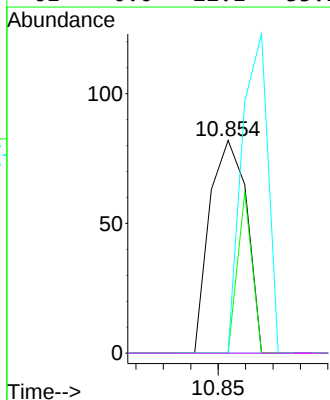
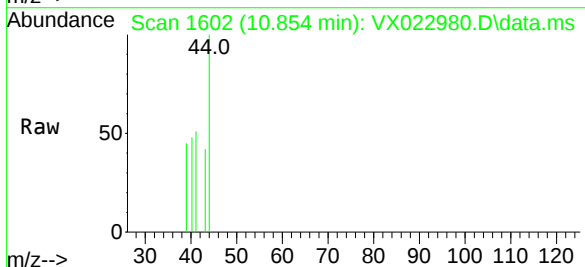




#76
1,2,3-Trichloropropane
Concen: 27.773 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49




Instrument :
MSVOA_X
ClientSampled :
MW-15


Tgt Ion: 75 Resp: 25236
Ion Ratio Lower Upper
75 100
77 1.3 19.1 57.5#

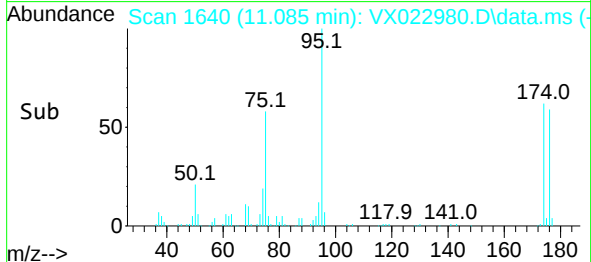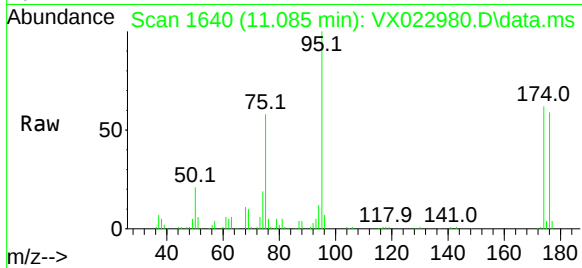

#81
trans-1,4-Dichloro-2-butene
Concen: 71.760 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.061 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49

Tgt Ion: 75 Resp: 25236
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#


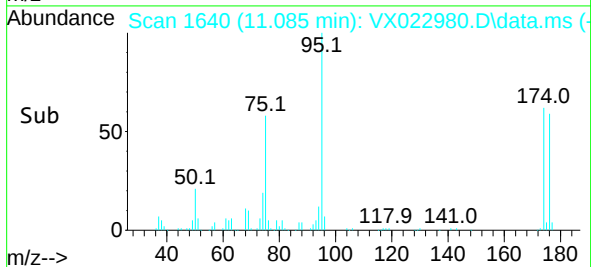

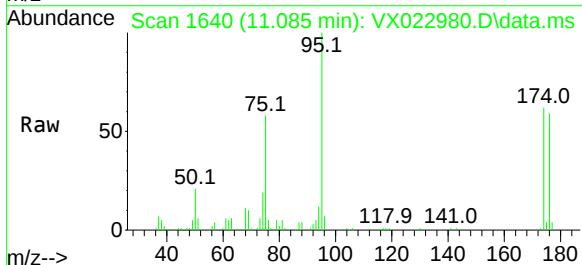




#85
 sec-Butylbenzene
 Concen: 0.229 ug/l
 RT: 11.896 min Scan# 1773
 Delta R.T. 0.000 min
 Lab File: VX022980.D
 Acq: 28 Jun 2021 15:49




Instrument :
 MSVOA_X
 ClientSampled :
 MW-15


Tgt Ion:105 Resp: 697
 Ion Ratio Lower Upper
 105 100
 134 11.6 10.0 29.8

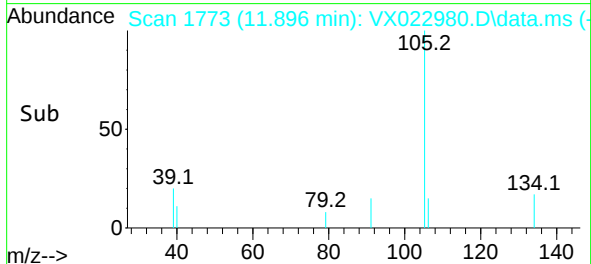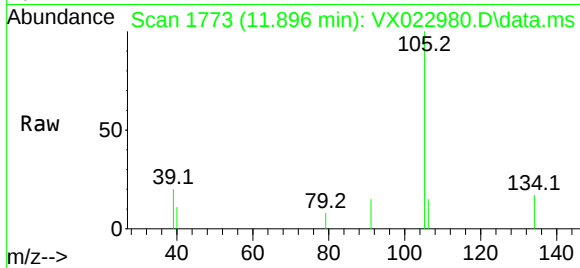

#86
 p-Isopropyltoluene
 Concen: 0.222 ug/l
 RT: 12.012 min Scan# 1792
 Delta R.T. -0.000 min
 Lab File: VX022980.D
 Acq: 28 Jun 2021 15:49

Tgt Ion:119 Resp: 537
 Ion Ratio Lower Upper
 119 100
 134 13.4 12.9 38.7
 91 39.5 11.7 35.0#


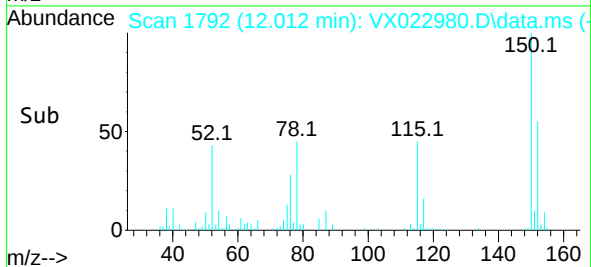

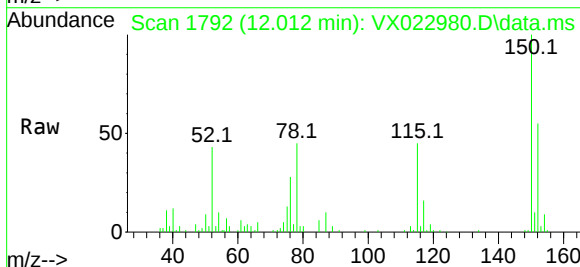




#87
1,3-Dichlorobenzene
Concen: 0.230 ug/l
RT: 11.981 min Scan# 1787
Delta R.T. 0.006 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49




Instrument :
MSVOA_X
ClientSampled :
MW-15


Tgt Ion:146 Resp: 269
Ion Ratio Lower Upper
146 100
111 0.0 20.2 60.5#
148 83.3 31.9 95.7

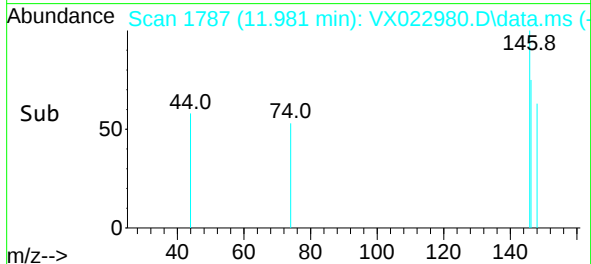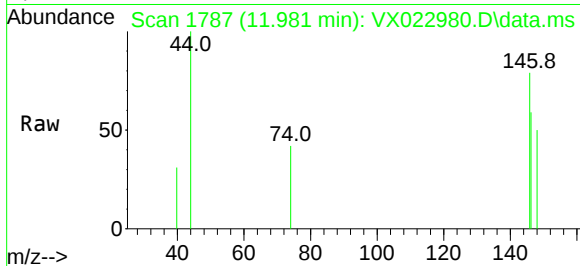

#88
1,4-Dichlorobenzene
Concen: 0.307 ug/l
RT: 12.048 min Scan# 1798
Delta R.T. 0.006 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49

Tgt Ion:146 Resp: 375
Ion Ratio Lower Upper
146 100
111 0.0 19.6 58.8#
148 124.8 31.6 95.0#


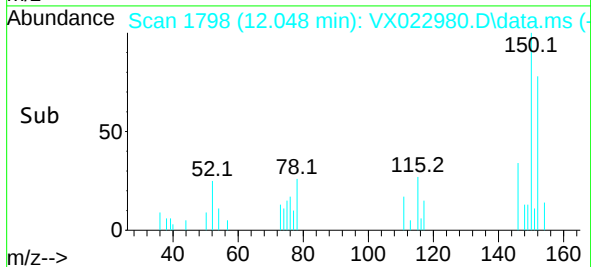

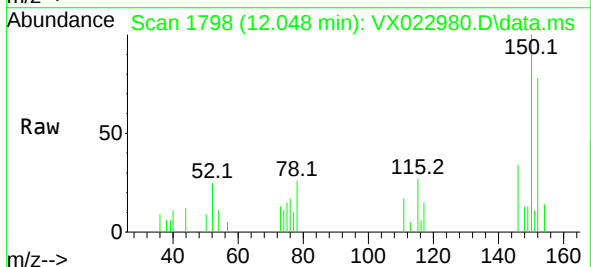




#89
n-Butylbenzene
Concen: 0.292 ug/l
RT: 12.341 min Scan# 1846
Delta R.T. 0.006 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49




Instrument :
MSVOA_X
ClientSampled :
MW-15


Tgt Ion: 91 Resp: 671
Ion Ratio Lower Upper
91 100
92 52.8 27.4 82.0
134 31.0 13.2 39.5

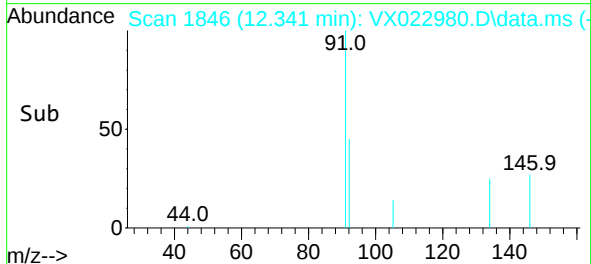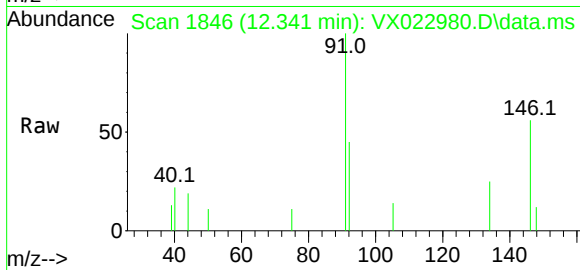

#91
1,2-Dichlorobenzene
Concen: 0.241 ug/l
RT: 12.341 min Scan# 1846
Delta R.T. 0.000 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49

Tgt Ion: 146 Resp: 275
Ion Ratio Lower Upper
146 100
111 0.0 20.8 62.2#
148 41.5 31.9 95.5


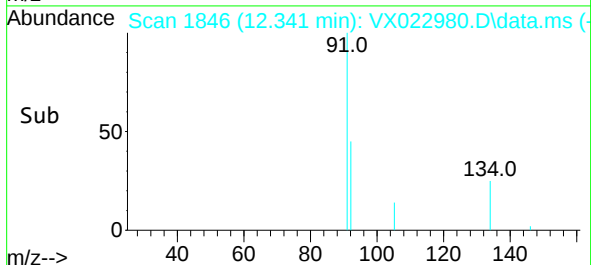
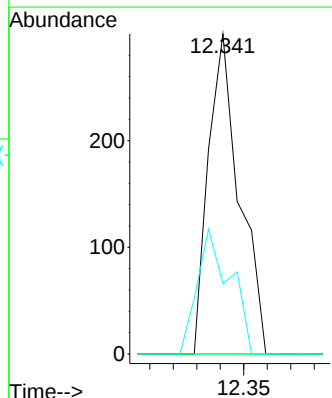
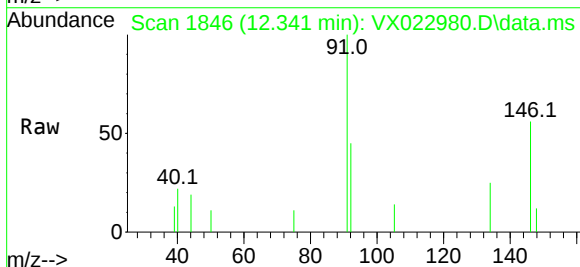




#93
 1,2,4-Trichlorobenzene
 Concen: 0.638 ug/l
 RT: 13.591 min Scan# 2051
 Delta R.T. -0.000 min
 Lab File: VX022980.D
 Acq: 28 Jun 2021 15:49




Instrument :
 MSVOA_X
 ClientSampled :
 MW-15


Tgt Ion:180 Resp: 403
 Ion Ratio Lower Upper
 180 100
 182 75.9 47.7 143.1
 145 27.8 15.0 45.0

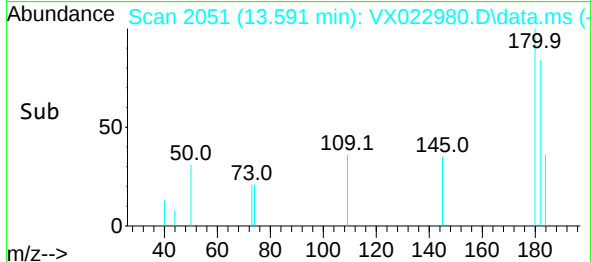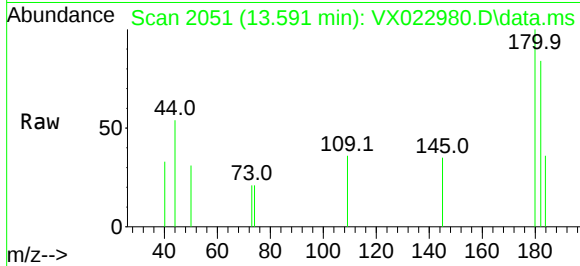

#94
 Hexachlorobutadiene
 Concen: 0.416 ug/l
 RT: 13.725 min Scan# 2073
 Delta R.T. 0.000 min
 Lab File: VX022980.D
 Acq: 28 Jun 2021 15:49

Tgt Ion:225 Resp: 103
 Ion Ratio Lower Upper
 225 100
 223 65.0 31.1 93.2
 227 64.1 31.6 95.0


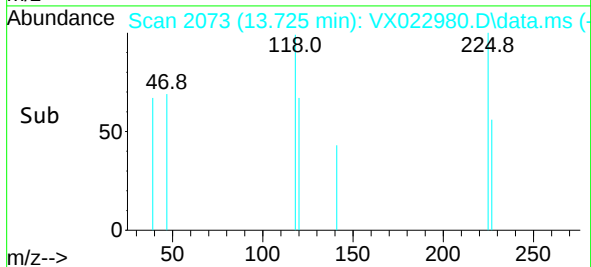

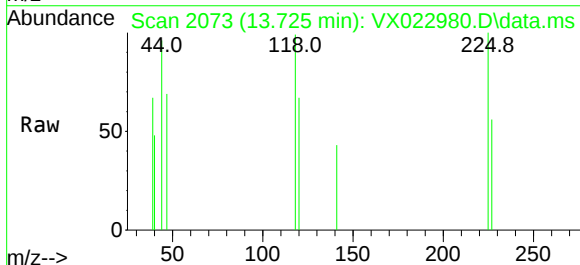




#95
Naphthalene
Concen: 2.230 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49

Instrument :
MSVOA_X
ClientSampled :
MW-15

Tgt Ion:128 Resp: 898
Ion Ratio Lower Upper
128 100
127 6.2 10.3 15.5#
129 0.0 8.8 13.2#

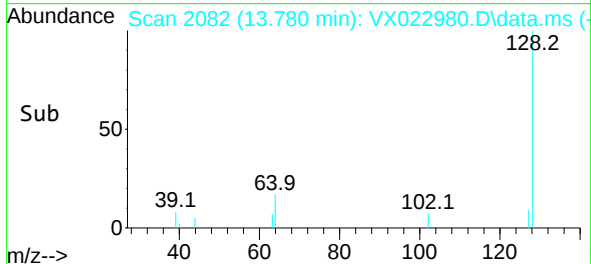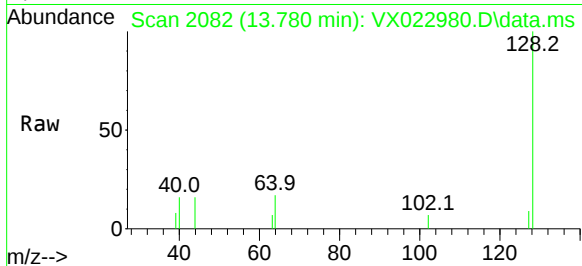

#96
1,2,3-Trichlorobenzene
Concen: 0.374 ug/l
RT: 13.969 min Scan# 2113
Delta R.T. 0.006 min
Lab File: VX022980.D
Acq: 28 Jun 2021 15:49

Tgt Ion:180 Resp: 238
Ion Ratio Lower Upper
180 100
182 56.3 47.6 142.9
145 0.0 16.1 48.3#

