

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062822\
 Data File : VX029840.D
 Acq On : 28 Jun 2022 19:49
 Operator : JC/MD
 Sample : N3494-09
 Misc : 5.16g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SP-EXC-1-4-GR

Quant Time: Jun 29 06:07:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 29 05:54:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	251284	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	422294	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	345462	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	145067	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	133672	42.024	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	84.040%		
35) Dibromofluoromethane	5.391	113	116937	44.309	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	88.620%		
50) Toluene-d8	8.653	98	478680	48.349	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	96.700%		
62) 4-Bromofluorobenzene	11.085	95	152990	43.715	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	87.440%		
Target Compounds						Qvalue
5) Bromomethane	1.612	94	1022	0.661	ug/l	87
6) Chloroethane	1.679	64	198	1.131	ug/l #	76
10) Methyl Iodide	2.429	142	1591	2.317	ug/l	98
11) Tert butyl alcohol	2.947	59	10902	13.105	ug/l #	81
13) Acrolein	2.246	56	88	Below Cal	#	14
17) Carbon Disulfide	2.483	76	2486	0.386	ug/l	98
18) Methyl Acetate	2.727	43	6042	1.259	ug/l	93
20) Methylene Chloride	2.782	84	2398	0.730	ug/l	91
29) Tetrahydrofuran	5.050	42	478	0.269	ug/l #	32
36) 1,1-Dichloropropene	5.550	75	18457	5.258	ug/l #	49
38) Carbon Tetrachloride	5.550	117	22695	7.462	ug/l #	18
39) Methylcyclohexane	7.373	83	1687	0.398	ug/l #	84
44) Trichloroethene	7.129	130	1566	0.512	ug/l	100
65) Chlorobenzene	10.080	112	165524	23.869	ug/l	98
67) Ethyl Benzene	10.195	91	3374	0.280	ug/l	96
68) m/p-Xylenes	10.305	106	1999	0.432	ug/l	94
69) o-Xylene	10.653	106	1096	0.234	ug/l	84
76) 1,2,3-Trichloropropane	11.085	75	68974	19.862	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.085	75	68974	63.076	ug/l #	13
84) 1,2,4-Trimethylbenzene	11.756	105	2417	0.277	ug/l	80
85) sec-Butylbenzene	11.890	105	2300	0.211	ug/l	86
87) 1,3-Dichlorobenzene	11.976	146	3991	0.823	ug/l	90
88) 1,4-Dichlorobenzene	11.976	146	3991	0.807	ug/l	93
89) n-Butylbenzene	12.335	91	2218	0.272	ug/l #	81
91) 1,2-Dichlorobenzene	12.341	146	77415	16.256	ug/l	100
93) 1,2,4-Trichlorobenzene	13.591	180	2475	0.858	ug/l	88
94) Hexachlorobutadiene	13.731	225	277	0.259	ug/l #	36
95) Naphthalene	13.780	128	5792	0.494	ug/l #	92
96) 1,2,3-Trichlorobenzene	13.963	180	1887	0.639	ug/l #	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062822\
Data File : VX029840.D
Acq On : 28 Jun 2022 19:49
Operator : JC/MD
Sample : N3494-09
Misc : 5.16g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-4-GR

Quant Time: Jun 29 06:07:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 29 05:54:51 2022
Response via : Initial Calibration




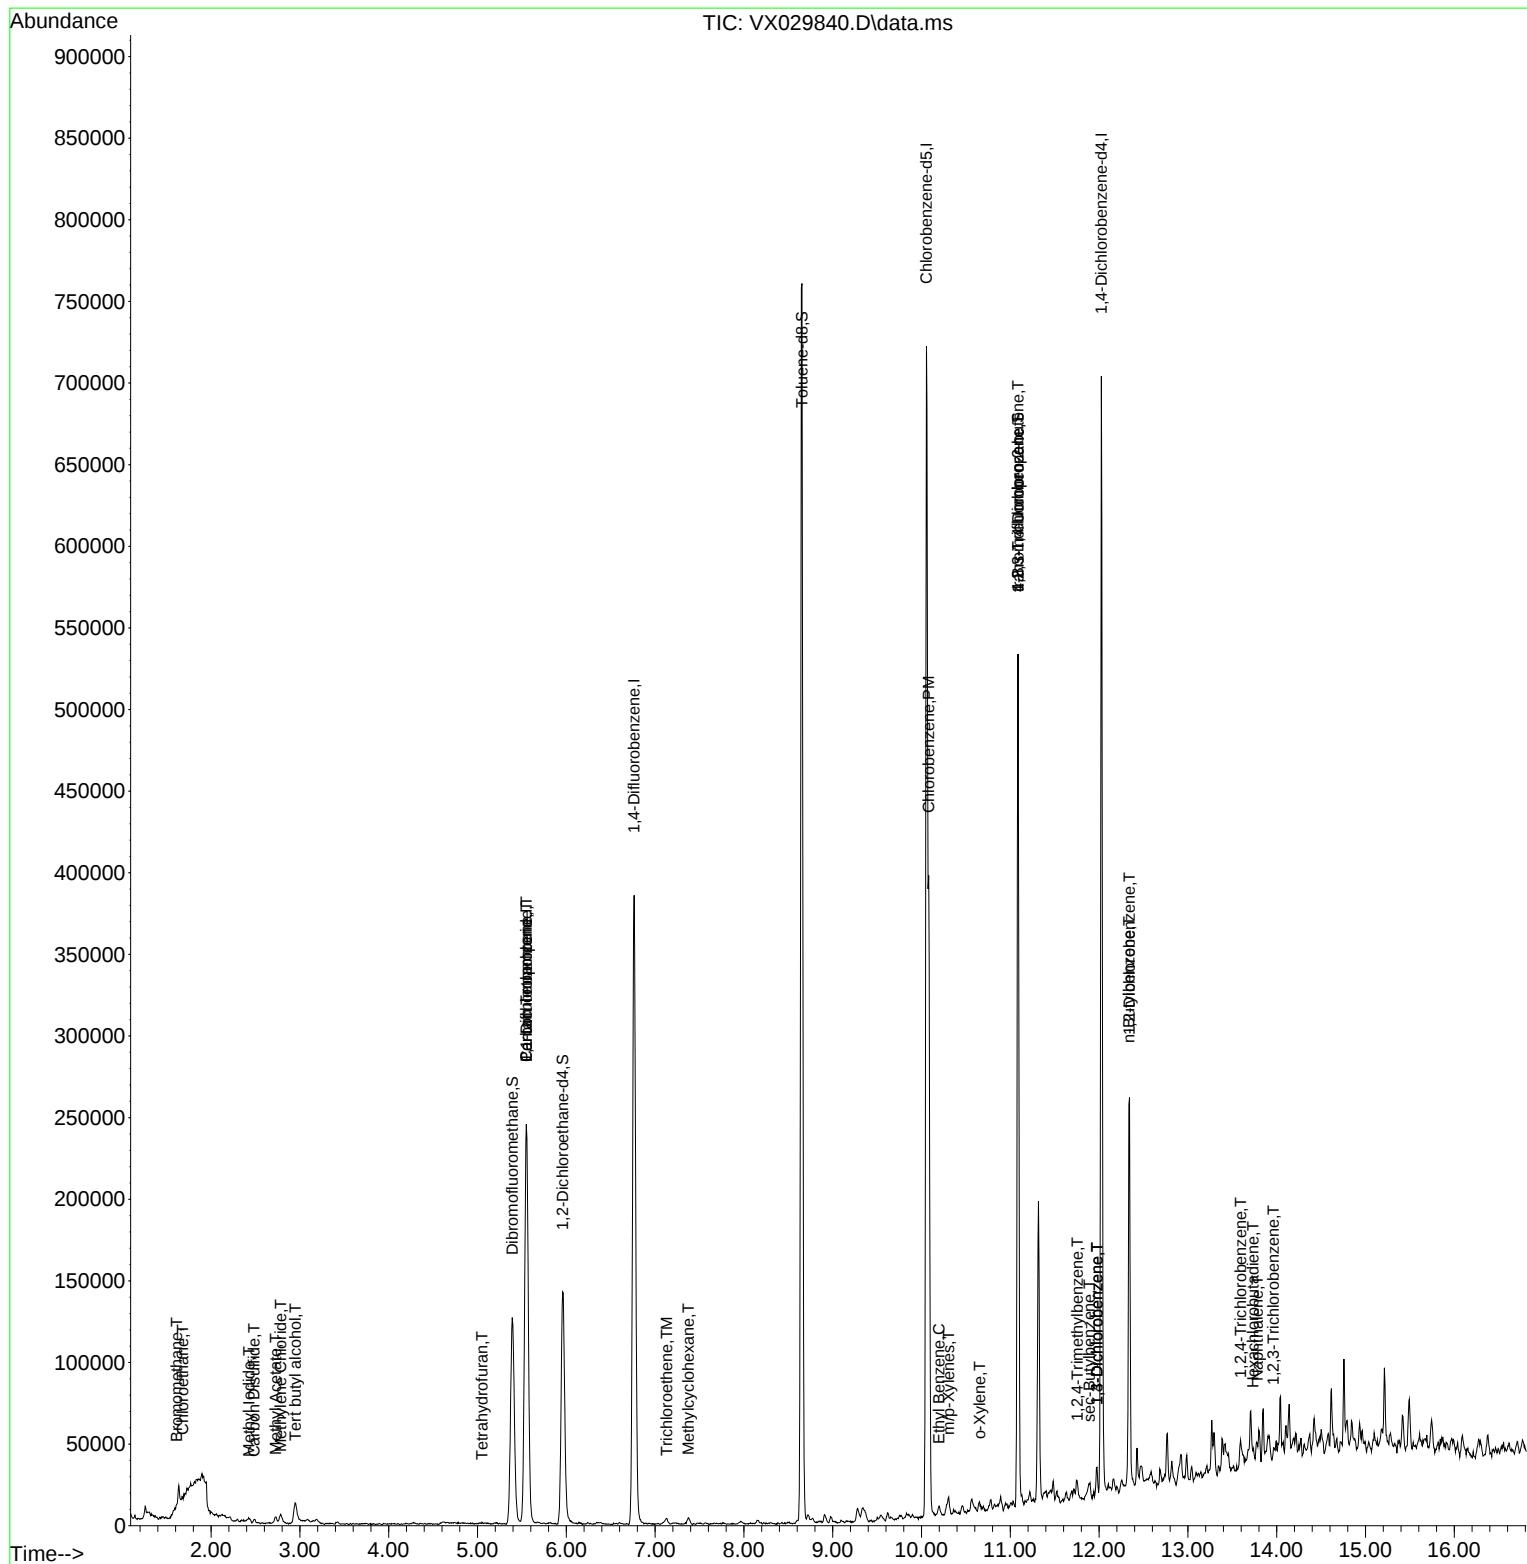




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX029840.D
Acq: 28 Jun 2022 19:49




Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-4-GR


Tgt Ion:168 Resp: 251284
Ion Ratio Lower Upper
168 100
99 51.5 44.0 66.0

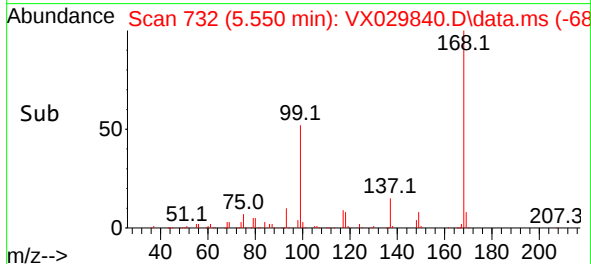

#5
Bromomethane
Concen: 0.661 ug/l
RT: 1.612 min Scan# 86
Delta R.T. 0.000 min
Lab File: VX029840.D
Acq: 28 Jun 2022 19:49

Tgt Ion: 94 Resp: 1022
Ion Ratio Lower Upper
94 100
96 83.7 76.9 115.3


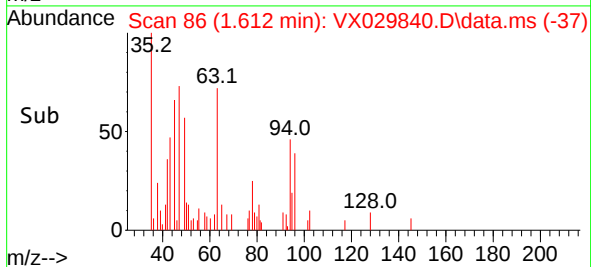

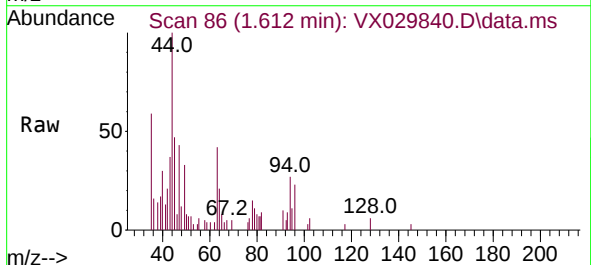


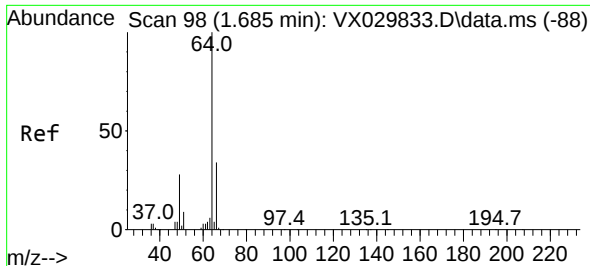

#6
Chloroethane
Concen: 1.131 ug/l
RT: 1.679 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX029840.D
Acq: 28 Jun 2022 19:49




Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-4-GR


Tgt Ion: 64 Resp: 198
Ion Ratio Lower Upper
64 100
66 20.2 27.2 40.8#

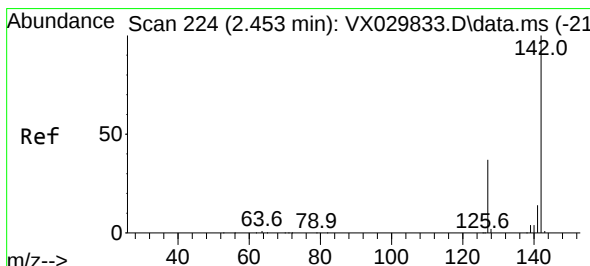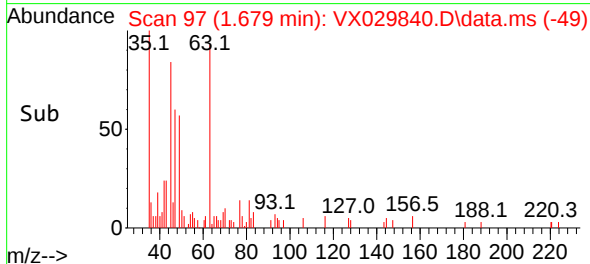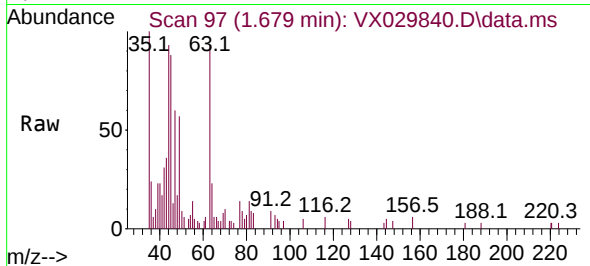

#10
Methyl Iodide
Concen: 2.317 ug/l
RT: 2.429 min Scan# 220
Delta R.T. -0.024 min
Lab File: VX029840.D
Acq: 28 Jun 2022 19:49

Tgt Ion: 142 Resp: 1591
Ion Ratio Lower Upper
142 100
127 36.0 30.2 45.2
141 13.6 11.3 16.9

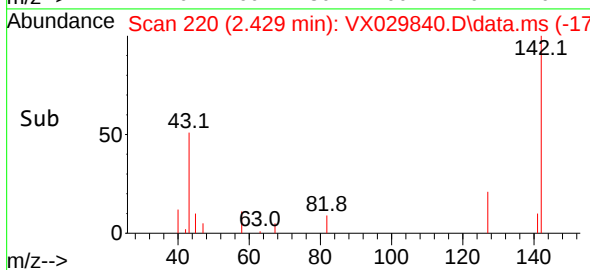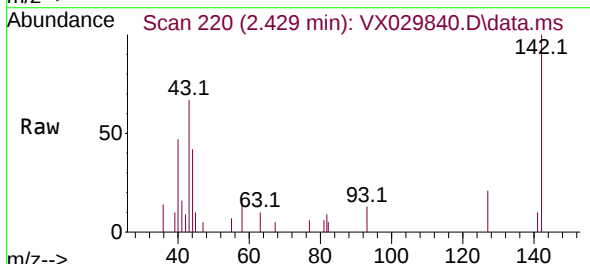

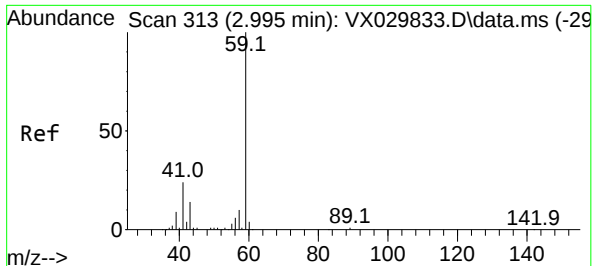

#11

Tert butyl alcohol

Concen: 13.105 ug/l

RT: 2.947 min Scan# 305

Delta R.T. -0.049 min

Lab File: VX029840.D

Acq: 28 Jun 2022 19:49

Instrument :

MSVOA_X

ClientSampleId :





SP-EXC-1-4-GR

Tgt Ion: 59 Resp: 10902

Ion Ratio Lower Upper

59 100

57 2.3 7.4 11.2#

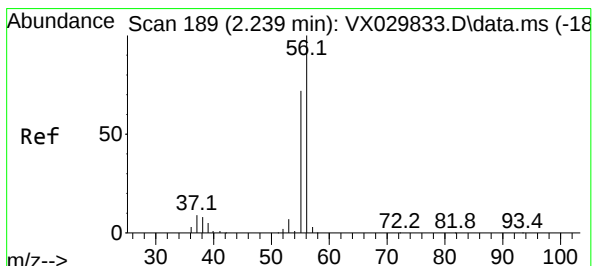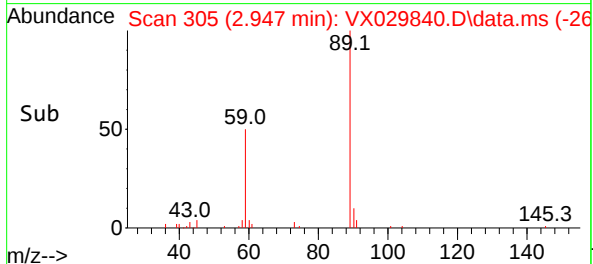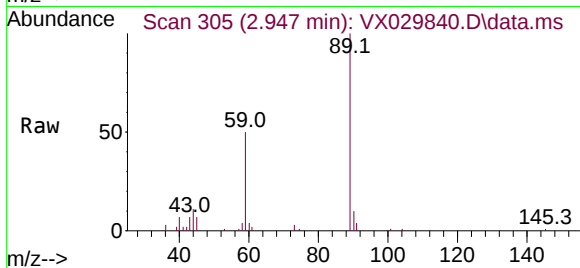

#13

Acrolein

Concen: Below Cal

RT: 2.246 min Scan# 190

Delta R.T. 0.007 min

Lab File: VX029840.D




Acq: 28 Jun 2022 19:49


Tgt Ion: 56 Resp: 88

Ion Ratio Lower Upper

56 100

55 0.0 56.6 84.8#


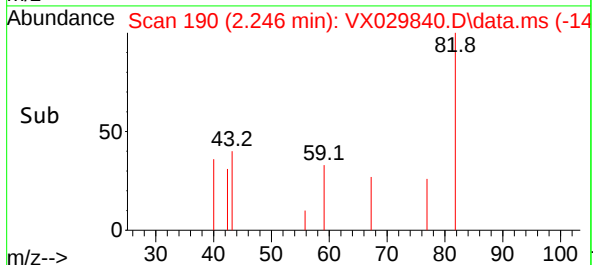

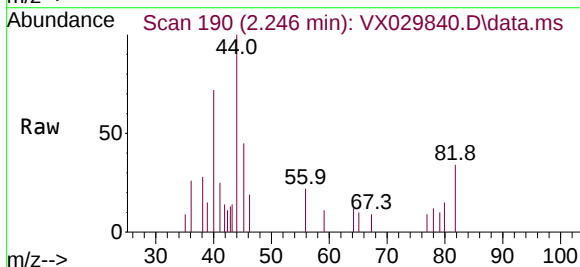




#17
Carbon Disulfide
Concen: 0.386 ug/l
RT: 2.483 min Scan# 21
Delta R.T. -0.030 min
Lab File: VX029840.D
Acq: 28 Jun 2022 19:49




Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-4-GR


Tgt Ion: 76 Resp: 2486
Ion Ratio Lower Upper
76 100
78 10.5 7.8 11.6

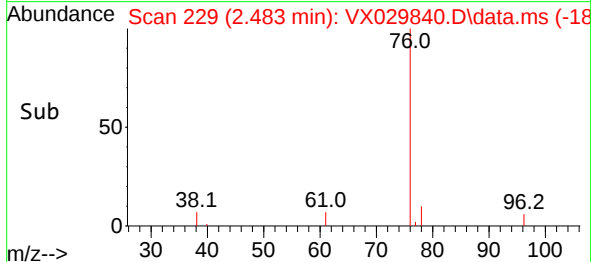

#18
Methyl Acetate
Concen: 1.259 ug/l
RT: 2.727 min Scan# 269
Delta R.T. 0.018 min
Lab File: VX029840.D
Acq: 28 Jun 2022 19:49

Tgt Ion: 43 Resp: 6042
Ion Ratio Lower Upper
43 100
74 20.9 19.4 29.2

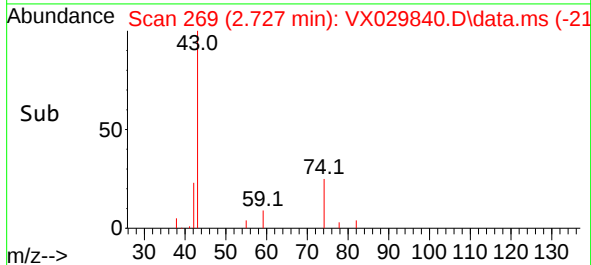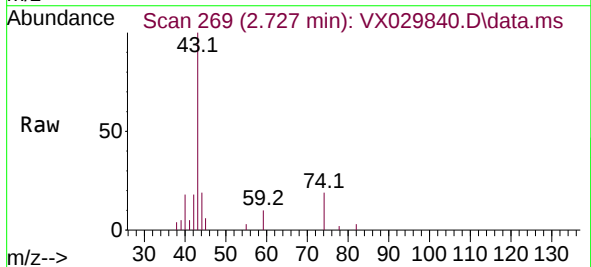




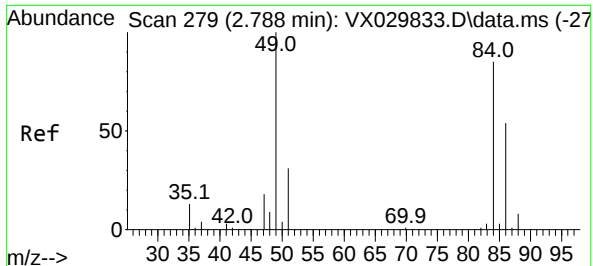


#20
Methylene Chloride
Concen: 0.730 ug/l
RT: 2.782 min Scan# 21
Delta R.T. -0.006 min
Lab File: VX029840.D
Acq: 28 Jun 2022 19:49

Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-4-GR

Tgt Ion: 84 Resp: 2398




Ion	Ratio	Lower	Upper
84	100		
49	102.0	93.8	140.6
51	31.3	29.4	44.0
86	64.1	51.0	76.4

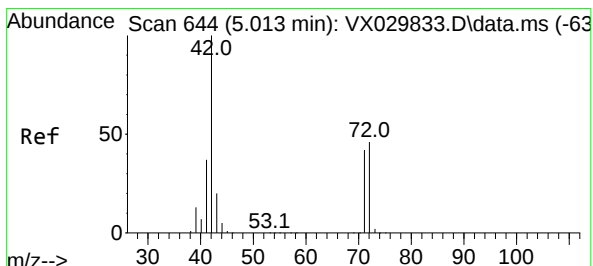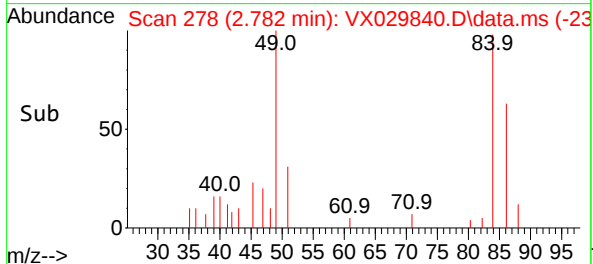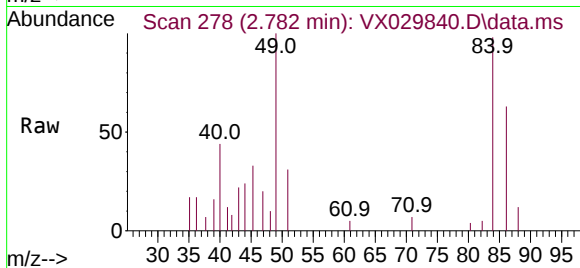


#29
Tetrahydrofuran
Concen: 0.269 ug/l
RT: 5.050 min Scan# 650
Delta R.T. 0.037 min
Lab File: VX029840.D
Acq: 28 Jun 2022 19:49

Tgt Ion: 42 Resp: 478

Ion	Ratio	Lower	Upper
42	100		
72	0.0	36.5	54.7#
71	0.0	33.9	50.9#

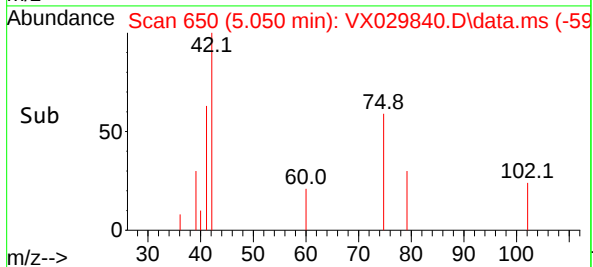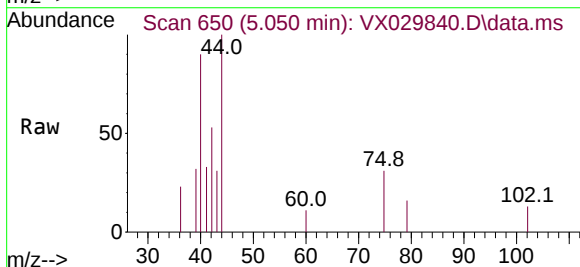



#33

1,2-Dichloroethane-d4

Concen: 42.024 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX029840.D

Acq: 28 Jun 2022 19:49

Instrument :

MSVOA_X

ClientSampleId :





SP-EXC-1-4-GR

Tgt Ion: 65 Resp: 133672

Ion Ratio Lower Upper

65 100

67 55.6 0.0 109.6

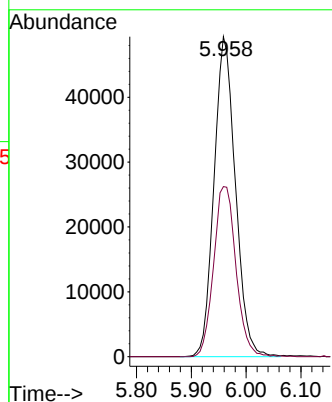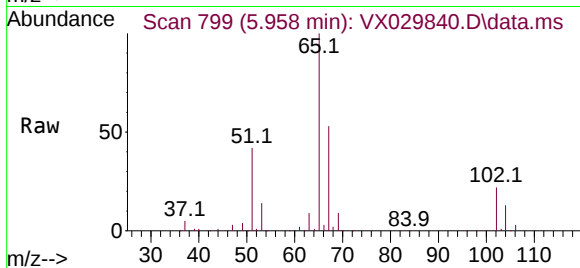

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.000 min

Lab File: VX029840.D

Acq: 28 Jun 2022 19:49




Tgt Ion: 114 Resp: 422294


Ion Ratio Lower Upper

114 100

63 18.6 0.0 38.4

88 14.9 0.0 31.8

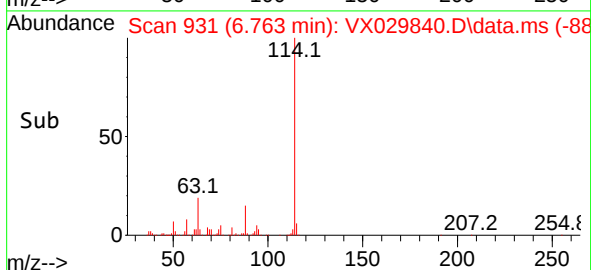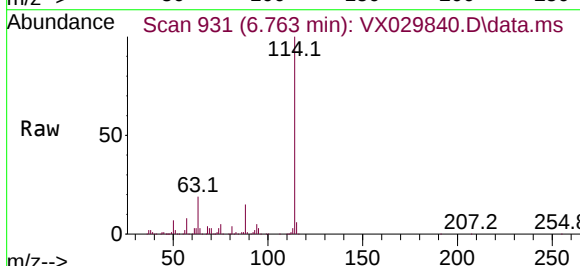

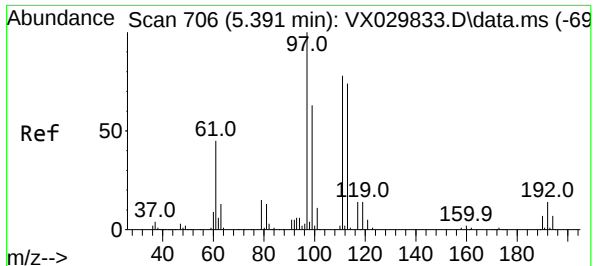

#35

Dibromofluoromethane

Concen: 44.309 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.000 min

Lab File: VX029840.D

Acq: 28 Jun 2022 19:49

Instrument :

MSVOA_X

ClientSampleId :

SP-EXC-1-4-GR





Tgt Ion:113 Resp: 116937

Ion Ratio Lower Upper

113 100

111 102.5 83.2 124.8

192 18.9 14.8 22.2

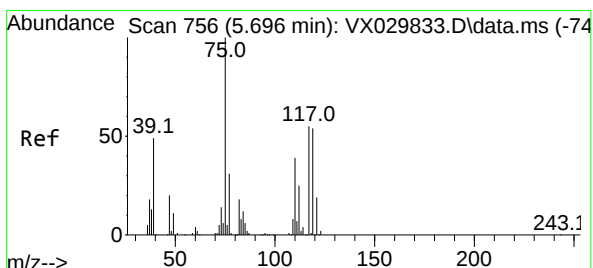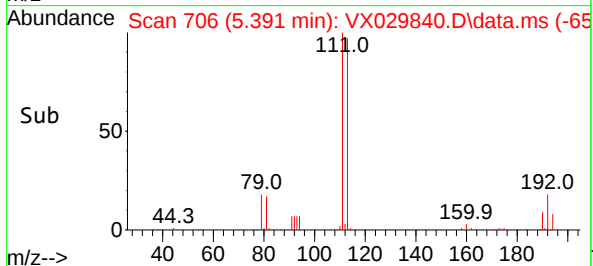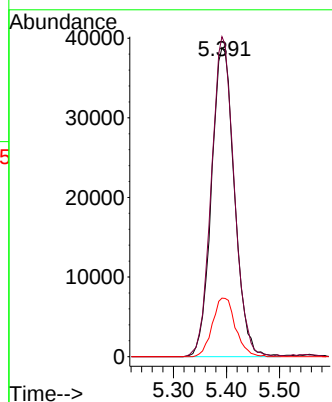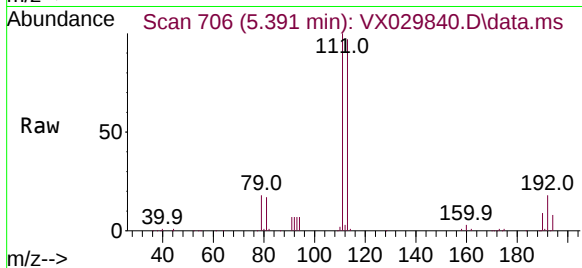

#36

1,1-Dichloropropene

Concen: 5.258 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.146 min

Lab File: VX029840.D

Acq: 28 Jun 2022 19:49




Tgt Ion: 75 Resp: 18457


Ion Ratio Lower Upper

75 100

110 9.2 19.3 57.9#

77 0.5 24.4 36.6#


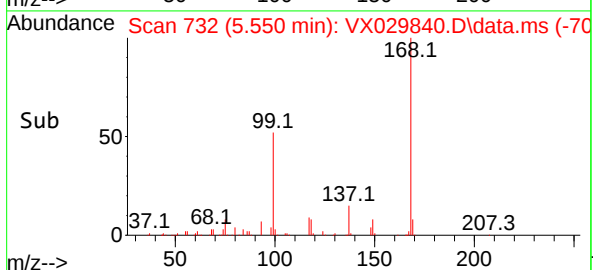

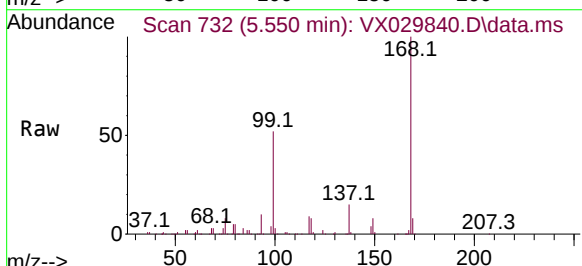


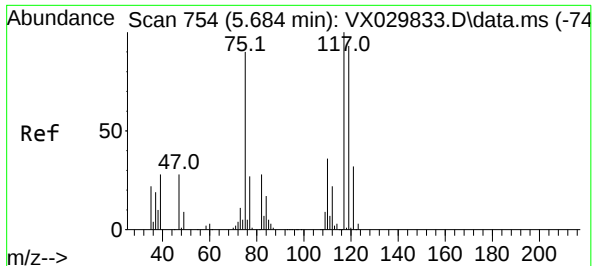

#38
Carbon Tetrachloride
Concen: 7.462 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.134 min
Lab File: VX029840.D
Acq: 28 Jun 2022 19:49




Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-4-GR


Tgt Ion:117 Resp: 22695
Ion Ratio Lower Upper
117 100
119 5.7 74.1 111.1#
121 0.0 25.8 38.8#

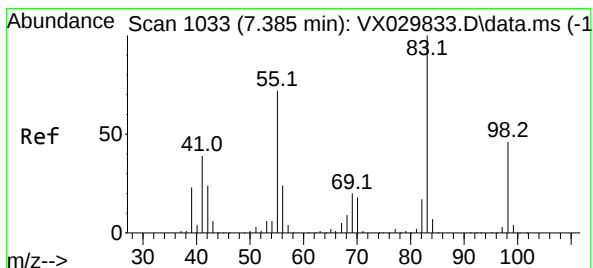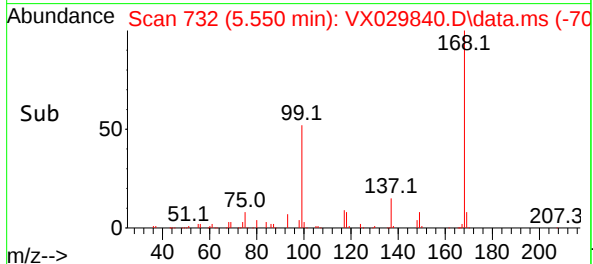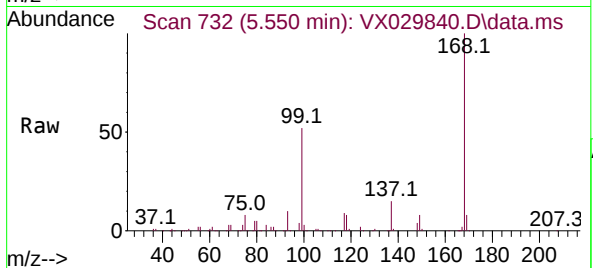

#39
Methylcyclohexane
Concen: 0.398 ug/l
RT: 7.373 min Scan# 1031
Delta R.T. -0.012 min
Lab File: VX029840.D
Acq: 28 Jun 2022 19:49

Tgt Ion: 83 Resp: 1687
Ion Ratio Lower Upper
83 100
55 85.3 57.7 86.5
98 35.6 36.5 54.7#


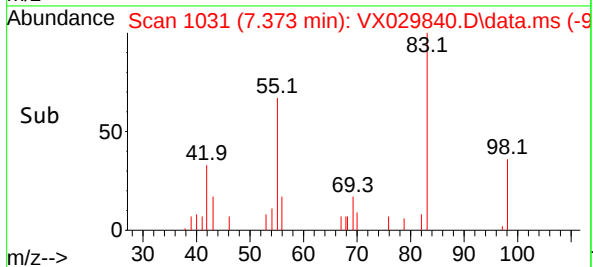

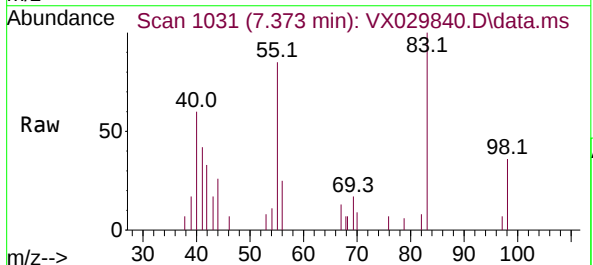


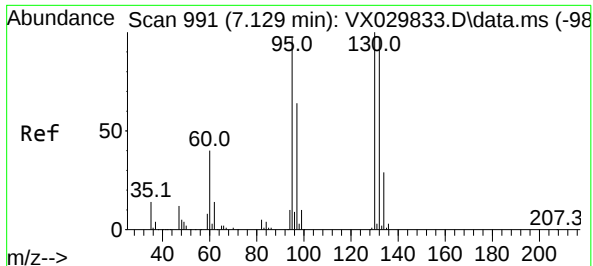

#44
 Trichloroethene
 Concen: 0.512 ug/l
 RT: 7.129 min Scan# 991
 Delta R.T. 0.000 min
 Lab File: VX029840.D
 Acq: 28 Jun 2022 19:49




Instrument :
 MSVOA_X
 ClientSampleId :
 SP-EXC-1-4-GR


Tgt Ion:130 Resp: 1566
 Ion Ratio Lower Upper
 130 100
 95 97.7 0.0 194.8

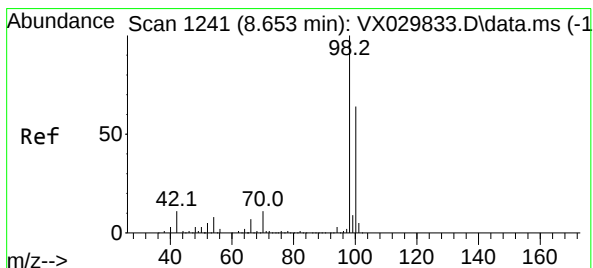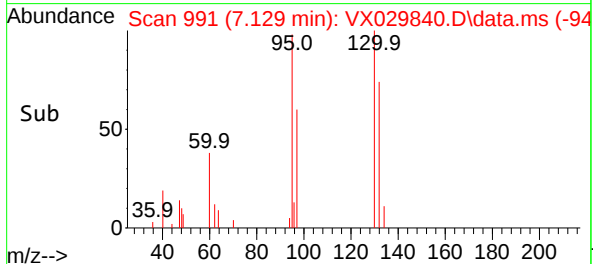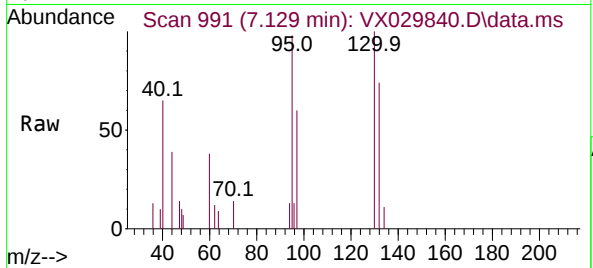

#50
 Toluene-d8
 Concen: 48.349 ug/l
 RT: 8.653 min Scan# 1241
 Delta R.T. 0.000 min
 Lab File: VX029840.D
 Acq: 28 Jun 2022 19:49

Tgt Ion: 98 Resp: 478680
 Ion Ratio Lower Upper
 98 100
 100 65.0 52.3 78.5


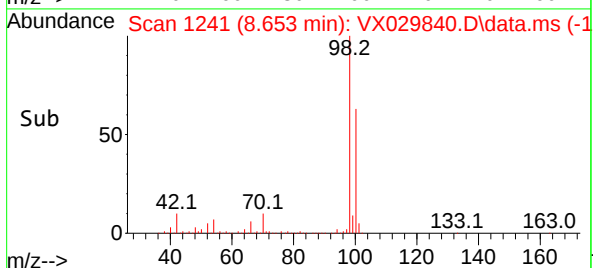

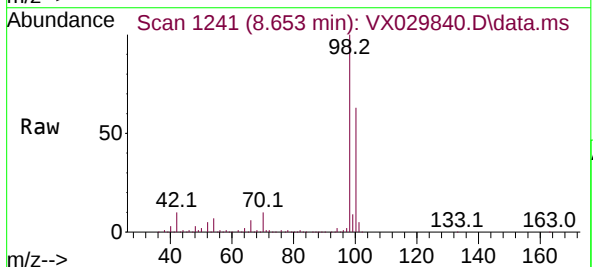




#62
4-Bromofluorobenzene
Concen: 43.715 ug/l
RT: 11.085 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX029840.D
Acq: 28 Jun 2022 19:49




Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-4-GR


Tgt Ion: 95 Resp: 152990
Ion Ratio Lower Upper
95 100
174 74.6 0.0 149.0
176 71.2 0.0 146.0

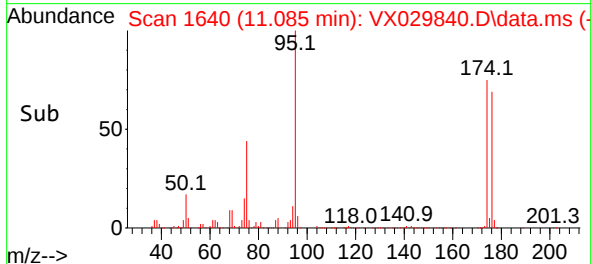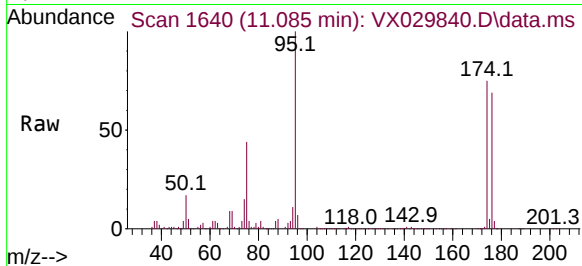

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX029840.D
Acq: 28 Jun 2022 19:49

Tgt Ion: 117 Resp: 345462
Ion Ratio Lower Upper
117 100
82 53.8 42.7 64.1
119 31.9 25.4 38.2


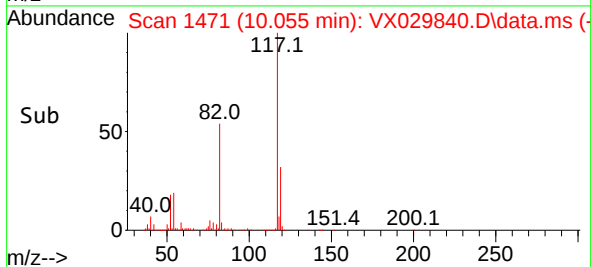

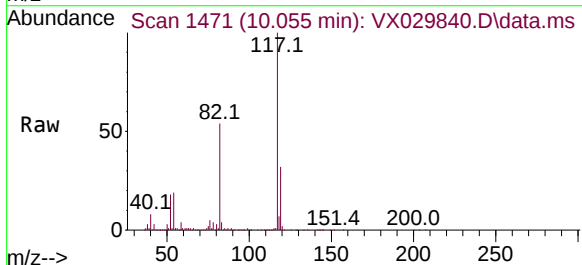




#65
Chlorobenzene
Concen: 23.869 ug/l
RT: 10.080 min Scan# 1475
Delta R.T. 0.000 min
Lab File: VX029840.D
Acq: 28 Jun 2022 19:49




Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-4-GR


Tgt Ion:112 Resp: 165524
Ion Ratio Lower Upper
112 100
114 31.8 24.6 36.8

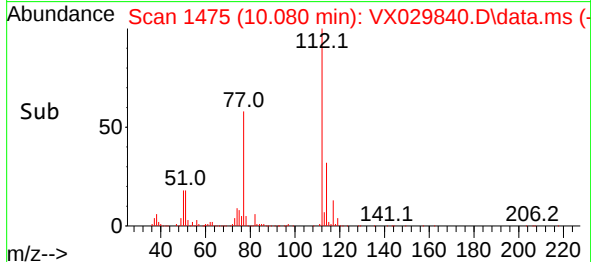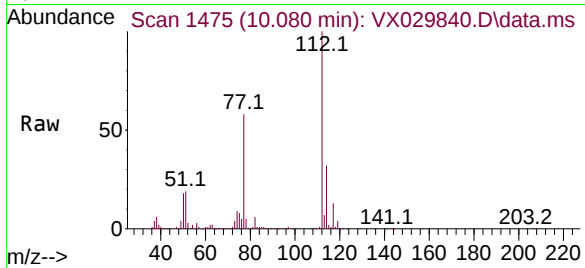

#67
Ethyl Benzene
Concen: 0.280 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX029840.D
Acq: 28 Jun 2022 19:49

Tgt Ion: 91 Resp: 3374
Ion Ratio Lower Upper
91 100
106 29.6 25.5 38.3


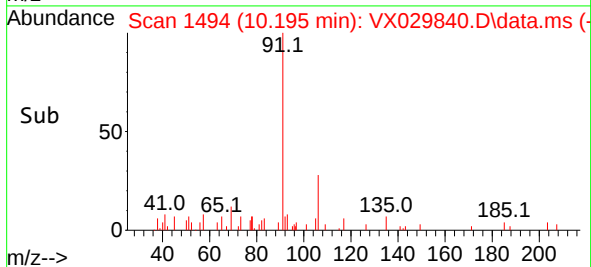

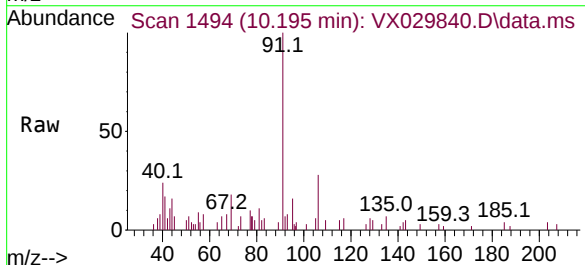




#68
m/p-Xylenes
Concen: 0.432 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX029840.D
Acq: 28 Jun 2022 19:49




Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-4-GR


Tgt Ion:106 Resp: 1999
Ion Ratio Lower Upper
106 100
91 207.5 158.2 237.4

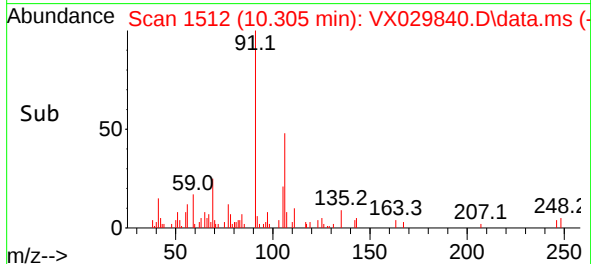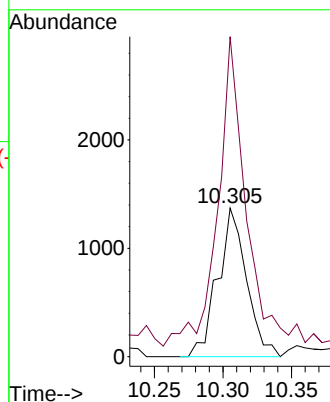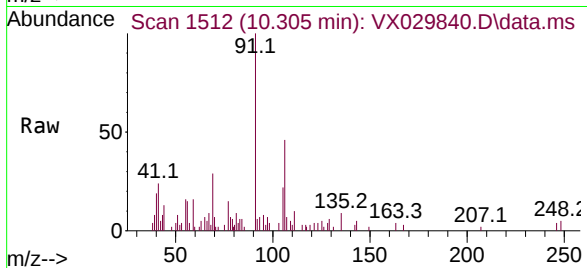

#69
o-Xylene
Concen: 0.234 ug/l
RT: 10.653 min Scan# 1569
Delta R.T. 0.006 min
Lab File: VX029840.D
Acq: 28 Jun 2022 19:49

Tgt Ion:106 Resp: 1096
Ion Ratio Lower Upper
106 100
91 183.2 103.8 311.6


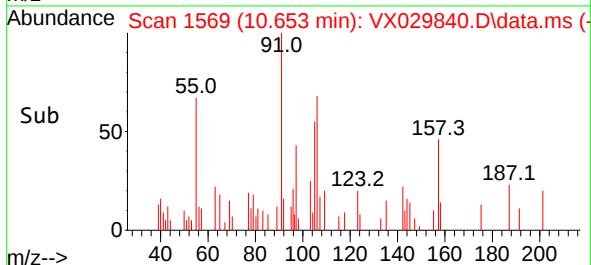

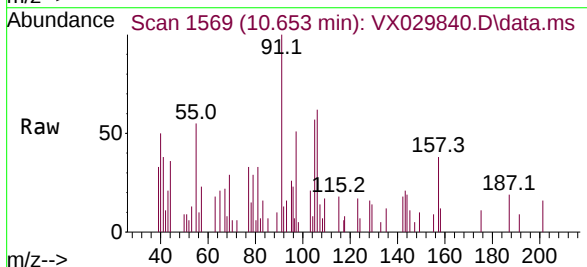


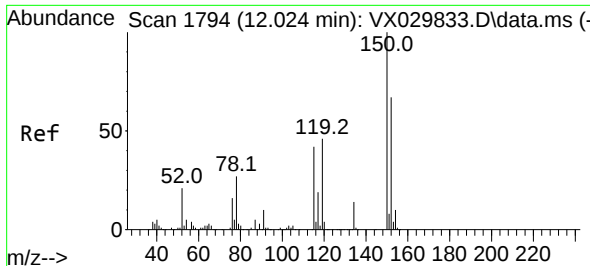

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX029840.D
 Acq: 28 Jun 2022 19:49




Instrument :
 MSVOA_X
 ClientSampleId :
 SP-EXC-1-4-GR


Tgt Ion:152 Resp: 145067
 Ion Ratio Lower Upper
 152 100
 115 58.3 40.5 121.5
 150 156.1 0.0 347.0

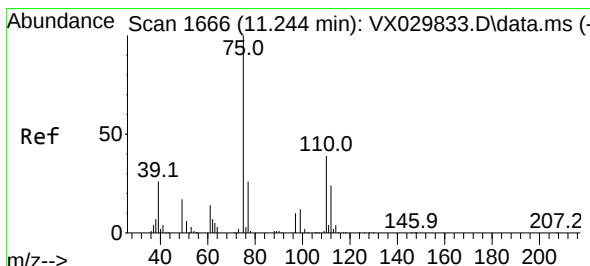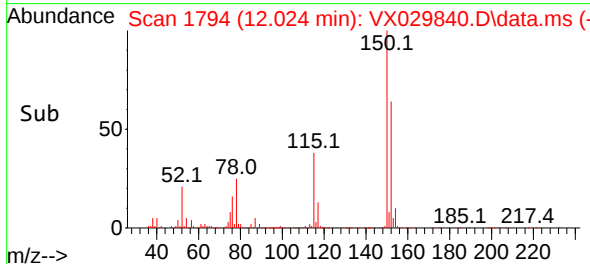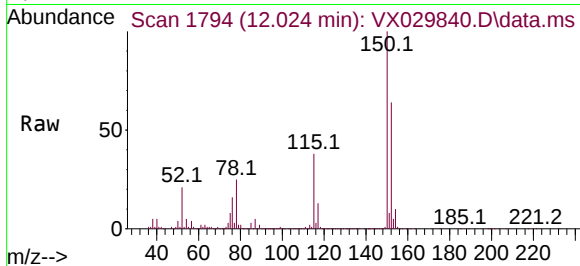

#76
 1,2,3-Trichloropropane
 Concen: 19.862 ug/l
 RT: 11.085 min Scan# 1640
 Delta R.T. -0.158 min
 Lab File: VX029840.D
 Acq: 28 Jun 2022 19:49

Tgt Ion: 75 Resp: 68974
 Ion Ratio Lower Upper
 75 100
 77 1.4 19.8 59.3#


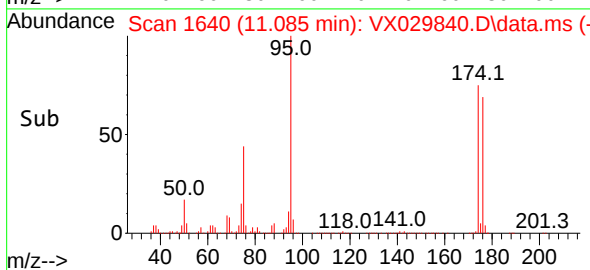

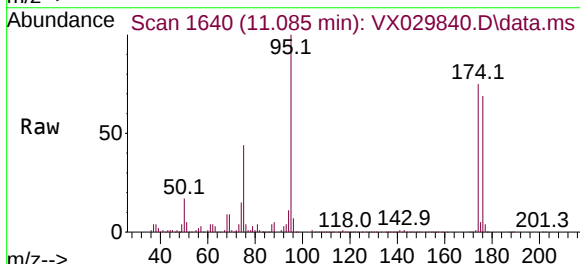




#81
trans-1,4-Dichloro-2-butene
Concen: 63.076 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.067 min
Lab File: VX029840.D
Acq: 28 Jun 2022 19:49




Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-4-GR


Tgt Ion: 75 Resp: 68974
Ion Ratio Lower Upper
75 100
53 0.2 74.2 111.4#
89 0.1 34.8 52.2#

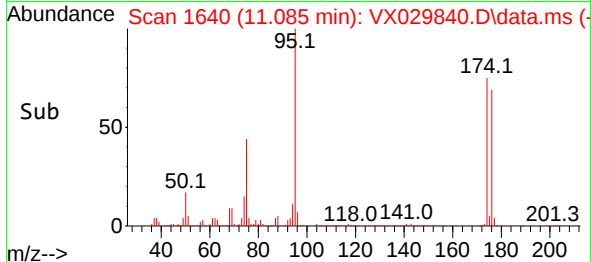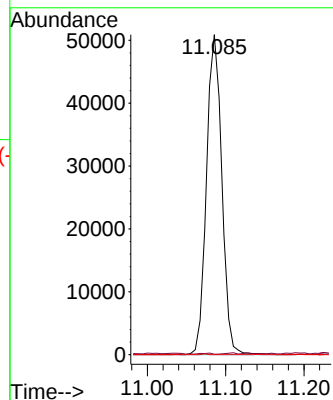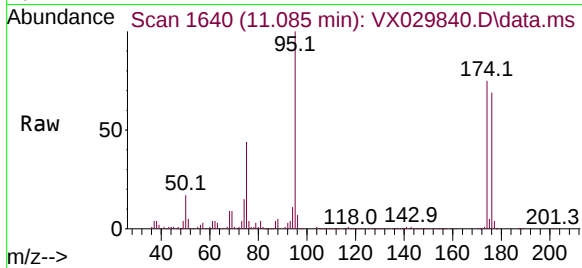

#84
1,2,4-Trimethylbenzene
Concen: 0.277 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.000 min
Lab File: VX029840.D
Acq: 28 Jun 2022 19:49

Tgt Ion: 105 Resp: 2417
Ion Ratio Lower Upper
105 100
120 32.8 22.9 68.8


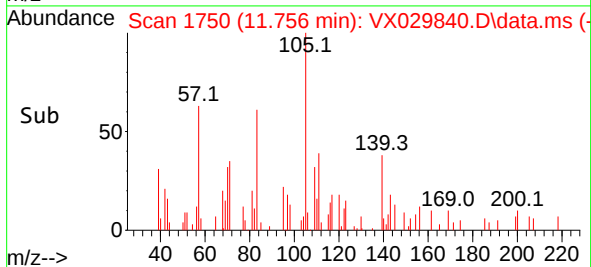
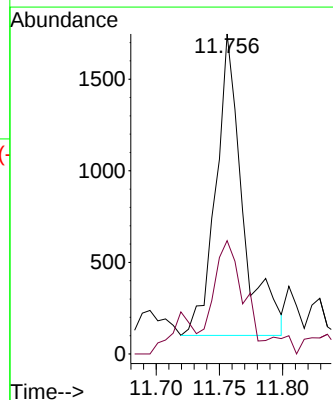
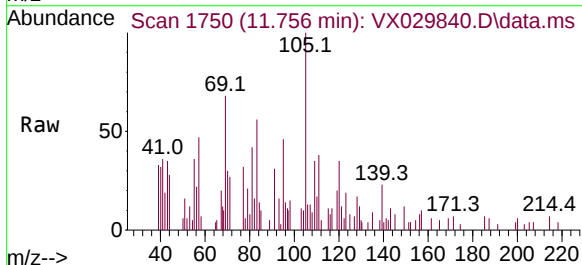




#85
 sec-Butylbenzene
 Concen: 0.211 ug/l
 RT: 11.890 min Scan# 1772
 Delta R.T. 0.000 min
 Lab File: VX029840.D
 Acq: 28 Jun 2022 19:49




Instrument :
 MSVOA_X
 ClientSampleId :
 SP-EXC-1-4-GR


Tgt Ion:105 Resp: 2300
 Ion Ratio Lower Upper
 105 100
 134 26.3 10.0 30.0

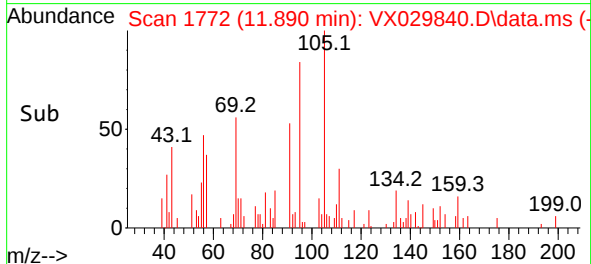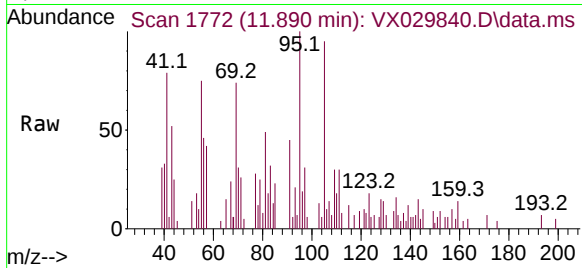

#87
 1,3-Dichlorobenzene
 Concen: 0.823 ug/l
 RT: 11.976 min Scan# 1786
 Delta R.T. 0.006 min
 Lab File: VX029840.D
 Acq: 28 Jun 2022 19:49

Tgt Ion:146 Resp: 3991
 Ion Ratio Lower Upper
 146 100
 111 55.1 20.3 60.8
 148 62.4 31.8 95.3


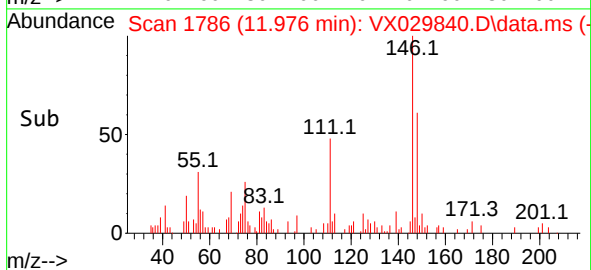

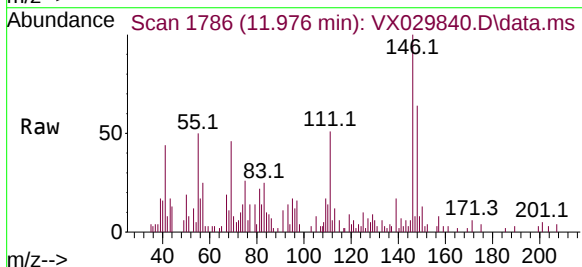




#88
1,4-Dichlorobenzene
Concen: 0.807 ug/l
RT: 11.976 min Scan# 1797
Delta R.T. -0.067 min
Lab File: VX029840.D
Acq: 28 Jun 2022 19:49




Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-4-GR


Tgt Ion:146 Resp: 3991
Ion Ratio Lower Upper
146 100
111 49.8 20.3 60.9
148 62.4 32.3 96.8

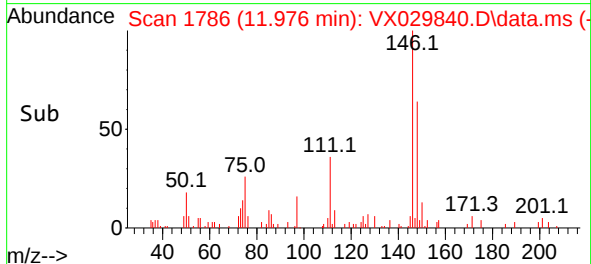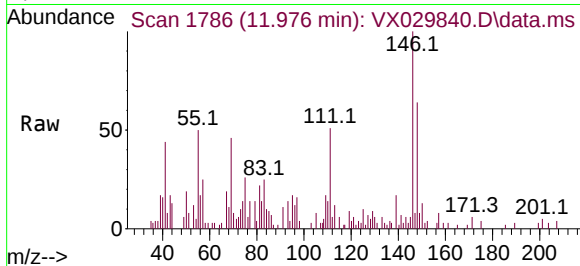

#89
n-Butylbenzene
Concen: 0.272 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX029840.D
Acq: 28 Jun 2022 19:49

Tgt Ion: 91 Resp: 2218
Ion Ratio Lower Upper
91 100
92 44.9 26.2 78.5
134 44.2 12.6 37.8#

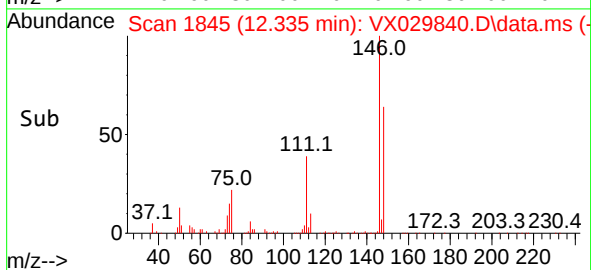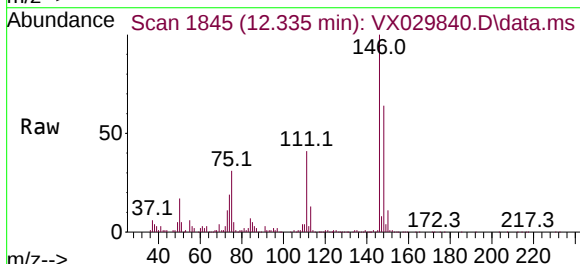



#91

1,2-Dichlorobenzene

Concen: 16.256 ug/l

RT: 12.341 min Scan# 1846

Delta R.T. 0.006 min

Lab File: VX029840.D

Acq: 28 Jun 2022 19:49

Instrument :

MSVOA_X

ClientSampleId :

SP-EXC-1-4-GR





Tgt Ion:146 Resp: 77415

Ion Ratio Lower Upper

146 100

111 41.3 20.7 62.1

148 64.3 32.0 96.2

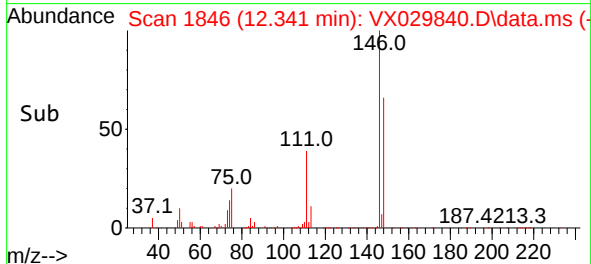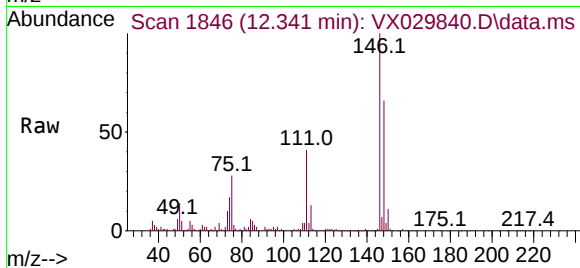

#93

1,2,4-Trichlorobenzene

Concen: 0.858 ug/l

RT: 13.591 min Scan# 2051

Delta R.T. 0.000 min

Lab File: VX029840.D

Acq: 28 Jun 2022 19:49




Tgt Ion:180 Resp: 2475


Ion Ratio Lower Upper

180 100

182 106.7 48.2 144.6

145 40.2 15.9 47.6

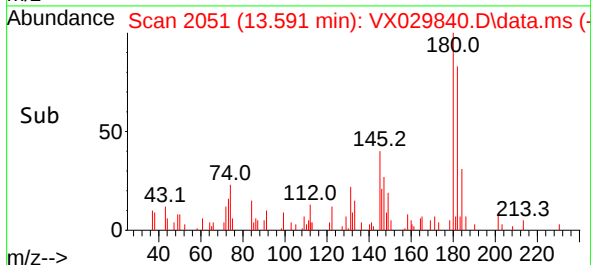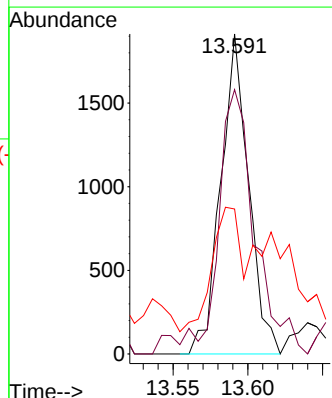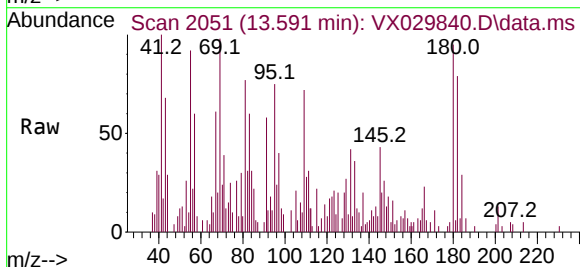



#94

Hexachlorobutadiene

Concen: 0.259 ug/l

RT: 13.731 min Scan# 2073

Delta R.T. 0.006 min

Lab File: VX029840.D

Acq: 28 Jun 2022 19:49

Instrument :

MSVOA_X

ClientSampleId :

SP-EXC-1-4-GR





Tgt Ion:225 Resp: 277

Ion Ratio Lower Upper

225 100

223 25.6 30.6 91.6#

227 0.0 31.9 95.9#

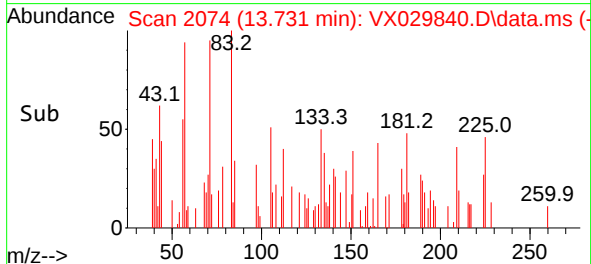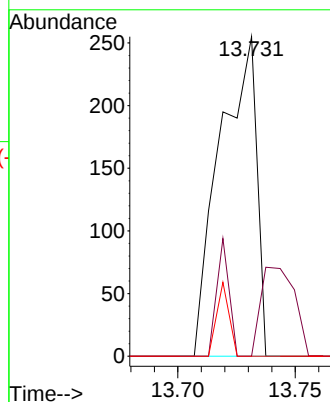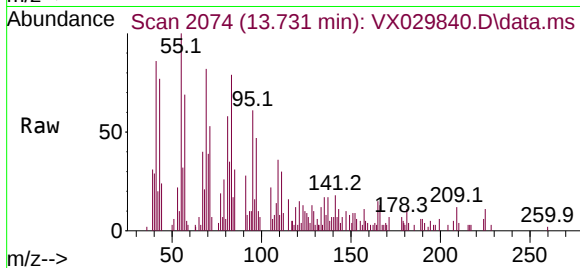

#95

Naphthalene

Concen: 0.494 ug/l

RT: 13.780 min Scan# 2082

Delta R.T. 0.000 min

Lab File: VX029840.D

Acq: 28 Jun 2022 19:49




Tgt Ion:128 Resp: 5792


Ion Ratio Lower Upper

128 100

127 18.0 10.2 15.2#

129 10.2 8.6 13.0

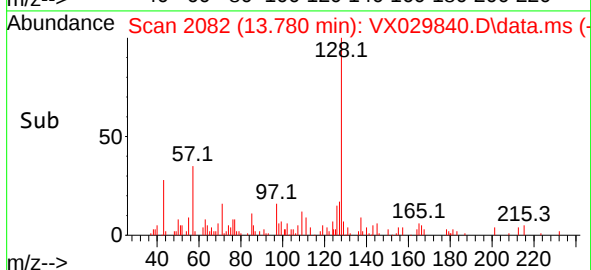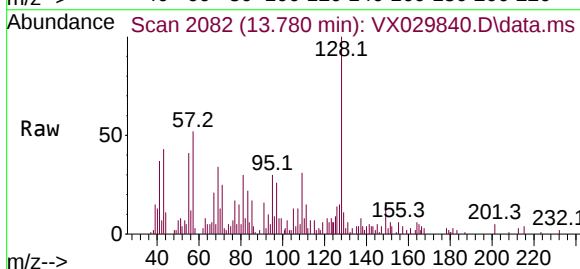

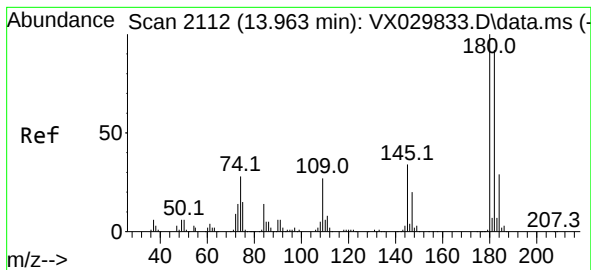

#96
 1,2,3-Trichlorobenzene
 Concen: 0.639 ug/l
 RT: 13.963 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VX029840.D
 Acq: 28 Jun 2022 19:49

Instrument :
 MSVOA_X
 ClientSampleId :
 SP-EXC-1-4-GR

Tgt Ion:180 Resp: 1887
 Ion Ratio Lower Upper
 180 100
 182 85.0 47.0 141.0
 145 64.6 17.0 50.9#

