

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062822\
 Data File : VX029845.D
 Acq On : 28 Jun 2022 21:46
 Operator : JC/MD
 Sample : N3494-34
 Misc : 5.67g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SP-EXC-1-1-GR

Quant Time: Jun 29 06:09:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 29 05:54:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	263143	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	440532	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	372354	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	166062	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	138159	41.477	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	82.960%		
35) Dibromofluoromethane	5.391	113	119350	43.351	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	86.700%		
50) Toluene-d8	8.647	98	500690	48.478	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	96.960%		
62) 4-Bromofluorobenzene	11.085	95	162038	44.384	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	88.760%		
Target Compounds						Qvalue
5) Bromomethane	1.612	94	736	0.454	ug/l #	76
6) Chloroethane	1.679	64	237	1.144	ug/l #	87
10) Methyl Iodide	2.447	142	620	2.038	ug/l #	72
11) Tert butyl alcohol	2.947	59	15997	18.364	ug/l #	77
13) Acrolein	2.191	56	54	Below Cal	#	1
16) Acetone	2.429	43	1054	0.647	ug/l #	68
18) Methyl Acetate	2.727	43	5234	1.042	ug/l	98
20) Methylene Chloride	2.782	84	1057	0.307	ug/l	85
31) Cyclohexane	5.477	56	2715	0.585	ug/l #	69
36) 1,1-Dichloropropene	5.544	75	18868	5.153	ug/l #	47
38) Carbon Tetrachloride	5.550	117	24517	7.727	ug/l #	18
39) Methylcyclohexane	7.373	83	2171	0.490	ug/l #	75
40) Benzene	6.032	78	4349	0.367	ug/l	94
44) Trichloroethene	7.123	130	1436	0.450	ug/l	64
49) 1,4-Dioxane	7.531	88	28	0.331	ug/l #	1
52) Toluene	8.720	92	2348	0.329	ug/l	100
65) Chlorobenzene	10.080	112	51430	6.881	ug/l	99
67) Ethyl Benzene	10.195	91	4297	0.331	ug/l #	88
68) m/p-Xylenes	10.305	106	3929	0.788	ug/l	92
69) o-Xylene	10.653	106	1316	0.261	ug/l	63
76) 1,2,3-Trichloropropane	11.085	75	74706	18.793	ug/l #	39
77) Bromobenzene	11.201	156	609	0.211	ug/l #	49
81) trans-1,4-Dichloro-2-b...	11.085	75	74706	59.681	ug/l #	13
84) 1,2,4-Trimethylbenzene	11.756	105	2290	0.229	ug/l	80
87) 1,3-Dichlorobenzene	11.976	146	5489	0.989	ug/l	90
88) 1,4-Dichlorobenzene	12.049	146	13278	2.345	ug/l	79
90) Hexachloroethane	12.549	117	356	0.219	ug/l	67
91) 1,2-Dichlorobenzene	12.341	146	90120	16.531	ug/l	99
93) 1,2,4-Trichlorobenzene	13.591	180	1172	0.355	ug/l #	61

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062822\
Data File : VX029845.D
Acq On : 28 Jun 2022 21:46
Operator : JC/MD
Sample : N3494-34
Misc : 5.67g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-1-GR

Quant Time: Jun 29 06:09:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 29 05:54:51 2022
Response via : Initial Calibration




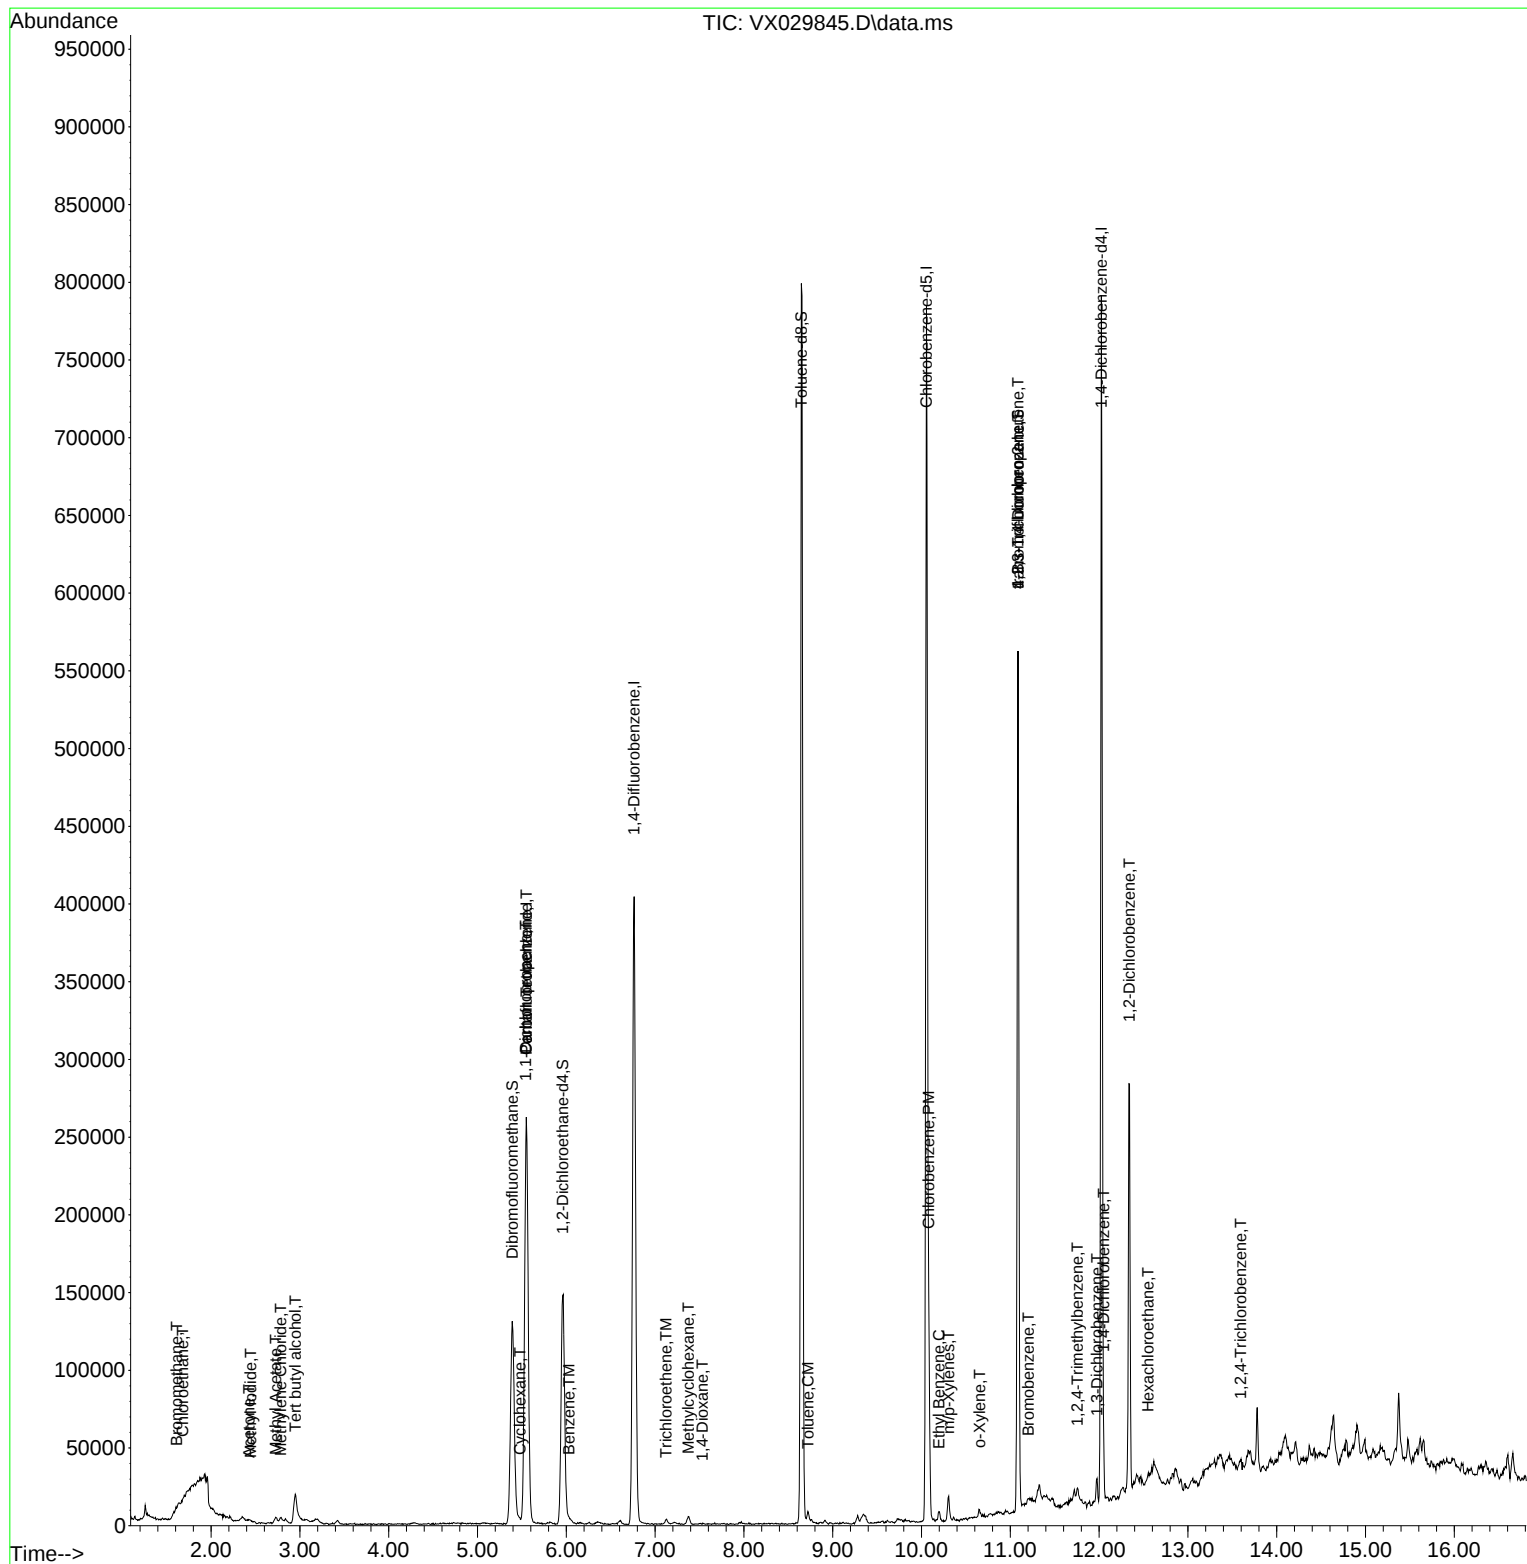




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX029845.D
Acq: 28 Jun 2022 21:46




Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-1-GR


Tgt Ion:168 Resp: 263143
Ion Ratio Lower Upper
168 100
99 52.0 44.0 66.0

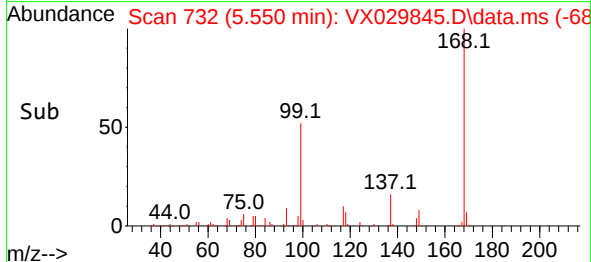

#5
Bromomethane
Concen: 0.454 ug/l
RT: 1.612 min Scan# 86
Delta R.T. 0.000 min
Lab File: VX029845.D
Acq: 28 Jun 2022 21:46

Tgt Ion: 94 Resp: 736
Ion Ratio Lower Upper
94 100
96 73.1 76.9 115.3#


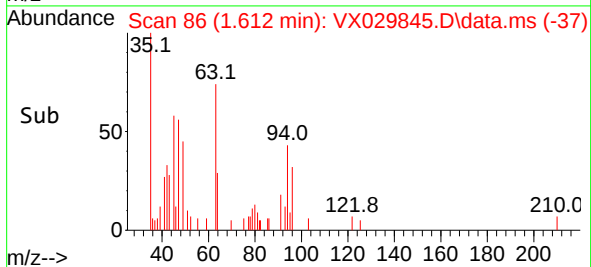

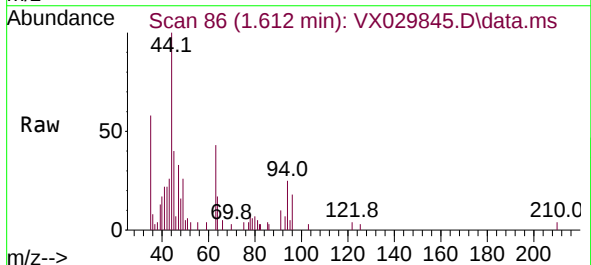


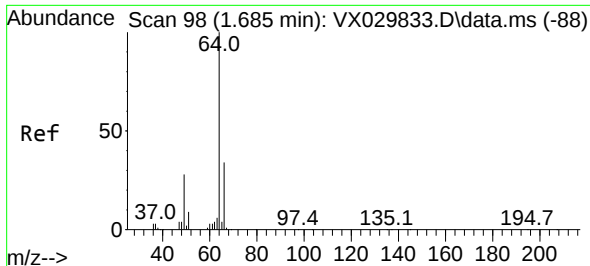

#6
Chloroethane
Concen: 1.144 ug/l
RT: 1.679 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX029845.D
Acq: 28 Jun 2022 21:46




Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-1-GR

Tgt Ion: 64 Resp: 237
Ion Ratio Lower Upper
64 100
66 41.5 27.2 40.8#

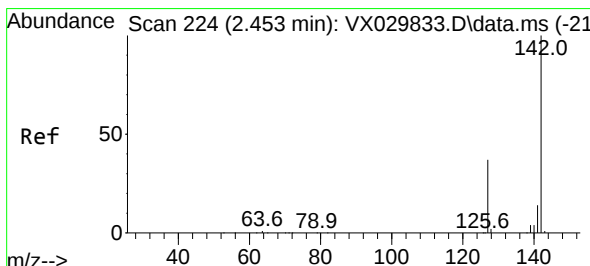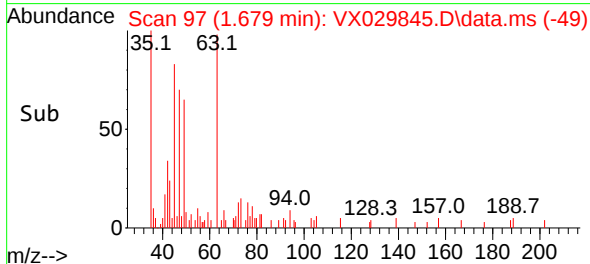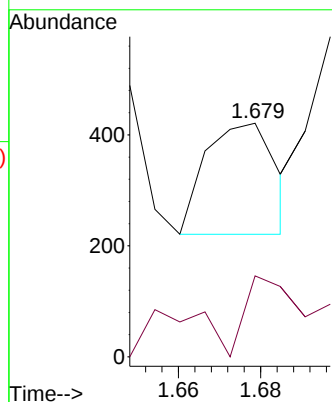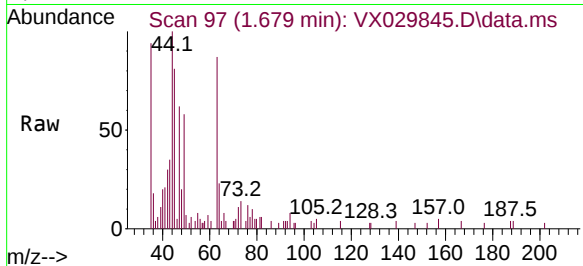

#10
Methyl Iodide
Concen: 2.038 ug/l
RT: 2.447 min Scan# 223
Delta R.T. -0.006 min
Lab File: VX029845.D
Acq: 28 Jun 2022 21:46

Tgt Ion: 142 Resp: 620
Ion Ratio Lower Upper
142 100
127 22.1 30.2 45.2#
141 0.0 11.3 16.9#

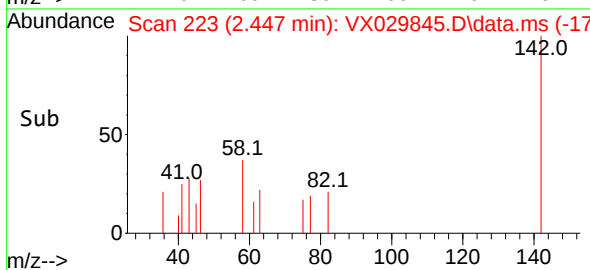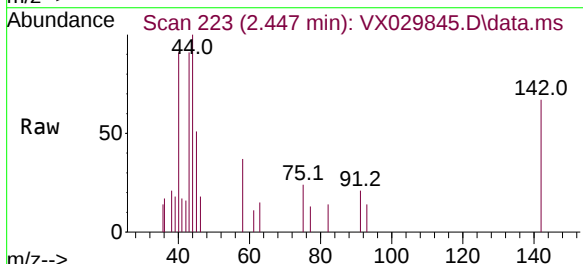



#11

Tert butyl alcohol

Concen: 18.364 ug/l

RT: 2.947 min Scan# 305

Delta R.T. -0.049 min

Lab File: VX029845.D

Acq: 28 Jun 2022 21:46

Instrument :

MSVOA_X

ClientSampleId :





SP-EXC-1-1-GR

Tgt Ion: 59 Resp: 15997

Ion Ratio Lower Upper

59 100

57 0.9 7.4 11.2#

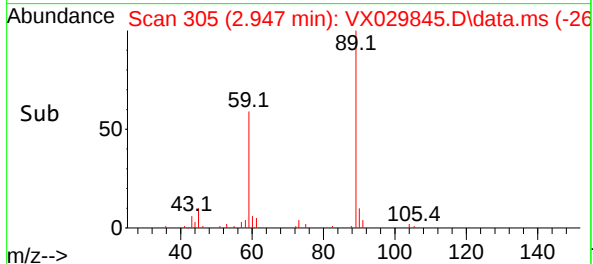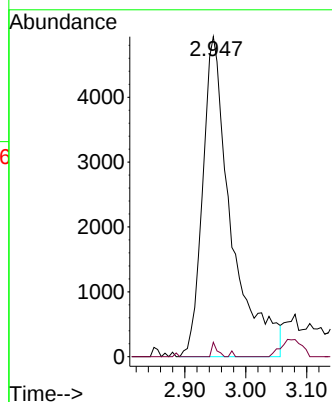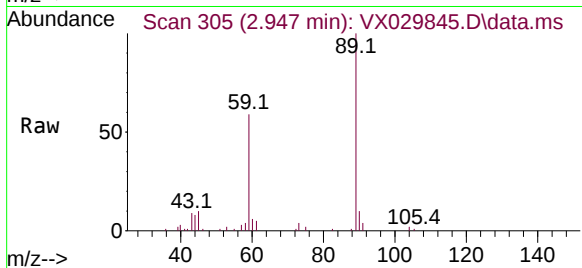

#13

Acrolein

Concen: Below Cal

RT: 2.191 min Scan# 181

Delta R.T. -0.048 min

Lab File: VX029845.D




Acq: 28 Jun 2022 21:46


Tgt Ion: 56 Resp: 54

Ion Ratio Lower Upper

56 100

55 190.7 56.6 84.8#


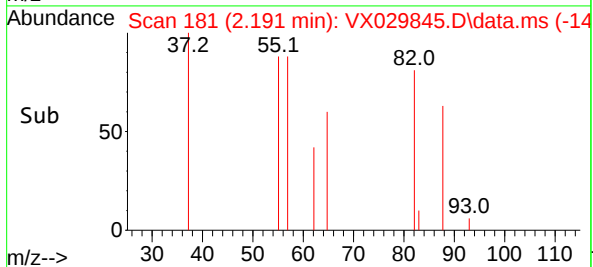
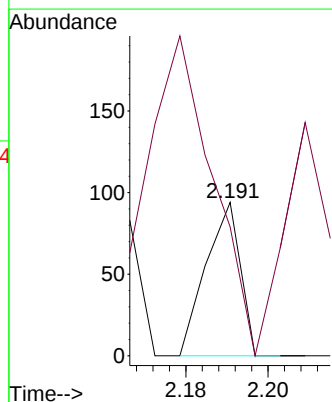
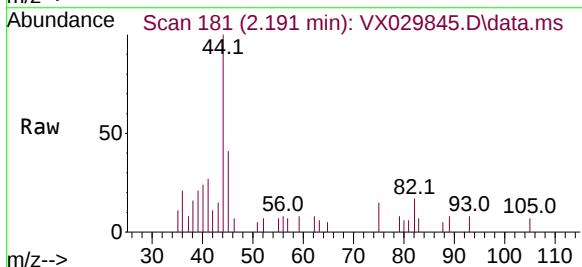


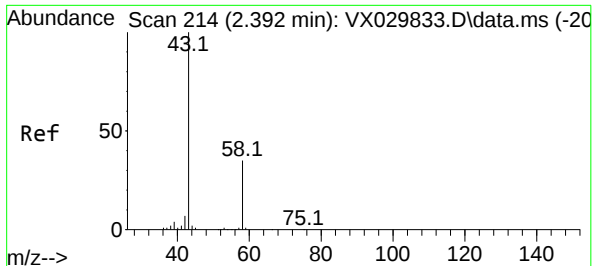

#16
Acetone
Concen: 0.647 ug/l
RT: 2.429 min Scan# 214
Delta R.T. 0.037 min
Lab File: VX029845.D
Acq: 28 Jun 2022 21:46




Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-1-GR


Tgt Ion: 43 Resp: 1054
Ion Ratio Lower Upper
43 100
58 16.2 27.7 41.5#

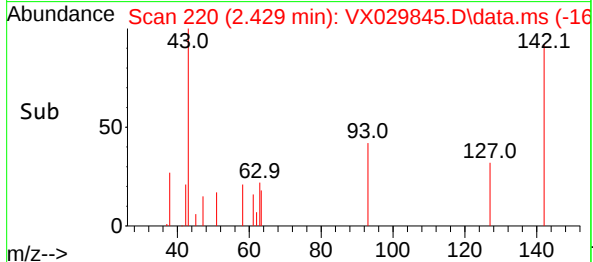

#18
Methyl Acetate
Concen: 1.042 ug/l
RT: 2.727 min Scan# 269
Delta R.T. 0.018 min
Lab File: VX029845.D
Acq: 28 Jun 2022 21:46


Tgt Ion: 43 Resp: 5234
Ion Ratio Lower Upper
43 100
74 23.5 19.4 29.2

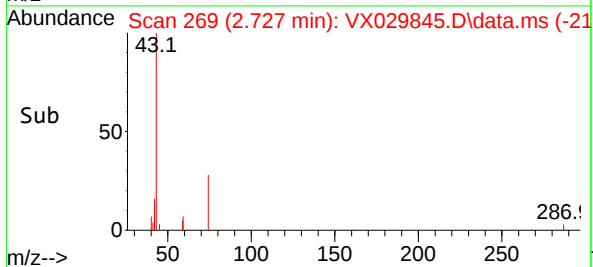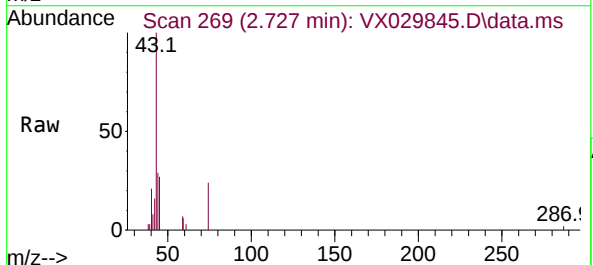



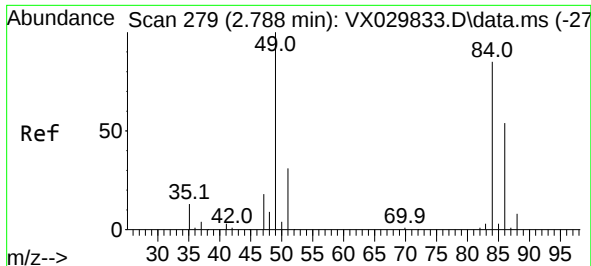


#20
Methylene Chloride
Concen: 0.307 ug/l
RT: 2.782 min Scan# 21
Delta R.T. -0.006 min
Lab File: VX029845.D
Acq: 28 Jun 2022 21:46


Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-1-GR





Tgt Ion: 84	Resp: 1057
Ion Ratio	Lower Upper
84 100	
49 136.9	93.8 140.6
51 41.2	29.4 44.0
86 52.2	51.0 76.4

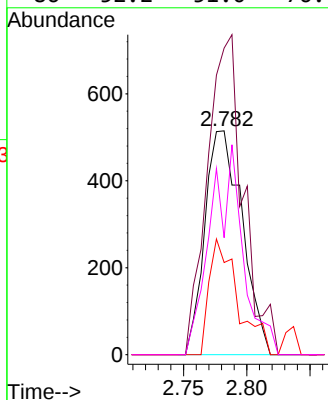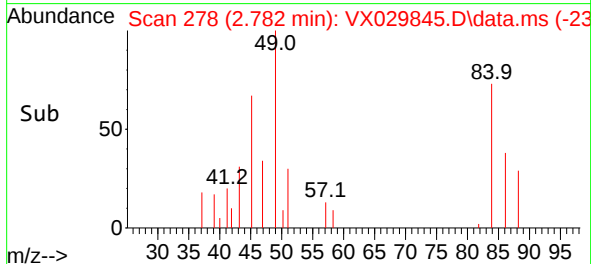


#31
Cyclohexane
Concen: 0.585 ug/l
RT: 5.477 min Scan# 720
Delta R.T. 0.006 min
Lab File: VX029845.D
Acq: 28 Jun 2022 21:46

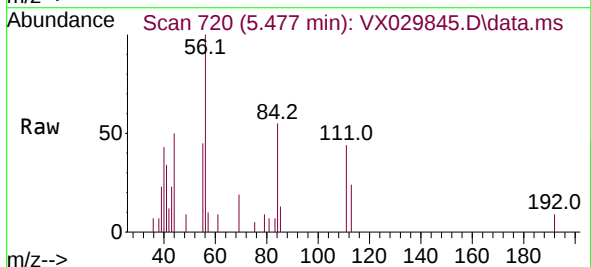

Tgt Ion: 56	Resp: 2715
Ion Ratio	Lower Upper
56 100	
69 18.8	25.4 38.0#
84 55.3	68.9 103.3#

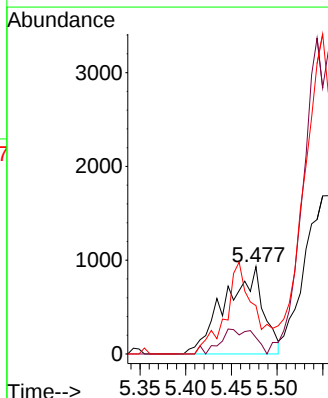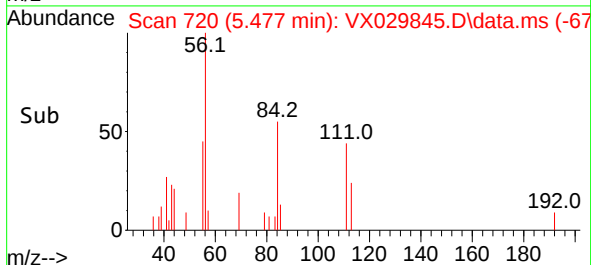

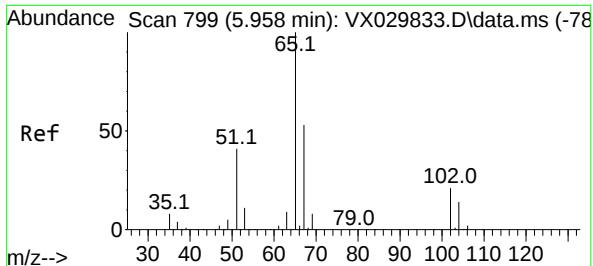

#33

1,2-Dichloroethane-d4

Concen: 41.477 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX029845.D

Acq: 28 Jun 2022 21:46

Instrument :

MSVOA_X

ClientSampleId :





SP-EXC-1-1-GR

Tgt Ion: 65 Resp: 138159

Ion Ratio Lower Upper

65 100

67 55.4 0.0 109.6

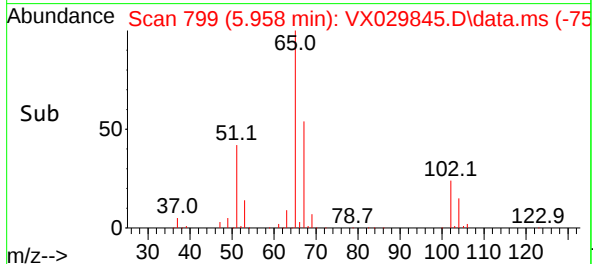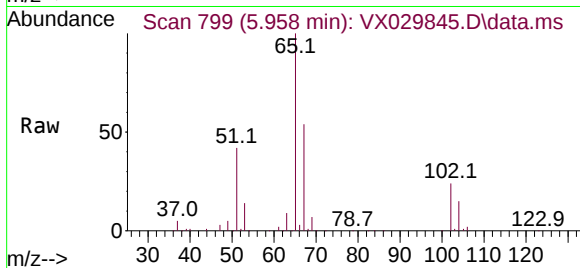

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.000 min

Lab File: VX029845.D

Acq: 28 Jun 2022 21:46




Tgt Ion: 114 Resp: 440532


Ion Ratio Lower Upper

114 100

63 18.4 0.0 38.4

88 15.0 0.0 31.8

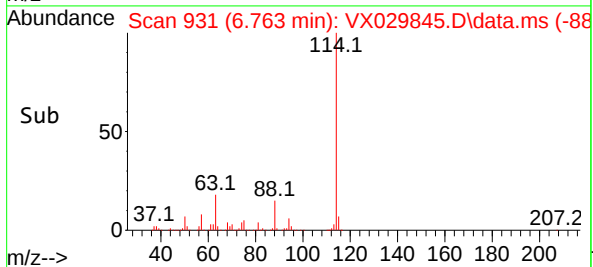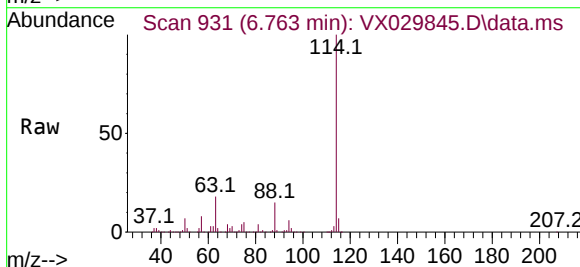

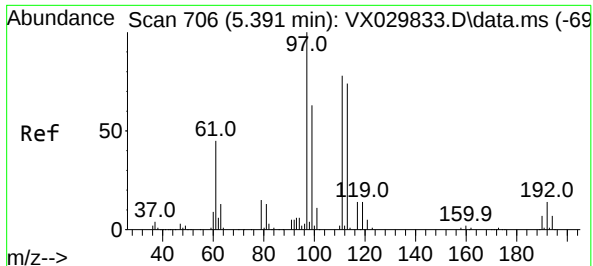

#35

Dibromofluoromethane

Concen: 43.351 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.000 min

Lab File: VX029845.D


Acq: 28 Jun 2022 21:46

Instrument :

MSVOA_X

ClientSampleId :

SP-EXC-1-1-GR

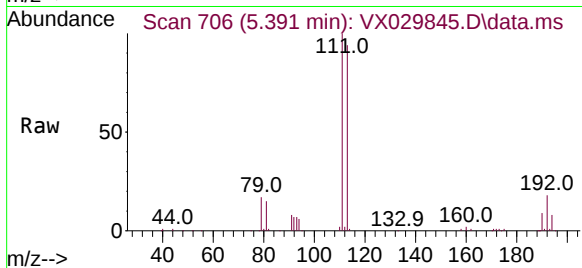




Tgt Ion:113 Resp: 119350

Ion Ratio Lower Upper

113 100

111 102.9 83.2 124.8

192 19.0 14.8 22.2

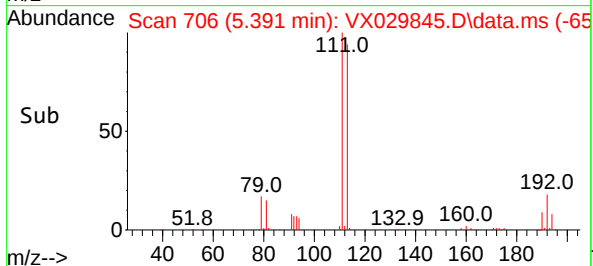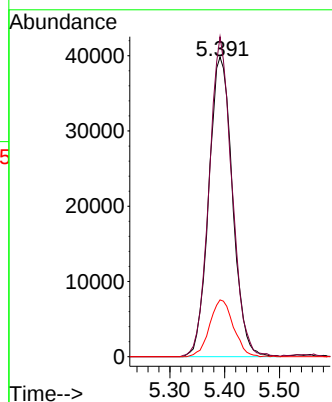

#36

1,1-Dichloropropene

Concen: 5.153 ug/l

RT: 5.544 min Scan# 731

Delta R.T. -0.152 min

Lab File: VX029845.D

Acq: 28 Jun 2022 21:46




Tgt Ion: 75 Resp: 18868


Ion Ratio Lower Upper

75 100

110 8.1 19.3 57.9#

77 0.0 24.4 36.6#


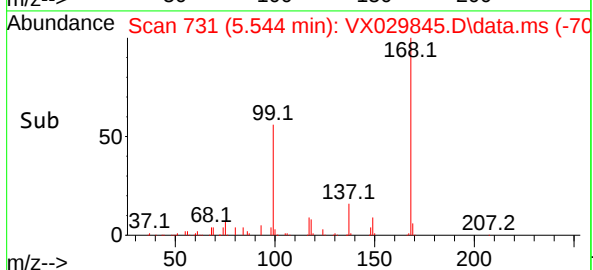

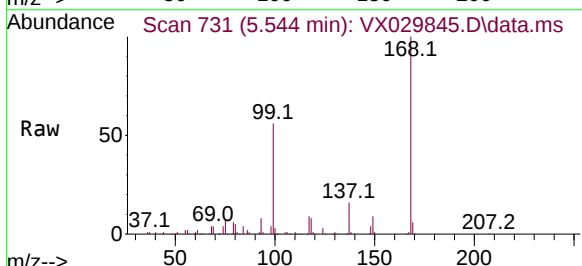


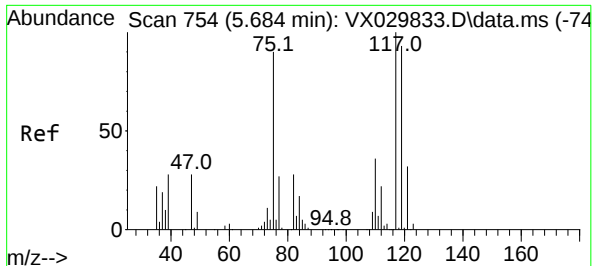

#38
Carbon Tetrachloride
Concen: 7.727 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.134 min
Lab File: VX029845.D
Acq: 28 Jun 2022 21:46




Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-1-GR


Tgt Ion:117 Resp: 24517
Ion Ratio Lower Upper
117 100
119 5.8 74.1 111.1#
121 0.0 25.8 38.8#

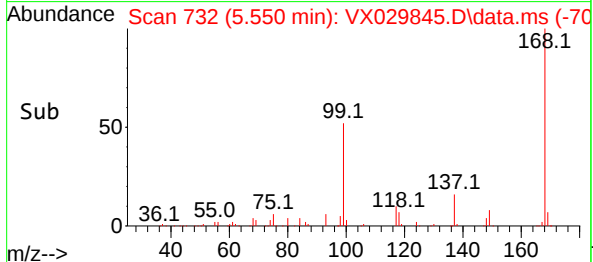

#39
Methylcyclohexane
Concen: 0.490 ug/l
RT: 7.373 min Scan# 1031
Delta R.T. -0.012 min
Lab File: VX029845.D
Acq: 28 Jun 2022 21:46

Tgt Ion: 83 Resp: 2171
Ion Ratio Lower Upper
83 100
55 89.0 57.7 86.5#
98 66.3 36.5 54.7#

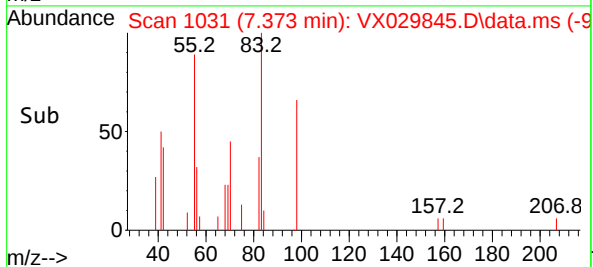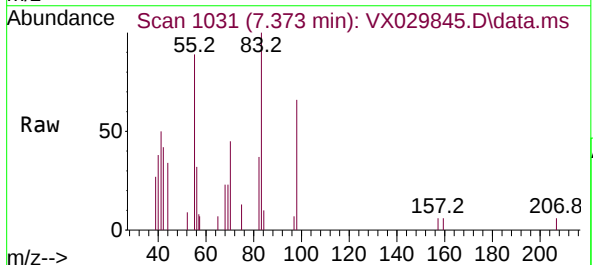

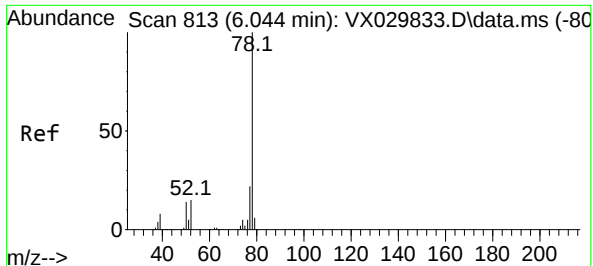

#40

Benzene

Concen: 0.367 ug/l

RT: 6.032 min Scan# 81

Delta R.T. -0.012 min

Lab File: VX029845.D

Acq: 28 Jun 2022 21:46

Instrument :

MSVOA_X

ClientSampleId :





SP-EXC-1-1-GR

Tgt Ion: 78 Resp: 4349

Ion Ratio Lower Upper

78 100

77 19.8 18.0 27.0

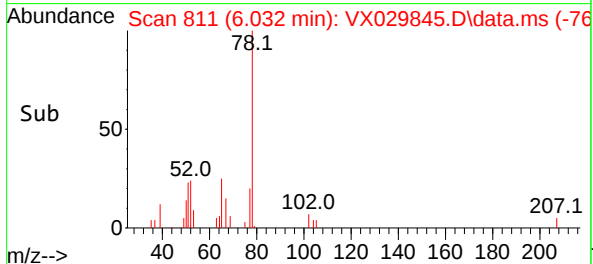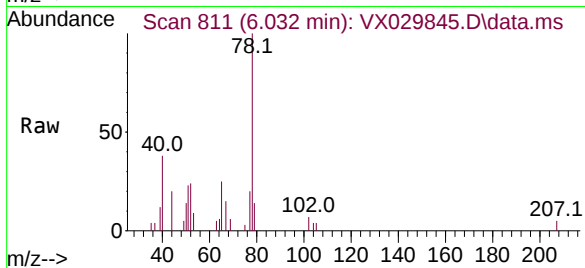

#44

Trichloroethene

Concen: 0.450 ug/l

RT: 7.123 min Scan# 990

Delta R.T. -0.006 min

Lab File: VX029845.D




Acq: 28 Jun 2022 21:46


Tgt Ion:130 Resp: 1436

Ion Ratio Lower Upper

130 100

95 62.3 0.0 194.8

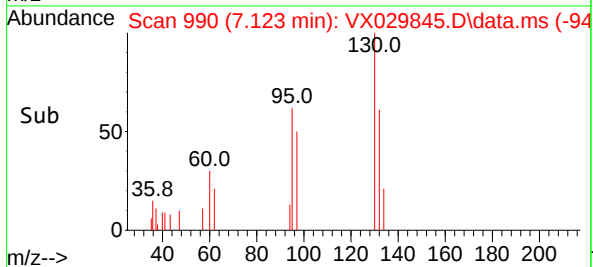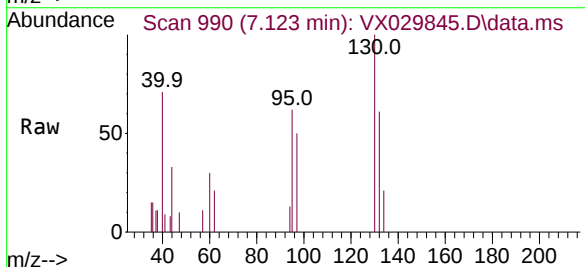

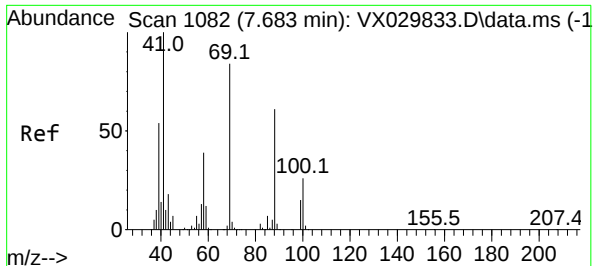

#49

1,4-Dioxane

Concen: 0.331 ug/l

RT: 7.531 min Scan# 1

Delta R.T. -0.152 min

Lab File: VX029845.D


Acq: 28 Jun 2022 21:46

Instrument :




MSVOA_X

ClientSampleId :

SP-EXC-1-1-GR



Tgt Ion:	88	Resp:	28
Ion	Ratio	Lower	Upper
88	100		
43	992.9	23.8	35.8#
58	0.0	53.8	80.6#

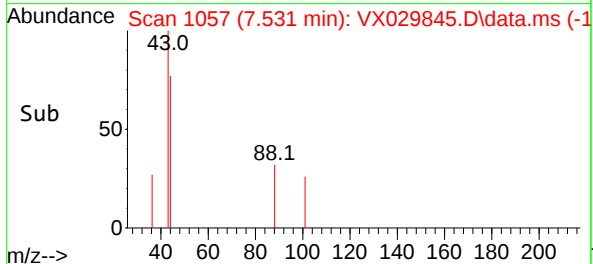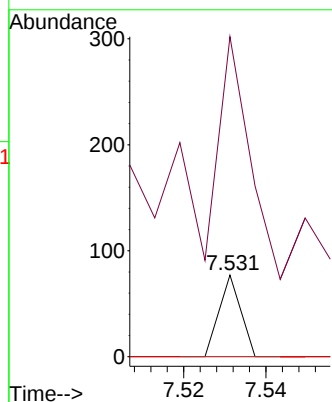

#50

Toluene-d8

Concen: 48.478 ug/l




RT: 8.647 min Scan# 1240


Delta R.T. -0.006 min

Lab File: VX029845.D

Acq: 28 Jun 2022 21:46

Tgt Ion:	98	Resp:	500690
Ion	Ratio	Lower	Upper
98	100		
100	65.5	52.3	78.5


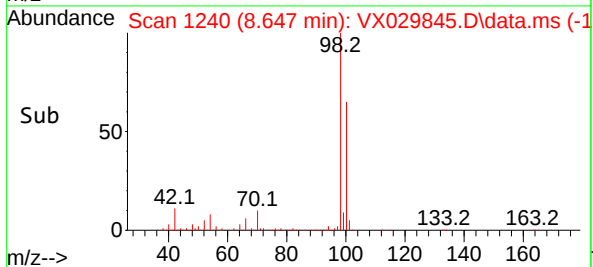
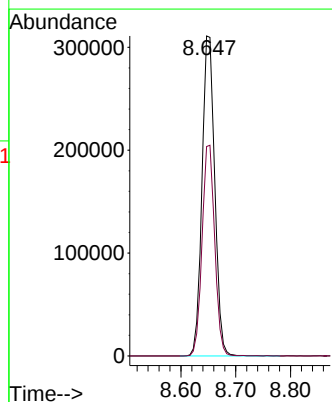
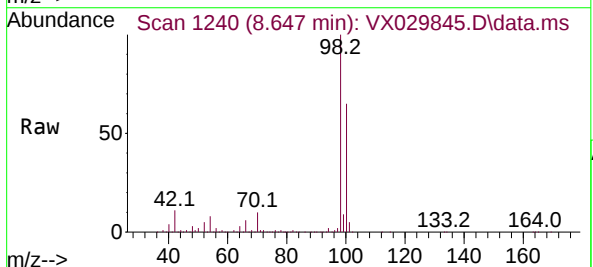


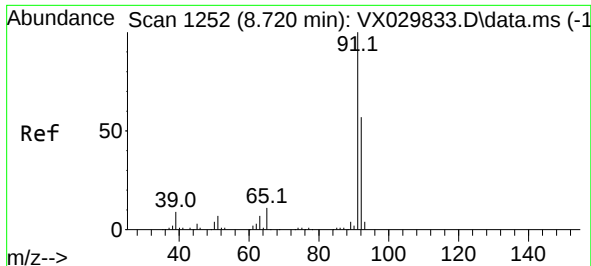

#52
Toluene
Concen: 0.329 ug/l
RT: 8.720 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX029845.D
Acq: 28 Jun 2022 21:46




Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-1-GR


Tgt Ion: 92 Resp: 2348
Ion Ratio Lower Upper
92 100
91 173.4 139.2 208.8

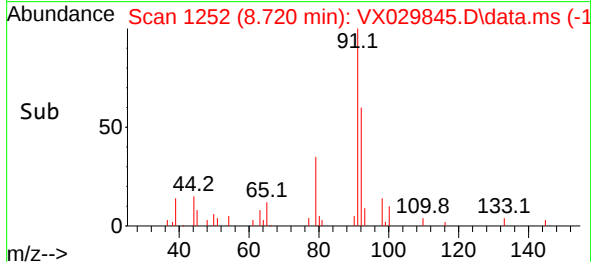

#62
4-Bromofluorobenzene
Concen: 44.384 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.006 min
Lab File: VX029845.D
Acq: 28 Jun 2022 21:46

Tgt Ion: 95 Resp: 162038
Ion Ratio Lower Upper
95 100
174 77.7 0.0 149.0
176 73.3 0.0 146.0

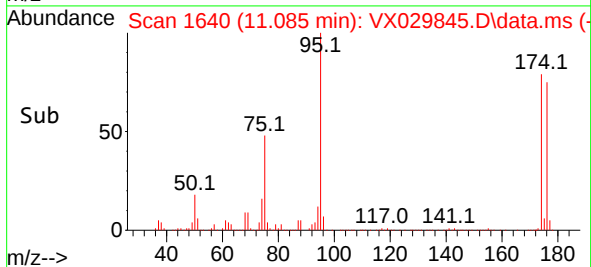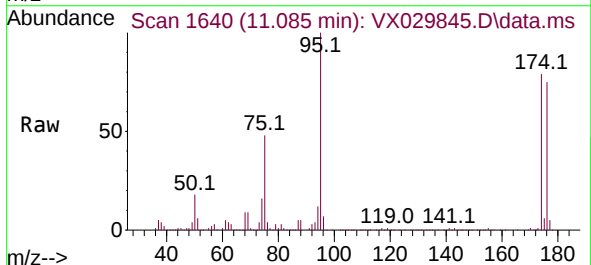

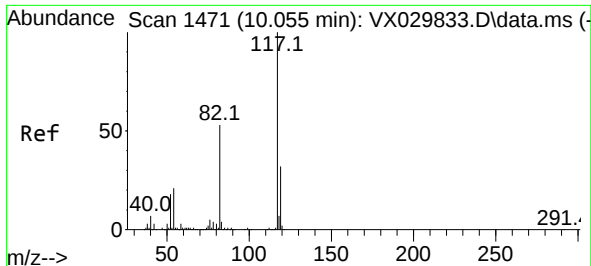

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX029845.D

Acq: 28 Jun 2022 21:46

Instrument :

MSVOA_X

ClientSampleId :

SP-EXC-1-1-GR





Tgt Ion:117 Resp: 372354

Ion Ratio Lower Upper

117 100

82 54.1 42.7 64.1

119 31.5 25.4 38.2

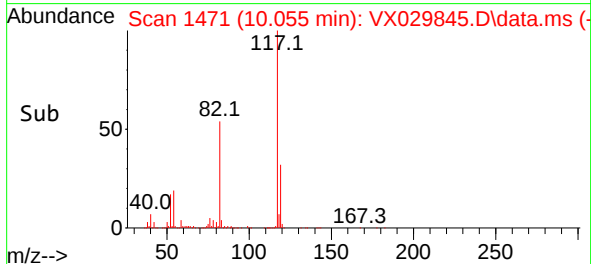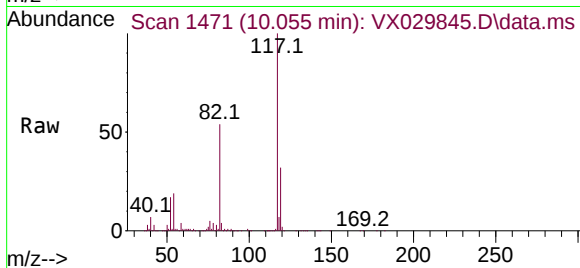

#65

Chlorobenzene

Concen: 6.881 ug/l

RT: 10.080 min Scan# 1475

Delta R.T. 0.000 min

Lab File: VX029845.D




Acq: 28 Jun 2022 21:46


Tgt Ion:112 Resp: 51430

Ion Ratio Lower Upper

112 100

114 31.1 24.6 36.8

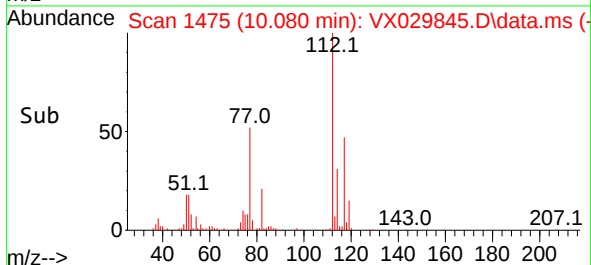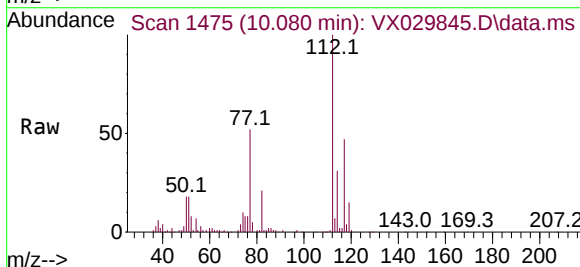

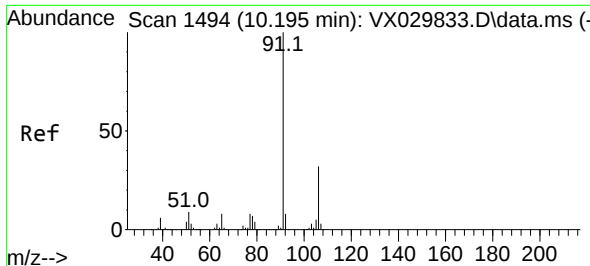

#67

Ethyl Benzene

Concen: 0.331 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. 0.000 min

Lab File: VX029845.D

Acq: 28 Jun 2022 21:46

Instrument :

MSVOA_X

ClientSampleId :





SP-EXC-1-1-GR

Tgt Ion: 91 Resp: 4297

Ion Ratio Lower Upper

91 100

106 38.4 25.5 38.3#

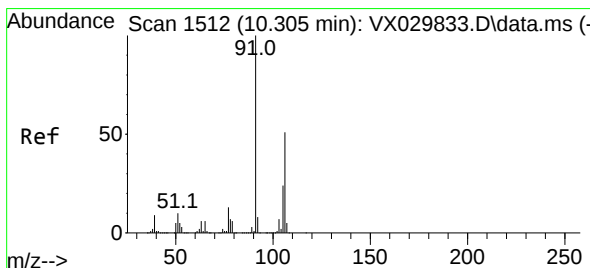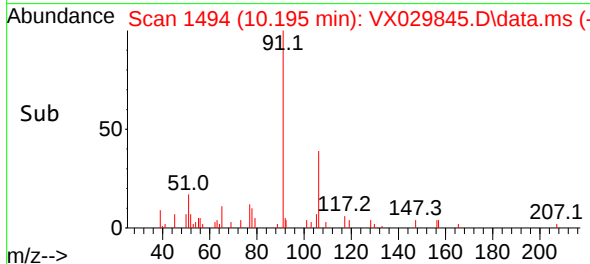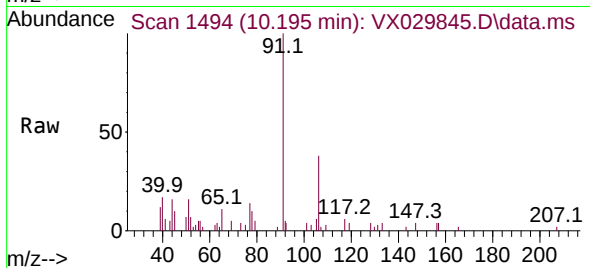

#68

m/p-Xylenes

Concen: 0.788 ug/l

RT: 10.305 min Scan# 1512

Delta R.T. 0.000 min

Lab File: VX029845.D




Acq: 28 Jun 2022 21:46


Tgt Ion: 106 Resp: 3929

Ion Ratio Lower Upper

106 100

91 209.7 158.2 237.4


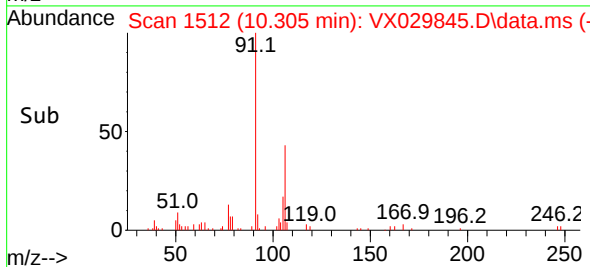

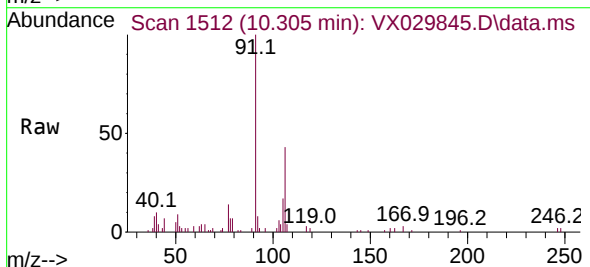


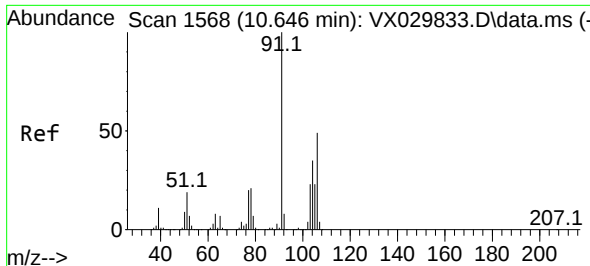

#69
o-Xylene
Concen: 0.261 ug/l
RT: 10.653 min Scan# 1569
Delta R.T. 0.006 min
Lab File: VX029845.D
Acq: 28 Jun 2022 21:46




Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-1-GR


Tgt Ion:106 Resp: 1316
Ion Ratio Lower Upper
106 100
91 150.9 103.8 311.6

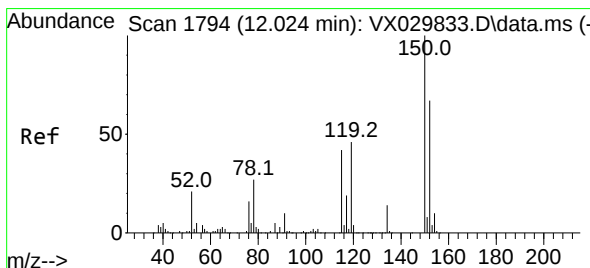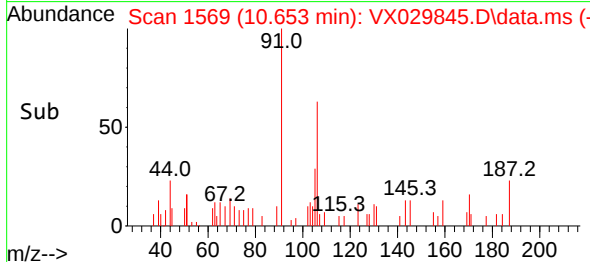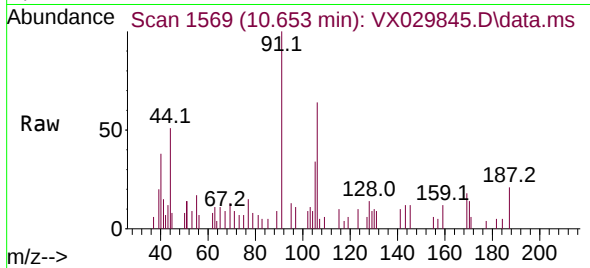

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX029845.D
Acq: 28 Jun 2022 21:46

Tgt Ion:152 Resp: 166062
Ion Ratio Lower Upper
152 100
115 57.3 40.5 121.5
150 154.1 0.0 347.0


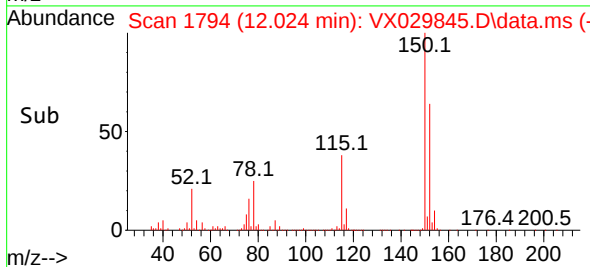

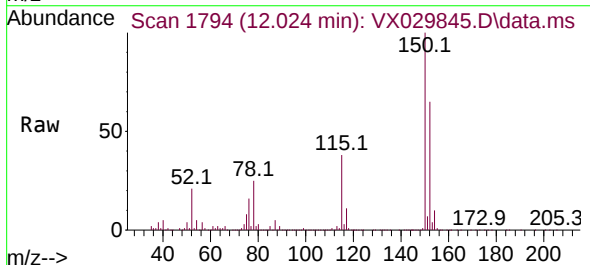


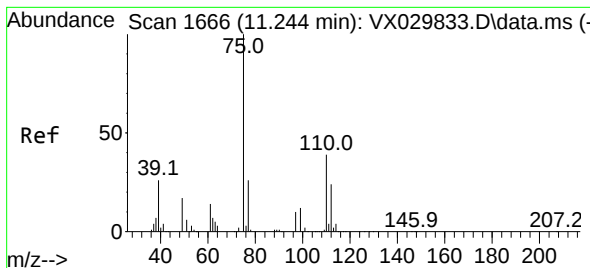

#76
1,2,3-Trichloropropane
Concen: 18.793 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.158 min
Lab File: VX029845.D
Acq: 28 Jun 2022 21:46




Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-1-GR


Tgt Ion: 75 Resp: 74706
Ion Ratio Lower Upper
75 100
77 2.0 19.8 59.3#

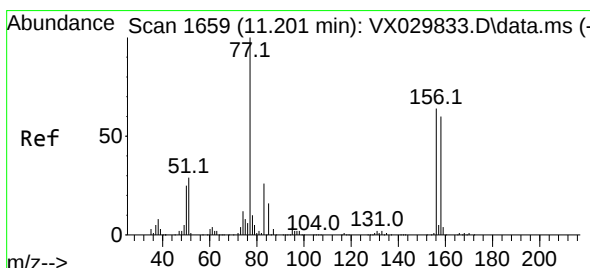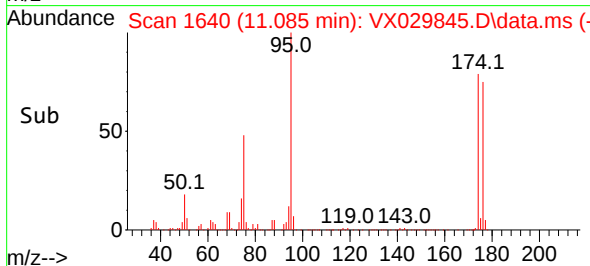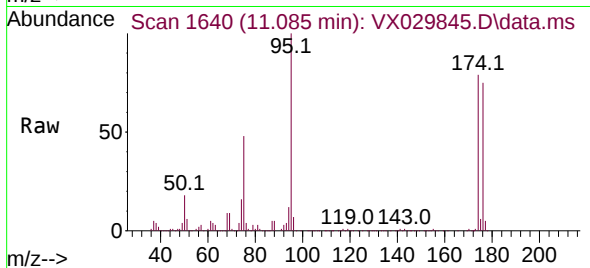

#77
Bromobenzene
Concen: 0.211 ug/l
RT: 11.201 min Scan# 1659
Delta R.T. 0.000 min
Lab File: VX029845.D
Acq: 28 Jun 2022 21:46

Tgt Ion: 156 Resp: 609
Ion Ratio Lower Upper
156 100
77 78.2 82.7 247.9#
158 67.3 47.5 142.5


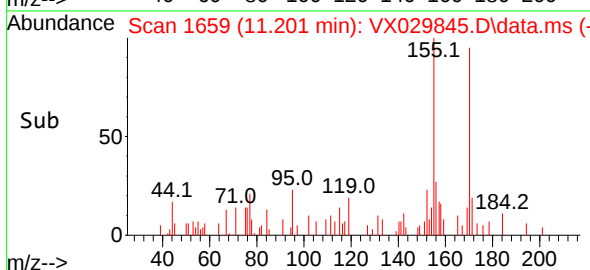

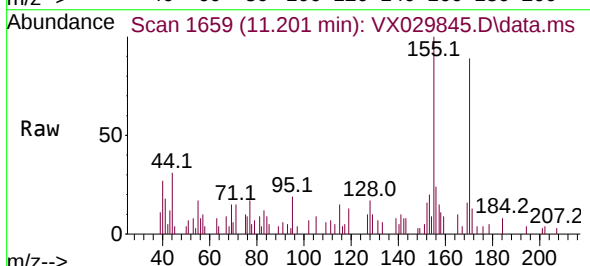


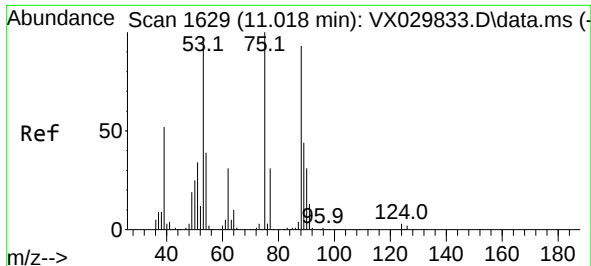

#81
 trans-1,4-Dichloro-2-butene
 Concen: 59.681 ug/l
 RT: 11.085 min Scan# 1640
 Delta R.T. 0.067 min
 Lab File: VX029845.D
 Acq: 28 Jun 2022 21:46




Instrument :
 MSVOA_X
 ClientSampleId :
 SP-EXC-1-1-GR


Tgt Ion: 75 Resp: 74706
 Ion Ratio Lower Upper
 75 100
 53 0.2 74.2 111.4#
 89 0.0 34.8 52.2#

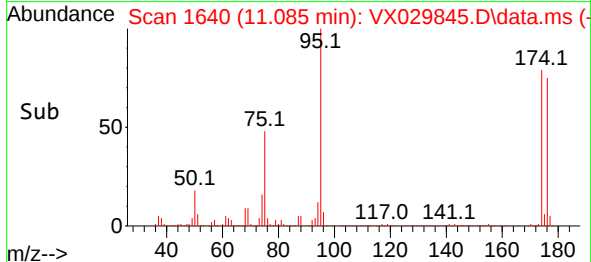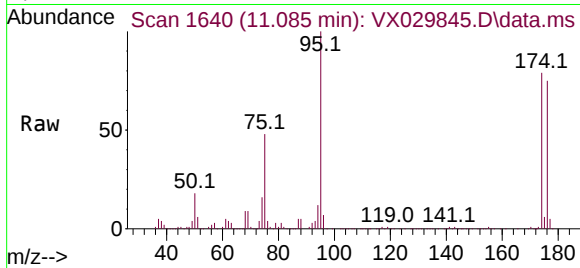

#84
 1,2,4-Trimethylbenzene
 Concen: 0.229 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. 0.000 min
 Lab File: VX029845.D
 Acq: 28 Jun 2022 21:46

Tgt Ion:105 Resp: 2290
 Ion Ratio Lower Upper
 105 100
 120 59.0 22.9 68.8


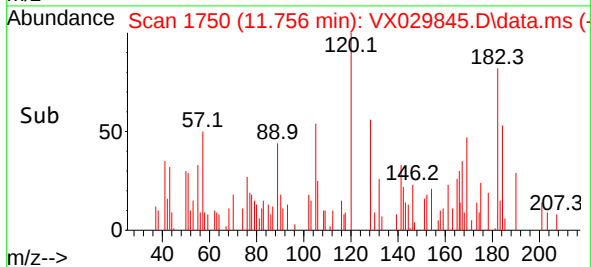

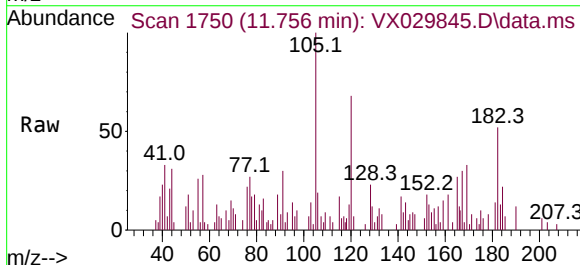


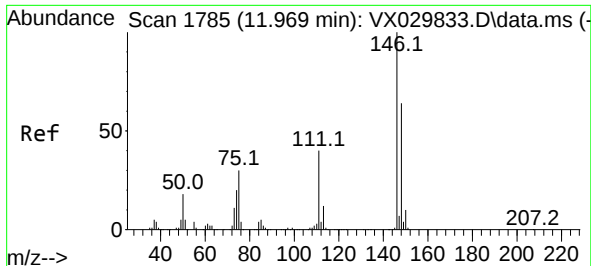

#87
1,3-Dichlorobenzene
Concen: 0.989 ug/l
RT: 11.976 min Scan# 1785
Delta R.T. 0.006 min
Lab File: VX029845.D
Acq: 28 Jun 2022 21:46




Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-1-GR


Tgt Ion:146 Resp: 5489
Ion Ratio Lower Upper
146 100
111 48.4 20.3 60.8
148 57.2 31.8 95.3

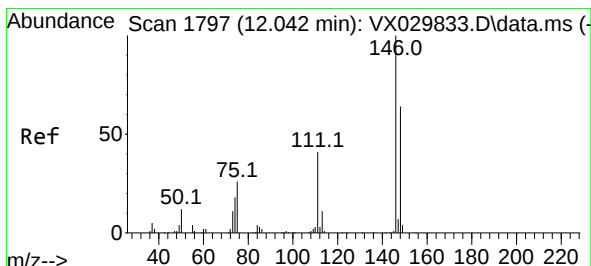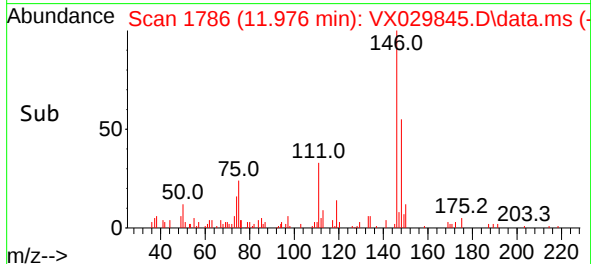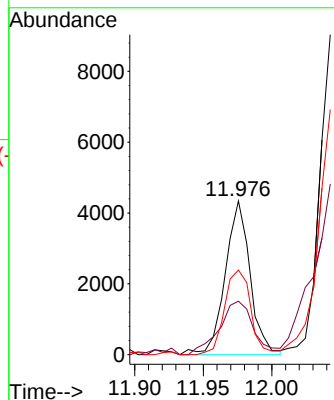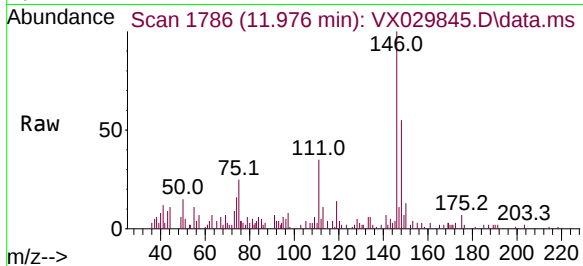

#88
1,4-Dichlorobenzene
Concen: 2.345 ug/l
RT: 12.049 min Scan# 1798
Delta R.T. 0.006 min
Lab File: VX029845.D
Acq: 28 Jun 2022 21:46

Tgt Ion:146 Resp: 13278
Ion Ratio Lower Upper
146 100
111 58.0 20.3 60.9
148 76.9 32.3 96.8


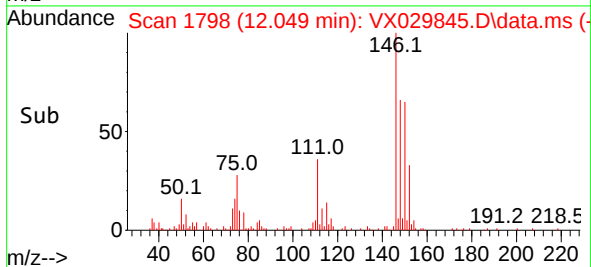
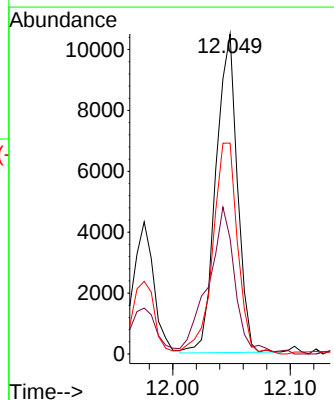
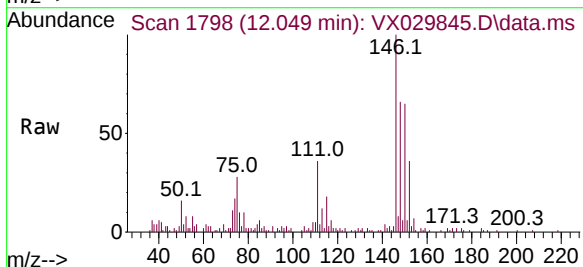




#90
Hexachloroethane
Concen: 0.219 ug/l
RT: 12.549 min Scan# 1880
Delta R.T. 0.006 min
Lab File: VX029845.D
Acq: 28 Jun 2022 21:46




Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-1-GR


Tgt Ion:117 Resp: 356
Ion Ratio Lower Upper
117 100
201 41.9 34.2 102.5

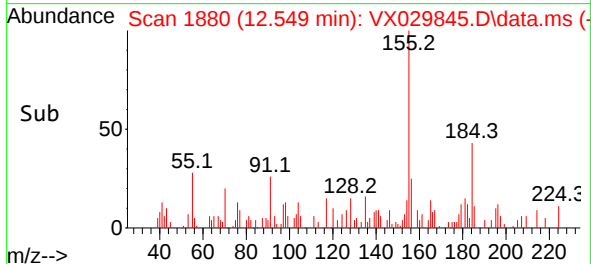

#91
1,2-Dichlorobenzene
Concen: 16.531 ug/l
RT: 12.341 min Scan# 1846
Delta R.T. 0.006 min
Lab File: VX029845.D
Acq: 28 Jun 2022 21:46

Tgt Ion:146 Resp: 90120
Ion Ratio Lower Upper
146 100
111 41.5 20.7 62.1
148 65.1 32.0 96.2

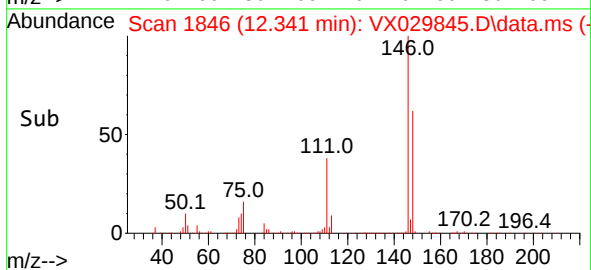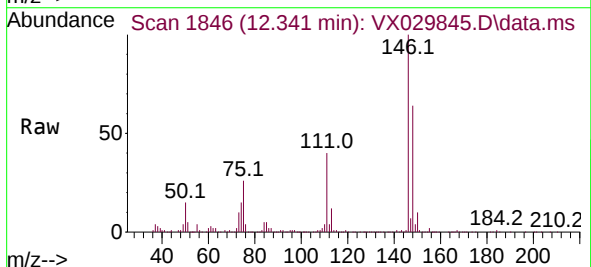



#93
 1,2,4-Trichlorobenzene
 Concen: 0.355 ug/l
 RT: 13.591 min Scan# 2051
 Delta R.T. 0.000 min
 Lab File: VX029845.D
 Acq: 28 Jun 2022 21:46

Instrument :
 MSVOA_X
 ClientSampleId :
 SP-EXC-1-1-GR

Tgt Ion:180 Resp: 1172
 Ion Ratio Lower Upper
 180 100
 182 64.7 48.2 144.6
 145 0.0 15.9 47.6#

