

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062822\
 Data File : VX029842.D
 Acq On : 28 Jun 2022 20:36
 Operator : JC/MD
 Sample : N3494-19
 Misc : 5.49g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SP-EXC-1-6-GR

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
 Title : SW846 8260

Signal : TIC: VX029842.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.636	74	90	93	rBV5	11898	41466	3.22%	0.481%
2	1.910	132	135	138	rBV3	13634	15286	1.19%	0.177%
3	2.727	263	269	274	rBV	9644	19934	1.55%	0.231%
4	2.947	297	305	319	rBV	16476	48732	3.79%	0.565%
5	3.075	319	326	332	rVB6	6882	16981	1.32%	0.197%
6	3.416	375	382	394	rVB3	13299	31579	2.45%	0.366%
7	4.288	515	525	531	rBV5	5053	14394	1.12%	0.167%
8	5.391	696	706	722	rBV	127974	397412	30.87%	4.610%
9	5.550	722	732	747	rVB	255418	729878	56.70%	8.466%
10	5.818	765	776	789	rVB6	5371	15965	1.24%	0.185%
11	5.958	789	799	808	rBV	153320	410196	31.87%	4.758%
12	6.031	808	811	820	rVV2	11256	27473	2.13%	0.319%
13	6.147	823	830	837	rVV9	4437	13558	1.05%	0.157%
14	6.355	854	864	871	rBV8	5240	14686	1.14%	0.170%
15	6.604	897	905	912	rVB3	13826	33361	2.59%	0.387%
16	6.763	918	931	950	rBV	403318	968157	75.22%	11.229%
17	7.373	1023	1031	1042	rVB2	25115	59609	4.63%	0.691%
18	8.598	1223	1232	1234	rBV2	9719	17111	1.33%	0.198%
19	8.653	1234	1241	1248	rVV	771394	1287172	100.00%	14.930%
20	8.720	1248	1252	1257	rVB	22357	32876	2.55%	0.381%
21	8.909	1278	1283	1289	rVB	17233	25631	1.99%	0.297%
22	8.976	1289	1294	1302	rBV5	9670	17837	1.39%	0.207%
23	9.275	1338	1343	1349	rBV4	6348	14551	1.13%	0.169%
24	9.348	1349	1355	1358	rBV2	5545	13146	1.02%	0.152%
25	9.561	1385	1390	1395	rVB2	13956	21665	1.68%	0.251%
26	10.055	1466	1471	1482	rVB	744449	1190161	92.46%	13.804%
27	10.195	1488	1494	1502	rBV	53786	77128	5.99%	0.895%
28	10.305	1502	1512	1518	rVV	91333	146069	11.35%	1.694%
29	10.360	1518	1521	1528	rVB2	24165	32790	2.55%	0.380%
30	10.585	1552	1558	1562	rBV6	7197	13417	1.04%	0.156%
31	10.646	1563	1568	1575	rVB2	17192	31113	2.42%	0.361%
32	10.781	1582	1590	1594	rBV3	17881	26838	2.09%	0.311%
33	10.860	1598	1603	1606	rVV3	13087	21525	1.67%	0.250%
34	10.963	1614	1620	1624	rBV2	15110	23858	1.85%	0.277%
35	11.085	1635	1640	1651	rVB	556332	759309	58.99%	8.807%
36	11.311	1672	1677	1684	rBV2	33528	68433	5.32%	0.794%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062822\
 Data File : VX029842.D
 Acq On : 28 Jun 2022 20:36
 Operator : JC/MD
 Sample : N3494-19
 Misc : 5.49g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SP-EXC-1-6-GR

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
 Title : SW846 8260

37	11.384	1685	1689	1690	rBV2	15506	17098	1.33%	0.198%
38	11.476	1701	1704	1710	rVB2	37198	51571	4.01%	0.598%
39	11.622	1723	1728	1733	rVB7	8246	17358	1.35%	0.201%
40	11.719	1740	1744	1746	rVV	26328	33022	2.57%	0.383%
41	11.756	1746	1750	1759	rVB	41497	72980	5.67%	0.846%
42	11.896	1767	1773	1777	rVB5	16356	24808	1.93%	0.288%
43	11.945	1777	1781	1782	rBV4	14007	13547	1.05%	0.157%
44	11.975	1783	1786	1789	rVB3	16375	20184	1.57%	0.234%
45	12.024	1789	1794	1801	rBV	738681	983844	76.43%	11.411%
46	12.171	1813	1818	1821	rBV6	8694	15638	1.21%	0.181%
47	12.250	1827	1831	1838	rBV5	21727	44591	3.46%	0.517%
48	12.341	1838	1846	1850	rBV	147148	219974	17.09%	2.551%
49	12.427	1856	1860	1863	rVV	34910	41098	3.19%	0.477%
50	12.469	1864	1867	1874	rVB7	14487	24630	1.91%	0.286%
51	12.616	1888	1891	1899	rVB	19003	28903	2.25%	0.335%
52	12.768	1913	1916	1921	rBV6	8884	12915	1.00%	0.150%
53	12.987	1946	1952	1955	rBV7	9973	16828	1.31%	0.195%
54	13.268	1994	1998	2000	rBV2	18076	24741	1.92%	0.287%
55	13.384	2013	2017	2020	rBV4	11266	14974	1.16%	0.174%
56	13.780	2078	2082	2089	rVB	49557	70123	5.45%	0.813%
57	14.640	2220	2223	2230	rVB	40360	53785	4.18%	0.624%
58	14.780	2244	2246	2254	rVB2	23844	32973	2.56%	0.382%
59	15.481	2356	2361	2371	rBV3	22439	48160	3.74%	0.559%
60	15.621	2380	2384	2386	rBV2	12214	15220	1.18%	0.177%
61	15.969	2436	2441	2449	rVB8	23393	43292	3.36%	0.502%


Sum of corrected areas: 8621554

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062822\
Data File : VX029842.D
Acq On : 28 Jun 2022 20:36
Operator : JC/MD
Sample : N3494-19
Misc : 5.49g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-6-GR

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

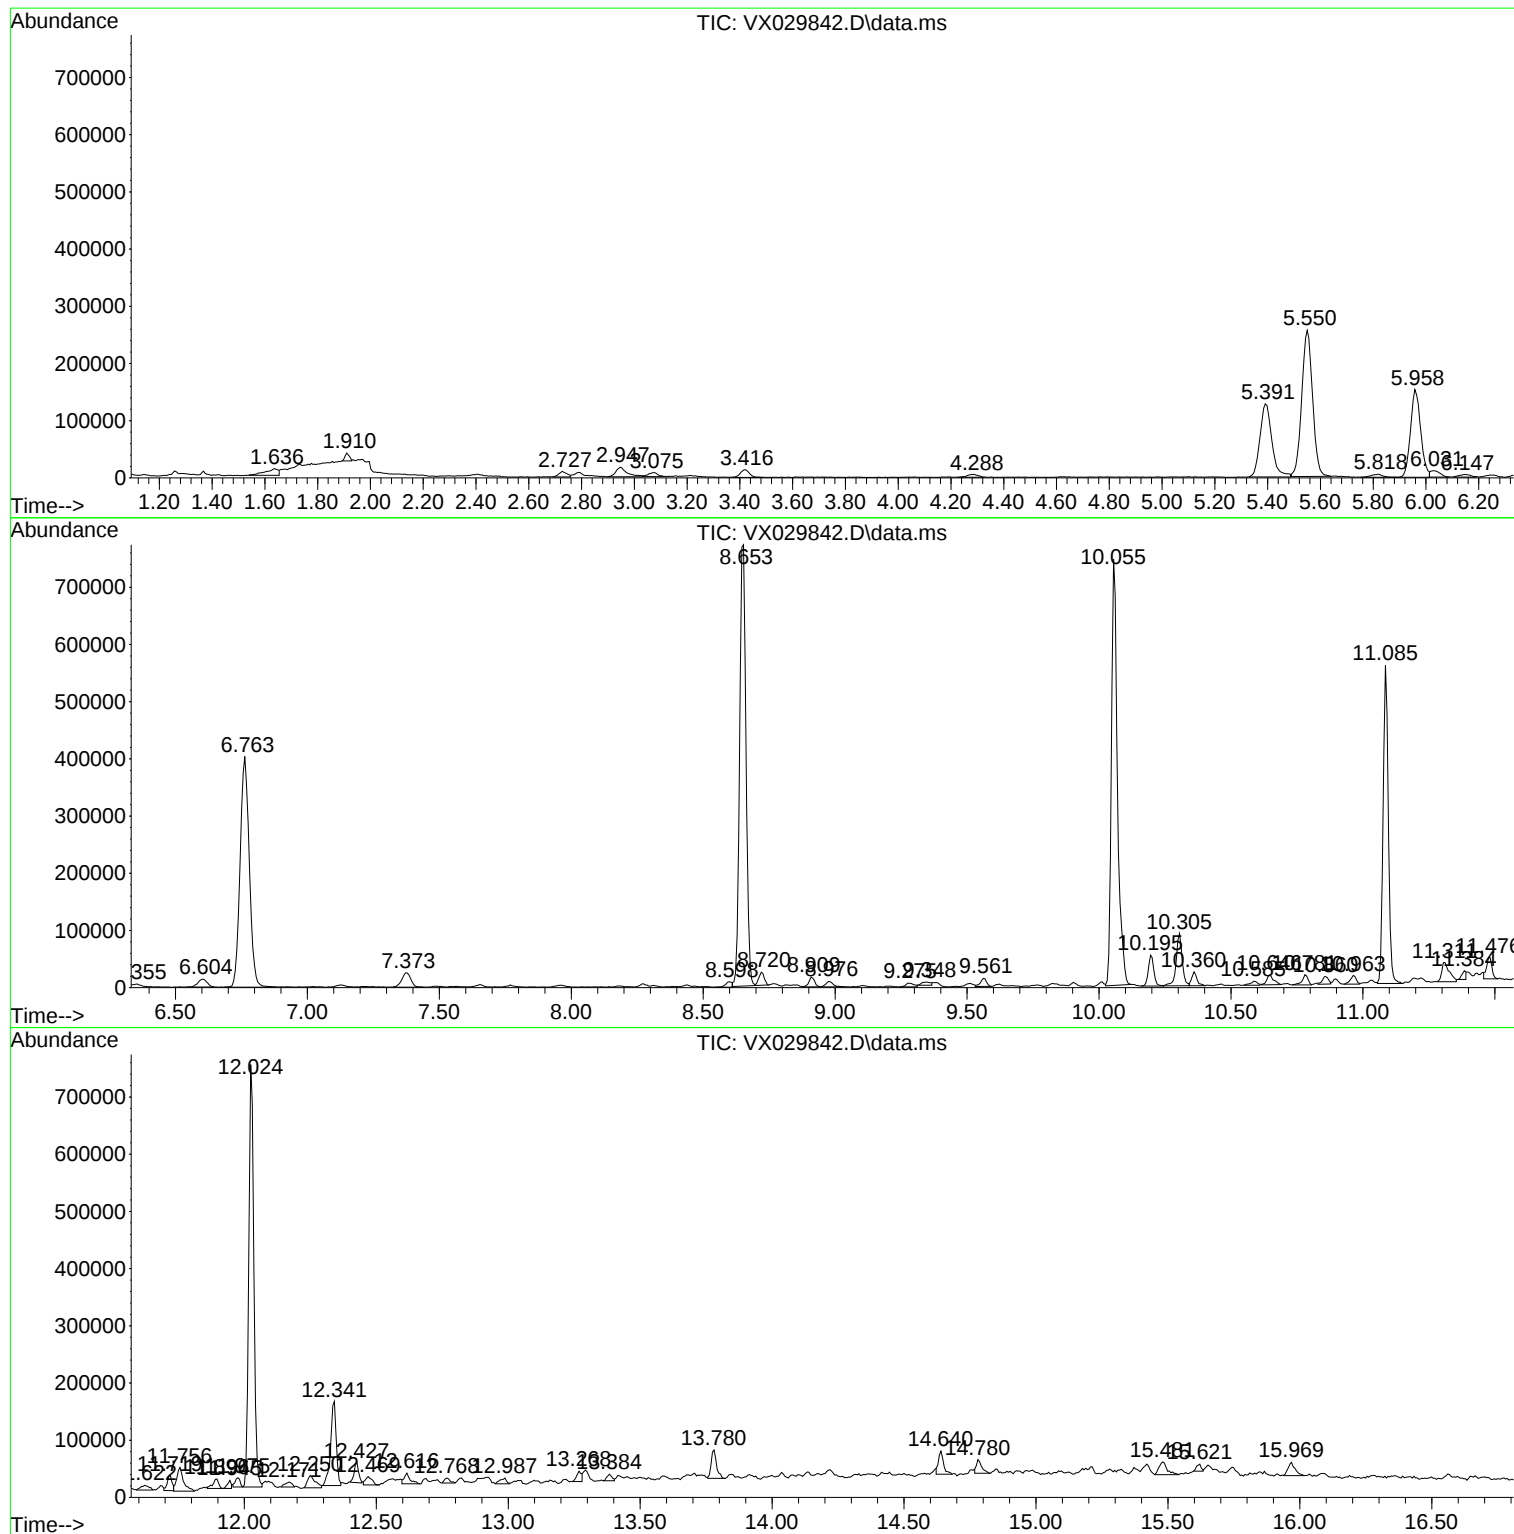

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062822\
Data File : VX029842.D
Acq On : 28 Jun 2022 20:36
Operator : JC/MD
Sample : N3494-19
Misc : 5.49g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-6-GR

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062822\
Data File : VX029842.D
Acq On : 28 Jun 2022 20:36
Operator : JC/MD
Sample : N3494-19
Misc : 5.49g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SP-EXC-1-6-GR

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc