

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062823\
 Data File : VX036358.D
 Acq On : 28 Jun 2023 10:50
 Operator : JC/MD
 Sample : VX0628WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0628WBL01

Quant Time: Jun 29 01:26:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 23 15:03:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	218592	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	385922	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	343347	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	159120	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	165610	52.854	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	105.700%
35) Dibromofluoromethane	5.385	113	127875	50.252	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	100.500%
50) Toluene-d8	8.647	98	462586	48.671	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	97.340%
62) 4-Bromofluorobenzene	11.079	95	165740	49.508	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	99.020%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062823\
Data File : VX036358.D
Acq On : 28 Jun 2023 10:50
Operator : JC/MD
Sample : VX0628WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0628WBL01

Quant Time: Jun 29 01:26:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 23 15:03:28 2023
Response via : Initial Calibration




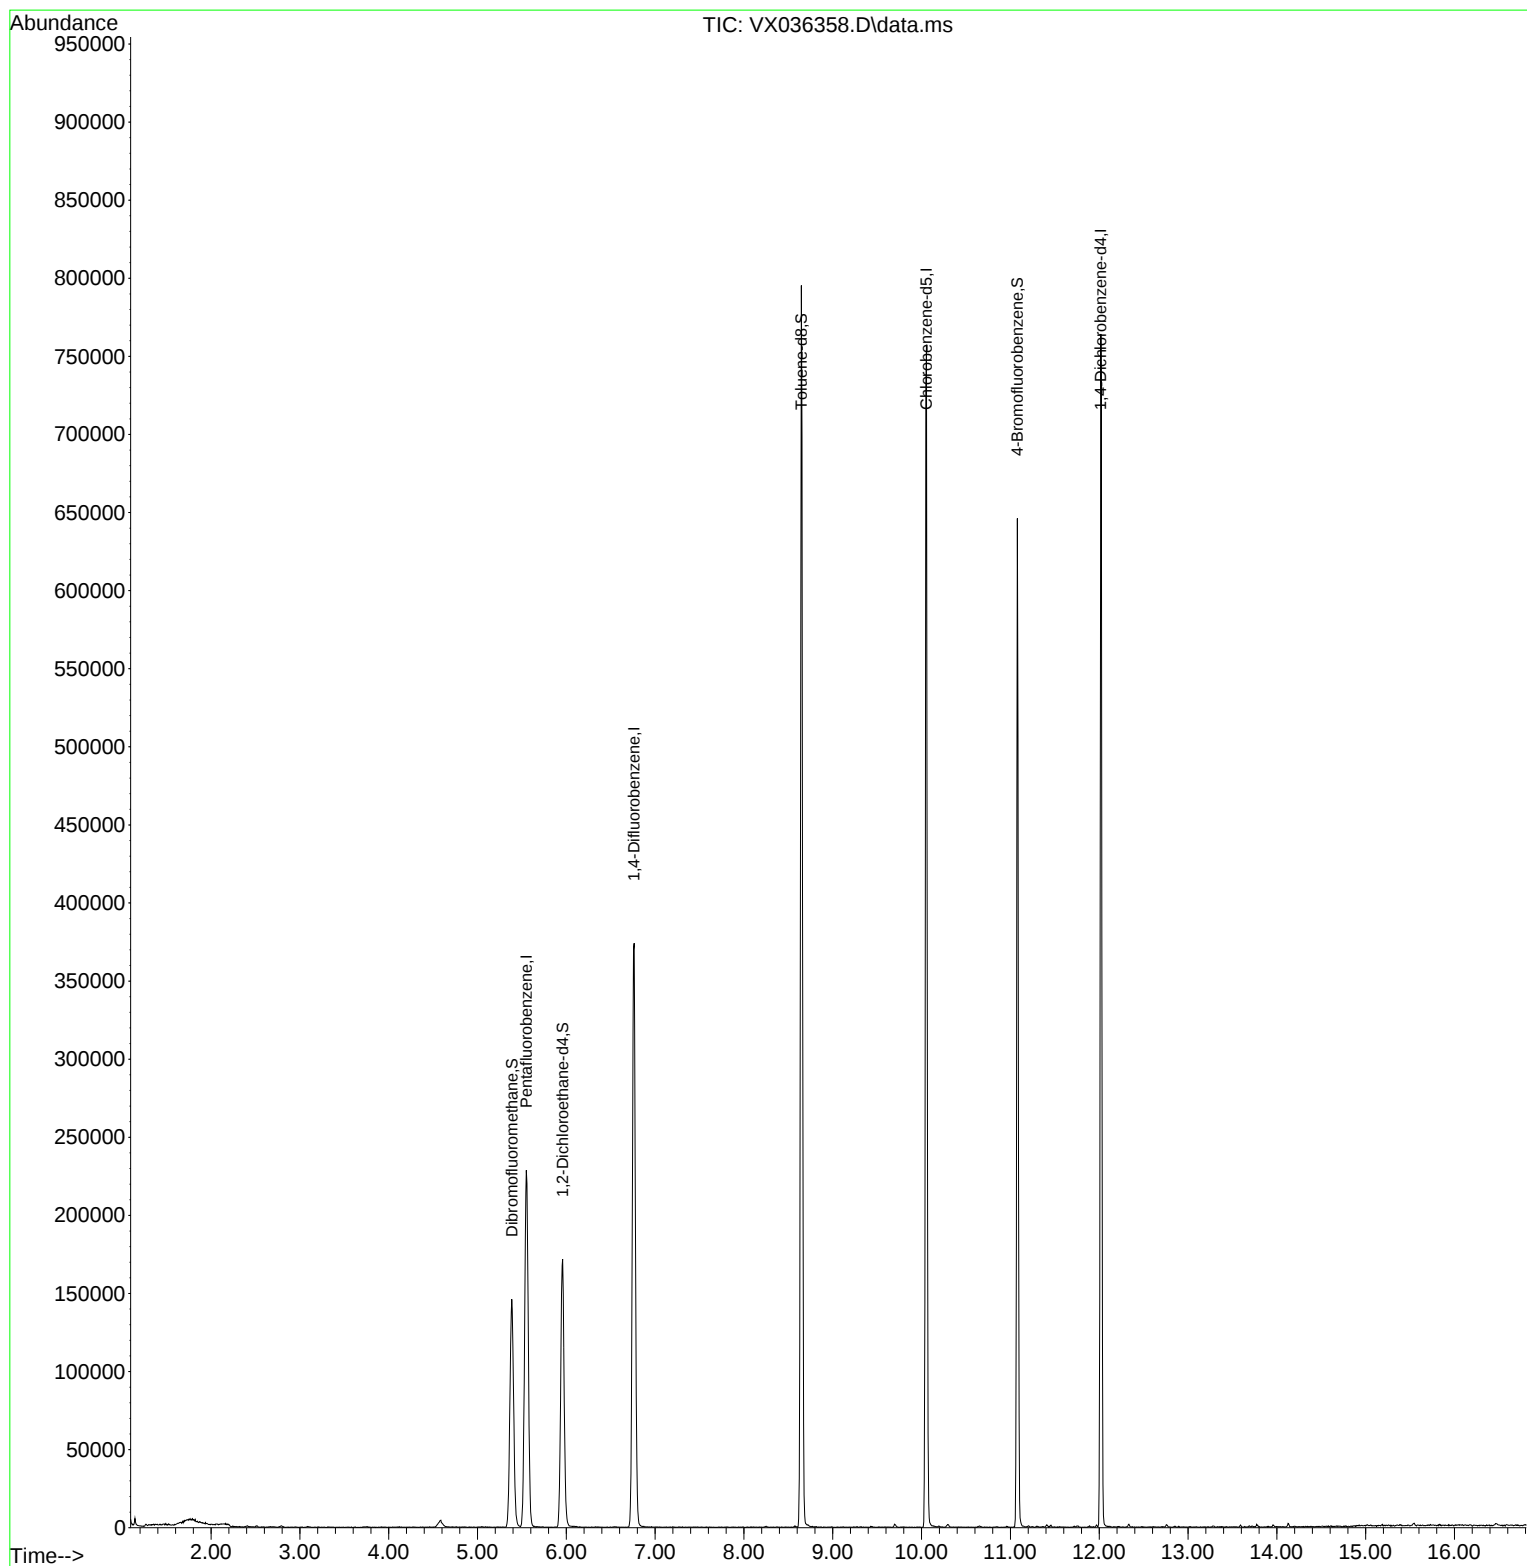


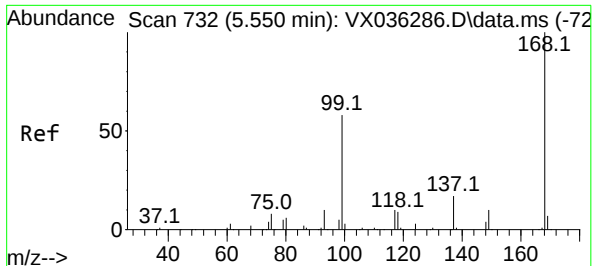

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 711
Delta R.T. 0.001 min
Lab File: VX036358.D
Acq: 28 Jun 2023 10:50




Instrument :
MSVOA_X
ClientSampleId :
VX0628WBL01


Tgt Ion:168 Resp: 218592
Ion Ratio Lower Upper
168 100
99 57.6 56.6 85.0

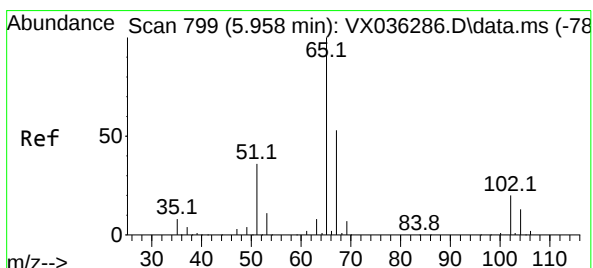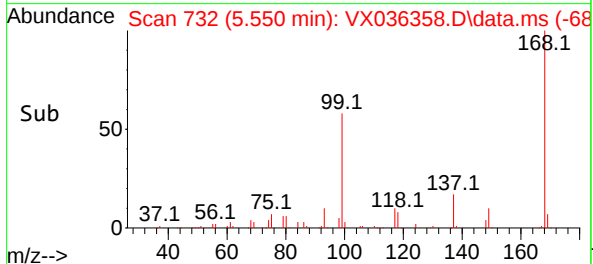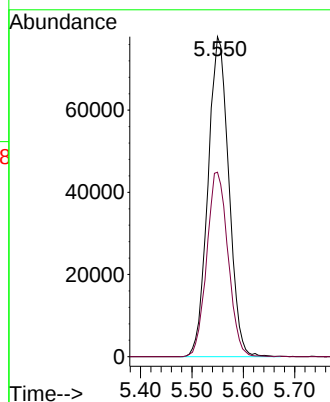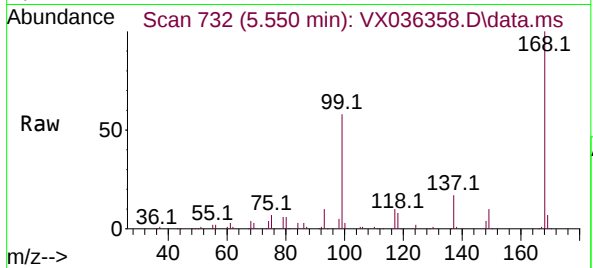

#33
1,2-Dichloroethane-d4
Concen: 52.854 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX036358.D
Acq: 28 Jun 2023 10:50

Tgt Ion: 65 Resp: 165610
Ion Ratio Lower Upper
65 100
67 51.7 0.0 100.2


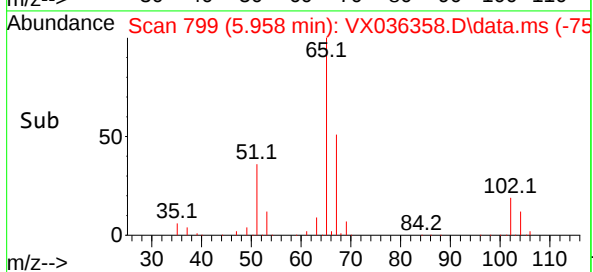
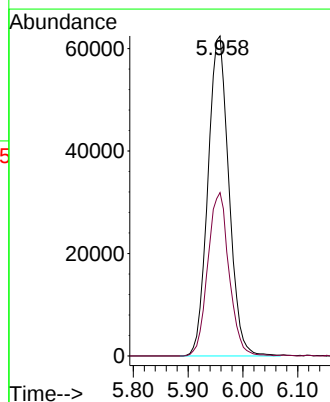
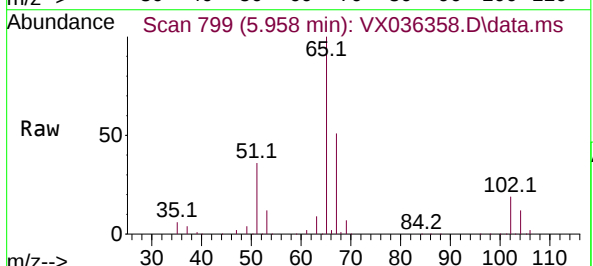


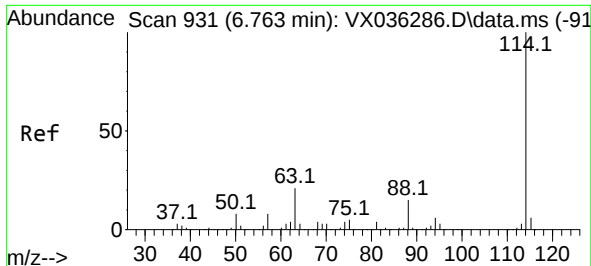

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX036358.D
Acq: 28 Jun 2023 10:50




Instrument :
MSVOA_X
ClientSampleId :
VX0628WBL01


Tgt Ion:114 Resp: 385922
Ion Ratio Lower Upper
114 100
63 19.9 0.0 45.0
88 16.1 0.0 36.6

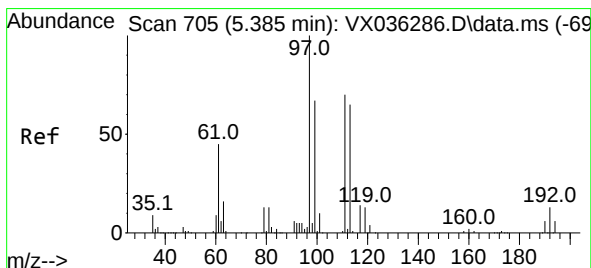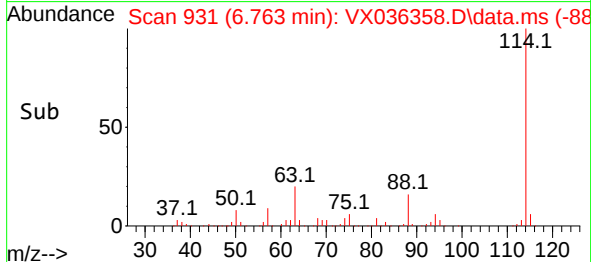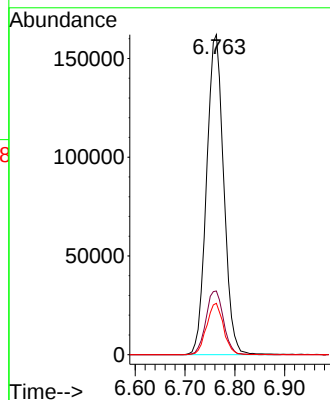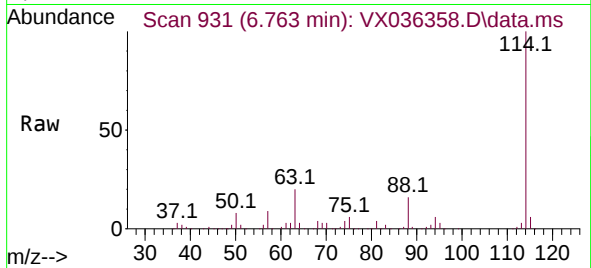

#35
Dibromofluoromethane
Concen: 50.252 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX036358.D
Acq: 28 Jun 2023 10:50

Tgt Ion:113 Resp: 127875
Ion Ratio Lower Upper
113 100
111 103.2 82.9 124.3
192 19.3 13.3 19.9

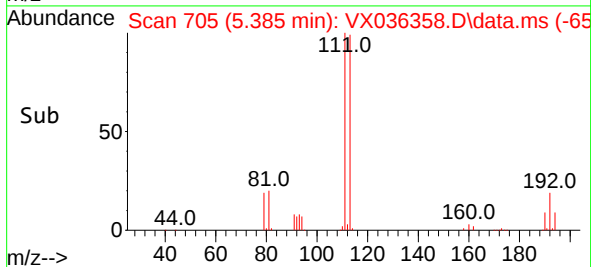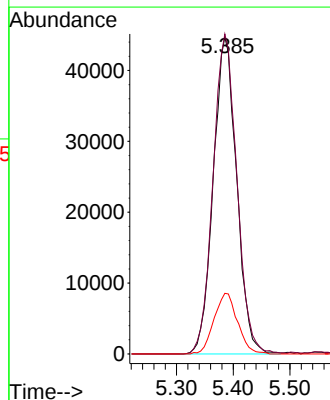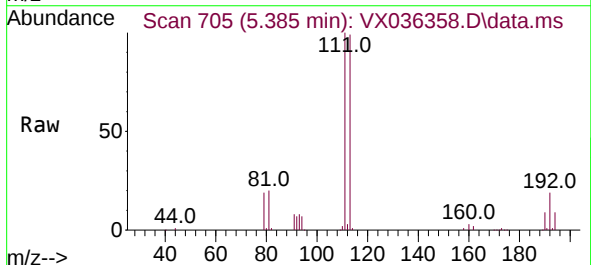

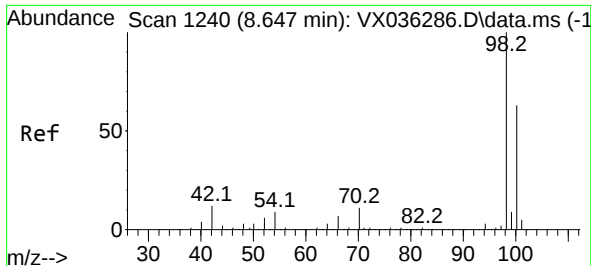

#50

Toluene-d8

Concen: 48.671 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.001 min

Lab File: VX036358.D

Acq: 28 Jun 2023 10:50

Instrument :

MSVOA_X

ClientSampleId :





VX0628WBL01

Tgt Ion: 98 Resp: 462586

Ion Ratio Lower Upper

98 100

100 64.0 53.1 79.7

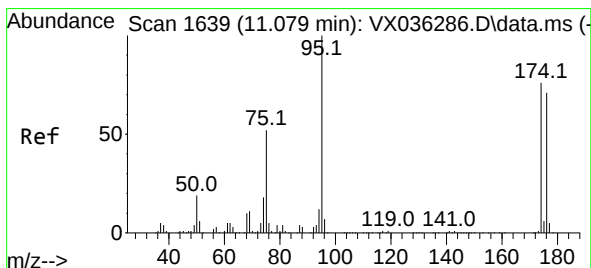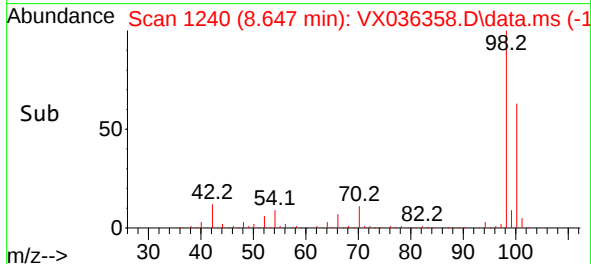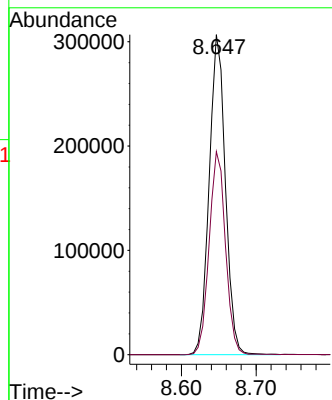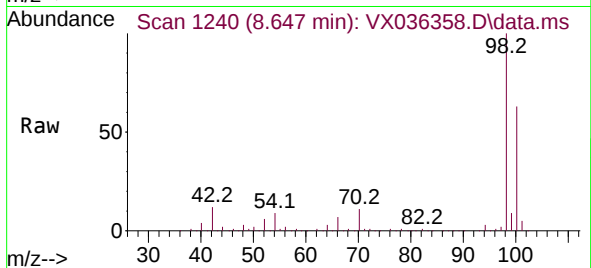

#62

4-Bromofluorobenzene

Concen: 49.508 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX036358.D

Acq: 28 Jun 2023 10:50




Tgt Ion: 95 Resp: 165740


Ion Ratio Lower Upper

95 100

174 78.7 0.0 135.6

176 75.3 0.0 131.0

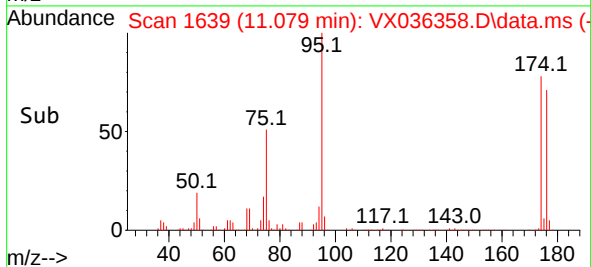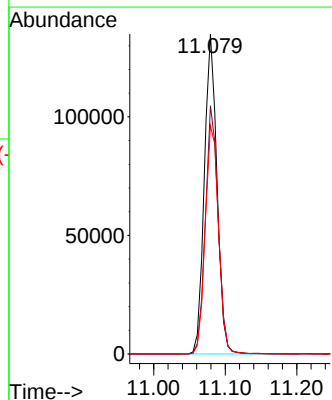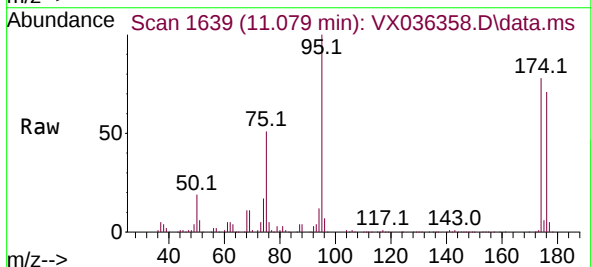

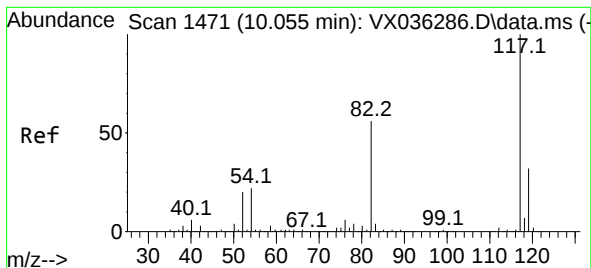

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX036358.D

Acq: 28 Jun 2023 10:50

Instrument :

MSVOA_X

ClientSampleId :

VX0628WBL01





Tgt Ion:117 Resp: 343347

Ion Ratio Lower Upper

117 100

82 56.0 46.2 69.4

119 32.7 25.5 38.3

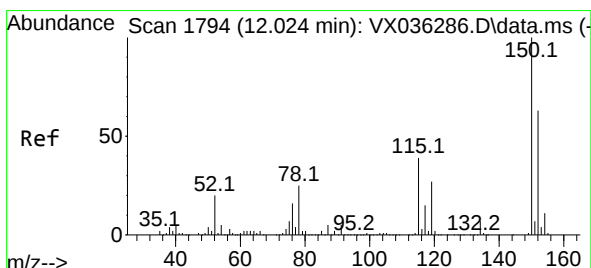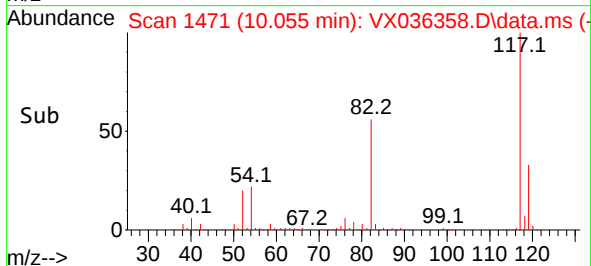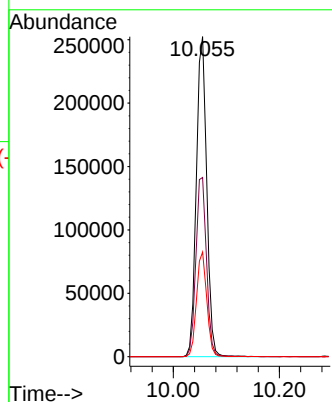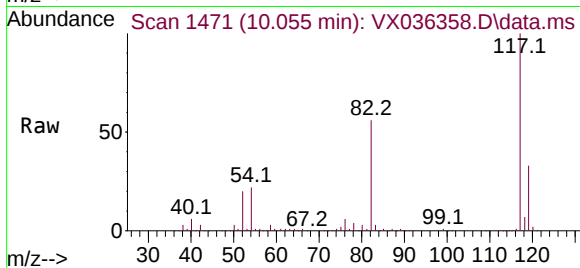

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. -0.006 min

Lab File: VX036358.D

Acq: 28 Jun 2023 10:50

Tgt Ion:152 Resp: 159120

Ion Ratio Lower Upper

152 100

115 58.6 43.3 129.9

150 155.3 0.0 345.0

