
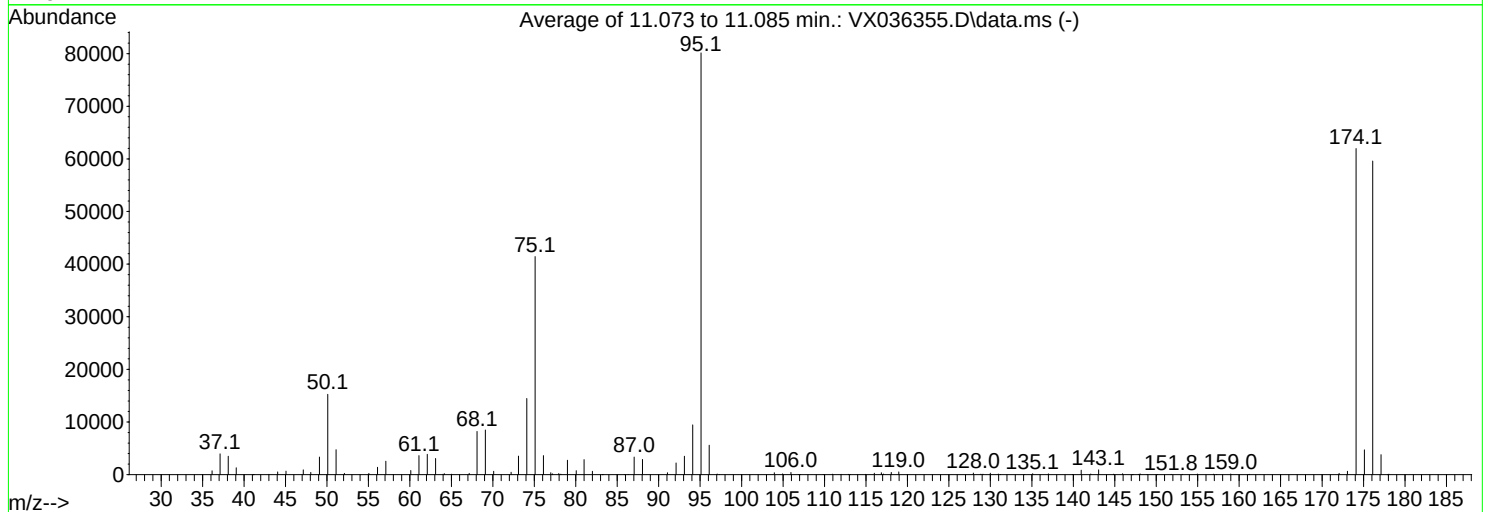


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062823\
Data File : VX036355.D
Acq On : 28 Jun 2023 09:27
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Title : SW846 8260
Last Update : Fri Jun 23 15:03:28 2023

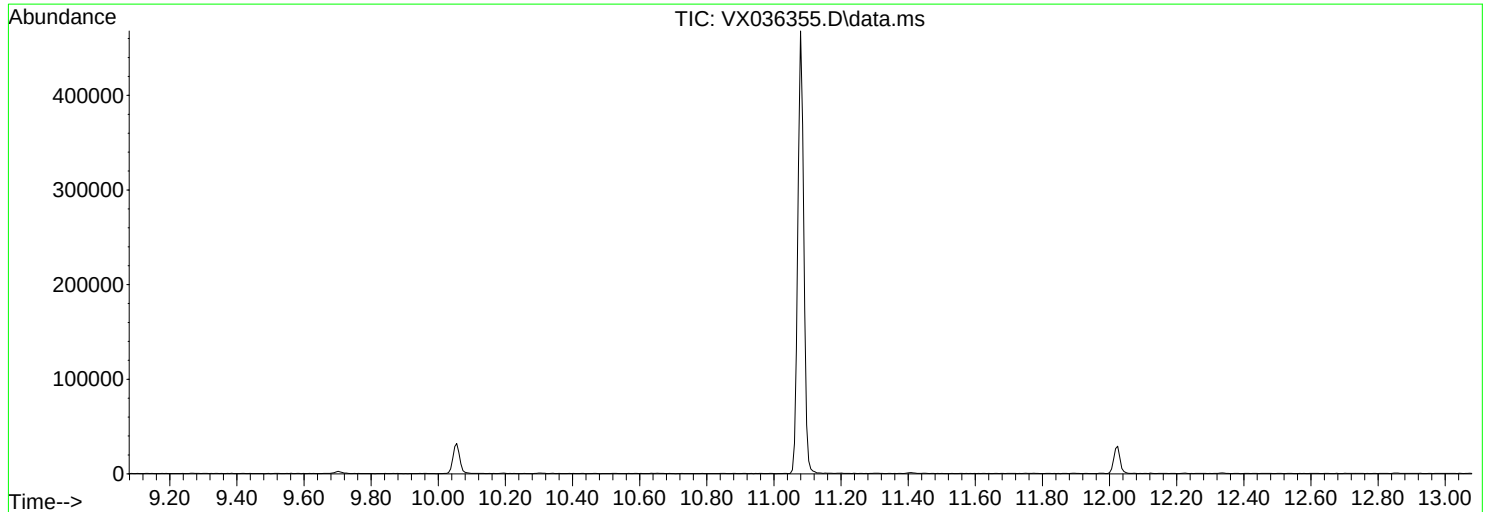

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.0	15267	PASS
75	95	30	60	51.7	41432	PASS
95	95	100	100	100.0	80149	PASS
96	95	5	9	7.0	5586	PASS
173	174	0.00	2	1.0	628	PASS
174	95	50	100	77.3	61949	PASS
175	174	5	9	7.6	4715	PASS
176	174	95	101	96.2	59584	PASS
177	176	5	9	6.4	3794	PASS