

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062918\
 Data File : VX003063.D
 Acq On : 30 Jun 2018 06:55
 Operator : JC/MD
 Sample : J3675-06
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S73-0215

Quant Time: Jun 30 09:28:00 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 25 14:38:05 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	291287	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	407280	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	378253	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	216680	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	192815	47.89	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.78%	
35) Dibromofluoromethane	5.51	113	154765	47.98	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.96%	
50) Toluene-d8	8.72	98	565867	48.04	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.08%	
62) 4-Bromofluorobenzene	11.14	95	204718	45.07	ug/l	0.00
Spiked Amount 50.000			Recovery	=	90.14%	
Target Compounds						
16) Acetone	2.45	43	7644	4.58	ug/l	Qvalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062918\
Data File : VX003063.D
Acq On : 30 Jun 2018 06:55
Operator : JC/MD
Sample : J3675-06
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S73-0215

Quant Time: Jun 30 09:28:00 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 25 14:38:05 2018
Response via : Initial Calibration

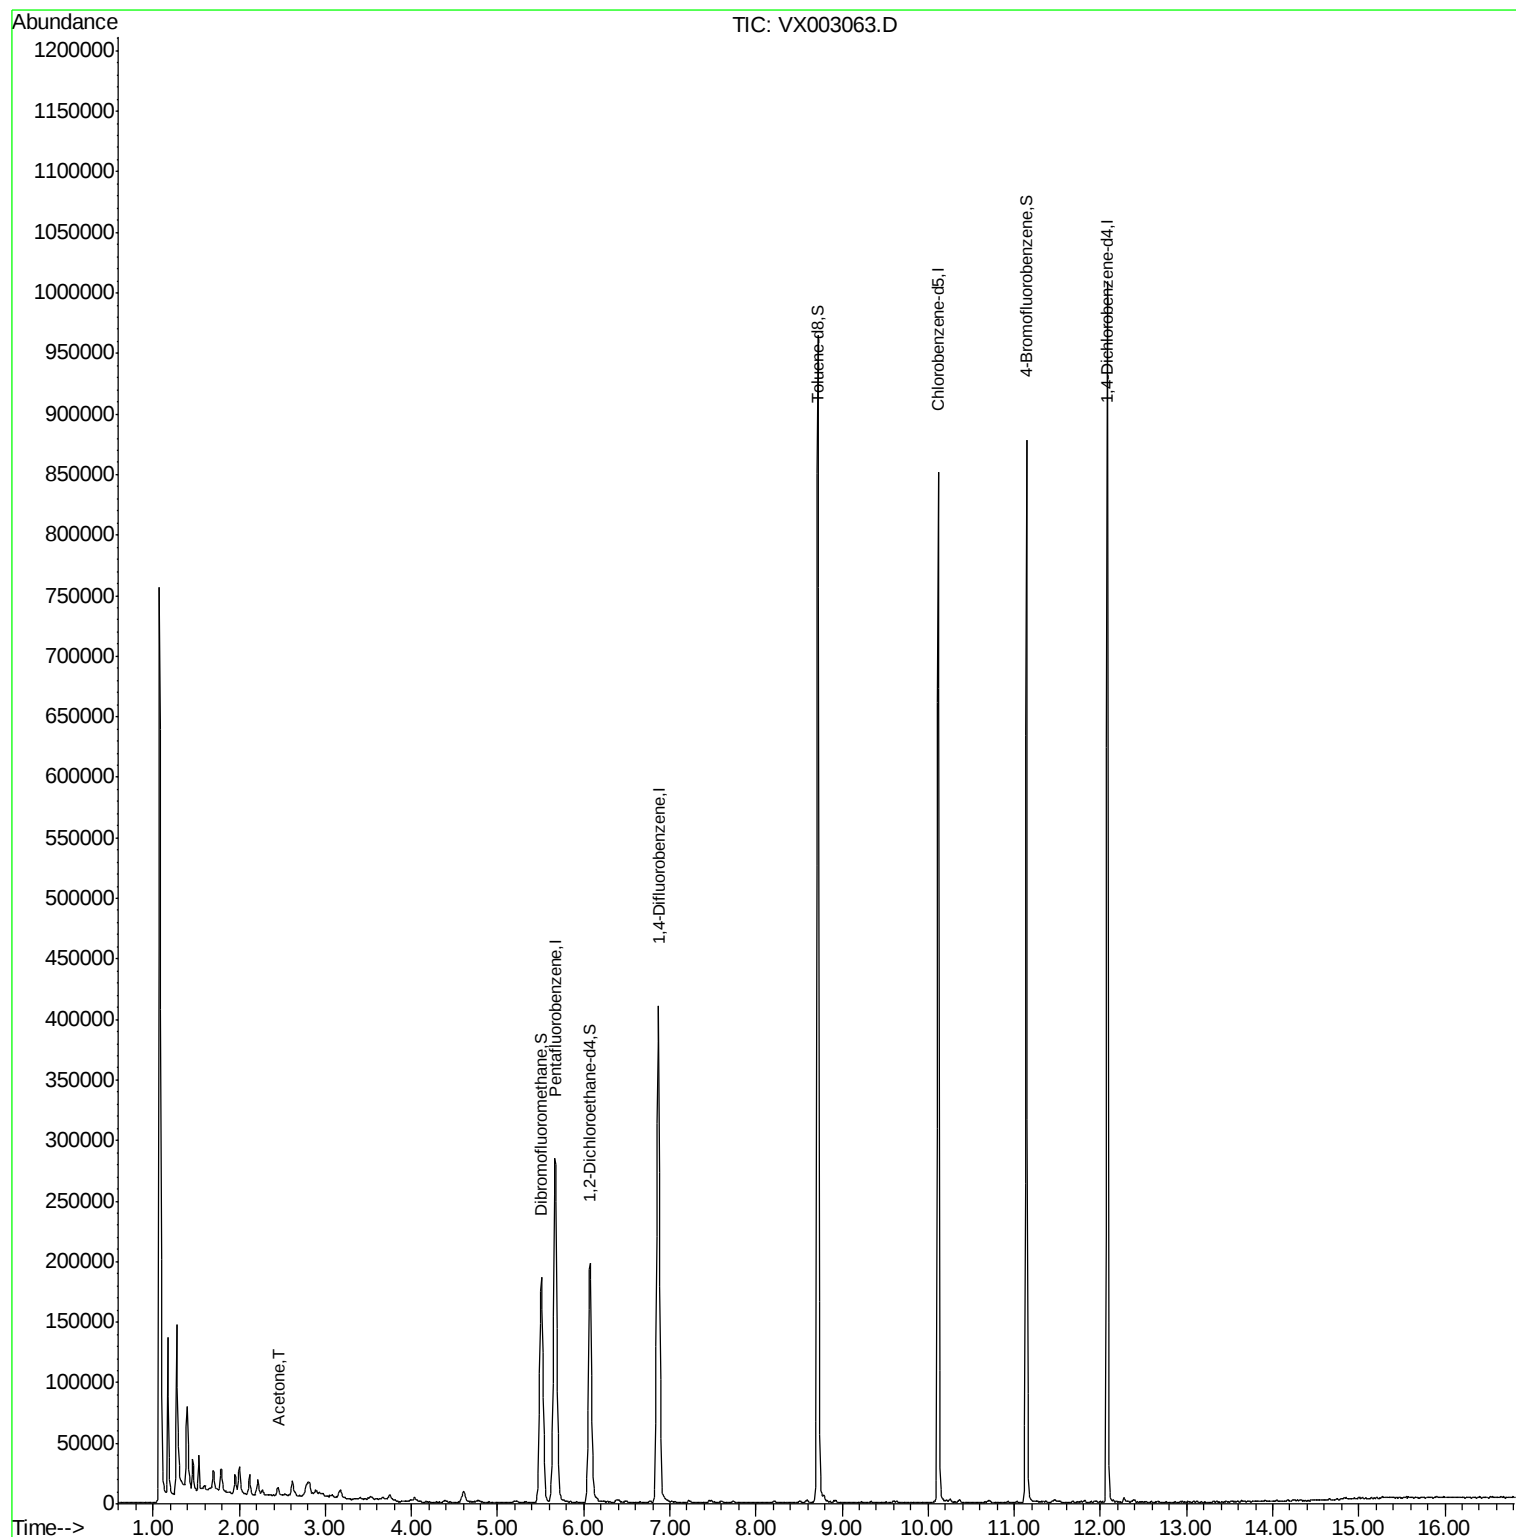



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 833

Delta R.T. -0.00 min

Lab File: VX003063.D

Acq: 30 Jun 2018 06:55

Instrument :

MSVOA_X

ClientSampleId :


S73-0215

Tot Ion:168 Resp: 291287

Ion Ratio Lower Upper

168 100

99 49.4 39.3 58.9

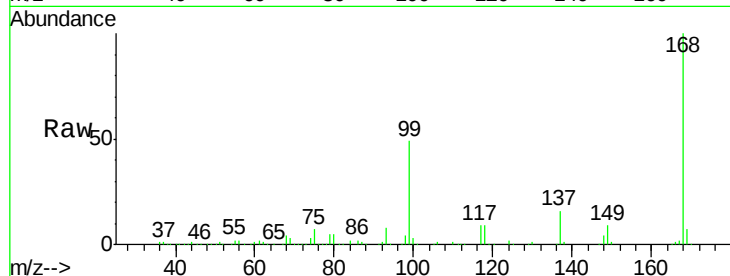

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

120000

100000

80000



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80

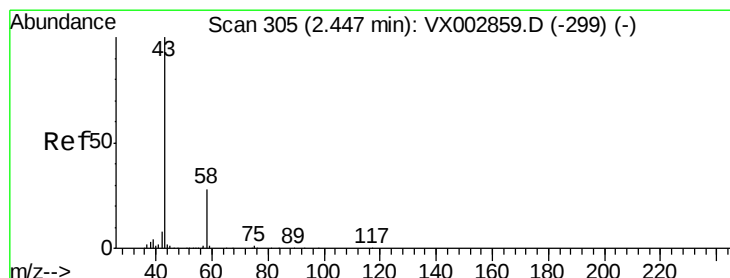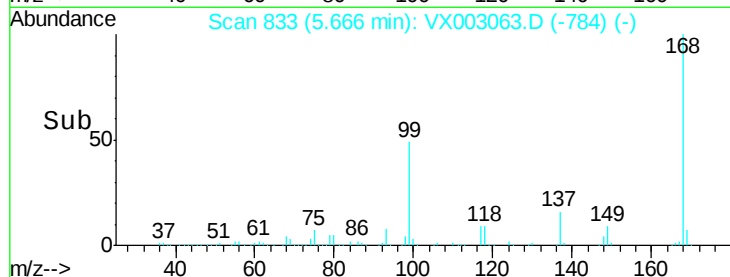

#16

Acetone

Concen: 4.58 ug/l

RT: 2.45 min Scan# 305

Delta R.T. -0.00 min

Lab File: VX003063.D


Acq: 30 Jun 2018 06:55

Tgt Ion: 43 Resp: 7644

Ion Ratio Lower Upper

43 100

58 26.1 22.1 33.1

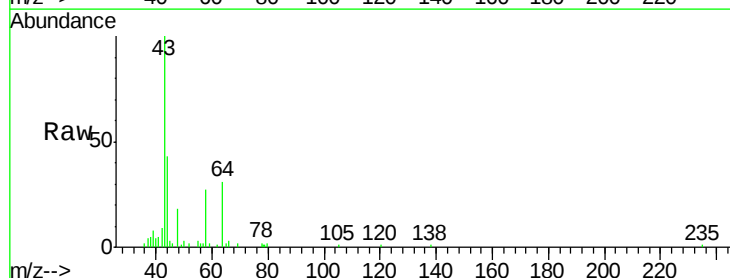

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

2.45

5000

4000


3000


2000

1000

0

Time--> 2.35 2.40 2.45 2.50




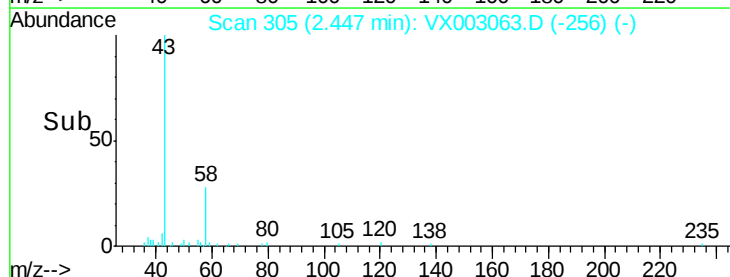


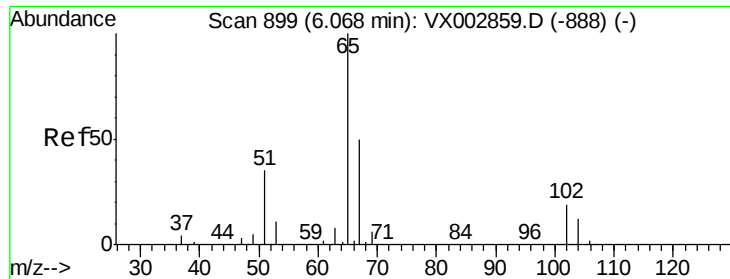

#33
 1,2-Dichloroethane-d4
 Concen: 47.89 ug/l
 RT: 6.07 min Scan# 900
 Delta R.T. 0.01 min
 Lab File: VX003063.D
 Acq: 30 Jun 2018 06:55




Instrument :
 MSVOA_X
 ClientSampleId :
 S73-0215


Tot Ion: 65 Resp: 192815
 Ion Ratio Lower Upper
 65 100
 67 50.5 0.0 102.6

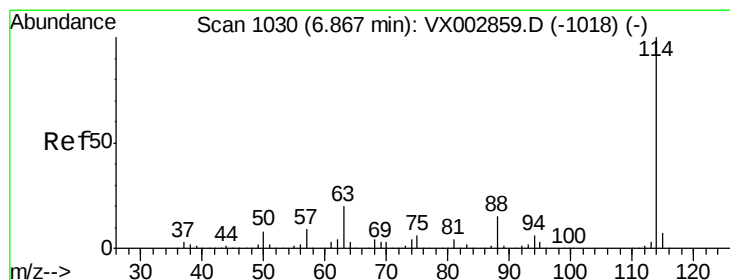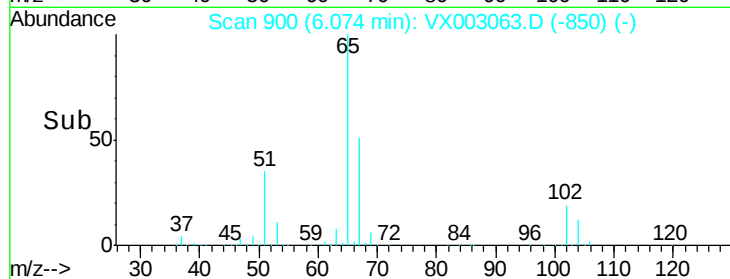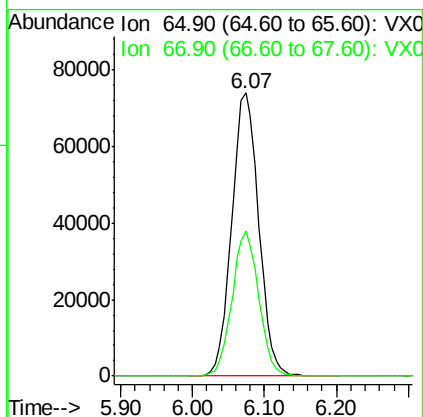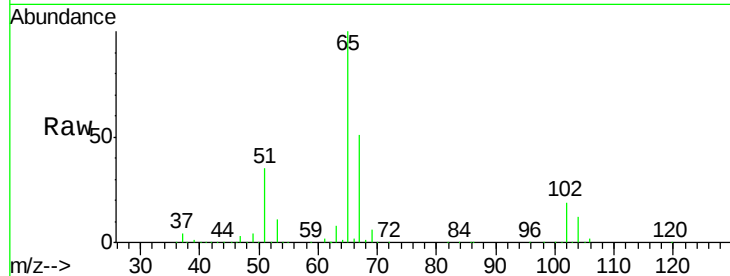

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 6.87 min Scan# 1030
 Delta R.T. -0.00 min
 Lab File: VX003063.D
 Acq: 30 Jun 2018 06:55

Tgt Ion: 114 Resp: 407280
 Ion Ratio Lower Upper
 114 100
 63 19.2 0.0 41.4
 88 13.8 0.0 30.0


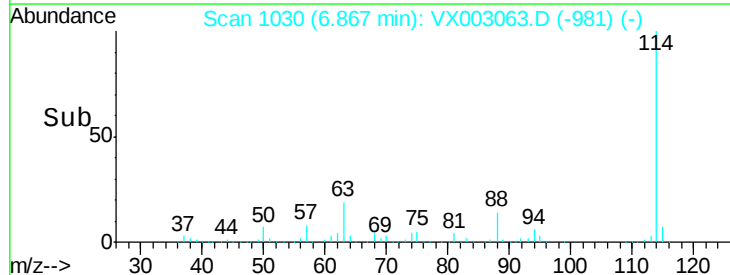
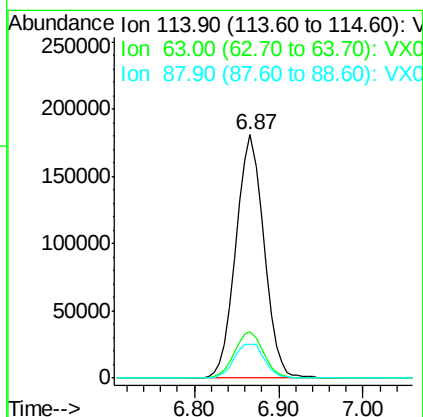
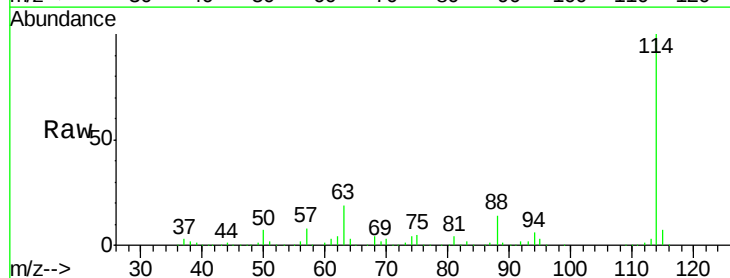


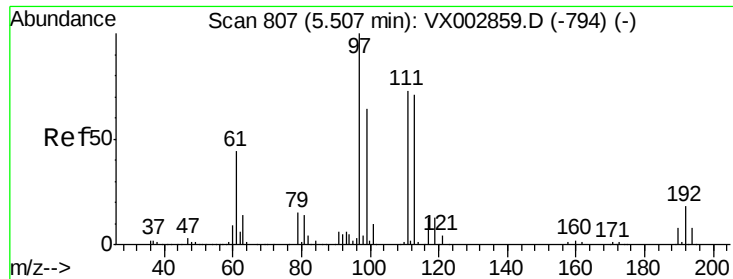

#35
 Dibromofluoromethane
 Concen: 47.98 ug/l
 RT: 5.51 min Scan# 807
 Delta R.T. -0.00 min
 Lab File: VX003063.D
 Acq: 30 Jun 2018 06:55




Instrument :
 MSVOA_X
 ClientSampleId :
 S73-0215


Tot Ion:113 Resp: 154765
 Ion Ratio Lower Upper
 113 100
 111 101.5 81.4 122.0
 192 24.7 19.1 28.7

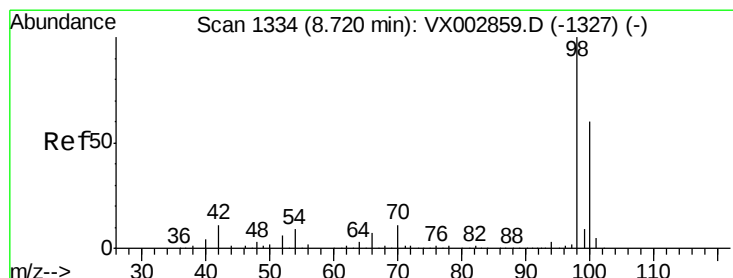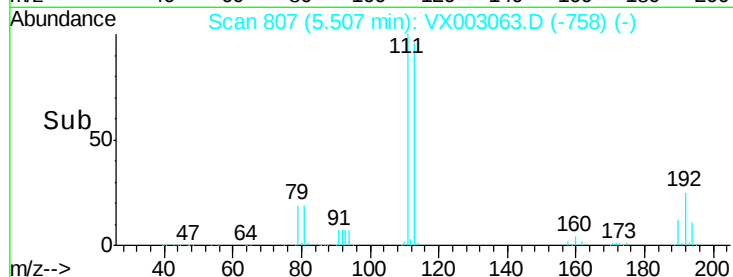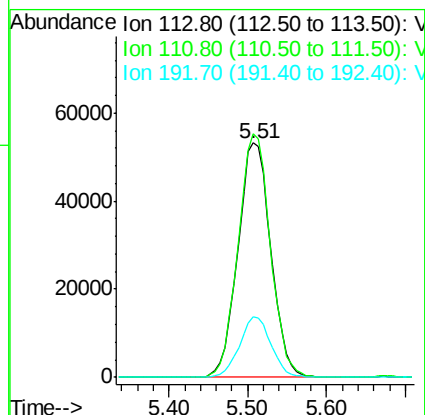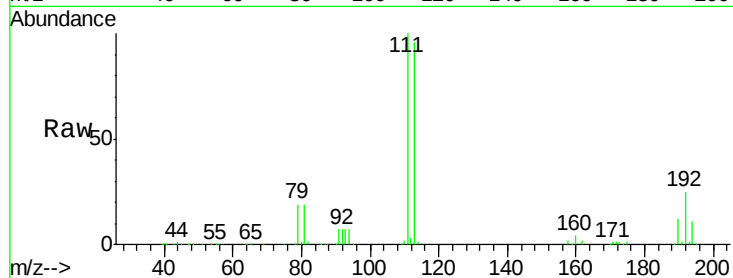

#50
 Toluene-d8
 Concen: 48.04 ug/l
 RT: 8.72 min Scan# 1334
 Delta R.T. 0.00 min
 Lab File: VX003063.D
 Acq: 30 Jun 2018 06:55

Tgt Ion: 98 Resp: 565867
 Ion Ratio Lower Upper
 98 100
 100 63.8 50.9 76.3


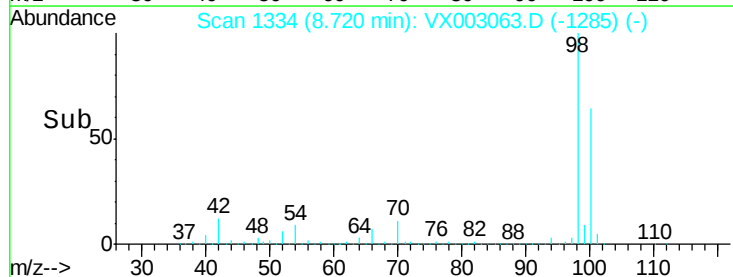
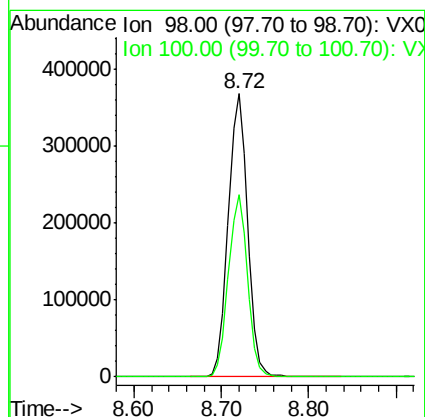
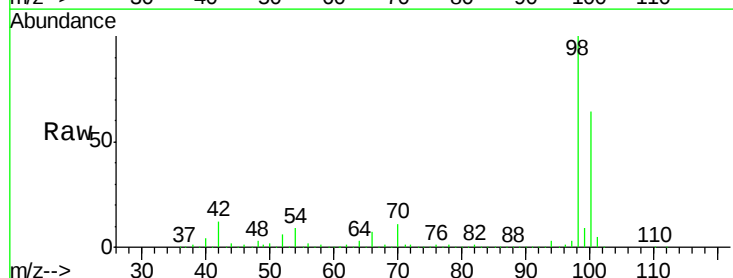


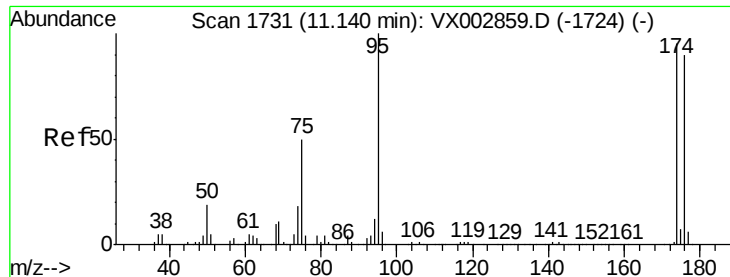

#62
4-Bromofluorobenzene
Concen: 45.07 ug/l
RT: 11.14 min Scan# 1731
Delta R.T. 0.00 min
Lab File: VX003063.D
Acq: 30 Jun 2018 06:55




Instrument :
MSVOA_X
ClientSampled :
S73-0215


Tot Ion: 95 Resp: 204718
Ion Ratio Lower Upper
95 100
174 97.6 0.0 187.4
176 93.8 0.0 181.0

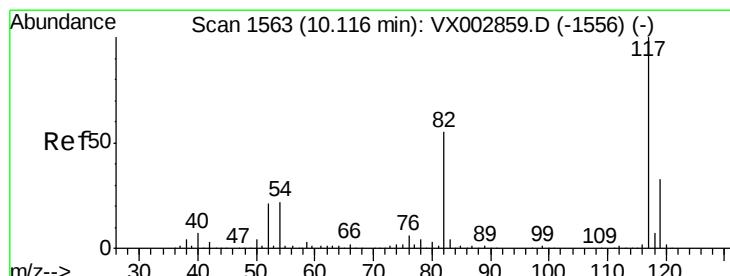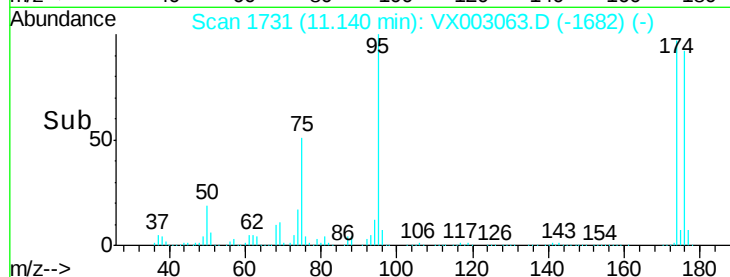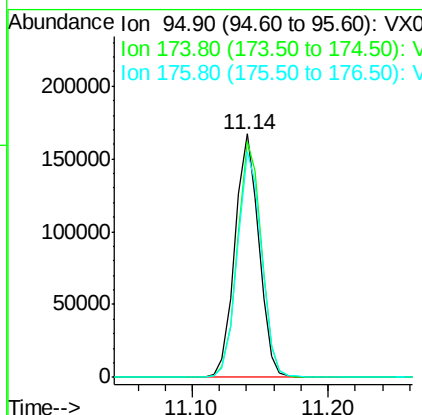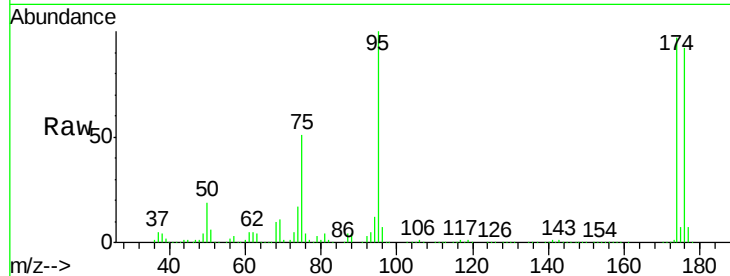

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1563
Delta R.T. -0.00 min
Lab File: VX003063.D
Acq: 30 Jun 2018 06:55

Tgt Ion: 117 Resp: 378253
Ion Ratio Lower Upper
117 100
82 53.2 45.0 67.4
119 32.7 25.8 38.6

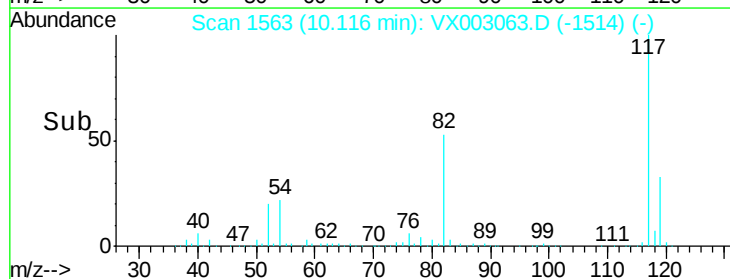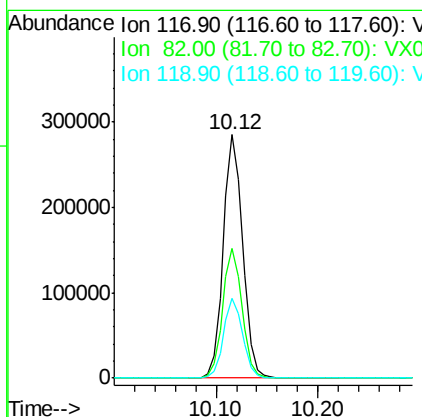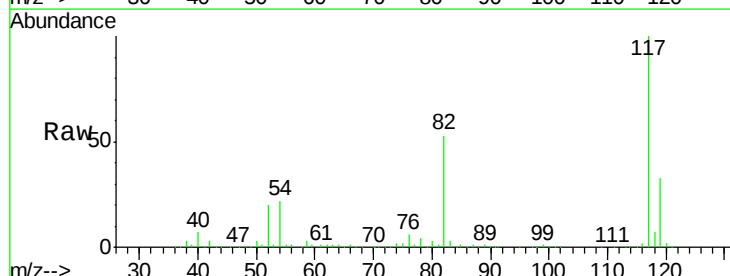

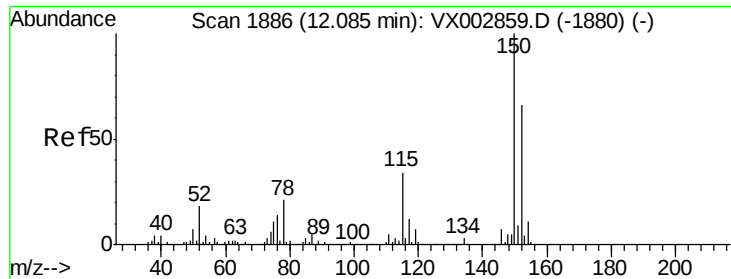

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 12.08 min Scan# 1885

Delta R.T. -0.01 min

Lab File: VX003063.D

Acq: 30 Jun 2018 06:55

Instrument :

MSVOA_X

ClientSampleId :

S73-0215


Tot Ion:152 Resp: 216680

Ion Ratio Lower Upper

152 100

115 54.1 40.1 120.2

150 157.2 0.0 347.2

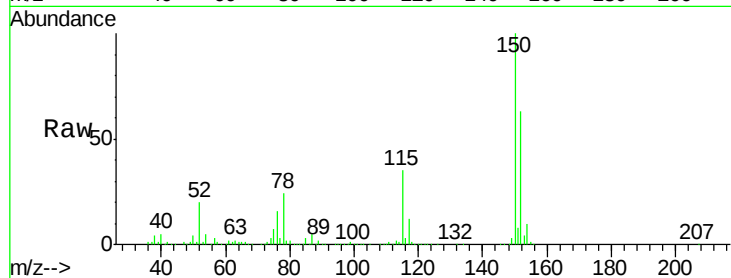

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

