

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062918\
 Data File : VX003068.D
 Acq On : 30 Jun 2018 09:07
 Operator : JC/MD
 Sample : J3675-11MSD
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S73-0217

Quant Time: Jun 30 11:05:12 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 25 14:38:05 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-5.67
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-6.87
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-10.12
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-12.09

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062918\
Data File : VX003068.D
Acq On : 30 Jun 2018 09:07
Operator : JC/MD
Sample : J3675-11MSD
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S73-0217

Quant Time: Jun 30 11:05:12 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 25 14:38:05 2018
Response via : Initial Calibration

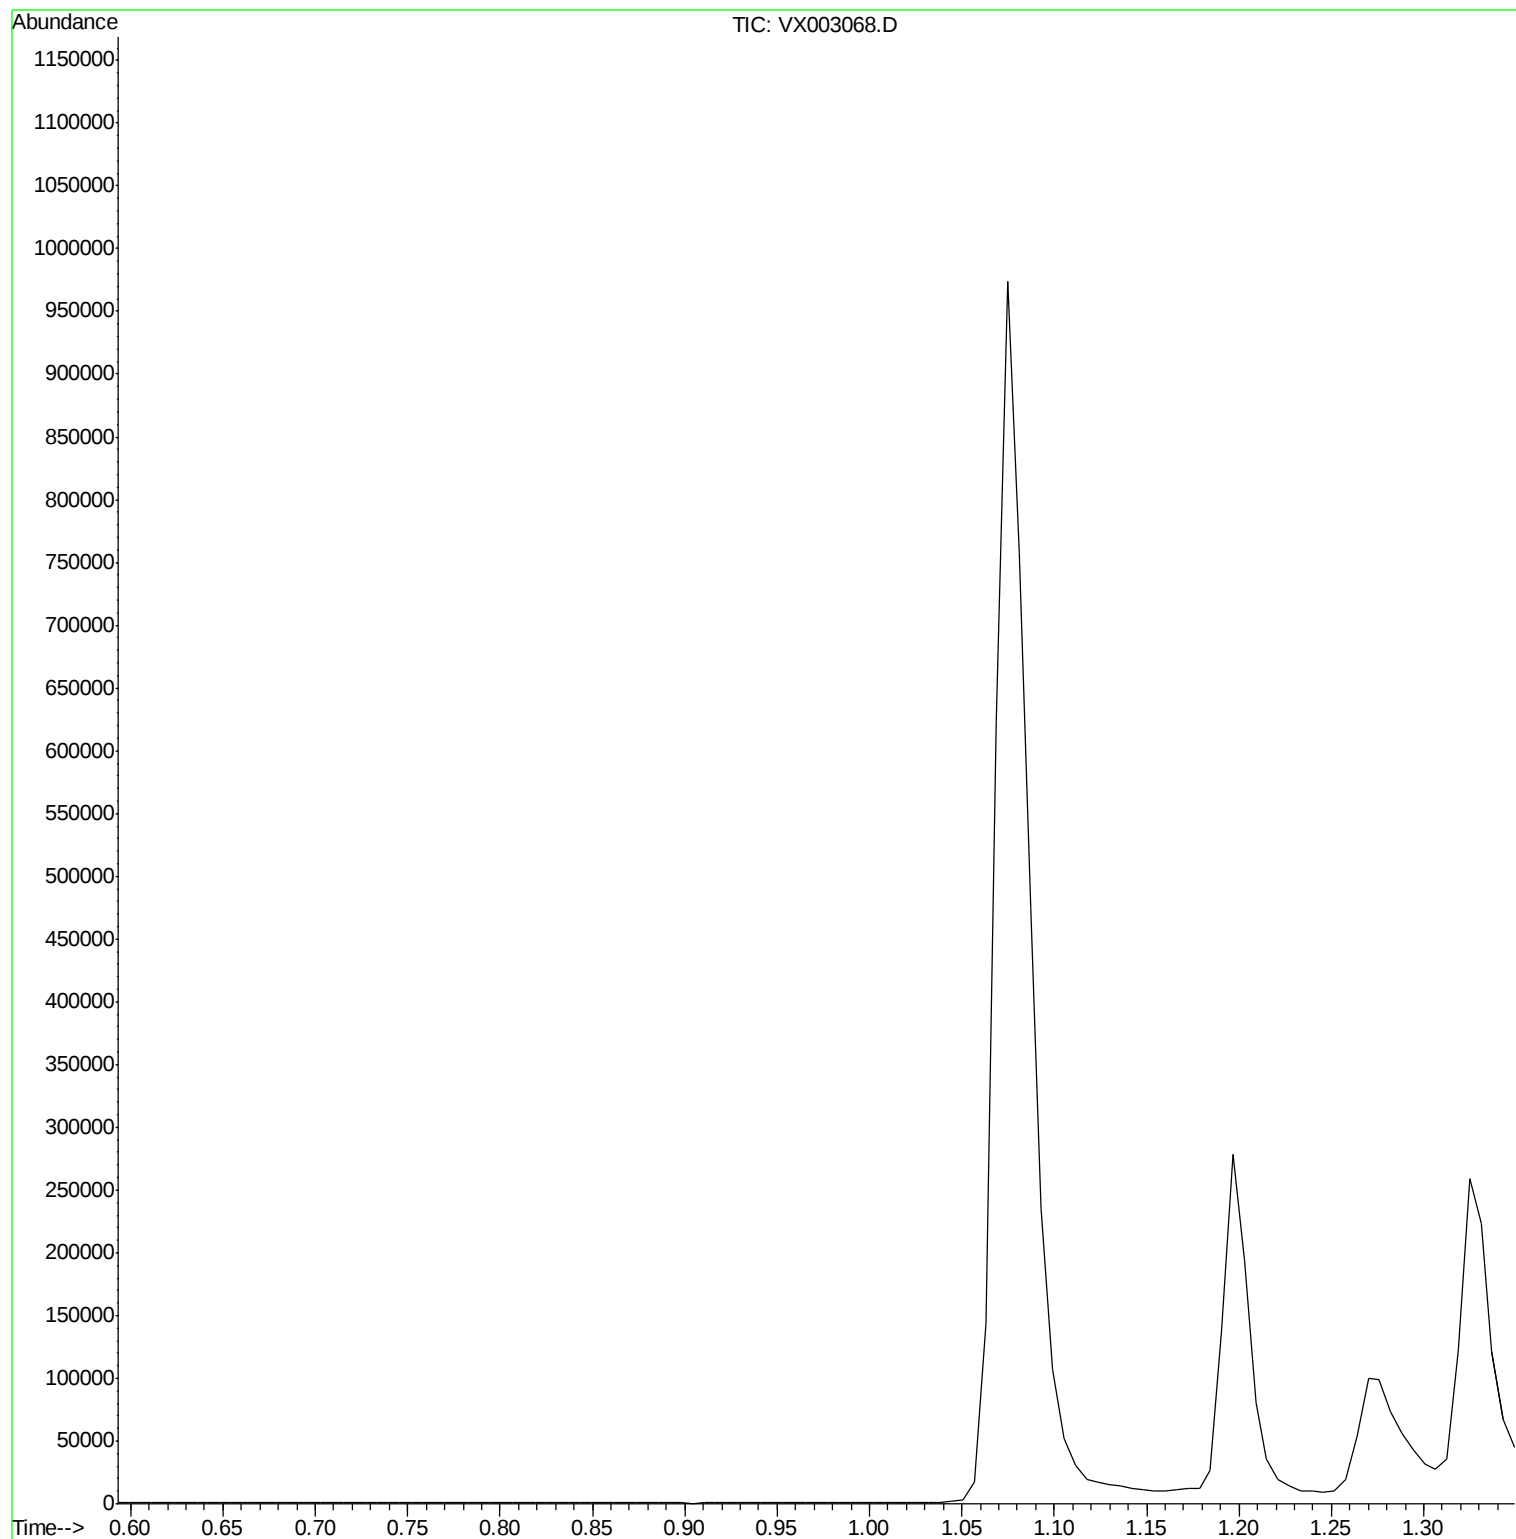


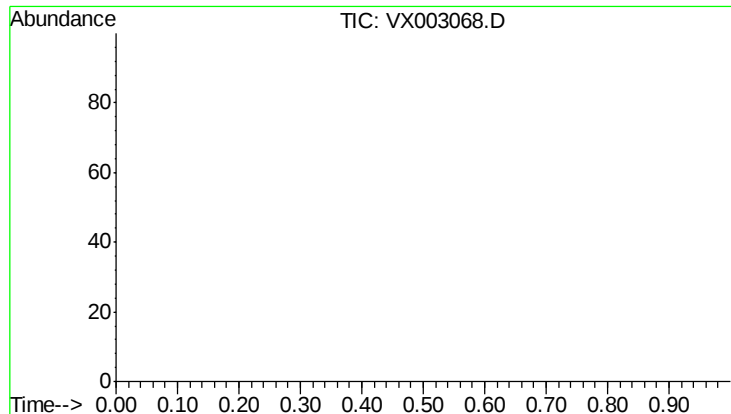


#1
Pentafluorobenzene
Concen: 0.00 ug/l
Expected RT: 5.67 min

Lab File: VX003068.D
Acq: 30 Jun 2018 09:07

Instrument :
MSVOA_X
ClientSampleId :
S73-0217


Tot Ion:	168
Sig	Exp Ratio
168	100
99	49.1

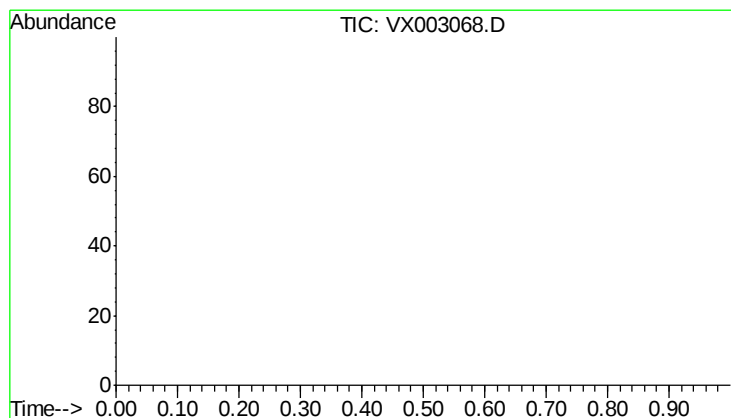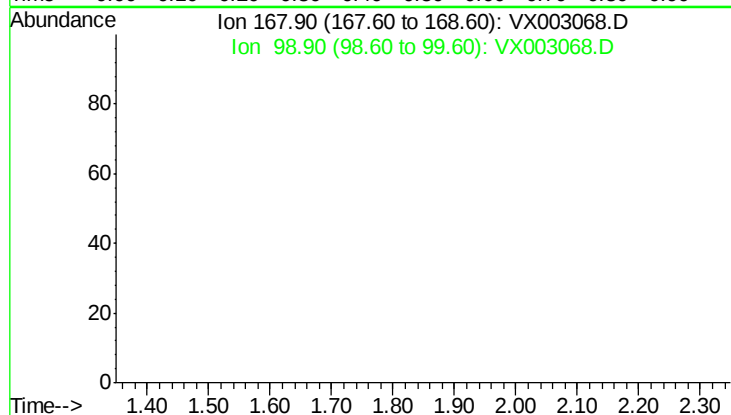


#33
1,2-Dichloroethane-d4
Concen: 0.00 ug/l
Expected RT: 6.07 min

Lab File: VX003068.D
Acq: 30 Jun 2018 09:07

Tgt Ion:	65
Sig	Exp Ratio
65	100
67	51.3


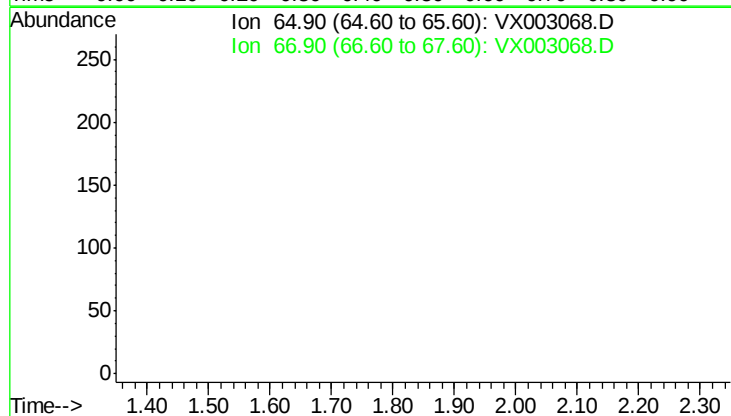


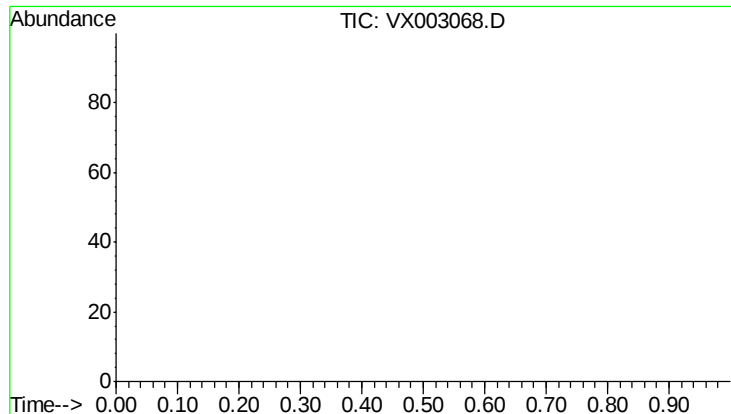

#34
 1,4-Difluorobenzene
 Concen: 0.00 ug/l
 Expected RT: 6.87 min
 Lab File: VX003068.D
 Acq: 30 Jun 2018 09:07


Instrument :
 MSVOA_X
 ClientSampleId :
 S73-0217


Tot Ion	114
Sig	Exp Ratio
114	100
63	20.7
88	15.0

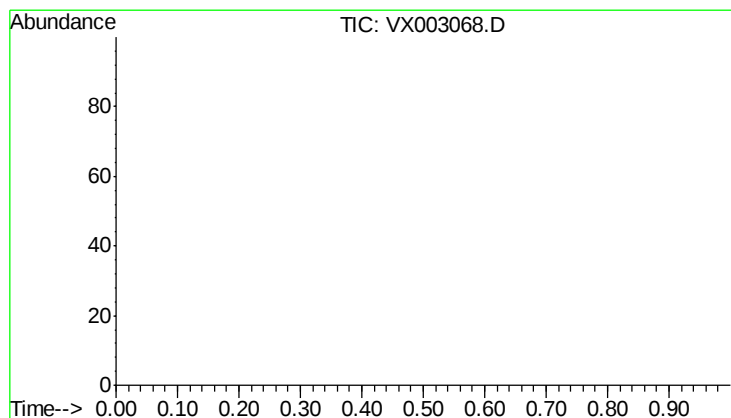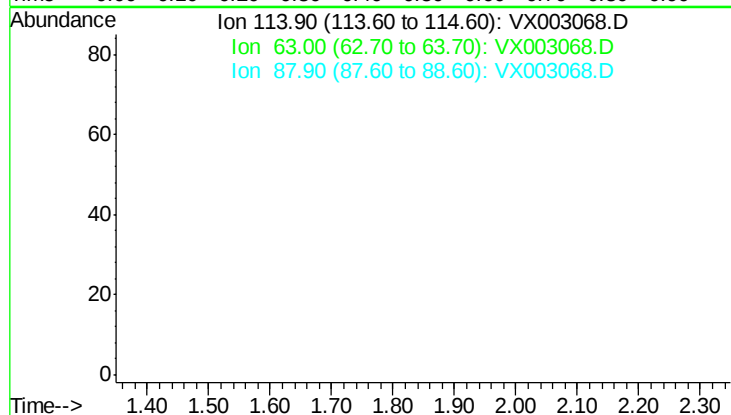

#35
 Dibromofluoromethane
 Concen: 0.00 ug/l
 Expected RT: 5.51 min
 Lab File: VX003068.D
 Acq: 30 Jun 2018 09:07

Tgt Ion	113
Sig	Exp Ratio
113	100
111	101.7
192	23.9

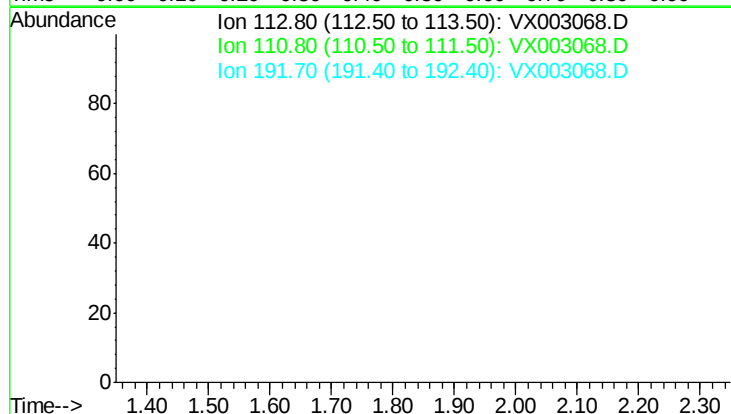


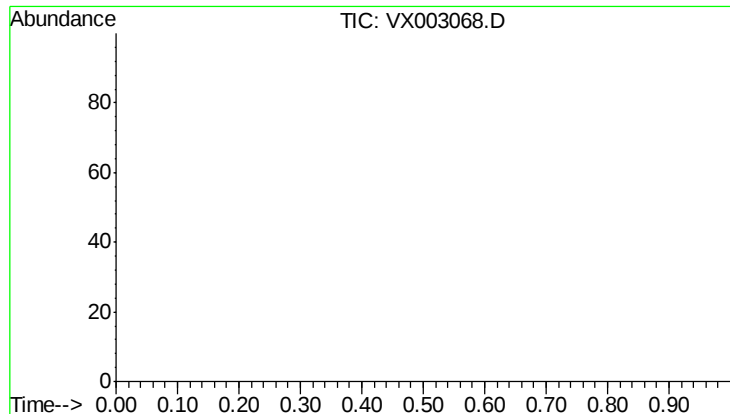


#50
Toluene-d8
Concen: 0.00 ug/l
Expected RT: 8.72 min

Lab File: VX003068.D
Acq: 30 Jun 2018 09:07

Instrument :
MSVOA_X
ClientSampleId :
S73-0217


Tot Ion	Sig	Exp Ratio
98	100	
100	63.6	

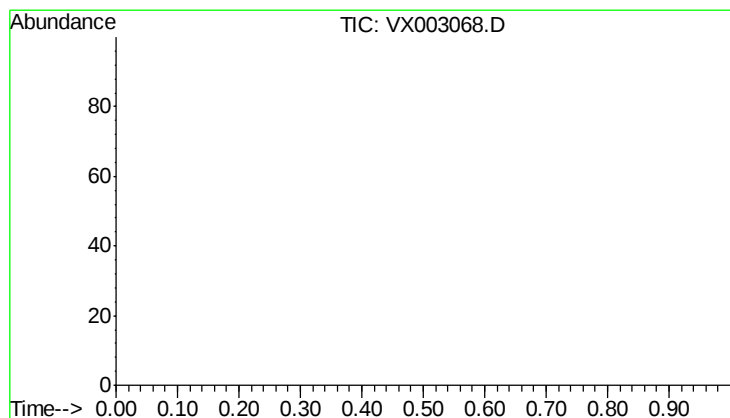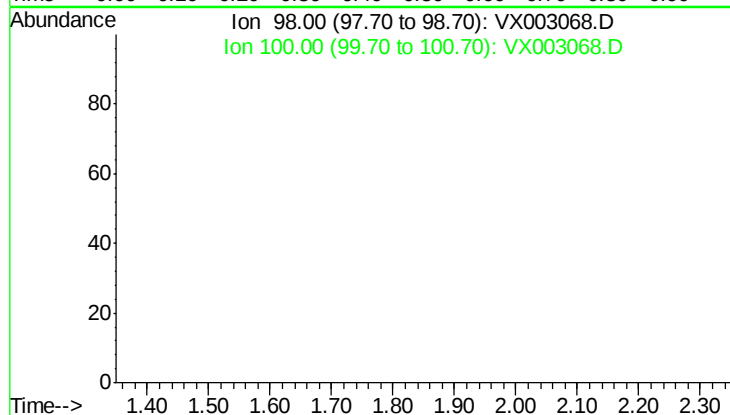


#62
4-Bromofluorobenzene
Concen: 0.00 ug/l
Expected RT: 11.14 min

Lab File: VX003068.D
Acq: 30 Jun 2018 09:07

Tgt Ion	Sig	Exp Ratio
95	100	
174	93.7	
176	90.5	


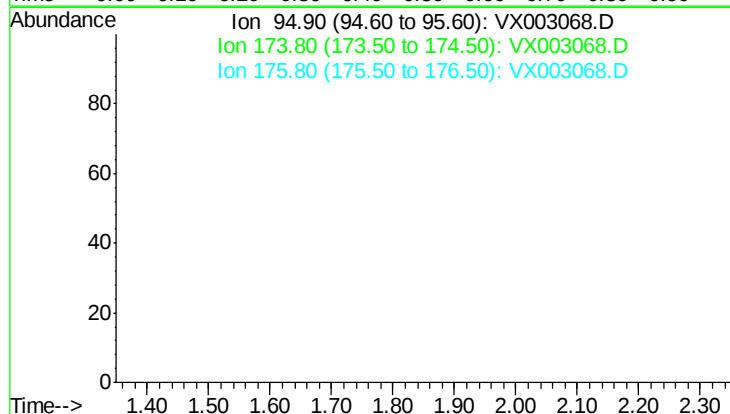


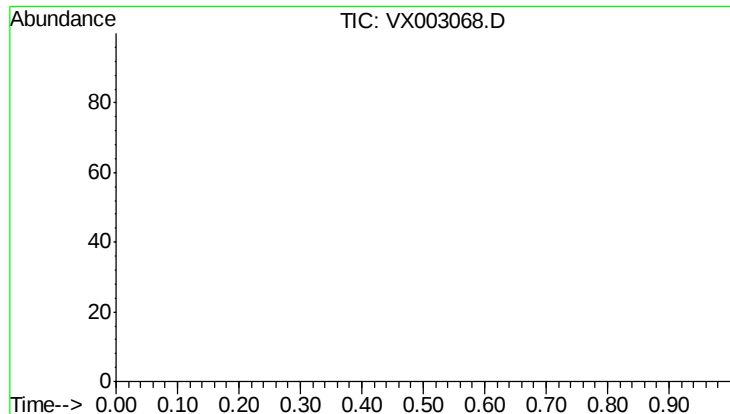

#63
 Chlorobenzene-d5
 Concen: 0.00 ug/l
 Expected RT: 10.12 min
 Lab File: VX003068.D
 Acq: 30 Jun 2018 09:07

Instrument :
 MSVOA_X
 ClientSampleId :
 S73-0217

Tot Ion: 117
 Sig Exp Ratio
 117 100
 82 56.2
 119 32.2

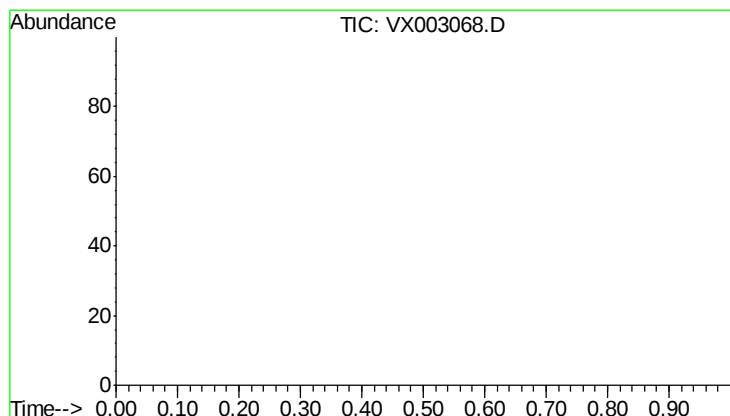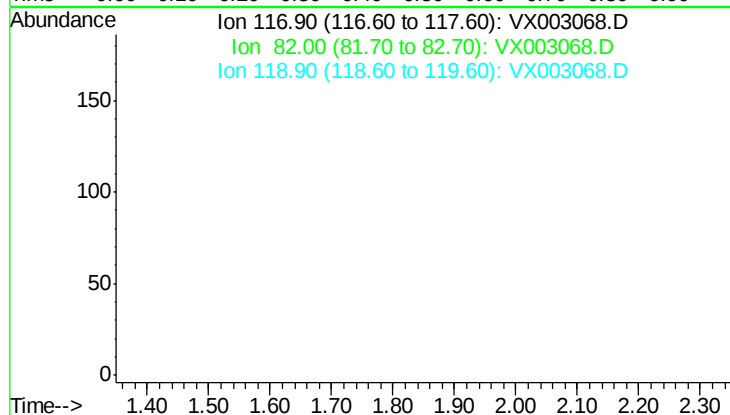

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.00 ug/l
 Expected RT: 12.09 min
 Lab File: VX003068.D
 Acq: 30 Jun 2018 09:07

Tgt Ion: 152
 Sig Exp Ratio
 152 100
 115 80.1
 150 173.6

