




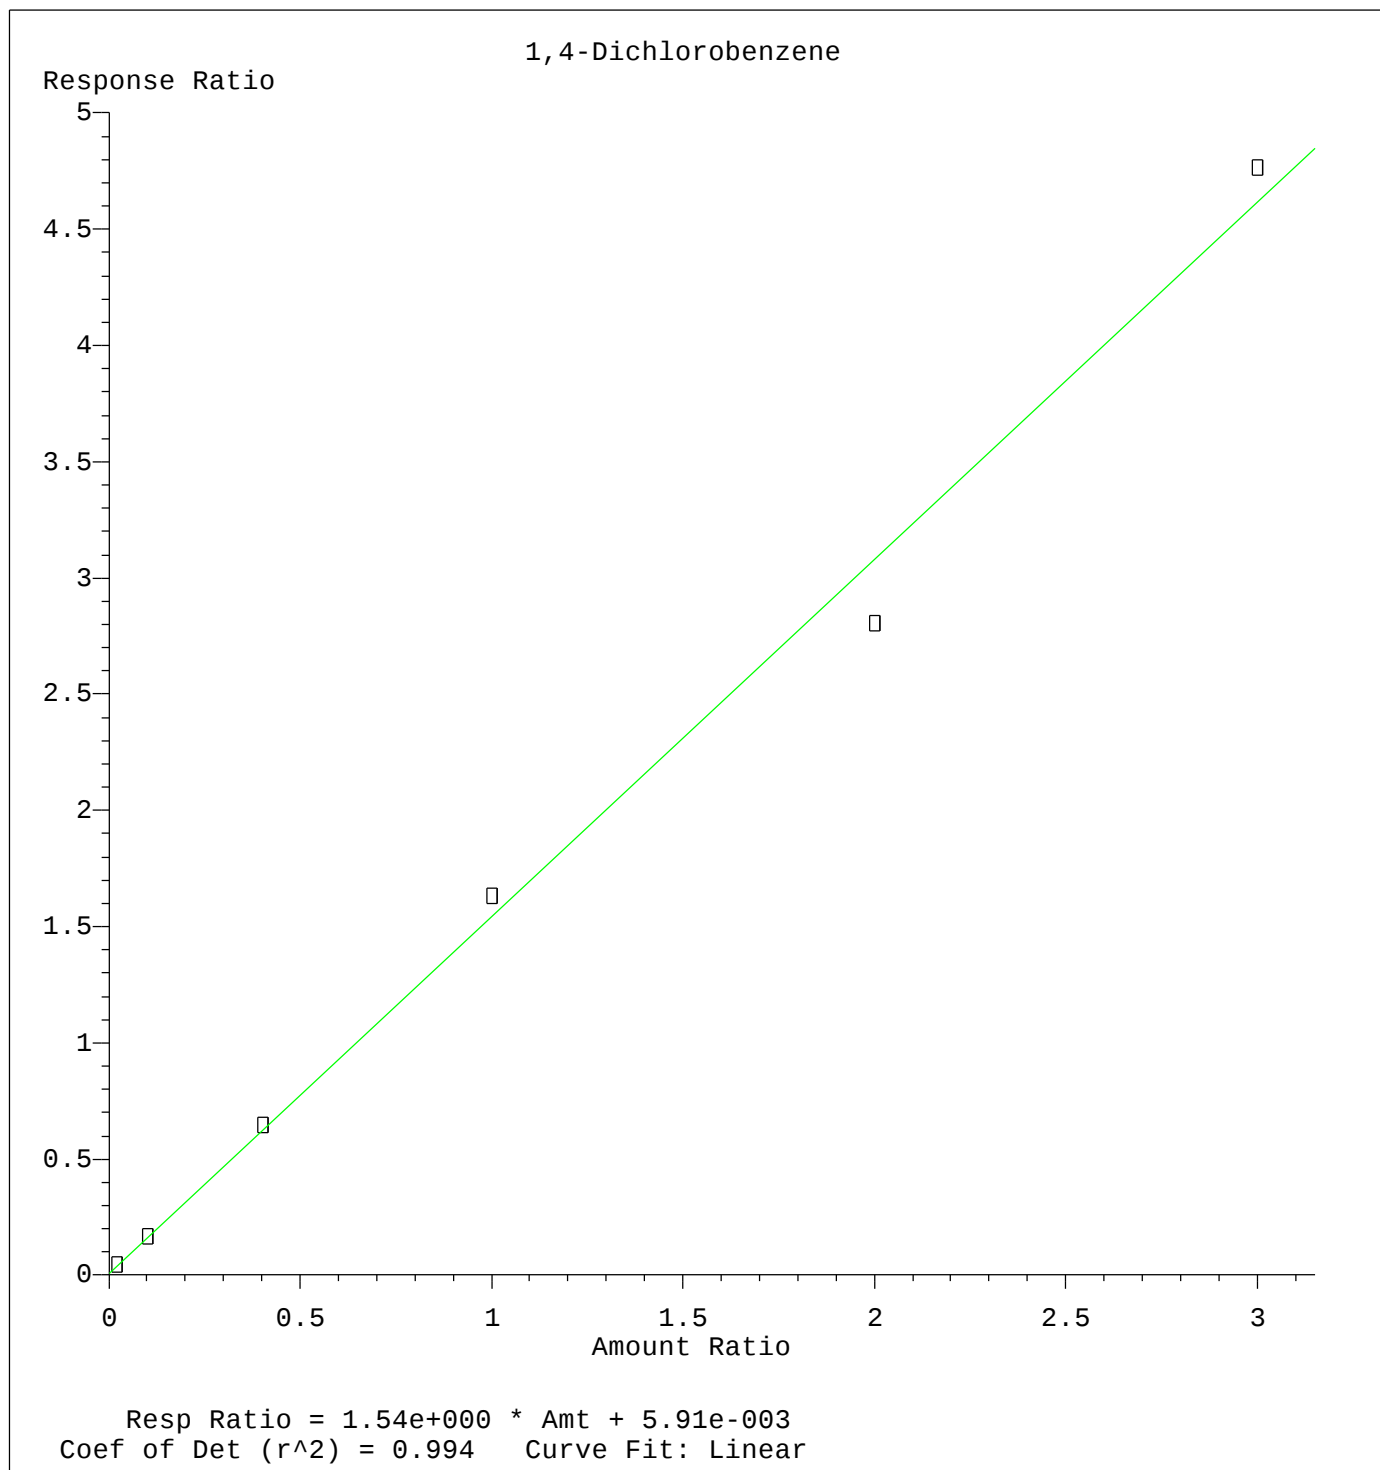


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
Calibration Table Last Updated: Mon Jun 29 17:10:38 2020

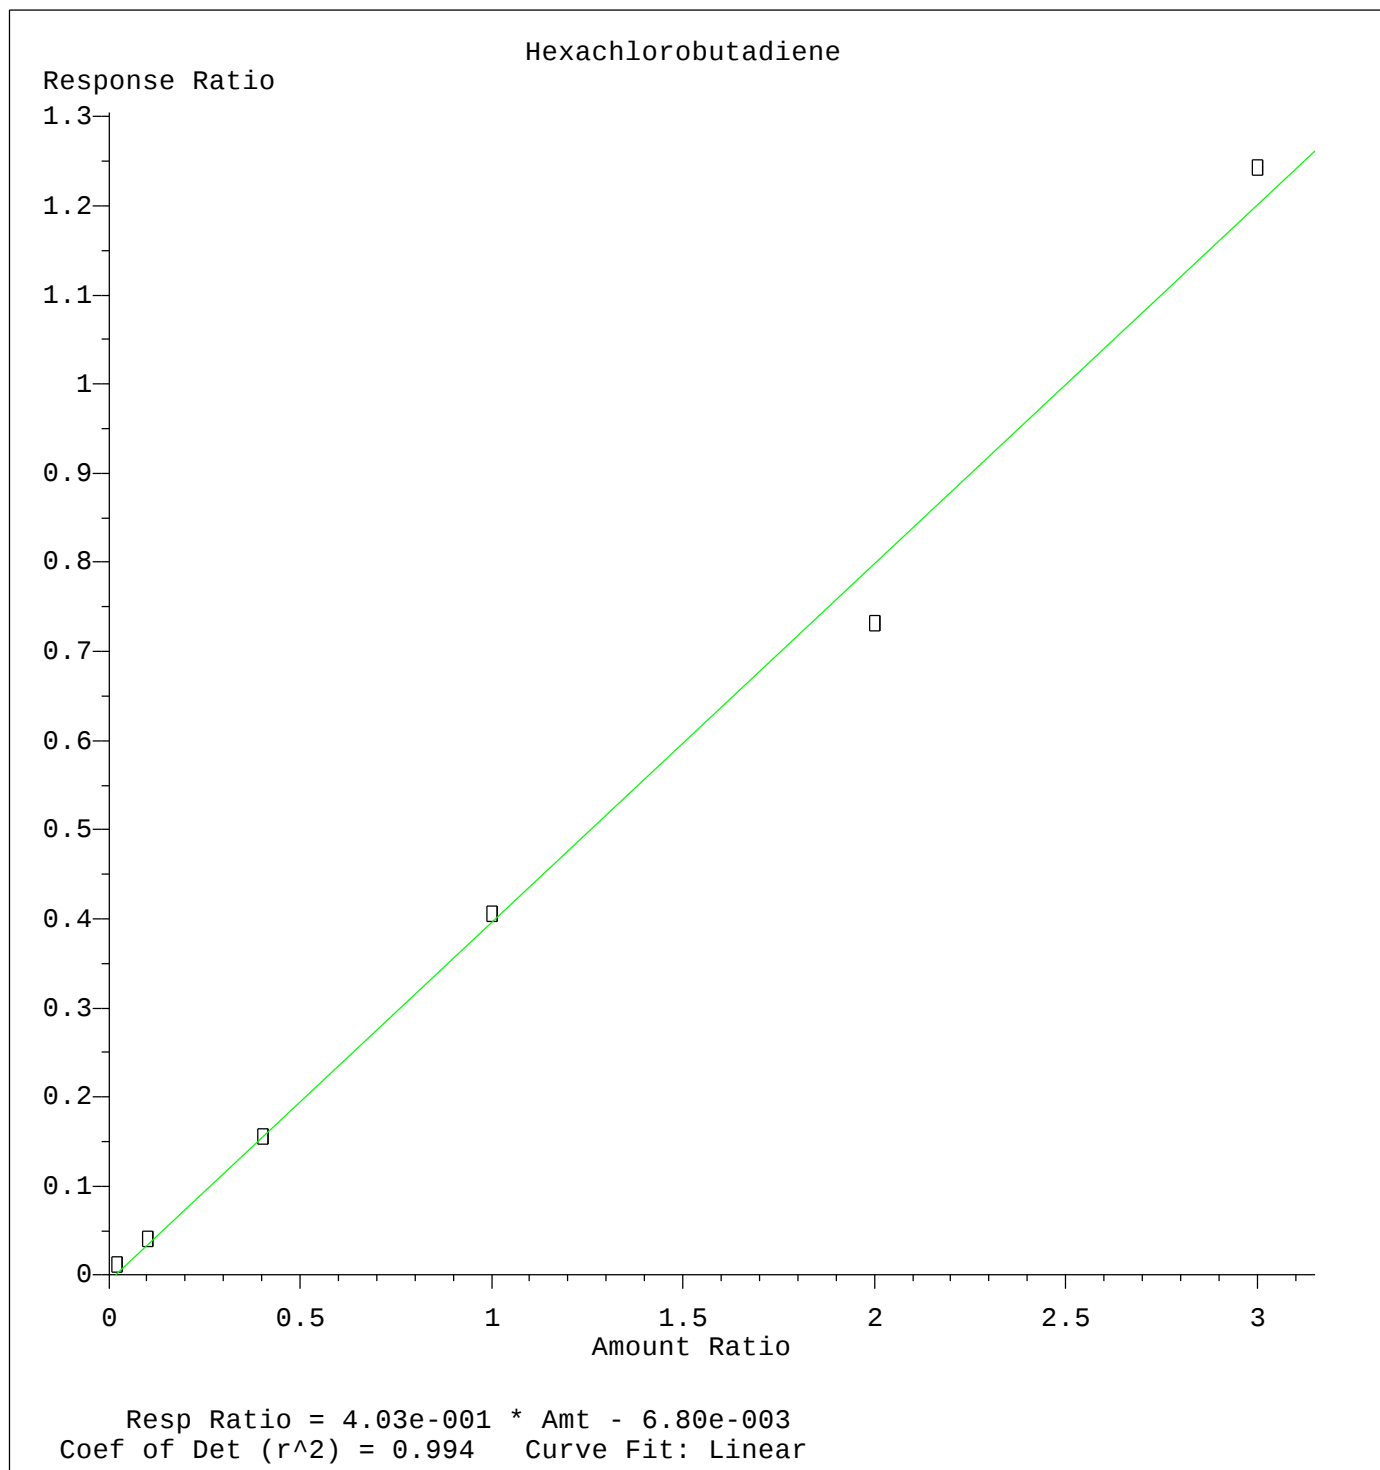

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
Calibration Table Last Updated: Mon Jun 29 17:10:38 2020

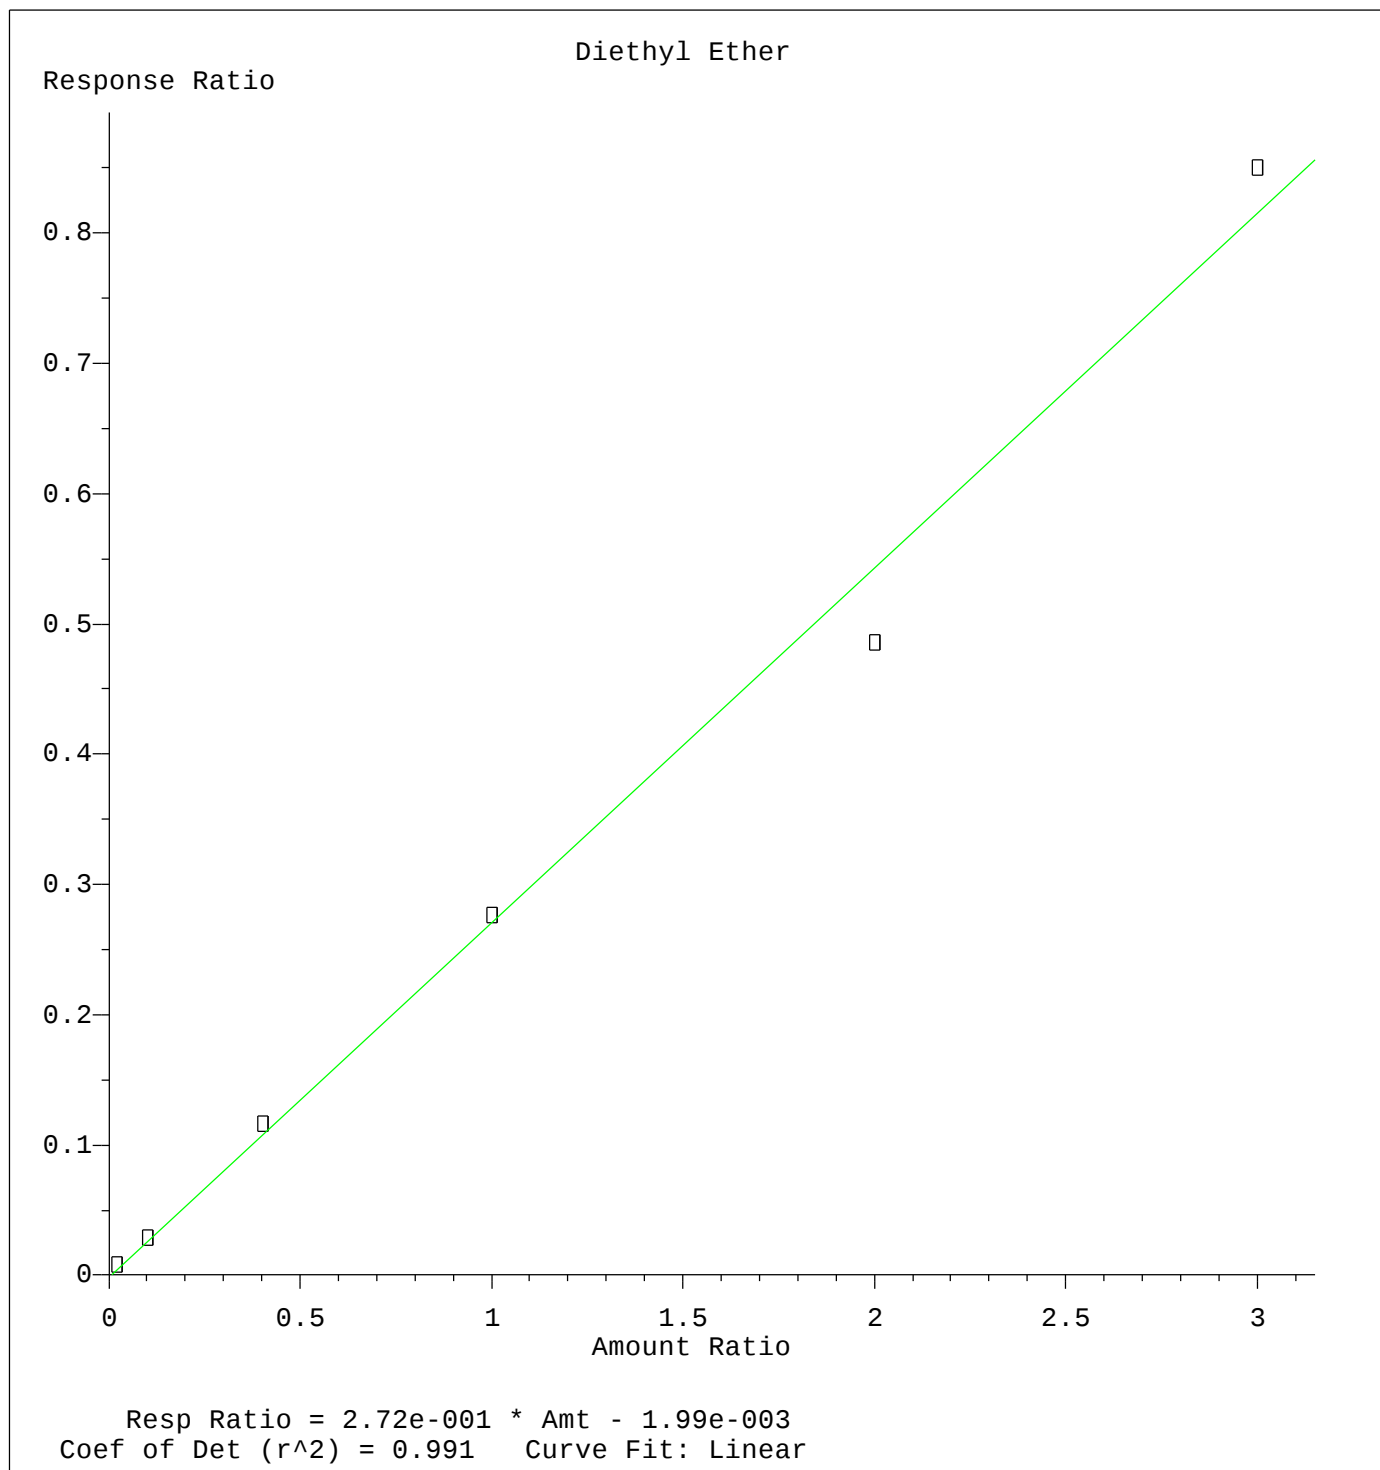


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
Calibration Table Last Updated: Mon Jun 29 17:10:38 2020

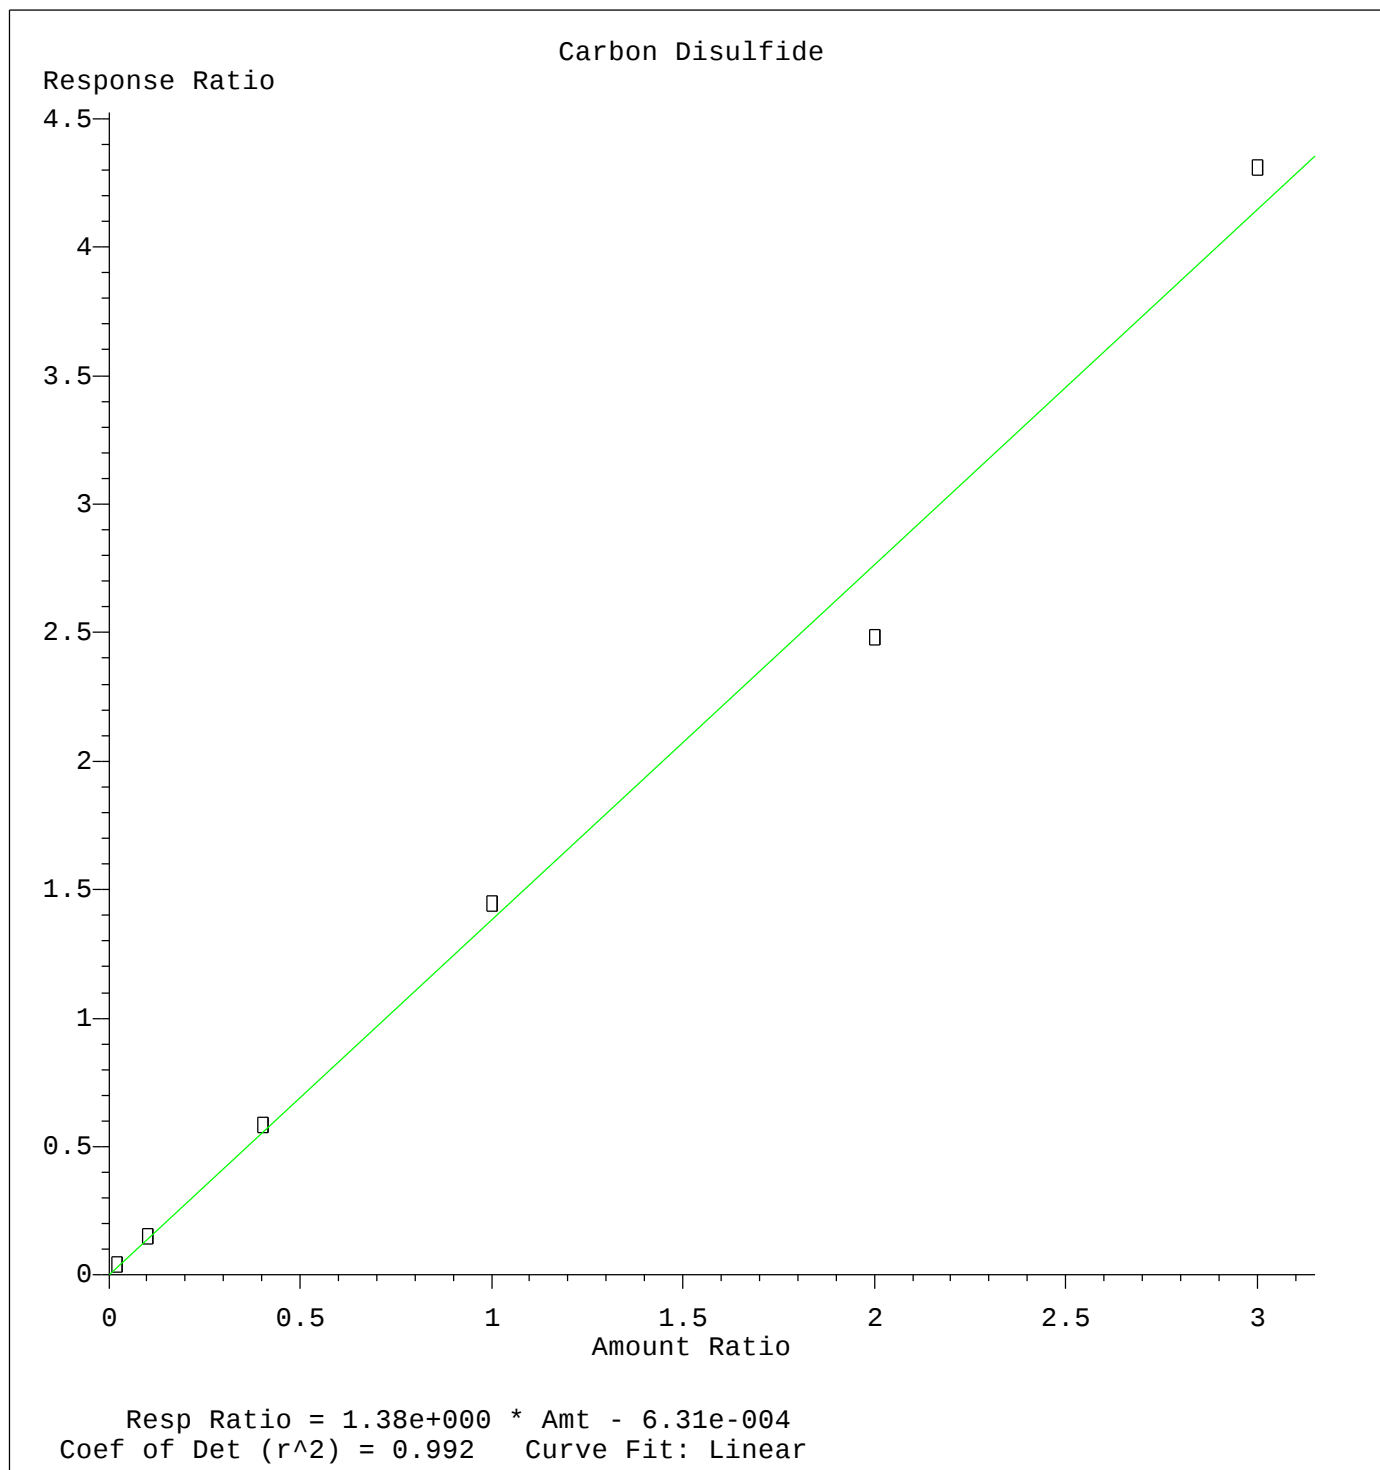

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
Calibration Table Last Updated: Mon Jun 29 17:10:38 2020


Methylene Chloride

Response Ratio

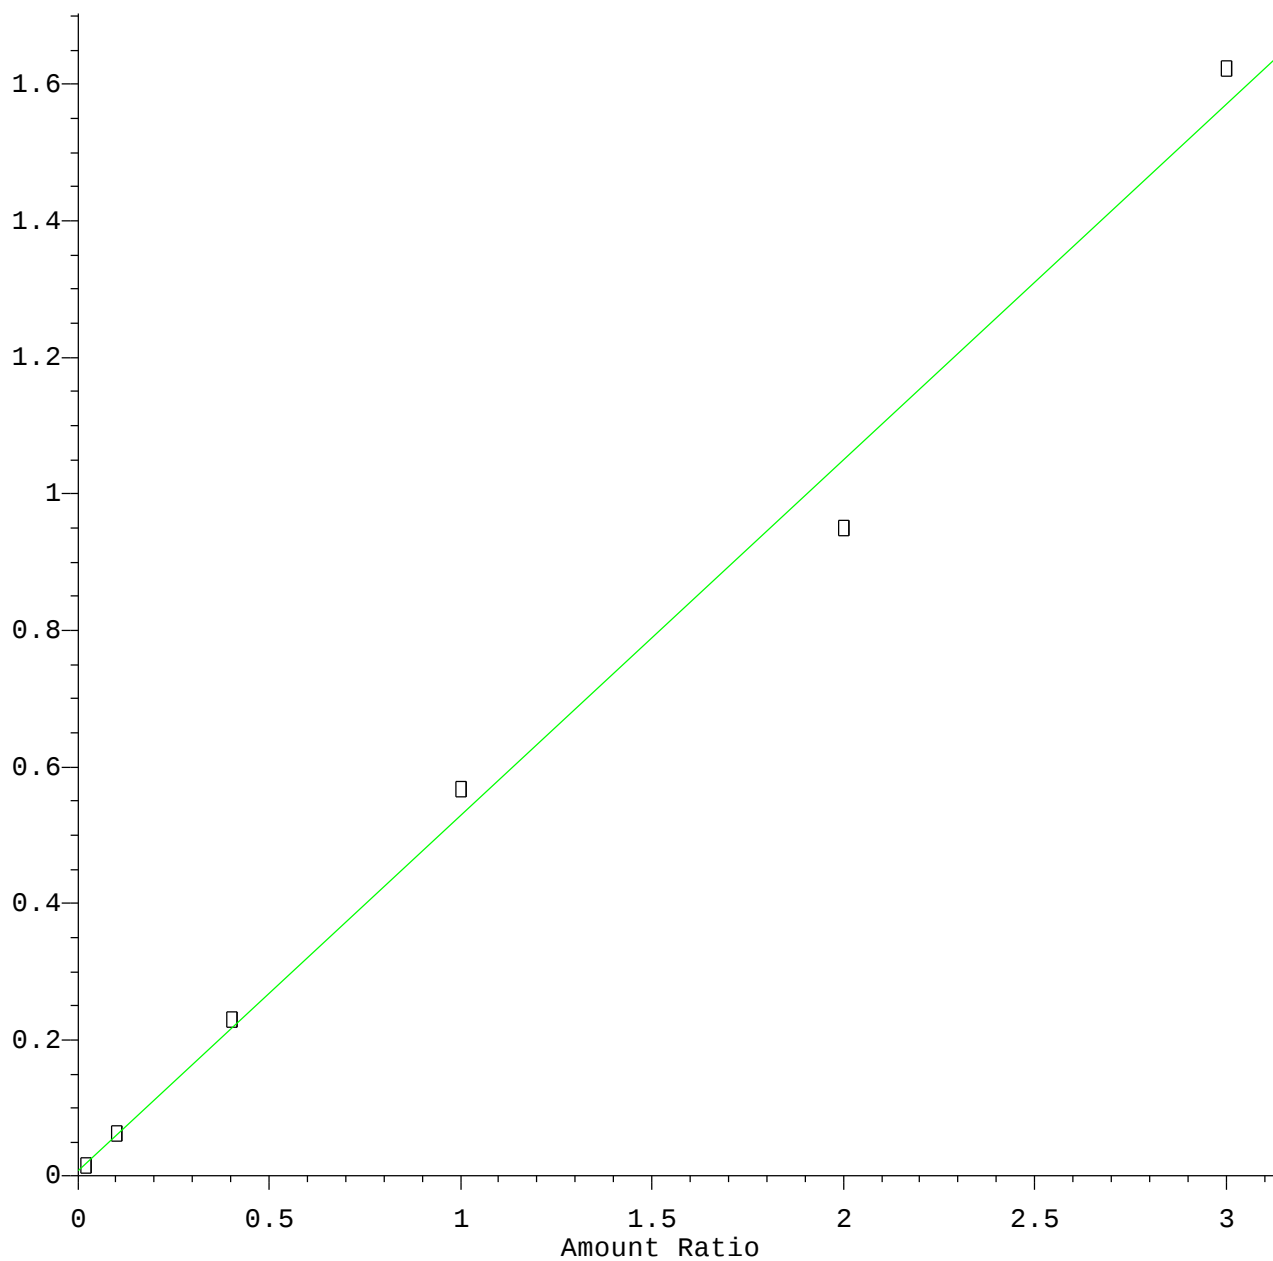

Resp Ratio = $5.21 \times 10^{-1} \times \text{Amt} + 8.28 \times 10^{-3}$
Coef of Det (r^2) = 0.993 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
Calibration Table Last Updated: Mon Jun 29 17:10:38 2020

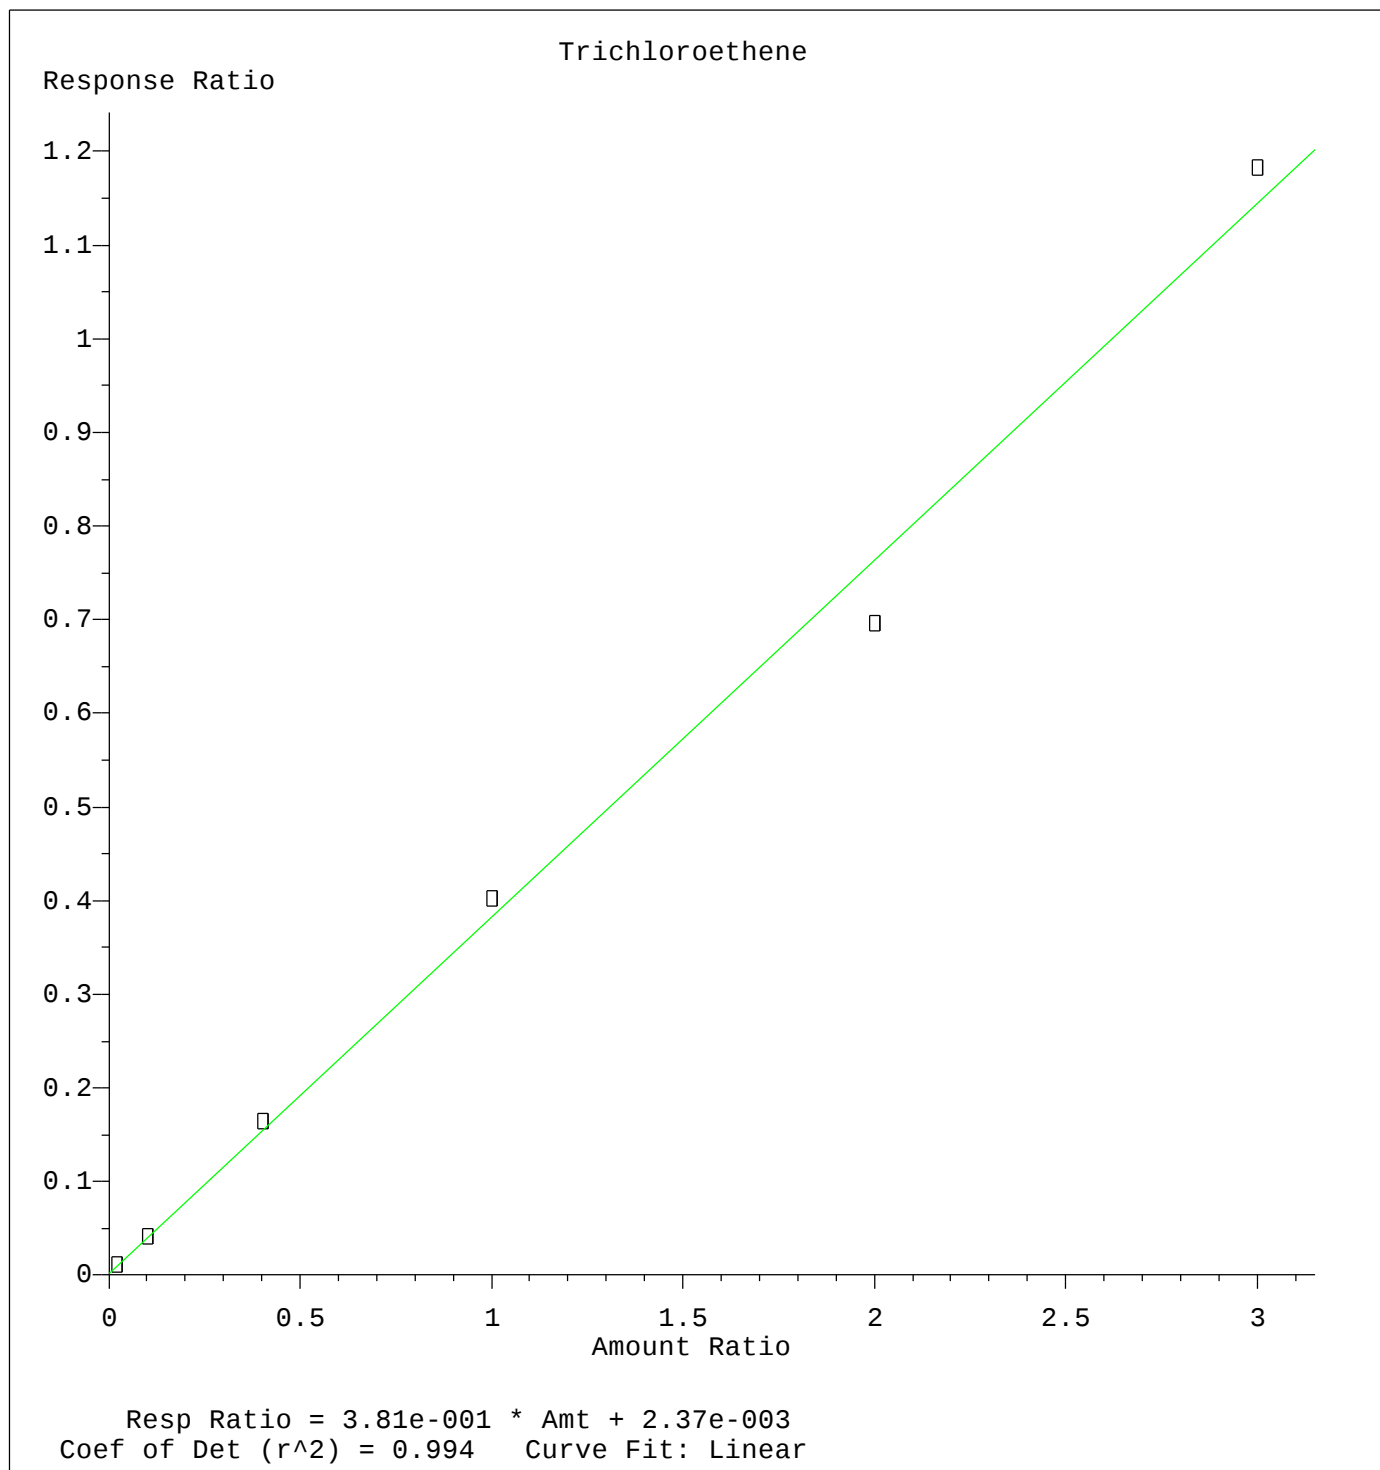

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
Calibration Table Last Updated: Mon Jun 29 17:10:38 2020