

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062921\
 Data File : VX023005.D
 Acq On : 29 Jun 2021 15:55
 Operator : JC/MD
 Sample : M2875-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-1A

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M

Title : SW846 8260

Signal : TIC: VX023005.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	37	rBV3	7011	12731	3.06%	0.461%
2	2.386	208	213	224	rVB	53062	85144	20.44%	3.084%
3	2.550	233	240	247	rBV	16418	29640	7.12%	1.074%
4	3.111	323	332	340	rBV5	1682	4430	1.06%	0.160%
5	5.397	695	707	718	rBV	42928	126103	30.28%	4.567%
6	5.562	723	734	755	rVB	76931	221554	53.19%	8.024%
7	5.824	768	777	778	rBV5	3024	4688	1.13%	0.170%
8	5.842	778	780	788	rVB4	3078	4829	1.16%	0.175%
9	5.964	790	800	808	rBV	62419	159168	38.22%	5.765%
10	6.044	808	813	825	rVB2	10028	26550	6.37%	0.962%
11	6.257	841	848	855	rVB4	3547	9282	2.23%	0.336%
12	6.769	920	932	943	rBV	129267	305827	73.43%	11.077%
13	7.379	1024	1032	1042	rBV5	4772	12648	3.04%	0.458%
14	7.988	1124	1132	1141	rVB5	3633	9387	2.25%	0.340%
15	8.110	1145	1152	1157	rBV2	4769	9697	2.33%	0.351%
16	8.586	1223	1230	1233	rBV4	4353	8464	2.03%	0.307%
17	8.653	1235	1241	1248	rVV	267635	416498	100.00%	15.085%
18	8.720	1248	1252	1259	rVB2	5487	8781	2.11%	0.318%
19	9.525	1376	1384	1388	rBV3	3783	6544	1.57%	0.237%
20	10.055	1466	1471	1478	rBV	259363	355999	85.47%	12.894%
21	10.195	1490	1494	1499	rVB2	11418	15458	3.71%	0.560%
22	10.305	1505	1512	1519	rVB	47958	66374	15.94%	2.404%
23	10.646	1563	1568	1575	rVB	15260	20106	4.83%	0.728%
24	11.085	1634	1640	1653	rBV	196078	255257	61.29%	9.245%
25	11.384	1684	1689	1696	rVB	8591	15898	3.82%	0.576%
26	11.457	1696	1701	1705	rBV2	6139	7963	1.91%	0.288%
27	11.616	1723	1727	1733	rVB2	5866	7854	1.89%	0.284%
28	11.756	1745	1750	1754	rVB	25488	31090	7.46%	1.126%
29	12.024	1789	1794	1801	rBV	241845	297188	71.35%	10.764%
30	12.091	1801	1805	1810	rVB	6973	8062	1.94%	0.292%
31	12.250	1823	1831	1838	rBV3	16847	31705	7.61%	1.148%
32	12.317	1838	1842	1848	rVB2	12705	17865	4.29%	0.647%
33	12.469	1862	1867	1873	rVB3	4946	6874	1.65%	0.249%
34	12.536	1873	1878	1880	rBV2	4592	6317	1.52%	0.229%
35	12.616	1887	1891	1895	rVV	11492	12139	2.91%	0.440%
36	12.701	1901	1905	1914	rVB4	5312	9974	2.39%	0.361%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062921\
 Data File : VX023005.D
 Acq On : 29 Jun 2021 15:55
 Operator : JC/MD
 Sample : M2875-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-1A

Integration Parameters: RTEINT.P
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
 Title : SW846 8260

37	12.927	1934	1942	1945	rVV2	5867	8142	1.95%	0.295%
38	12.963	1945	1948	1952	rVB	8914	10075	2.42%	0.365%
39	13.170	1973	1982	1986	rBV4	5269	8557	2.05%	0.310%
40	13.292	1999	2002	2008	rVB3	9126	12372	2.97%	0.448%
41	13.426	2020	2024	2032	rVB4	3683	5494	1.32%	0.199%
42	13.548	2040	2044	2047	rBV	3739	5193	1.25%	0.188%
43	13.585	2047	2050	2056	rVV3	4943	9183	2.20%	0.333%
44	13.670	2060	2064	2069	rVB5	3632	5958	1.43%	0.216%
45	13.780	2074	2082	2091	rVB	33411	45697	10.97%	1.655%
46	14.640	2217	2223	2229	rBV	10114	12807	3.07%	0.464%
47	14.780	2242	2246	2250	rBV	7494	9436	2.27%	0.342%


Sum of corrected areas: 2761002

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062921\
Data File : VX023005.D
Acq On : 29 Jun 2021 15:55
Operator : JC/MD
Sample : M2875-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-1A

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

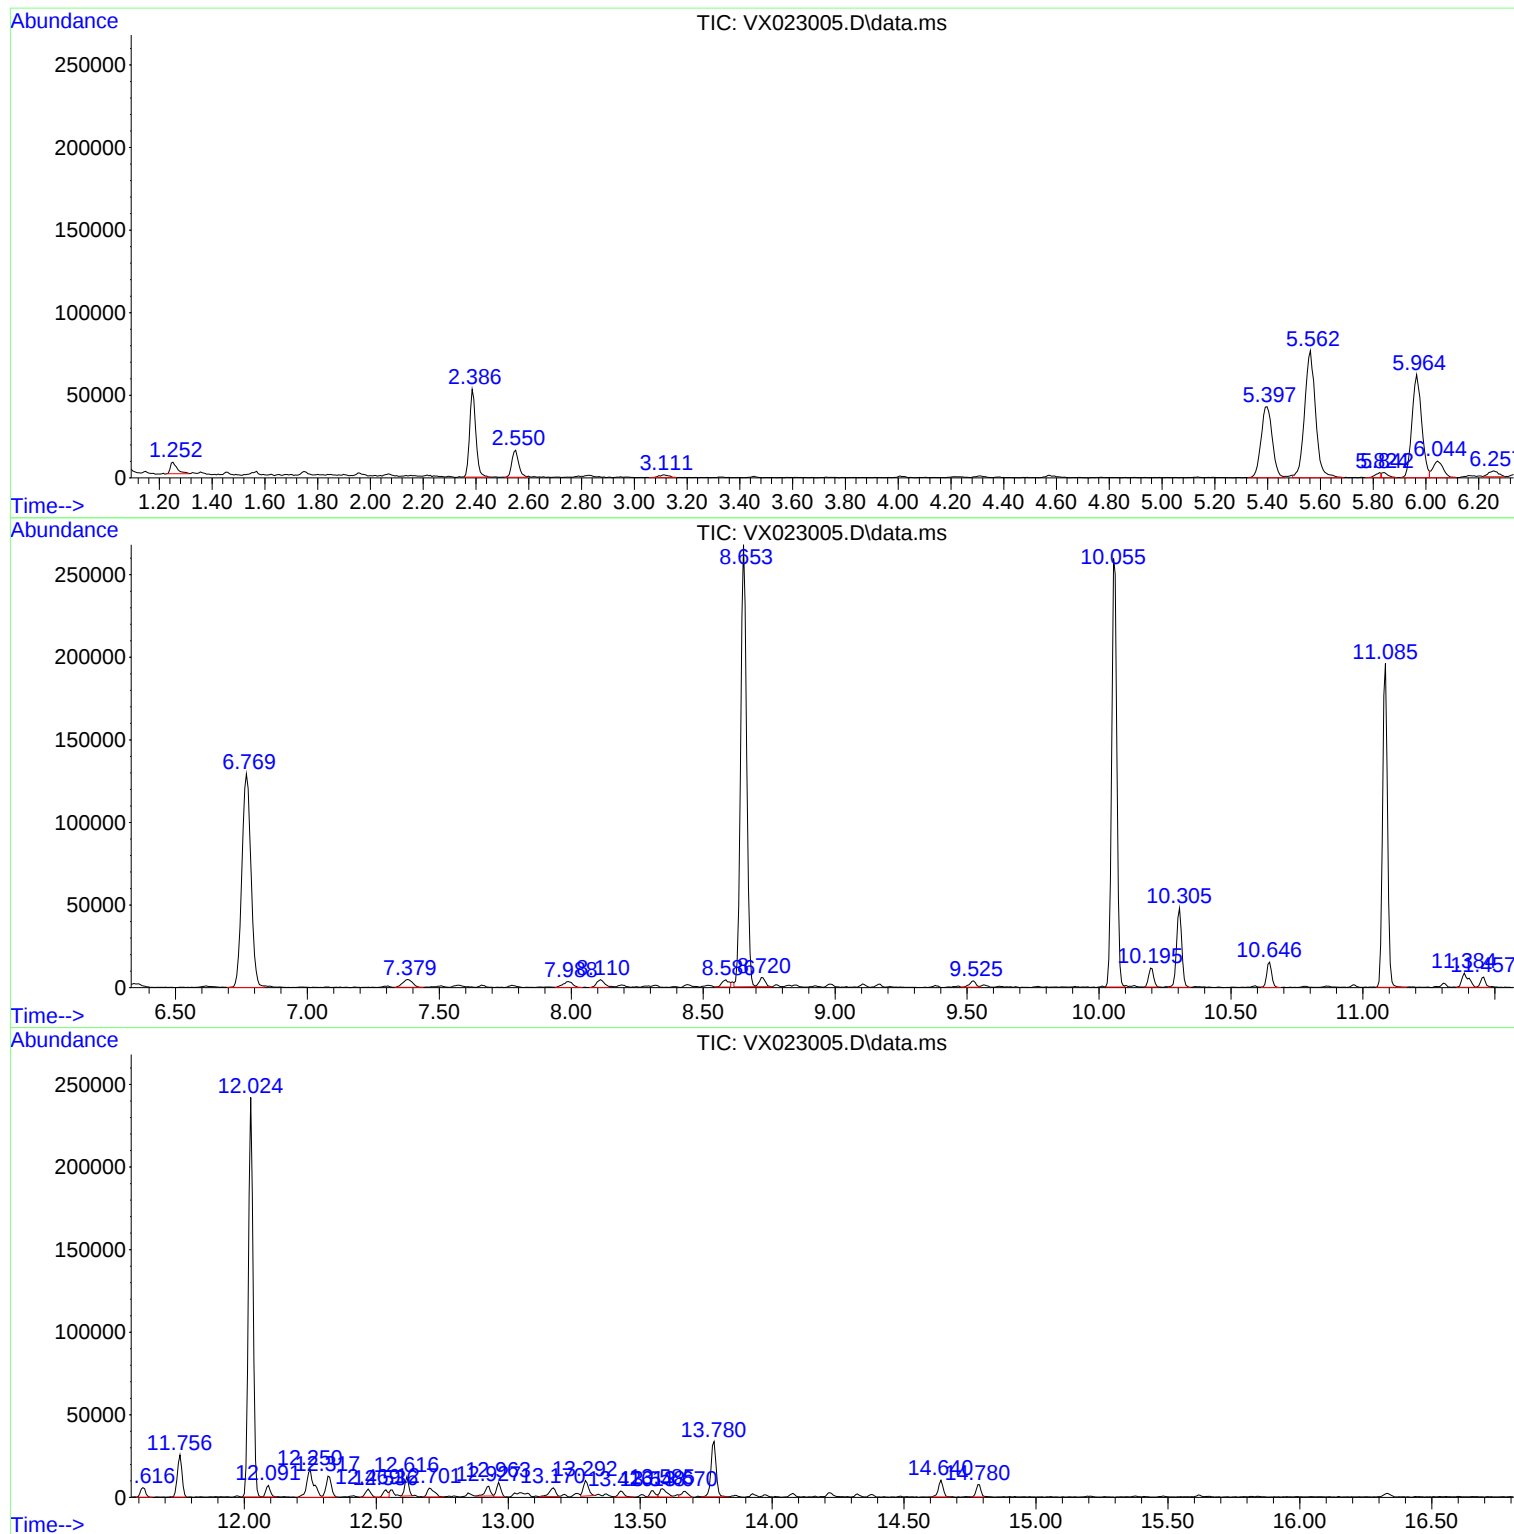

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062921\
Data File : VX023005.D
Acq On : 29 Jun 2021 15:55
Operator : JC/MD
Sample : M2875-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-1A










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown2.550 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.550	6.69 ug/l	29640	Pentafluorobenzene	5.562

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	40
2			Ethylamine	45	C2H7N	000075-04-7	5
3			2-Propanone, 1-methoxy-	88	C4H8O2	005878-19-3	4
4			4-Penten-2-ol	86	C5H10O	000625-31-0	4
5			Oxirane, (methoxymethyl)-	88	C4H8O2	000930-37-0	4

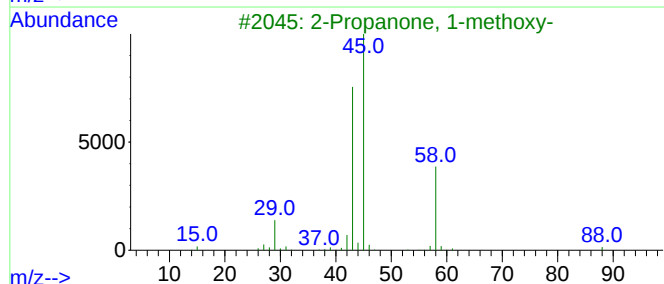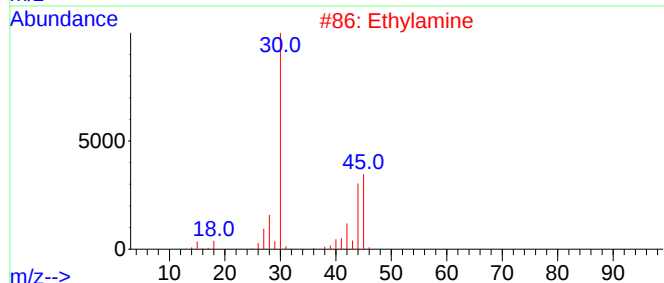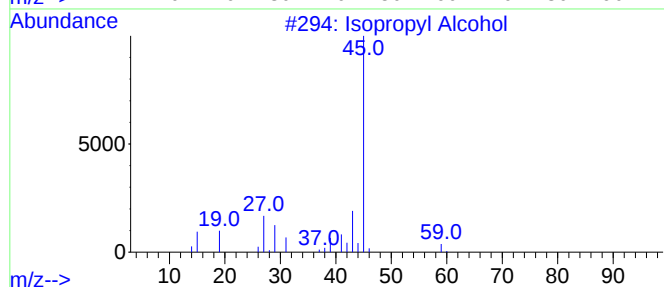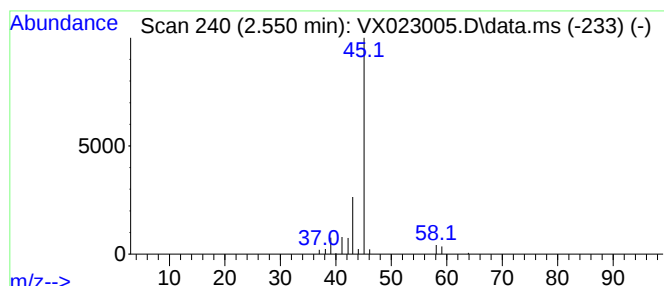

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062921\
Data File : VX023005.D
Acq On : 29 Jun 2021 15:55
Operator : JC/MD
Sample : M2875-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-1A










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Benzene, 1-propenyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.250	5.33 ug/l	31705	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1-propenyl-	118	C9H10	000637-50-3	90
2			Bicyclo[4.2.0]octa-1,3,5-triene,...	118	C9H10	055337-80-9	60
3			Indane	118	C9H10	000496-11-7	60
4			Benzene, 2-propenyl-	118	C9H10	000300-57-2	60
5			Benzene, cyclopropyl-	118	C9H10	000873-49-4	49

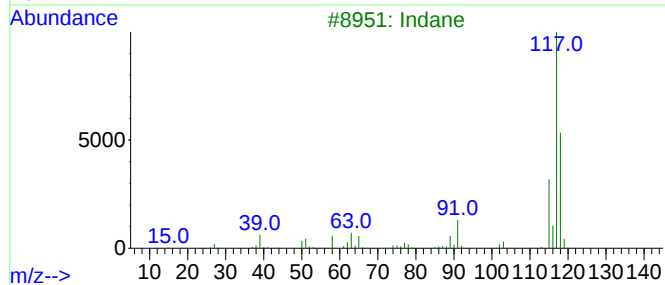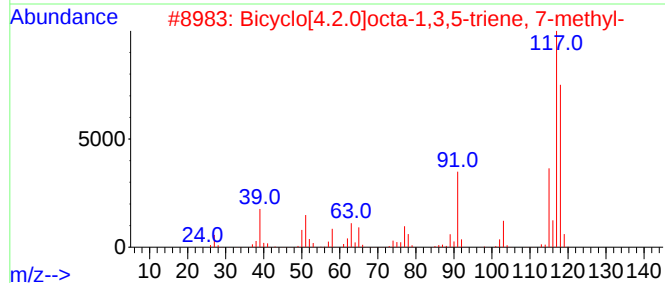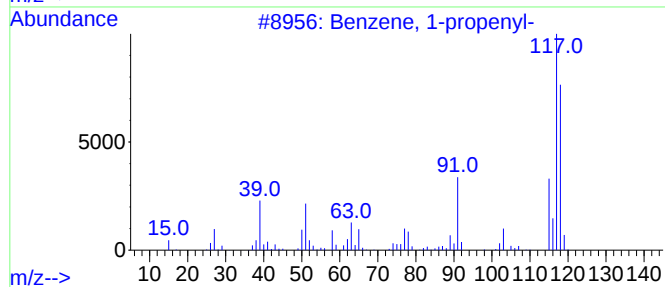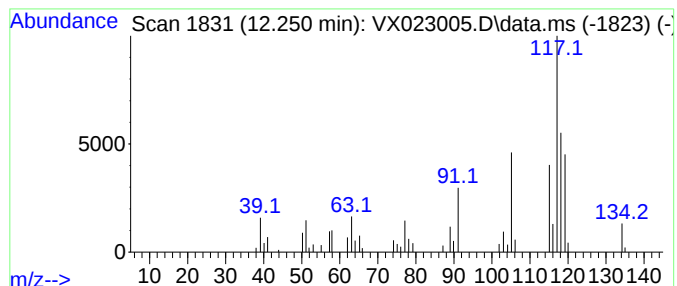

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062921\
Data File : VX023005.D
Acq On : 29 Jun 2021 15:55
Operator : JC/MD
Sample : M2875-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-1A

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown2.550	2.550	6.7	ug/l	29640	1	5.562	221554	50.0
Benzene, 1-prop...	12.250	5.3	ug/l	31705	4	12.024	297188	50.0